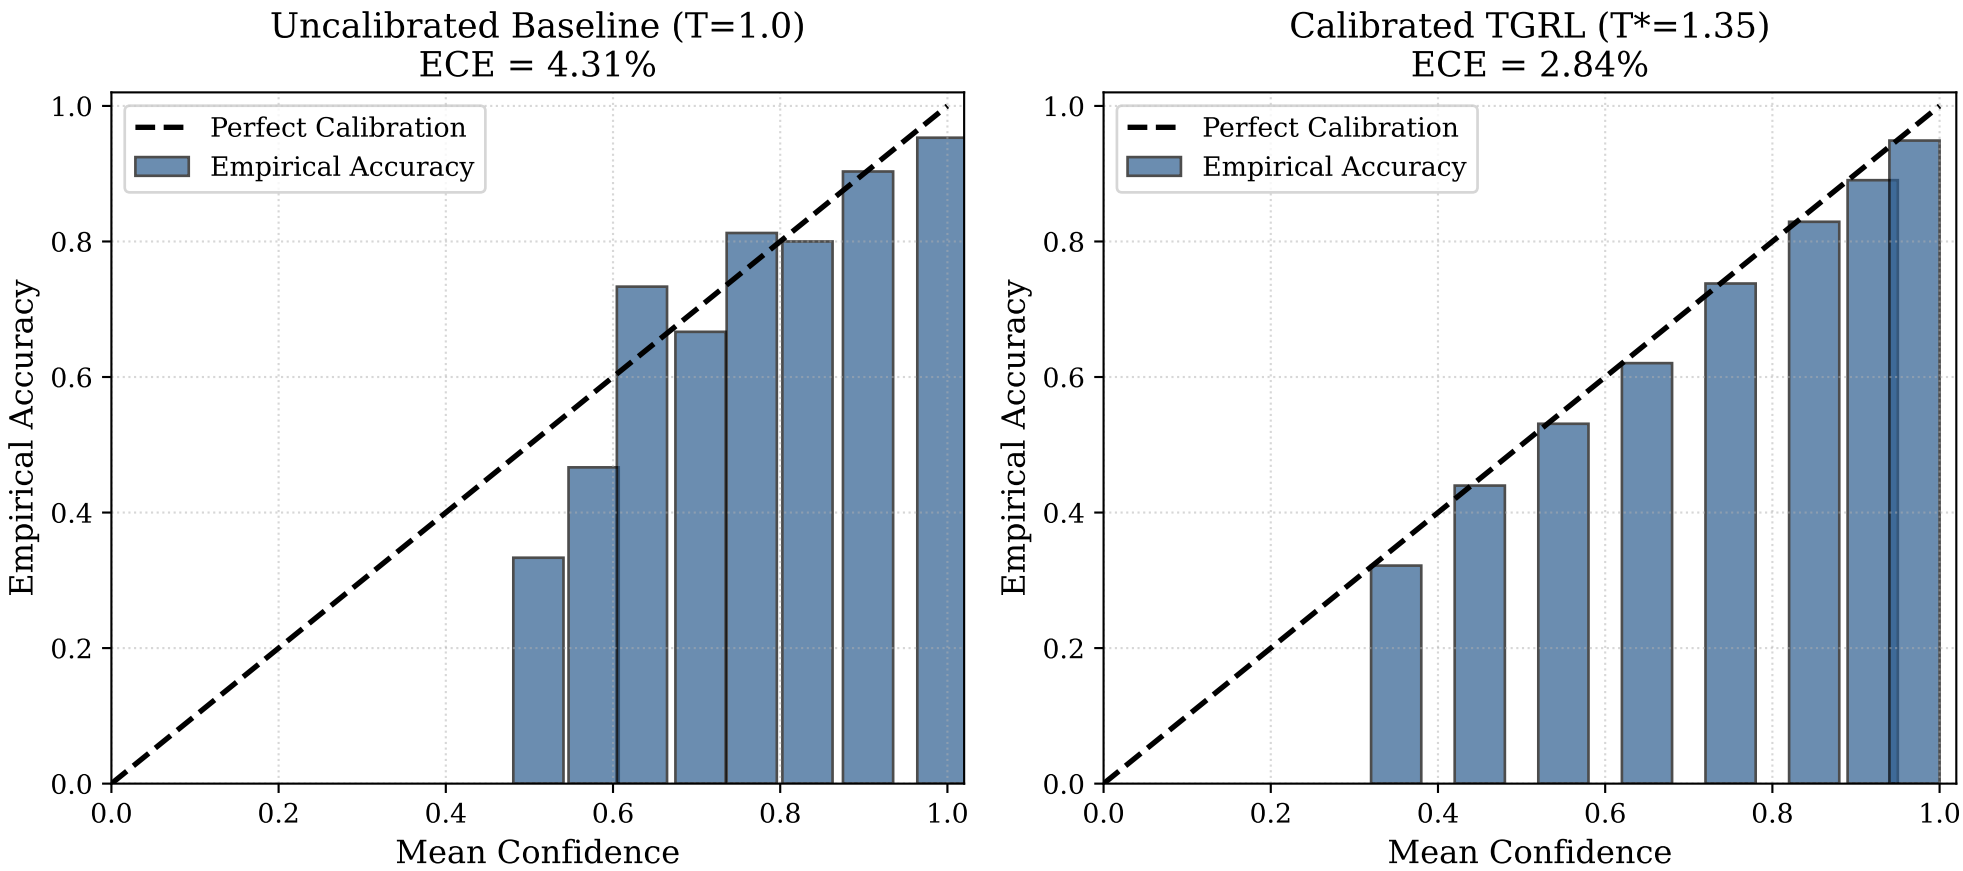
Uncalibrated Baseline (T=1.0)
ECE = 4.31%
Perfect Calibration
Empirical Accuracy
Empirical Accuracy
Mean Confidence
0.0
0.2
0.4
0.6
0.8
1.0
Calibrated TGRL (T*=1.35)
ECE = 2.84%
Perfect Calibration
Empirical Accuracy
Empirical Accuracy
Mean Confidence