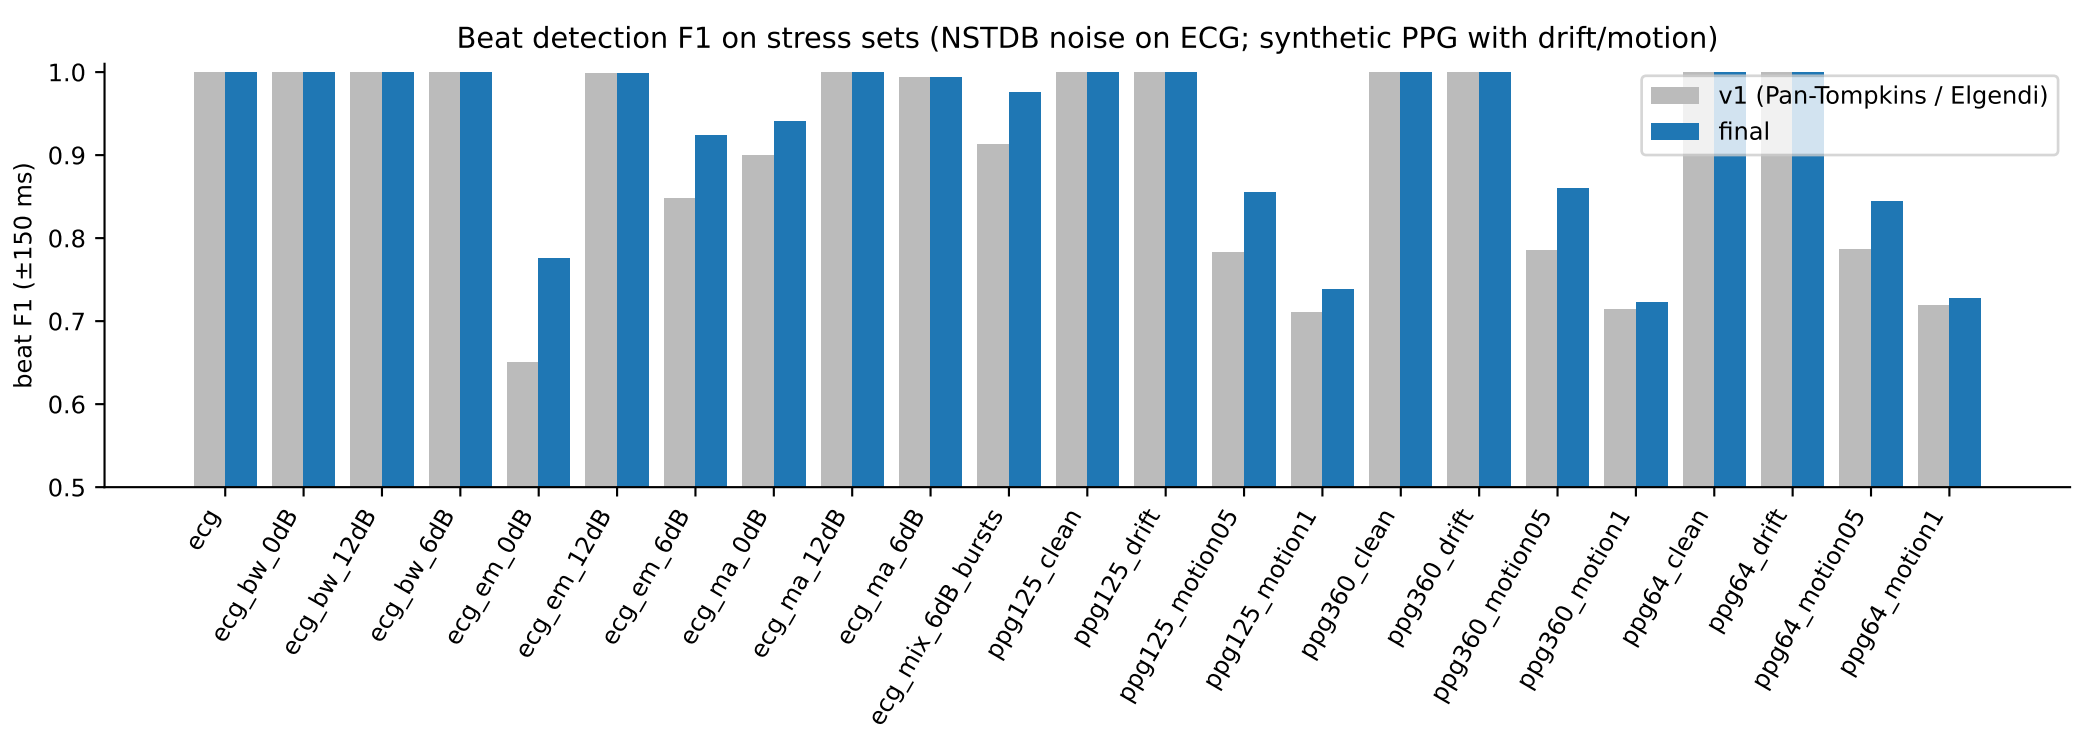
Beat detection F1 on stress sets (NSTDB noise on ECG; synthetic PPG with drift/motion)
beat F1 (±150 ms)
1.0
0.9
0.8
0.7
0.6
0.5
v1 (Pan-Tompkins / Elgendi)
final
ecg
ecg_bw_0dB
ecg_bw_12dB
ecg_bw_6dB
ecg_em_0dB
ecg_em_12dB
ecg_em_6dB
ecg_ma_0dB
ecg_ma_12dB
ecg_ma_6dB
ecg_mix_6dB_bursts
ppg125_clean
ppg125_drift
ppg125_motion05
ppg125_motion1
ppg360_clean
ppg360_drift
ppg360_motion05
ppg360_motion1
ppg64_clean
ppg64_drift
ppg64_motion05
ppg64_motion1