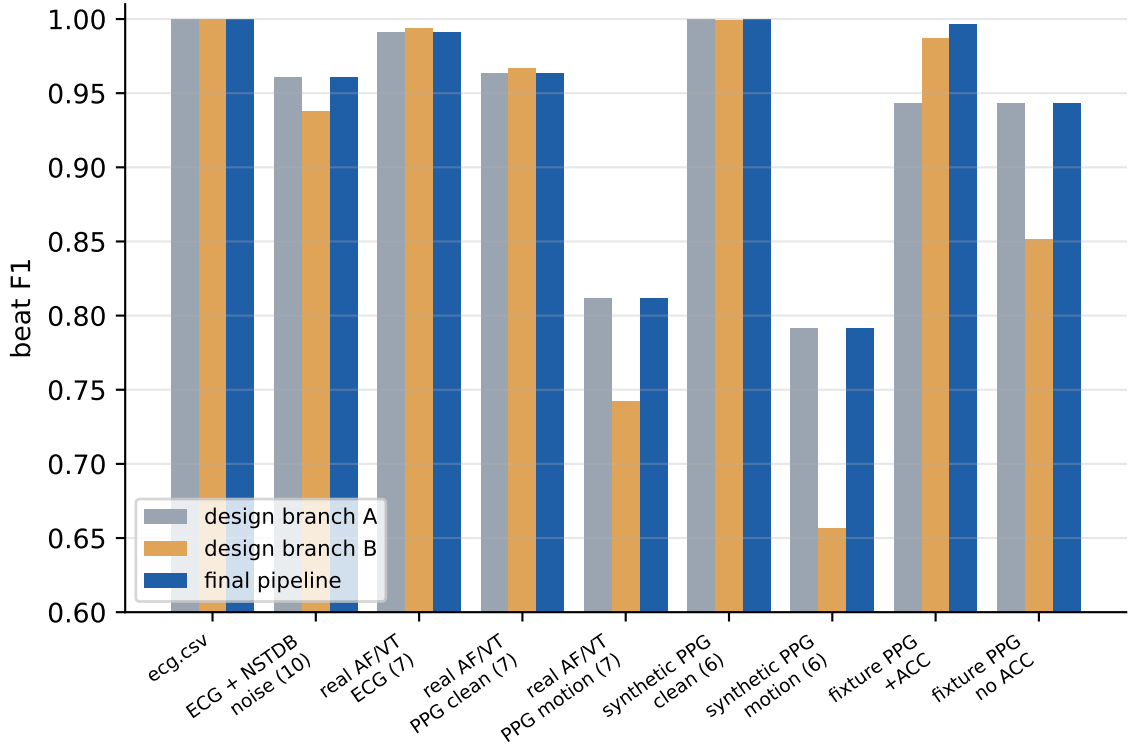
beat F1
1.00
0.95
0.90
0.85
0.80
0.75
0.70
0.65
0.60
design branch A
design branch B
final pipeline
ecg.csv
ECG + NSTDB noise (10)
real AF/VT ECG (7)
real AF/VT PPG clean (7)
real AF/VT PPG motion (7)
synthetic PPG clean (6)
synthetic PPG motion (6)
fixture PPG +ACC
fixture PPG no ACC

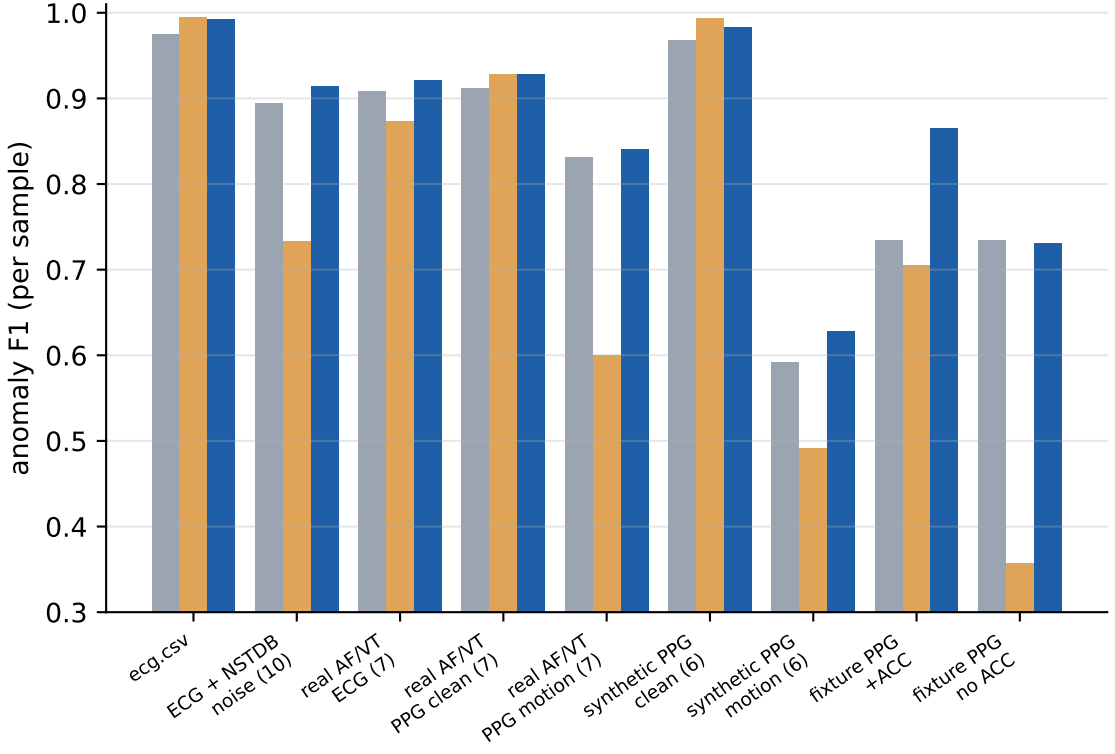
anomaly F1 (per sample)
1.0
0.9
0.8
0.7
0.6
0.5
0.4
0.3
ecg.csv
ECG + NSTDB noise (10)
real AF/VT ECG (7)
real AF/VT PPG clean (7)
real AF/VT PPG motion (7)
synthetic PPG clean (6)
synthetic PPG motion (6)
fixture PPG +ACC
fixture PPG no ACC