


GetSnap User Manual

Capture and save instrument screen images / waveform data with a single hotkey

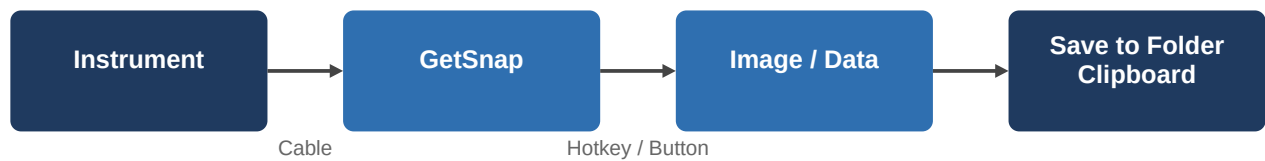

Screen-capture commands are initial defaults based on each vendor's commonly published command set. They may differ by model/firmware. You can adjust them directly from the app (see "5. Adding & Editing Instruments").

1. Launching the App

Method	Action
exe file (recommended)	Double-click dist\GetSnap.exe
From Python	venv\Scripts\activate → python app.py

GPIB connections require NI-VISA or Keysight IO Libraries Suite (see "6. Troubleshooting").

2. Screen Layout

Tab	Contents
Capture	Capture buttons, legend, preview, history
Devices	VISA resource list, connect
Settings	Save location, background mode, hotkeys, instruments, legend, language

 Save to Folder


 Copy to Clipboard

 Save Data (CSV, etc.)



Enable legend (applies to folder save & clipboard copy)

Asset No.	TR-2024-0012
Date	2026/08/21
Operator	Yamada
...	

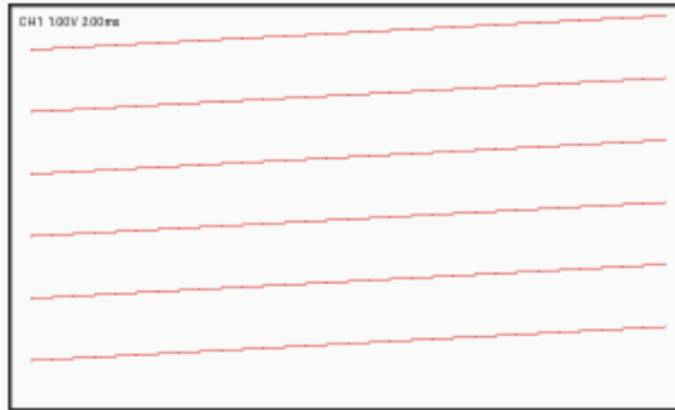


History

2026-08-21 21:58:04 [Yokogawa] Clipboard

2026-08-21 21:58:04 [Yokogawa] Folder -> D:\\Reports\\c

Capture tab (legend, preview, history)

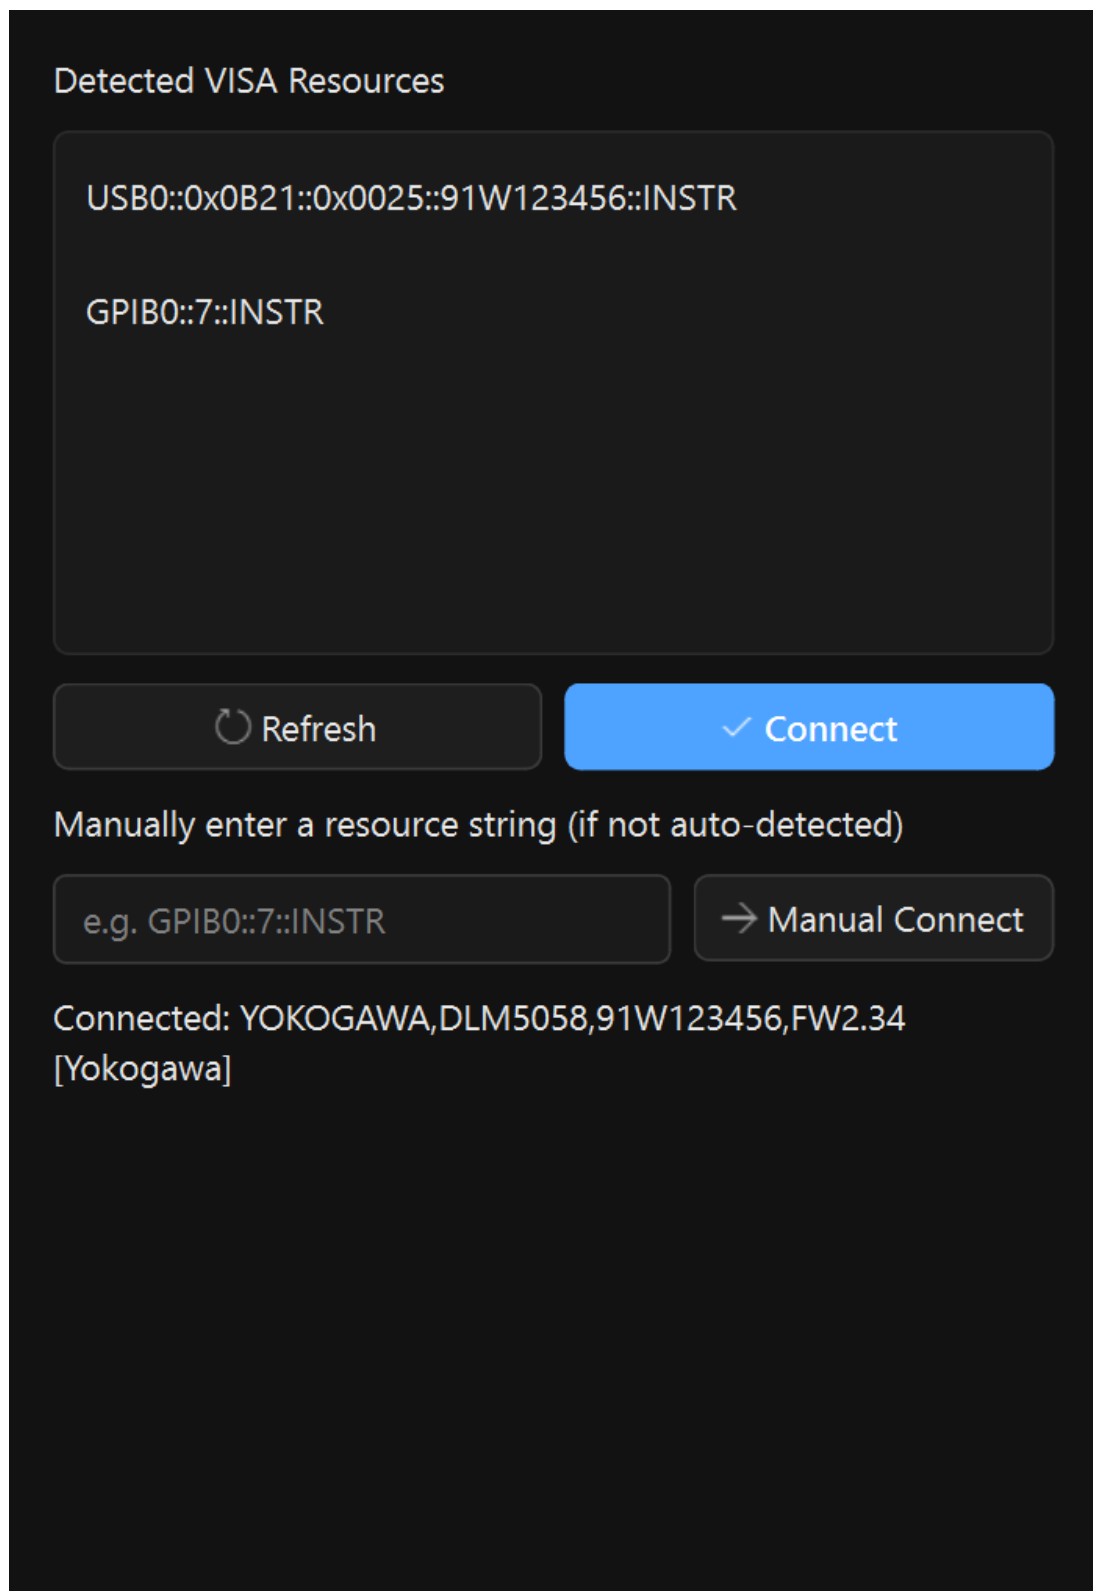

Devices tab

3. Basic Operation

Step	Action
① Connect	"Devices" tab → "Refresh" → select target → "Connect"
② Capture	Hotkey, or the buttons on the "Capture" tab

Step	Action
③ Check	Review the preview/history on the "Capture" tab
④ Paste	Ctrl+V in Excel, etc. (when copied to clipboard)

Hotkeys

Purpose	Key
Save to folder	Ctrl + Alt + F1
Copy to clipboard	Ctrl + W

When an Error Occurs

The [①...] shown at the start of the error dialog indicates which step failed.

Step shown	Meaning
Instrument not connected / Preset not registered	Not yet connected, or no preset is registered
①Connecting to VISA resource / ①Sending command / receiving response	Communication issue (cable, address, VISA runtime)
②Identifying model / ②Decoding image	Response data format issue
③Post-processing	Image processing issue (background conversion, legend)
④Saving / ④Copying	Permissions or disk space issue at the destination


4. Supported Instruments

The actual commands can always be reviewed and edited from the dialog in "5. Adding & Editing Instruments".

Vendor	Image Format	Data Export	Notes
Tektronix	PNG	Yes	
Keysight	PNG	Yes	VNA (E5000 series) uses a separate preset
Yokogawa	PNG	Yes	Return-to-local uses GTL only (see 5.5)
Rohde & Schwarz	PNG	Yes	Spectrum analyzer models use separate presets
Rigol	BMP	Yes	Spectrum analyzer / VNA models use separate presets

5. Adding & Editing Instruments

Go to "Settings" → "Instrument Settings..." to add or edit supported instruments. Your edits persist across app restarts.

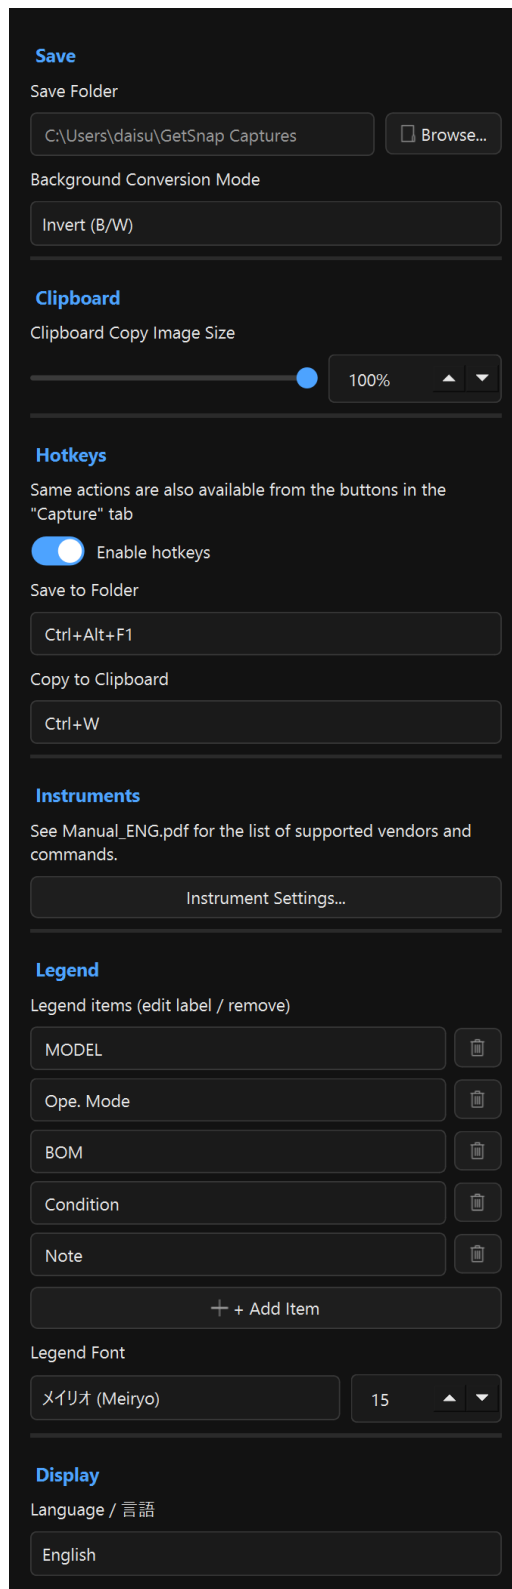

Settings tab (Instrument Settings button)

5.1 First, find the model match string

Before adding a new instrument, connect to it once from the "Devices" tab. You can connect even without a registered preset — the ***IDN?** response string is shown as-is on screen. Use part of that string (e.g. the vendor name) as the "model match string".

5.2 Editing an existing preset

Select an instrument from the list to open its form, edit the fields and press "Save" to override that instrument's settings only. Built-in presets cannot be renamed. "Reset to Default" restores the original content at any time.

Registered instruments

- Tektronix
- Keysight VNA (E5000 Series)
- Keysight
- Yokogawa**
- Rohde & Schwarz FSC
- Rohde & Schwarz FSVA
- Rohde & Schwarz FSWX
- Rohde & Schwarz
- Rigol RSA Spectrum Analyzer
- Rigol DSA Spectrum Analyzer
- Rigol VNA (DNA Series)
- Rigol

+ Add New

This is a built-in preset. Its name cannot be changed (use "+ Add New" to register it under a different name instead). Editing and saving overrides this instrument's settings only.

Name

Yokogawa

Model match string (substring of the *IDN? response, matched case-insensitively)

yokogawa

Image save commands (one per line, last line is the query)

:IMAGe:FORMat PNG
:IMAGe:SEND?

Fallback commands (used if the save commands fail; leave blank to reuse the commands above)

:IMAGe:FORMat PNG
:IMAGe:SEND?

Image Format

PNG

Delay Between Commands

0.00 s

Data export commands (optional, one per line)

:WAVeform:FORMat ASCII
:WAVeform:SEND?

Data export format (optional, e.g. CSV)

CSV

Return-to-local commands (optional, SCPI)

Optional. GPIB/USB connections already use VISA-level GTL (go-to-local) as the primary mechanism, so this can usually be left blank.

Notes (optional)

要検証：DLM/DLシリーズを想定した一般的な構成例。ハードコピー専用の白背景出力コマンドを確認できていないため、save_function_commandsとfallback_commandsは同一としている。機種別の構成例は、各機種ごとのマニュアルを参照してください。

Save

Reset to Default

Preset edit screen (Yokogawa example)

5.3 Adding a new instrument

Press "+ Add New" at the bottom left to open a blank form. Fill in the required fields (name, model match string, image save commands) and press "Save" to add it to the list. "Delete" removes it at any time.

Registered instruments

Tektronix

Keysight VNA (E5000 Series)

Keysight

Yokogawa

Rohde & Schwarz FSC

Rohde & Schwarz FSVA

Rohde & Schwarz FSWX

Rohde & Schwarz

Rigol RSA Spectrum Analyzer

Rigol DSA Spectrum Analyzer

Rigol VNA (DNA Series)

Rigol

+ Add New

Name

Anritsu

Model match string (substring of the *IDN? response, matched case-insensitively)

anritsu

Image save commands (one per line, last line is the query)

:HCOPy:SDUMp:DATA?

Fallback commands (used if the save commands fail; leave blank to reuse the commands above)

:DISPlay:DATA?

Image Format

PNG

Delay Between Commands

0.00 s

Data export commands (optional, one per line)

Optional (leave blank if data export is not supported)

Data export format (optional, e.g. CSV)

CSV

Return-to-local commands (optional, SCPI)

Optional. GPIB/USB connections already use VISA-level GTL (go-to-local) as the primary mechanism. so this can usually be left blank.

Notes (optional)

Save

Delete

Preset add-new screen (Anritsu example)

5.4 Field Reference

Field	Description	Example
Name	Display name in the list (built-in presets cannot be renamed)	Anritsu
Model match string	Substring of the *IDN? response, matched case-insensitively; first match from the top of the list wins	anritsu
Image save commands	Screen capture commands, one per line; the last line is the query that returns the image	:HCOPy:SDUMp:DATA?
Fallback commands	Used if the save commands fail. Leave blank to reuse the save commands	:DISPlay:DATA?
Image format	Image format of the returned data	PNG / BMP

Field	Description	Example
Delay between commands	Wait time between multiple commands, in seconds	0.0-1.0
Data export commands (optional)	Waveform data retrieval commands	:WAVEform:SEND?
Data export format (optional)	Roughly, the saved file's extension	CSV
Return-to-local commands (optional)	Extra command(s) to restore the front panel after capture	Usually blank (see 5.5)
Notes (optional)	Free text	-

5.5 Leave "Return-to-local commands" blank in most cases

For GPIB/USB connections, GetSnap already restores the front panel automatically after capture via VISA-level GTL (Go To Local). Entering a command the instrument doesn't recognize here can actually cause a command-error message or leave the panel locked (**confirmed through real hardware testing on a Yokogawa DLM5058**). Only enter a command here if GTL alone does not restore the panel for your instrument.

6. Troubleshooting

Symptom	Fix
Instrument doesn't appear in the list over GPIB	Install NI-VISA or Keysight IO Libraries Suite
Connects fine but capture fails	Check the failing step at the start of the error, then review commands in "5."
Want to change the image background color	Toggle "Background Conversion Mode" on the "Settings" tab
Hotkey doesn't respond	May conflict with another app; use the buttons on the "Capture" tab instead
Front panel unresponsive after capture	See "5.5"