



DEPARTMENT OF ENGINEERING CYBERNETICS

TTK4550

Specialization Project

Authors:

Anders Haarberg Eriksen, Øyvind Stavdahl & Devon Rohlf

Date: 22nd May 2026

Project Assignment

Candidate	Anders Haarberg Eriksen
Programme	Cybernetics and Robotics
Project title	Adaptive Control and Parameter Estimation for Motion Control in a Tendon-Driven Hand Exoskeleton
Norwegian title	Adaptiv regulering og parameterestimering for bevegelsesstyring i et senedrevet h�ndeksoskjelett
Supervisors	�yvind Stavdahl, Devon Rolhf
Institution	Department of Engineering Cybernetics, NTNU, in collaboration with the N-squared Lab, FAU, Erlangen, Germany

Modern hand exoskeletons require precise and reliable control of the relevant mechanical states to enable natural, predictable, and safe interaction with the environment. However, the current implementation of the present glove–cable system introduces nonlinearities, uncertain mechanical parameters, and inconsistent finger positioning, making accurate control difficult. To address these challenges, an adaptive control framework is desired that can estimate system parameters in real time, compensate for nonlinearities, and ensure stable behavior during both free motion and object interaction.

The goal of this project is to design an adaptive controller for a 6-DOF hand exoskeleton, capable of regulating both torque and fingertip positioning. This includes identifying relevant mechanical parameters and creating a nonlinear model of the system. Additionally, modifications to the glove mechanics and integration of fingertip sensors could enable better positioning and torque estimation and facilitate switching between control modes and should therefore be investigated. The final system should allow reliable, intuitive control of finger motion while providing insight into system properties such as friction and internal forces.

The work should thus include the following:

- Development of a nonlinear model of a single finger to support adaptive control.
- Design of an adaptive control architecture for both torque output and finger positioning.
- Estimation of mechanical parameters and internal forces.
- Evaluation of fingertip sensors to support mode switching and refined control.
- Documentation and of the system architecture, experiments, and control performance.

Contents

1	Introduction	1
2	Theory	2
2.1	Anatomy	2
2.1.1	Anatomical directional terms	2
2.1.2	Anatomical terms of movement	2
2.1.3	Hand anatomy	3
2.2	Modelling	6
2.2.1	Homogenous transformations	6
2.3	Control	7
2.3.1	State-Space representation	7
2.3.2	Controllability	7
2.3.3	MRAC	7
3	Modelling	10
3.1	Finger model	10
3.1.1	Kinetic energy	12
3.1.2	Potential energy	13
3.1.3	Generalized forces	14
3.1.4	Rigid-body dynamics	14
3.2	Brushed DC Motor model	16
3.2.1	Estimating motor parameters	17
3.2.2	Estimating the armature inductance and rotor inertia	18
3.2.3	Mass-spring-damper load	21
3.2.4	State-space model of brushed DC motor with load	21
4	Controller design	22
4.1	Current controller	22
4.1.1	Discretization of current controller	23
4.1.2	Stability analysis and tuning of controller	23
4.1.3	Simulation of current controller	24

4.1.4	Evaluation of controller	27
4.2	Torque control	27
4.2.1	Force control with integrated fingertip force sensors	29
4.3	Model reference adaptive control (MRAC) for position control	30
4.3.1	Controllability of the system	31
4.3.2	MRAC implementation	31
4.3.3	Connecting the motors to the finger through a cable	33
4.3.4	Simulation of MRAC scheme with updated dynamics	35
4.3.5	Evaluation of MRAC scheme	36
5	Discussion	41
5.1	Current control	41
5.2	Torque and force control	42
5.3	Position controller using MRAC	43
5.4	Model assumptions and limitations	44
5.5	Practical implementation considerations	45

List of Figures

1.1	Planned setup for one motor controlling one finger.	1
2.1	The anatomical position, with the corresponding directional terms. Image from TeachMeAnatomy, 2026a	3
2.2	Anatomical terms of movement. Image from TeachMeAnatomy, 2026b	3
2.3	The bones of the hand. Image from author.	4
2.4	The joints of the hand. Image from author.	5
3.1	Schematic of the finger model, with three revolute joints, torsional springs and dampers.	11
3.2	Table of model parameters.	11
3.3	Schematic of the homogenous transformation frames.	13
3.4	Circuit diagram of armature circuit of the DC motor model, with output torque and angular position.	16
3.5	Parameter identification of the armature inductance L_a and rotor inertia J_m using a step input in the armature voltage E_a	20
4.1	Armature current step response for discrete-time P+FF and P controllers tracking a 1 A reference, with $T_s = 0.2$ ms and initial motor speed $\omega_0 = 5$ rad s ⁻¹	25
4.2	Armature current step response for discrete-time P+FF and P controllers tracking a 1 A reference, with $T_s = 0.2$ ms and initial motor speed $\omega_0 = 0$ rad s ⁻¹	25
4.3	Effect of current measurement noise on the armature current response using a discrete-time P+FF controller with $T_s = 0.2$ ms.	26
4.4	Effect of current measurement noise on the armature current response using a discrete-time P+FF controller with $T_s = 1.0$ ms.	26
4.5	Torque control with a P controller when gripping a rigid object.	29
4.6	Force control with friction. With and without force sensors in fingertips. Both controllers have $T_s = 0.2$ ms.	30

4.7	Force application on the finger. The flexion motor applies a force F_f on the flexion cable, which gets distributed to the three phalanges through the whiffle tree. Similarly, the extension motor applies a force F_e on the extension cable, which also gets distributed to the three phalanges through its own whiffle tree.	36
4.8	Simulation results of the MRAC scheme for flexion and extension motor over 10 s.	37
4.9	Simulation results of the MRAC scheme for flexion and extension motor after 90 s.	37
4.10	Adaptive gains and error over time for MRAC scheme for 100 s, where K_1 and L keep growing together.	39
4.11	Simulation results of the MRAC scheme for flexion and extension motor over 10 s, with the adaptive gains found in Figure 4.10 after 100 s, but with the gains fixed instead of adaptive.	40

List of Tables

3.1	Constants in system matrices.	16
3.2	Relevant motor parameters extracted from the datasheet of the motor.	18
4.1	Physical parameters used for the finger model.	38

Chapter 1

Introduction

Hand exoskeletons have gained increasing attention in recent years due to their potential in rehabilitation, assistive technology, and human motion augmentation. By providing controlled support to the hand and fingers, such systems may help restore function in individuals with impaired motor ability, while also serving as platforms for studying human biomechanics and control. Because the hand is mechanically complex and highly dexterous, the development of effective hand exoskeletons requires accurate models of finger motion and dynamics.

A key challenge in the design of such systems is the interaction between the mechanical structure of the exoskeleton and the physiological properties of the human finger. The finger is a multi-joint system with coupled motion, passive elastic properties, and nonlinear dynamics. To design controllers that achieve stable and precise movement assistance, it is therefore important to establish a mathematical model that captures the essential kinematic and dynamic behavior of the finger, while remaining suitable for simulation and control design.

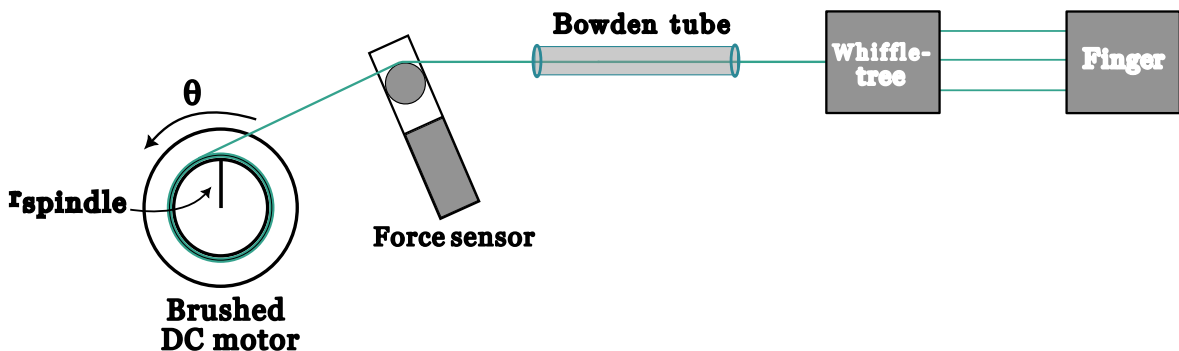


Figure 1.1: Planned setup for one motor controlling one finger.

Chapter 2

Theory

2.1 Anatomy

The hand is a complex biomechanical system, comprised of many different bones, muscles, tendons, and ligaments. To explain different aspects of the hand in relation to one another, we use *anatomical terminology* [National Cancer Institute, 2026], or more specifically *anatomical directional terms*. Additionally when describing actions of muscles upon the skeleton, we use *anatomical terms of movement* [TeachMeAnatomy, 2026b].

2.1.1 Anatomical directional terms

Anatomical directional terms are used in relation to the *anatomical position*, shown in Figure 2.1, where the body is assumed standing upright, with arms at the sides and palms facing forward. Relevant terms include: *proximal*, *distal*.

- **Proximal** means toward or nearest the point of origin of a part.
- **Distal** means away from or farthest from the point of origin of a part.

2.1.2 Anatomical terms of movement

To explain the actions of muscles upon the skeleton, we use anatomical terms of movement, which describes the movement of a body part in relation to the anatomical position. Relevant terms include: *flexion*, *extension*, *abduction*, *adduction*.

- **Flexion** is a movement that decreases the angle between two body parts.
- **Extension** is a movement that increases the angle between two body parts.
- **Abduction** is a movement away from the midline of the body.

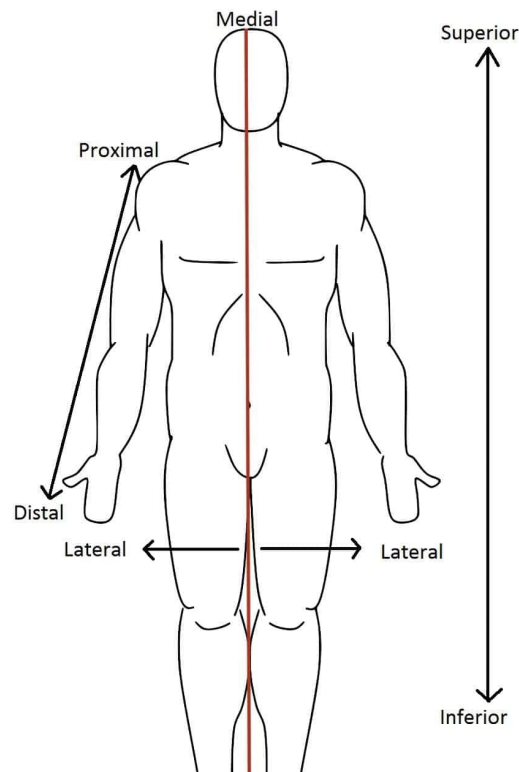


Figure 2.1: The anatomical position, with the corresponding directional terms. Image from TeachMeAnatomy, [2026a](#).

- **Adduction** is a movement toward the midline of the body.

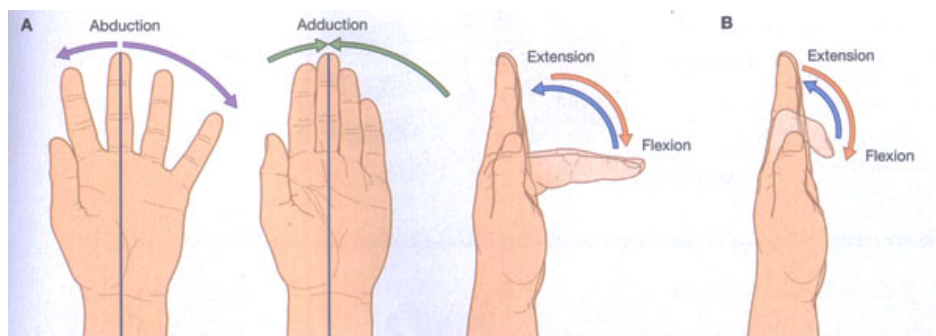


Figure 2.2: Anatomical terms of movement. Image from TeachMeAnatomy, [2026b](#).

2.1.3 Hand anatomy

The hand is comprised of several bones, muscles, tendons, and ligaments. The bones, illustrated in Figure 2.3, include the *carpals*, *metacarpals*, and *phalanges*. The carpals make out the wrist, the metacarpals make out the palm, and the phalanges make out the fingers. The thumb has two phalanges, while the other fingers have three. The bones of interest are the phalanges (marked in green), as they are the ones being moved by the exoskeleton. The metacarpals are assumed stationary for the task at hand, as the exoskeleton will provide stiffness to the palm and wrist.

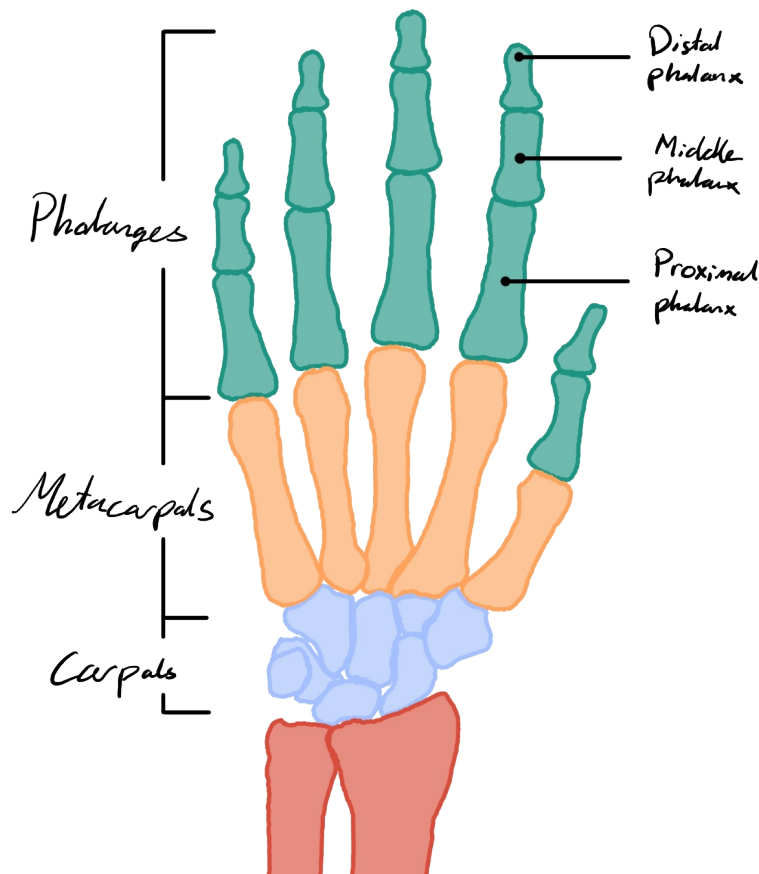


Figure 2.3: The bones of the hand. Image from author.

The phalanges are further divided into three sections: the *proximal phalanges*, the *middle phalanges*, and the *distal phalanges*. The proximal phalanges are the ones closest to the palm, while the distal phalanges are the ones furthest from the palm. The middle phalanges are the ones in between. The thumb does not have a middle phalanx, as it only has two phalanges.

Further details about the joints are shown in Figure 2.4. The joints of interest are the *metacarpophalangeal joints* (MCP), the *proximal interphalangeal joints* (PIP), and the *distal interphalangeal joints* (DIP). The MCP joints are the ones between the metacarpals and the proximal phalanges, while the PIP joints are the ones between the proximal phalanges and the middle phalanges, and the DIP joints are the ones between the middle phalanges and the distal phalanges. The thumb only has an MCP joint and an interphalangeal joint (IP), as it does not have a middle phalanx.

At each of the joints, there are collateral ligaments that provide stability. For the PIP, IP and DIP joints, they provide stiffness that prevents side to side motion. For the MCP joints they're relaxed when the finger is extended, facilitating for adduction and abduction, but stiff when the finger is flexed.

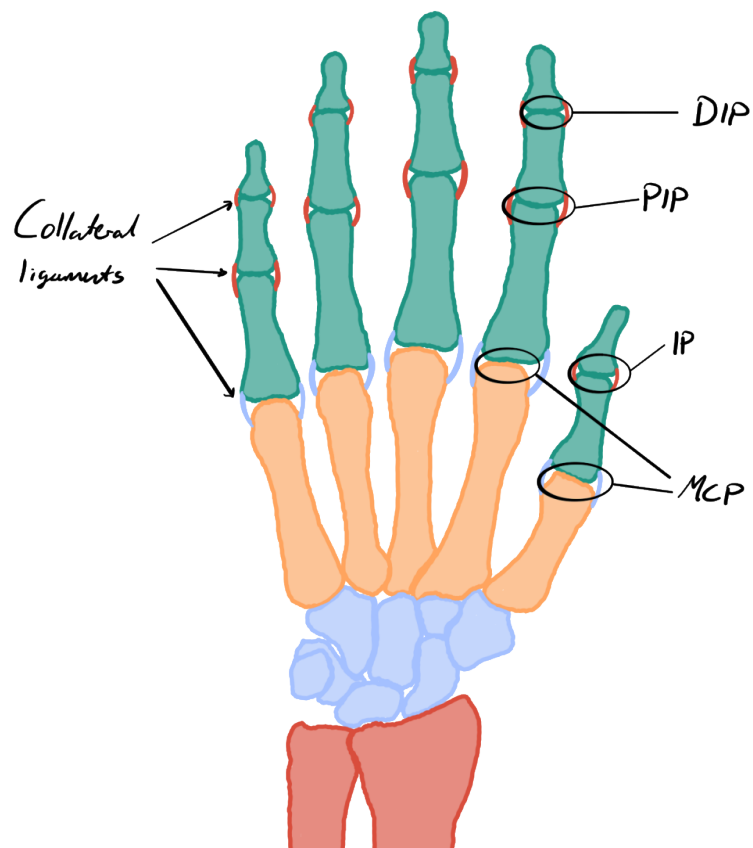


Figure 2.4: The joints of the hand. Image from author.

2.2 Modelling

2.2.1 Homogenous transformations

When modelling kinematic chains, we often need to move between frames. This often includes both rotation and translation. An efficient way to represent this is by using *homogenous transformations*.

Definition

For a 2D system, the rotation matrix for a counter-clockwise rotation by an angle θ is given by:

$$\mathbf{R}(\theta) = \begin{bmatrix} \cos(\theta) & -\sin(\theta) \\ \sin(\theta) & \cos(\theta) \end{bmatrix}. \quad (2.1)$$

Given a translation vector from frame i to frame j , written in terms of frame i , $\mathbf{d}_i^j = \begin{bmatrix} d_x^i \\ d_y^i \end{bmatrix}$, the homogenous transformation matrix from frame j to frame i , describing the rotation θ and translation $\mathbf{d}_i^j$ from frame i to frame j , can be expressed as:

$$\mathbf{H}_j^i = \begin{bmatrix} \mathbf{R}(\theta) & \mathbf{d}_i^j \\ \mathbf{0}_{1 \times 2} & 1 \end{bmatrix}. \quad (2.2)$$

Points represented in terms of homogenous transformations are represented as a 3D vector, where the first two elements represent the coordinates of the point in the plane, and the third element is always 1. For example, a point $\mathbf{p}_n$ in frame n with coordinates (x, y) can be represented as:

$$\mathbf{p}_n = \begin{bmatrix} p_x^n \\ p_y^n \\ 1 \end{bmatrix}. \quad (2.3)$$

Useful properties

Given a kinematic chain of size n , we can express the homogenous transformation from frame n to frame 1 as the product of the homogenous transformations between each consecutive frame:

$$\mathbf{H}_n^1 = \mathbf{H}_2^1 \mathbf{H}_3^2 \cdots \mathbf{H}_n^{n-1}. \quad (2.4)$$

Given a point $\mathbf{p}_n$ in frame n , we can express it in frame 1 as:

$$\mathbf{p}_1 = \begin{bmatrix} p_x^1 \\ p_y^1 \\ 1 \end{bmatrix} = \mathbf{H}_2^1 \mathbf{H}_3^2 \cdots \mathbf{H}_n^{n-1} \mathbf{p}_n = \mathbf{H}_n^1 \mathbf{p}_n. \quad (2.5)$$

2.3 Control

2.3.1 State-Space representation

A way to express a n 'th order ordinary differential equation (ODE) is to express it as a system of n first order ODEs. This is called the *state-space representation* of the system. A state-space representation commonly used in control theory for linear time-invariant (LTI) systems is the following:

$$\begin{aligned} \dot{\mathbf{x}}(t) &= \mathbf{A}\mathbf{x}(t) + \mathbf{B}\mathbf{u}(t) + \mathbf{d}(t), & \mathbf{x}(t) &\in \mathbb{R}^n, & \mathbf{u}(t) &\in \mathbb{R}^m, & \mathbf{y}(t) &\in \mathbb{R}^p, & \mathbf{d}(t) &\in \mathbb{R}^n, \\ \mathbf{y}(t) &= \mathbf{C}\mathbf{x}(t), & \mathbf{A} &\in \mathbb{R}^{n \times n}, & \mathbf{B} &\in \mathbb{R}^{n \times m}, & \mathbf{C} &\in \mathbb{R}^{p \times n}. \end{aligned} \quad (2.6)$$

Here, $\mathbf{x}(t)$ is the state vector, which contains all the information about the system at time t . $\mathbf{u}(t)$ is the input vector at time t . $\mathbf{y}(t)$ is the output vector, which contains all the measurements of the system at time t . $\mathbf{d}(t)$ is a disturbance vector.

2.3.2 Controllability

A system is said to be *controllable* if it is possible to drive the state of the system from any initial state to any desired final state in finite time, using an appropriate control input. For a LTI system, controllability can be determined by the rank of the controllability matrix $\mathcal{C}$, defined as:

$$\mathcal{C} = [\mathbf{B}, \mathbf{A}\mathbf{B}, \mathbf{A}^2\mathbf{B}, \dots, \mathbf{A}^{n-1}\mathbf{B}]. \quad (2.7)$$

If $\text{rank}(\mathcal{C}) = n$, where n is the dimension of the state vector $\mathbf{x}$, then the system is controllable.

2.3.3 MRAC

Model Reference Adaptive Control (MRAC) is a control strategy that aims to make the output of a system follow the output of a reference model, even in the presence of uncertainties or disturbances. The following definition of MRAC is based on Ioannou and Sun (2012, pp. 325–327).

Given the n th order LTI-system in state-space form,

$$\frac{d}{dt}\mathbf{x}(t) = \mathbf{A}\mathbf{x}(t) + \mathbf{B}\mathbf{u}(t), \quad \mathbf{x}(t) \in \mathbb{R}^n, \mathbf{u}(t) \in \mathbb{R}^m, \quad (2.8)$$

and the reference model,

$$\frac{d}{dt}\mathbf{x}_m(t) = \mathbf{A}_m\mathbf{x}_m(t) + \mathbf{B}_m\mathbf{r}(t), \quad \mathbf{x}_m(t) \in \mathbb{R}^n, \mathbf{r}(t) \in \mathbb{R}^m. \quad (2.9)$$

The reference model and input $\mathbf{r}(t)$ are chosen so that $\mathbf{x}_m(t)$ represents the desired trajectory that $\mathbf{x}(t)$ should follow. Crucially, $\mathbf{A}_m$ must be a stable matrix, and $(\mathbf{A}, \mathbf{B})$ must be *controllable* for this to work. If matrices $\mathbf{A}$ and $\mathbf{B}$ are known, then the control input $\mathbf{u}(t)$ can be designed as follows:

$$\mathbf{u}(t) = -\mathbf{K}^*\mathbf{x}(t) + \mathbf{L}^*\mathbf{r}(t), \quad \mathbf{K}^* \in \mathbb{R}^{m \times n}, \mathbf{L}^* \in \mathbb{R}^{m \times m}. \quad (2.10)$$

This obtains the closed loop system:

$$\frac{d}{dt}\mathbf{x}(t) = (\mathbf{A} - \mathbf{B}\mathbf{K}^*)\mathbf{x}(t) + \mathbf{B}\mathbf{L}^*\mathbf{r}(t). \quad (2.11)$$

If we choose $\mathbf{K}^*$ and $\mathbf{L}^*$ such that,

$$\mathbf{A} - \mathbf{B}\mathbf{K}^* = \mathbf{A}_m, \quad \mathbf{B}\mathbf{L}^* = \mathbf{B}_m, \quad (2.12)$$

then the closed loop system becomes:

$$\frac{d}{dt}\mathbf{x}(t) = \mathbf{A}_m\mathbf{x}(t) + \mathbf{B}_m\mathbf{r}(t). \quad (2.13)$$

Hence the closed-loop dynamics of $\mathbf{x}(t)$ is the same to Equation (2.9), and $\mathbf{x}(t) \rightarrow \mathbf{x}_m(t)$ exponentially fast. But for most cases, $\mathbf{A}$ and $\mathbf{B}$ are not known, which means that $\mathbf{K}^*$ and $\mathbf{L}^*$ has to be estimated online. Assuming that $\mathbf{K}^*$ and $\mathbf{L}^*$ exist, we'll change the input in Equation (2.10) to:

$$\mathbf{u}(t) = -\mathbf{K}(t)\mathbf{x}(t) + \mathbf{L}(t)\mathbf{r}(t), \quad \mathbf{K}(t) \in \mathbb{R}^{m \times n}, \mathbf{L}(t) \in \mathbb{R}^{m \times m}. \quad (2.14)$$

Adaptive Law

Defining the tracking error $\mathbf{e}(t)$ as:

$$\mathbf{e}(t) = \mathbf{x}(t) - \mathbf{x}_m(t). \quad (2.15)$$

Solving for $\mathbf{P}$ for a $\mathbf{Q} = \mathbf{Q}^T > 0$ in the Lyapunov equation:

$$\mathbf{A}_m^T \mathbf{P} + \mathbf{P} \mathbf{A}_m = -\mathbf{Q}, \quad (2.16)$$

we have the adaptive law:

$$\begin{aligned}\dot{\mathbf{K}}(t) &= \mathbf{B}_m^T \mathbf{P} \mathbf{e} \mathbf{x}^T \operatorname{sgn}(l), \\ \dot{\mathbf{L}}(t) &= -\mathbf{B}_m^T \mathbf{P} \mathbf{e} \mathbf{r}^T \operatorname{sgn}(l).\end{aligned}\tag{2.17}$$

Ioannou and Sun, [2012](#) proves that with this adaptive law, that $\mathbf{K}(t)$, $\mathbf{L}(t)$, and $\mathbf{e}(t)$ are bounded, and the tracking error $\mathbf{e}(t) \rightarrow 0$ as $t \rightarrow \infty$.

Chapter 3

Modelling

3.1 Finger model

For modelling the finger, we're assuming that the motion is limited to a 2D-plane. This is mostly true, due to the collateral ligaments at the DIP- and the PIP-joint, preventing excessive side-to-side bending, as discussed in Section 2.1.3. The MCP joint doesn't have the same support-structure, so it's free to move side to side, but this isn't as relevant to model for the task at hand, as the lateral movement from the cable pulling on the finger is minimal.

For our model, we assume that the finger is composed of three links, with three revolute joints, like a *planar manipulator* (**Reference to theory: planar manipulator**). To model the stiffness from the tendons and ligaments, we'll add a torsional spring at each joint. The springs will have a non-zero equilibrium angle, representing the natural resting position of the finger joints. The damping from the soft tissue will be modeled by torsional dampers. A schematic of the model can be seen in Figure 3.1. We'll model the links as rigid cylinders, with uniform mass distribution, and the joints as ideal revolute joints, with no friction. The parameters of the model are listed in Figure 3.2.

To model the dynamics of the finger, we'll use the Euler-Lagrange equations as shown in (**Add reference to theory: Euler-Lagrange Equations**). We'll define our generalized coordinates as the relative joint angles, φ_{MCP} , φ_{PIP} and φ_{DIP} :

$$\mathbf{q} \triangleq \begin{bmatrix} \varphi_{\text{MCP}} \\ \varphi_{\text{PIP}} \\ \varphi_{\text{DIP}} \end{bmatrix} \implies \dot{\mathbf{q}} = \begin{bmatrix} \dot{\varphi}_{\text{MCP}} \\ \dot{\varphi}_{\text{PIP}} \\ \dot{\varphi}_{\text{DIP}} \end{bmatrix} \implies \ddot{\mathbf{q}} = \begin{bmatrix} \ddot{\varphi}_{\text{MCP}} \\ \ddot{\varphi}_{\text{PIP}} \\ \ddot{\varphi}_{\text{DIP}} \end{bmatrix}. \quad (3.1)$$

To derive the equations of motion, we need to define the kinetic energy, T , and the potential energy, V of our system.

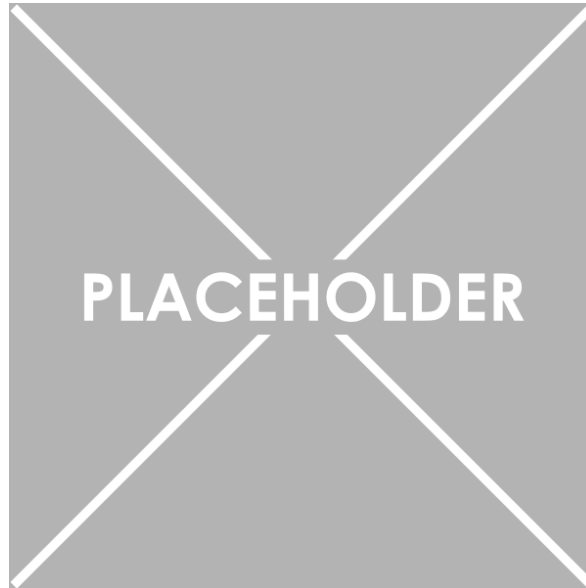


Figure 3.1: Schematic of the finger model, with three revolute joints, torsional springs and dampers.

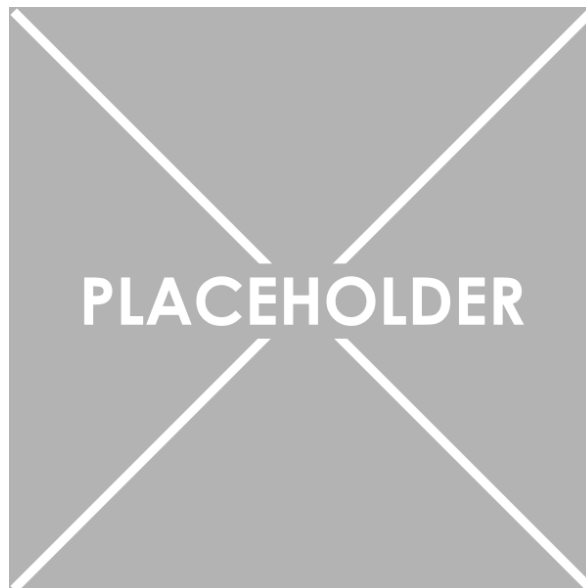


Figure 3.2: Table of model parameters.

3.1.1 Kinetic energy

The kinetic energy will be the sum of the kinetic energy of each link, which can be decomposed into the rotational and translational kinetic energy, defined as:

$$T_{\text{tot}} = T_{\text{rot}} + T_{\text{trans}}. \quad (3.2)$$

Rotational kinetic energy

The rotational kinetic energy of the system is rather straightforward to derive, as the angular velocity of each link is equal to the time derivative of the joint angle. Since the angles are relative, the total angular velocity of each link is the sum of the time derivatives of the joint angles up to that link. Hence, the rotational kinetic energy can be expressed as:

$$T_{\text{rot}} = \frac{1}{2}J_{\text{MCP}}\dot{\varphi}_{\text{MCP}}^2 + \frac{1}{2}J_{\text{PIP}}(\dot{\varphi}_{\text{MCP}} + \dot{\varphi}_{\text{PIP}})^2 + \frac{1}{2}J_{\text{DIP}}(\dot{\varphi}_{\text{MCP}} + \dot{\varphi}_{\text{PIP}} + \dot{\varphi}_{\text{DIP}})^2. \quad (3.3)$$

Translational kinetic energy

The translational kinetic energy is a bit more complex to derive, as the linear velocity of each link depends on the geometry of the system. The linear velocity of each link can be derived by finding the position of the center of mass of each link and taking the time derivative. To find the position of the center of mass, we'll use homogenous transformations, as described in Section 2.2.1.

Let's start by defining frames for moving between the links. We'll define the static world frame as frame i , attached to the MCP joint, where the x-axis is alligned with the metacarpal. The next is frame PP , attached to the PIP joint, where the x-axis is alligned with the proximal phalanx. Subsequently we have frame MP , attached to the DIP joint, where the x-axis is alligned with the middle phalanx. Finally, we have frame DP , attached to the tip of the finger, where the x-axis is alligned with the distal phalanx. The frames are shown in Figure 3.3. The homogenous transformations between these frames can be expressed as:

$$\begin{aligned} \mathbf{H}_{PP}^i &= \begin{bmatrix} \mathbf{R}(\varphi_{\text{MCP}}) & \mathbf{R}(\varphi_{\text{MCP}})\mathbf{e}_1l_{\text{PP}} \\ \mathbf{0}_{1 \times 2} & 1 \end{bmatrix}, \\ \mathbf{H}_{MP}^{PP} &= \begin{bmatrix} \mathbf{R}(\varphi_{\text{PIP}}) & \mathbf{R}(\varphi_{\text{PIP}})\mathbf{e}_1l_{\text{MP}} \\ \mathbf{0}_{1 \times 2} & 1 \end{bmatrix}, \\ \mathbf{H}_{DP}^{MP} &= \begin{bmatrix} \mathbf{R}(\varphi_{\text{DIP}}) & \mathbf{R}(\varphi_{\text{DIP}})\mathbf{e}_1l_{\text{DP}} \\ \mathbf{0}_{1 \times 2} & 1 \end{bmatrix}. \end{aligned} \quad (3.4)$$



Figure 3.3: Schematic of the homogenous transformation frames.

Assuming the the center of mass of each link is located at the midpoint of the link, we can express the position of the center of mass of each link in the world frame as:

$$\begin{aligned}
 \mathbf{p}_{PP,CM}^i &= \mathbf{H}_{PP}^i \begin{bmatrix} -l_{PP}/2 \\ 0 \\ 1 \end{bmatrix}, \\
 \mathbf{p}_{MP,CM}^i &= \mathbf{H}_{PP}^i \mathbf{H}_{MP}^{PP} \begin{bmatrix} -l_{MP}/2 \\ 0 \\ 1 \end{bmatrix}, \\
 \mathbf{p}_{DP,CM}^i &= \mathbf{H}_{PP}^i \mathbf{H}_{MP}^{PP} \mathbf{H}_{DP}^{MP} \begin{bmatrix} -l_{DP}/2 \\ 0 \\ 1 \end{bmatrix}.
 \end{aligned} \tag{3.5}$$

Extracting the x and y components of the position, defining them as $\mathbf{r}_{PP,CM}$, $\mathbf{r}_{MP,CM}$, and $\mathbf{r}_{DP,CM}$, we can take the time derivative to find the linear velocity of each center of mass, which can then be used to calculate the translational kinetic energy as:

$$T_{\text{trans}} = \frac{1}{2} \left[m_{PP} \dot{\mathbf{r}}_{PP,CM}^T \dot{\mathbf{r}}_{PP,CM} + m_{MP} \dot{\mathbf{r}}_{MP,CM}^T \dot{\mathbf{r}}_{MP,CM} + m_{DP} \dot{\mathbf{r}}_{DP,CM}^T \dot{\mathbf{r}}_{DP,CM} \right]. \tag{3.6}$$

3.1.2 Potential energy

For the potential energy one would normally consider the gravitational potential energy. However, since the finger is relatively light and the motion during gripping tasks is mostly in the horizontal plane, we'll omit the gravitational potential energy for simplicity. Also, for clarity we'll model the torsional springs as generalized forces,

instead of including them in the potential energy. Hence, the potential energy of the system can be expressed as:

$$V = 0. \quad (3.7)$$

3.1.3 Generalized forces

The generalized forces in our system will be the torques from the torsional springs and dampers, aswell as the torques from the cable pulling on the finger, and other external torques when the finger interacts with objects. The torques from the torsional springs can be expressed as:

$$\begin{aligned} \boldsymbol{\tau}_{\text{spring}} &= \begin{bmatrix} k_{\text{MCP}}(\varphi_{\text{MCP}} - \varphi_{\text{MCP,eq}}) \\ k_{\text{PIP}}(\varphi_{\text{PIP}} - \varphi_{\text{PIP,eq}}) \\ k_{\text{DIP}}(\varphi_{\text{DIP}} - \varphi_{\text{DIP,eq}}) \end{bmatrix} = \mathbf{K}(\mathbf{q} - \mathbf{q}_{\text{eq}}) \\ \mathbf{K} &\triangleq \begin{bmatrix} k_{\text{MCP}} & 0 & 0 \\ 0 & k_{\text{PIP}} & 0 \\ 0 & 0 & k_{\text{DIP}} \end{bmatrix}, \quad \mathbf{q}_{\text{eq}} \triangleq \begin{bmatrix} \varphi_{\text{MCP,eq}} \\ \varphi_{\text{PIP,eq}} \\ \varphi_{\text{DIP,eq}} \end{bmatrix}. \end{aligned} \quad (3.8)$$

The torques from the torsional dampers can be expressed as:

$$\boldsymbol{\tau}_{\text{damper}} = \begin{bmatrix} b_{\text{MCP}}\dot{\varphi}_{\text{MCP}} \\ b_{\text{PIP}}\dot{\varphi}_{\text{PIP}} \\ b_{\text{DIP}}\dot{\varphi}_{\text{DIP}} \end{bmatrix} = \mathbf{B}\dot{\mathbf{q}}, \quad \mathbf{B} \triangleq \begin{bmatrix} b_{\text{MCP}} & 0 & 0 \\ 0 & b_{\text{PIP}} & 0 \\ 0 & 0 & b_{\text{DIP}} \end{bmatrix}. \quad (3.9)$$

The total generalized forces can then be expressed as:

$$\boldsymbol{\tau} = \boldsymbol{\tau}_{\text{ext}} + \boldsymbol{\tau}_{\text{cable}} - \boldsymbol{\tau}_{\text{spring}} - \boldsymbol{\tau}_{\text{damper}}. \quad (3.10)$$

3.1.4 Rigid-body dynamics

For rigid-body mechanical systems, like the one we're modelling, the Euler-Lagrange equations can be expressed in matrix form as (**Add reference to theory: Rigid-body dynamics**):

$$\mathbf{M}(\mathbf{q})\ddot{\mathbf{q}} + \mathbf{C}(\mathbf{q}, \dot{\mathbf{q}})\dot{\mathbf{q}} + \mathbf{G}(\mathbf{q}) = \boldsymbol{\tau}. \quad (3.11)$$

The *inertia matrix* $\mathbf{M}(\mathbf{q})$ is a symmetric positive-definite matrix that represents the mass distribution of the system. We'll define $\varphi_{\text{MCP}} \triangleq \varphi_1$, $\varphi_{\text{PIP}} \triangleq \varphi_2$, and $\varphi_{\text{DIP}} \triangleq \varphi_3$, the cumulative angles $\varphi_{12} \triangleq \varphi_1 + \varphi_2$, $\varphi_{23} \triangleq \varphi_2 + \varphi_3$, and the shorthand form $c_\varphi \triangleq \cos(\varphi)$, $s_\varphi \triangleq \sin(\varphi)$. Based on the E.L.-equations the inertia matrix in our system then equates to:

$$\mathbf{M}(\mathbf{q}) = \begin{bmatrix} p_1 + p_2 c_{\varphi_2} + p_3 c_{\varphi_{23}} + p_4 c_{\varphi_3} & p_4 c_{\varphi_3} + p_5 + p_6 c_{\varphi_2} + p_7 c_{\varphi_{23}} & p_7 c_{\varphi_{23}} + p_8 + p_9 c_{\varphi_3} \\ p_4 c_{\varphi_3} + p_5 + p_6 c_{\varphi_2} + p_7 c_{\varphi_{23}} & p_4 c_{\varphi_3} + p_5 & p_8 + p_9 c_{\varphi_3} \\ p_7 c_{\varphi_{23}} + p_8 + p_9 c_{\varphi_3} & p_8 + p_9 c_{\varphi_3} & p_8 \end{bmatrix}, \quad (3.12)$$

where the different p_i 's are shown in Table 3.1. The *coriolis and centrifugal matrix* $\mathbf{C}(\mathbf{q}, \dot{\mathbf{q}})$ represents the coriolis and centrifugal forces that arise from the motion of the system. For our system, it equates to:

$$\mathbf{C}(\mathbf{q}, \dot{\mathbf{q}}) = \frac{1}{2} \begin{bmatrix} \gamma_{11} & \gamma_{12} & \gamma_{13} \\ \gamma_{21} & \gamma_{22} & \gamma_{23} \\ \gamma_{31} & \gamma_{32} & 0 \end{bmatrix}, \quad (3.13)$$

where

$$\begin{aligned} \gamma_{11} &= -p_2 \dot{\varphi}_2 s_{\varphi_2} - p_3 \dot{\varphi}_{2-3} s_{\varphi_{23}} - p_4 \dot{\varphi}_3 s_{\varphi_3}, \\ \gamma_{12} &= -(p_2 \dot{\varphi}_1 + 2p_6 \dot{\varphi}_2) s_{\varphi_2} - (p_3 \dot{\varphi}_1 + 2p_7 \dot{\varphi}_{2-3}) s_{\varphi_{23}} - p_4 \dot{\varphi}_3 s_{\varphi_3}, \\ \gamma_{13} &= -(p_3 \dot{\varphi}_1 + 2p_7 \dot{\varphi}_{2-3}) s_{\varphi_{23}} - (p_4 \dot{\varphi}_{1-2} + 2p_9 \dot{\varphi}_3) s_{\varphi_3}, \\ \gamma_{21} &= \dot{\varphi}_1 (p_2 s_{\varphi_2} + p_3 s_{\varphi_{23}}) - \dot{\varphi}_3 p_4 s_{\varphi_3}, \\ \gamma_{22} &= -\dot{\varphi}_3 p_4 s_{\varphi_3}, \\ \gamma_{23} &= -(p_4 \dot{\varphi}_{1-2} + 2p_9 \dot{\varphi}_3) s_{\varphi_3}, \\ \gamma_{31} &= \dot{\varphi}_1 p_3 s_{\varphi_{23}} + p_4 \dot{\varphi}_{1-2} s_{\varphi_3}, \\ \gamma_{32} &= p_4 \dot{\varphi}_{1-2} s_{\varphi_3}. \end{aligned}$$

The generalized forces $\boldsymbol{\tau}$ are the same as in Equation (3.10). The *gravity vector* $\mathbf{G}(\mathbf{q})$ represents the gravitational forces acting on the system. Since we're omitting the effects of gravity, the gravity vector is zero:

$$\mathbf{G}(\mathbf{q}) = \mathbf{0}. \quad (3.14)$$

Inserting all the results above, and solving for $\ddot{\mathbf{q}}$, we can express the equations of motion of our system as:

$$\ddot{\mathbf{q}} = \mathbf{M}(\mathbf{q})^{-1} [\boldsymbol{\tau}_{\text{ext}} + \boldsymbol{\tau}_{\text{cable}} - (\mathbf{C}(\mathbf{q}, \dot{\mathbf{q}}) + \mathbf{B}) \dot{\mathbf{q}} - \mathbf{K}(\mathbf{q} - \mathbf{q}_{\text{eq}})]. \quad (3.15)$$

Table 3.1: Constants in system matrices.

Constant	Value
p_1	$J_{MCP} + J_{PIP} + J_{DIP} + \frac{l_{PP}^2}{4}m_{PP} + \left(l_{PP}^2 + \frac{l_{MP}^2}{4}\right)m_{MP} + \left(l_{PP}^2 + l_{MP}^2 + \frac{l_{DP}^2}{4}\right)m_{DP}$
p_2	$l_{PP}l_{MP}(m_{MP} + 2m_{DP})$
p_3	$l_{PP}l_{DP}m_{DP}$
p_4	$l_{MP}l_{DP}m_{DP}$
p_5	$J_{PIP} + J_{DIP} + \frac{l_{MP}^2}{4}m_{MP} + \left(l_{MP}^2 + \frac{l_{DP}^2}{4}\right)m_{DP}$
p_6	$\frac{1}{2}l_{PP}l_{MP}(m_{MP} + 2m_{DP})$
p_7	$\frac{1}{2}l_{PP}l_{DP}m_{DP}$
p_8	$J_{DIP} + \frac{l_{DP}^2}{4}m_{DP}$
p_9	$\frac{1}{2}l_{MP}l_{DP}m_{DP}$

3.2 Brushed DC Motor model

In our system we're using a 12 V Brushed DC motor from Pololu ('Pololu - Brushed DC Motor', 2026). The dynamical model is based on Rahman and Mat Yahya, 2021. The circuit diagram of a brushed DC motor is shown in Figure 3.4. Equation (3.16) describes the mechanical dynamics of the motor, and Equation (3.17) describes the electrical dynamics of the motor, defined as:

$$J_m \frac{d^2\theta}{dt^2} + B_m \frac{d\theta}{dt} = \tau_m - \tau_l \quad (3.16)$$

$$R_a I_a + L_a \frac{dI_a}{dt} + E_b = E_a. \quad (3.17)$$

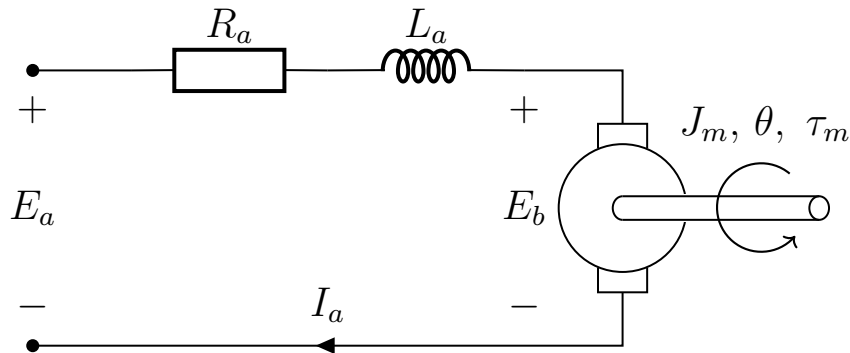


Figure 3.4: Circuit diagram of armature circuit of the DC motor model, with output torque and angular position.

Here, θ defines the angle of the motor. The torque generated by the motor is given by $\tau_m = K_t I_a$, where K_t is the torque constant of the motor. The load torque τ_l represents the torque exerted by the finger on the motor through the cable, as well as friction between the motor and the finger. The friction within the rotor of the motor is

modeled with $B_m \frac{d\theta}{dt}$, where B_m is a constant friction coefficient. The inertia of the rotor is given by J_m . The back electromotive force (EMF) is given by $E_b = K_b \frac{d\theta}{dt}$, where K_b is the back EMF constant of the motor. The armature voltage E_a is the control input to the system. R_a and L_a are the armature resistance and inductance, respectively. With the change to τ_m and E_b , we can rewrite the equations as:

$$J_m \frac{d^2\theta}{dt^2} + B_m \frac{d\theta}{dt} = K_t I_a - \tau_l \quad (3.18)$$

$$R_a I_a + L_a \frac{dI_a}{dt} + K_b \frac{d\theta}{dt} = E_a. \quad (3.19)$$

3.2.1 Estimating motor parameters

To estimate the parameters of the motor, we will use the datasheet from the manufacturer ('Pololu 25D Metal Gearmotors', 2021). Relevant information extracted from the datasheet is shown in Table 3.2. Considering the motor at stall, we have $I_a = I_{a,stall}$ and $\tau_l = \tau_{l,stall}$. In addition we have $\frac{d\theta}{dt} \equiv 0$, and at stationarity, $\frac{dI_a}{dt} \equiv 0$. This allows us to rewrite Equation (3.19) as:

$$R_a I_{a,stall} = E_a \implies R_a = \frac{E_a}{I_{a,stall}} \approx 2.44 \Omega. \quad (3.20)$$

Further, when the motor is stalled, we should expect the torque generated by the motor to equal the stall torque, giving us:

$$K_t I_{a,stall} = \tau_{l,stall} \implies K_t = \frac{\tau_{l,stall}}{I_{a,stall}} \approx 0.44 \text{ N m A}^{-1}. \quad (3.21)$$

For the case when the motor is running at no-load speed, we have $I_a = I_{a,nl}$ and $\frac{d\theta}{dt} = \omega_{nl}$, and at stationarity, $\frac{dI_a}{dt} \equiv 0$. This allows us to rewrite Equation (3.19) as:

$$R_a I_{a,nl} + K_b \omega_{nl} = E_a \implies K_b = \frac{E_a - R_a I_{a,nl}}{\omega_{nl}} \approx 0.845 \text{ V s rad}^{-1}. \quad (3.22)$$

Further, at no-load speed, we have $\tau_l \equiv 0$, and $\frac{d^2\theta}{dt^2} \equiv 0$. This allows us to rewrite Equation (3.18) as:

$$B_m \omega_{nl} = K_t I_{a,nl} \implies B_m = \frac{K_t I_{a,nl}}{\omega_{nl}} \approx 6.47 \text{ mN m s rad}^{-1}. \quad (3.23)$$

Sadly it's not possible to estimate the inertia of the rotor J_m , nor the armature inductance L_a from the datasheet. For simulation purposes, the parameters are chosen as $J_m = 0.093 \text{ kg m}^2$ and $L_a = 6 \text{ mH}$, reported as example brushed DC motor values by Rahman and Mat Yahya (2021). Even though the values are currently unknown, they can be estimated through a calibration step later. One way that's possibly the most

Table 3.2: Relevant motor parameters extracted from the datasheet of the motor.

Parameter	Symbol	Value
Armature Voltage	E_a	12 V
Stall Torque	$\tau_{l, stall}$	2.158 N m
Stall Current	$I_{a, stall}$	4.9 A
No-load Speed	ω_{nl}	13.61 rad/sec
No-load Current	$I_{a, nl}$	0.20 A

convenient, is to use a parameter identification method.

3.2.2 Estimating the armature inductance and rotor inertia

To estimate the armature inductance and rotor inertia, we can use a parameter identification method. We'll start by converting Equation (3.19) to the Laplace domain, giving us:

$$E_a(s) = (L_a s + R_a)I_a(s) + K_b s\theta(s). \quad (3.24)$$

Since we only measure $I_a(t)$ and not its derivative, we have to apply a proper filter of order 1, defined as:

$$\Lambda_{I_a}(s) = s + \lambda_0, \quad \lambda_0 > 0. \quad (3.25)$$

Applying the filter to Equation (3.24) gives us:

$$\frac{1}{\Lambda_{I_a}(s)}E_a(s) = \frac{1}{\Lambda_{I_a}(s)}(L_a s + R_a)I_a(s) + \frac{1}{\Lambda_{I_a}(s)}K_b s\theta(s).$$

Ordering it around, moving all measured signals and known parameters to the left, and all factors with the unknown parameter L_a to the right, we get:

$$\underbrace{\frac{1}{\Lambda_{I_a}(s)}[E_a(s)] - \frac{1}{\Lambda_{I_a}(s)}[R_a I_a(s)] - \frac{s}{\Lambda_{I_a}(s)}[K_b \theta(s)]}_{z_{L_a}} = \underbrace{\frac{s}{\Lambda_{I_a}(s)}[I_a(s)]}_{\Phi_{L_a}} \underbrace{L_a}_{\theta_{L_a}^*} \quad (3.26)$$

$$\implies z_{L_a} = \theta_{L_a}^* \Phi_{L_a}.$$

Hence we've transformed the system to a SPM like discussed in [**Add reference to Theory:SPM**]. We can do the same for the inertia of the rotor J_m . We'll start by converting Equation (3.18) to the Laplace domain, assuming there is no external load ($\tau_l \equiv 0$), giving us:

$$(J_m s^2 + B_m s)\theta(s) = K_t I_a(s). \quad (3.27)$$

Since we're only measuring $\theta(t)$ and not its derivatives, we have to apply a proper filter of order 2, defined as:

$$\Lambda_\theta(s) = s^2 + \lambda_1 s + \lambda_0, \quad \lambda_0, \lambda_1 > 0. \quad (3.28)$$

Applying the filter to Equation (3.27), moving all measured signals and known parameters to the left, and all factors with the unknown parameter J_m to the right, we get:

$$\underbrace{\frac{1}{\Lambda_\theta(s)}[K_t I_a(s)] - \frac{s}{\Lambda_\theta(s)}[B_m \theta(s)]}_{z_{J_m}} = \underbrace{\frac{s^2}{\Lambda_\theta(s)}[\theta(s)]}_{\Phi_{J_m}} \underbrace{J_m}_{\theta_{J_m}^*}. \quad (3.29)$$

$$\implies z_{J_m} = \theta_{J_m}^* \Phi_{J_m}.$$

Combining Equation (3.26) and Equation (3.29), we can express them both in SPM form as:

$$\underbrace{\begin{bmatrix} z_{L_a} \\ z_{J_m} \end{bmatrix}}_{\mathbf{z}} = \underbrace{\begin{bmatrix} L_a & J_m \end{bmatrix}}_{\boldsymbol{\theta}^{*\top}} \underbrace{\begin{bmatrix} \Phi_{L_a} \\ \Phi_{J_m} \end{bmatrix}}_{\boldsymbol{\Phi}}. \quad (3.30)$$

$$\implies \mathbf{z} = \boldsymbol{\theta}^{*\top} \boldsymbol{\Phi}.$$

Using the gradient method developed in [Add reference to Theory: Gradient method], with

$$\lambda_{0,L_a} = 10, \quad \lambda_{0,J_m} = 0.1, \quad \lambda_{1,J_m} = 0.1, \quad \boldsymbol{\Gamma} = \begin{bmatrix} 10 & 0 \\ 0 & 1000 \end{bmatrix},$$

$$\hat{\boldsymbol{\theta}}_0 = \begin{bmatrix} \hat{L}_a(0) \\ \hat{J}_m(0) \end{bmatrix} = \begin{bmatrix} 1 \text{ mH} \\ 0.01 \text{ kg m}^2 \end{bmatrix}, \quad \boldsymbol{\theta}^* = \begin{bmatrix} L_a \\ J_m \end{bmatrix} = \begin{bmatrix} 6 \text{ mH} \\ 0.093 \text{ kg m}^2 \end{bmatrix},$$

while applying a step input $E_a = 12 \text{ V}$ at $t = 50 \text{ ms}$, the resulting estimates of $\hat{L}_a(t)$ and $\hat{J}_m(t)$ are shown in Section 3.2.2. It is clear that the estimates converge exponentially fast to the true values. Since these are static parameters that only needs to be estimated once, L_a and J_m will be assumed known for further controller design.

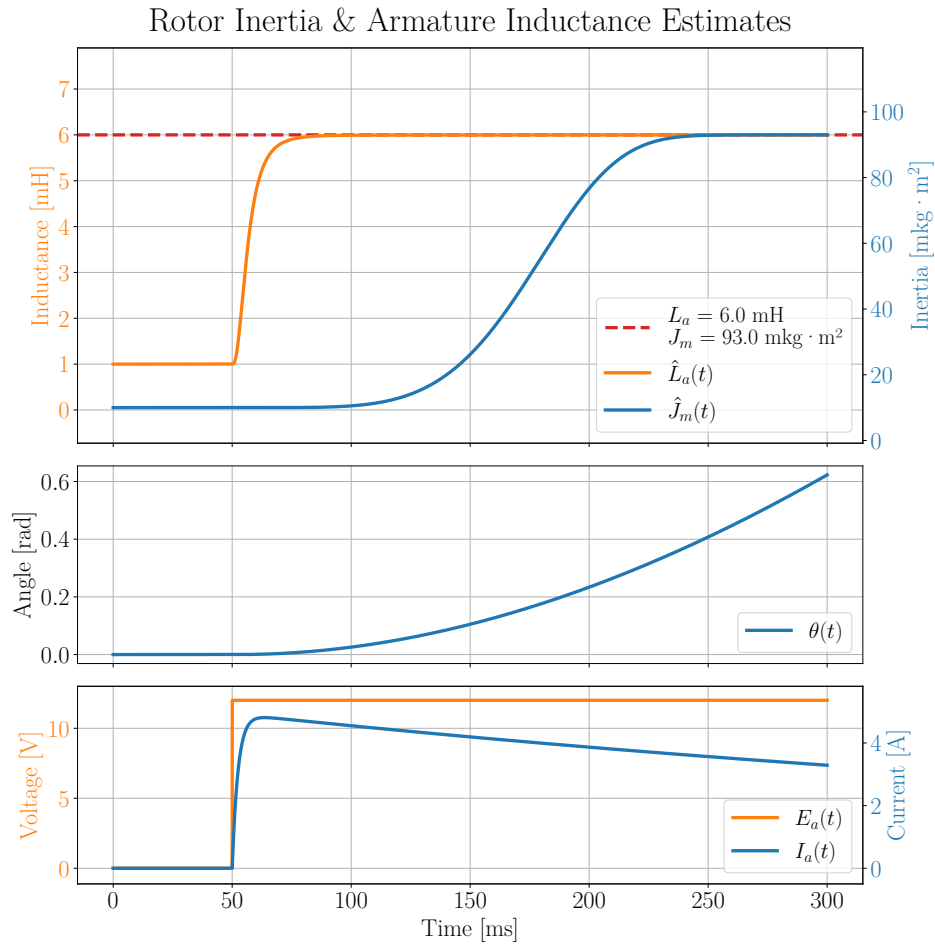


Figure 3.5: Parameter identification of the armature inductance L_a and rotor inertia J_m using a step input in the armature voltage E_a .

3.2.3 Mass-spring-damper load

In Section 3.1 we assumed that the finger could be modelled as several torsional mass-spring-damper systems. Since we can't measure the finger-angles, in addition to that the configuration of the whiffle tree is unknown, the full finger model isn't observable, and can't be used for position control design. Instead, we'll assume that finger can be modelled as a single mass-spring-damper system, acting on the motor as τ_l . This is a simplification, but it allows for a better analysis of the system. Hence we'll model the load torque τ_l as:

$$\tau_l = J \frac{d^2\theta}{dt^2} + c \frac{d\theta}{dt} + k(\theta - \theta_{eq}), \quad (3.31)$$

where J is the 'total' inertia of the finger, c is the 'total' damping coefficient of the finger, k is the 'total' stiffness of the finger, and θ_{eq} is a kind of equilibrium angle of the finger. Substituting this into Equation (3.18), we get the updated mechanical dynamics:

$$(J_m + J) \frac{d^2\theta}{dt^2} + (B_m + c) \frac{d\theta}{dt} + k\theta = K_t I_a + k\theta_{eq} \quad (3.32)$$

3.2.4 State-space model of brushed DC motor with load

To analyze the position controller for the motor with load, discussed further in Section 4.3, we need to express the dynamics in Equation (3.32) in state-space representation, as shown in Section 2.3.1. Assuming that I_a can be treated as an input, explained in Section 4.1, and defining $\omega \triangleq \frac{d\theta}{dt}$, we can rewrite the Equation (3.32) and as:

$$\frac{d\omega}{dt} = \frac{1}{J_m + J} (K_t I_a - (B_m + c)\omega - k(\theta - \theta_{eq})). \quad (3.33)$$

Written in state-space form, we have:

$$\begin{aligned} \underbrace{\frac{d}{dt} \begin{bmatrix} \theta \\ \omega \end{bmatrix}}_{\frac{d}{dt} \mathbf{x}} &= \underbrace{\begin{bmatrix} 0 & 1 \\ -\frac{k}{J_m+J} & -\frac{B_m+c}{J_m+J} \end{bmatrix}}_{\mathbf{A}} \underbrace{\begin{bmatrix} \theta \\ \omega \end{bmatrix}}_{\mathbf{x}} + \underbrace{\begin{bmatrix} 0 \\ \frac{K_t}{J_m+J} \end{bmatrix}}_{\mathbf{B}} \underbrace{I_a}_{\mathbf{u}} + \underbrace{\begin{bmatrix} 0 \\ \frac{k\theta_{eq}}{J_m+J} \end{bmatrix}}_{\mathbf{d}} \\ &\implies \frac{d}{dt} \mathbf{x} = \mathbf{Ax} + \mathbf{Bu} + \mathbf{d}. \end{aligned} \quad (3.34)$$

In addition we have an encoder measuring θ . Hence the output of the system is given by:

$$\begin{aligned} \underbrace{\begin{bmatrix} \theta \end{bmatrix}}_{\mathbf{y}} &= \underbrace{\begin{bmatrix} 1 & 0 \end{bmatrix}}_{\mathbf{C}} \underbrace{\begin{bmatrix} \theta \\ \omega \end{bmatrix}}_{\mathbf{x}} \\ &\implies \mathbf{y} = \mathbf{Cx}. \end{aligned} \quad (3.35)$$

Chapter 4

Controller design

4.1 Current controller

To help facilitate the design of the position and torque controllers, we will first design a controller for the armature current I_a with the armature voltage E_a . This will allow us to treat the armature current as a control input in the position control design, simplifying the dynamics significantly. As the dynamics of the armature current is so fast, the controller has to be as cheap as possible to compute. Hence, it will be designed as a simple proportional (P) controller, but with a feedforward (FF) term to account for the back EMF. Let's first consider the electrical dynamics of the motor from Equation (3.19):

$$L_a \frac{dI_a}{dt} + R_a I_a + K_b \frac{d\theta}{dt} = E_a. \quad (4.1)$$

Given the time varying reference current $r(t)$, we can design the input voltage $E_a(t)$ as:

$$E_a(t) = \underbrace{K_b \frac{d\theta(t)}{dt}}_{\text{Feedforward term}} + \underbrace{L_a K_p (r(t) - I_a(t))}_{\text{P controller}}. \quad (4.2)$$

Substituting Equation (4.2) into Equation (4.1), we get:

$$\frac{dI_a(t)}{dt} + R_a I_a(t) = K_p (r(t) - I_a(t)) \triangleq u(t). \quad (4.3)$$

This controller is supposed to be ran in real time on a microcontroller. That way it won't have access to continuous time signals, but rather discrete time signals. Hence, we will need to discretize the controller for stability analysis and tuning. For this analysis we will assume that the dynamics of the motor are slow enough such that the feedforward term can be treated as a constant. This is a reasonable assumption since the feedforward term is based on the angular velocity, which changes relatively slowly

compared to the armature current.

4.1.1 Discretization of current controller

Suppose the controller is ran with a update period of T_s . Assuming that the input voltage E_a is held constant between sampling times, i.e.,

$$u(t) = u[k] = K_p(r[k] - I_a[k]), \quad kT_s \leq t < (k+1)T_s, \quad (4.4)$$

the dynamics in Equation (4.3) then becomes:

$$\frac{dI_a(\tau)}{d\tau} + R_a I_a(\tau) = u[k], \quad \tau = t - kT_s \in [0, T_s]. \quad (4.5)$$

To solve it, let's multiply by the integrating factor $e^{R_a\tau}$, which gives:

$$e^{R_a\tau} \left[\frac{dI_a(\tau)}{d\tau} + R_a I_a(\tau) \right] = u[k] e^{R_a\tau}. \quad (4.6)$$

Notice how this can be rewritten as:

$$\frac{d}{d\tau} \left(e^{R_a\tau} I_a(\tau) \right) = u[k] e^{R_a\tau}. \quad (4.7)$$

Integrating both sides of Equation (4.7) with respect to τ , over the entire interval from 0 to T_s , we get the discretized dynamics of the current controller:

$$\begin{aligned} [e^{R_a\tau} I_a(\tau)]_{\tau=0}^{\tau=T_s} &= u[k] \int_0^{T_s} e^{R_a\tau} d\tau, \\ \implies e^{R_a T_s} \underbrace{I_a(T_s)}_{I_a[k+1]} - \underbrace{I_a(0)}_{I_a[k]} &= u[k] \frac{e^{R_a T_s} - 1}{R_a}, \\ \implies I_a[k+1] &= \underbrace{e^{-R_a T_s} I_a[k]}_{\triangleq a} + u[k] \underbrace{\frac{1 - e^{-R_a T_s}}{R_a}}_{\triangleq b}, \\ \implies I_a[k+1] &= a I_a[k] + b u[k]. \end{aligned} \quad (4.8)$$

Substituting in $u[k]$ from Equation (4.4), we get:

$$\begin{aligned} I_a[k+1] &= a I_a[k] + b K_p(r[k] - I_a[k]), \\ \implies I_a[k+1] &= (a - b K_p) I_a[k] + b K_p r[k]. \end{aligned} \quad (4.9)$$

4.1.2 Stability analysis and tuning of controller

To guarantee stability of the current controller, we can look at the z-transform of the system. Taking the z-transform of Equation (4.9), disregarding any initial conditions, we get:

$$\begin{aligned}
[z - (a - bK_p)] I_a(z) &= bK_p r(z), \\
\implies \frac{I_a(z)}{r(z)} &= \frac{bK_p}{z - (a - bK_p)}.
\end{aligned} \tag{4.10}$$

Clearly, Equation (4.10) has a pole at $z = a - bK_p$. As discussed in [ADD REFERENCE TO THEORY: DISCRETIZED SYSTEMS], for the system to be stable, we need the pole to be inside the unit circle. In other words, we need:

$$\begin{aligned}
|a - bK_p| < 1 &\implies \left| e^{-R_a T_s} - K_p \frac{1 - e^{-R_a T_s}}{R_a} \right| < 1, \\
\implies K_p &< R_a \frac{1 + e^{-R_a T_s}}{1 - e^{-R_a T_s}} \triangleq K_{p,\max}(T_s).
\end{aligned} \tag{4.11}$$

One downside to using a P controller is that there will be a steady-state error. To eliminate this, we can artificially give the controller a higher reference current. To do this we will need to know the steady-state value of the current for a given reference. Assuming we apply a step reference of $r[k] = r_0$ for all $k \geq 0$. Provided we choose a K_p that satisfies Equation (4.11), the recursion will converge, and as we let $t \rightarrow \infty \implies k \rightarrow \infty$, Equation (4.9) becomes:

$$\begin{aligned}
I_a[\infty] &= (a - bK_p)I_a[\infty] + bK_p r_0, \\
\implies I_a[\infty] &= r_0 \frac{bK_p}{1 - a + bK_p} = r_0 \frac{\frac{1-a}{R_a} K_p}{1 - a + \frac{1-a}{R_a} K_p} = r_0 \frac{K_p}{R_a + K_p}.
\end{aligned} \tag{4.12}$$

Hence to eliminate the steady-state error, we can choose the reference to be:

$$r_1 = \frac{R_a + K_p}{K_p} r_0 \implies I_a[\infty] = r_1 \frac{K_p}{R_a + K_p} = r_0. \tag{4.13}$$

4.1.3 Simulation of current controller

To evaluate the controller, we will simulate it applied to the motor model developed in Section 3.2. Using $K_p = \frac{1}{2}K_{p,\max}(T_s)$, where the reference current is a step input of 1 A, and scaled with regards to Equation (4.13). Additionally there is a saturation put on $E_a = \pm 12$ V. Figure 4.1 and Figure 4.2 shows a simulation of the P+FF controller aswell as just the P controller, with $T_s = 0.2$ ms, where the motor is initially spinning at $\omega_0 = 5 \text{ rad s}^{-1}$ and $\omega_0 = 0 \text{ rad s}^{-1}$, respectively. Figure 4.3 and Figure 4.4 shows the simulation of the P+FF controller with and without noise to the measurement of I_a , with $T_s = 0.2$ ms and $T_s = 1.0$ ms, respectively. The noise is a zero-mean Gaussian noise with a standard deviation of $\sigma_{I_a} = 50$ mA, which is higher than is expected for the system, but it will help us evaluate the robustness of the controller.

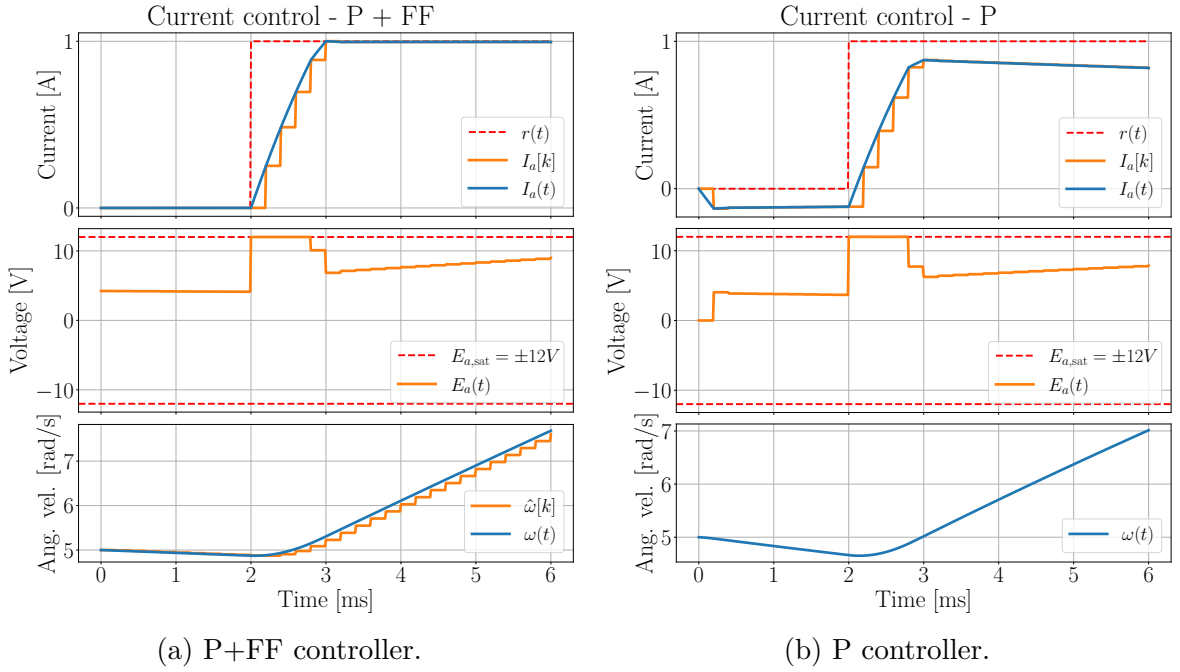


Figure 4.1: Armature current step response for discrete-time P+FF and P controllers tracking a 1 A reference, with $T_s = 0.2$ ms and initial motor speed $\omega_0 = 5$ rad s⁻¹.

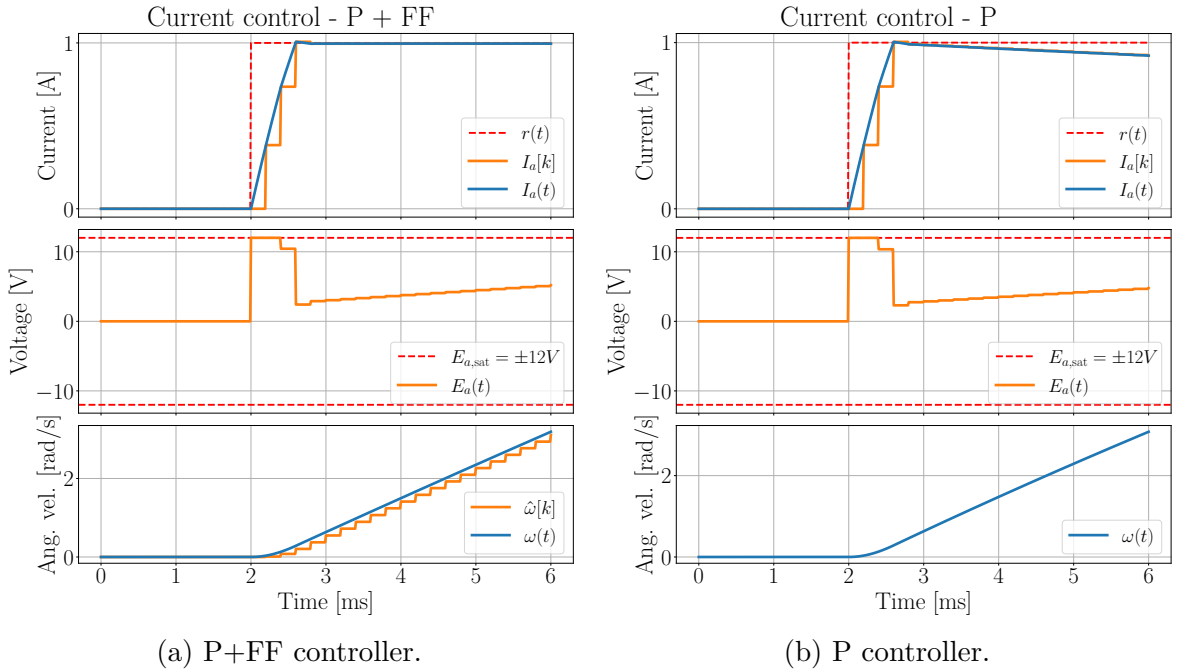


Figure 4.2: Armature current step response for discrete-time P+FF and P controllers tracking a 1 A reference, with $T_s = 0.2$ ms and initial motor speed $\omega_0 = 0$ rad s⁻¹.

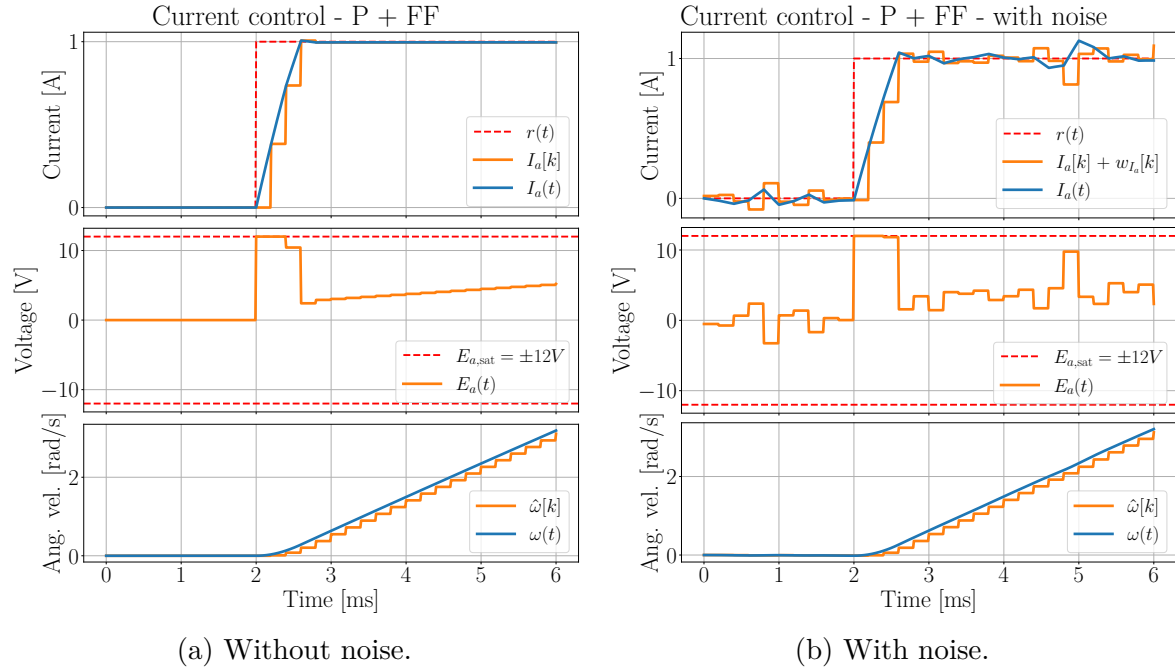


Figure 4.3: Effect of current measurement noise on the armature current response using a discrete-time P+FF controller with $T_s = 0.2$ ms.

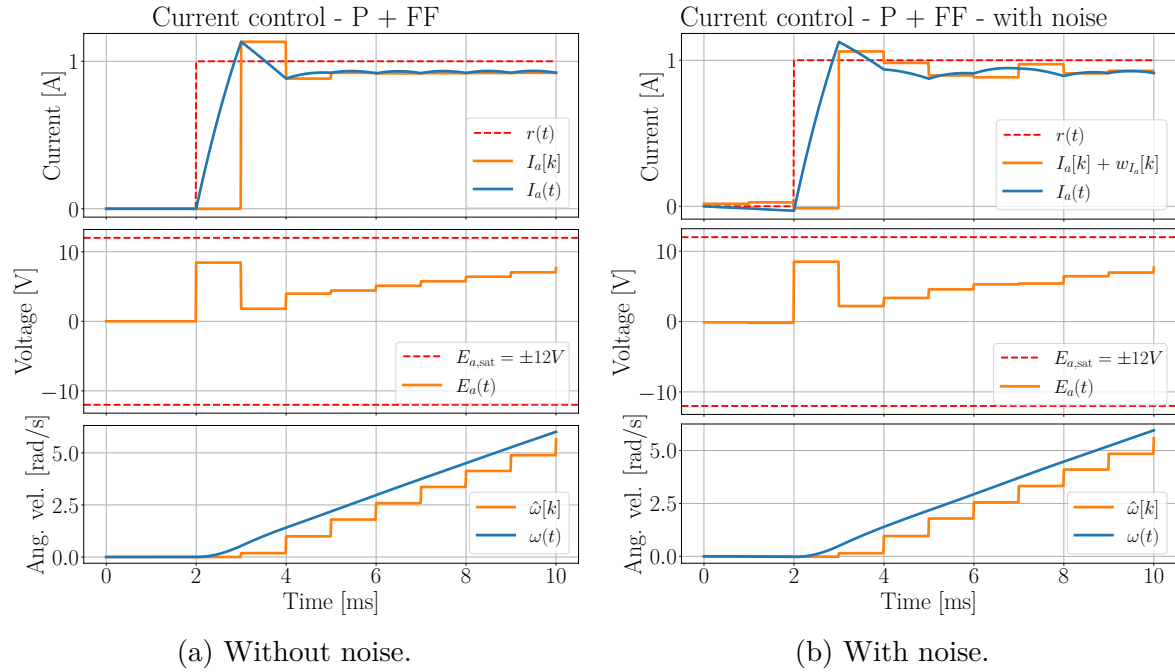


Figure 4.4: Effect of current measurement noise on the armature current response using a discrete-time P+FF controller with $T_s = 1.0$ ms.

4.1.4 Evaluation of controller

When the motor is starting from still, both the P+FF and P controllers are able to reach the target current fast. But as the motor picks up speed, the back-EMF becomes significant, and the P controller struggles to keep up, and the current starts to deviate from the reference current, as can be seen in Figure 4.2b. The P+FF controller on the other hand continues to perform well, as it can account for the back-EMF, as shown in Figure 4.2a. When the motor is already spinning at a high speeds, the differences between the two controllers becomes even more significant. At no point does the P controller reach its target current. In fact, it deviates more and more over time, as can be seen in Figure 4.1b. The P+FF controller on the other hand continues to perform well, as it can account for the back-EMF, as shown in Figure 4.1a.

As can be seen in Figure 4.3 and Figure 4.4, the added noise to the current measurements doesn't really affect the stability of the controller. The current oscillates slightly when there's noise present, compared to the noise-free. There is however a clear difference between longer and shorter update periods. With a longer update period of $T_s = 1.0\text{ ms}$, the current gets a slight steady-state-error, which is not present with the shorter update period of $T_s = 0.2\text{ ms}$. The reason for this is that the assumption of a constant speed between updates is less valid with a longer update period, which causes the feedforward term to be less accurate, which in turn causes the steady-state error. With a shorter update period, the assumption of a constant speed is more valid, which allows the feedforward term to be more accurate, which in turn allows the controller to track the reference current better.

Overall, the P+FF controller shows promising results for controlling the armature current in our system. Due to the saturation in the voltage of $E_a = \pm 12\text{ V}$, there is a maximum rate of change for the current. During simulation it was found to be $\dot{I}_{a_{\max}} \approx 2.0\text{ kA s}^{-1}$, when the motor was starting from still, which is more or less instantaneous seen from the dynamics of the mechanical system. Hence, we will treat the armature current as a control input for further control design.

4.2 Torque control

When the hand interacts with objects, trying to control the position of the hand becomes irrelevant, as the hand will be constrained by the object. Instead, we want to control the torque generated by the motor, which in turn will allow us to control the force applied to the object.

When grasping an object, assuming the object is rigid and that the cable is inelastic, the angular velocity and acceleration of the motor will be $\frac{d\theta}{dt} \equiv 0$ and $\frac{d^2\theta}{dt^2} \equiv 0$, respectively. Based on Equation (3.18), this results in the following relation:

$$\tau_m = K_t I_a = \tau_l. \quad (4.14)$$

Hence, all the torque generated by the motor, which is proportional to the current, would be applied to the load. This means the applied torque can be controlled directly through the current. In Section 4.1 we designed a controller for the armature current I_a through the input armature voltage E_a . With $\frac{d\theta}{dt} \equiv 0$, the back-EMF will be $K_b \frac{d\theta}{dt} \equiv 0$. Therefore we can also simplify the current controller in Equation (4.2) to just a P controller, as there is no back-EMF to account for. This will reduce the computational load on the microcontroller. For a given reference torque r_{τ_m} , we can calculate the reference current r_{I_a} as:

$$r_{I_a} = \frac{r_{\tau_m}}{K_t}. \quad (4.15)$$

If it's more convenient to control the force applied to the object instead of the torque, we can easily convert between the two using the relation $\tau_m = F_m r_{\text{spindle}}$, where r_{spindle} is the radius of the spindle mounted on the motor. Hence, for a given reference force r_F , we can calculate the reference current r_{I_a} as:

$$r_{I_a} = r_F \frac{r_{\text{spindle}}}{K_t}. \quad (4.16)$$

Figure 4.5 shows emulated scenarios of the finger grasping a rigid object, assuming no elasticity in the cable, and no friction between the motor and the finger. The motor is supplied with 3 V for the first 5 ms. Then at $t = 5$ ms, the finger makes contact with the object, and $\frac{d\theta}{dt} = \frac{d^2\theta}{dt^2} \equiv 0$. At the same time, the torque controller is activated, and the reference torque is set to $r_{\tau_m} = 1.5$ N m. For the current controller, the proportional gain is set to $K_p = \frac{1}{2} K_{p,max}$, like in Section 4.1.3. Figure 4.5a and Figure 4.5b show the results for $T_s = 0.2$ ms and $T_s = 1.0$ ms, respectively. As can be seen in the figures, the motor torque τ_m quickly converges to the reference torque r_{τ_m} for both cases.

Ideally, if there was no friction between the motor and the finger, $\tau_l = \tau_{\text{finger}}$. In reality, because of the bowden tube the cable is running through, and other inconsistencies in the setup, there will be some friction. Therefore, we can expect $\tau_l = \tau_{\text{finger}} + \tau_{\text{friction}}$, where τ_{friction} is the torque lost to friction. Hence, without any direct measurement of the applied force to the finger, we would expect that the applied force to the finger will be less than the reference force. However, with integrated force sensors in the fingertip, this wouldn't be an issue.

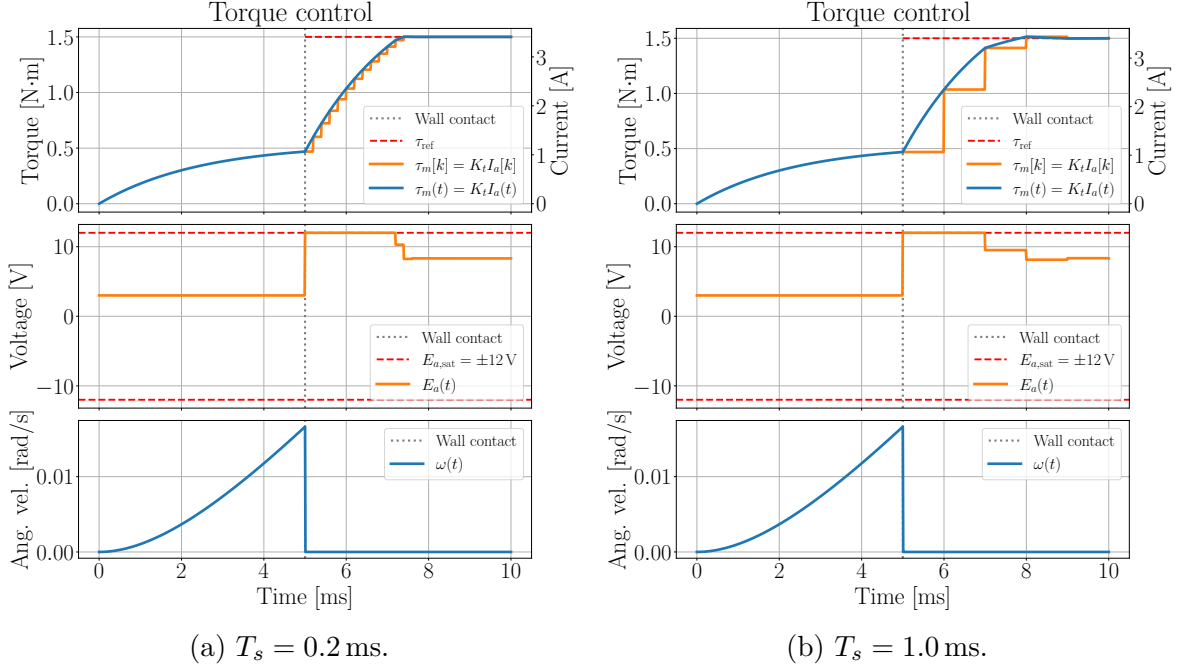


Figure 4.5: Torque control with a P controller when gripping a rigid object.

4.2.1 Force control with integrated fingertip force sensors

With integrated force sensors in the fingertip, we could use a cascade control approach. Since the motor torque and force are proportional to the armature current, we could then define the reference current r_{I_a} as a feedforward and PI controller with the reference force r_F and the measured force F_{meas} as input:

$$r_{I_a}(t) = \underbrace{\frac{r_F r_{\text{spindle}}}{K_t}}_{\text{Feedforward}} + \underbrace{K_p(r_F - F_{meas}(t)) + K_i \int_{t_0}^t (r_F - F_{meas}(\tau)) d\tau}_{\text{PI controller}}. \quad (4.17)$$

In our system, the cables are running through bowden tubes. This introduces a significant amount of friction. Therefore the original assumption in Equation (4.14) that all the torque generated by the motor is applied to the load, becomes invalid. Jeong and Cho, 2015 proposes the friction from cables going through bowden tubes to be proportional with the applied force. We then get the following relation:

$$F_{\text{finger}} = F_m (1 - \exp(-\mu\Phi)), \quad (4.18)$$

where μ is the friction coefficient, and Φ is the total wrap angle of the cable around the bowden tube. In theory one could include this in the feedforward term, but for the time being, I'll assume it to be unknown. For simulation purposes, I'll assume that $\exp(-\mu\Phi) \equiv 0.1$. This means that only 90% of the motor force is applied to the finger. Figure 4.6 shows the simulation of the force control with and without the integrated

fingertip force sensors, with $T_s = 0.2$ ms and $r_F = 100$ N. Here the controller parameters were chosen simply through repeated simulation, where $K_p = 0.001$ and $K_i = 8$. These will most likely have to be retuned in the actual system. As can be seen in Figure 4.6a, without the integrated fingertip force sensors, the applied force to the finger never reaches its target, as is expected due to the friction. With the integrated fingertip force sensors, as shown in Figure 4.6b, the applied force to the finger quickly converges to the reference force, despite the friction.

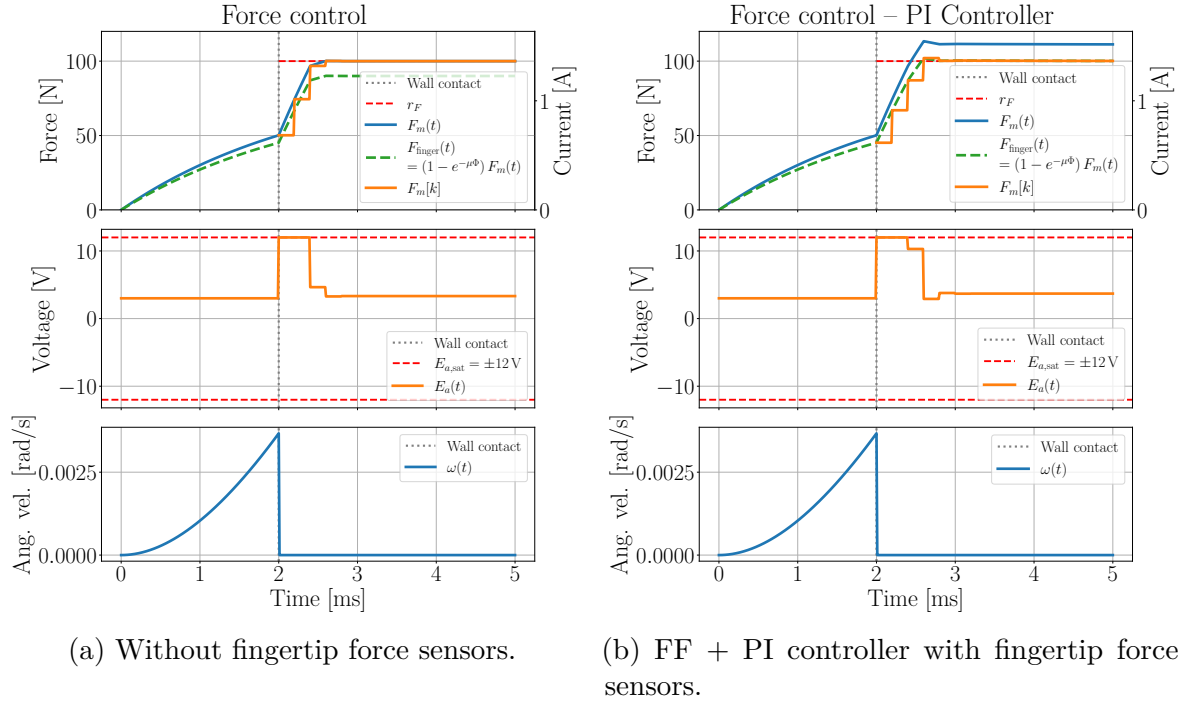


Figure 4.6: Force control with friction. With and without force sensors in fingertips. Both controllers have $T_s = 0.2$ ms.

4.3 Model reference adaptive control (MRAC) for position control

When the hand is not in contact with any objects, we want to control the position of the hand. However, due to the big differences in mass, stiffness and dampening in the hand between patients, it becomes difficult to design a controller that can guarantee good performance for all patients. To address this issue, we will implement a model reference adaptive control (MRAC) scheme, which will allow us to adapt the controller parameters online based on the observed behavior of the system. To be clear, this is mostly just to speed up the tuning process of the controller, and get good enough control for tests when frequently switching between patients. I would however recommend to use a simpler control approach if the system is to be used several times by the same

patient. This will be discussed in more detail in Chapter 5.

As discussed in Section 3.2.3, because of modelling uncertainties and the fact that we don't measure anything at the hand, the finger model from Section 3.1 becomes unobservable. Therefore controlling the angles of the fingers directly becomes infeasible. Instead we will focus on controlling the position of the motor precisely, as it's connected directly to the finger through a cable. For this we will use the MRAC scheme introduced in Section 2.3.3. It calls for the system to be controllable. Using the simplified model of the finger dynamics as a torsional mass-spring-damper system acting on the motor, from Section 3.2.4, we can check if the simplified system is controllable.

4.3.1 Controllability of the system

Based on the state-space representation our system in Section 3.2.4, we can check if the system is controllable, as described in Section 2.3.2. The controllability matrix $\mathcal{C}$ for our system is given by:

$$\mathcal{C} = [\mathbf{B}, \mathbf{AB}]. \quad (4.19)$$

Substituting for our specific $\mathbf{A}$ and $\mathbf{B}$, we get:

$$\mathcal{C} = \begin{bmatrix} 0 & \frac{K_t}{J_m+J} \\ \frac{K_t}{J_m+J} & -\frac{K_t(B_m+c)}{(J_m+J)^2} \end{bmatrix}. \quad (4.20)$$

Clearly, $\text{rank}(\mathcal{C}) = 2$, which is equal to the number of states. Therefore, the simplified system is controllable.

4.3.2 MRAC implementation

The MRAC scheme that will be implemented is based on Section 2.3.3. In our physical model of the system, we will use the finger model developed in Section 3.1, connected to the brushed DC motor as a load, through a cable connected to a whiffle tree to spread the force to all three phalanges. From the motor side, the dynamics can be described through the state-space representation:

$$\underbrace{\frac{d}{dt} \begin{bmatrix} \theta \\ \omega \end{bmatrix}}_{\dot{\mathbf{x}}} = \underbrace{\begin{bmatrix} 0 & 1 \\ 0 & -\frac{B_m}{J_m} \end{bmatrix}}_{\mathbf{A}} \underbrace{\begin{bmatrix} \theta \\ \omega \end{bmatrix}}_{\mathbf{x}} + \underbrace{\begin{bmatrix} 0 \\ \frac{K_t}{J_m} \end{bmatrix}}_{\mathbf{B}} \underbrace{I_a}_u + \underbrace{\begin{bmatrix} 0 \\ \frac{\tau_l}{J_m} \end{bmatrix}}_{\mathbf{d}}, \quad y(t) = \underbrace{\begin{bmatrix} 1 & 0 \end{bmatrix}}_{\mathbf{C}} \underbrace{\begin{bmatrix} \theta \\ \omega \end{bmatrix}}_{\mathbf{x}}, \quad (4.21)$$

where θ is the angle of the motor, ω is the angular velocity of the motor, I_a is the armature current, and τ_l is the load torque applied to the motor by the finger. The output $y(t)$ is the angle of the motor, which we want to control. The MRAC scheme

calls for a reference model, which the system should follow as closely as possible. Since our system is a second-order system, we will use a second-order reference model, in the standard form:

$$\underbrace{\frac{d}{dt} \begin{bmatrix} \theta_m \\ \omega_m \end{bmatrix}}_{\dot{\mathbf{x}}_m} = \underbrace{\begin{bmatrix} 0 & 1 \\ -\omega_n^2 & -2\zeta\omega_n \end{bmatrix}}_{\mathbf{A}_m} \underbrace{\begin{bmatrix} \theta_m \\ \omega_m \end{bmatrix}}_{\mathbf{x}_m} + \underbrace{\begin{bmatrix} 0 \\ \omega_n^2 \end{bmatrix}}_{\mathbf{B}_m} r_\theta, \quad (4.22)$$

where ω_n is the natural frequency of the system, ζ is the damping ratio, and r_θ is the reference angle for the motor that we want the system to follow. The MRAC scheme requires that the reference model is stable. The eigenvalues of $\mathbf{A}_m$ in Equation (4.22) are given by:

$$\lambda = -\zeta\omega_n \pm \omega_n\sqrt{\zeta^2 - 1}. \quad (4.23)$$

Therefore, as long as $\zeta, \omega_n > 0$, the reference model will be stable. Similarly to the torque controller, we'll use the current controller designed in Section 4.1, such that we can treat I_a as the control input for the MRAC scheme. We can therefore define the reference current r_{I_a} as:

$$r_{I_a}(t) = -\mathbf{K}^T(t)\mathbf{x}(t) + L(t)r_\theta(t), \quad (4.24)$$

where $\mathbf{K}(t) \in \mathbb{R}^2$ and $L(t) \in \mathbb{R}$ are the adaptive parameters that will be updated online based on the observed behavior of the system. Defining the tracking error $\mathbf{e}(t)$ as:

$$\mathbf{e}(t) = \mathbf{x}(t) - \mathbf{x}_m(t). \quad (4.25)$$

Solving for $\mathbf{P}$ for a $\mathbf{Q} = \mathbf{Q}^T > 0$ in the Lyapunov equation:

$$\mathbf{A}_m^T \mathbf{P} + \mathbf{P} \mathbf{A}_m = -\mathbf{Q}, \quad (4.26)$$

we can define the adaptive law as:

$$\begin{aligned} \dot{\mathbf{K}}(t) &= \mathbf{\Gamma}_K \mathbf{x} \mathbf{B}_m^T \mathbf{P} \mathbf{e}, \\ \dot{L}(t) &= -\gamma_L \mathbf{B}_m^T \mathbf{P} \mathbf{e} r_\theta(t), \end{aligned} \quad (4.27)$$

where $\mathbf{\Gamma}_K \in \mathbb{R}^{2 \times 2}$ and $\gamma_L \in \mathbb{R}$ are positive definite matrices that determine the adaptation rate of the parameters.

4.3.3 Connecting the motors to the finger through a cable

For the simulation of the position controller, we will simulate two motors, one for flexion and one for extension, as is the case in our physical system. The motors will be pulling on each their cables, where force the motors generate gets distributed to the three phalanges through their own whiffle tree, with $w_1 = \frac{1}{2}$ of the force going to the proximal phalanx, $w_2 = \frac{1}{3}$ of the force going to the middle phalanx, and $w_3 = \frac{1}{6}$ of the force going to the distal phalanx. The force application is shown in Figure 4.7.

Cable tension

To emulate the cable connecting the motor to the finger, the following constraint is added to the system:

$$g(\theta, \mathbf{q}) \triangleq r_{spindle}\theta + L_{finger}(\mathbf{q}) - C = 0, \quad \mathbf{q} = \begin{bmatrix} \varphi_{MCP} \\ \varphi_{PIP} \\ \varphi_{DIP} \end{bmatrix}, \quad (4.28)$$

where $r_{spindle}$ is the radius of the spindle mounted on the motor, θ is the angle of the motor, $L_{finger}(\mathbf{q})$ is an estimate for the total length of cable from the finger to the whiffle tree. C is a constant defining the total cable length in the system, which then constraints the angle of the motor and the relative angles of the finger. The estimate of the total cable going from the finger to the whiffle tree is defined as:

$$L_{finger}(\mathbf{q}) = \sum_{i=1}^3 w_i \|\mathbf{r}_{a,i} - \mathbf{r}_{t,i}\|, \quad (4.29)$$

where $\mathbf{r}_{a,i}$ and $\mathbf{r}_{t,i}$ are the attachment and target points of the i -th phalanx, respectively, shown in Figure 4.7. The distance between the attachment and target points of each phalanx is scaled with the force ratios w_i to get a better estimate of the total length of cable with the whiffle tree. Differentiating the constraint, we get the velocity constraint:

$$\dot{g}(\omega, \mathbf{q}, \dot{\mathbf{q}}) = r_{spindle}\omega + \frac{\partial L_{finger}}{\partial \mathbf{q}} \dot{\mathbf{q}} = 0, \quad (4.30)$$

and further once more we get the acceleration constraint:

$$\ddot{g}(\dot{\omega}, \mathbf{q}, \dot{\mathbf{q}}, \ddot{\mathbf{q}}) = r_{spindle}\dot{\omega} + \frac{\partial L_{finger}}{\partial \mathbf{q}} \ddot{\mathbf{q}} + \dot{\mathbf{q}}^T \frac{\partial^2 L_{finger}}{\partial \mathbf{q}^2} \dot{\mathbf{q}} = 0. \quad (4.31)$$

To reduce numerical drift, Baumgarte stabilization is added, to combine all the constraints into a single equation:

$$\ddot{g} + 2\alpha\dot{g} + \beta^2 g = 0, \quad \alpha, \beta > 0. \quad (4.32)$$

The final constraint in Equation (4.32) is defined separately for the flexion and extension cables. The corresponding Lagrange multipliers are treated as the cable tensions T_f and T_e for the flexion and extension cable, respectively, and are solved simultaneously at each timestep.

Since the cables only can pull on the finger, we further impose that the cable tensions must be non-negative:

$$T_f, T_e \geq 0. \quad (4.33)$$

To be clear, this implementation of the cable tension is not a perfect emulation of the real system. In reality, the cable is slightly elastic, and the whiffle trees will provide some friction. There will also be more cable in the system. However, considering that the position of the attachment points, target points, and configuration of whiffle trees are not yet decided in the real system, this should provide a good enough approximation to test the position controller, and get a better understanding of the dynamics of the system.

Updated dynamics with the cable tension

Given the cable tension T_x prior to the whiffle tree for the x -th cable, the x -th brushed DC motor experiences a load torque of $\tau_l = r_{spindle}T_x$, giving the updated mechanical dynamics from Equation (3.18):

$$J_m \frac{d^2\theta_x}{dt^2} + B_m \frac{d\theta_x}{dt} = K_t I_a - r_{spindle}T_x. \quad (4.34)$$

Similarly, the finger experiences a generalized load torque. Since the cable tension acts along the line from the attachment point $\mathbf{r}_{a,i}$ to the target point $\mathbf{r}_{t,i}$, the force applied to the i -th phalanx is

$$\mathbf{F}_{x,i} = w_i T_x \frac{\mathbf{r}_{x,t,i} - \mathbf{r}_{x,a,i}}{\|\mathbf{r}_{x,t,i} - \mathbf{r}_{x,a,i}\|}. \quad (4.35)$$

The generalized torque contribution from this force is computed with:

$$\boldsymbol{\tau}_{x,i} = \frac{\partial(\mathbf{r}_{x,a,i} - \mathbf{r}_{x,t,i})^T}{\partial \mathbf{q}} \mathbf{F}_{x,i}, \quad (4.36)$$

which leads to the total generalized cable torque on the finger:

$$\boldsymbol{\tau}_{x,cable} = \sum_{i=1}^3 \boldsymbol{\tau}_{x,i}. \quad (4.37)$$

Given that we have two motors pulling on the finger with their own cables, we can calculate the total generalized torque from both the flexion and extension cables on the finger as:

$$\boldsymbol{\tau}_{cable} = \sum_{i=1}^3 \frac{\partial(\mathbf{r}_{f,a,i} - \mathbf{r}_{f,t,i})^T}{\partial \mathbf{q}} \mathbf{F}_{f,i} + \sum_{i=1}^3 \frac{\partial(\mathbf{r}_{e,a,i} - \mathbf{r}_{e,t,i})^T}{\partial \mathbf{q}} \mathbf{F}_{e,i}. \quad (4.38)$$

This gives us the updated finger dynamics from Equation (3.15):

$$\mathbf{M}(\mathbf{q})\ddot{\mathbf{q}} + (\mathbf{C}(\mathbf{q}, \dot{\mathbf{q}}) + \mathbf{B})\dot{\mathbf{q}} + \mathbf{K}(\mathbf{q} - \mathbf{q}_{eq}) = \boldsymbol{\tau}_{ext} + \boldsymbol{\tau}_{cable}. \quad (4.39)$$

4.3.4 Simulation of MRAC scheme with updated dynamics

Equation (4.39) is used for simulating the dynamics of the finger, while two sets of Equation (4.34) are used for simulating the dynamics of the two motors. To connect the models, a cable constraint is added to emulate the cables connecting the motors and the finger, as discussed in Section 4.3.3. The parameters for the motor and finger model are given in Table 4.1. The estimation of the motor parameters are done in Section 3.2.1. The parameters of the finger model are not taken from any literature, but were selected empirically through repeated simulations of the unloaded finger to obtain realistic motion.

Both cables are initialized to be under tension when the finger is in a straight position, i.e. when $\varphi_{MCP} = \varphi_{PIP} = \varphi_{DIP} = 0$. The flexion motor is initialized to $\theta_f(0) = 0$ rad, while the extension motor is initialized to $\theta_e(0) = \frac{\pi}{2}$ rad. To make sure the motors aren't working against each other, they receive an opposite reference angle. This ensures that as one motor pulls on the finger, increasing the tension in its cable, the other motor will be rotating in the opposite direction, decreasing the tension in its cable. When the motors are decreasing the tension in their cables, the motor would experience $\tau_l \approx 0$ N m. Therefore the dynamics would change, throwing off the adaptive gains. To account for this, we switch to a pretuned (PT) controller, tuned for a unloaded motor. At the same time we turn off the adaptive law. Once the motor receives a reference that will increase the tension in the cable, we switch back to the adaptive controller, and turn on the adaptive law. The pretuned controller is tuned through the exact same adaptive controller, just with an unloaded motor for 100 s. When the pretuned controller is active, these final values of $\mathbf{K}$ and L are used instead of the adaptive gains. The reference angles for the flexion motor and the extension motor is given by:

$$r_{\theta_f}(t) = \begin{cases} \frac{\pi}{2} & \text{if } \sin\left(\frac{6}{10}\pi\theta_f(t)\right) > 0 \\ 0 & \text{else} \end{cases} \quad (4.40)$$

$$r_{\theta_e}(t) = \theta_e(0) - r_{\theta_f}(t).$$

The reference models parameters from Equation (4.22) are set to $\omega_n = 8$ and $\zeta = 1$. $\mathbf{Q} = \begin{bmatrix} 10 & 0 \\ 0 & 1 \end{bmatrix} \Rightarrow \mathbf{P} \approx \begin{bmatrix} 3.56 & 0.078 \\ 0.078 & 0.036 \end{bmatrix}$. The adaptive gain matrices are set to

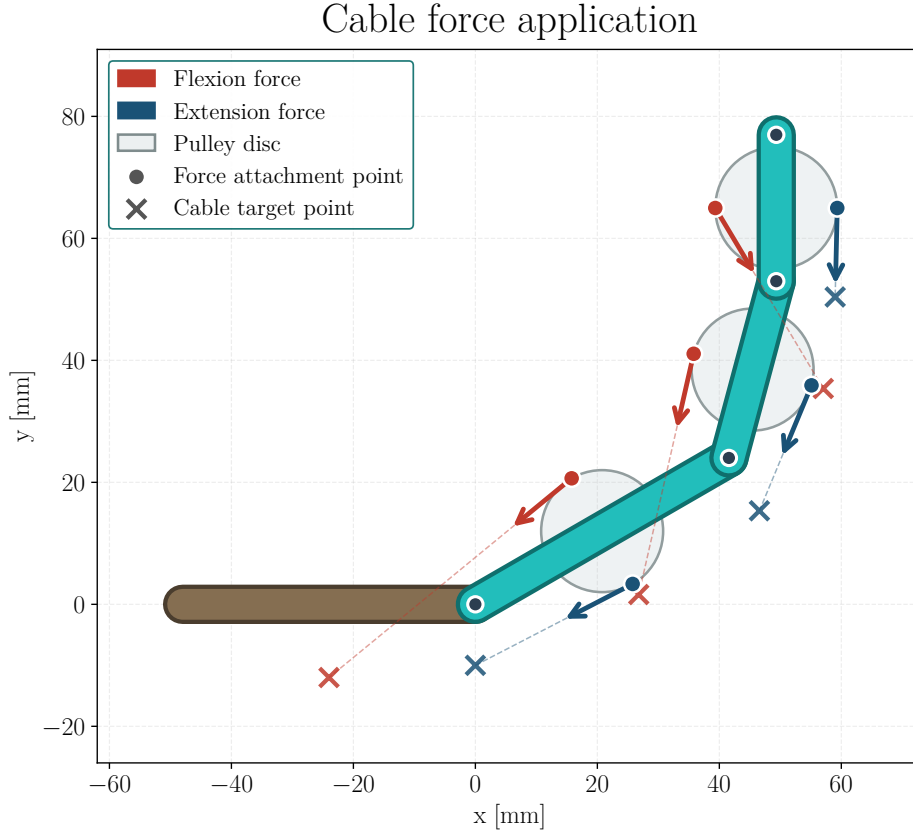


Figure 4.7: Force application on the finger. The flexion motor applies a force F_f on the flexion cable, which gets distributed to the three phalanges through the whiffle tree. Similarly, the extension motor applies a force F_e on the extension cable, which also gets distributed to the three phalanges through its own whiffle tree.

$\mathbf{\Gamma}_K = \begin{bmatrix} 3 & 0 \\ 0 & 0.5 \end{bmatrix}$ and $\gamma_L = 2$. The adaptive gains are initialized to $\mathbf{K}(0) = \begin{bmatrix} 0.0 \\ 0.0 \end{bmatrix}$ and $L(0) = 1$.

4.3.5 Evaluation of MRAC scheme

Figure 4.8 shows a simulation of the MRAC controller over 10 s. While the MRAC scheme is active, indicated in orange, the motor angles θ_f and θ_e initially oscillate around the reference model. Over time, however, the adaptive gains $\mathbf{K}$ and L change to values that allow the system to track the reference model more closely, and the oscillations become less prominent. While the pretuned controller is active, indicated in grey, the motor tracks the reference model quite closely. Interestingly it seems to have a slightly faster response than the reference model. This might be due some inconsistencies with the cable tensioning implementation.

Continuing the simulation to 100 s, Figure 4.10 shows the evolution of the adaptive gains, aswell as the error between the motor angles and their respective reference model angles. Figure 4.9 shows the simulation results for 10 s after 90 s. Looking at Figure 4.10,

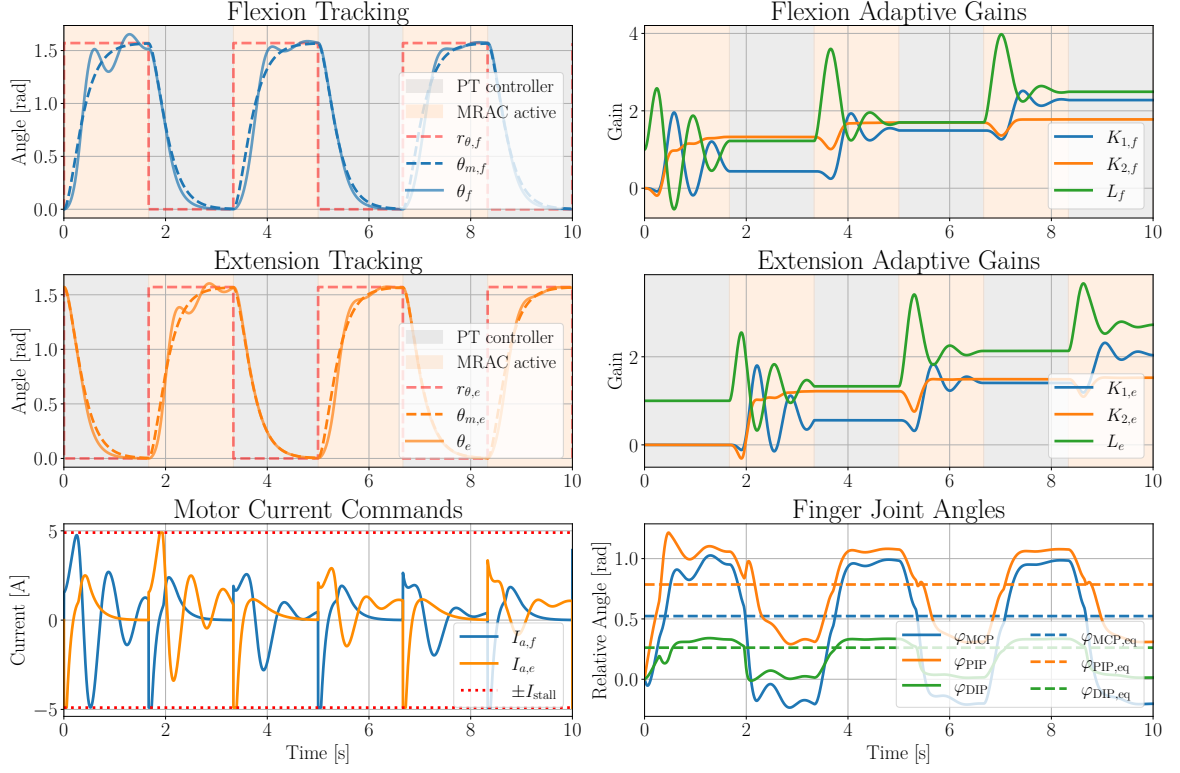


Figure 4.8: Simulation results of the MRAC scheme for flexion and extension motor over 10s.

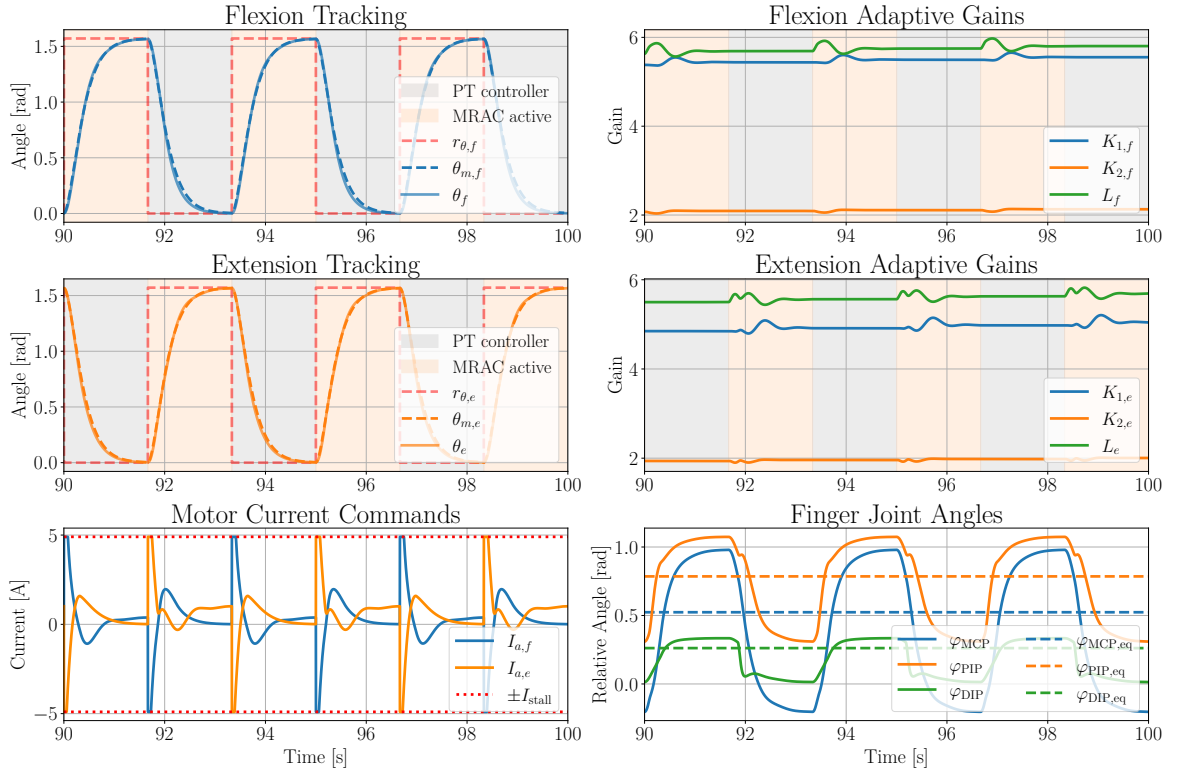


Figure 4.9: Simulation results of the MRAC scheme for flexion and extension motor after 90 s.

Table 4.1: Physical parameters used for the finger model.

Phalanx parameters			
Phalanx	m [kg]	l [cm]	r [mm]
Proximal Phalanx	0.020	4.8	8.5
Middle Phalanx	0.015	3.0	8.5
Distal Phalanx	0.020	2.4	8.5
Joint parameters			
Joint	k [N m rad ⁻¹]	b [N m s rad ⁻¹]	φ_{eq} [rad]
MCP Joint	0.5	0.05	$\pi/6$
PIP Joint	0.5	0.05	$\pi/4$
DIP Joint	0.5	0.05	$\pi/12$

after ~ 10 s, K_2 seem to converge to a certain value, while K_1 and L eventually keeps growing together, almost logarithmically. The continued growth of K_1 and L might be due to the fact that the system is trying to find gains that can track the reference model better, but is limited by the maximum current that the motor can provide. Looking at the current commands going to the motors in Figure 4.9, it can be observed that they are clipped by the maximum stall current of 4.9 A. Looking back at Figure 4.10, it's clear that the error between the motor angles and their respective reference model decrease over time as the adaptive gains update. However they don't go to zero, but end up with some steady-state error, though quite small. This tells us that the adaptive controller gains at some point reach a local optimum. Therefore, to combat the ever increasing gains, we may want to switch to a fixed-gain controller once the gains have converged.

Figure 4.11 shows a simulation over 10 s using the adaptive gains found in Figure 4.10 after 100 s, but with the gains fixed instead of adaptive. Here we can see that the motors are able to track their reference angles rather well, only with a slight error in the transition to a new reference angle. Hence we may conclude that the MRAC scheme could prove useful in quickly tuning a position controller, when frequently switching between patients.

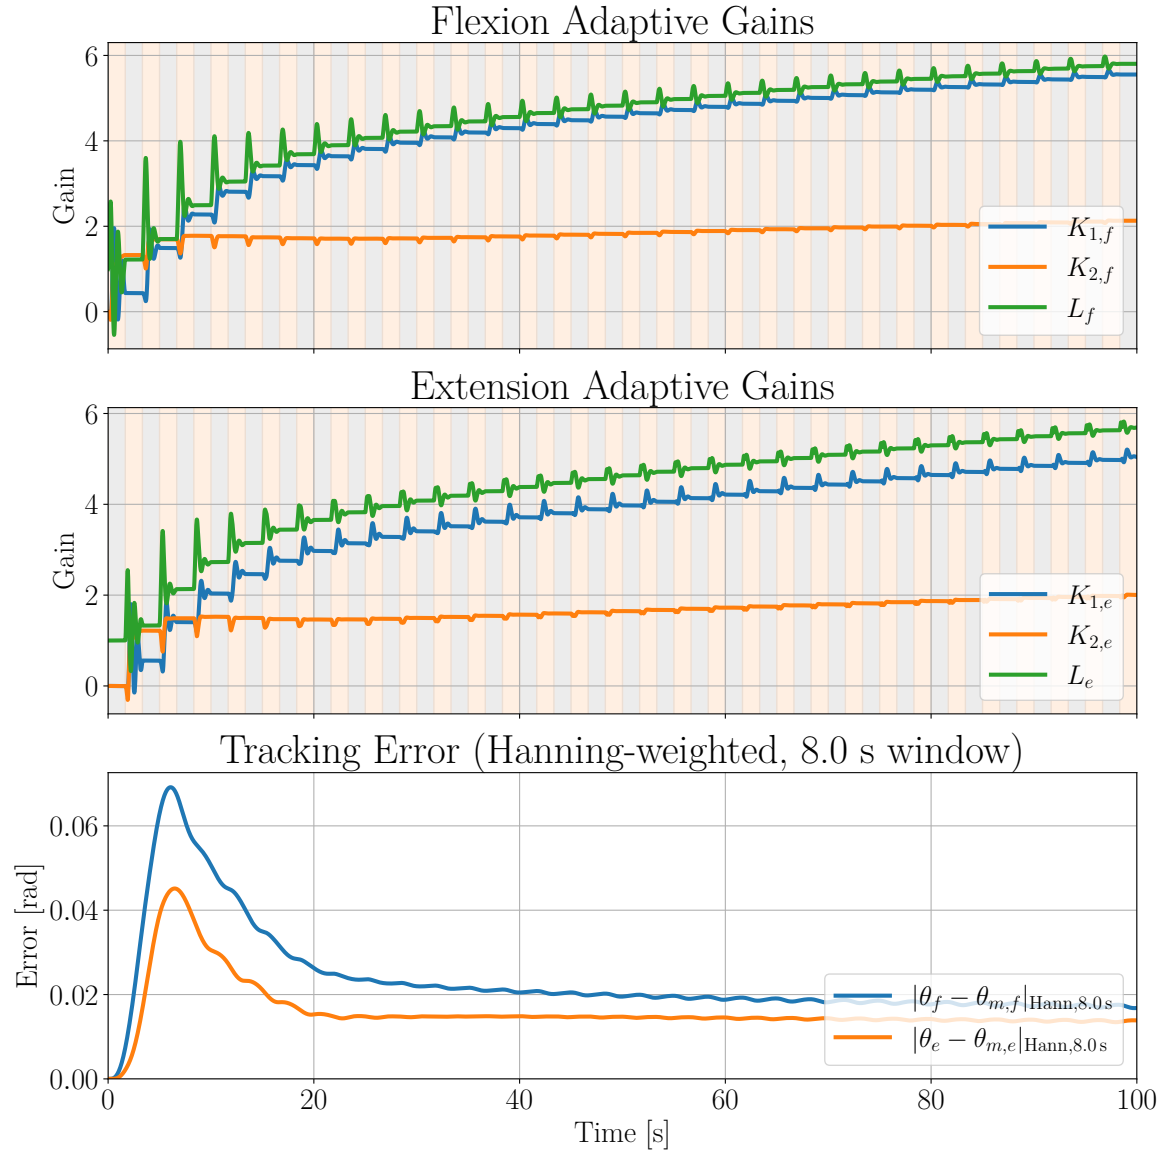


Figure 4.10: Adaptive gains and error over time for MRAC scheme for 100 s, where K_1 and L keep growing together.

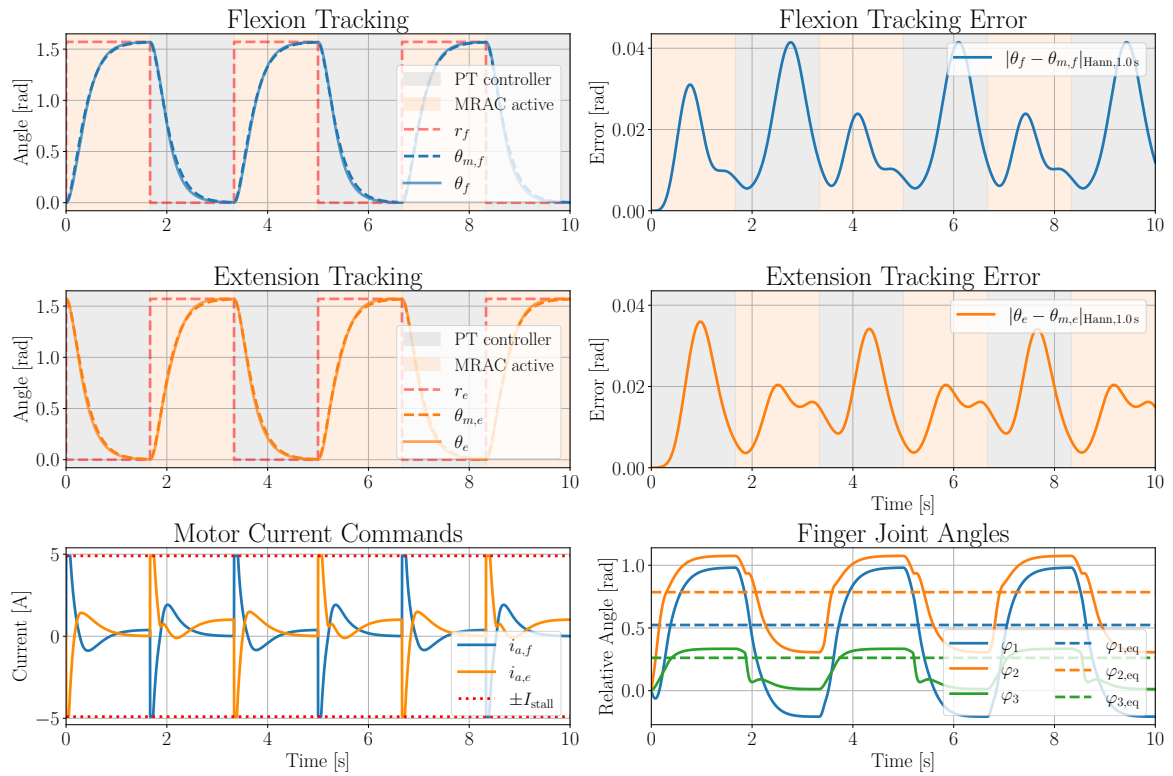


Figure 4.11: Simulation results of the MRAC scheme for flexion and extension motor over 10 s, with the adaptive gains found in Figure 4.10 after 100 s, but with the gains fixed instead of adaptive.

Chapter 5

Discussion

5.1 Current control

In Section 4.1, a current controller for the brushed DC motor was designed. The purpose of the controller was not only to make the armature current I_a track a reference current, but also to make it possible to treat the armature current as a control input for the slower mechanical dynamics of the motor. Considering that the generated motor torque is given by $\tau_m = K_t I_a$, controlling the armature current precisely and fast is crucial for precise torque and position control of the motor. The controller was designed as a feedforward (FF) and proportional (P) controller, shown in Equation (4.2). The feedforward term is designed to cancel out the back-EMF voltage, generated while the motor is spinning, where the proportional term is designed to stabilize the system and ensure that the armature current tracks the reference current.

Simulation showed that the feedforward term is important. Only using the proportional feedback, the controller performs reasonably well starting from rest, but the performance deteriorates as the motor speeds up. This is due to the fact that the back-EMF voltage increases linearly with the motor speed, and without the feedforward term, the controller cannot compensate for this voltage, leading to a steady-state error in the armature current. With the feedforward term included, the controller can effectively cancel out the back-EMF voltage, allowing for precise control of the armature current even at higher speeds.

Considering the fast dynamics of the armature current, the dynamics was discretized with a sampling period T_s , assuming constant angular velocity between each sample. An upper bound for the proportional gain K_p , $K_{p,\max}(T_s)$, was derived to ensure stability of the discrete-time system. Simulations showed that a gain below this upper bound resulted in a stable response, where $K_p = \frac{1}{2}K_{p,\max}(T_s)$, generally yielded a fast damped response. The sampling time showed to have a significant effect on the performance of the controller. A smaller sampling time, like $T_s = 0.2\text{ ms}$, resulted in a

fast damped response, reaching the reference current. A higher sampling time however, like $T_s = 1$ ms, resulted in an underdamped response, where the armature current got a steady-state error from the reference current. This is likely because the assumption of constant angular velocity over each sampling interval becomes less accurate as the sampling time increases. Hence the feedforward term becomes unable to account for the increasing back-EMF voltage, leading to steady-state error, like for the case with only proportional feedback. Considering that the motor inertia is unknown, and only estimated, the angular acceleration could be very different in the real system compared to the simulation. Therefore, the effect of the increasing back-EMF voltage during the sampling period could be more or less significant in the real system, compared to the simulation. The results here should hence only be seen as an indication of the effect of the sampling time, and not a precise prediction of the performance of the controller in the real system.

The noise simulations indicate that the current controller is relatively robust to current measurement noise. In general, noisy measurements would merely lead to oscillations around the steady-state value for the controller without noise present. This is an advantage of the simple structure of the controller, where no derivative actions are used, which would be very susceptible to noise.

A limitation of the current controller is that it relies on relatively accurate estimates of the parameters R_a , L_a and K_b . The parameter identification method developed in Section 3.2.2 can be used to get an estimate of the armature inductance L_a . Similar methods can also be used to estimate the armature resistance R_a and the back-EMF constant K_b . However, it remains to be seen how well this works in the real system, as there might be modelling inconsistencies throwing off the estimates.

Overall, the P+FF current controller designed in Section 4.1 shows promising results for controlling the armature current of the brushed DC motor. The simulated maximum current rate of change, approximately $\dot{I}_{a,\max} \approx 2.0 \text{ kA s}^{-1}$, is fast compared to the mechanical dynamics of the finger. It is therefore reasonable to treat the armature current as a control input in the torque and position control design.

5.2 Torque and force control

In Section 4.2, torque control was considered using the current controller from Section 4.1 as an inner loop. Since the generated motor torque is given by $\tau_m = K_t I_a$, controlling the armature current gives an indirect way to control the motor torque. The performance of the torque controller is hence highly dependent on the performance of the current controller, and the advantages and limitations of the current controller, as discussed in Section 5.1, also apply here.

As discussed in Section 4.2, there will be friction acting on the cable between the

motor and the finger, from going through the a bowden tube. Hence, the generated force pulling on the cable from the motor, will not be equal to the applied force on the finger. Therefore, without any feedback on the applied force, the applied force on the finger will generally have a steady-state error from the reference force unless the friction is compensated for. By assuming a constant friction, this can be calibrated for by artificially increasing the reference force by the estimated friction force. However, this is not a very robust solution, as the friction can change over time due to wear and tear, and also depends on the configuration of the finger.

The integration of force sensors in the fingertips appears to be a more robust solution. With direct measurements of the applied force, the controller no longer has to rely solely on the current measurements as an estimate of the applied force to the finger. In Section 4.2, a feedforward (FF) and a proportional and integral (PI) controller for the reference current was designed. Simulations showed that the controller was able to reach the desired applied force in a well-damped manner, using a artificially higher reference force for the motor to compensate for the friction.

It should be noted that the performance of the FF+PI controller is dependent on the friction from the bowden tube. The proportional and integral gains were also just tuned empirically, and it is not clear how they would perform in the real system. The performance of the controller should hence be seen as an indication of the potential performance, rather than a precise prediction of the performance in the real system. And the controller gains should therefore be tuned carefully in the real system.

5.3 Position controller using MRAC

In Section 4.3, a position controller was designed, with the assumption that the current could be treated as a control input, using the current controller from Section 4.1 as an inner loop. The performance of the position controller is hence highly dependent on the performance of the current controller, and the advantages and limitations of the current controller, as discussed in Section 5.1, also apply here.

Considering the system is meant to be used by multiple different subjects, a pretuned controller is not guaranteed to work well for all participants. Some participants may have much stiffer joints due to little movement, and others may have more flexible joints. Many other factors can also play a role in changing the dynamics between participants. Hence, an adaptive controller, that can adapt to the dynamics of the individual user, was designed. The adaptive controller was designed as a model reference adaptive controller (MRAC), where the parameters of the controller are adapted online to make the output of the system follow the output of a reference model. The tracking of a reference model can also prove advantageous in providing more control over the acceleration of the gripping movement, fascilitating a more comfortable user experience.

Simulations showed that the MRAC scheme was able to make the system follow the reference model. In the beginning the motor angles were oscillating around the reference model, but as the adaptive gains were updated, the oscillations were damped out and the motor angles followed the reference model closely. As discussed in Section 4.3.5, the controller gains just keeps growing. This is likely due to the saturation in the reference current to $I_{a,\text{stall}}$, making it a non-linearity the adaptive gains are not able to account for. We can also note that the error between the motor angles and the reference model is not going to zero, but does converge to very small value, making it almost negligible.

The performance of the MRAC scheme does make sense considering the assumptions made in the design of the controller in Section 2.3.3. It assumes that the system is LTI, and that the dynamics can be written in state-space form. The model of the brushed DC motor can be written in state-space form, but the dynamics of the finger is more complex. With the cable constraint, the dynamics is hardly linear, and the equilibrium position of the finger would definitely add a constant disturbance term to the dynamics, which isn't accounted for in the MRAC derivation. In addition, the MRAC scheme, given its original assumptions, guarantees that the error between the state vector and that of the reference model goes to zero, and that the adaptive gains remain bounded. Considering the non-linearities and the saturation in the system, it is not surprising that the error doesn't go to zero, and that the adaptive gains keeps growing. However, the fact that the error converges to a very small value, and that the system is able to follow the reference model closely, indicates that the MRAC scheme is still able to provide good performance even with the non-linearities and saturation in the system.

The issue of continuously growing adaptive gains, discussed in Section 4.3.5, can be mitigated by freezing the adaptation once the tracking error between the motor angles and the reference model no longer decreases, or after a predefined adaptation period. In this way, the controller can still adapt to the dynamics of the individual user, thereby simplifying the tuning process for the position controller. At the same time, preventing further adaptation ensures that the controller performance does not degrade over time as a result of unbounded growth in the adaptive gains.

5.4 Model assumptions and limitations

In the modelling of the system, several assumptions and simplifications were made. In the modelling of the finger, each phalange was modelled as a rigid body, and the joints were modelled as ideal revolute joints, with linear torsional springs and dampers. In reality, the phalanges can't rotate freely around the joints, where they have a certain range of motion. Hence, the stiffness of the joints is not linear, but rather changes with the angle of the joint. Also the values for the parameters used during simulations were not based on measurements from the real system, but rather just estimated empirically

to get a natural movement. The performance of the controller in the real system might hence be very different from the simulations. Therefore it remains to be seen how well the model captures the dynamics of the real system.

The cable connecting the motor and the finger was also simplified as a constraint between the angle of the motor and the travel of the finger. It ignores any elasticity in the cable, and also doesn't model the friction from the bowden tube, which can have a significant effect on the performance of the controller. Additionally the length of the cable is not accurate compared to the real system, where it most likely is a lot longer. The performance of the controller in the real system might hence be very different from the simulations. Therefore it remains to be seen how well the cable constraint captures the dynamics of the real system.

Therefore, the performance of the MRAC scheme discussed in Section 5.3, in the real system might be different from the simulations. The performance of the controller should hence be seen as an indication of the potential performance, rather than a precise prediction of the performance in the real system. It remains to be seen how well the MRAC scheme performs in the real system, and whether it can provide a good user experience for multiple different users. If the controller works poorly in the real system, it might be a good idea to pivot to a simple PD controller, and tune the gains for each individual user. This would likely provide better performance than a poorly performing MRAC scheme, but it would also require more time tuning the controller for each user. If there is too much friction in the system, it might also be a good idea to include an integral term in the controller, to compensate for the steady-state error from the friction. However, this would also make the tuning process more difficult, and could more easily lead to instability.

With all the assumptions and simplifications made, the performance of the controllers in the real system might be very different from the simulations. The results in this thesis should hence only be viewed as a possible proof of concept, and not a precise prediction of the performance in the real system. The controllers should be tuned carefully in the real system, and it will likely be necessary to make modifications to the controllers to get good performance in the real system.

5.5 Practical implementation considerations

Bibliography

- Ioannou, P. A., & Sun, J. (2012, December 19). *Robust Adaptive Control*. Courier Corporation.
- Jeong, U., & Cho, K.-J. (2015). Feedforward friction compensation of Bowden-cable transmission via loop routing. *2015 IEEE/RSJ International Conference on Intelligent Robots and Systems (IROS)*, 5948–5953. <https://doi.org/10.1109/IROS.2015.7354223>
- National Cancer Institute. (2026). *Anatomical Terminology / SEER Training*. Retrieved March 13, 2026, from <https://training.seer.cancer.gov/anatomy/body/terminology.html>
- Pololu - 75:1 Metal Gearmotor 25Dx54L mm HP 12V. (2026, May 15). <https://www.pololu.com/product/3206/resources>
- Pololu 25D Metal Gearmotors. (2021). <https://www.pololu.com/file/0J1829/pololu-25d-metal-garmotors.pdf>
- Rahman, N., & Mat Yahya, N. (2021). A mathematical model of a brushed DC motor system. *Data Analytics and Applied Mathematics (DAAM)*, 2, 60–68. <https://doi.org/10.15282/daam.v2i2.6830>
- TeachMeAnatomy. (2026a). *Anatomical terms of location*. Retrieved March 14, 2026, from <https://teachmeanatomy.info/the-basics/anatomical-terminology/terms-of-location/>
- TeachMeAnatomy. (2026b). *Anatomical terms of movement*. Retrieved March 15, 2026, from <https://teachmeanatomy.info/the-basics/anatomical-terminology/terms-of-movement/>