

Monitoring multiple medical signs through a wireless ear probe

by

André Bestbier



*Thesis presented in partial fulfilment of the requirements for
the degree of Master of Engineering (Mechanical) in the
Faculty of Engineering at Stellenbosch University*

Supervisor: Prof. PF. Fourie

September 2017

Declaration

By submitting this thesis electronically, I declare that the entirety of the work contained therein is my own, original work, that I am the sole author thereof (save to the extent explicitly otherwise stated), that reproduction and publication thereof by Stellenbosch University will not infringe any third party rights and that I have not previously in its entirety or in part submitted it for obtaining any qualification.

Date: 2017/09/09

Copyright © 2017 Stellenbosch University
All rights reserved.

Abstract

Monitoring multiple medical signs through a wireless ear probe

A. Bestbier

*Department of Mechanical and Mechatronic Engineering,
University of Stellenbosch,
Private Bag X1, Matieland 7602, South Africa.*

Thesis: MEng (Mech)

September 2017

Add abstract.

Uittreksel

Monitering van kern temperatuur, hartklop, respiratoriese tempo, bloed suurstof versadiging en EEG deur middel van 'n draadlose oor probe

*(“Monitoring core temperature, heart rate, respiratory rate, blood oxygen saturation
and electrical brain activity through a wireless ear probe”)*

A. Bestbier

*Departement Meganiese en Megatroniese Ingenieurswese,
Universiteit van Stellenbosch,
Privaatsak X1, Matieland 7602, Suid Afrika.*

Tesis: MIng (Meg)

September 2017

Voeg uittreksel by.

Acknowledgements

I would like to express my sincere gratitude to the following people and organisations ...

Dedications

Hierdie tesis word opgedra aan ...

Contents

Declaration	i
Abstract	ii
Uittreksel	iii
Acknowledgements	iv
Dedications	v
Contents	vi
List of Figures	ix
List of Tables	x
Nomenclature	xi
1 Introduction	1
1.1 Aim/Research Question	2
1.2 Motivation	2
2 Biology Literature Review	4
2.1 Ear Anatomy	4
2.1.1 Auricle	4
2.1.2 Ear Canal	5
2.1.3 Tympanic Membrane	6
2.2 Medical Sign Physiology	7
2.2.1 Core Temperature	7
2.2.2 Heart Rate	8
2.2.3 Respiratory Rate	9
2.2.4 Blood Oxygen Saturation	9
2.2.5 Electrical Brain Activity	10
3 Theory Literature Review	11
3.1 Core Temperature	11

3.1.1	Contact Thermometers	12
3.1.2	Non-contact Thermometers	13
3.1.3	Commercial Temperature Monitoring Devices	14
3.2	Heart Rate	16
3.2.1	Electrocardiography	16
3.2.2	Photoplethysmography	17
3.2.3	Ballistocardiography	20
3.2.4	Other Heart Rate Methods	21
3.3	Respiratory Rate	22
3.3.1	Respiratory Rate Ear Sensors	22
3.3.2	Respiratory related Heart Rate Characteristics	22
3.4	Blood Oxygen Saturation	23
3.4.1	Pulse Oximetry Theory	24
3.4.2	Work done by others in ear pulse oximetry	26
3.5	Electrical Brain Activity	27
4	Concept Design	28
4.1	Temperature	28
4.1.1	Temperature measurement method	28
4.1.2	Temperature measurement sensor	30
4.2	Heart Rate	31
4.2.1	Heart rate measurement method	32
4.2.2	Heart rate measurement sensor	35
4.3	Respiratory Rate	37
4.3.1	Respiratory rate measuring method	37
4.4	Blood oxygen saturation	38
4.5	Final concept	38
5	Detailed Design	40
5.1	Hardware	40
5.1.1	Temperature sensor	40
6	Experimental Procedure	43
6.1	Overview	43
6.2	Theory	44
6.3	Ethical Consent	44
6.4	Subjects	44
6.5	Benchmark Validation	44
6.6	Method	44
6.6.1	Benchmark Apparatus	44
6.6.2	Comparing Data	44
6.7	Results	45
	Appendices	46

List of Figures

2.1	Anatomical structures of the auricle (Get source from: goo.gl/mmLnFx)	5
2.2	Structure of the ear (Drake et al: Gray's Anatomy for Students)	6
2.3	The results from 20 studies with strong or fairly strong evidence of normal oral, rectal and tympanic temperature ($^{\circ}\text{C}$) in adult men and women are presented. Temperature is obtainable as mean value(bold lines), 1st and 3rd quartiles (unfilled bars) and range (thin lines).	8
2.4	EEG rhythms	10
3.1	Plot showing how Planck's law can be used to determine the dominant radiation wavelength at certain temperature	14
3.2	IR Thermometer diagram (V Polyzoev et al: Demystifying Thermopile IR Temp Sensors)	15
3.3	CAD model of the <i>degree</i> $^{\circ}$ from the <i>cosinuss</i> $^{\circ}$ website (include ref)	15
3.4	Ear-worn device developed by Winokur <i>et al.</i> (2012)	16
3.5	The two modes of Photoplethysmography (Tamura <i>et al.</i> , 2014)	17
3.6	Basic operating principles of PPG (Tamura <i>et al.</i> , 2014)	18
3.7	Pulse oximetry diagram (Poh <i>et al.</i> , 2010)	19
3.8	Pulse oximetry diagram (Da He <i>et al.</i> , 2010)	20
3.9	https://www.cosinuss.com/en/products/one	20
3.10	Device to measure in ear pulse waves due to the heart beat (Park <i>et al.</i> , 2015)	21
3.11	Breathing detected through microphones inside the ear canal (Goverdovsky <i>et al.</i> , 2016)	22
3.12	Baseline osculations in behind the ear BCG due to breathing (Da He <i>et al.</i> , 2010)	23
3.13	Absorption spectra of oxy- and deoxyhemoglobin	24
4.1	ST60Micro diagram from the datasheet	31
4.2	NJL5501R diagram from the datasheet	35
4.3	MAX30100 block diagram from the datasheet	36
5.1	Flow of information in a typical telemedicine set-up	40
5.2	TMP006 pre-mounted boards, cut-out and four connections	41

List of Tables

3.1	Results of the respiratory rate extraction through neural networks (Johansson, 2003)	24
4.1	Contact thermometers evaluation	29
4.2	Non-contact thermometers evaluation	30
4.3	Ear ECG	32
4.4	Ear PPG	33
4.5	Ear BCG	34
4.6	Ear Phonocardiogram	34
4.7	Ear Accelerometer	37
4.8	Ear Microphone	37
4.9	Respiratory related heart rate characteristics	38

Nomenclature

Constants

$$g = 9.81 \text{ m/s}^2$$

Variables

Re_D	Reynolds number (diameter)	[]
x	Coordinate	[m]
\ddot{x}	Acceleration	[m/s ²]
θ	Rotation angle	[rad]
τ	Moment	[N·m]

Vectors and Tensors

$$\vec{v} \quad \text{Physical vector, see equation ...}$$

Subscripts

a	Adiabatic
a	Coordinate

Chapter 1

Introduction

This thesis document reports on a project undertaken in the biomedical field of wearable electronics. Great advances in miniaturization of electronics and wireless communication have challenged and transformed the norm of the how we use electronics to listen to the language of our bodies.

This project revolves around the continuous measurement of medical signs. These are objective parameters that give an indication about physical well-being and the state of essential physiological functions. For example, infections are indicated by a rise in core temperature, pneumonia can be detected by a shortness in breath, an abnormal decrease in respiratory rate during sleep can be a warning sign for sudden infant death syndrome, a rise in heart rate can indicate physical stress and abnormal brain activity can be detected at the onset of a seizure. These signs can be detected electronically before traditionally observable symptoms appear. In many cases the deciding factor in the success of a treatment is whether the illness is detected early enough.

Because of this, the importance and usefulness of a continuous, wearable health monitor should not be underestimated. Access to accurate, long term data can lead to improved diagnosis of health issues and a better understanding of how our bodies react to drugs, exercise, emotions and the environment around us. Traditionally, medical sign monitoring is done with a stationary, dedicated device for each signal to be measured. It is easy to see that this is not suitable for continuous and mobile medical sign monitoring.

This project concerns the design, development and testing of a proof of concept device that will overcome the limitations of these traditional methods. The device is to be worn on the ear like an earphone or hearing aid. It will make multi-parameter medical sign measurements and transmit collected data through a wireless connection to a supporting system for storage and analysis. In this project, the supporting system will be on a laptop, but it can also be on the smart-phone of the wearer or on a cloud server. This supporting system can be used by a physician, caretaker or the wearer self, to monitor and track his/her health.

From here onwards, this device will be referred to as the *Ear-Monitor*. This report will discuss the project aim and objectives, relevant literature and the design, manufacturing and testing of the Ear-Monitor.

1.1 Aim/Research Question

To develop and test a proof of concept wearable device that can monitor medical signs and transmit collected data wirelessly to a warning and storage system. Medical signs include core temperature, heart rate, respiratory rate, blood oxygen saturation and electrical brain activity.

(or in the form of a Research Question:)

Is the external ear canal a feasible location for the continuous monitoring of core temperature, heart rate, respiratory rate, blood oxygen saturation and electrical brain activity by means of a ear worn device?

In order to achieve the aim of of this project the following three objectives have to be met:

- Develop an ear worn device to measure core temperature, heart rate, respiratory rate, blood oxygen saturation and electrical brain activity through the external ear.
- Conduct a trail to determine the functionality of this device.
- Subsequently, evaluate the feasibility of an ear worm medical sign monitor

1.2 Motivation

This project arose from a need found in medical practise and expressed by the proposer/advocate of this topic. It is the need for better vital sign monitoring methods for neonates and infants in hospital nurseries and a home. High-risk patients are placed in ICUs and are thoroughly monitored, whereas lower risk patients are left in the nursery or sent home. These patients are poorly monitored while at a fragile age, increasing the risk of health issues. This insufficient health monitoring for neonates and infants is due to to the lack of a practical monitoring method. The solution to this issue is the development of a unobtrusive, wearable health monitor.

While contemplating and researching this idea, it was found that a much larger group can benefit from such a device. This lead to the project pivoting toward a more general purpose medical sign monitoring devise. This device will prove if it is practical to measure the mentioned medical signs through the

external ear canal. If this proof of concept is successful, the methods developed during this project can be used to develop specialized ear-worn devices from various applications. In practice, such a device can transmit health statistics and warnings in real time to a physician or caretaker. Applications include:

- Monitoring neonate- and infant health in nurseries and at home.
- Monitoring health of patients with chronic illnesses.
- Studying the effect of prescription drugs or other treatments.
- Monitoring vital signs and brain activity, like thalamic modulation, of patients during anaesthesia.
- Monitoring patients with a high seizure/epilepsy risk
- Monitoring the health of people working under strenuous conditions like heavy machinery operators and soldiers.
- Tracking the health and fitness of athletes.

The ear was chosen as location for the following reasons. The anatomy of the ear and the proximity of an ear-worn device to the tympanic membrane and brain, means that all the medical signs mentioned can theoretically be measured from this location. This eliminates the need for multiple devices or the need for wires connecting sensors on different parts of the body. The absence of sensors on traditional locations such as the chest or limbs and the absence of connective wires means that the ear-worn device is minimally obstructive for the wearer, especially through freeing up the hands and allowing him/her to move around. The shape of the external ear is ideal for supporting a device without the need for straps or adhesives. Furthermore, the head remains relatively still in relation to the rest of the body. This will reduce the risk of motion artefacts corrupting the signals of interest. An ear-worn device can be embedded in the already familiar shape of a earphone or hearing aid. The final motivation for using the ear as location for the health monitor is its novelty. As will be apparent in the literature review chapter of this document, there is opportunity for research to be done in the unsaturated field of ear-worn health monitors.

The five mentioned medical signs were chosen because...?

Chapter 2

Biology Literature Review

This chapter aims to describe the biological context within which the project is undertaken. An overview will be given about the anatomy of the ear which is relevant to this study. After which, background will be given about the physiology of each of the five medical signs.

2.1 Ear Anatomy

The area that is available for the Ear-Monitor to make the medical sign measurements is the external ear. It includes the auricle, ear canal with surrounding tissue and the lateral side of the tympanum. Each part of the ear anatomy will be discussed, especially with regards to its ability to emit information about medical signs or to support the device in another way.

2.1.1 Auricle

The auricle is the visible part of the ear. It forms a C-shaped funnel that protrudes from the skull. Its structure is predominantly formed by yellow elastic cartilage covered in skin. Its complex folded shape differs from person to person, but certain structures are present in all normal auricles and have been named. As can be seen on Figure 2.1 the concha is the indented part next to the ear canal. This area is an ideal location for a wearable device. The device can be held in place by the tragus and a probe can easily extend into the ear canal.

The external ear is supplied with blood from the auricular arteries. These arteries branch from the carotid artery which supplies the rest of the brain with blood. Being made mostly of cartilage and being at an extremity of the body, the auricle is not a suitable location for taking temperature measurements for its temperature is easily influenced by the ambient conditions.

The layer of skin covering the auricle contains blood vessels and the earlobe is a popular location for traditional pulse oximetry measurements. This is a

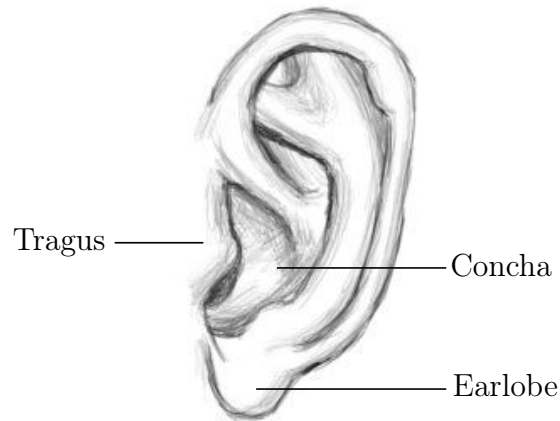


Figure 2.1: Anatomical structures of the auricle (Get source from: goo.gl/mmLnFx)

possible location for a ear-worn device to make a heart rate and SpO_2 measurement (Poh *et al.*, 2010). The earlobe's blood vessels are, however, susceptible to vasoconstriction due to cold or hypovolaemia (WorldHealthOrganization, 2011). This will reduce the blood perfusion of the subcutaneous tissue making it harder to get accurate heart rate and SpO_2 measurements.

The auricle is used in EEG systems as a location for a reference electrode. It is far enough from the brain for it to have an extremely small electrical potential (Nunez and Srinivasan, 2006).

2.1.2 Ear Canal

The external ear canal is the tube running from the floor of the auricle to the middle ear, ending blindly at the tympanic membrane or tympanum. Figure 2.2 depicts the structure of the ear as seen from a coronal plane section. The auricle is visible and the shape and relative size of the canal can be observed.

The ear canal in adults is approximately 25 mm long and have a diameter of 5 to 7 mm (Alvord and Farmer, 1997). The outer third of the external ear canal is surrounded by cartilage and fibrous tissue (of Encyclopædia Britannica, 2015). The inner two thirds are surrounded by the temporal bone. Thin skin from the lining of the canal and contains glands secreting ear wax. Hairs are found in the outer part of the canal. The ear canal of infants starts out relatively straight, but obtains a definite S-shape as the head develops (Alvord and Farmer, 1997). This S-shape is important to keep in mind while placing a sensor to measure tympanic temperature. Ear canal size also varies from

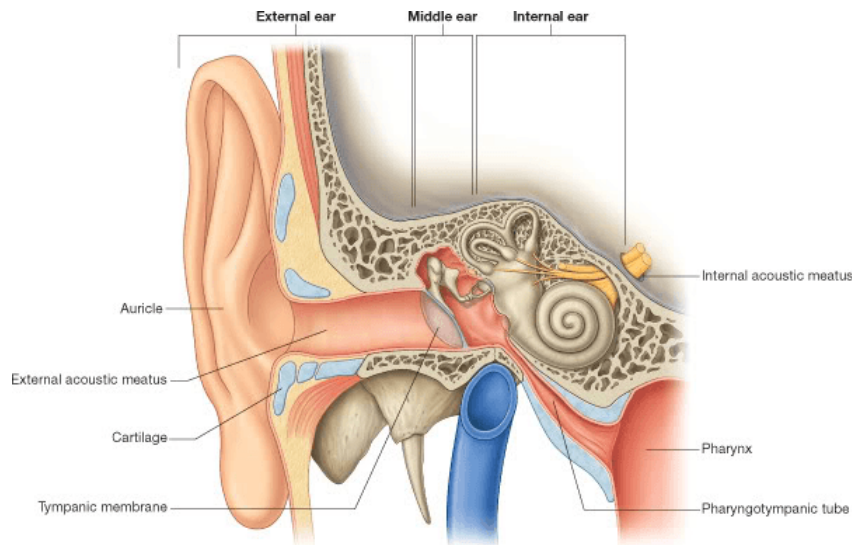


Figure 2.2: Structure of the ear (Drake et al: Gray's Anatomy for Students)

person to person. Therefore, an ear probe should be designed to fit in a variety of in ear canal shapes and sizes.

The secluded nature of the ear canal means that it has a relative constant temperature. Air trapped in the canal by a plug of high thermal resistance will reach thermal equilibrium close to the temperature of the canal wall and tympanum. This is a better location for a core temperature measurement, but will still be influenced by the ambient temperature.

The wall of the ear canal is well supplied with blood. Blood vessels just beneath the thin layer of skin makes the ear canal a possible location for measuring heart rate and blood oxygen saturation. The still nature of the head will minimize movement artefacts.

The ear canal extend toward the brain and electrical brain activity is present due to the conductive nature of the tissue. According to Nunez and Srinivasan (2006) currents from brain potentials can be focused through holes in the skull, like the ear and nose. The farther away the origin of the signal is from the electrode, the weaker the measured signal will be. Therefore, an electrode in the ear canal will detect electrical brain activity near the ear better, including the temporal lobe and brain stem.

2.1.3 Tympanic Membrane

The tympanum forms the medial boundary of the external ear canal. It is a smooth elliptical membrane with a thickness of about 0.074 mm (Alvord and Farmer, 1997). The membrane is slanted with regards to the external ear canal.

As with the rest of the external ear, the tympanum is supplied with blood from a branch of the carotid artery, therefore sharing its supply with the brain including the hypothalamus, the thermoregulation centre of the body. It is the most medial part of the external ear, and is therefore the least susceptible to influence by the ambient temperature. This is the reason that the tympanum is one of the best locations to measure core body temperature. The location is used by physicians to measure core temperature for it is quick and minimally invasive. Variations in body temp can be sensed faster on the tympanic membrane than on other locations on the body. Contact with the tympanum can cause discomfort and harm to the patient, so non-contact infra-red thermometers are usually used.

2.2 Medical Sign Physiology

This section reviews the theory and research done about the physiological aspects of each medical sign that the Ear-Monitor is required to measure. The importance of each of the five medical signs will be discussed, including the typical range of measurements expected from healthy adults and the causes and implications of deviations from these healthy measurements.

2.2.1 Core Temperature

Thermoregulation is the body's way of keeping its internal temperature within certain bounds to create a favourable environment for chemical reactions to take place. The temperature control centre of the body is in the hypothalamus and it regulates temperature by maintaining a fine balance between heat production and heat loss. Normal human core temperature varies between 36.5°C and 37.5°C (Jones, 2010). Inability to maintain this balance may indicate problems in the well-being of a person. Elevated temperature (hyperthermia) due to a fever can indicate the presents of an infectious disease. Abnormally low temperature (hypothermia) can be caused by cold exposure, metabolic disorders or infection. Both hyper- and hypothermia can be life threatening. A core temperature measurement is often a key indication to start a treatment or not. Therefore, temperature measurement is part of a full clinical examination and part of the vital sings group of medical signs.

The location where temperature is measured is a key factor, for temperature is not constant throughout the body. This is because heat production and heat loss are not constant throughout the body, meaning extremities are usually cooler than the core. Traditional locations for measuring temperature are the tympanic membrane, axilla, mouth, rectum, oesophagus, forehead and urinary bladder. The mean temperature of these areas varies as well. A systematic literature review done by Sund-Levander *et al.* (2002) combined the results of

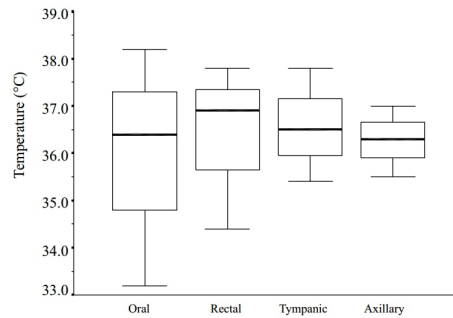


Figure 2.3: The results from 20 studies with strong or fairly strong evidence of normal oral, rectal and tympanic temperature ($^{\circ}\text{C}$) in adult men and women are presented. Temperature is obtainable as mean value (bold lines), 1st and 3rd quartiles (unfilled bars) and range (thin lines).

20 studies to identify oral, rectal, tympanic and axillary temperature ranges in healthy humans. Table 2.3 shows the results.

Studies have also been done comparing measurements at distinct locations to pulmonary artery temperature in ill patients. A study has shown ear-based $0.07 \pm 0.41^{\circ}\text{C}$; urinary bladder $0.03 \pm 0.23^{\circ}\text{C}$; oral $0.05 \pm 0.26^{\circ}\text{C}$; and axillary $-0.68 \pm 0.57^{\circ}\text{C}$. The accuracy of each method varied with the level of pulmonary artery temperature. Repeated measurements with all four methods had mean standard deviation values within $\pm 0.2^{\circ}\text{C}$ (Erickson and Kirklin, 1993).

A second study done by Lefrant *et al.* (2003) showed the following results: oesophageal $0.11 \pm 0.30^{\circ}\text{C}$, rectal $-0.07 \pm 0.40^{\circ}\text{C}$, axillary $0.27 \pm 0.45^{\circ}\text{C}$, inguinal $0.17 \pm 0.48^{\circ}\text{C}$, urinary bladder $-0.21 \pm 0.20^{\circ}\text{C}$.

The location of the device in development is restricted to the ear, therefore the tympanic membrane is the preferred location to take temperature measurements. The referenced studies show that the tympanic membrane is a valid location to measure accurate core temperature.

2.2.2 Heart Rate

The presence of a heart beat is paramount to sustain the vital cardiac output, supplying blood to the whole body. Heart rate can be controlled or maintained through two different regulatory systems: The intrinsic conduction system and the nervous system. The intrinsic conduction system works through the rhythmic contraction and relaxation of the heart muscle tissue. The heart rhythm is regulated by the sinoatrial node. The nervous system can influence the heart rate through sympathetic and parasympathetic nerves running from the cardiovascular centres in the medulla oblongata to the heart. The heart beat rate is varied to control the blood flow and blood pressure in the body.

The heart is the source of a group of biosignals. The firing of nodes and propagation of electrical charges through neurons and the conductive cardiac muscle gives of an electrical signals that can be detected. The contraction of the ventricles forces blood into the arteries, causing a temporary increase in blood pressure. This pressure increase propagates through the arteries as a wave, causing a temporary local increase on blood volume. Pressure- and volume changes can be detected. Blood turbulence and the opening and closing of heart valves causes the characteristic heart sound and chest movements, both indications of heart rate.

Heart rate is influenced by numerous physiological factors including O_2 , CO_2 , H^+ levels, blood pressure, stress and exercise. Pathological factors can include fever, sepsis, heart disease and anaemia. Tachycardia is abnormally high resting heart rate, generally above 100 bpm, whereas bradycardia is a lower than normal resting heart rate, usually below 60 bpm (Laskowski, 2015). Although these two conditions are not necessarily danger signs, it may be an indication of health problems and therefore heart rate measurement is part of any medical examination and one of the vital signs group of medical signs.

2.2.3 Respiratory Rate

Respiration is the first step in the chain of events to get oxygen to the body's cells for metabolism to provide the body with energy. Respiration ventilates the lungs with air through inhalation and exhalation. The respiratory rate of a healthy adult at rest is usually between 12 and 20 breaths per minute (Charbek, 2015). This can vary drastically if the body is experiencing physical or emotional stress. In increase in respiratory rate can be cause by a fever, pulmonary dysfunction or any one of numerous medical conditions. Respiratory rate is also part of the vital signs group of medical signs.

Respiratory rate monitoring is especially useful for diagnosing sleep apnoea. Symptoms include regular pauses in respiration or periods of shallow breathing (hypopnea) during sleep. This causes an oxygen deficiency in the body and lowers the quality of sleep. Short term symptoms include excessive daytime sleepiness, morning headaches, impaired alertness, and vision problems. If left untreated sleep apnoea can lead to high blood pressure, diabetes, depression, worsening of ADHD, stroke, heart failure, irregular heartbeats, and heart attacks (Blahd, 2016). Sufferers may be unaware of their condition and a sure-fire method of diagnosing it is my monitoring respirator rate during sleep, traditionally done during an overnight sleep study.

2.2.4 Blood Oxygen Saturation

Haemoglobin is the oxygen transporter protein found in the red blood cells of blood. Blood gets oxygenated in the lungs and then carries O_2 to the rest

of the body for aerobic respiration necessary to produce energy. The correct levels of oxygen in the blood is vital to the health of the individual.

Oxygen saturation, SO_2 , refers to the concentration fraction of oxygenated haemoglobin to total concentration of haemoglobin in the blood:

$$SO_2 = \frac{C(HbO_2)}{C(HbO_2) + C(Hb)}$$

Where $C(HbO_2)$ is the concentration of deoxygenated haemoglobin (de-oxyhaemoglobin) and $C(Hb)$ is the concentration of oxygenated haemoglobin (oxyhaemoglobin).

Blood oxygen saturation of 95-100% is normal in healthy humans. Hypoxaemia is the condition when the saturation is below 90%. This can be an indication of circulatory or ventilatory problems, anaemia or sleep apnoea. Levels below 80% can hinder organ function and can lead to organ failure and cardiac- or respiratory arrest. The brain is extremely susceptible to damage due to a lack of oxygen. Cerebral hypoxia is the insufficient supply of oxygen to the brain. This can cause brain damage and in severe cases, brain death.

2.2.5 Electrical Brain Activity

EEG, or electroencephalography, is the non invasive recording of the electrical activity in the brain over time. The neurons in the brain conduct electrical current

Bickford (1987)

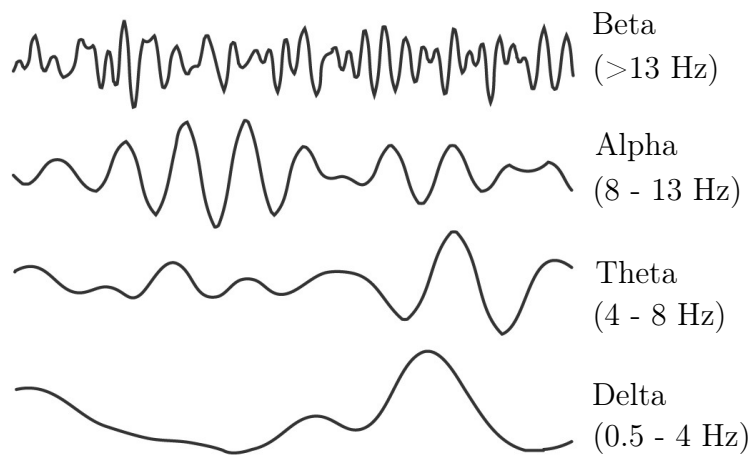


Figure 2.4: EEG rhythms

Chapter 3

Theory Literature Review

This chapter will accumulate a thorough understanding of the theory and current state of technology relevant to the measurement of each medical sign required of the Ear-Monitor. Attention will be given to the different methods available to determine each medical sign. This section will also make reference to various articles and studies done by other researchers in this field of study. The aim is to gather all the relevant information in order to make an informed selection of the methods and sensors the Ear-Monitor will use to measure each medical sign.

3.1 Core Temperature

Various methods are available for measuring core temperature. Non-electric, fluid-filled thermometers was the first to be used. The mercury-filled thermometer was used by early physicians to study the thermoregulation of the human body and crudely identify fevers. Since then, the mercury has been replaced by coloured alcohol or another heat sensitive liquid, due to toxicity of mercury.

Another type of fluid-filled thermometer is the liquid-crystal thermometer. It contains liquid crystals that changes colour when at different temperatures. The use of these two types of fluid-filled thermometers has decreased significantly due to the accuracy, speed and convenience of digital thermometers.

Electrical thermometers are now the industry standard of measuring core temperature. Central to any digital thermometer lies a transducer that convert temperature to an electrical signal. Resistance temperature detectors, thermocouples thermistor and thermopiles will be discussed. They can be divided into contact and non-contact thermometers.

3.1.1 Contact Thermometers

These are a family of thermometers that measure their own temperature with the assumption they and the object whose temperature is of interest, are in thermal equilibrium. Therefore, they are usually placed in contact with the object. When using a contact thermometer in the ear, the sensor part of the thermometer can be placed in contact with the ear canal wall, the air inside the canal or with the tympanic membrane self.

3.1.1.1 Resistance Temperature Detector

Resistance temperature detectors (RTDs) uses the temperature-resistance relationship for metals to measure temperature. Thin wire coils or films of platinum, copper or nickel are usually preferred for they have a stable and repeatable temperature-resistance relationship over a large temperature range.

3.1.1.2 Thermocouple

Thermocouples make use of the thermo-electric effect to make a temperature measurement. They consist of two dissimilar conductors connected at the one end, known as the hot junction (measuring junction). The other ends of the two wires are known as the cold junction (reference junction) and are connected to a voltage meter via common conductors. A voltage is generated dependant to the temperature difference between the measuring- and reference junctions. Thermocouples do not respond to absolute temperature; therefore, their accuracy depends on how well the reference temperature can be defined. Reference temperatures are usually determined by a precise thermistor. Thermocouples are very versatile and widely used in clinical applications, but the downsides are that their output signal is low and non-linear, therefore requiring a sensitive and stable voltage measuring device (Jones, 2010).

Thermocouples can be connected in series and are then called thermopiles. This configuration sums the output voltages, resulting in temperature averaging. This method improves accuracy by reducing noise.

3.1.1.3 Thermistor

A thermistor is a type of semiconductor whose resistance varies with changes in temperature. They differ from RTDs in that they are usually made of ceramics, they have higher precision over a smaller temperature range and they can have a negative relation to temperature. Thermistors are preferred above RTDs and thermocouples for use as biomedical sensors due to their faster response time and higher sensitivity over a smaller range and. The smaller range does not matter, for the temperature range of interest in biosensors are small and well defined.

3.1.1.4 Contact Thermometer Application

In the case of RTDs and thermistors, the measuring element is placed in position and a current is sent through the sensor. By measuring the voltage across the resistive element, it is possible to calculate the resistance and subsequently determine the temperature. In the case of the thermocouple, the hot junction can be placed in contact with the canal wall or tympanum. Typically, the hot junction will be enclosed with a soft material to protect the canal and tympanum. The canal is sealed off and time is allowed for the area to equilibrate to tympanic temperature.

Placing a thermometer in contact with the tympanic membrane will give an accurate measurement, but can cause discomfort to the wearer. There is also a risk of harming the tympanic membrane. Sensors in contact with the ear canal wall or the air inside the canal run the risk of making errors by measuring the temperature of objects that are not in thermal equilibrium with the tympanic membrane. Therefore, non-contact thermometers will be considered.

3.1.2 Non-contact Thermometers

Thermopiles can be used to detect thermal radiation without being in contact with the object. All matter with temperatures above 0 K radiates electromagnetic radiation according to the Stefan-Boltzmann law. The thermal radiation, Q , per unit area is given by the equation:

$$Q = \varepsilon \sigma T^4.$$

Where ε is the emissivity, σ the Stefan-Boltzmann constant and T the temperature of the object.

The wavelength distribution varies according to the temperature of the object and is described by Planck's law:

$$B_\lambda(\lambda, T) = \frac{2hc^2}{\lambda^5} \frac{1}{e^{\frac{hc}{\lambda k_B T}} - 1}.$$

Where B_λ is the spectral radiance, λ the radiation wavelength, h Planck's constant, k_B Boltzmann's constant c the speed of light and T the object's temperature. Through maximizing B_λ , it is possible to find the dominant wavelength that is emitted at a certain temperature. Figure 3.1 shows a plot made of spectral radiance versus wavelength at $T = 37^\circ\text{C}$, the core temperature of humans. It can be seen that the dominant wavelength is at $9.35\ \mu\text{m}$. This is in the infrared range, and therefore this type of thermal radiation thermometer is called an infrared thermometer.

In the case of measuring the temperature of the tympanic membrane, the hot junction's temperature will be determined by the radiation received from the tympanum minus the radiation radiated by the sensor self.

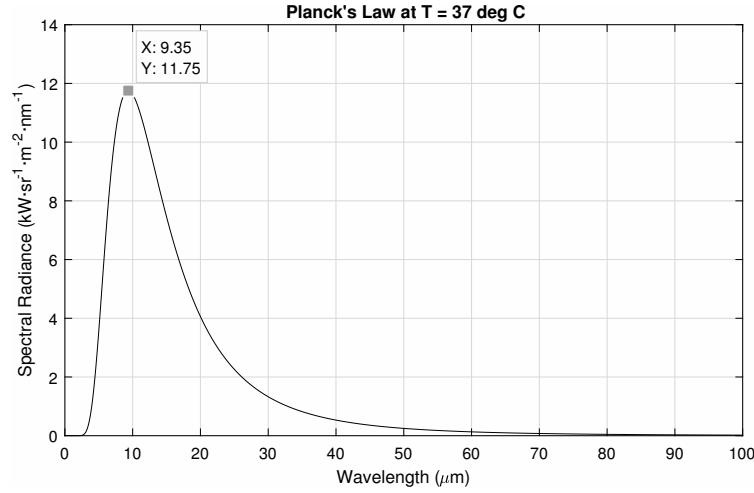


Figure 3.1: Plot showing how Planck's law can be used to determine the dominant radiation wavelength at certain temperature

When talking about thermal radiation, an important aspect is emissivity. Emissivity is the ability of an object to radiate thermal energy. It is quantified as a ratio of thermal energy emitted by a surface relative to the thermal energy emitted by an ideal black body at the same temperature. A black body is an idealized surface that reflects no radiation, meaning all energy radiated from the surface are due to the temperature of the surface. Thus, a black body have an emissivity of 1 and have the maximum theoretical radiation at a given temperature. The accuracy of an infrared sensor depends on the ability of the object to emit sufficient thermal radiation for the sensor to detect. Cross-referencing various emissivity tables, it was found that the emissivity of human skin is 0.98, meaning that it is an excellent emitter of thermal energy (Stumme *et al.*, 2003) (ThermoWorks) (Optotherm, 2017). The ear drum is covered with skin, making it an ideal target object for a non-contact thermometer.

An infrared thermometer generally consists out of a thermophile attached to a blackbody and shielded by an infrared filter that also acts as a lens to focus infrared waves (Karaki and Polyziev, 2014). This setup, shows in Figure 3.2, allows for the non-contact temperature sensing of the tympanic membrane. Unlike pulse rate, breathing and electrical brain activity, the core body temperature varies slowly. It takes minutes to vary significantly. Therefore, the sampling period of core temperature can be as long as 10 seconds.

3.1.3 Commercial Temperature Monitoring Devices

Ear thermometers are widely used at home and in hospitals. Ear contact thermometers like Novatemp[®] and Starboard[®] claims a ± 0.2 °C accuracy. Non-contact infrared ear thermometers usually have a similar rated accuracy. None of these are, however, wearable devices.

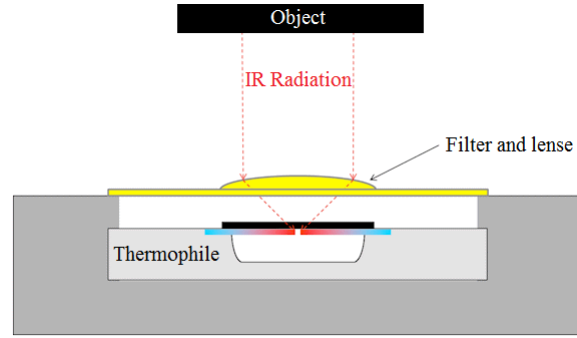


Figure 3.2: IR Thermometer diagram (V Polyzoev et al: Demystifying Thermopile IR Temp Sensors)

The *degree*[°], Figure 3.3, is a continuous in-ear thermometer for children, developed by *cosinuss*[°], a company specialising in wearable sensors. The bulk of the device is worn behind the ear, and there is a wire running over the auricle to the ear canal, in which a probe is placed. The device takes its temperature measurements with a sensor placed in contact with the canal wall. The manufacturer claims an accuracy of ± 0.1 °C. It monitors temperature continuously and sends real time data to a mobile phone.

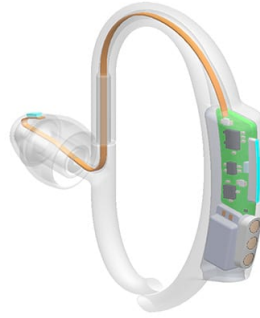


Figure 3.3: CAD model of the *degree*[°] from the *cosinuss*[°] website (include ref)

Apart from the *degree*[°], there are not much literature on wearable ear thermometers. Two patents were found describing similar devices: US 6556852 B1 and US 20090221888 A1. The first of which proposes the use of an infrared sensor pointed at the tympanic membrane, and the latter not specifying the method of measuring. Hopefully, the tests planned for this study can add to this insufficient body of knowledge.

3.2 Heart Rate

The heart is a very dynamic organ whose influence can be felt throughout the body. Therefore there are many options available to monitor heart rate. Electronic monitoring methods include electrocardiography (ECG), photoplethysmography (PPG), ballistocardiography (BCG), phonocardiography and doppler flow-meters.

3.2.1 Electrocardiography

ECG is a recording of the electrical activity of the heart over a period of time. Electrical activity arise from the depolarization and repolarization of the heart muscle during the cardiac cycle. The most prominent electrical charge is the QRS complex, which corresponds to the ventricular depolarization and is visible on the electrocardiogram as a sharp peak in the millivolt range. ECG is the the recommended way of monitoring heart rate in most intensive care units. A cardiologist will use a 12 lead ECG with 10 electrodes placed in a specific configuration on the chest. Various wearable devices use ECG to measure heart rate. Fitness monitors normally uses a chest strap with electrodes to detect the heart's electrical activity. Studies have been done developing wearable ECG devices for clinical use.

The latest in wearable ECG electrodes is the use of dry polymer-based materials (Wang *et al.*, 2010) or non-contact electrodes that can be place on top of clothing (Lin *et al.*, 2013). This is an improvement above the standard conductive gels or adhesives and can be used repeatedly. But these electrodes still needs to be place on the chest.

An ear located ECG monitor have been developed by Winokur *et al.* (2012). This device uses a single lead set-up with one electrode place on the mastoid bone behind the ear and a reference electrode placed on the neck. This configuration relies on the conductive properties of human tissue to carry electrical charges form the heart to the ear. They where able to used the electrocardiogram in conjunction with PPG and BCG to determine various heart intervals and track changes in mean arterial blood pressure. Figure 3.4 shows Winokur *et al.* (2012)'s device and a plot of its electrocardiogram. No heart rate information was extracted.

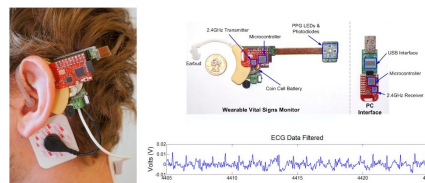


Figure 3.4: Ear-worn device developed by Winokur *et al.* (2012)

3.2.2 Photoplethysmography

PPG produces an optically obtained plethysmogram, which is a plot of volume the change of an organ over time. PPG can be used to measure the change in the volume of blood vessels close to the skin surface. When the left ventricle contracts a pressure pulse propagates through the arteries from the heart to the extremities of the body. This wave corresponds to the systolic blood pressure. Blood vessels walls contain elastic fibres that allow them to stretch. This means that the diameter of vessels will increase when the blood pressure increase, causing arteries to stretch and contract with each cardiac cycle. PPG can be used to determine heart rate by measuring this volumetric variation.

A photoplethysmograph can non-invasively determine peripheral arterial blood volume by shining light through the skin surface, into the dermis and subcutaneous tissue and collecting the light transmitter or reflected. Light shined into the tissue can either be reflected, absorbed or allowed to transmit through. This leads to the two modes of PPG operation depicted by Figure 3.5.

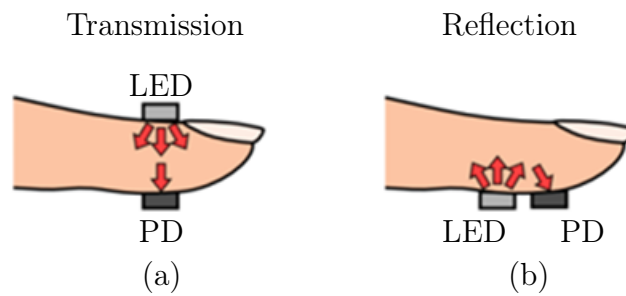


Figure 3.5: The two modes of Photoplethysmography (Tamura *et al.*, 2014)

In (a) the emitter and detector faces each other and are separated by tissue that can transmit the light, leading to a transmission mode PPG. Transmittance mode PPG is limited to locations on the body where transmitted light can be detected, like the finger, ear lobe, concha and tragus. These locations have limited blood profusion, especially at low temperatures. In (b) the emitter and detector is placed on the same plane and both faces toward the tissue. Light from the emitter is reflected by the tissue and captured by the detector, leading the reflection mode PPG. The emitter and collector needs to be optically isolated so that light cannot pass from the one to the other without going through the tissue. Reflectance mode PPG can be used at more locations, but they are more susceptible to motion artefacts (Tamura *et al.*, 2014).

According to Lambert's law, the amount of light absorbed is proportional to the length of the path that the light must travel in the absorbing substance (Encyclopædia-Britannica). Therefore, a change in blood vessel diameter will increase the distance the light must travel causing a change in light absorption.

This can be detected by measuring reflected or transmitted light. Variation in the light reflected or transmitted will be synchronised with the heart rate.

Shorter light wavelengths are mostly absorbed by the tissue, while longer wavelengths can penetrate deeper. Red and near infrared light are preferred for transmission PPG. While green light is becoming more popular for shallow reflectance PPG, due to larger light variations during the cardiac cycle and less noise than near infrared PPG (Tamura *et al.*, 2014).

The signal read by the photo detector of the pulse oximeter consists of a AC component superimposed on a DC signal. The DC component is the due to the constant transmission or reflection of light by the body's tissue: skin, fat, venous blood and the non-pulsating arterial blood. The AC components is the variation in transmitted or reflected light due to the change in diameter of the arteries and therefore, synchronised to the heart rate. The AC component is usually between 0.5 - 2% of the DC component (Tavakoli Dastjerdi, 2006). Figure 3.6 illustrates the way in which the heart rate is visible in a photoplethysmograph. It can be seen that the blood volume increase with each heartbeat, and that this causes more light to be absorbed, thus less detected by the photodiode.

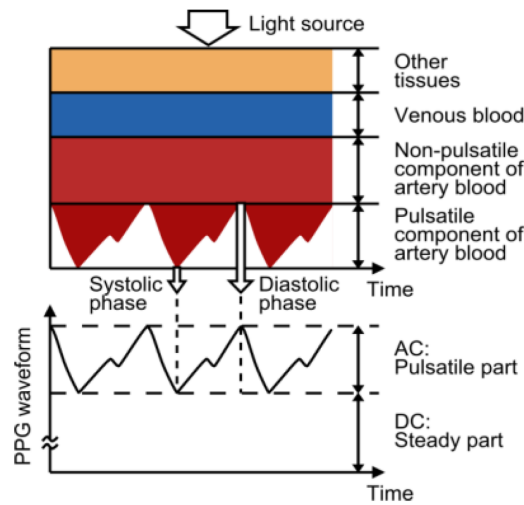


Figure 3.6: Basic operating principles of PPG (Tamura *et al.*, 2014)

3.2.2.1 Work done by others in Ear PPG

At this point, PPG is the most attractive option for the Ear-Monitor to measure heart rate and it is given extra attention during the literature review. A review of work done by others in the field of ear PPG revealed six devices relevant to this study.

Shin *et al.* (2009) presents a wearable music headset with an integrated transmission PPG ear clip that attaches to the ear lobe. The device includes an accelerometer to aid in the removal of motion artefacts. Evaluation was done through a study comparing the HR from the device to that made with a conventional ECG recorder. This study revealed a heart rate error of 0.6% was found.

Poh *et al.* (2010) designed a wearable PPG with a magnetic earring sensor. The bulk of device sits in front ear canal and held in place by the auricle. A reflective PPG sensor is held against the ear lobe by placing a magnet on the opposite side. The device also includes an accelerometer to make baseline measurements for motion artefact cancellation. A study was conducted to compare the PPG signals measured by the wearable device to chest ECG signals collected by a FDA-approved commercial system. Whilst standing motionless, the study found a very high agreement between the ear PPG and the chest ECG with a mean bias of $0.62 \pm 4.51\%$ with ECG reference measurements.

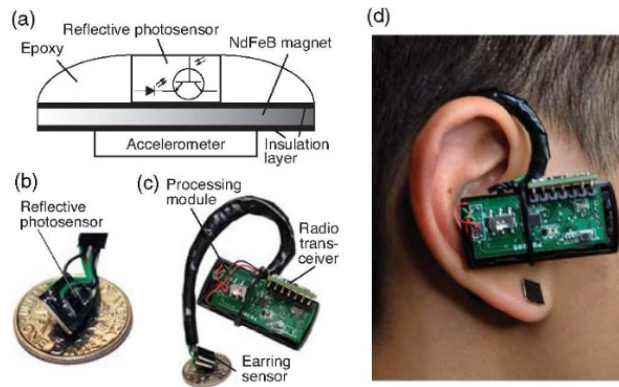


Figure 3.7: Pulse oximetry diagram (Poh *et al.*, 2010)

Da He *et al.* (2010) researched an ear worn heart rate monitor containing PPG sensor in reflectance mode. Red light is shined into the tissue behind the ear and collected by a photodiode chip with an integrated transimpedance amplifier. Signals were not digitalised on the device, but recorded and processed on MATLAB. They compared their collected signal with a transition finger PPG and a chest ECG. Figure 3.8 shows this comparison.

Winokur *et al.* (2012) developed a similar device that shines 660nm and 940nm light waves through tissue at the mastoid bone and collecting the reflected light with 4 photodetectors. A PPG front end conditioned the signals and their device sent the raw heart beat information to a PC through a radio connection. This is the same device that records ECG and is used to analyse heart intervals and mean blood pressure rather than heart rate.

Buske *et al.* proposed yet another location. They modified a pair of headphones to measure a transmission PPG from the concha. During the testing

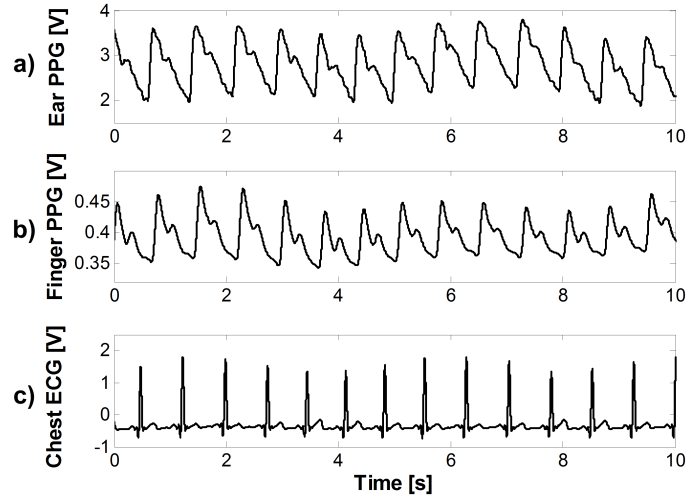


Figure 3.8: Pulse oximetry diagram (Da He *et al.*, 2010)

phase, the device showed an average heart rate accuracy of around 85% when compared to an ECG.

The *cosinuss° one*[®] is a commercial device that monitors heart rate through the ear canal. The earpiece presses against the ear canal wall and records a PPG in reflection mode. It is marketed to athletes that want to monitor their bodies during exercise.



Figure 3.9: <https://www.cosinuss.com/en/products/one>

3.2.3 Ballistocardiography

BCG is the measurement of the mechanical effects of the beating heart on the body over time. Typically accelerometers or pressure sensors will be used

to measure movement or forces on the surface of the body. BCG has been researched for use in ear heart rate extraction.

In a wearable device proposed by Da He *et al.* (2010), mechanical vibrations associated with heart rate are converted to electronic signals through capacitive sensing electrodes placed behind the ear. This method works by measuring the change in capacitance between the two electrodes as the distance between them changes due to heart rate vibrations.

A study by Winokur *et al.* (2012) proposed measuring the head-to-foot axis recoil due to the blood-volume shift during cardiac ejection. This is done by placing an MEMS accelerometer behind the auricle. Due to the movement dependent method of operation this technology is extremely susceptible to motion artefacts and it can only be used during which the body is stationary.

A variation of this technology is discussed in a article by Park *et al.* (2015). They propose using a scissor shaped hinge mechanism in the ear canal that measures the change in the canal size due to the in-ear blood pulse waves. The mechanical movement is converted to an electrical signal through a piezoelectric film sensor. Figure 3.10 shows an drawing of this device from Park's 2015 article.

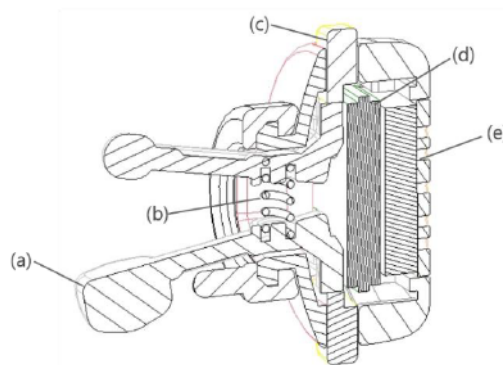


Figure 3.10: Device to measure in ear pulse waves due to the heart beat
(Park *et al.*, 2015)

3.2.4 Other Heart Rate Methods

Electronic stethoscopes uses an microphone to record heart sounds. The hears makes a distinct series of sounds during the cardiac cycle due to blood turbulence and the shutting of heart valves. The period of this sound series can be used to determine heart rate and does not require skin-contact.

A Doppler flow-meter can be used to detect the alternating blood current component in near-surface arteries. This component is synchronised to the

heart rate frequency. The device can use ultrasound, microwaves or light to achieve the Doppler shift.

3.3 Respiratory Rate

Unlike the other medical signs, a person cannot measure his or her own respiratory rate. As soon as a person is consciously thinking about respiration, breathing usually slows. Measuring needs to happen while the person's thoughts are otherwise occupied. Therefore, a continuous measuring method are preferred. Typically, a nasal mask or chest strap will be used to measure respiration.

3.3.1 Respiratory Rate Ear Sensors

Ear located devices that extract respiration information are rare, but some literature sources are available.

Goverdovsky *et al.* (2016) tested an ear probe with two embedded microphones. The microphones could detect the sound created by turbulence in the airways for breathing rates higher than 12 breaths per minute. Figure 3.11 shows a plot of the normalised sound amplitude at two different breathing rates. Variation during breathing can be seen in both recordings.

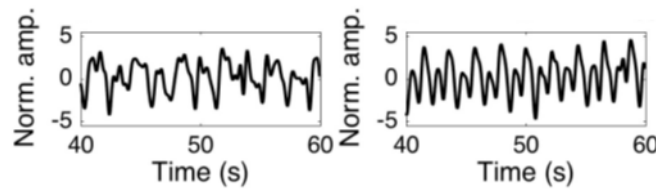


Figure 3.11: Breathing detected through microphones inside the ear canal (Goverdovsky *et al.*, 2016)

Da He *et al.* (2010) did extensive research on the ear as a location for medical sign monitoring. They extracted respiratory rate from baseline oscillations in a BCG signal recorded by capacitive electrodes placed behind the ear. Mechanical movement is converted to electrical signals by these electrodes. Therefore, the movement of the head due to respiration is seen on the BCG as baseline oscillations, Figure 3.12.

3.3.2 Respiratory related Heart Rate Characteristics

A different approach is to extract respiratory rate by looking at the heart rate. A PPG signal contains three distinct respiratory related characteristics:

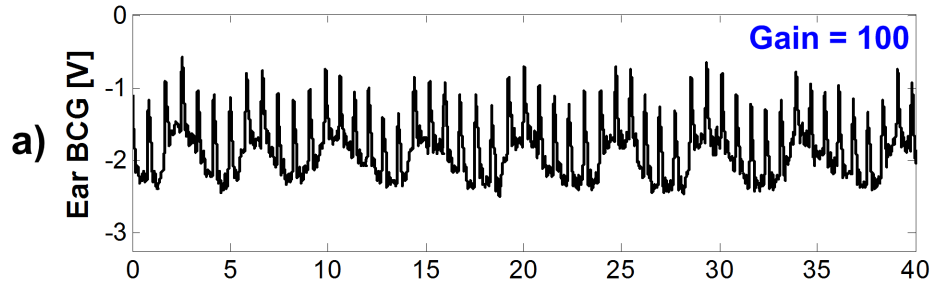


Figure 3.12: Baseline oscillations in behind the ear BCG due to breathing (Da He *et al.*, 2010)

amplitude modulation (AM), respiratory-induced intensity variation (RIIV) and frequency modulation (Johansson, 2003).

Amplitude modulation is due to blood pressure changes during the respiratory cycle called Pulsus Paradoxus. RIIV is changes in the volume of the dermis and subcutaneous capillary bed. It is visible as baseline variation in the PPG signal. Frequency modulation of the heart rate synchronised to respiration rate, called respiratory sinus arrhythmia (RSA).

RSA can also be detected in ECG, but differ from the fluctuations seen in chest ECG, due to electrodes movement relative to the heart and changes in chest impedance during the respiratory cycle (Moody *et al.*, 1986). These fluctuations cannot be detected in the ear. RSA is observed as baseline oscillation in heart rate in synchrony with the respiratory rate. Heart rate increase during inspiration and a decrease during expiration (Yasuma and Hayano, 2004). According to a study done by Stratton *et al.* (2003), the variation in heart rate due to RSA is higher in younger test subjects with 74% increase in children vs. 52% increase in adults.

Research was been done to develop algorithms to utilise these characteristics to extract respiratory rate from PPG signals. Clifton *et al.* (2007) used wavelet analysis, achieved a respiratory rate accurate to within 1 breath per minute and Leonard *et al.* (2006) documented a respiratory rate error of 7.9%. Johansson (2003) developed two neural network algorithms that uses the different respiratory related characteristics of PPG signals to detect breaths. Table 3.1 shows the results of the best algorithm.

3.4 Blood Oxygen Saturation

Oxygen saturation can be measured by means of an arterial blood gas test resulting an arterial oxygen saturation reading. This requires drawing a blood sample for testing and therefore is not relevant to this study. An alternative method is pulse oximetry. This method estimates peripheral capillary oxygen

Table 3.1: Results of the respiratory rate extraction through neural networks (Johansson, 2003)

Respiratory Related Characteristics	False Positive (%)	False Negative (%)
RSA	3.7	6.9
AM	5.2	4.7
RIIV	5.2	5.9

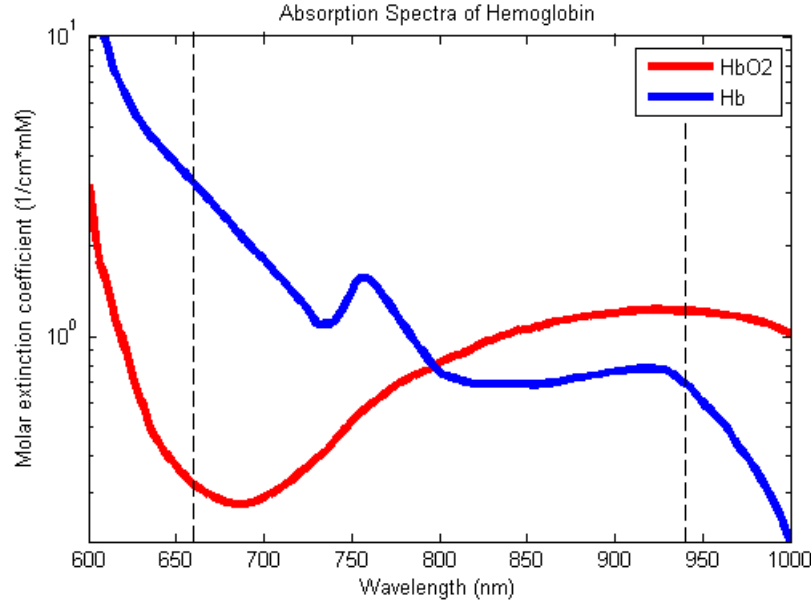


Figure 3.13: Absorption spectra of oxy- and deoxyhemoglobin

saturation, SpO_2 , through the spectrophotometric analysis of PPG signals captured at two different wavelengths. This is a clinically excepted estimation of the arterial oxygen saturation.

3.4.1 Pulse Oximetry Theory

Blood oxygen saturation estimation through pulse oximetry relies on the different adsorption spectra of oxyhaemoglobin and deoxyhaemoglobin. Figure 3.13 shows the absorption spectra of oxy- and deoxyhaemoglobin.

It can be noted that deoxyhaemoglobin has a significantly higher absorption of red light while oxyhaemoglobin has a slightly higher absorption of infrared light.

According to Beers law, the amount of light absorbed by a dissolved substance is proportional to its concentration (Encyclopædia-Britannica). Therefore, oxygenated blood (with a higher concentration of oxyhaemoglobin) will

absorb more infrared light and reflect more red light. Whereas deoxygenated blood (with a higher concentration of deoxyhaemoglobin) will absorb more red light and reflect more infrared light. This explains why oxygenated blood appears bright red, while deoxygenated blood is a darker shade of red.

Red and infrared light are shined into the peripheral tissue and the light reflected or transmitted is measured for both wavelengths. Literature and commercial devices usually uses wavelengths of 660 nm (red) and 940 nm (near infrared) (Tytler and Seeley, 1986) (Chan and Underwood, 2005) (Bagha and Shaw, 2011) (Bheema lingaiah *et al.*, 2013) (Duun *et al.*, 2007). The ratio of reflected or transmitted light is unique to a certain level of blood oxygen saturation and is used to estimate blood oxygen saturation.

The Beer-Lambert law describes the absorption of a specific wavelength of light by a substance in a homogeneous solution (Bagha and Shaw, 2011).

$$A = \varepsilon cL = \ln \left(\frac{I_o}{I} \right)$$

$$I = I_o e^{-\varepsilon \lambda cL}$$

Where A is the dimensionless adsorption, ε is the wavelength dependant molar absorptivity, c is the concentration of the substance and L is the path length the light needs to travel through the substance. I_o is the intensity of the light entering the solution and I is the intensity of light passing through the solution.

When applying this law to measuring O_2 saturation, a concentration ratio can be calculated. Factoring out L , I_o , and the constants in ε , the ration can be written as:

$$R = \frac{\log(I_{red}) \cdot \lambda_{red}}{\log(I_{ir}) \cdot \lambda_{ir}}$$

Where I is the light intensities and λ is the wavelength (Chan and Underwood, 2005). Red and infrared light sources are alternated and intensity measurements are made for both separately.

In practice, a different modulated relationship is used to compensate for the different DC absorption between patients (König *et al.*, 1998) (Duun *et al.*, 2007) (Bheema lingaiah *et al.*, 2013) (Bagha and Shaw, 2011) (Nitzan *et al.*, 2014) (Oak and Aroul, 2015)

$$R = \frac{\left(\frac{AC}{DC} \right)_{red}}{\left(\frac{AC}{DC} \right)_{IR}}$$

This ensures that the O_2 saturation of only the arterial blood is calculated. The ration can be checked against an empirical determined curve. The standard formula for this curve is found in literature as $\% SpO_2 = 110 - 25R$, (Oak and Aroul, 2015) but it can vary from device to device.

As mentioned, SpO_2 can be calculated using reflected or transmitted light. Light that is not absorbed or scattered by tissue can be either reflected, or transmitted. Thus, both reflected and transmitted light is proportional to the mount of light absorbed. Transmittance mode pulse oximeters are more common, but their use is restricted to parts of the body that will allow for light to pass through, like a fingertip or earlobe.

A big challenge to conventional pulse oximeters is noise due to movement (Barker *et al.*, 2002).

3.4.2 Work done by others in ear pulse oximetry

Standard locations for pulse oximetry includes the fingertip, earlobe, ankle and forehead. A study comparing fingertip and earlobe pulse oximetry to an arterial blood gas test found that finger pulse oximetry differed by a mean of -0,71% and earlobe pulse oximetry differed by a mean of +4.2% (Olive *et al.*, 2016). Literature and commercial wearable pulse oximeters typically utilise a finger clip to measuring SpO_2 (Watthanawisuth *et al.*, 2010) (Pujary *et al.*, 2003) (Huang *et al.*, 2014) (Khalifa *et al.*, 2014). This location is not ideal for continuous monitoring and is especially susceptible to motion artefacts. Although the fingertip location is not of interest to this study, the literature is still reviewed for similar principals can be applies to ear pulse oximetry.

Ear lobe pulse oximetry usually done through a sensor that clips to the ear lobe, which is attached to a stationary device. Wearable ear pulse oximetry, is still novel and not well covered in literature. There are some patents filled for such devices (US 20050177034 A1) (US 4086915 A) (US 3412729 A) (US 6556852 B1) and commercial devices like but little academic material is available.

A study done by (Aziz *et al.*, 2006) tested a wireless earlobe-mounted pulse oximeter on a group of subjects. Subjects were tested while sitting, walking and running. During the sitting and walking phases they recorded an SpO_2 reading of above 95%, which is “as expected” according to them. But during the running phase they could not obtain any accurate reading.

During running, they could not take an SpO_2 reading, but Literature on ear PPG, only uses infrared light to determine heart rate. Theoretically, infrared light can be added in the same way to produce and red PPG and a R value can be calculated to estimate SpO_2 .

Pulse oximetry patch

3.5 Electrical Brain Activity

Chapter 4

Concept Design

This chapter builds upon the knowledge gained in the literature review and explains the logic used to select the methods and sensors to realize each medical sign monitoring requirement of the Ear-Monitor. Selections will be made by analysing advantages and disadvantages of each option and combining it with sound engineering judgement.

4.1 Temperature

The Ear-Monitor will measure core temperature from the inside of the ear canal. The main limitations are sensor size and measurement accuracy. The method selection and sensor selection is discussed separately.

4.1.1 Temperature measurement method

Two temperature measuring method were considered, namely contact- and non-contact thermometers.

4.1.1.1 Contact thermometers

A contact RTD, thermocouple or thermistor is placed in contact with the canal wall, canal air or tympanic membrane.

Table 4.1: Contact thermometers evaluation

Image	Advantages <ul style="list-style-type: none"> • Available in small sizes, ideal for the size restrictions of the ear canal. • Good accuracy. • Converting transducer's voltage to temperature is simpler than with non-contact thermometers.
Sensor size: 0.5×2.3 mm Measurement accuracy: 0.15 °C	Disadvantages <ul style="list-style-type: none"> • Canal wall and canal air temperature measurements can easily be influenced by ambient temperature. • Tympanic membrane contact can cause discomfort and harm to the wearer. • More time is needed to take measurement, for sensor needs to be in thermal equilibrium with the object.

4.1.1.2 Non-contact Thermometers

A non-contact, infrared sensor is placed inside the ear canal and pointed at the tympanic membrane.

Table 4.2: Non-contact thermometers evaluation

Image	Advantages <ul style="list-style-type: none"> • The sensor can measure the temperature of the tympanic membrane, which is the best representation of core temperature. • Temperature conversion compensates for different ambient temperature conditions. • No contact with the tympanic membrane lower the risk to the user significantly.
Sensor size: 1.6 - 4 mm \varnothing Measurement accuracy: 0.2 - 0.5 $^{\circ}C$	Disadvantages <ul style="list-style-type: none"> • Non-contact temperature sensors are typically bigger than contact thermometers, adding the -size limitation challenge. • If the tympanic membrane does not fill a considerable fraction of the sensor's field of view, erroneous measurements can occur.

4.1.1.3 Temperature measurement method choice

A non-contact, infrared sensor is selected for the Ear-Monitor. User safety, without performance compromise gives it the superiority over contact thermometers for this application. The lower accuracy is justified by the fact that the tympanic membrane is a better representation of the core body temperature.

4.1.2 Temperature measurement sensor

To realize non-contact temperature measurement two infrared sensors are considered: The TMP006 from Texas Instruments and the ST60 Micro from Dexter Research Center Inc.

4.1.2.1 ST60 Micro

The ST60 Micro is a one channel, 80-junction, completely analogue temperature sensing device. It is enclosed in a Micro-TO package which is 4.09 mm in diameter as shown by figure ST60Micro shown in Figure (ST60Micro). The manufacturer emphasizes the ST60 Micro's versatility and proposes use in tympanic ear thermometers. There is an option for a die temperature thermistor. This option will be required for ambient temperature compensation, meaning that all four terminals will be connected.

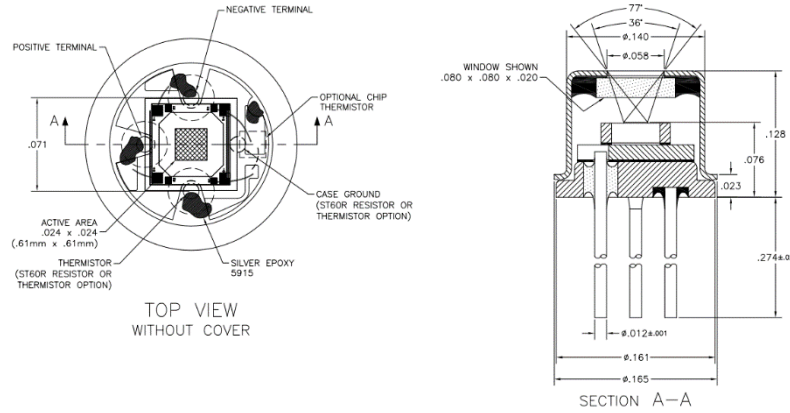


Figure 4.1: ST60Micro diagram from the datasheet

4.1.2.2 TMP006

The TMP006 is a fully integrated IR sensor measuring only $1.6 \times 1.6 \times 0.8$ mm, far better suited for a narrow ear canal than the ST60 Micro. Thermophile voltage and sensor temperature, are made digitally available through hardware registers. These two values can be used to calculate the object temperature. Registers are accessed by a MCU though I2C communication. Values are digitalized by a 16-bit on-chip ADC, eliminating the need for supporting analogue filters and amplifiers. The TMP006's user guide suggest that is be used to calculate the surface temperature of target objects with emissivity values greater than 0.7, and preferably greater than 0.9. The literature study revealed that the emissivity of the eardrum is 0.98, placing it well within the required range.

4.1.2.3 Temperature measurement sensor choice

The smaller package size and on-chip ADC led to the selection of the TMP006 for use in the Ear-Monitor. The TMP006 needs no separate analogue filter and amplifier. Furthermore, the manufacturer supplies detailed calibration documentation, allowing for more accurate and time effective calibration. The simple shape of the ST60 Micro makes it easy to mount, but the diameter of the package may not fit in smaller ear canals and leave little room for the other sensors. Therefore, the ST60 Micro is eliminated.

4.2 Heart Rate

The Ear-Monitor will extract heart rate from in or around the ear canal. The main criteria are sensor size, unobtrusiveness and robust signal acquisition. The method selection and sensor selection is discussed separately.

4.2.1 Heart rate measurement method

The following five methods from literature are considered to measure heart rate.

4.2.1.1 Ear ECG

As shown by Winokur *et al.* (2012), an electrocardiogram can be detected behind the ear. One electrode is placed behind the ear on the mastoid bone and the other on the back of the neck. A differential amplifier and ADC is used to acquire the signal.

Table 4.3: Ear ECG

Image	Advantages <ul style="list-style-type: none"> • ECG is the standard method used by cardiologists to measure heart rate. • Other cardiac information can be extracted from ECG i.e. heart rhythm, heart damage and the state of heart conduction tissue. • Not pulse transit time delay.
Sensor size: 10 mm \varnothing electrodes Unobtrusiveness: Bad - electrode needed behind ear and on neck Signal robustness: Noisy (Figure Winokur).	Disadvantages <ul style="list-style-type: none"> • The sensor cannot be fitted entirely inside the ear canal. • Two electrodes will be needed. • Separate signal acquisition electronics are needed.

4.2.1.2 Ear PPG

A LED and photodiode are used to detect variation in subcutaneous tissue blood volume due to the beating heart. Literature identifies three possible locations: Inside the ear canal, the earlobe and the concha. With unobtrusiveness in mind, the ear canal method is selected. This means reflective PPG is used.

Table 4.4: Ear PPG

Image	<p>Advantages</p> <ul style="list-style-type: none"> • A substantial pressure pulse can be detected in and around the ear. • Pulse oximetry, a type of PPG, is a tried and tested way of measuring heart rate. • Respiratory related characteristics like amplitude modulation, respiratory-induced intensity variation and frequency modulation can be found only in PPG signals and can be used to determine respiratory rate.
<p>Sensor size: Smallest - $1.9 \times 2.6 \times 0.8$ mm</p> <p>Unobtrusiveness: Good - fits inside ear canal</p> <p>Signal robustness: Good - clear pressure wave visible (Figure da2010ear)</p>	<p>Disadvantages</p> <ul style="list-style-type: none"> • PPG is susceptible to motion artefacts and variation in blood perfusion. • Few PPG sensor packages are available to fit inside the ear canal. • Using separate LEDs and photodetectors increases to complicity and size for the proof of concept Ear-Monitor.

4.2.1.3 Ear BCG

A pressure sensitive sensor or accelerometer is placed inside the ear canal to detect the mechanical effects of the pulsating heart.

Table 4.5: Ear BCG

Image	Advantages <ul style="list-style-type: none"> • Pressure sensors can be made small enough for the limited space in the ear canal. • Accelerometer can also be used to measure respiratory rate.
Sensor size: Smallest - $3 \times 3 \times 1$ mm [3] Unobtrusiveness: A part of the sensor protrudes from the ear, can be made smaller Signal robustness: Noisy (da2010ear) (winokur2012wearable)	Disadvantages <ul style="list-style-type: none"> • The signal detected by Da He <i>et al.</i> (2010) and Winokur <i>et al.</i> (2012) appears noisy and detecting beats will be troublesome. • This method will be influenced by motion artefacts to such an extent that it will be impractical for most forms of practical use.

4.2.1.4 Phonocardiogram

A microphone is placed inside the ear canal and identifies heart beats by analysing the sound produced by the cardiac cycle.

Table 4.6: Ear Phonocardiogram

Image	Advantages <ul style="list-style-type: none"> • Can be used to detect breathing as well, as shown by Goverdovsky <i>et al.</i> (2016).
Sensor size: Smallest - $3.35 \times 2.5 \times 0.98$ mm Unobtrusiveness: Can fit inside the canal [5] Signal robustness: Noisy	Disadvantages <ul style="list-style-type: none"> • Sounds from other sources like movement and speaking can corrupt the signal.

4.2.1.5 Heart rate method choice

Ear PPG is selected as the Ear-Monitor's method of measuring heart rate. PPG produces a clear signal that will allow for accurate beat detection. This method can also be in cooperated into the SpO_2 measurement sensor, eliminating the need for two different sensors. The entire sensor can fit inside the ear canal making it unobtrusive. This method is also less susceptible to noise than ear BCG of a phonocardiogram.

4.2.2 Heart rate measurement sensor

Reflexive ear canal PPG is selected to measure heart rate. Three PPG sensors options are considered: separate LEDs and photodetector, the NJL5501R from JRC and the MAX30100 by Maxum Integrated.

4.2.2.1 Separate LEDs and photodetector

SMD LEDs will be used along with one or more photodetectors. The components will be mounted on a thin PCB and placed on the ear probe. The LEDs and photodetectors can be placed in various precise configurations and a wider choice of individual transducers that can be used. Additional analogue electronics are needed to drive the LEDs, conditioning the detector signal output and compensate for ambient lighting. A commercial integrated analogue from end chip like Texas Instruments' AFE4400 can be used to perform this task.

4.2.2.2 NJL5501R

The NJL5501R is a surface mounted photoemitter and -detector contained in one $1.9 \times 2.6 \times 0.8$ mm package shown in Figure (NJL5501R). Red and IR LEDs makes it suitable for reflective pulse oximetry and heart beat detection. Its small size will allow it to fit in the ear canal while leaving adequate space for other sensors. It requires all the same supporting electronics as using separate LEDs and a photodetector.

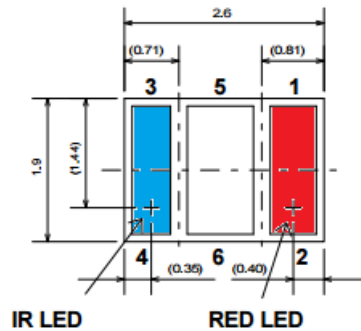


Figure 4.2: NJL5501R diagram from the datasheet

4.2.2.3 MAX30100

The MAX30100 is single chip pulse oximeter and heart rate detector. It has red and IR LEDs, a photodetector, a 16-bit ADC and digital filters all in one $5.6 \times 2.8 \times 1.2$ mm, 14-Pin package. The LEDs and photodetector are in the same plane, meaning it operates in reflective mode. Like the TMP006 it uses

the I2C protocol to communicate with a MCU. Configuration registers allow the designer to specify sample rate, LED currents and LED pulse width.

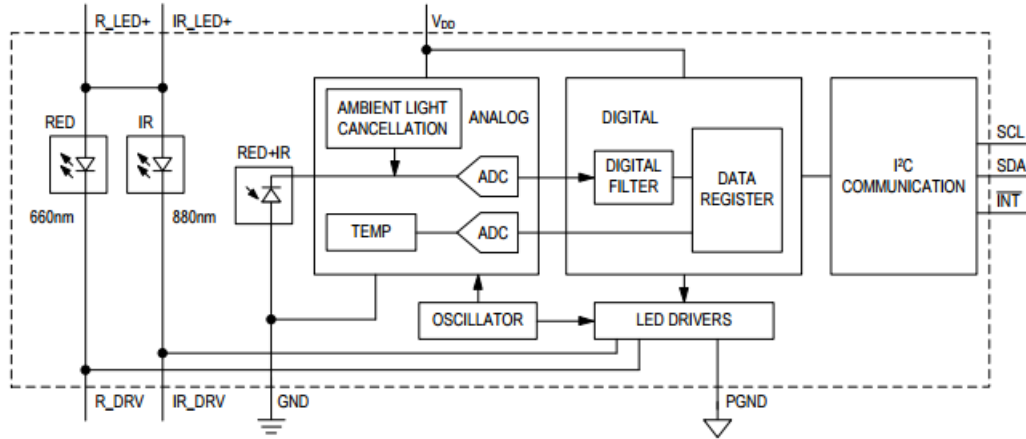


Figure 4.3: MAX30100 block diagram from the datasheet

The MAX30100 uses a 3.3V supply and programmable current sources to drive the LEDs, whilst digital operations are done at 1.8V. It draws between 6 and 12 mA while recording red and IR PPGs. It has a digital 50Hz/60Hz notch filter to reject powerline interference. LEDs can be individually supplied with 0 mA to 50 mA and LED pulse width can be varied from 0.2 ms to 1.6 ms. A sample rate can be chosen between 5 and 1000 samples per second. An important feature of the MAX30100 is its 64-byte deep FIFO register which is used to store the output values. Each output set consists of a 16-bit red and 16-bit IR value, meaning that there are 4 bytes per output and therefore 16 sets of output values can be held in the FIFO at any time. The MCU will read 4 bytes at a time from the FIFO to obtain the latest red and IR values.

4.2.2.4 Heart rate sensor choice

The MAX30100 is selected for use in the Ear-Monitor. It has optimized optics to guide outgoing and incoming light. It has integrated ambient light cancellation. Its entire AFE is integrated meaning that no additional electronics are needed, apart from the I2C lines and power regulators. This gives it a big advantage over the more complex separate LEDs and photodetector method. Its small size and reflective mode of operation, allows it to be placed inside of the ear canal. Data recorded by the MAX30100 will be used to calculate heart rate and blood oxygen saturation.

4.3 Respiratory Rate

The Ear-Monitor will measure respiratory rate from inside the ear canal. The main criteria are sensor size and susceptibility to noise corruption.

4.3.1 Respiratory rate measuring method

The following three respiratory rate measuring methods from literature are considered.

4.3.1.1 Accelerometer

A small MEMS accelerometer is placed inside the ear canal and measures the movement of the head due to breathing.

Table 4.7: Ear Accelerometer

Image	Advantages <ul style="list-style-type: none"> • The accelerometer can be server the dual purpose of measuring breathing and heart rate, thus saving space.
Sensor size: $3 \times 3 \times 1$ mm [3] Noise susceptibility: Very high	Disadvantages <ul style="list-style-type: none"> • This method is extremely vulnerable to noise form other movements.

4.3.1.2 Microphone

A microphone is placed inside the ear canal and record the sound of air moving through the respiratory tracts, allowing the respiratory rate to be determined.

Table 4.8: Ear Microphone

Image	Advantages <ul style="list-style-type: none"> • The microphone can serve the dual purpose of measuring breathing and heart rate, thus saving space.
Sensor size: ? Noise susceptibility: Very high	Disadvantages <ul style="list-style-type: none"> • This method is extremely vulnerable to noise form other sounds like talking or ambient noise.

4.3.1.3 Respiratory related heart rate characteristics

The variations in heart rate is used to determine the berating rate. These include amplitude modulation, respiratory-induced intensity variation and frequency modulation of the heart rate in synchronization with the respiration rate.

Table 4.9: Respiratory related heart rate characteristics

Image	Advantages <ul style="list-style-type: none"> • No dedicated sensor is needed. • Less susceptible to noise the acceleration or microphone method.
Sensor size: No sensor needed Noise susceptibility: Low	Disadvantages <ul style="list-style-type: none"> • Only steady and relatively slow respiratory rates can be detected.

4.3.1.4 Respiratory rate choice

The Ear-Monitor will determine respiratory rate by analysing respiratory related heart rate characteristics, of which heart rate frequency modulation (RSA) is found to be the most detectable. This method saves space by not requiring a dedicated sensor. It is also the lest susceptible to noise from other sources of the three methods considered. No sensor selection is needed for this medical sign, as all the work is done by the MCU.

4.4 Blood oxygen saturation

Pulse oximetry is the only practical way for the Ear-Monitor to measure blood oxygen saturation. The MAX30100 selected for measuring heart rate is equipped for this task. A red and infrared LED as well as a photodetector is available for the joint function for measuring heart rate and blood oxygen saturation.

4.5 Final concept

The final concept is obtained by combining the methods and sensors selected in this chapter. To summarise: the Ear-Monitor will used the TMP006 infrared sensor pointed at the tympanic membrane to measure core body temperature. The MAX30100 reflective pulse oximeter will be placed on on the side of the ear probe facing the canal wall. Red and infrared PPGs from the MAX30100

will be used to extract heart rate and SpO_2 . Finally, respiratory rate will be determined by analysing the respiratory sinus arrhythmia.

Chapter 5

Detailed Design

This chapter documents the detailed design of the subsystems of the Ear-Monitor. The hardware and software sides are discussed separately.

5.1 Hardware

A typical telemedicine configuration is used for the Ear-Monitor and its supporting system. Similar to that used in Wang *et al.* (2010) and Prawiro *et al.* (2016). The ear-probe is the signal acquisition module, data is sent by means of a wireless transceiver to a device running supporting software and finally used data is stored for later access. Figure X illustrates the flow of information through the hardware set-up.



Figure 5.1: Flow of information in a typical telemedicine set-up

This section documents the detailed design of each of the key parts of hardware found in the Ear-Monitor.

5.1.1 Temperature sensor

The non-contact, infrared TMP006 is selected to measure tympanic membrane temperature in the Ear-Monitor. Four wires are connected for power and communication. The package has eight solder balls for surface mounting on a PCB. A big challenge was to mount this micro-component. Various methods were tested.

First, a PCB was designed and manufactured. Mounting the TMP006 on this PCB proved to be problematic. Next, the device footprint and wire connection pads were etched into copper clad flexible PCB sheets. Solder paste and a heat gun was used to mount the TMP006. This method worked, but mounting proved to be unreliable, for connections were sometimes not made properly. Finally, it was decided to buy pre-mounted boards, cut away excess material and solder wires to the exposed tracks. This method was necessitated by the lack of advanced facilities to mount micro SMT components. The flex PCB method will be preferable when a SMT component placement system is available. Figure 5.2 shows the bought, pre-mounted boards and the cut-out component along with the four connections.

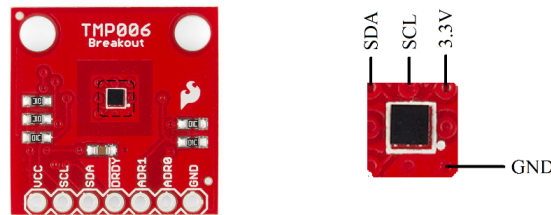


Figure 5.2: TMP006 pre-mounted boards, cut-out and four connections

According to the TMP006 used guide, the sensor captures radiation from almost its entire 180° field of view, but the majority of the received signal comes from sources that are parallel to and precisely in front of the sensor. The final target object temperature is an integration of all the radiation signals captured across the field of view of the sensor.

The user guide also states that the smaller the object is the closer it should be placed to the sensor to prevent other objects from entering the field of vision. It is suggested that a round object be placed at a distance of one half of its radius from the sensor, relating to 1.75 mm in the case of the tympanic membrane. This is not nor practical or necessary in the case of the Ear-Monitor.

The goal is to place the sensor at least 5mm from the membrane. This will remove the risk of contact with the membrane, while still ensuring thermal radiation from the canal is detected. Energy from the ear canal self will inevitably be detected by the sensor, but it is assumed that the wall near the membrane is in thermal equilibrium with the membrane with in an acceptable margin.

It is suggested that the sensor be placed at a distance no further than one-half of the radius of the target object. The minimum ear canal diameter of the test population will be 5mm, therefore the sensor must be placed 1.75 mm from the eardrum. Figure X shows the relationship between the target object

size, distance from the sensor and percentage radiation captured from target object.

Energy radiated or conducted between the PCB and the sensor can cause temperature calculation errors. To prevent this the sensor and PCB should be kept at the same temperature. The ear probe setup of this device is favourable for this task, for the PCB is very small and contains no other heat generating components. Also, the target object, tympanum, will stay at a constant temperature, so the sensor will experience no heat fluctuations. It will, however, be necessary to allow time for the sensor and PCB to reach thermal equilibrium once placed inside the ear canal, before accurate measurements can be taken.

The TMP006 is placed in the tip of the ear probe.

Chapter 6

Experimental Procedure

6.1 Overview

This chapter will discuss the experimental set-ups used to test the functionality and performance of the developed device. The aim of the study is to determine if the developed device can indeed measure accurate vital sign data from the ear canal. This, in turn, will answer the research question. Each measured vital sign needs to be validated, in order to prove that it is indeed accurate data.

Two types of validation will be used in this study: Benchmark validation for core temperature, heart rate, respiratory rate and SpO₂; and event related potential detection to validate EEG.

Healthy adult volunteers will partake in this study. These volunteers will be fitted with the developed device and with the industry standard medical device. Device and benchmark data will be collected simultaneously and compared afterwards.

This study will test the actual data measured and also the processing of this data. For example the extraction of heart rate from PPG and the extraction of breathing rate from heart rate.

Tests will involve comparing time varying signals (PPG), time invariant signals and calculated figures (Breathing rate, SpO₂, Temp?)

6.2 Theory

6.3 Ethical Consent

6.4 Subjects

6.5 Benchmark Validation

Core temperature, heart rate, respiratory rate and SpO₂ measurements will be tested through benchmark validation. This entails comparing the measurements made by the developed device to measurements made, in the same conditions, by a industry standard medical device. In this study, a device that conforms to the EC requirements is seen as industry standard device. This is a valid assumption, for the CE mark is sign that the device complies with the EU legislation that is applicable to the product (what does this mean?).

Three devices was selected to provide the benchmark measurements.

The vital sign measurements of the device will be compared to selected benchmarks. These benchmarks will be measurements made by various industry standard medical devices.

6.6 Method

6.6.1 Benchmark Apparatus

Benchmark devices are chosen to measure the same physiological signs as the developed device. The Nexus-10 physiological monitoring platform will be used to provide the benchmark measurements for PPG, heart rate and respiratory rate. The SureSense blablabla will be used for the SpO₂ benchmark and an ear thermometer for the core temperature benchmark.

Mind Media's Nexus-10 is a ten channel biofeedback system. It comes with a array of sensors that can acquire a range of different bio-signals. In this study the blood volume pulse, and respiration sensor will be used. The device can collect data at 128 samples per second.

SureSense blablabla is a ...

Ear thermometer...

with photoplethysmograph was used. Photoplethysmograms was compared and average heart rate readings as well. This will evaluate the feasibility of measuring a PPG from the ear canal ass well as the extracting a heart rate from this signal.

6.6.2 Comparing Data

Comparing the device PPG to the Mexus BVP

6.7 Results

Appendices

List of References

- Alvord, L.S. and Farmer, B.L. (1997). Anatomy and orientation of the human external ear. *Journal-American academy of audiology*, vol. 8, pp. 383–390.
- Aziz, O., Lo, B., King, R., Darzi, A. and Yang, G.-Z. (2006). Pervasive body sensor network: an approach to monitoring the post-operative surgical patient. In: *Wearable and Implantable Body Sensor Networks, 2006. BSN 2006. International Workshop on*, pp. 4–pp. IEEE.
- Bagha, S. and Shaw, L. (2011). A real time analysis of ppg signal for measurement of spo2 and pulse rate. *International journal of computer applications*, vol. 36, no. 11, pp. 45–50.
- Barker, S., Hay, W., Miyasaka, K. and Poets, C. (2002). Principles of pulse oximetry technology.
Available at: <http://www.oximetry.org/pulseox/principles.htm>
- Bheema lingaiah, T., Hanumesh Kumar, D. and Nagaraja, C. (2013). Measurement of pulse rate and spo2 using pulse oximeter developed using labview. *Journal of Electrical and Electronics Engineering*, vol. 8.
- Bickford, R. (1987). Electroencephalography. *Adelman G. ed. Encyclopedia of Neuroscience, Birkhauser, Cambridge (USA)*, pp. 371–373.
- Blaht, W. (2016 09). Mebmd sleep apnea.
Available at: <http://www.webmd.com/sleep-disorders/sleep-apnea/sleep-apnea>
- Buske, O., Neils, C. and Regnier, M. (). Heartbeat: Design and development of a headphone.
- Chan, V. and Underwood, S. (2005 11). *A Single-Chip Pulsorimeter Design Using the MSP430*. Texas Instruments. Rev. Feb 2012.
- Charbek, E. (2015 08). Medscape normal vital vings.
Available at: <http://emedicine.medscape.com/article/2172054-overview>
- Clifton, D., Douglas, J.G., Addison, P.S. and Watson, J.N. (2007). Measurement of respiratory rate from the photoplethysmogram in chest clinic patients. *Journal of clinical monitoring and computing*, vol. 21, no. 1, pp. 55–61.

Da He, D., Winokur, E.S., Heldt, T. and Sodini, C.G. (2010). The ear as a location for wearable vital signs monitoring. In: *Engineering in Medicine and Biology Society (EMBC), 2010 Annual International Conference of the IEEE*, pp. 6389–6392. IEEE.

Duun, S., Haahr, R.G., Birkelund, K., Raahauge, P., Petersen, P., Dam, H., Nørgaard, L. and Thomsen, E.V. (2007). A novel ring shaped photodiode for reflectance pulse oximetry in wireless applications. In: *Sensors, 2007 IEEE*, pp. 596–599. IEEE.

Encyclopædia-Britannica, T.E.O. (). Spectrophotometry.
Available at: <https://www.britannica.com/science/spectrophotometry>

Erickson, R.S. and Kirklin, S.K. (1993). Comparison of ear-based, bladder, oral, and axillary methods for core temperature measurement. *Critical care medicine*, vol. 21, no. 10, pp. 1528–1534.

Goverdovsky, V., von Rosenberg, W., Nakamura, T., Looney, D., Sharp, D.J., Papavassiliou, C., Morrell, M.J. and Mandic, D.P. (2016). Hearables: Multimodal physiological in-ear sensing. *arXiv preprint arXiv:1609.03330*.

Huang, C.-Y., Chan, M.-C., Chen, C.-Y. and Lin, B.-S. (2014). Novel wearable and wireless ring-type pulse oximeter with multi-detectors. *Sensors*, vol. 14, no. 9, pp. 17586–17599.

Johansson, A. (2003). Neural network for photoplethysmographic respiratory rate monitoring. *Medical and Biological Engineering and Computing*, vol. 41, no. 3, pp. 242–248.

Jones, D. (2010). *Biomedical Sensors*. Sensor technology series. Momentum Press. ISBN 9781606500569.
Available at: <https://books.google.co.za/books?id=7cI83Y0IUtkC>

Karaki, H. and Polyziev, V. (2014). Demystifying thermopile ir temp sensors.
Available at: <http://www.sensorsmag.com/components/demystifying-thermopile-ir-temp-sensor>

Khalifa, O.O., Khan, T. and HM, H. (2014). Development of wearable pulse oximetry for telehealth monitoring system. *Journal of Electrical Engineering*, vol. 14, no. 4, pp. 1–6.

König, V., Huch, R. and Huch, A. (1998). Reflectance pulse oximetry—principles and obstetric application in the zurich system. *Journal of Clinical Monitoring and Computing*, vol. 14, no. 6, pp. 403–412.

Laskowski, E.R. (2015). What’s a normal resting heart rate?
Available at: <http://www.mayoclinic.org/healthy-lifestyle/fitness/expert-answers/heart-ra>

Lefrant, J.-Y., Muller, L., de La Coussaye, J.E., Benbabaali, M., Lebris, C., Zeitoun, N., Mari, C., Saissi, G., Ripart, J. and Eledjam, J.-J. (2003). Temperature measurement in intensive care patients: comparison of urinary bladder, oesophageal,

- rectal, axillary, and inguinal methods versus pulmonary artery core method. *Intensive care medicine*, vol. 29, no. 3, pp. 414–418.
- Leonard, P.A., Douglas, J.G., Grubb, N.R., Clifton, D., Addison, P.S. and Watson, J.N. (2006). A fully automated algorithm for the determination of respiratory rate from the photoplethysmogram. *Journal of clinical monitoring and computing*, vol. 20, no. 1, pp. 33–36.
- Lin, B.-S., Chou, W., Wang, H.-Y., Huang, Y.-J. and Pan, J.-S. (2013). Development of novel non-contact electrodes for mobile electrocardiogram monitoring system. *IEEE journal of translational engineering in health and medicine*, vol. 1, pp. 1–8.
- Moody, G.B., Mark, R.G., Bump, M.A., Weinstein, J.S., Berman, A.D., Mietus, J.E. and Goldberger, A.L. (1986). Clinical validation of the ecg-derived respiration (edr) technique. *Group*, vol. 1, no. 3.
- Nitzan, M., Noach, S., Tobal, E., Adar, Y., Miller, Y., Shalom, E. and Engelberg, S. (2014). Calibration-free pulse oximetry based on two wavelengths in the infrared-a preliminary study. *Sensors*, vol. 14, no. 4, pp. 7420–7434.
- Nunez, P.L. and Srinivasan, R. (2006). *Electric fields of the brain: the neurophysics of EEG*. Oxford University Press, USA.
- Oak, S. and Aroul, P. (2015 3). *How to Design Peripheral Oxygen Saturation (SpO2) and Optical Heart Rate Monitoring (OHRM) Systems Using the AFE4403*. Texas Instruments.
- of Encyclopædia Britannica, T.E. (2015 01). External auditory canal.
Available at: <https://global.britannica.com/science/external-auditory-canal>
- Olive, S., Twentyman, O. and Ramsay, C. (2016). Comparison of fingertip and earlobe pulse oximetry with arterial blood gas results.
- Optotherm (2017). Emissivity table.
Available at: <http://www.optotherm.com/emiss-table.htm>
- Park, J.-H., Jang, D.-G., Park, J.W. and Youm, S.-K. (2015). Wearable sensing of in-ear pressure for heart rate monitoring with a piezoelectric sensor. *Sensors*, vol. 15, no. 9, pp. 23402–23417.
- Poh, M.-Z., Swenson, N.C. and Picard, R.W. (2010). Motion-tolerant magnetic earring sensor and wireless earpiece for wearable photoplethysmography. *IEEE Transactions on Information Technology in Biomedicine*, vol. 14, no. 3, pp. 786–794.
- Prawiro, E.A.P.J., Yeh, C.-I., Chou, N.-K., Lee, M.-W. and Lin, Y.-H. (2016). Integrated wearable system for monitoring heart rate and step during physical activity. *Mobile Information Systems*, vol. 2016.

- Pujary, C., Savage, M. and Mendelson, Y. (2003). Photodetector size considerations in the design of a noninvasive reflectance pulse oximeter for telemedicine applications. In: *Bioengineering Conference, 2003 IEEE 29th Annual, Proceedings of*, pp. 148–149. IEEE.
- Shin, K., Kim, Y., Bae, S., Park, K. and Kim, S. (2009). A novel headset with a transmissive ppg sensor for heart rate measurement. In: *13th International Conference on Biomedical Engineering*, pp. 519–522. Springer.
- Stratton, J.R., Levy, W.C., Caldwell, J.H., Jacobson, A., May, J., Matsuoka, D. and Madden, K. (2003). Effects of aging on cardiovascular responses to parasympathetic withdrawal. *Journal of the American College of Cardiology*, vol. 41, no. 11, pp. 2077–2083.
- Stumme, L.D., Baldini, T.H., Jonassen, E.A. and Bach, J.M. (2003). Emissivity of bone. In: *Summer Bioengineering Conference*, pp. 25–29.
- Sund-Levander, M., Forsberg, C. and Wahren, L.K. (2002). Normal oral, rectal, tympanic and axillary body temperature in adult men and women: a systematic literature review. *Scandinavian journal of caring sciences*, vol. 16, no. 2, pp. 122–128.
- Tamura, T., Maeda, Y., Sekine, M. and Yoshida, M. (2014). Wearable photoplethysmographic sensors-past and present. *Electronics*, vol. 3, no. 2, pp. 282–302.
- Tavakoli Dastjerdi, M. (2006). *An analog VLSI front end for pulse oximetry*. Ph.D. thesis, Massachusetts Institute of Technology.
- ThermoWorks (). Emissivity table.
Available at: http://www.thermoworks.com/learning/emissivity_table
- Tytler, J. and Seeley, H. (1986). The nellcor n-101 pulse oximeter. *Anaesthesia*, vol. 41, no. 3, pp. 302–305.
- Wang, I.-J., Liao, L.-D., Wang, Y.-T., Chen, C.-Y., Lin, B.-S., Lu, S.-W. and Lin, C.-T. (2010). A wearable mobile electrocardiogram measurement device with novel dry polymer-based electrodes. pp. 379–384.
- Watthanawisuth, N., Lomas, T., Wisitsoraat, A. and Tuantranont, A. (2010). Wireless wearable pulse oximeter for health monitoring using zigbee wireless sensor network. In: *Electrical Engineering/Electronics Computer Telecommunications and Information Technology (ECTI-CON), 2010 International Conference on*, pp. 575–579. IEEE.
- Winokur, E.S., Da He, D. and Sodini, C.G. (2012). A wearable vital signs monitor at the ear for continuous heart rate and pulse transit time measurements. In: *Engineering in Medicine and Biology Society (EMBC), 2012 Annual International Conference of the IEEE*, pp. 2724–2727. IEEE.
- WorldHealthOrganization (2011). Using the pulse oximeter.
Available at: http://www.who.int/patientsafety/safesurgery/pulse_oximetry/who_ps_pulse_ox

- Yasuma, F. and Hayano, J.-i. (2004). Respiratory sinus arrhythmia: why does the heartbeat synchronize with respiratory rhythm? *Chest Journal*, vol. 125, no. 2, pp. 683–690.