



TEC data, Variac autotransformer turned off

Power input

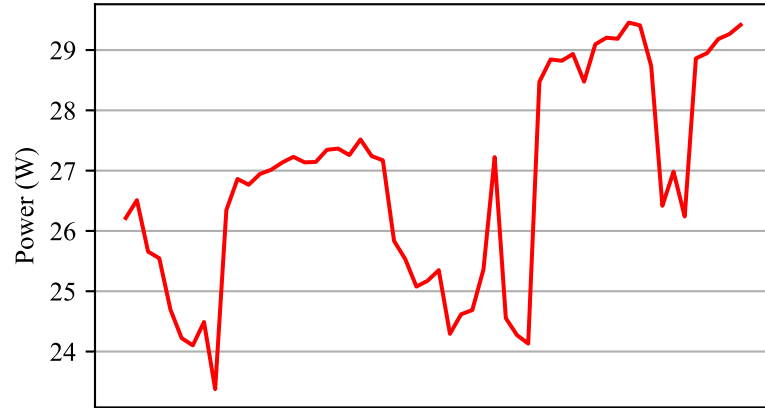

Temperature change

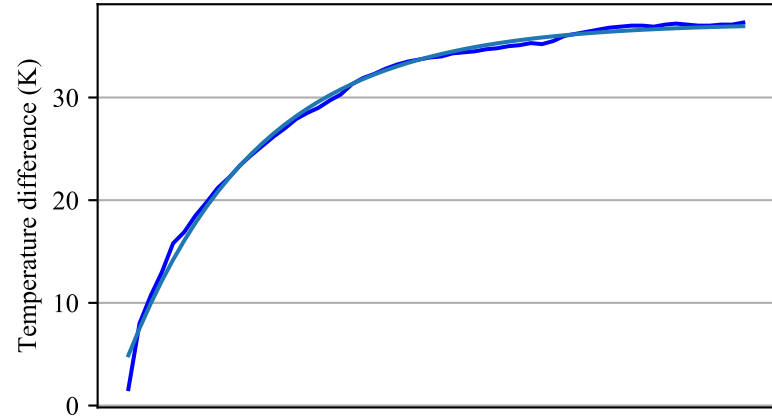

Temperature difference vs. time fit residuals

