


Sepsis Early-Warning System (One-Pager)


Goal: predict sepsis hours before onset using ICU vitals and labs, and optimize an early-warning policy rather than just AUROC.

Key P


- AUROC: 0.847
- AUPRC: 0.128
- Patient AUROC: 0.860
- Patient AUPRC: 0.444
- Brier score: 0.017
- Utility score: 0.132
- Official utility: 0.132
- Accuracy: 0.971
- F-measure: 0.165
- Early detection rate: 0.260
- False alert rate: 0.022

Utility Curve

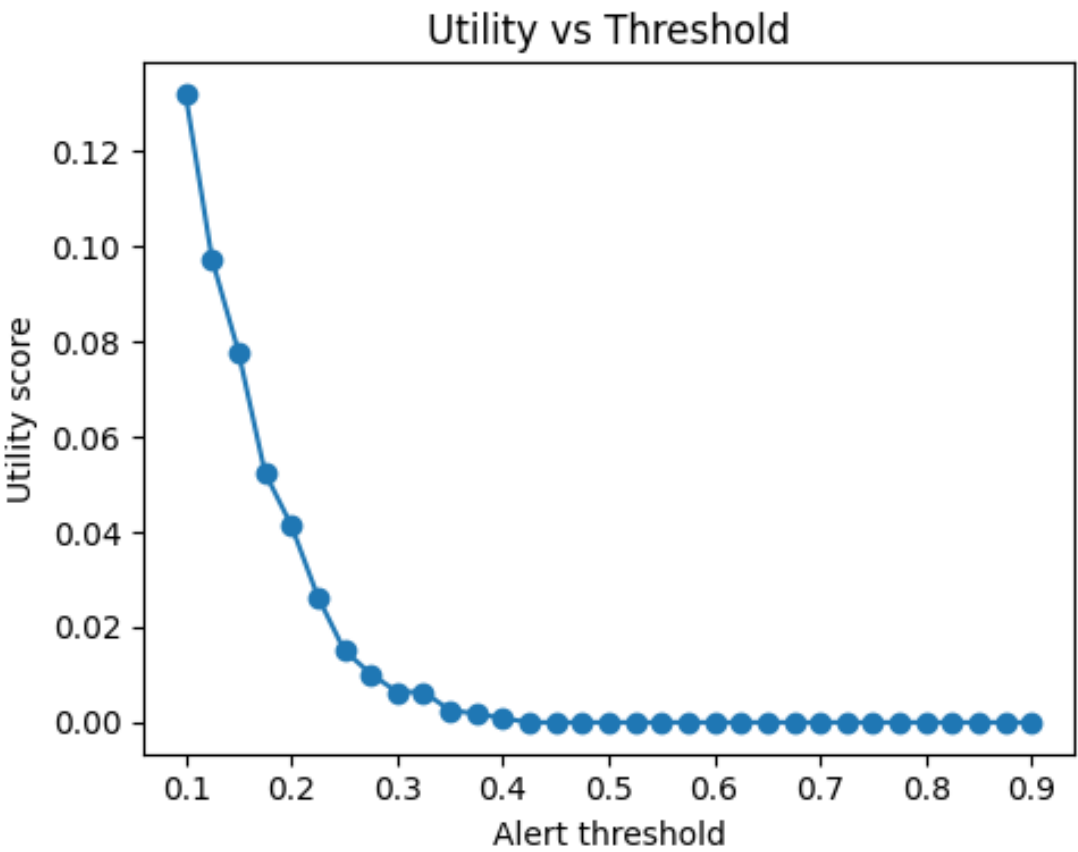

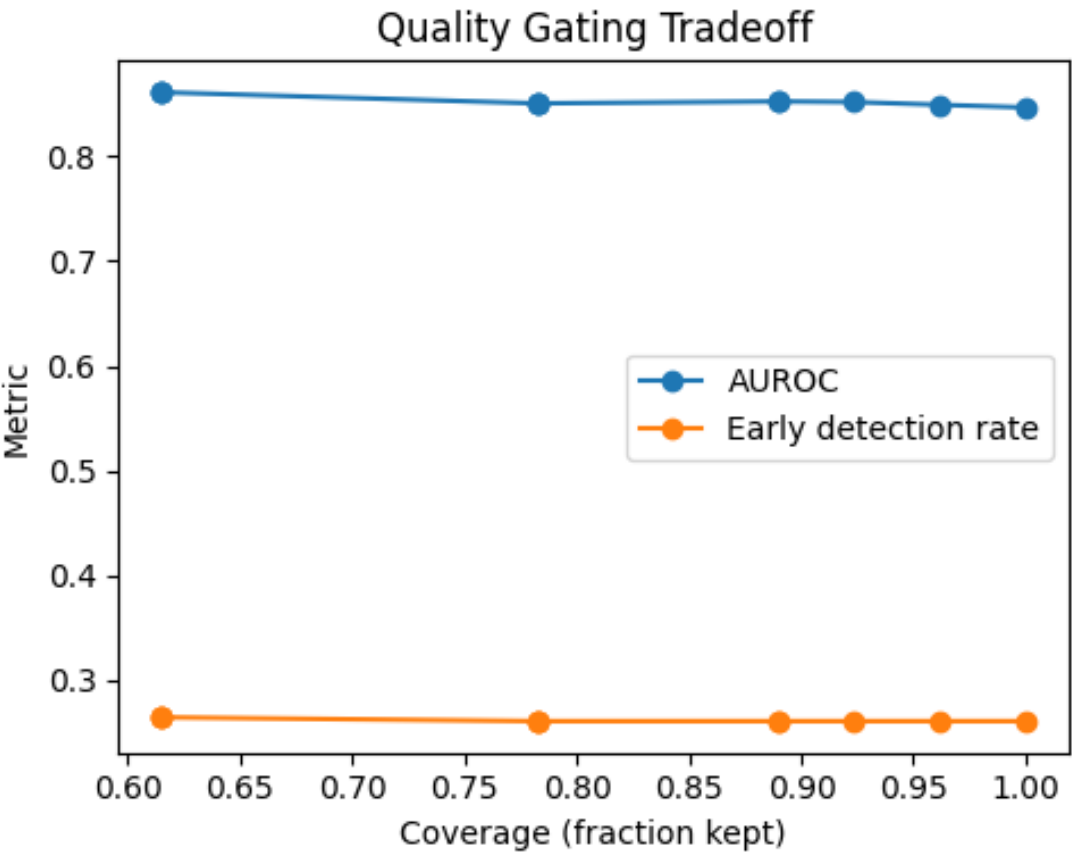

Calibration Curve

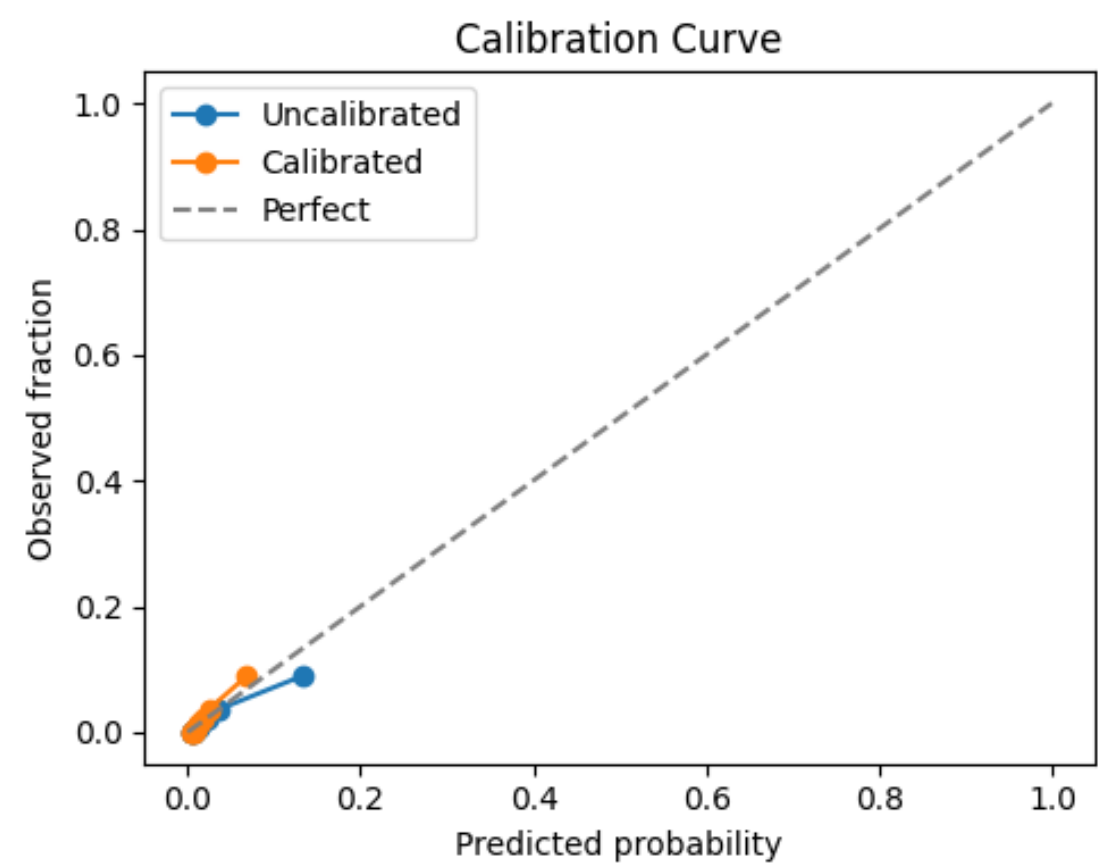

Lead Time Distribution

