



(a) Per-session calibration closes the cross-population gap for every patient, on two independent stroke datasets

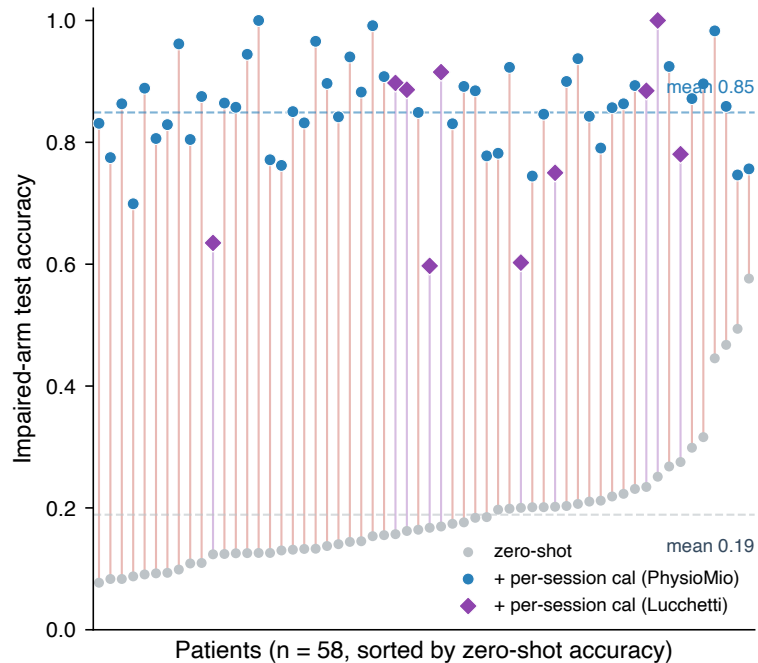

(b) One-time cal degrades across sessions per-session recalibration is necessary

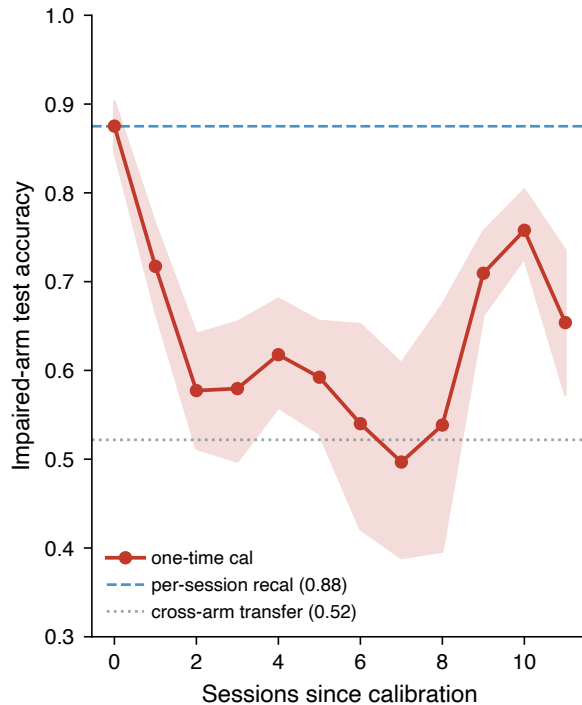

(c) Real-device deployment characterisation

£180

BOM, full hardware

< 50 ms

single-cycle ML on CPU

~275 ms

end-to-end intent
to motor command

99.2 %

live device, within-session
held-out (12-min cued)

97.7 %

cued grasps successfully
completed (Stage 2 deployment)

149 ms

time-to-correct command
(12-min cued)