




Brier loss 1 norm

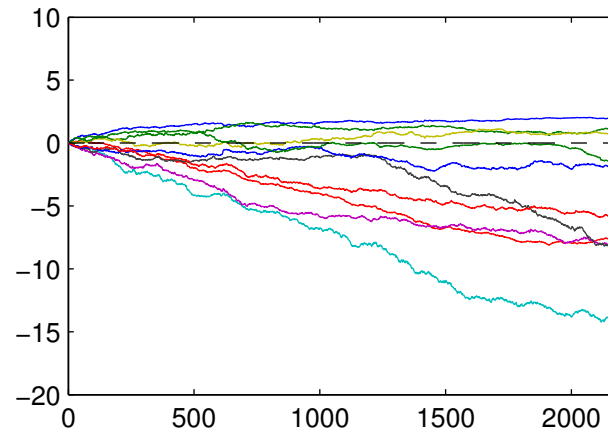

Calibration loss 1norm epsilon:0.03

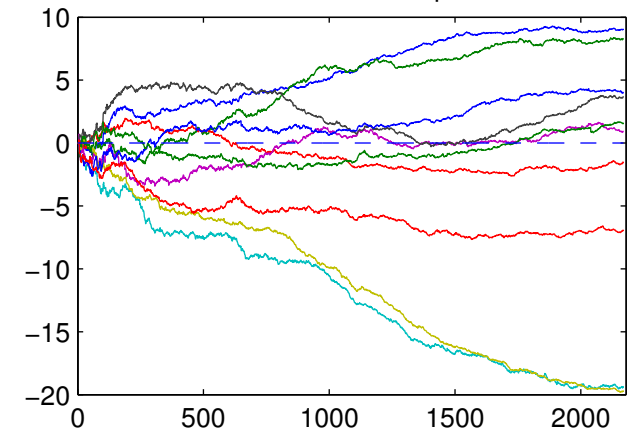

Calibration loss 1norm epsilon:0.05

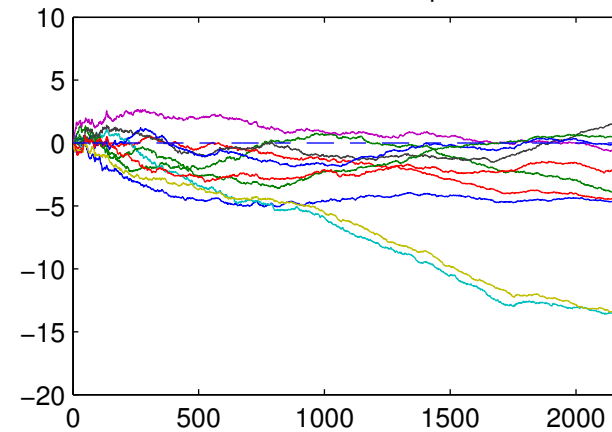

Calibration loss 1norm epsilon:0.07

