



The corrected estimator is sound across the ratio range (1:2 ... 5:7)

A Specificity: identifies the true ratio

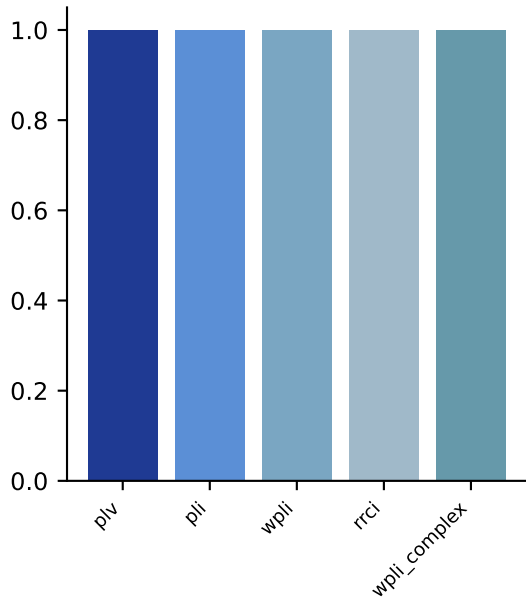

B Monotone dose-response

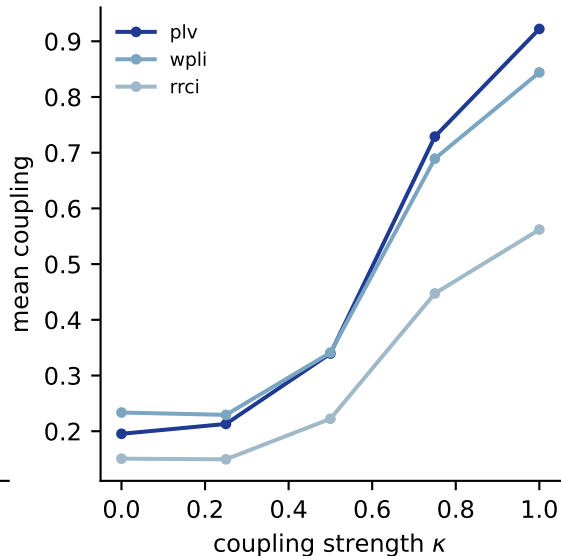

C Sensitivity vs noise

