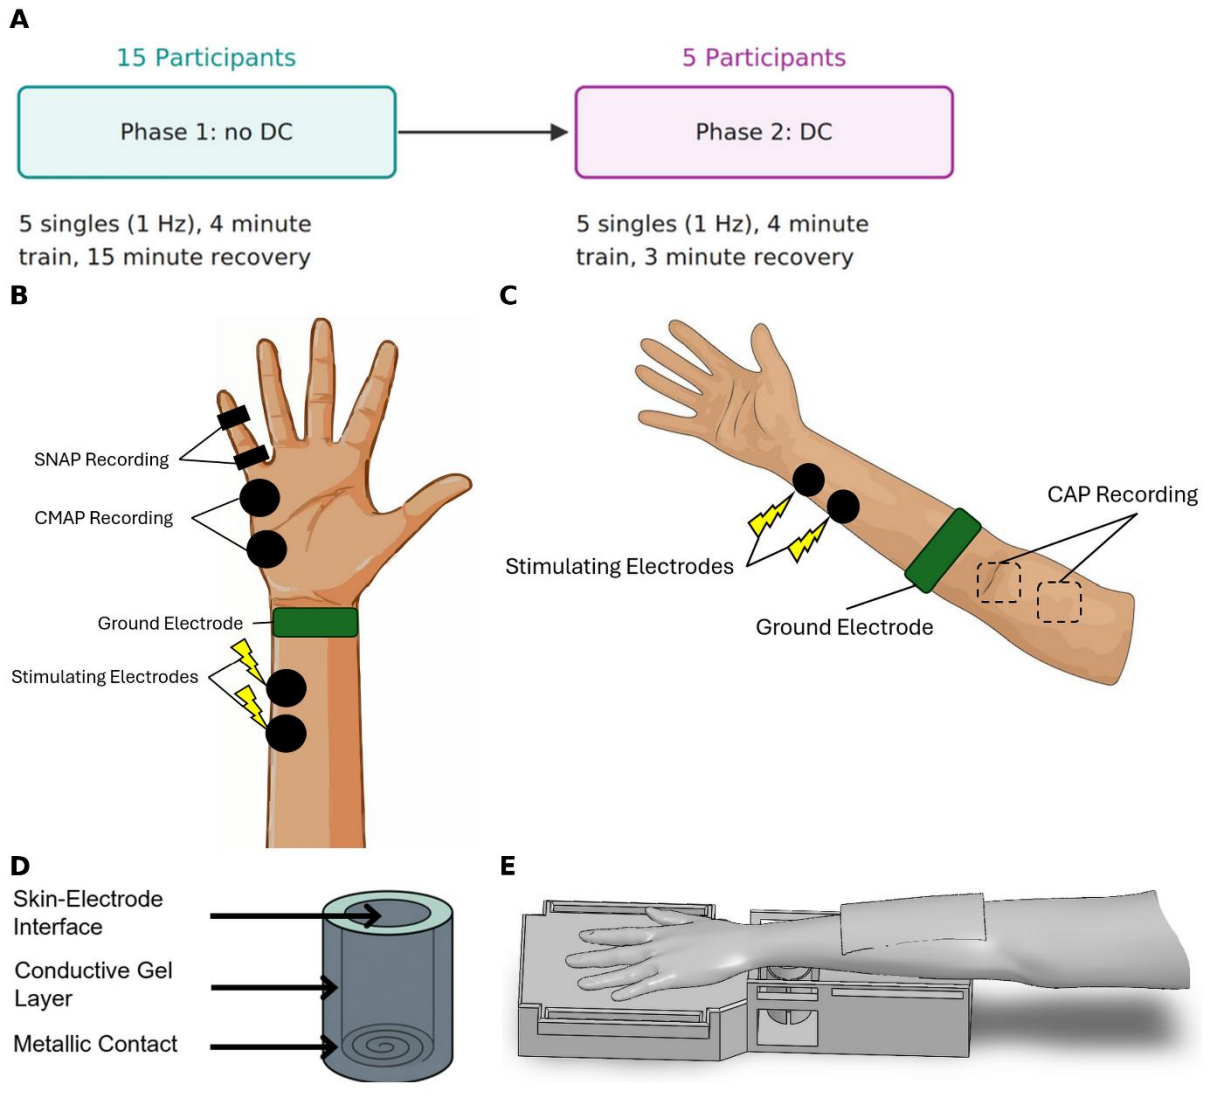

A
15 Participants
5 Participants
Phase 1: no DC
Phase 2: DC
5 singles (1 Hz), 4 minute train, 15 minute recovery
5 singles (1 Hz), 4 minute train, 3 minute recovery
B
SNAP Recording
CMAP Recording
Ground Electrode
Stimulating Electrodes
C
CAP Recording
Stimulating Electrodes
Ground Electrode
D
Skin-Electrode Interface
Conductive Gel Layer
Metallic Contact
E