



ALS Laboratory: EM Melbourne

RECEIVED BY:

DATE TIME:

DATE TIME:

EMAIL INVOICES TO:

Biohazard info:

/ EM2020DEPWAT0003

**LABORATORY USE ONLY (Circle)**

Yes      No      N/A

Yes      No      N/A

 $\cdot^{\circ}\text{C}$ 

Other comments:

## SAMPLE DETAILS

### ANALYSIS REQUIRED

SAMPLE	NAME	DESCRIPTION	DATE / TIME	MATRIX	TOTAL BOTTLES	ON HOLD	Water Testing WATER	ALTERNATIVE ANALYSIS	ADDITIONAL INFORMATION
001	US Tauwitschere		28/09/2022 12:56 PM	Water	ALS: 6 Non ALS: 0	No	X		
002	DS Tauwitschere		28/09/2022 12:58 PM	Water	ALS: 6 Non ALS: 0	No	X		
003	Long Point		28/09/2022 02:08 PM	Water	ALS: 6 Non ALS: 0	No	X		
004	Noonameena		28/09/2022 02:42 PM	Water	ALS: 6 Non ALS: 0	No	X		
005	Bonneys		28/09/2022 03:01 PM	Water	ALS: 6 Non ALS: 0	No	X		
006	McGrath Flat North		28/09/2022 03:30 PM	Water	ALS: 6 Non ALS: 0	No	X		
007	Tilley Swamp Drain D/S Nth Outlet		29/09/2022 10:54 AM	Water	ALS: 6 Non ALS: 0	No	X		
008	Morella Basin @ outlet regulator		29/09/2022 09:19 AM	Water	ALS: 6 Non ALS: 0	No	X		
009	Morella Creek @ gauge		29/09/2022 09:03 AM	Water	ALS: 6 Non ALS: 0	No	X		

Work Order Reference  
**EM2218950**



Telephone : + 61-3-8549 9600





ALS Laboratory: EM Melbourne

RECEIVED BY:

RECEIVED BY:

DATE TIME:

DATE TIME:

**CLIENT:** DEPWAT - Dept for Environment & Water

**PROJECT:** HCHB Monitoring Program

**SITE:** HCBC Land 28/29th September

ORDER NO:

**PROJECT MANAGER:** Darcy Morris

PRIMARY SAMPLER: Darcy Morris

EMAIL REPORTS TO:

EMAIL INVOICES TO:

TURNAROUND REQUIREMENTS : 5 Days

**Biohazard info:**

**LABORATORY USE ONLY (Circle)**

**Custody Seal intact?**

Yes      No      N/A

Free ice / frozen ice bricks present upon receipt?

Yes No N/A

Random Sample Temperature on Receipt:

•C

Other comments:


CONTACT PH: 0437 299 362


SAMPLER MOBILE: 0437 299 362

QUOTE NO: AD/052/20 V2

/ EM2020DEPWAT0003

SAMPLE	SAMPLE NAME	BOTTLE NAME	VOLUME	BARCODE	TYPE	FILTERED	REASON
001	US Tauwitchen	White Plastic Bottle-Lugols Iodine	250 mL	00270820001564	Green	No	
001	US Tauwitchen	Amber DOC Filtered- Sulfuric Preserved	40 mL	00180822027867	Purple	No	
001	US Tauwitchen	Amber TOC Vial - Sulfuric Acid	40 mL	00180822027866	Purple	No	
001	US Tauwitchen	Clear Plastic Bottle - Sulfuric Acid	60 mL	00100322007322	Purple	No	
001	US Tauwitchen	Clear Plastic Bottle - Natural	250 mL	00070821165249	Green	No	
001	US Tauwitchen	White Plastic Bottle - Unpreserved	1000 mL	00060522003764	Green	No	
002	DS Tauwitchen	Amber DOC Filtered- Sulfuric Preserved	40 mL	00180822027865	Purple	No	
002	DS Tauwitchen	Amber TOC Vial - Sulfuric Acid	40 mL	00180822027864	Purple	No	
002	DS Tauwitchen	White Plastic Bottle - Unpreserved	1000 mL	00060522003753	Green	No	
002	DS Tauwitchen	Clear Plastic Bottle - Natural	250 mL	00070821165097	Green	No	
002	DS Tauwitchen	White Plastic Bottle-Lugols Iodine	250 mL	00270820001535	Green	No	
002	DS Tauwitchen	Clear Plastic Bottle - Sulfuric Acid	60 mL	00100322007251	Purple	No	
003	Long Point	Amber DOC Filtered- Sulfuric Preserved	40 mL	00180822027898	Purple	No	
003	Long Point	Amber TOC Vial - Sulfuric Acid	40 mL	00180822027916	Purple	No	
003	Long Point	White Plastic Bottle - Unpreserved	1000 mL	00060121005001	Green	No	
003	Long Point	White Plastic Bottle-Lugols Iodine	250 mL	00270820001515	Green	No	
003	Long Point	Clear Plastic Bottle - Natural	250 mL	00070821165237	Green	No	
003	Long Point	Clear Plastic Bottle - Sulfuric Acid	60 mL	00100322007738	Purple	No	
004	Noonameena	Amber TOC Vial - Sulfuric Acid	40 mL	00180822027901	Purple	No	
004	Noonameena	Clear Plastic Bottle - Natural	250 mL	00070821165151	Green	No	
004	Noonameena	Amber DOC Filtered- Sulfuric Preserved	40 mL	00180822027900	Purple	No	
004	Noonameena	White Plastic Bottle-Lugols Iodine	250 mL	00270820001510	Green	No	
004	Noonameena	Clear Plastic Bottle - Sulfuric Acid	60 mL	00100322007598	Purple	No	
004	Noonameena	White Plastic Bottle - Unpreserved	1000 mL	00060522003756	Green	No	
005	Bonneys	White Plastic Bottle-Lugols Iodine	250 mL	00270820001580	Green	No	
005	Bonneys	Amber TOC Vial - Sulfuric Acid	40 mL	00180822027895	Purple	No	

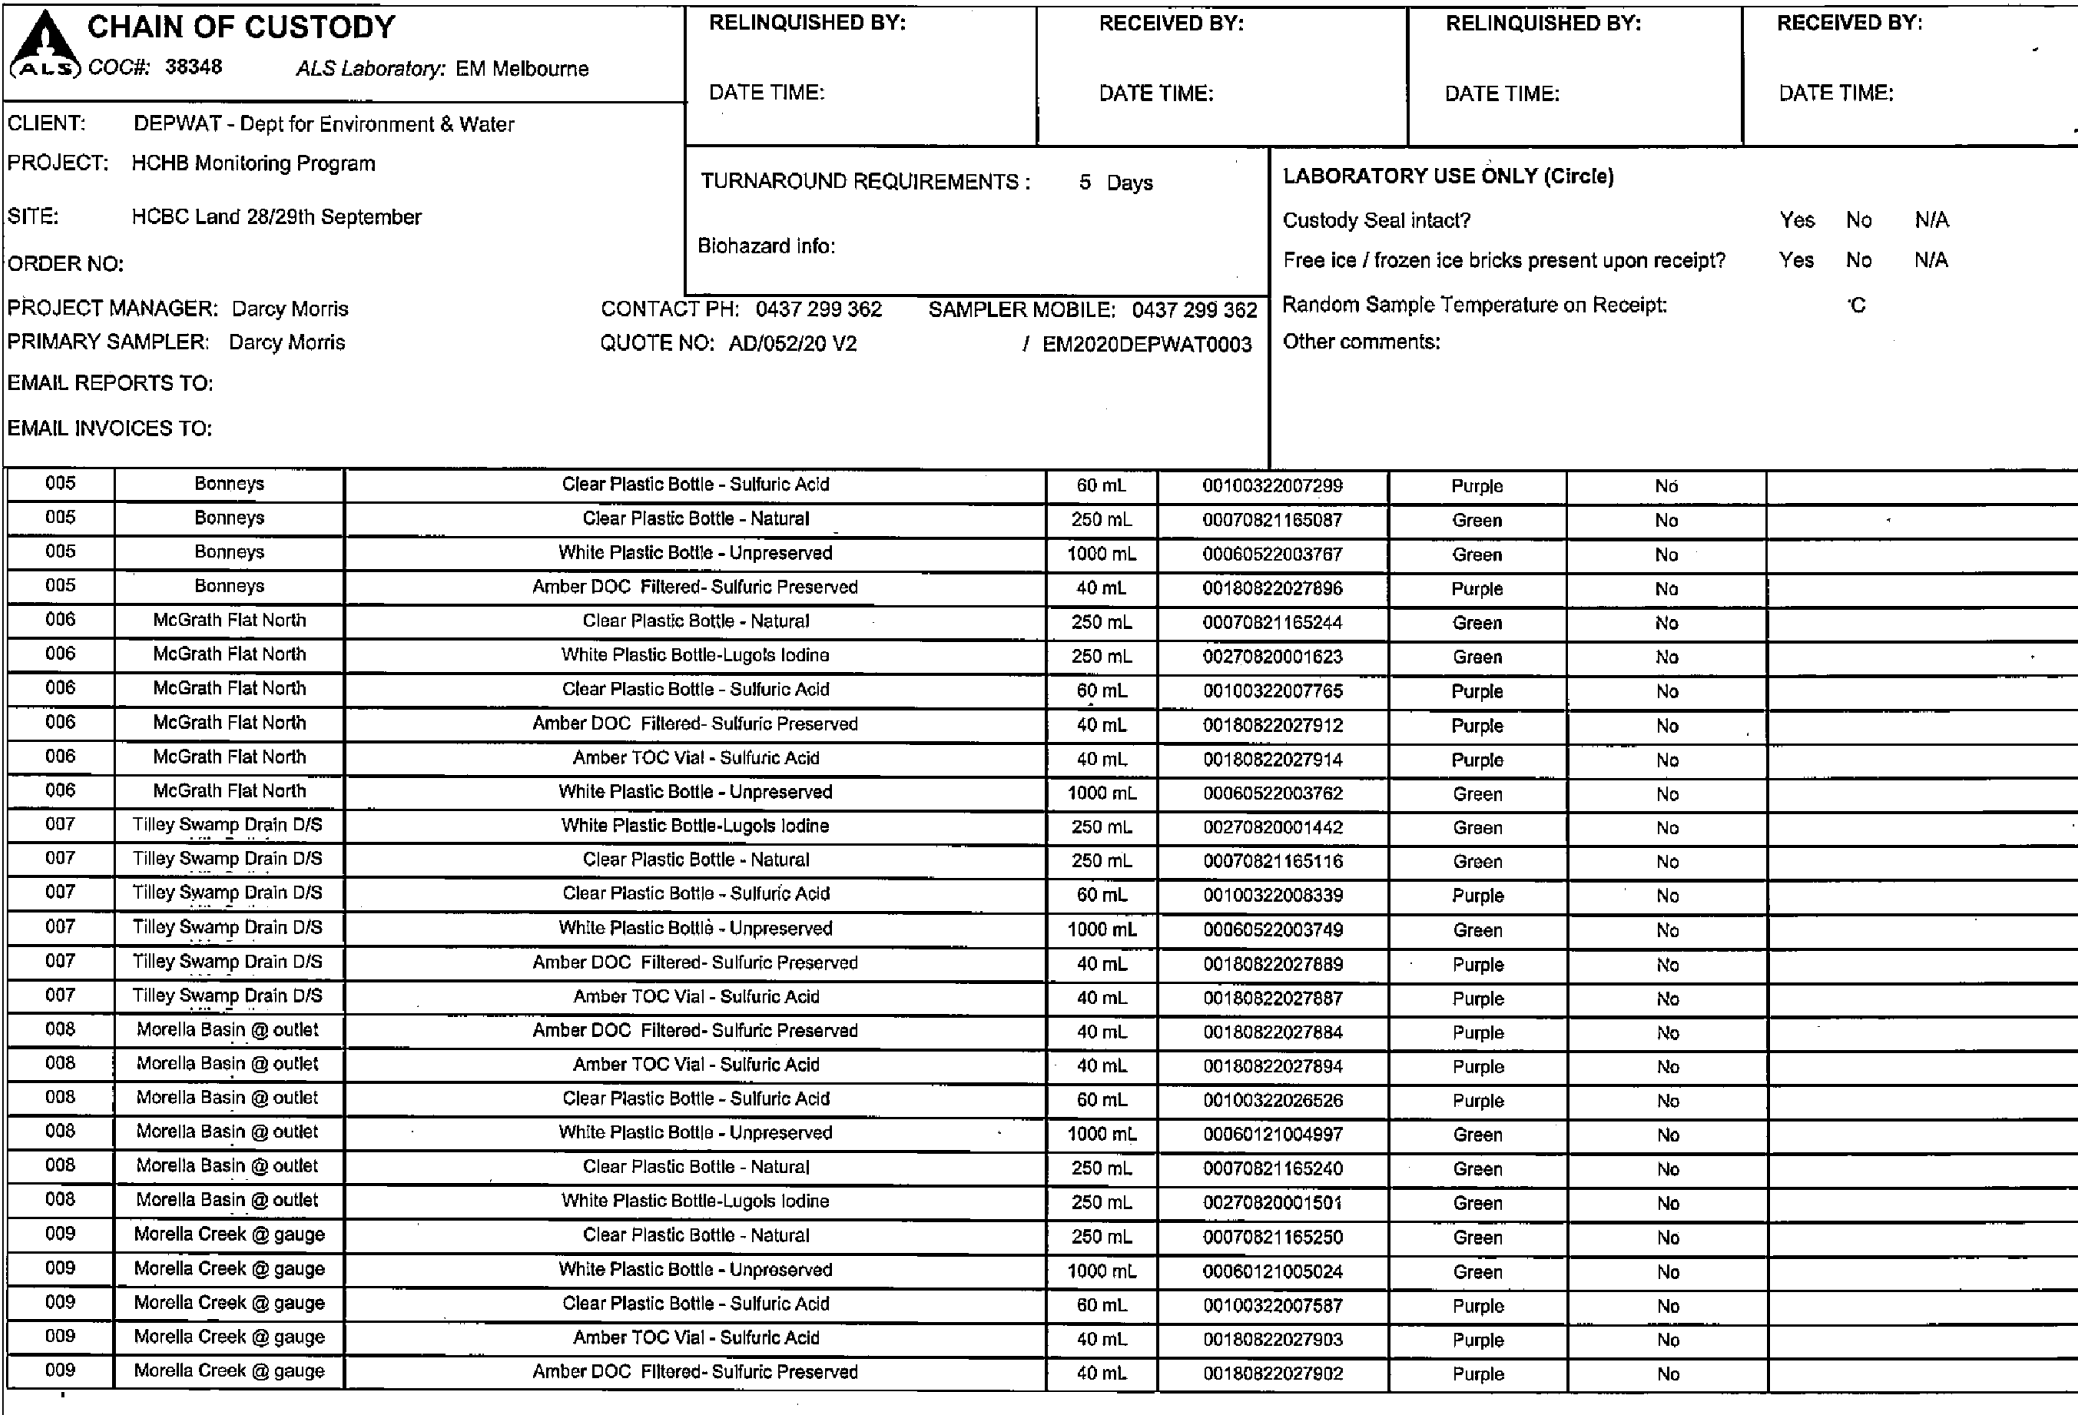

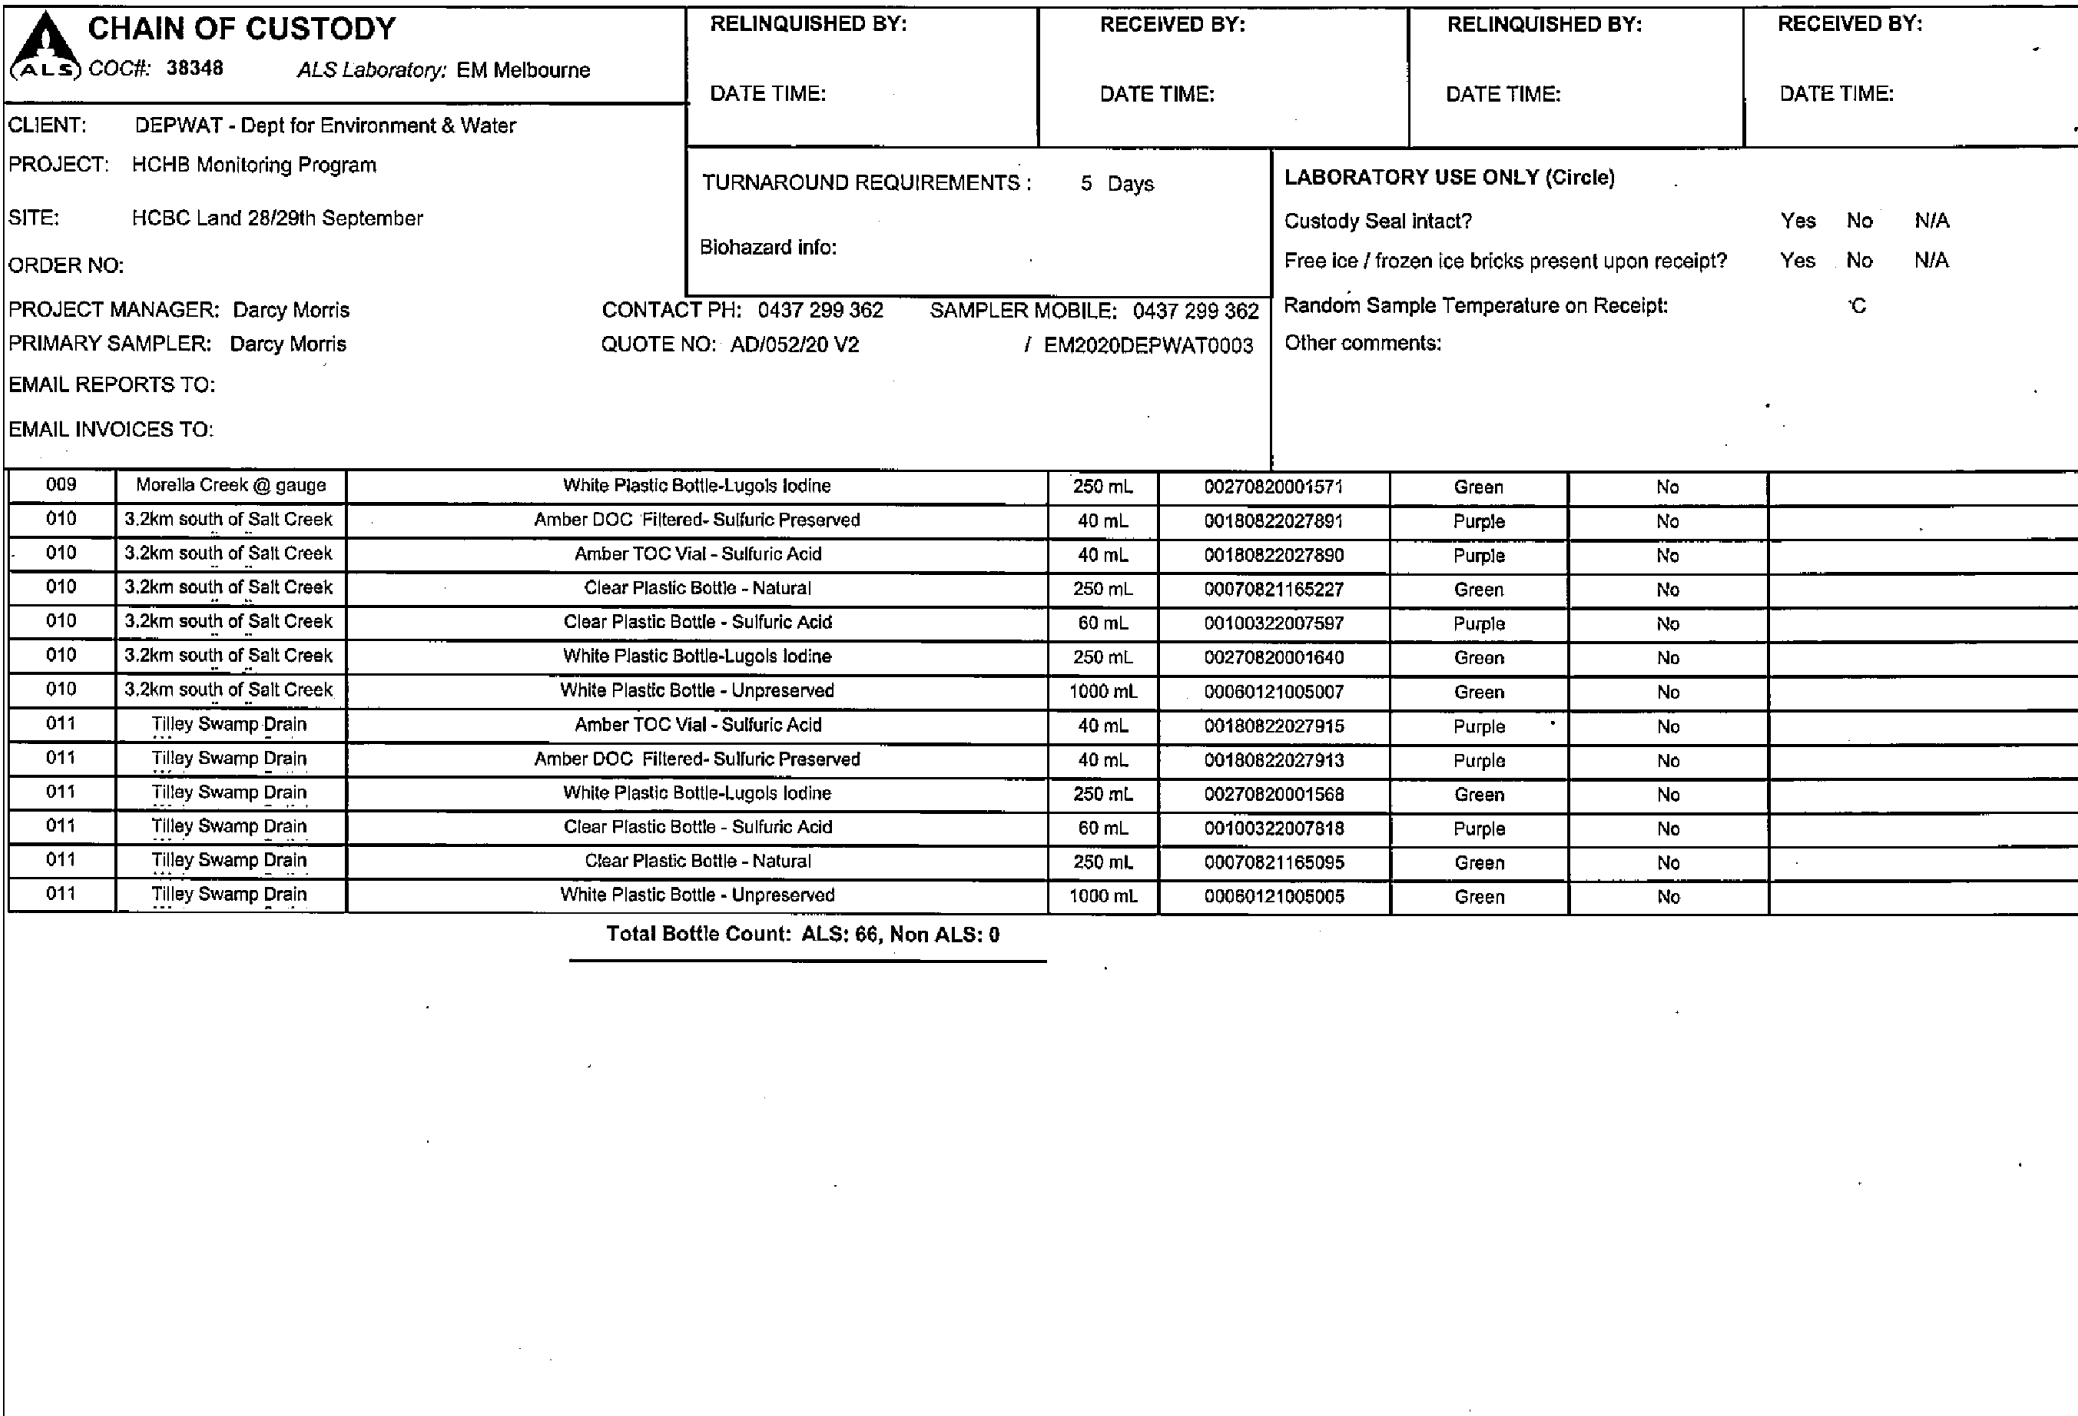

3:40:28 AM



ALS Use Only



## Custody Document for Submissions via ALS Compass App

Project: HCHB Client: DEW Project Manager: Frank Mangeruca  
Phone: ( )  
ALS Compass COC Reference: 38354 # Samples: 22 kits Sampler: D'Arcy Morris  
38348 Phone: ( 0437 299 362 )  
Turnaround Requirements: Standard                      Urgent                     

### Special Instructions:

*Tilley Swamp U/S Morella sample, not taken due to unsafe conditions.  
21 samples present instead of usual 22.*

### Custody:

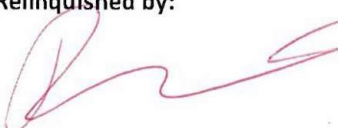Relinquished by:	Received by:	Relinquished by:	Received by:
			
Date / Time:	Date / Time:	Date / Time:	Date / Time:
		<u>14:30 29/9/2022</u>	<u>30/9, 14:00</u>