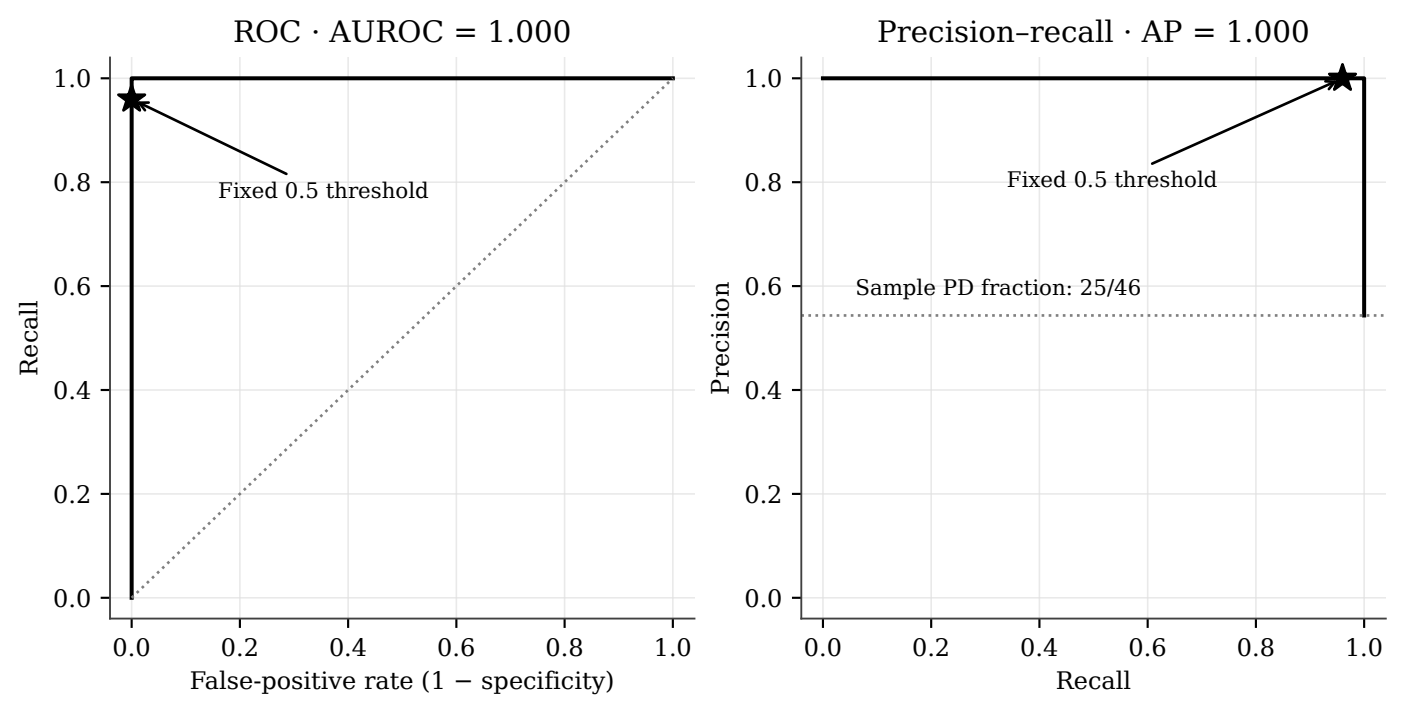
ROC · AUROC = 1.000
Recall
False-positive rate (1 − specificity)
Fixed 0.5 threshold
0.0
0.2
0.4
0.6
0.8
1.0
Precision–recall · AP = 1.000
Precision
Recall
Fixed 0.5 threshold
Sample PD fraction: 25/46