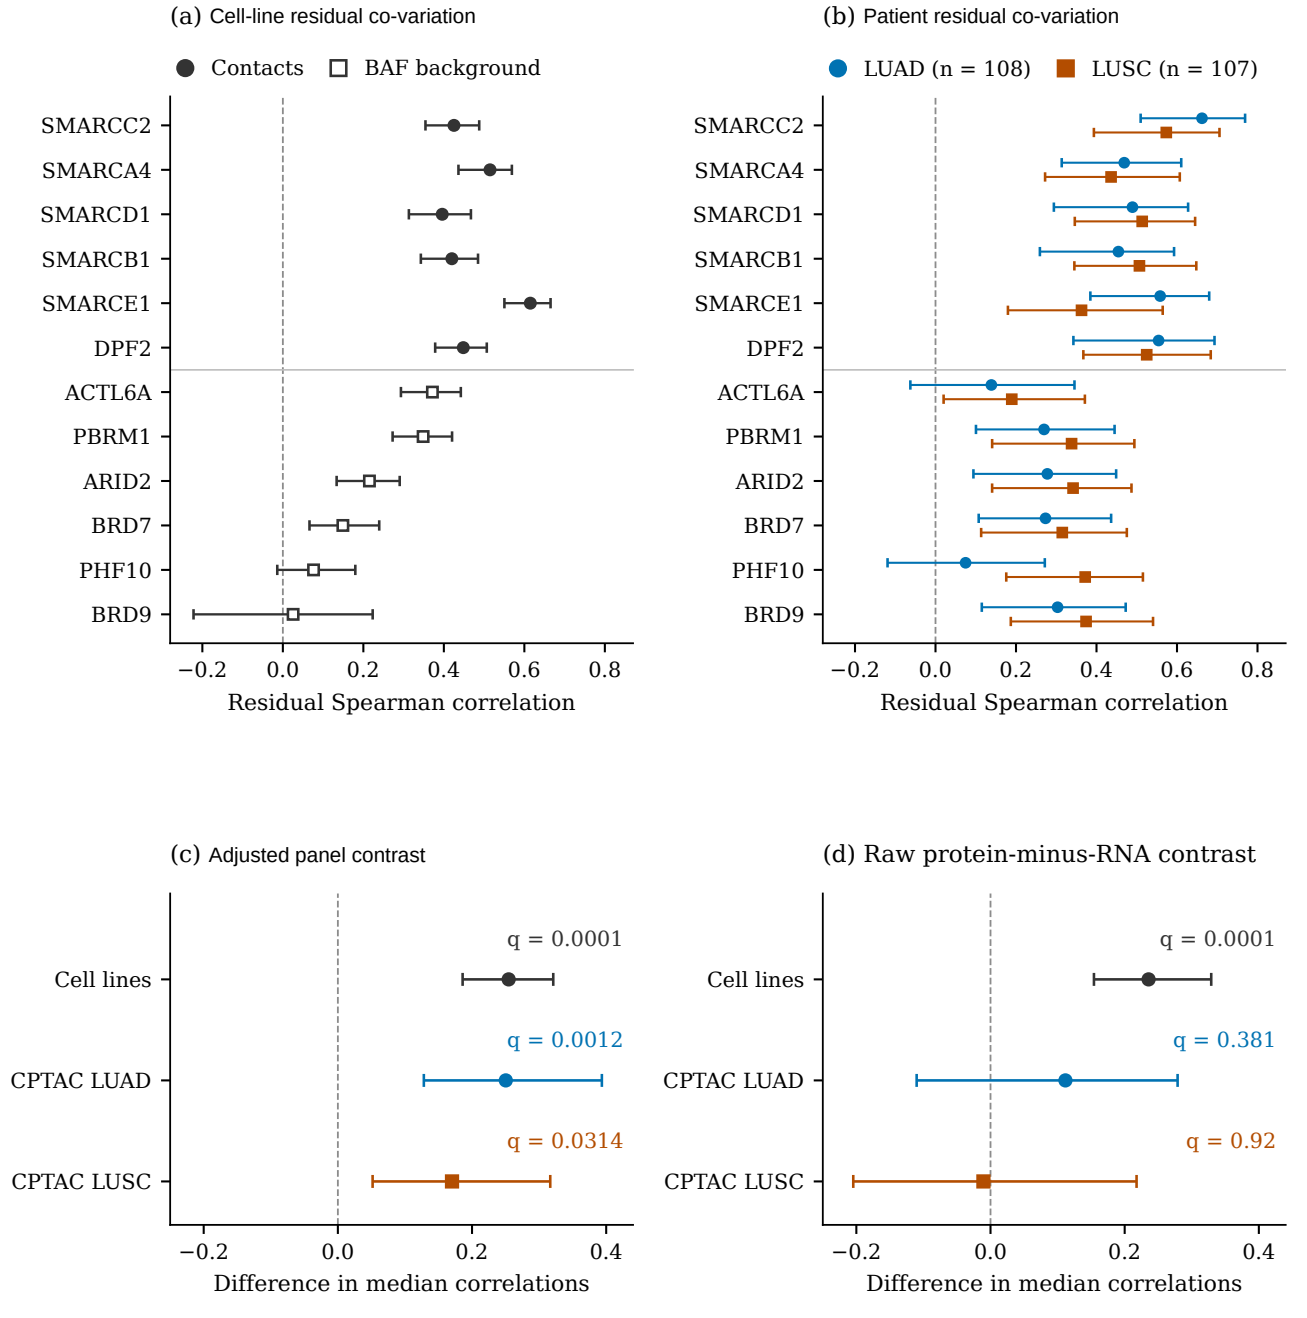

Points: estimates; bars: 95% shared-row refit bootstrap intervals (10,000 draws).
Fixed 6-contact / 6-background panel; raw layer contrast is corrected-null in both patient cohorts.