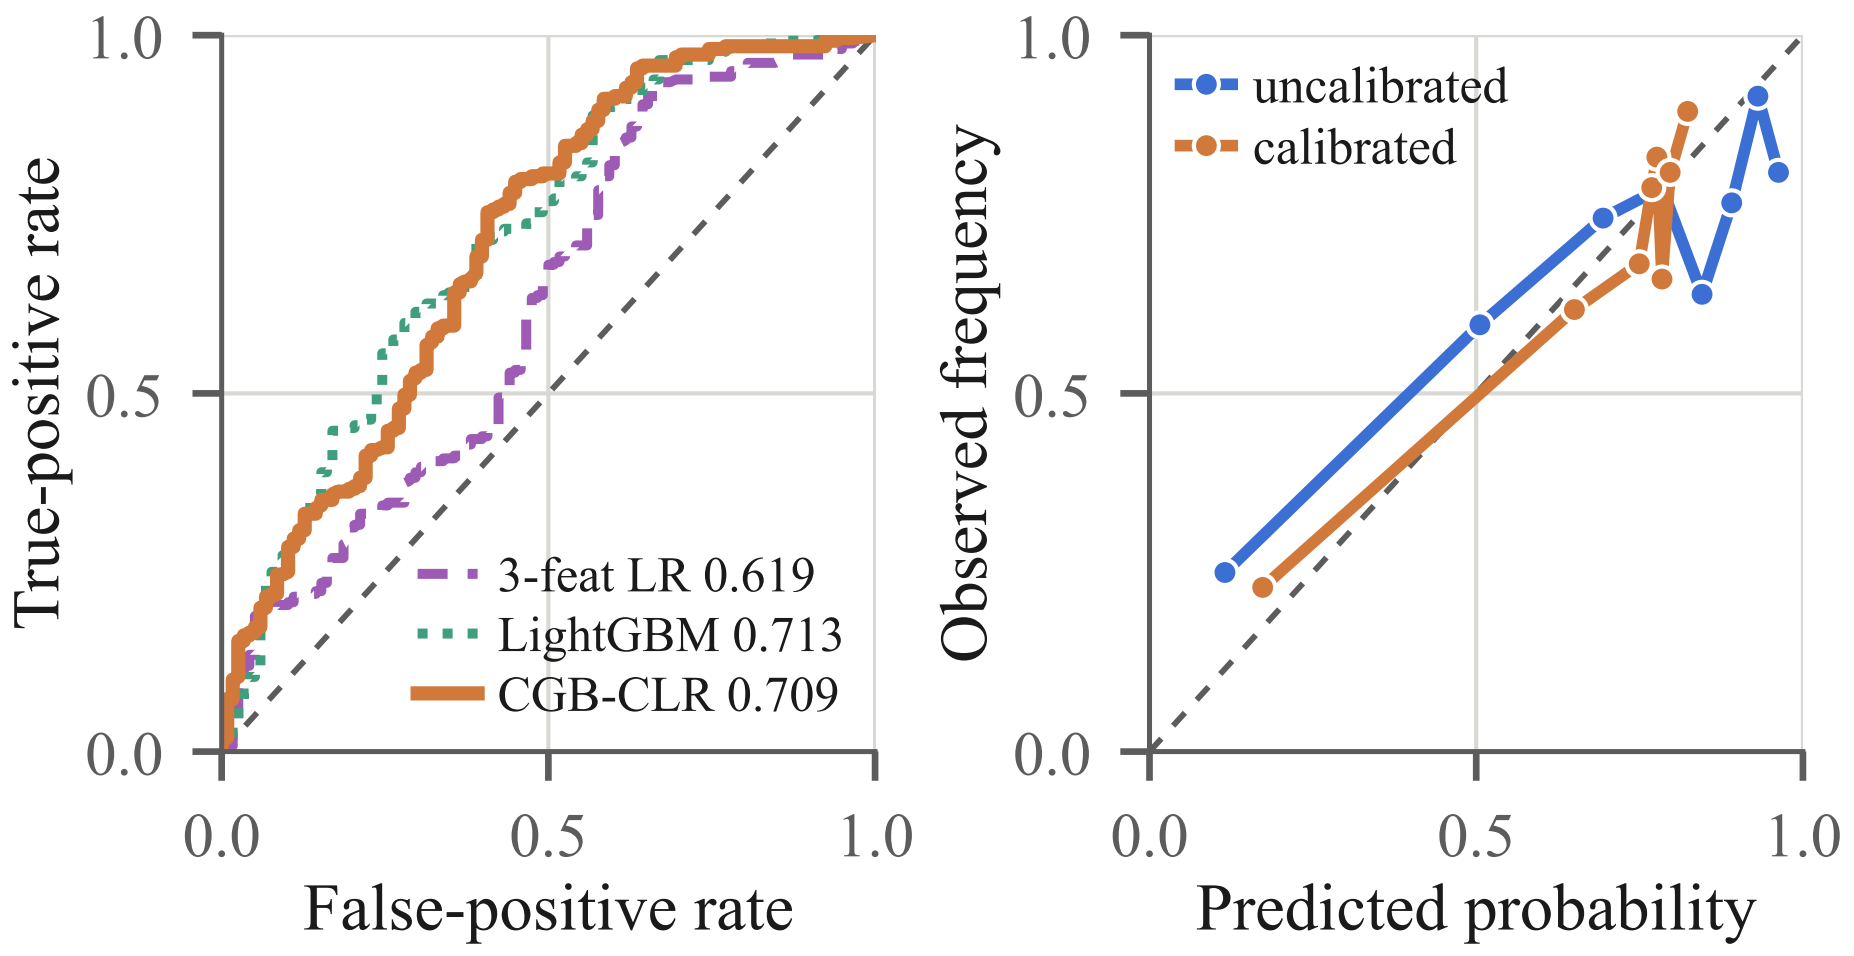
1.0
0.5
0.0
True-positive rate
0.0
0.5
1.0
False-positive rate
3-feat LR 0.619
LightGBM 0.713
CGB-CLR 0.709
1.0
0.5
0.0
Observed frequency
0.0
0.5
1.0
Predicted probability
uncalibrated
calibrated