ANALOG DEVICES

UX Version：ADI_UX_200730_V1.7

Designer :Holiday

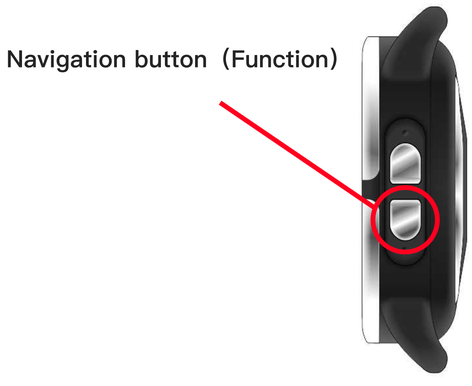

Gestures specifications

Navigation button		starting up/next
Action button		confirm
Navigation button Long press		restart
Navigation button ＋ Action button Long press		upgrade
		Automatic jump

Gesture Specifications for Automatic shutdown

		static page	dynamic page	power on
Automatic shutdown	BLE Disconnected	30s+1min	60s+1min	 Navigation button Long press
	USB cable Disconnected			
	Filesystem Logging stopped			
	No Key Press and screen touch detected			

Dynamic Page

updating　　Heart rate measurement　　Waveform measurement

Starting up、Power off、Bluetooth pairing

starting up

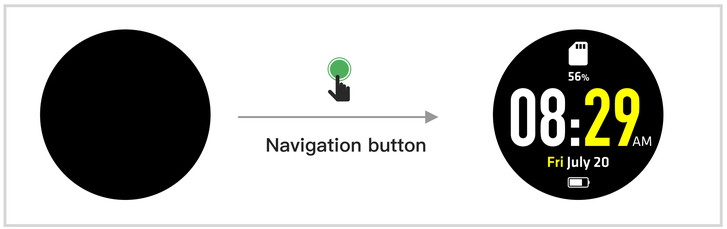

In power off mode, press the Navigation button for 1s to start the machine

starting up in shipment mode

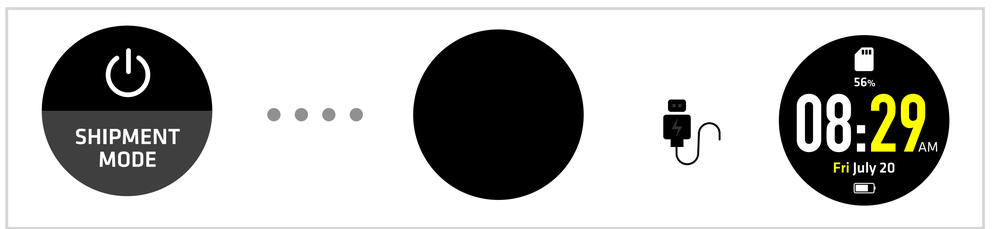

It must be started with a charging cable

restart

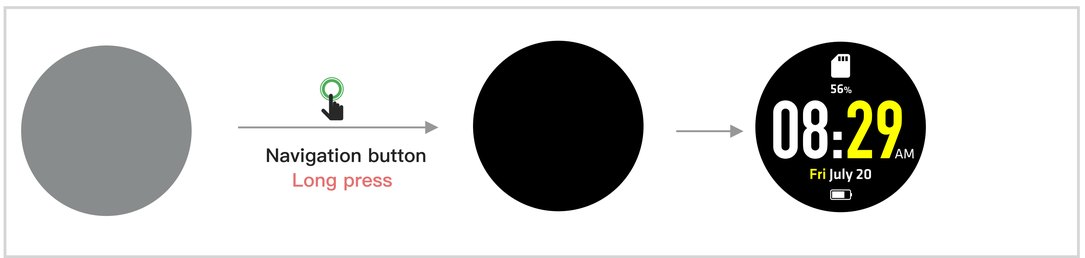

upgrade

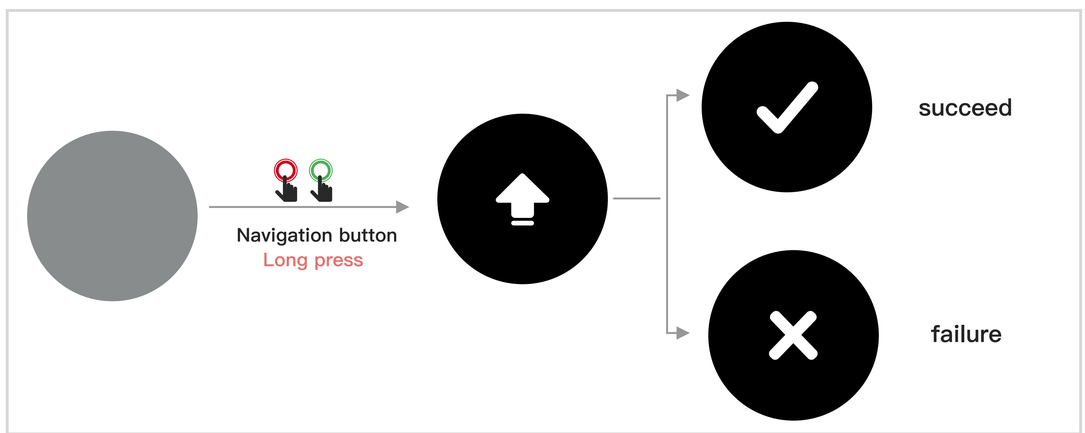

Main interface（static page）

No action in current Page：Backlight will auto close after 30s

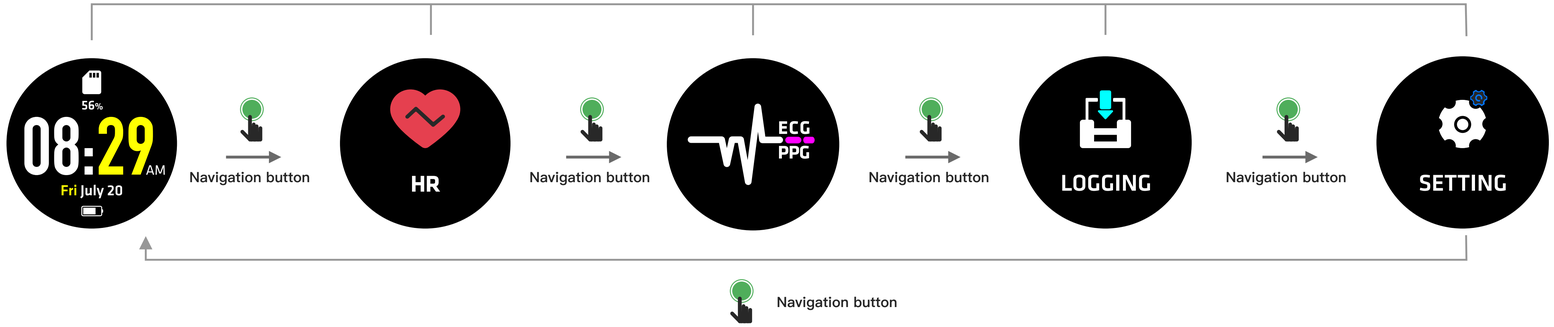

Heart rate

No action in current Page：Backlight will auto close after 60s

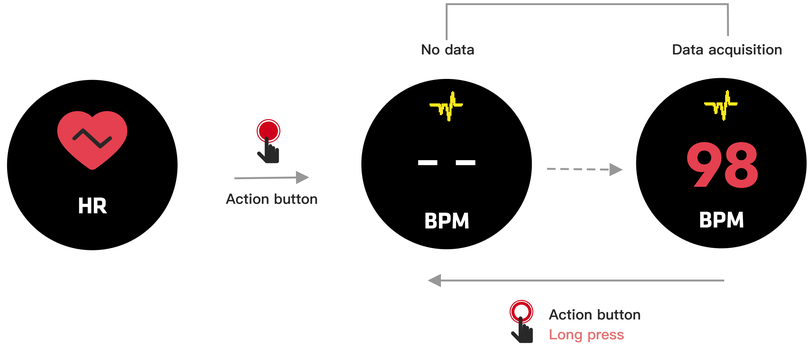

Waveform

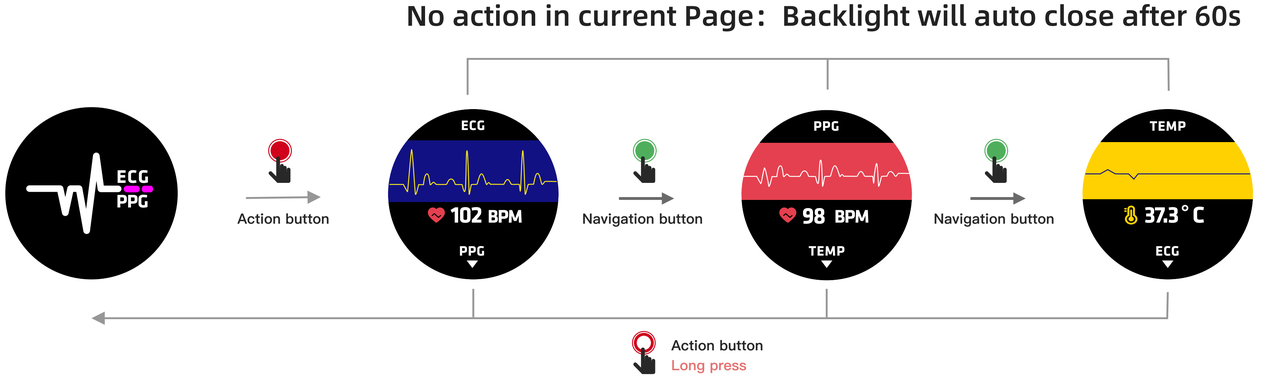
No action in current Page：Backlight will auto close after 60s
ECG
PPG
Action button
ECG
102 BPM
PPG
Navigation button
PPG
98 BPM
TEMP
Navigation button
TEMP
37.3 ° C
ECG
Action button
Long press

Logging（static page）

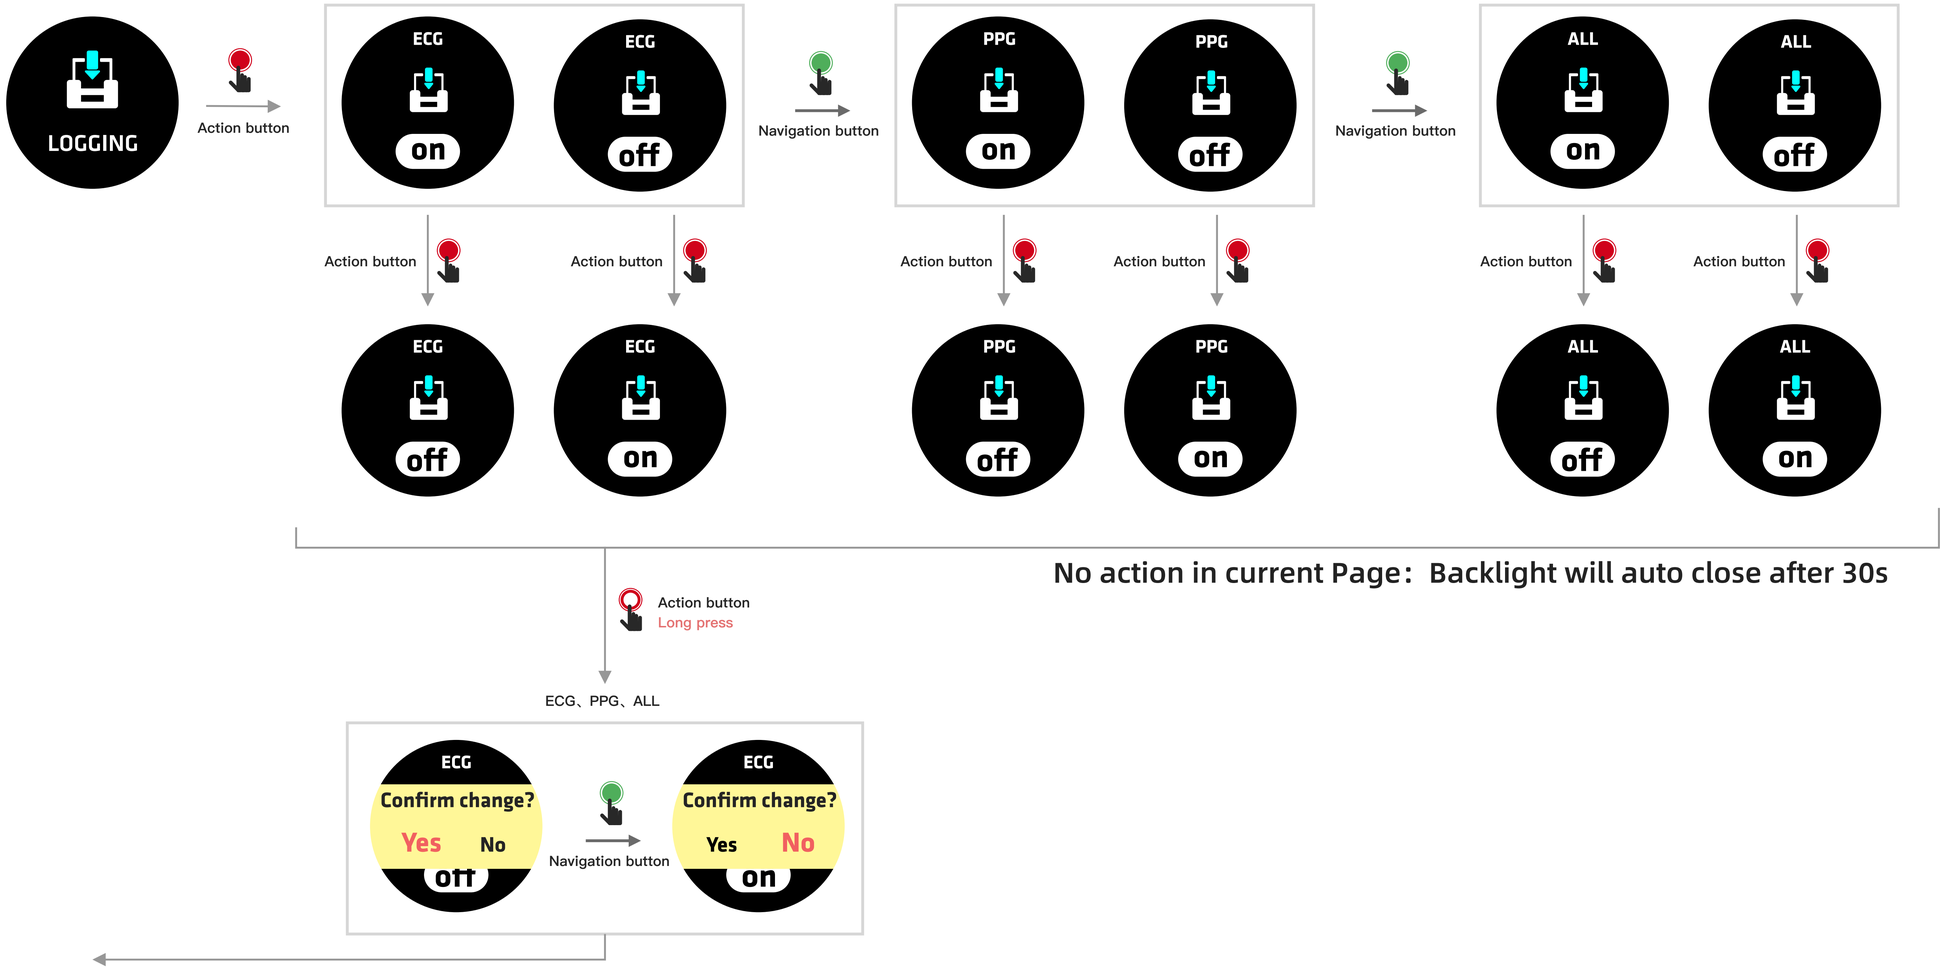
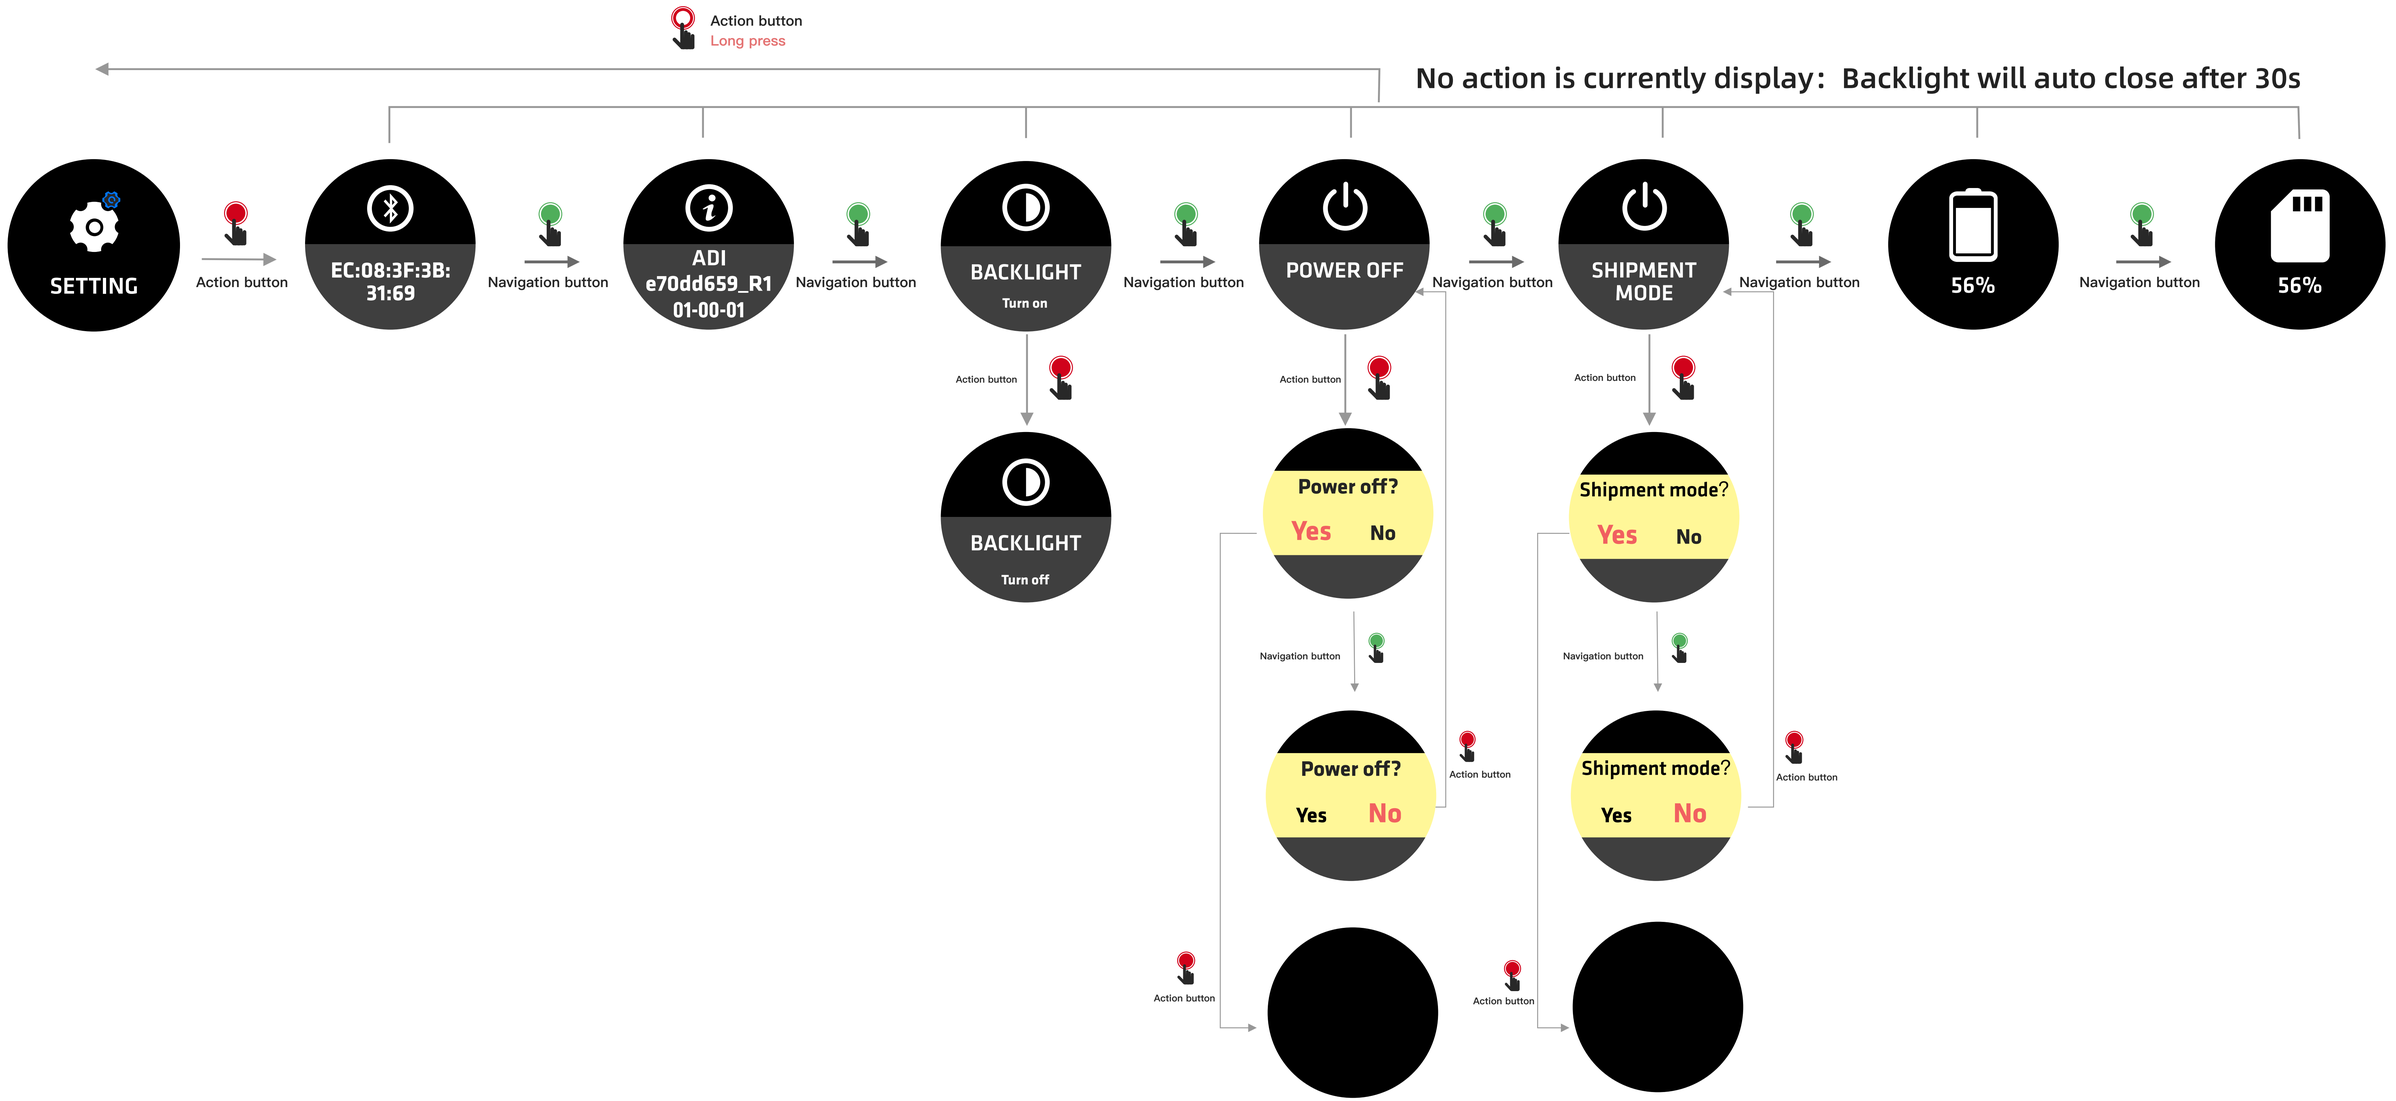
Setting（static page）