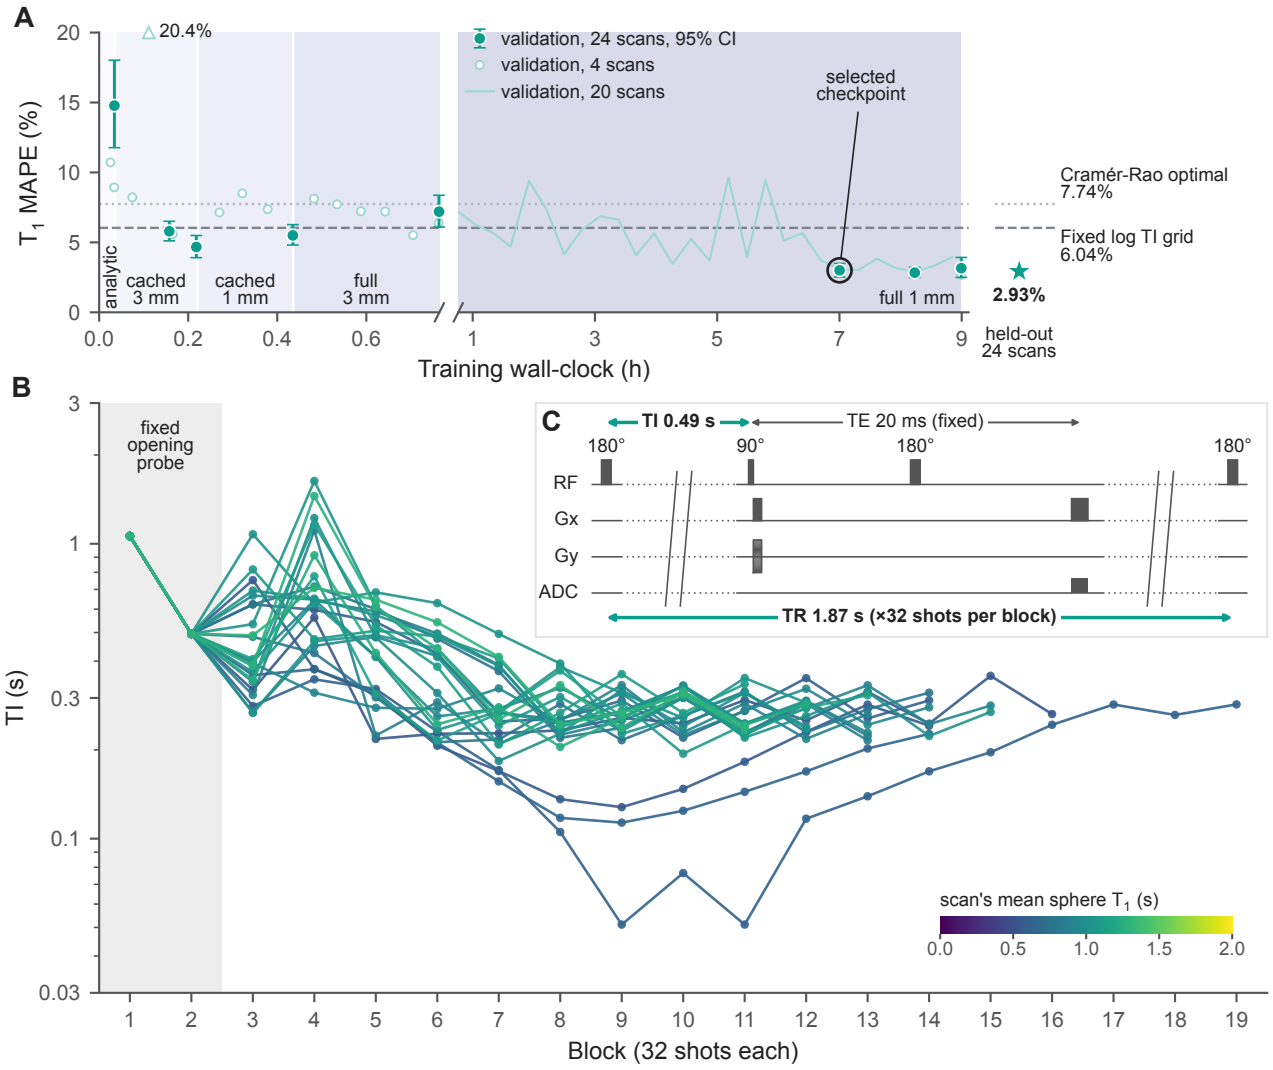

A
20.4%
validation, 24 scans, 95% CI
validation, 4 scans
validation, 20 scans
selected checkpoint
Cramér-Rao optimal 7.74%
Fixed log TI grid 6.04%
2.93%
held-out 24 scans
T1 MAPE (%)
analytic
cached 3 mm
cached 1 mm
full 3 mm
full 1 mm
Training wall-clock (h)
B
fixed opening probe
TI (s)
C
TI 0.49 s
TE 20 ms (fixed)
180°
90°
180°
180°
RF
Gx
Gy
ADC
TR 1.87 s (×32 shots per block)
scan's mean sphere T1 (s)
Block (32 shots each)