

DRISHTI – DR Screening Report

Patient ID: 005b95c28852 · Generated 20260924_001242

ENGINEERING DEMO – NOT a clinical device.

1. Screening Summary

Quality: **WARNING** (score 0.65)

NOT REFERABLE model score 1% (threshold 0.600)

2. Diabetic Retinopathy Grade

Grade 0.000/4

Stage NO DR

Model confidence: 100%


3. Image Quality Assessment

Metric	Value	Status
Overall quality	score 0.65	WARNING


Recapture advice: Image is usable but may benefit from recapture.

4. Visual Evidence (Grad-CAM)

Grad-CAM highlights the retinal regions that most influenced the model decision.

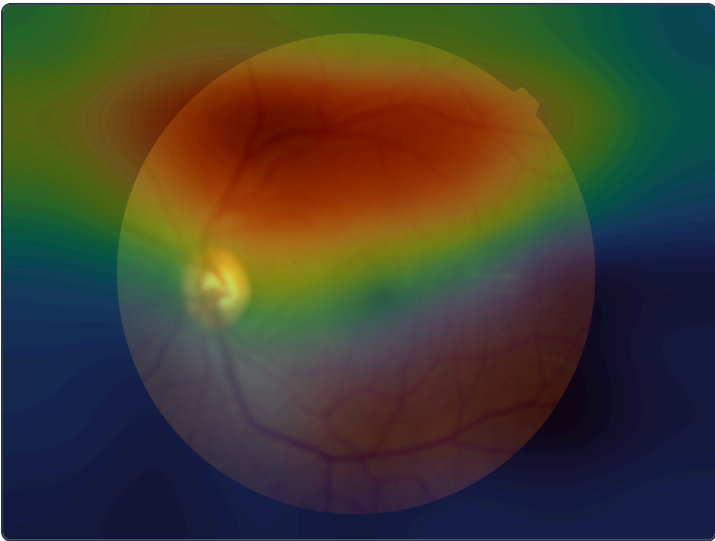

Grad-CAM overlay

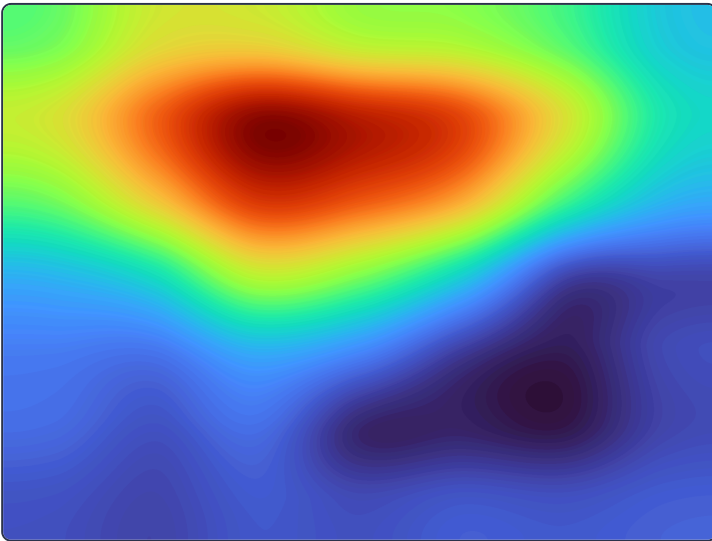

Heat map

5. Interpretation

This analysis is an engineering demonstration and is NOT intended for clinical use or diagnosis. DR severity assessed as No DR (grade 0): no visible diabetic-retinopathy features detected, with model confidence 100.0%. Screening interpretation at the locked referability threshold

(0.60): the image is flagged NON-REFERABLE (P(referable) = 0.9%). Temperature calibration (T=1.00) was applied; the adjusted P(referable) remains 0.9% (delta < 1 pp from raw). Lesion-candidate scan found 0 microaneurysms, 4 haemorrhages and 26 hard exudate regions; haemorrhages are spread across 4 of 4 quadrants (TR/TL/BL/BR = 1/1/1/1), indicating more extensive involvement, and the optic disc was located and excluded from exudate counting (exudate-to-fovea distance not available — fovea localization is not reliable in this build; supply a fovea center to enable it). These are automated candidate counts (not clinical-grade measurements) and serve as supportive evidence only. Image quality: WARNING (score 0.65). The quality flags advise caution in accepting the prediction. The confidence router marked the case CLEAR (high confidence, clear class margin, and screen/grader agreement). Dual-evidence check: Branch B (an independent lesion-feature model) agrees with Branch A (P(referable)=29%). No referable DR features were detected by the screening model; routine follow-up per clinical schedule is advised.

Cascade route: CLEAR

Lesion candidates: MA 0 · HE 4 · EX 26

Runtime: 5.84 s

6. Recommendation

Referable DR: NOT REFERABLE model score 1% (threshold 0.600)

No referable DR features were detected by the screening model; routine follow-up per clinical schedule is advised.