


e51 ablation: completion & detection across 4 variants
(40-course primary ensemble, level=1.0 noise, rate=1000 Hz)

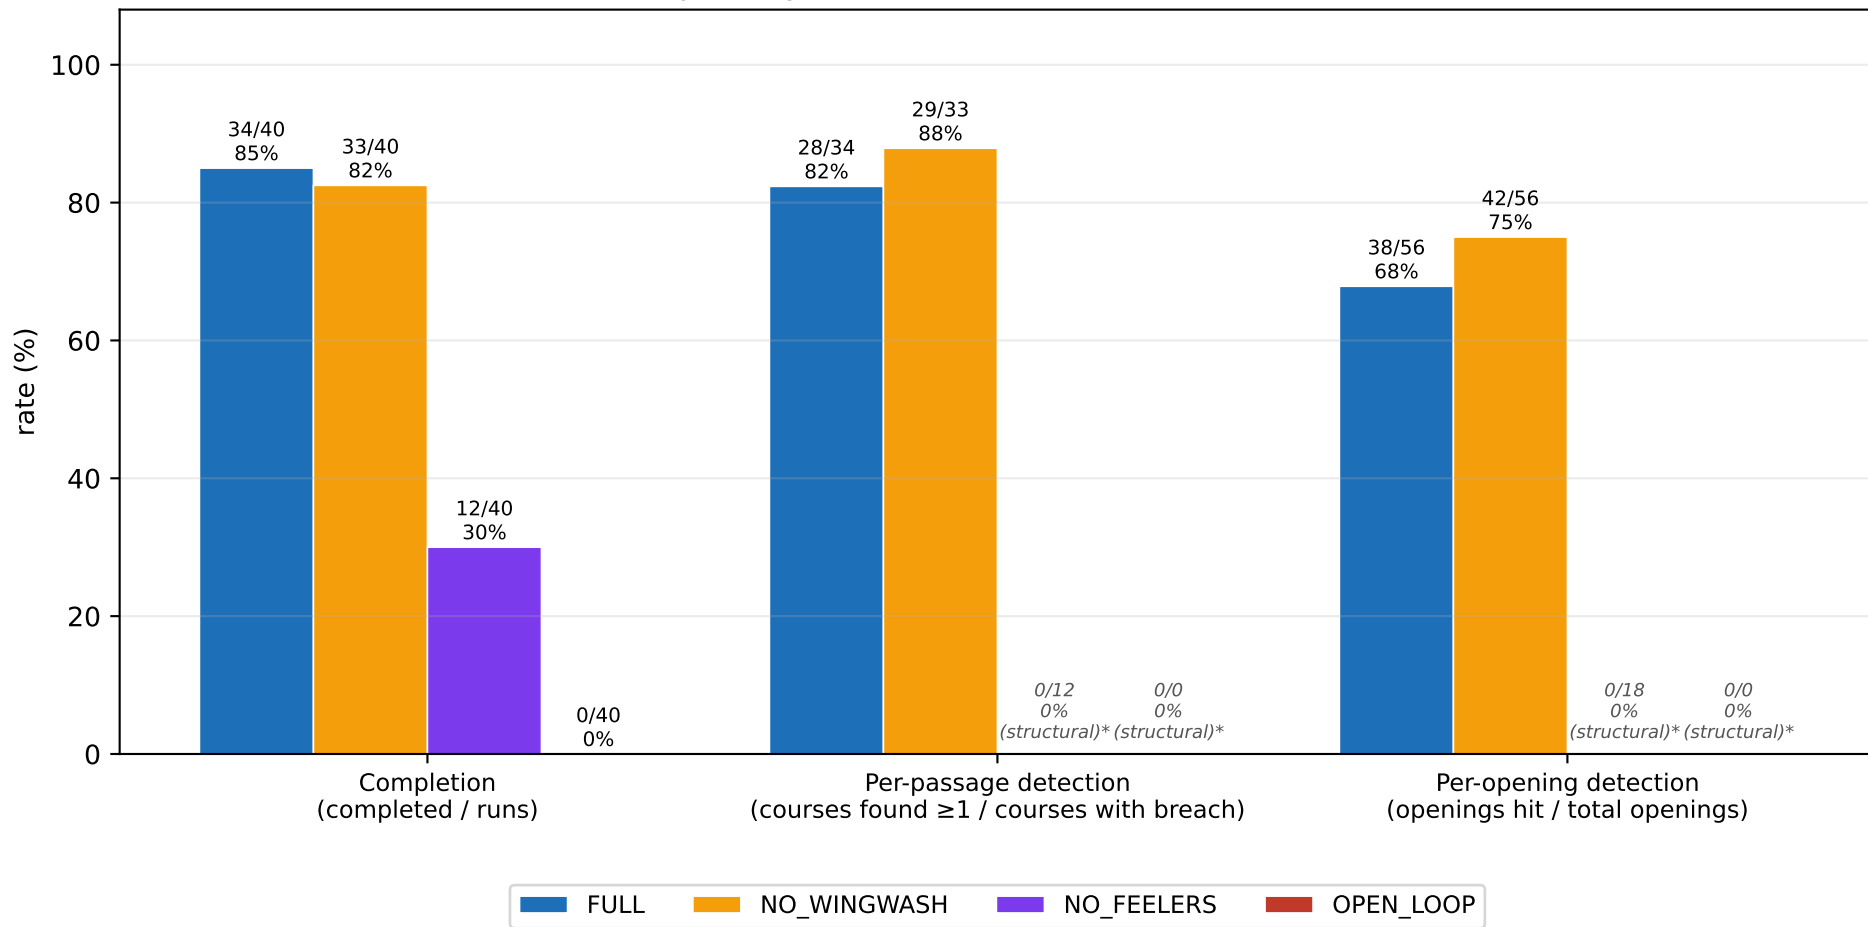

* NO_FEELERS (use_feelers=False) and OPEN_LOOP (open_loop=True, which also forces use_feelers=False) structurally disable the breach logger in e48_mission.py (the `if use\_feelers and (not open\_loop) and ...` guard, e48_mission.py:86) -- 0% is an untried metric, not an observed miss.