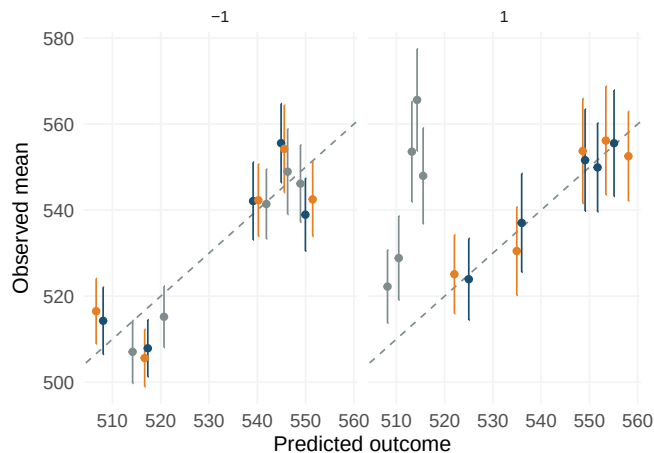
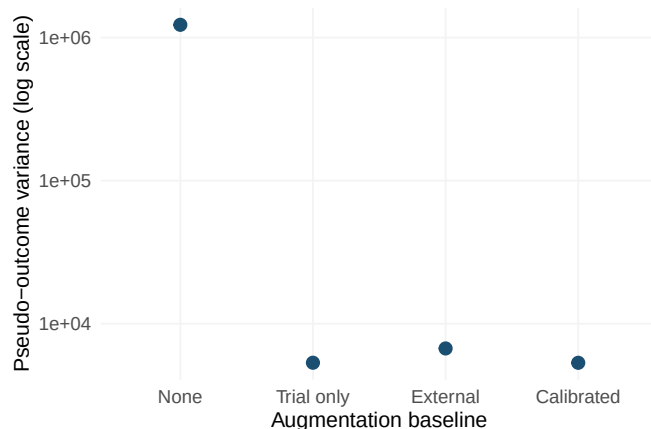
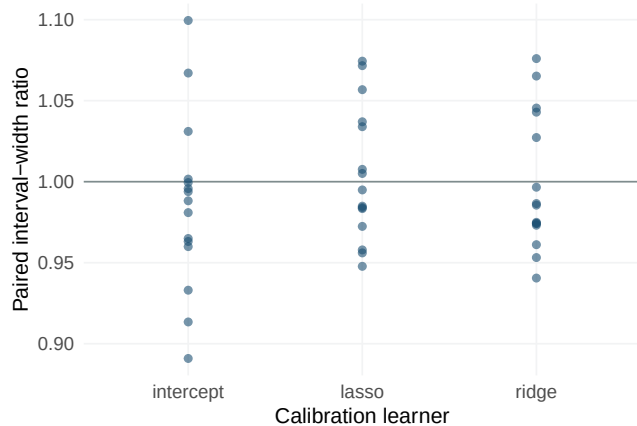


**A****Held-Out Calibration**

stage — calibrated — external — trial\_only

**B****Baseline Comparison****C****Calibration Sensitivity****D****Borrowing Diagnostic**