Rec : 28.08.2031 15:35 Name : **A** 100Years F Ref.Dr.: Consult Dr.:

00cms 00kg PM : n 0:00:10 00/00 mmHg Indian Drug1: No Medication Drug2: No Medication

ID : 0000599 **Hospital : ABCDEFG1234567890HOSPITAL** Diagnosis : Normal

Clinician's Comments :

Rec : 28.08.2031 15:35 Name : **A**
100Years F 00cms 00kg Indian
PM : n 00/00 mmHg **ID : 0000599**

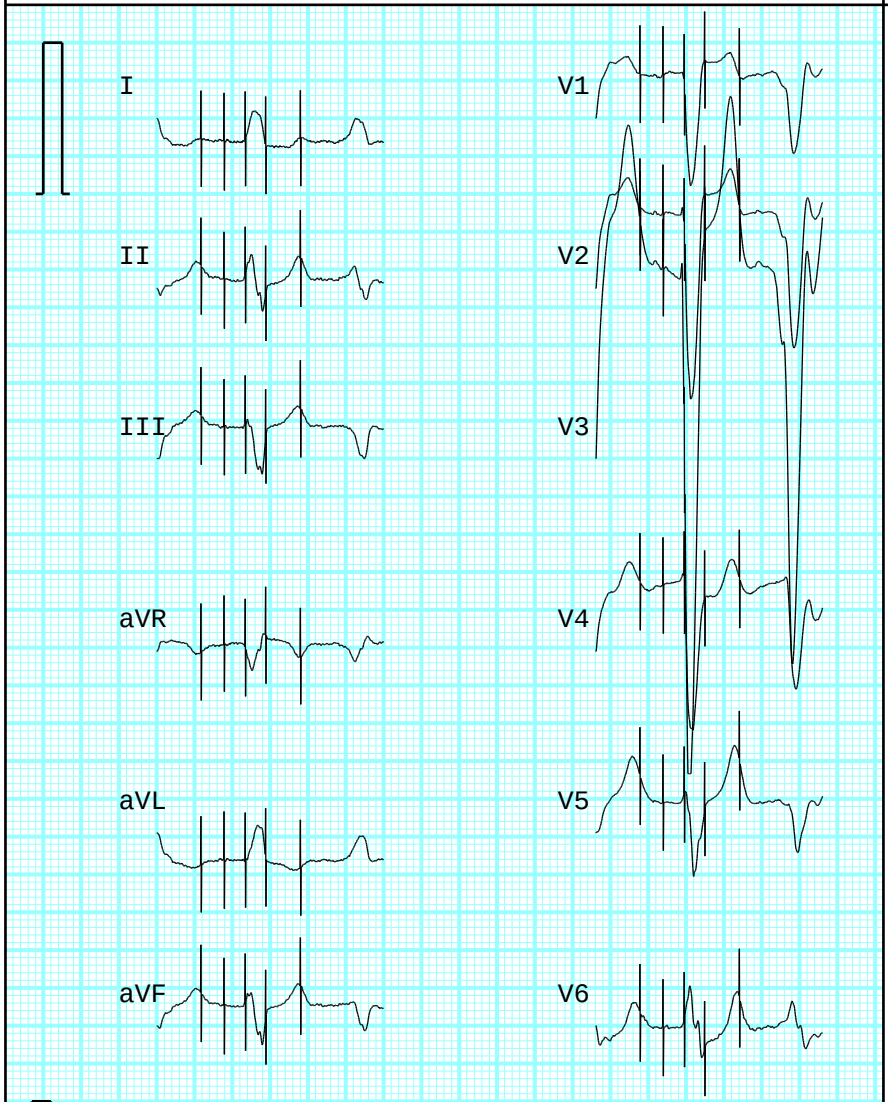

Heart Rate	109 bpm	HRV	433
STFrontalAxis	-143 deg.	TFrontalAxis	90 deg.
ST Duration	72 ms	PR Interval	218 ms
Q-T Interval	366 ms	QTc Hodges	452 ms
QT Dispersion	70 ms		
P Terminal Force	0 ms.uv		

Average beat fiducial point sample number

	Onset	Termination	Duration(ms)
P	232	354	122
QRS	450	586	136
T	658	816	158

*** ACUTE MI / ISCHEMIA ***
Sinus tachycardia with sinus arrhythmia
~ with borderline 1st degree A-V block
Left axis deviation

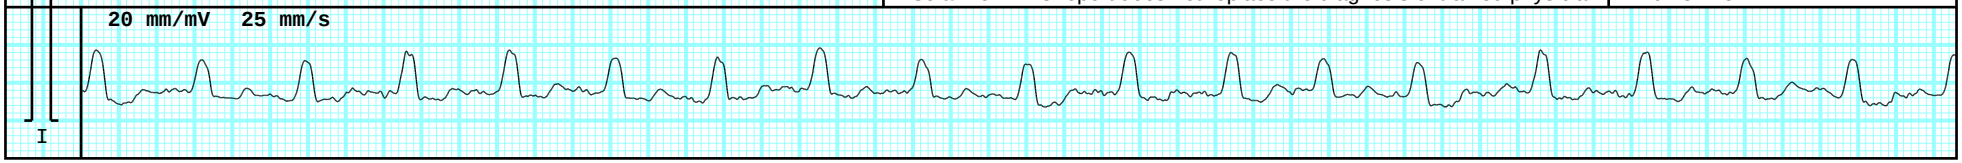

Disclaimer : This report does not replace the diagnosis of trained physician 2.102.841.5

BPL CARDIART GenX3 Measurement Matrix

ID : 0000599 Name : A

Abnormal ECG
of a trained physician

	I	II	III	aVR	aVL	aVF	V1	V2	V3/V4R	V4	V5	V6
P Ons(ms)	232	232	232	232	232	232	232	232	232	232	232	232
P Dur(ms)	122	122	122	122	122	122	122	122	122	122	122	122
QRS Ons	466	460	460	462	478	460	460	450	450	450	452	454
QRS Dur(ms)	108	126	126	90	102	126	98	108	108	128	134	132
Q Dur(ms)	0	0	0	90	0	0	98	0	0	0	0	0
R Dur(ms)	108	63	40	0	102	53	0	13	7	17	33	92
S Dur(ms)	0	62	85	0	0	72	0	94	100	110	100	39
R’ Dur(ms)	0	0	0	0	0	0	0	0	0	0	0	0
S’ Dur(ms)	0	0	0	0	0	0	0	0	0	0	0	0
R’’ Dur(ms)	0	0	0	0	0	0	0	0	0	0	0	0
S’’ Dur(ms)	0	0	0	0	0	0	0	0	0	0	0	0
ST Dur(ms)	116	92	82	138	88	84	84	108	100	82	78	88
T Ons	690	678	668	690	668	670	642	666	658	660	664	674
T Dur(ms)	68	138	148	126	146	146	174	114	154	100	150	138
P+ Dur(ms)	122	122	122	0	28	122	0	122	122	0	122	122
T+ Dur(ms)	28	138	148	0	0	146	110	114	154	84	150	138
QRS IntD	52	40	20	0	54	38	0	8	6	10	22	44
P+ Amp(mV)	28	131	103	0	11	117	0	74	502	0	236	139
P- Amp(mV)	0	0	0	-79	-37	0	-41	0	0	-88	0	0
P2P Amp(mV)	257	470	454	227	289	430	932	1586	4480	1295	704	594
Q Amp(mV)	0	0	0	-227	0	0	-932	0	0	0	0	0
R Amp(mV)	257	221	68	0	289	113	0	62	113	54	94	346
S Amp(mV)	0	-249	-386	0	0	-317	0	-1524	-4367	-1241	-610	-248
R’ Amp(mV)	0	0	0	0	0	0	0	0	0	0	0	0
S’ Amp(mV)	0	0	0	0	0	0	0	0	0	0	0	0
R’’ Amp(mV)	0	0	0	0	0	0	0	0	0	0	0	0
S’’ Amp(mV)	0	0	0	0	0	0	0	0	0	0	0	0
ST Amp(mV)	-30	-36	-5	33	-12	-21	89	166	405	-134	0	-125
ST80 Amp(mV)	-36	5	42	15	-39	24	111	232	812	-47	113	-51
STT28 Amp(mV)	-33	-10	30	25	-35	10	93	182	577	-133	67	-90
STT38 Amp(mV)	-33	9	45	14	-41	27	124	215	910	-93	144	-37
T+ Amp(mV)	31	203	176	0	0	188	167	380	1490	171	470	298
T- Amp(mV)	-45	0	0	-117	-83	0	-52	0	0	-73	0	0
QRS Area	879	-22	-902	-428	891	-462	-2591	-4206	-12239	-4037	-1357	208
P Area	-80	-522	-441	300	181	-481	-115	-334	-2031	-337	-1122	-657
T Area	-219	671	828	-257	-492	750	761	2070	8159	-5	2135	551
P Morph	1	1	1	-1	-2	1	-1	1	1	-1	1	1
T Morph	-2	1	1	-1	-1	1	2	1	1	-2	1	1
R Notch	0	0	0	0	0	0	0	0	0	0	0	0