Rec : 28.08.2031 15:37 Name : **A** 100Years F

00cms 00kg PM : n 0:00:10 00/00 mmHg Indian

ID : 0000601 **Hospital : ABCDEFG1234567890HOSPITAL**

Ref.Dr.: Consult Dr.:

Drug1: No Medication Drug2: No Medication

Diagnosis : Normal Page 1/3

Clinician's Comments :

Rec : 28.08.2031 15:37 Name : **A**
100Years F 00cms 00kg Indian
PM : n 00/00 mmHg **ID : 0000601**

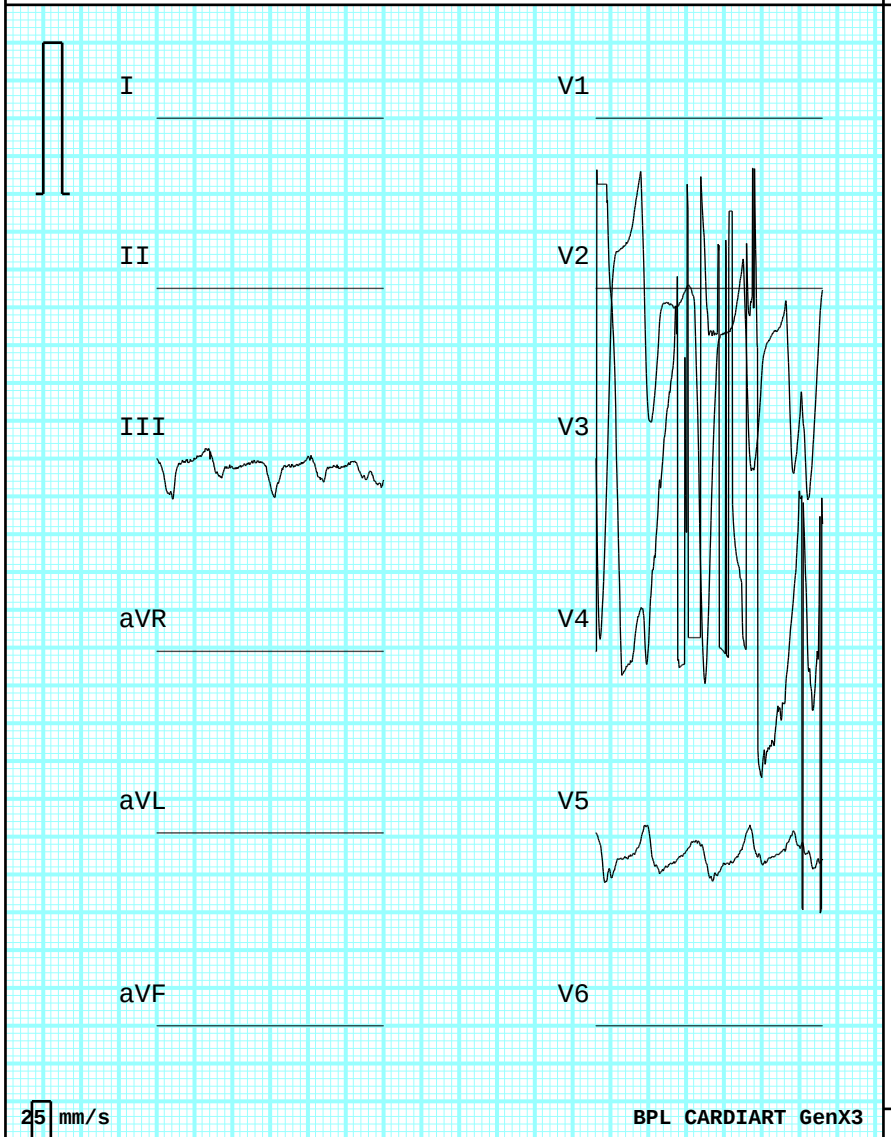

Heart Rate 129 bpm HRV 0

QrsFrontalAxis **** PFrontalAxis ****
STFrontalAxis **** deg. TFrontalAxis **** deg.
ST Duration 6 ms PR Interval ****
Q-T Interval 280 ms QTc Hodges 401 ms
QT Dispersion 60 ms
P Terminal Force ****

Average beat fiducial point sample number

	Onset	Termination	Duration(ms)
P	294	448	154
QRS	466	574	108
T	580	746	166

*** CONSIDER ACUTE STEMI ***
Atrial fibrillation
~ with rapid ventricular response
Demand pacing

Lead(s) unsuitable for analysis:

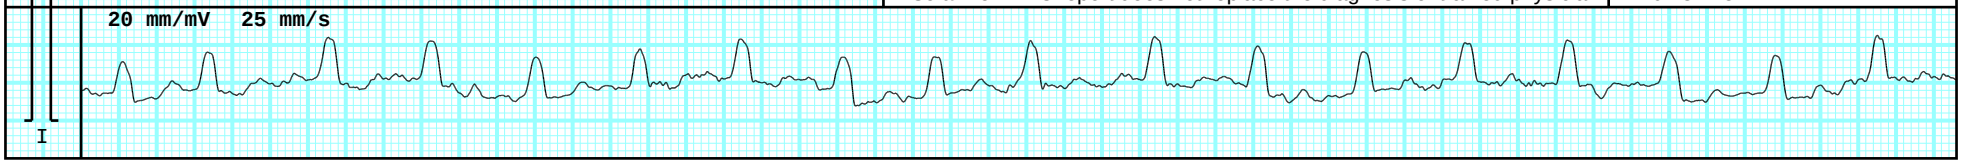

Disclaimer : This report does not replace the diagnosis of trained physician | 2.102.841.5

BPL CARDIART GenX3 Measurement Matrix

ID : 0000601 Name : A

~ V6

of a trained physician

*** ANTERIOR INFARCT - POSSIBLY ACUTE ***

Small inferior Q waves: infarct cannot be excluded

Lateral ST-T abnormality

~ is nonspecific

P Ons(ms)	***	***	***	***	***	***	***	***	***	***	***	***
P Dur(ms)	***	***	***	***	***	***	***	***	***	***	***	***

Tall T waves - consider acute ischemia or hyperkalemia

Abnormal ECG

Q Dur(ms)	***	***	0	***	***	***	***	***	0	0	0	***
R Dur(ms)	***	***	50	***	***	***	***	***	46	108	104	***
S Dur(ms)	***	***	0	***	***	***	***	***	0	0	0	***
R′ Dur(ms)	***	***	0	***	***	***	***	***	0	0	0	***
S′ Dur(ms)	***	***	0	***	***	***	***	***	0	0	0	***
R′′ Dur(ms)	***	***	0	***	***	***	***	***	0	0	0	***
S′′ Dur(ms)	***	***	0	***	***	***	***	***	0	0	0	***
ST Dur(ms)	***	***	32	***	***	***	***	***	68	18	34	***
T Ons	***	***	580	***	***	***	***	***	580	596	608	***
T Dur(ms)	***	***	166	***	***	***	***	***	166	90	138	***
P+ Dur(ms)	***	***	***	***	***	***	***	***	***	***	***	***
T+ Dur(ms)	***	***	0	***	***	***	***	***	0	90	0	***
QRS IntD	***	***	18	***	***	***	***	***	26	26	60	***
P+ Amp(mV)	***	***	***	***	***	***	***	***	***	***	***	***
P- Amp(mV)	***	***	***	***	***	***	***	***	***	***	***	***
P2P Amp(mV)	***	***	***	***	***	***	***	***	***	***	***	***
Q Amp(mV)	***	***	0	***	***	***	***	***	0	0	0	***
R Amp(mV)	***	***	32	***	***	***	***	***	80	6987	121	***
S Amp(mV)	***	***	0	***	***	***	***	***	0	0	0	***
R′ Amp(mV)	***	***	0	***	***	***	***	***	0	0	0	***
S′ Amp(mV)	***	***	0	***	***	***	***	***	0	0	0	***
R′′ Amp(mV)	***	***	0	***	***	***	***	***	0	0	0	***
S′′ Amp(mV)	***	***	0	***	***	***	***	***	0	0	0	***
ST Amp(mV)	***	***	-18	***	***	***	***	***	-3188	3442	-8	***
ST80 Amp(mV)	***	***	-100	***	***	***	***	***	-377	1425	-141	***
STT28 Amp(mV)	***	***	-263	***	***	***	***	***	-1434	2739	-213	***
STT38 Amp(mV)	***	***	-169	***	***	***	***	***	-643	2727	-165	***
T+ Amp(mV)	***	***	0	***	***	***	***	***	0	2859	0	***
T- Amp(mV)	***	***	-274	***	***	***	***	***	-3189	0	-213	***
QRS Area	***	***	46	***	***	***	***	***	-4719	24701	423	***
P Area	***	***	***	***	***	***	***	***	***	***	***	***
T Area	***	***	-777	***	***	***	***	***	-8108	11535	-904	***
P Morph	***	***	***	***	***	***	***	***	***	***	***	***
T Morph	***	***	-1	***	***	***	***	***	-1	1	-1	***
R Notch	***	***	0	***	***	***	***	***	0	1	0	***