Rec : 28.08.2031 15:36 Name : **A** 100Years F Ref.Dr.: Consult Dr.:

00cms 00kg PM : n 0:00:10 00/00 mmHg Indian Drug1: No Medication Drug2: No Medication

ID : 0000600 **Hospital : ABCDEFG1234567890HOSPITAL** Diagnosis : Normal Page 1/3

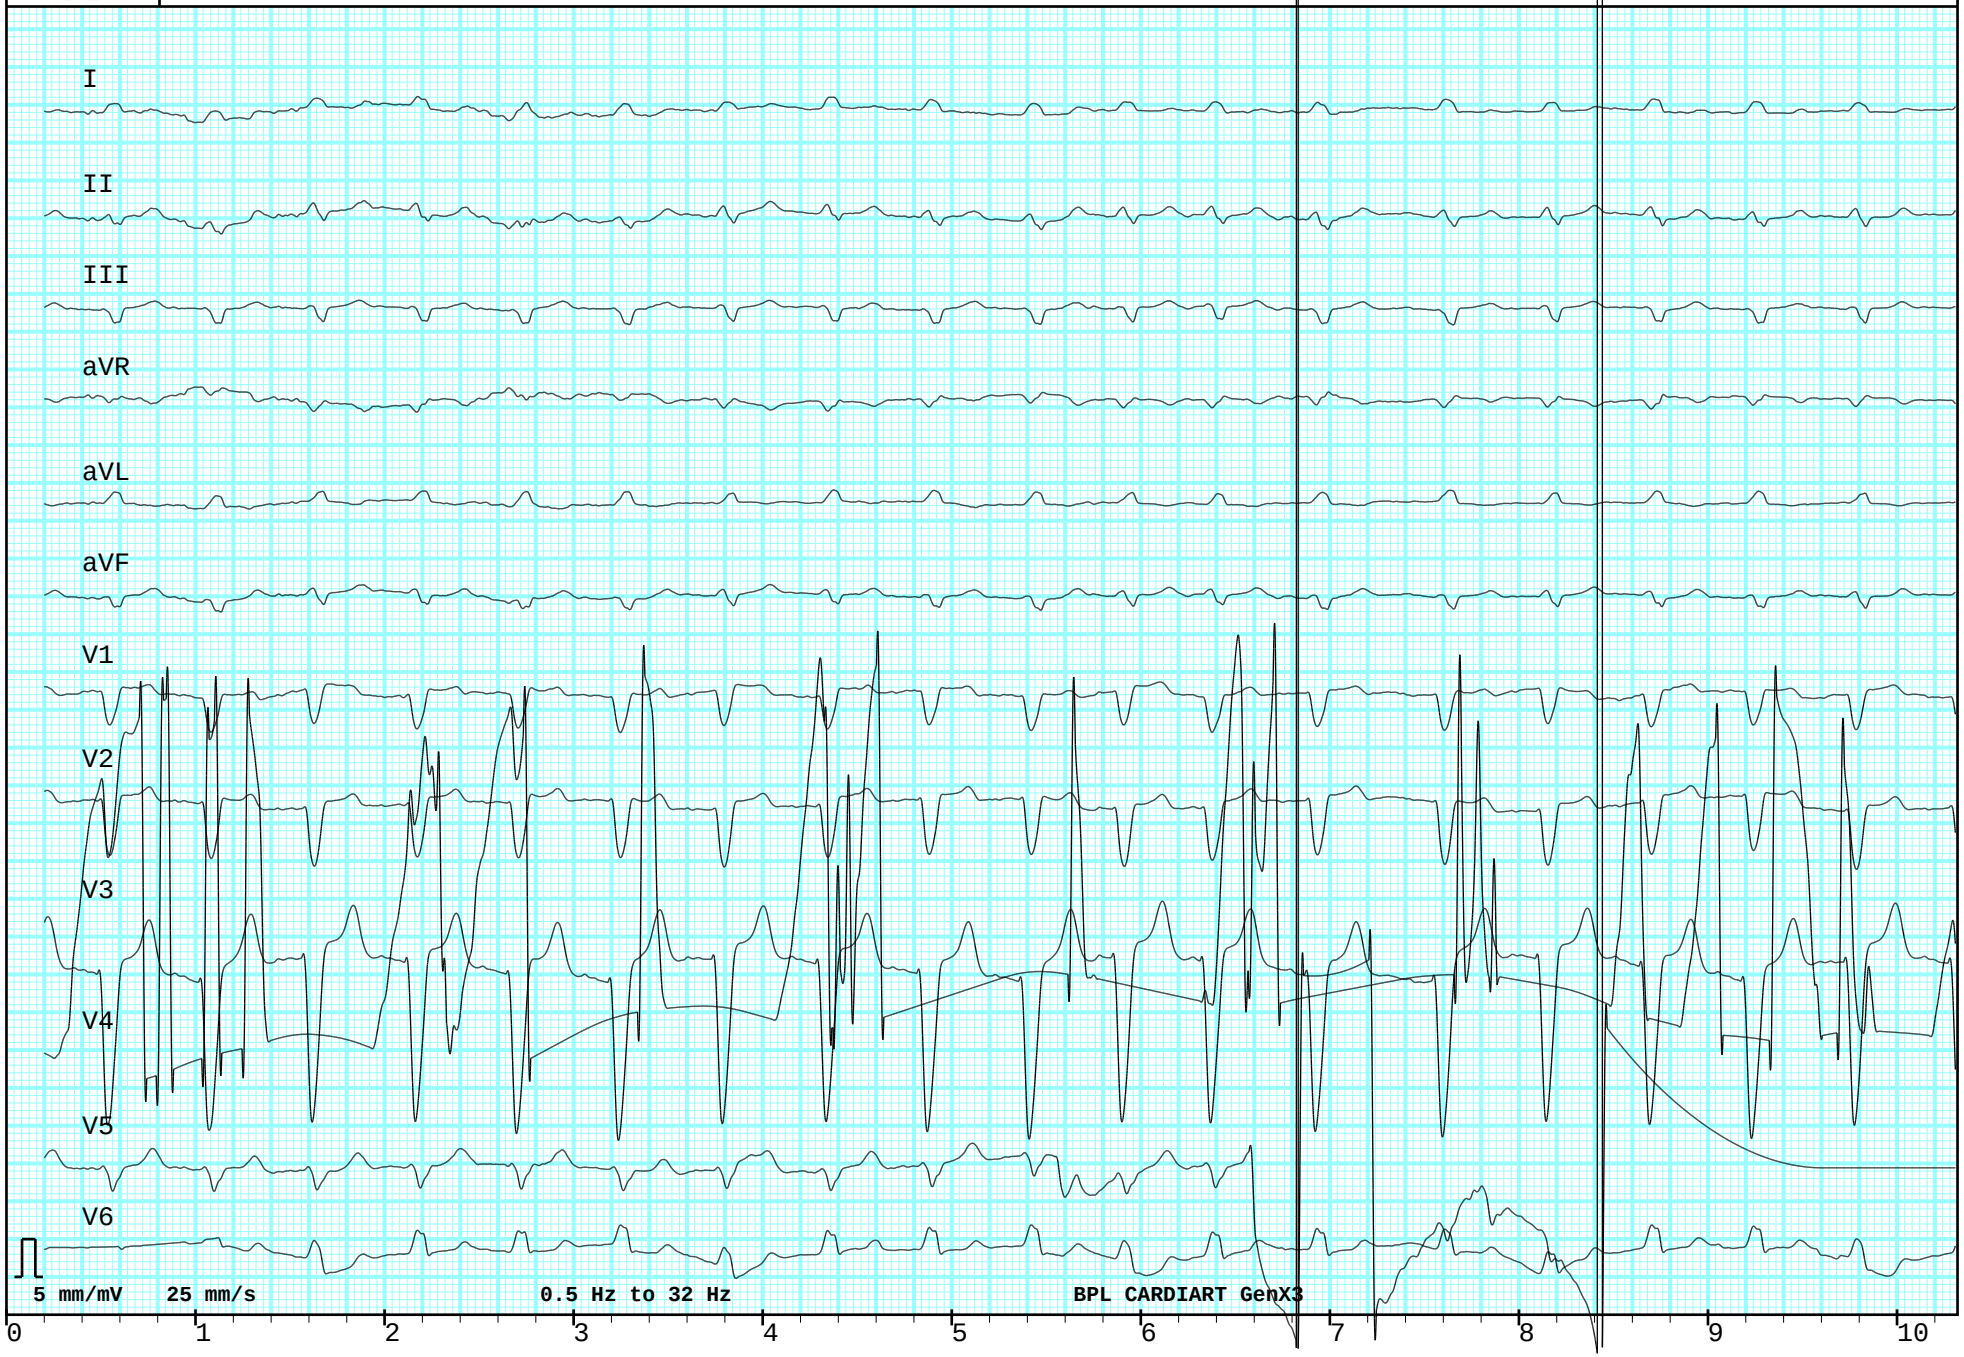

Clinician's Comments :

Rec : 28.08.2031 15:36 Name : **A**
100Years F 00cms 00kg Indian
PM : n 00/00 mmHg **ID : 0000600**

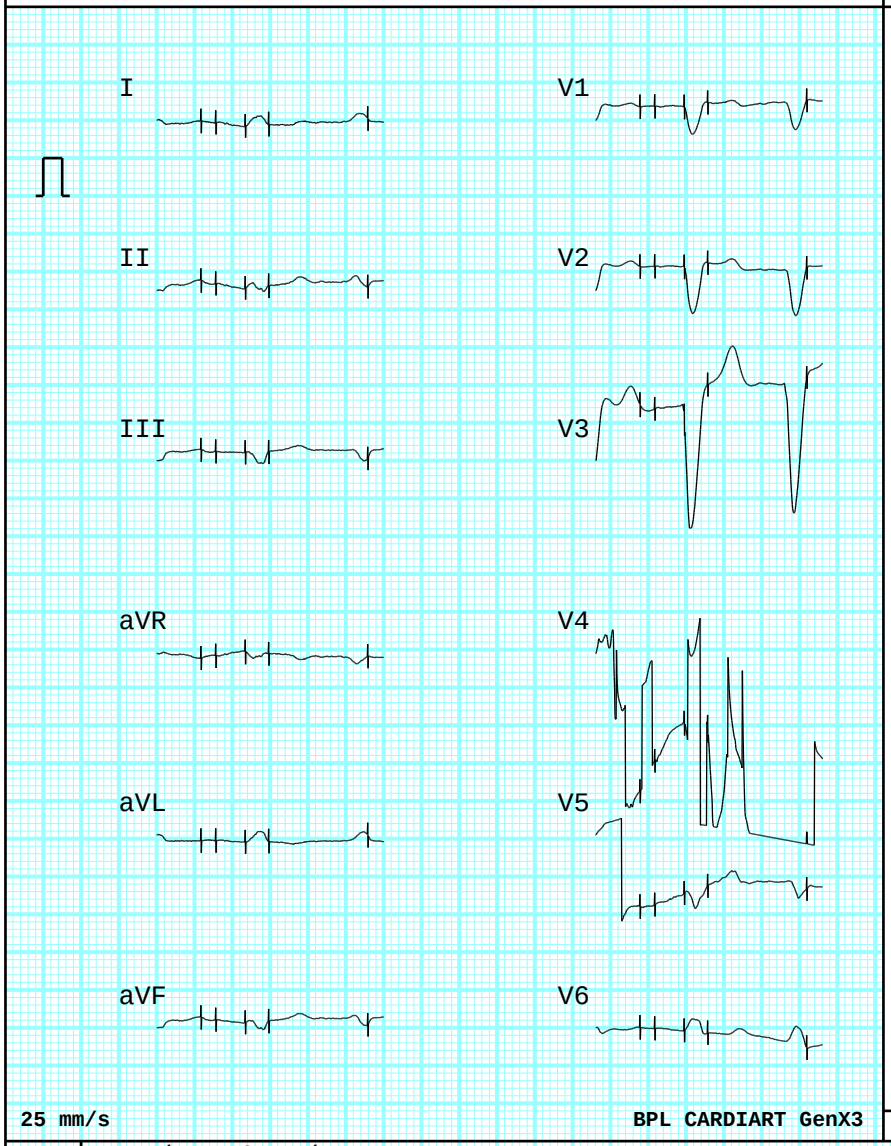

Heart Rate	36 bpm	HRV	0
QrsFrontalAxis	-14	PFrontalAxis	50
STFrontalAxis	49 deg.	TFrontalAxis	28 deg.
ST Duration	2 ms	PR Interval	****
Q-T Interval	654 ms	QTc Hodges	612 ms
QT Dispersion	40 ms		
P Terminal Force	****		

Average beat fiducial point sample number

	Onset	Termination	Duration(ms)
P	232	310	78
QRS	460	598	138
T	600	1114	514

*** EXTREME BRADYCARDIA ***
Atrial fibrillation
~ with slow ventricular response
~ with PVC(s)

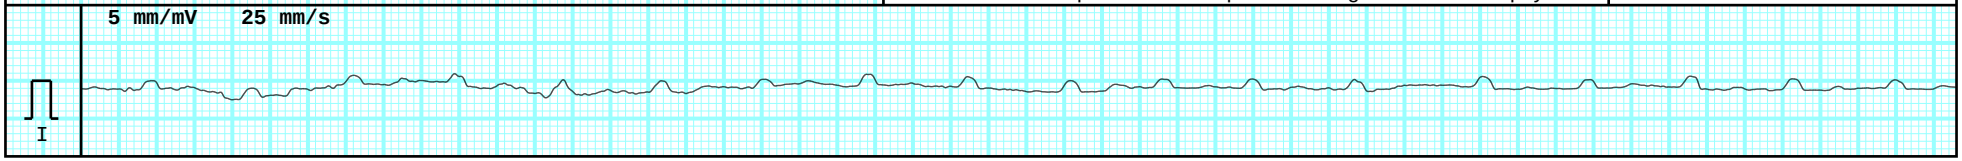

Disclaimer : This report does not replace the diagnosis of trained physician | 2.102.841.5

BPL CARDIART GenX3 Measurement Matrix

ID : 0000600 Name : A

~ may be due to the hypertrophy and/or ischemia
of a trained physician

Tall T waves - consider acute ischemia or hyperkalemia
Low QRS voltages in limb leads
Abnormal ECG

	I	II	III	aVR	aVL	aVF	V1	V2	V3/V4R	V4	V5	V6
P Ons(ms)	***	***	***	***	***	***	***	***	***	***	***	***
P Dur(ms)	***	***	***	***	***	***	***	***	***	***	***	***
QRS Ons	466	462	466	464	480	462	466	468	460	460	460	468
QRS Dur(ms)	124	116	122	104	112	122	98	130	102	138	104	96
Q Dur(ms)	0	0	0	104	0	0	98	130	102	0	0	0
R Dur(ms)	124	94	27	0	112	55	0	0	0	10	40	96
S Dur(ms)	0	21	94	0	0	66	0	0	0	14	63	0
R′ Dur(ms)	0	0	0	0	0	0	0	0	0	68	0	0
S′ Dur(ms)	0	0	0	0	0	0	0	0	0	44	0	0
R′′ Dur(ms)	0	0	0	0	0	0	0	0	0	0	0	0
S′′ Dur(ms)	0	0	0	0	0	0	0	0	0	0	0	0
ST Dur(ms)	10	22	12	80	8	16	58	48	38	2	36	38
T Ons	600	600	600	648	600	600	622	646	600	600	600	602
T Dur(ms)	514	500	514	466	514	492	484	468	498	502	470	492
P+ Dur(ms)	***	***	***	***	***	***	***	***	***	***	***	***
T+ Dur(ms)	514	500	460	0	514	492	394	0	412	178	470	304
QRS IntD	84	48	16	0	70	28	0	0	0	90	24	42
P+ Amp(mV)	***	***	***	***	***	***	***	***	***	***	***	***
P- Amp(mV)	***	***	***	***	***	***	***	***	***	***	***	***
P2P Amp(mV)	***	***	***	***	***	***	***	***	***	***	***	***
Q Amp(mV)	0	0	0	-256	0	0	-917	-1559	-4154	0	0	0
R Amp(mV)	367	221	36	0	353	98	0	0	0	41	134	407
S Amp(mV)	0	-77	-355	0	0	-211	0	0	0	-429	-441	0
R′ Amp(mV)	0	0	0	0	0	0	0	0	0	3492	0	0
S′ Amp(mV)	0	0	0	0	0	0	0	0	0	-3365	0	0
R′′ Amp(mV)	0	0	0	0	0	0	0	0	0	0	0	0
S′′ Amp(mV)	0	0	0	0	0	0	0	0	0	0	0	0
ST Amp(mV)	72	108	36	-90	18	73	128	122	680	-396	330	-60
ST80 Amp(mV)	57	170	113	-113	-27	142	131	133	1278	-2284	582	-98
STT28 Amp(mV)	70	267	209	-174	-69	225	197	251	1928	20	781	-66
STT38 Amp(mV)	174	357	162	-254	6	271	7	-116	840	-1594	432	34
T+ Amp(mV)	437	447	244	0	340	321	197	0	1940	1610	804	156
T- Amp(mV)	0	0	-269	-429	0	0	-768	-1620	-3569	-3954	0	-341
QRS Area	1414	465	-948	-936	1180	-237	-2516	-4463	-11379	2732	-256	1160
P Area	***	***	***	***	***	***	***	***	***	***	***	***
T Area	4384	6407	2097	-5413	1153	4375	219	-5183	10268	-7903	11196	-2874
P Morph	***	***	***	***	***	***	***	***	***	***	***	***
T Morph	1	1	2	-1	1	1	2	-1	2	2	1	-2
R Notch	0	0	0	0	0	0	0	0	0	0	0	0