Rec : 28.08.2031 15:40 Name : **A** 100Years F Ref.Dr.: Consult Dr.:

00cms 00kg PM : n 0:00:10 00/00 mmHg Indian Drug1: No Medication Drug2: No Medication

ID : 0000604 **Hospital : ABCDEFG1234567890HOSPITAL** Diagnosis : Normal

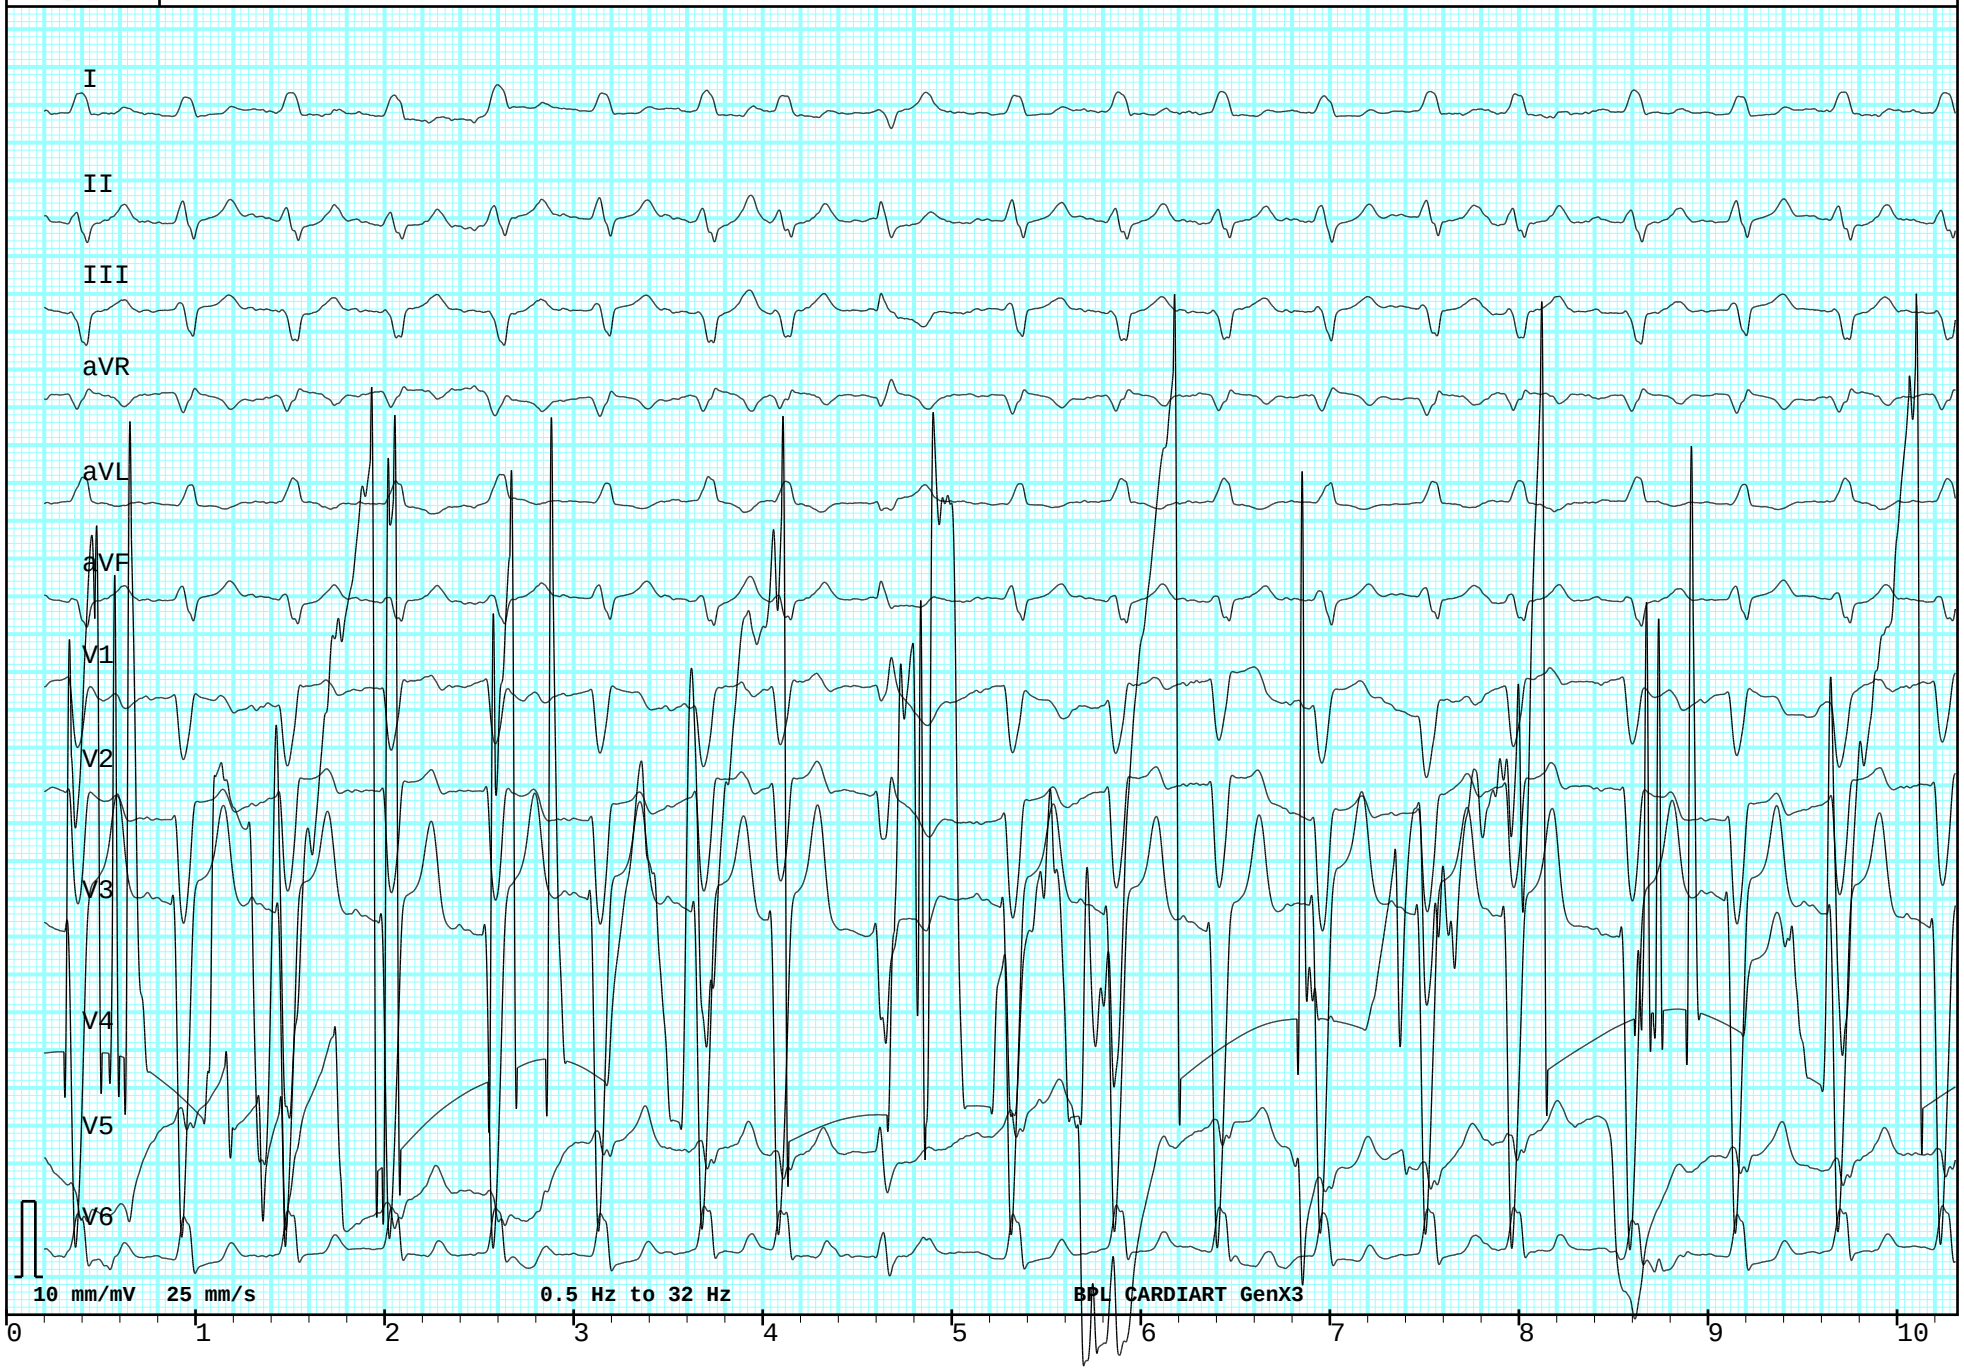

Clinician's Comments :

Rec : 28.08.2031 15:40 Name : **A**
100Years F 00cms 00kg Indian
PM : n 00/00 mmHg **ID : 0000604**

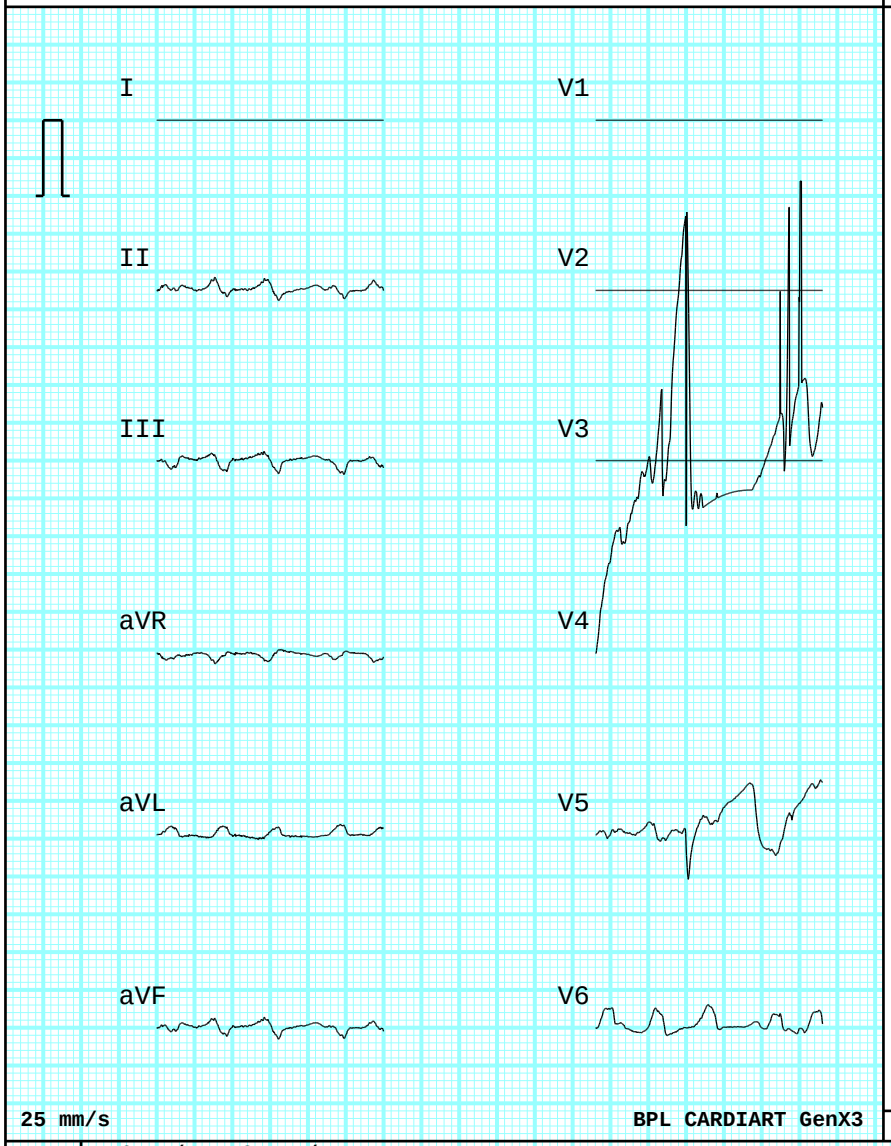

Heart Rate 110 bpm HRV 0

STFrontalAxis	**** deg.	TFrontalAxis	**** deg.
ST Duration	42 ms	PR Interval	66 ms
Q-T Interval	336 ms	QTc Hodges	424 ms
QT Dispersion	50 ms		
P Terminal Force	-32768 ms.uv		

Average beat fiducial point sample number

	Onset	Termination	Duration(ms)
P	262	320	58
QRS	328	488	160
T	530	664	134

Sinus tachycardia
Demand pacing
Lead(s) unsuitable for analysis:
~ I

~ V1

Disclaimer : This report does not replace the diagnosis of trained physician | 2.102.841.5

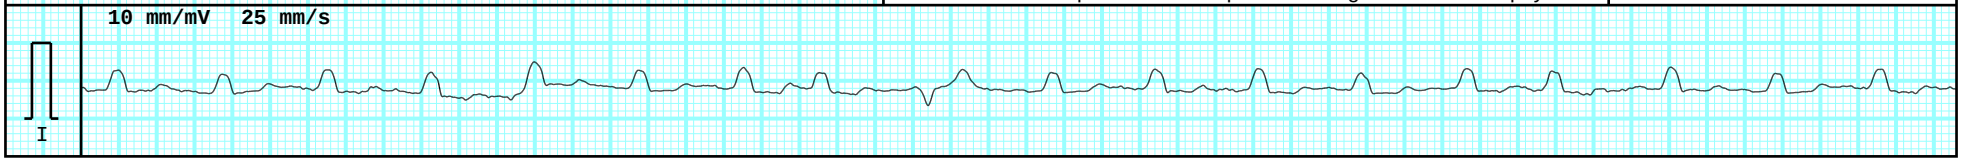

BPL CARDIART GenX3 Measurement Matrix

ID : 0000604 Name : A

Inferior infarct - age undetermined
Possible lateral infarct - age undetermined
Anterior T wave abnormality
~ is nonspecific
Low QRS voltages in limb leads
Abnormal ECG

	I	II	III	aVR	aVL	aVF	V1	V2	V3/V4R	V4	V5	V6
P Ons(ms)	***	262	262	262	262	262	***	***	***	262	262	262
P Dur(ms)	***	56	58	56	58	56	***	***	***	56	58	58
QRS Ons	***	328	330	328	332	328	***	***	***	328	334	336
QRS Dur(ms)	***	160	52	152	42	86	***	***	***	160	154	144
Q Dur(ms)	***	160	52	0	0	70	***	***	***	0	15	144
R Dur(ms)	***	0	0	152	42	15	***	***	***	23	16	0
S Dur(ms)	***	0	0	0	0	0	***	***	***	40	8	0
R′ Dur(ms)	***	0	0	0	0	0	***	***	***	96	103	0
S′ Dur(ms)	***	0	0	0	0	0	***	***	***	0	11	0
R′′ Dur(ms)	***	0	0	0	0	0	***	***	***	0	0	0
S′′ Dur(ms)	***	0	0	0	0	0	***	***	***	0	0	0
ST Dur(ms)	***	60	172	52	164	134	***	***	***	28	16	54
T Ons	***	548	554	532	538	548	***	***	***	530	526	534
T Dur(ms)	***	116	74	88	86	116	***	***	***	132	96	88
P+ Dur(ms)	***	56	58	26	0	56	***	***	***	0	58	0
T+ Dur(ms)	***	58	56	52	0	58	***	***	***	0	96	48
QRS IntD	***	0	0	52	16	72	***	***	***	153	135	0
P+ Amp(mV)	***	133	189	98	0	144	***	***	***	0	283	0
P- Amp(mV)	***	0	0	-59	-151	0	***	***	***	-697	0	-313
P2P Amp(mV)	***	183	119	137	42	179	***	***	***	4695	843	397
Q Amp(mV)	***	-183	-119	0	0	-151	***	***	***	0	-35	-397
R Amp(mV)	***	0	0	137	42	28	***	***	***	848	28	0
S Amp(mV)	***	0	0	0	0	0	***	***	***	-918	-24	0
R′ Amp(mV)	***	0	0	0	0	0	***	***	***	3777	180	0
S′ Amp(mV)	***	0	0	0	0	0	***	***	***	0	-663	0
R′′ Amp(mV)	***	0	0	0	0	0	***	***	***	0	0	0
S′′ Amp(mV)	***	0	0	0	0	0	***	***	***	0	0	0
ST Amp(mV)	***	-38	131	103	-150	46	***	***	***	-1019	-173	-251
ST80 Amp(mV)	***	104	213	1	-160	158	***	***	***	-1096	386	-39
STT28 Amp(mV)	***	17	182	85	-177	92	***	***	***	-1091	184	-202
STT38 Amp(mV)	***	87	185	50	-156	146	***	***	***	-1008	289	-140
T+ Amp(mV)	***	112	213	92	0	159	***	***	***	0	387	110
T- Amp(mV)	***	-241	-82	-25	-177	-192	***	***	***	-1115	0	-208
QRS Area	***	-727	372	908	-737	-180	***	***	***	10527	-34	-2402
P Area	***	263	35	-241	99	154	***	***	***	259	91	527
T Area	***	-289	721	246	-687	138	***	***	***	-7773	1354	-386
P Morph	***	1	1	2	-1	1	***	***	***	-1	1	-1
T Morph	***	2	2	-2	-1	2	***	***	***	-1	1	-2
R Notch	***	0	0	2	0	0	***	***	***	0	0	0