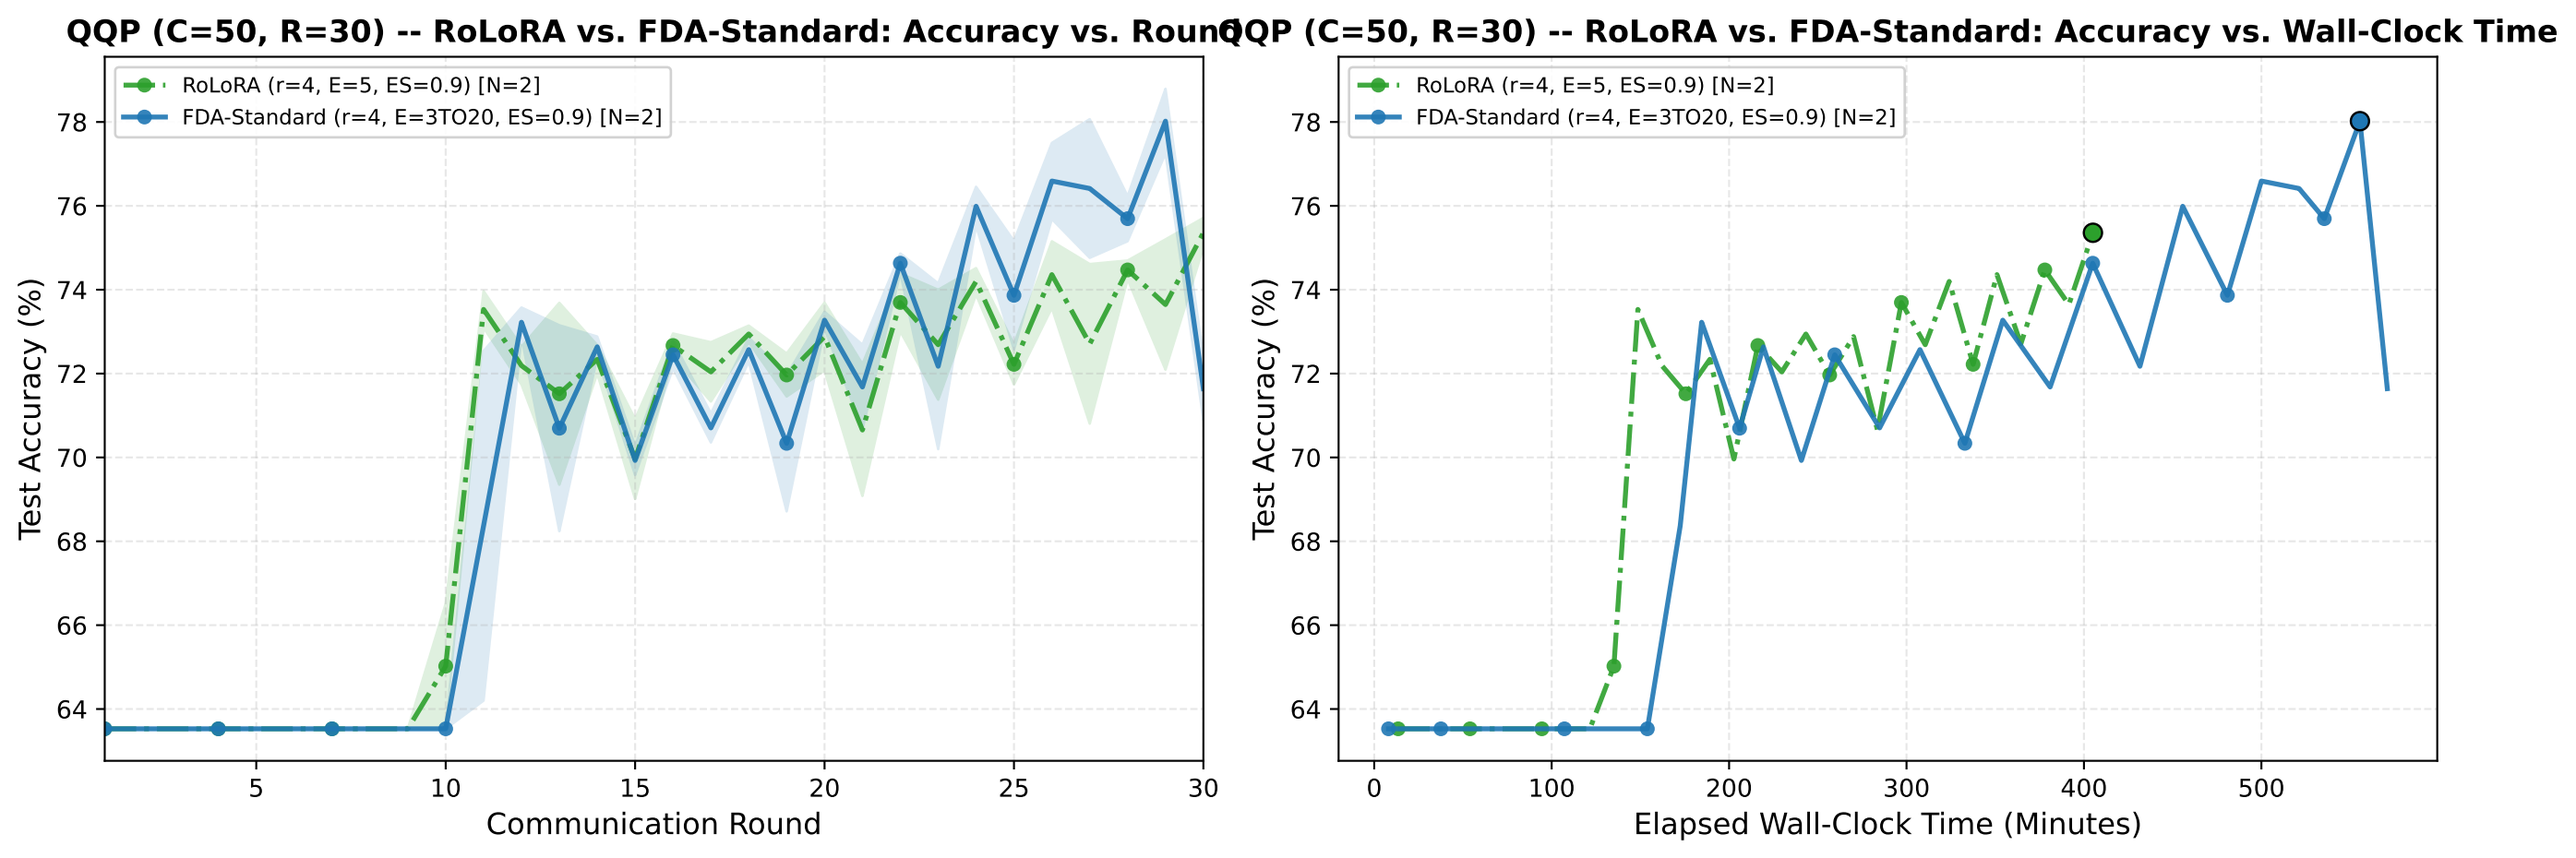
QQP (C=50, R=30) -- RoLoRA vs. FDA-Standard: Accuracy vs. Round
RoLoRA (r=4, E=5, ES=0.9) [N=2]
FDA-Standard (r=4, E=3TO20, ES=0.9) [N=2]
Test Accuracy (%)
Communication Round
QQP (C=50, R=30) -- RoLoRA vs. FDA-Standard: Accuracy vs. Wall-Clock Time
RoLoRA (r=4, E=5, ES=0.9) [N=2]
FDA-Standard (r=4, E=3TO20, ES=0.9) [N=2]
Test Accuracy (%)
Elapsed Wall-Clock Time (Minutes)