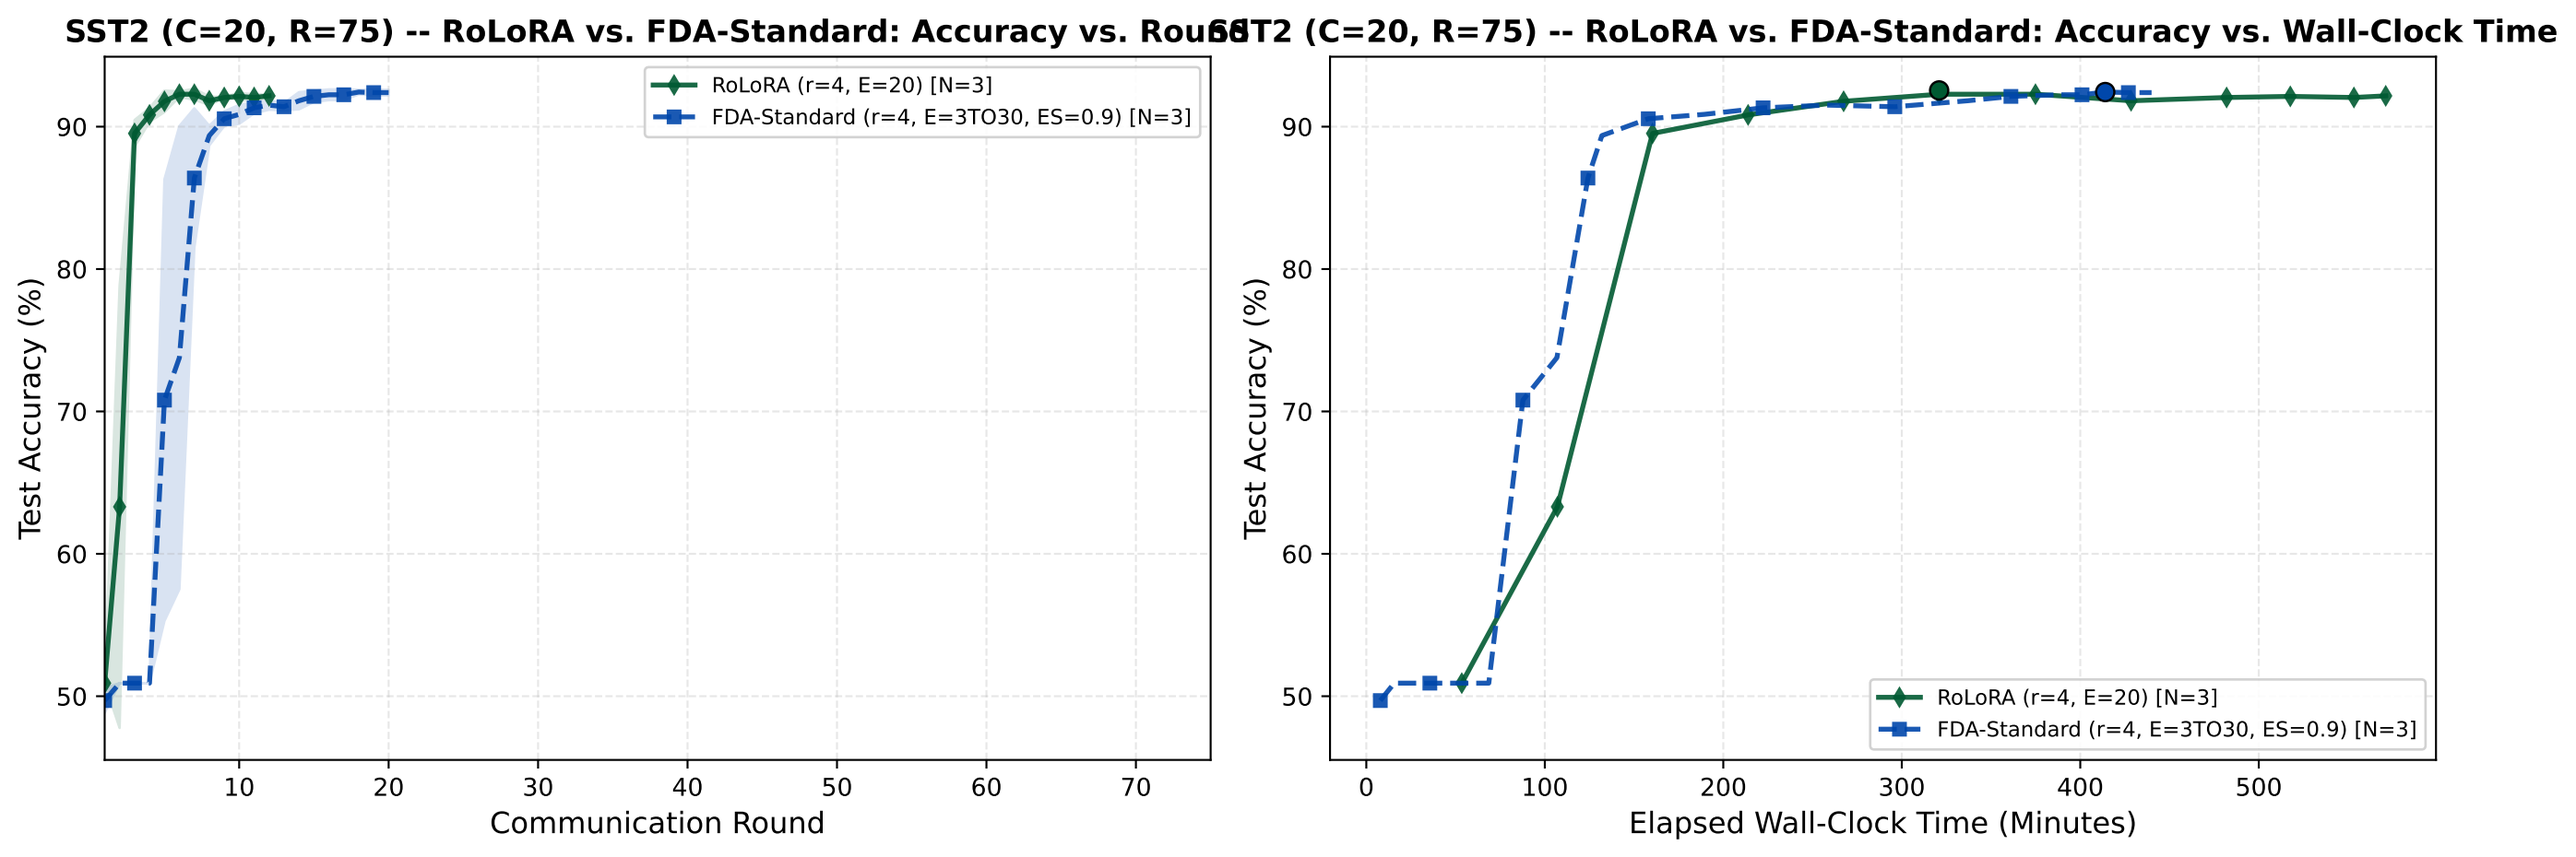
SST2 (C=20, R=75) -- RoLoRA vs. FDA-Standard: Accuracy vs. Round
Test Accuracy (%)
Communication Round
RoLoRA (r=4, E=20) [N=3]
FDA-Standard (r=4, E=3TO30, ES=0.9) [N=3]
SST2 (C=20, R=75) -- RoLoRA vs. FDA-Standard: Accuracy vs. Wall-Clock Time
Test Accuracy (%)
Elapsed Wall-Clock Time (Minutes)
RoLoRA (r=4, E=20) [N=3]
FDA-Standard (r=4, E=3TO30, ES=0.9) [N=3]