Cross-Benchmark Peak Test Accuracy: Calibrated FDA vs. Baselines (Rank $r = 4$)

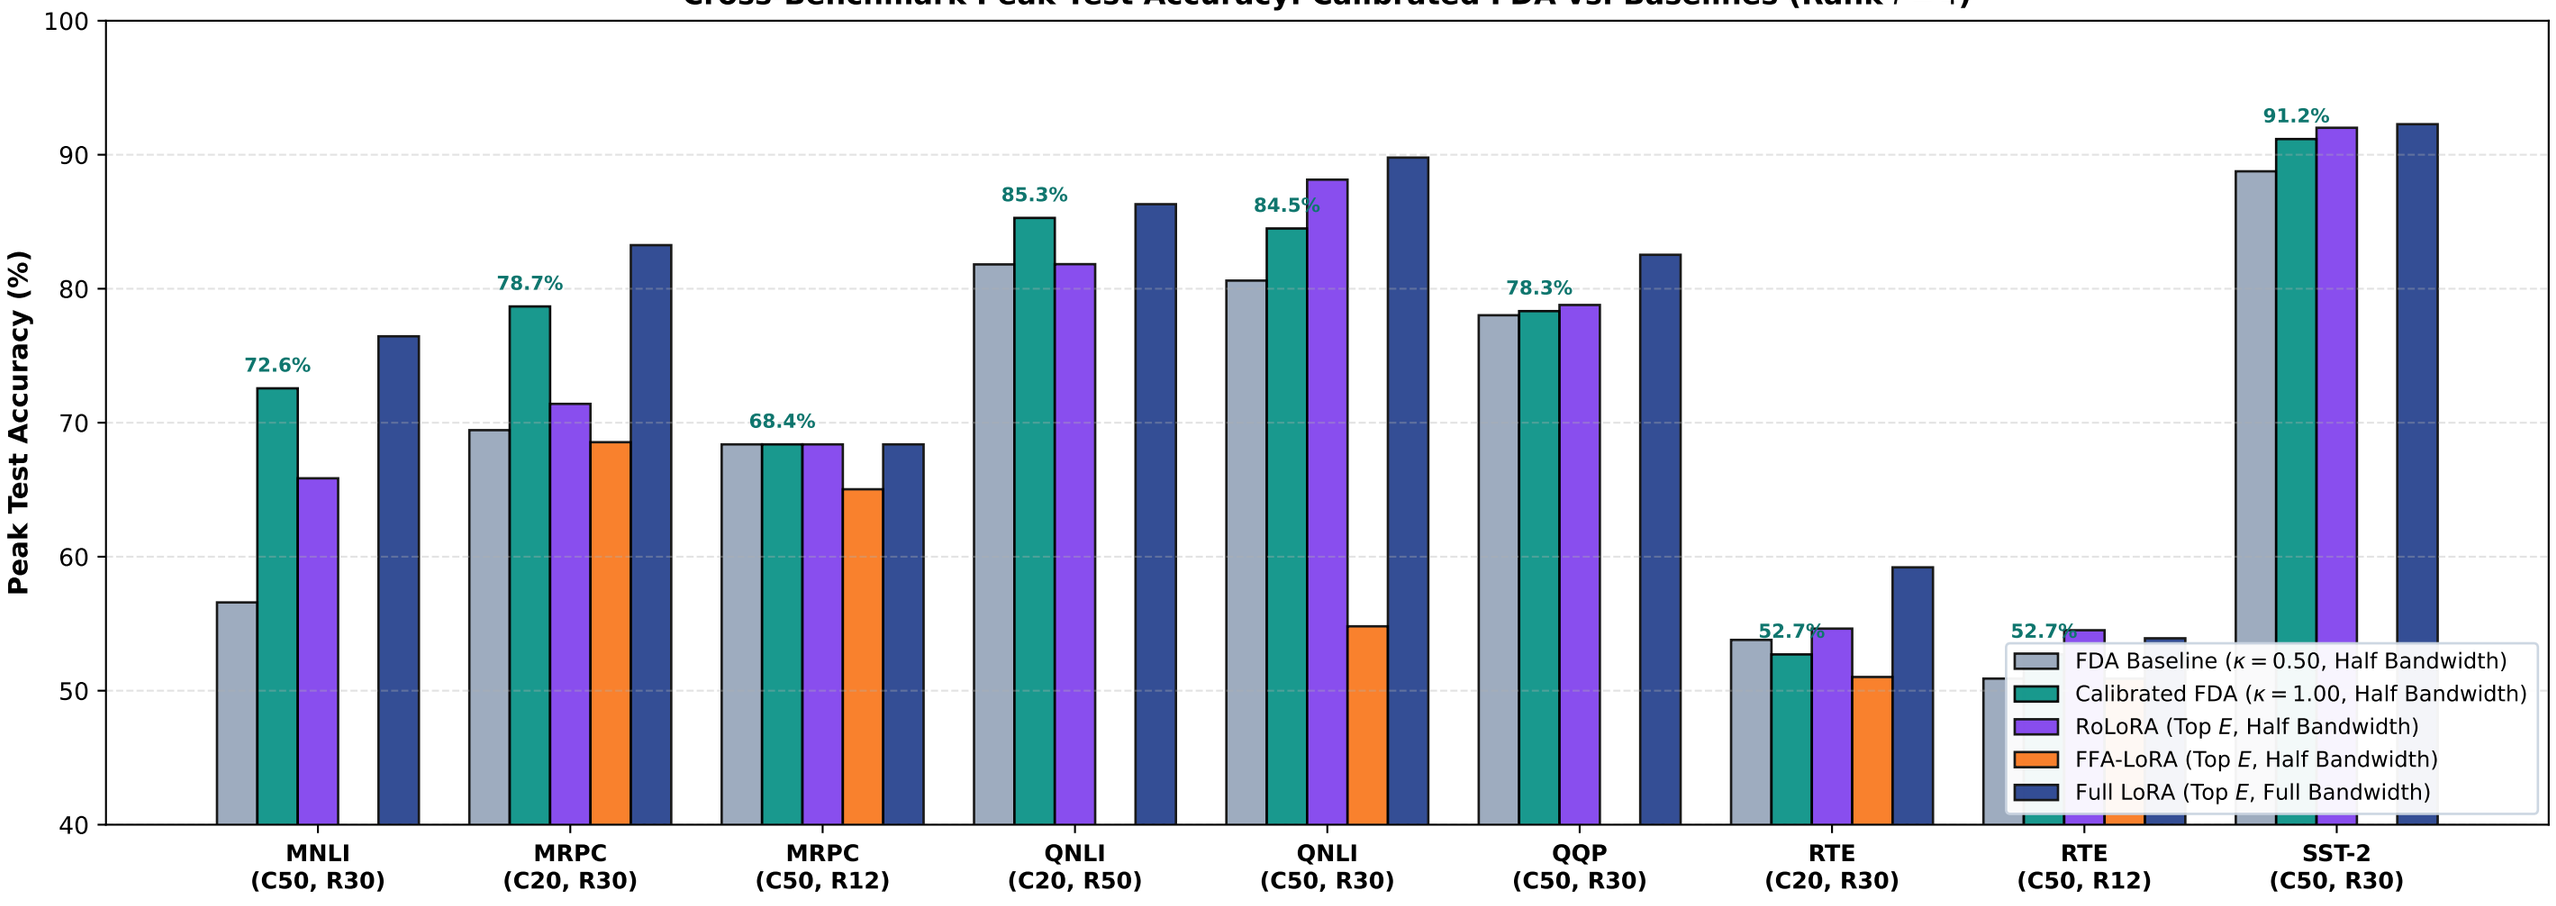
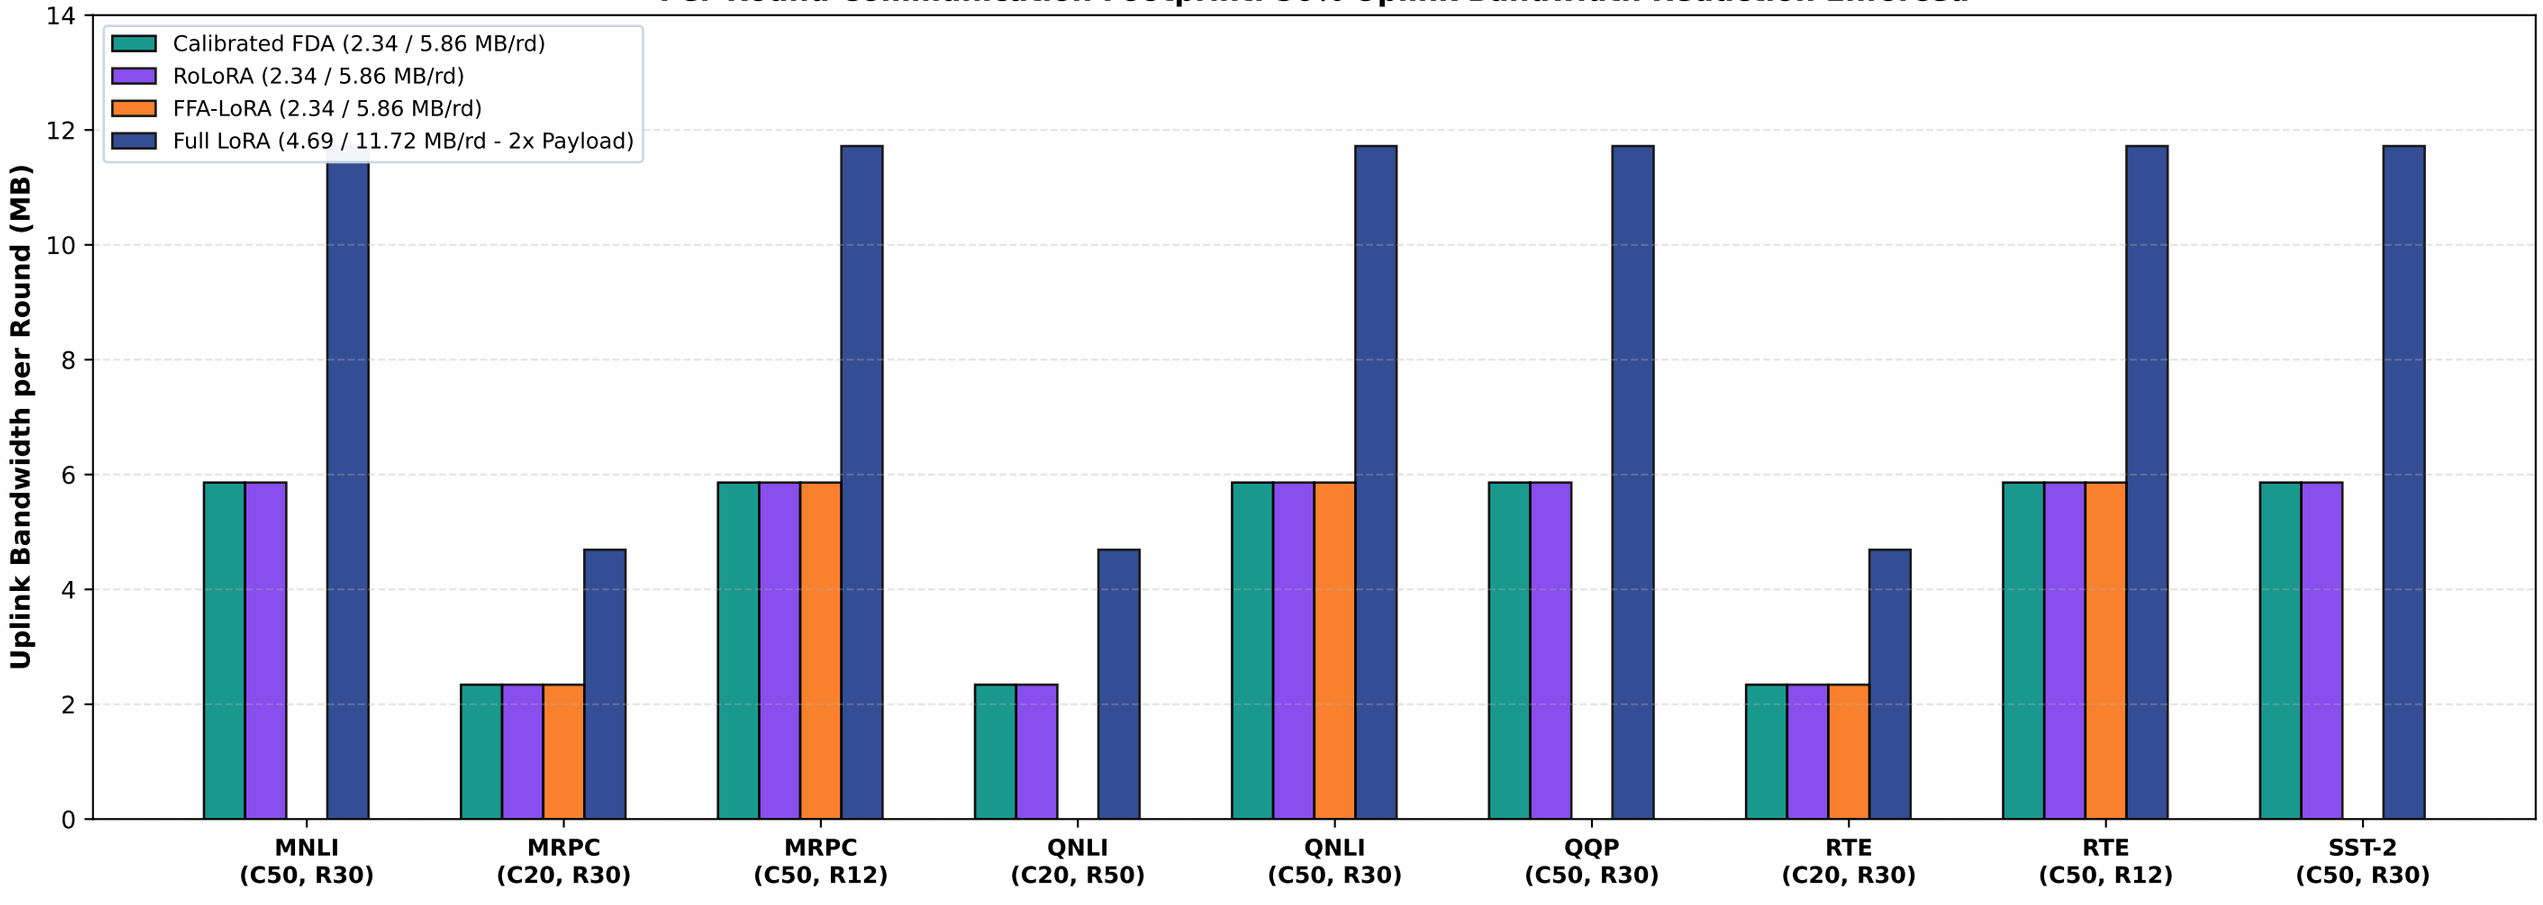
Per-Round Communication Footprint: 50% Uplink Bandwidth Reduction Enforced