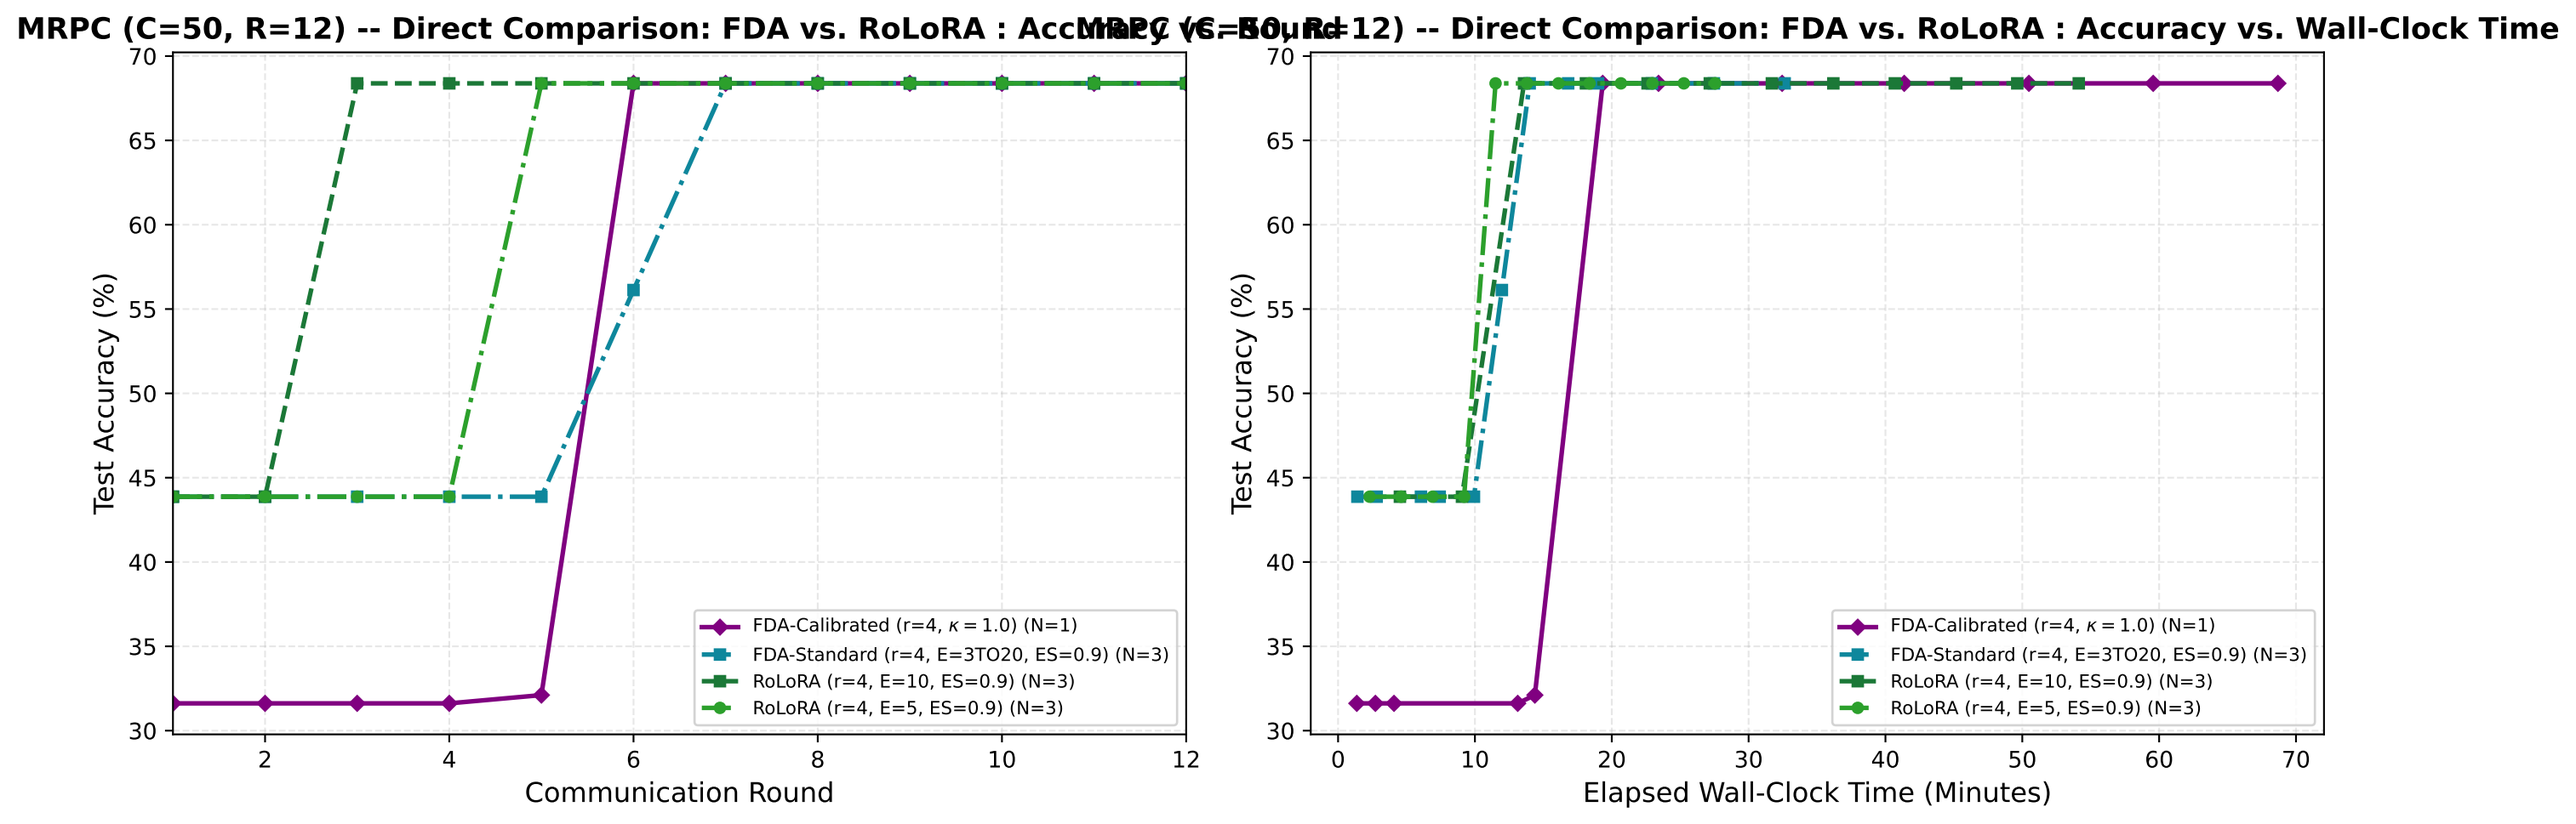
MRPC (C=50, R=12) -- Direct Comparison: FDA vs. RoLoRA : Accuracy vs. Communication Round
Test Accuracy (%)
Communication Round
FDA-Calibrated (r=4, κ = 1.0) (N=1)
FDA-Standard (r=4, E=3TO20, ES=0.9) (N=3)
RoLoRA (r=4, E=10, ES=0.9) (N=3)
RoLoRA (r=4, E=5, ES=0.9) (N=3)
MRPC (C=50, R=12) -- Direct Comparison: FDA vs. RoLoRA : Accuracy vs. Wall-Clock Time
Test Accuracy (%)
Elapsed Wall-Clock Time (Minutes)
FDA-Calibrated (r=4, κ = 1.0) (N=1)
FDA-Standard (r=4, E=3TO20, ES=0.9) (N=3)
RoLoRA (r=4, E=10, ES=0.9) (N=3)
RoLoRA (r=4, E=5, ES=0.9) (N=3)