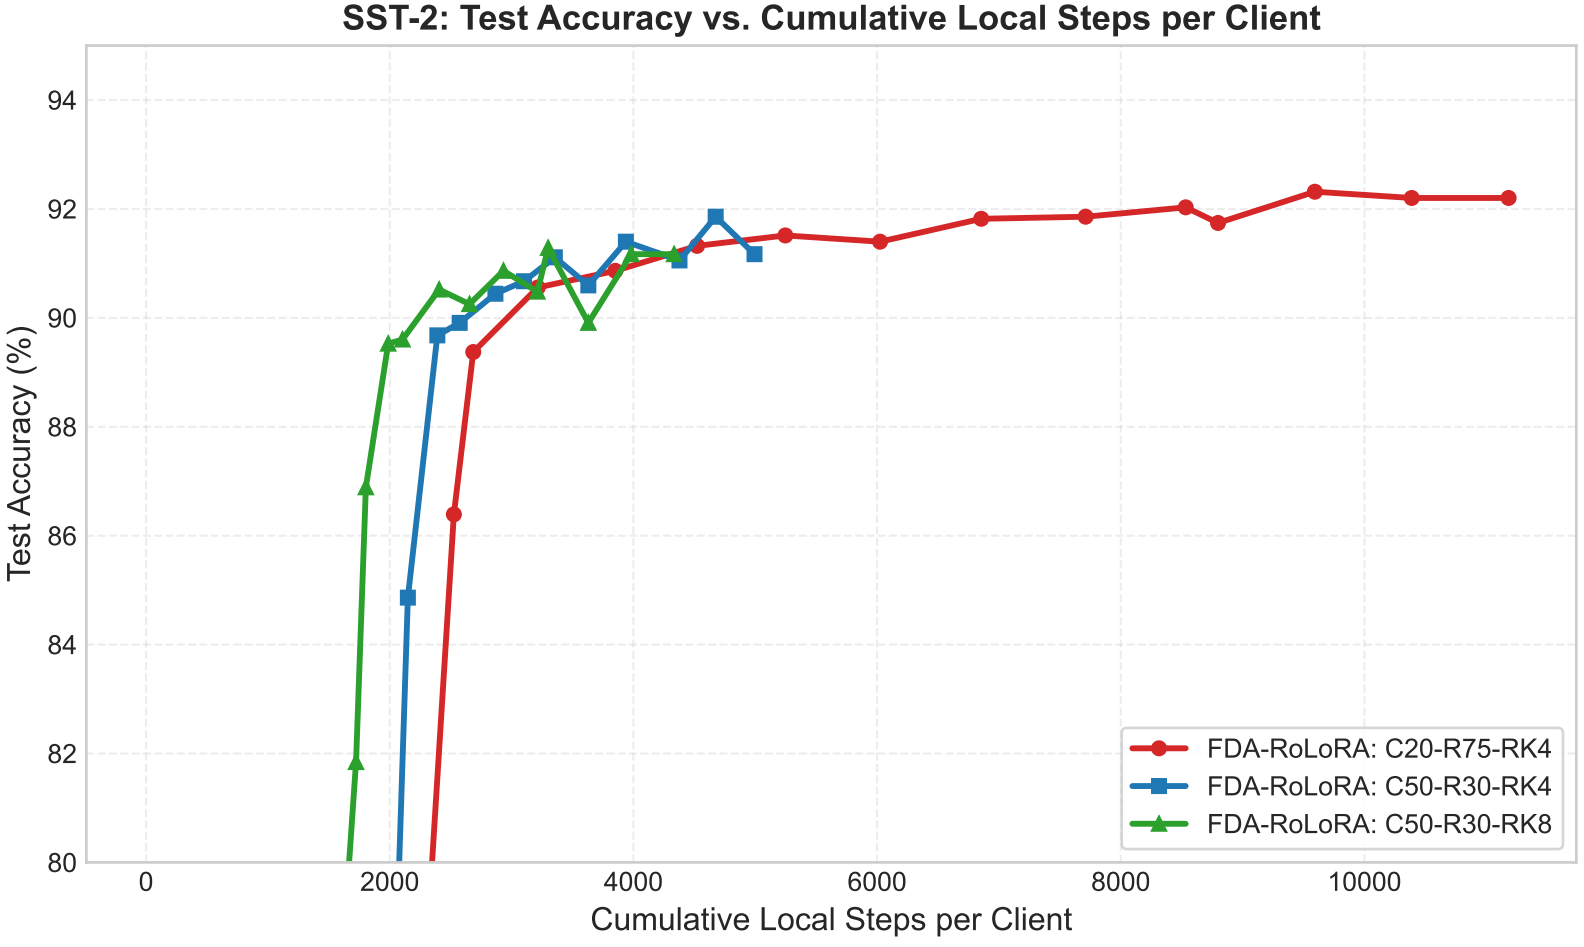
SST-2: Test Accuracy vs. Cumulative Local Steps per Client
Test Accuracy (%)
94
92
90
88
86
84
82
80
0
2000
4000
6000
8000
10000
Cumulative Local Steps per Client
FDA-RoLoRA: C20-R75-RK4
FDA-RoLoRA: C50-R30-RK4
FDA-RoLoRA: C50-R30-RK8