eSole 3D Plantar Scanner Data Report

No.	**20251104001**	Date	2025-11-04	Time	23:26:05	Store	tuerqi020001	Address
Name	**qq**	Gender	Male	Age	424	Tel	121	

Hallux analysis:

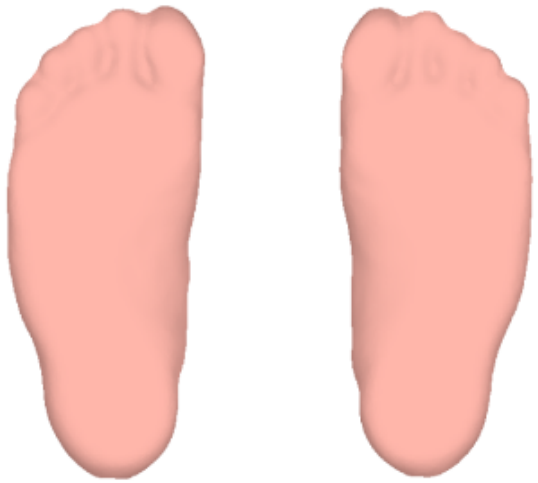

Left foot		Right foot
2.4	Hallux angle(°)	1.1
Normal Hallgux	Type	Normal Hallgux

Evaluation criteria: Normal: 0 °~10 °Mild: 10°~20 °Moderate:20°~30 °
Severity: > 30 °

Heel Analysis:

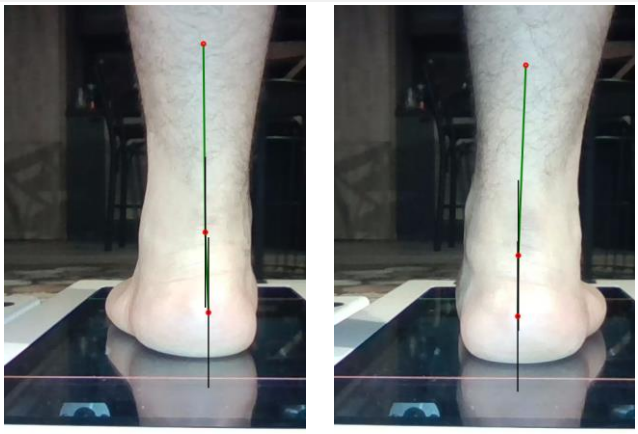

Left foot		Right foot
2.2	Heel angle(°)	0.6
Normal Heel	Heel type	Normal Heel
0.6	Knee angle(°)	2.3
Normal Heel	Knee type	Normal Heel

Normal: 0 °~4 ° Mild: 4 ° ~ 8 ° Moderate: 8 °~15 °Severity: >15 °

Schematic diagram of heel inversion:

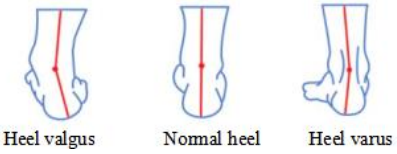

Arch analysis:

Left foot		Right foot
Severe Flat	Arch Type	Severe Flat
0.326	Arch Index	0.306

low Left foot high

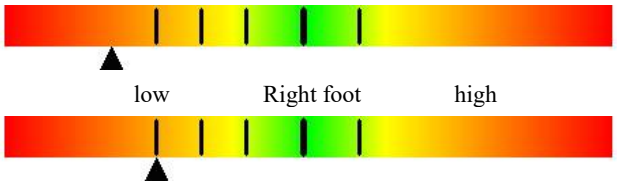

low Right foot high

High arch foot: < 0.21Normal arch: 0.21 ~ 0.26Mild flatfoot: 0.26 ~ 0.28
Moderate flatfoot: 0.28 ~ 0.3

Arch height:

Left foot		Right foot
13.5	Arch height（mm)	12.4
0.462	Arch width Index	0.341

Schematic diagram of arch width coefficient:

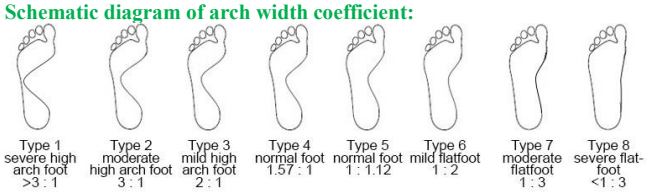

Parameter dimension measurement

Length measurement

Item description	Left foot（mm）	Right foot（mm）
Foot length	250.8	248.8
Sole length	242.0	239.9
Arch length	102.8	102.1
First meta length	181.8	163.5
Fifth meta length	159.3	158.0
Hallux bumps length	224.4	222.6
Foot flank length	102.8	102.0
Heel center length	39.0	39.0
Heel margin length	8.8	8.9

Width measurement

Item description	Left foot（mm）	Right foot（mm）
Foot width	102.4	101.8
Slant width	104.9	102.0
Toe width	100.4	99.0
Arch outside width	30.4	32.7
Foot flank width	9.7	5.3
Heel center width	66.1	68.6
Total heel width	41.4	40.9

Height measurement

Item description	Left foot（mm）	Right foot（mm）
Arch height	13.5	12.4
First meta joint height	4.2	3.8
Heel protrusion height	18.6	14.4

Angle measurement

Item description	Left foot(°)	Right foot(°)
Hallux angle	-2.4	1.1
Pronator angle	2.2	-0.6
Knee angle	0.6	-2.3

Shoe size/Insole recommendation

Item description	Left foot	Right foot
Shoe size	40(WE)	40(WE)
Insole recommendation	40(WE)	40(WE)

Service demand

Item description		
Customized insole service	☐Yes	☐No

Recommendation：

Contact address Low arch and heel valgus usually indicate excessive pronation (foot rolling inward in the gait cycle). Excessive varus may cause foot, ankle and knee injuries, and further affect the balance of pelvis, spine and shoulder. Stability shoes and motion control shoes have solid inner support, which is most suitable for over-pronated foot type;High arch and heel inversion, neutral shock absorption shoes are the most suitable. Normal arch and heel are most suitable for stabilizing shoes.For any type of arch or heel deformity, proper design and manufacture of foot correction insole can promote the normal biomechanical function of lower limbs, better adjust your whole body, improve your posture, and prevent injury or damage to your body。