

External Calibration Certificate


Applicant's Data : Laboratorium Telkom Test House (TTH)
Jl. Gegerkalong Hilir No. 47 Bandung 40152.

Equipment Data

Equipment name : OPTICAL POWER METER
Brand : EXFO
Type/Model : 1750
Serial number : 1636843
Asset Number : 215/CAL

Calibration Information

Delivery Date : May 28, 2025
Calibration By : Lab Kalibrasi Telkom Jakarta (LK-016-IDN)
Certificate Number : JCL/25/0346/HS, JCL/25/0347/HS, JCL/25/0348/HS, JCL/25/0349/HS
Calibration Date : May 28, 2025
Calibration Due : May 28, 2026

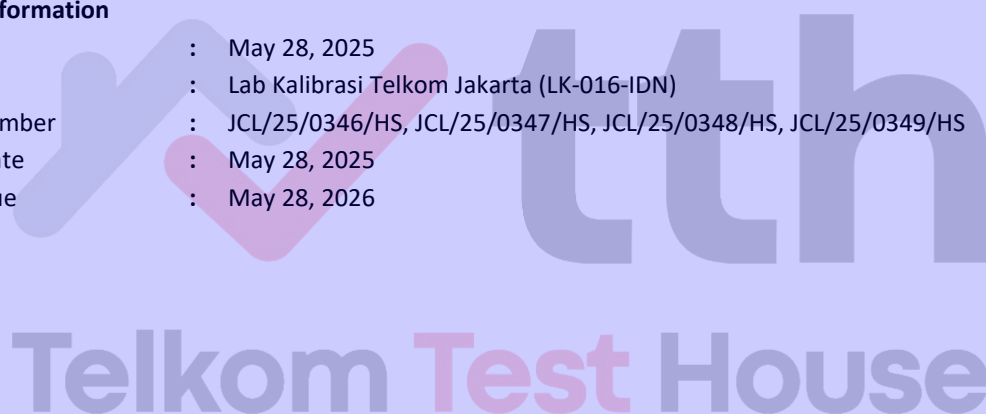

Agreed by:

Bandung, 18 Juli 2025

Reviewed by:


I GEDE ASTAWA

SM Infrastructure Service Research & Assurance

AHMAD ARIF RAHMAN

Mgr. Standardization & Suitability Assurance



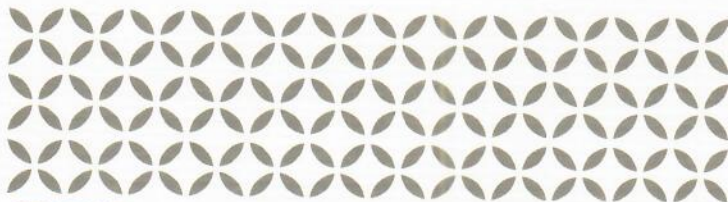

No. Dokumen : Form TCL-QP-19-01

No. / Tgl. Terbit : 01 / 20 Juli 2017

No. / Tgl. Revisi : 02 / 04 Januari 2021



CERTIFICATE OF CALIBRATION

PT TELKOM INDONESIA Tbk
KAN ACCREDITED CALIBRATION LABORATORY (LK-016-IDN)

Jakarta : Jl. Percetakan Negara No.17-19 Jakarta Pusat 10570 Phone 021-21480341
Medan : Jl. Gaharu No. 1 Medan 20235 Phone 061-4531311
Surabaya : Jl. Gayungan PTT No. 17-19 Surabaya 60235 Phone 031-8283678
Makassar : Jl. AP Pettarani No. 4 Makassar 90221 Phone 0411-861153

CS Support
☎ 081-16-4-17025

Certificate Number
JCL/25/0346/HS

Approved Signatory

M. Ilyas

Date of Issue : 02-Jun-2025
Submitted by : PT. TELKOM INDONESIA, Tbk.
Laboratorium Telkom Test House (TTH)
Attention : Mgr. Standardization & Suitability Assurance
Description : OPTICAL POWER METER
Manufacturer/Model : EXFO / FTBx-1750-031-4
Serial Number : 1636843- CH1 (215/CAL)
Environment : 22.4 °C ± 0.8 °C 57 % ± 1.2 % RH
Calibration Location : Onsite
Date Calibrated : 28-May-2025
Date Received : 27-May-2025

PT. Telkom Indonesia, Tbk. - Telkom Certifies that this instrument has been calibrated under the environmental condition stated above using telkom standard (s) which is (are) traceable to the international system of Units (SI) through SCL Hong Kong.

Method of Calibration :

The calibration was carried out based on the established Standard Telkom Calibration Procedure, TCL-WI-O011 and by comparison against the following standard(s) and instrument(s) which is (are) calibrated on schedule to maintain traceability and required accuracy :

Description	S/N	Cal Date	Due Date
1. Optical Fiber Power Meter	1030788-CH1	11-Apr-2025	10-Apr-2028
2. Variable Optical Broadband Source	1082690	23-May-2025	22-May-2026
3. Optical Varibel Attenuator	1025153	11-Apr-2025	10-Apr-2028

CERTIFICATE OF CALIBRATION

Checked By : *H*

Certificate Number : JCL/25/0346/HS

1. ABSOLUTE POWER CALIBRATION (1310.0 nm)

No.	APPLIED VALUE	UUT INDICATED VALUE	CORRECTION	UNCERTAINTY
1.	0.588 dBm	0.296 dBm	0.292 dB	± 0.25 dB

2. LINEARITY TEST (1310.0 nm)

No.	APPLIED VALUE	UUT INDICATED VALUE	CORRECTION	UNCERTAINTY
1	-1.279 dBm	-1.579 dBm	0.300 dB	± 0.25 dB
2	-4.243 dBm	-4.535 dBm	0.292 dB	± 0.25 dB
3	-7.263 dBm	-7.557 dBm	0.294 dB	± 0.25 dB
4	-10.255 dBm	-10.553 dBm	0.298 dB	± 0.25 dB
5	-13.265 dBm	-13.561 dBm	0.296 dB	± 0.25 dB
6	-16.254 dBm	-16.549 dBm	0.295 dB	± 0.25 dB
7	-19.259 dBm	-19.551 dBm	0.292 dB	± 0.25 dB
8	-22.253 dBm	-22.554 dBm	0.301 dB	± 0.25 dB
9	-25.262 dBm	-25.553 dBm	0.291 dB	± 0.25 dB
10	-28.261 dBm	-28.549 dBm	0.288 dB	± 0.25 dB
11	-31.230 dBm	-31.530 dBm	0.300 dB	± 0.25 dB
12	-34.228 dBm	-34.528 dBm	0.300 dB	± 0.25 dB
13	-37.217 dBm	-37.520 dBm	0.303 dB	± 0.25 dB
14	-40.237 dBm	-40.505 dBm	0.268 dB	± 0.25 dB
15	-43.208 dBm	-43.499 dBm	0.291 dB	± 0.25 dB
16	-46.186 dBm	-46.496 dBm	0.310 dB	± 0.25 dB
17	-49.119 dBm	-49.484 dBm	0.365 dB	± 0.25 dB
18	-52.120 dBm	-52.493 dBm	0.373 dB	± 0.25 dB

CERTIFICATE OF CALIBRATION

Checked By : 


Certificate Number : JCL/25/0346/HS

3. ABSOLUTE POWER CALIBRATION (1550.0 nm)

No.	APPLIED VALUE	UUT INDICATED VALUE	CORRECTION	UNCERTAINTY
1.	0.341 dBm	0.151 dBm	0.190 dB	± 0.25 dB

4. LINEARITY TEST (1550.0 nm)

No.	APPLIED VALUE	UUT INDICATED VALUE	CORRECTION	UNCERTAINTY
1	-1.387 dBm	-1.577 dBm	0.190 dB	± 0.25 dB
2	-4.348 dBm	-4.501 dBm	0.153 dB	± 0.25 dB
3	-7.366 dBm	-7.518 dBm	0.152 dB	± 0.25 dB
4	-10.366 dBm	-10.516 dBm	0.150 dB	± 0.25 dB
5	-13.374 dBm	-13.522 dBm	0.148 dB	± 0.25 dB
6	-16.368 dBm	-16.514 dBm	0.146 dB	± 0.25 dB
7	-19.366 dBm	-19.515 dBm	0.149 dB	± 0.25 dB
8	-22.381 dBm	-22.520 dBm	0.139 dB	± 0.25 dB
9	-25.380 dBm	-25.517 dBm	0.137 dB	± 0.25 dB
10	-28.384 dBm	-28.523 dBm	0.139 dB	± 0.25 dB
11	-31.366 dBm	-31.511 dBm	0.145 dB	± 0.25 dB
12	-34.357 dBm	-34.505 dBm	0.148 dB	± 0.25 dB
13	-37.358 dBm	-37.503 dBm	0.145 dB	± 0.25 dB
14	-40.354 dBm	-40.498 dBm	0.144 dB	± 0.25 dB
15	-43.363 dBm	-43.503 dBm	0.140 dB	± 0.25 dB
16	-46.365 dBm	-46.505 dBm	0.140 dB	± 0.25 dB
17	-49.366 dBm	-49.504 dBm	0.138 dB	± 0.25 dB
18	-52.383 dBm	-52.525 dBm	0.142 dB	± 0.25 dB

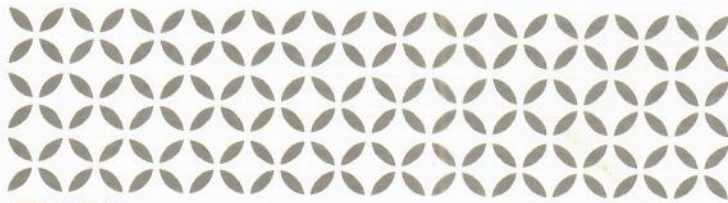

No. Dokumen : Form TCL-QP-19-01

No. / Tgl. Terbit : 01 / 20 Juli 2017

No. / Tgl. Revisi : 02 / 04 Januari 2021



CERTIFICATE OF CALIBRATION

PT TELKOM INDONESIA Tbk
KAN ACCREDITED CALIBRATION LABORATORY (LK-016-IDN)

Certificate Number
JCL/25/0347/HS

Approved Signatory

Jakarta : Jl. Percetakan Negara No.17-19 Jakarta Pusat 10570 Phone 021-21480341
Medan : Jl. Gaharu No. 1 Medan 20235 Phone 061-4531311
Surabaya : Jl. Gayungan PTT No. 17-19 Surabaya 60235 Phone 031-8283678
Makassar : Jl. AP Pettarani No. 4 Makassar 90221 Phone 0411-861153

CS Support
☎ 081-16-4-17025


M. Ilyas

Date of Issue : 02-Jun-2025
Submitted by : PT. TELKOM INDONESIA, Tbk.
Laboraturium Telkom Test House (TTH)
Attention : Mgr. Standardization & Suitability Assurance
Description : OPTICAL POWER METER
Manufacturer/Model : EXFO / FTBx-1750-031-4
Serial Number : 1636843- CH2 (215/CAL)
Environment : 22.4 °C ± 0.8 °C 57 % ± 1.2 % RH
Calibration Location : Onsite
Date Calibrated : 28-May-2025
Date Received : 27-May-2025

PT. Telkom Indonesia, Tbk. - Telkom Certifies that this instrument has been calibrated under the environmental condition stated above using telkom standard (s) which is (are) traceable to the international system of Units (SI) through SCL Hong Kong.

Method of Calibration :

The calibration was carried out based on the established Standard Telkom Calibration Procedure, TCL-WI-0011 and by comparison against the following standard(s) and instrument(s) which is (are) calibrated on schedule to maintain traceability and required accuracy :

Description	S/N	Cal Date	Due Date
1. Optical Fiber Power Meter	1030788-CH1	11-Apr-2025	10-Apr-2028
2. Variable Optical Broadband Source	1082690	23-May-2025	22-May-2026
3. Optical Varibel Attenuator	1025153	11-Apr-2025	10-Apr-2028

CERTIFICATE OF CALIBRATION

Checked By : *11*

Certificate Number : JCL/25/0347/HS

1. ABSOLUTE POWER CALIBRATION (1310.0 nm)

No.	APPLIED VALUE	UUT INDICATED VALUE	CORRECTION	UNCERTAINTY
1.	0.588 dBm	0.274 dBm	0.314 dB	± 0.25 dB

2. LINEARITY TEST (1310.0 nm)

No.	APPLIED VALUE	UUT INDICATED VALUE	CORRECTION	UNCERTAINTY
1	-1.279 dBm	-1.610 dBm	0.331 dB	± 0.25 dB
2	-4.243 dBm	-4.581 dBm	0.338 dB	± 0.25 dB
3	-7.263 dBm	-7.608 dBm	0.345 dB	± 0.25 dB
4	-10.255 dBm	-10.609 dBm	0.354 dB	± 0.25 dB
5	-13.265 dBm	-13.616 dBm	0.351 dB	± 0.25 dB
6	-16.254 dBm	-16.609 dBm	0.355 dB	± 0.25 dB
7	-19.259 dBm	-19.612 dBm	0.353 dB	± 0.25 dB
8	-22.253 dBm	-22.616 dBm	0.363 dB	± 0.25 dB
9	-25.262 dBm	-25.614 dBm	0.352 dB	± 0.25 dB
10	-28.261 dBm	-28.611 dBm	0.350 dB	± 0.25 dB
11	-31.230 dBm	-31.594 dBm	0.364 dB	± 0.25 dB
12	-34.228 dBm	-34.590 dBm	0.362 dB	± 0.25 dB
13	-37.217 dBm	-37.583 dBm	0.366 dB	± 0.25 dB
14	-40.237 dBm	-40.563 dBm	0.326 dB	± 0.25 dB
15	-43.208 dBm	-43.560 dBm	0.352 dB	± 0.25 dB
16	-46.186 dBm	-46.556 dBm	0.370 dB	± 0.25 dB
17	-49.119 dBm	-49.547 dBm	0.428 dB	± 0.25 dB
18	-52.120 dBm	-52.555 dBm	0.435 dB	± 0.25 dB

CERTIFICATE OF CALIBRATION

Checked By : *HK*

Certificate Number : JCL/25/0347/HS

3. ABSOLUTE POWER CALIBRATION (1550.0 nm)

No.	APPLIED VALUE	UUT INDICATED VALUE	CORRECTION	UNCERTAINTY
1.	0.341 dBm	0.115 dBm	0.226 dB	± 0.25 dB

4. LINEARITY TEST (1550.0 nm)

No.	APPLIED VALUE	UUT INDICATED VALUE	CORRECTION	UNCERTAINTY
1	-1.387 dBm	-1.604 dBm	0.217 dB	± 0.25 dB
2	-4.348 dBm	-4.565 dBm	0.217 dB	± 0.25 dB
3	-7.366 dBm	-7.582 dBm	0.216 dB	± 0.25 dB
4	-10.366 dBm	-10.581 dBm	0.215 dB	± 0.25 dB
5	-13.374 dBm	-13.586 dBm	0.212 dB	± 0.25 dB
6	-16.368 dBm	-16.580 dBm	0.212 dB	± 0.25 dB
7	-19.366 dBm	-19.584 dBm	0.218 dB	± 0.25 dB
8	-22.381 dBm	-22.590 dBm	0.209 dB	± 0.25 dB
9	-25.380 dBm	-25.589 dBm	0.209 dB	± 0.25 dB
10	-28.384 dBm	-28.593 dBm	0.209 dB	± 0.25 dB
11	-31.366 dBm	-31.585 dBm	0.219 dB	± 0.25 dB
12	-34.357 dBm	-34.577 dBm	0.220 dB	± 0.25 dB
13	-37.358 dBm	-37.579 dBm	0.221 dB	± 0.25 dB
14	-40.354 dBm	-40.578 dBm	0.224 dB	± 0.25 dB
15	-43.363 dBm	-43.582 dBm	0.219 dB	± 0.25 dB
16	-46.365 dBm	-46.585 dBm	0.220 dB	± 0.25 dB
17	-49.366 dBm	-49.586 dBm	0.220 dB	± 0.25 dB
18	-52.383 dBm	-52.605 dBm	0.222 dB	± 0.25 dB

No. Dokumen : Form TCL-QP-19-01

No. / Tgl. Terbit : 01 / 20 Juli 2017

No. / Tgl. Revisi : 02 / 04 Januari 2021

CERTIFICATE OF CALIBRATION

P T TELKOM INDONESIA Tbk
KAN ACCREDITED CALIBRATION LABORATORY (LK-016-IDN)

Jakarta : Jl. Percetakan Negara No.17-19 Jakarta Pusat 10570 Phone 021-21480341
Medan : Jl. Gaharu No. 1 Medan 20235 Phone 061-4531311
Surabaya : Jl. Gayungan PTT No. 17-19 Surabaya 60235 Phone 031-8283678
Makassar : Jl. AP Pettarani No. 4 Makassar 90221 Phone 0411-861153

CS Support
☎ 081-16-4-17025

Certificate Number
JCL/25/0348/HS

Approved Signatory


M. Ilyas

Date of Issue : 02-Jun-2025
Submitted by : PT. TELKOM INDONESIA, Tbk.
Laboratorium Telkom Test House (TTH)
Attention : Mgr. Standardization & Suitability Assurance
Description : OPTICAL POWER METER
Manufacturer/Model : EXFO / FTBx-1750-031-4
Serial Number : 1636843- CH3 (215/CAL)
Environment : 22.4 °C ± 0.8 °C 57 % ± 1.2 % RH
Calibration Location : Onsite
Date Calibrated : 28-May-2025
Date Received : 27-May-2025

PT. Telkom Indonesia, Tbk. - Telkom Certifies that this instrument has been calibrated under the environmental condition stated above using telkom standard (s) which is (are) traceable to the international system of Units (SI) through SCL Hong Kong.

Method of Calibration :

The calibration was carried out based on the established Standard Telkom Calibration Procedure, TCL-WI-O011 and by comparison against the following standard(s) and instrument(s) which is (are) calibrated on schedule to maintain traceability and required accuracy :

Description	S/N	Cal Date	Due Date
1. Optical Fiber Power Meter	1030788-CH1	11-Apr-2025	10-Apr-2028
2. Variable Optical Broadband Source	1082690	23-May-2025	22-May-2026
3. Optical Varibel Attenuator	1025153	11-Apr-2025	10-Apr-2028

CERTIFICATE OF CALIBRATION

Checked By : *11*

Certificate Number : JCL/25/0348/HS

1. ABSOLUTE POWER CALIBRATION (1310.0 nm)

No.	APPLIED VALUE	UUT INDICATED VALUE	CORRECTION	UNCERTAINTY
1.	0.588 dBm	0.270 dBm	0.318 dB	± 0.25 dB

2. LINEARITY TEST (1310.0 nm)

No.	APPLIED VALUE	UUT INDICATED VALUE	CORRECTION	UNCERTAINTY
1	-1.279 dBm	-1.581 dBm	0.302 dB	± 0.25 dB
2	-4.243 dBm	-4.554 dBm	0.311 dB	± 0.25 dB
3	-7.263 dBm	-7.581 dBm	0.318 dB	± 0.25 dB
4	-10.255 dBm	-10.581 dBm	0.326 dB	± 0.25 dB
5	-13.265 dBm	-13.589 dBm	0.324 dB	± 0.25 dB
6	-16.254 dBm	-16.581 dBm	0.327 dB	± 0.25 dB
7	-19.259 dBm	-19.584 dBm	0.325 dB	± 0.25 dB
8	-22.253 dBm	-22.588 dBm	0.335 dB	± 0.25 dB
9	-25.262 dBm	-25.586 dBm	0.324 dB	± 0.25 dB
10	-28.261 dBm	-28.582 dBm	0.321 dB	± 0.25 dB
11	-31.230 dBm	-31.565 dBm	0.335 dB	± 0.25 dB
12	-34.228 dBm	-34.562 dBm	0.334 dB	± 0.25 dB
13	-37.217 dBm	-37.555 dBm	0.338 dB	± 0.25 dB
14	-40.237 dBm	-40.538 dBm	0.301 dB	± 0.25 dB
15	-43.208 dBm	-43.533 dBm	0.325 dB	± 0.25 dB
16	-46.186 dBm	-46.528 dBm	0.342 dB	± 0.25 dB
17	-49.119 dBm	-49.520 dBm	0.401 dB	± 0.25 dB
18	-52.120 dBm	-52.527 dBm	0.407 dB	± 0.25 dB

CERTIFICATE OF CALIBRATION

Checked By : 

Certificate Number : JCL/25/0348/HS

3. ABSOLUTE POWER CALIBRATION (1550.0 nm)

No.	APPLIED VALUE	UUT INDICATED VALUE	CORRECTION	UNCERTAINTY
1.	0.341 dBm	0.113 dBm	0.228 dB	± 0.25 dB

4. LINEARITY TEST (1550.0 nm)

No.	APPLIED VALUE	UUT INDICATED VALUE	CORRECTION	UNCERTAINTY
1	-1.387 dBm	-1.578 dBm	0.191 dB	± 0.25 dB
2	-4.348 dBm	-4.536 dBm	0.188 dB	± 0.25 dB
3	-7.366 dBm	-7.553 dBm	0.187 dB	± 0.25 dB
4	-10.366 dBm	-10.551 dBm	0.185 dB	± 0.25 dB
5	-13.374 dBm	-13.556 dBm	0.182 dB	± 0.25 dB
6	-16.368 dBm	-16.551 dBm	0.183 dB	± 0.25 dB
7	-19.366 dBm	-19.554 dBm	0.188 dB	± 0.25 dB
8	-22.381 dBm	-22.560 dBm	0.179 dB	± 0.25 dB
9	-25.380 dBm	-25.558 dBm	0.178 dB	± 0.25 dB
10	-28.384 dBm	-28.563 dBm	0.179 dB	± 0.25 dB
11	-31.366 dBm	-31.554 dBm	0.188 dB	± 0.25 dB
12	-34.357 dBm	-34.547 dBm	0.190 dB	± 0.25 dB
13	-37.358 dBm	-37.550 dBm	0.192 dB	± 0.25 dB
14	-40.354 dBm	-40.547 dBm	0.193 dB	± 0.25 dB
15	-43.363 dBm	-43.552 dBm	0.189 dB	± 0.25 dB
16	-46.365 dBm	-46.554 dBm	0.189 dB	± 0.25 dB
17	-49.366 dBm	-49.554 dBm	0.188 dB	± 0.25 dB
18	-52.383 dBm	-52.574 dBm	0.191 dB	± 0.25 dB

No. Dokumen : Form TCL-QP-19-01

No. / Tgl. Terbit : 01 / 20 Juli 2017

No. / Tgl. Revisi : 02 / 04 Januari 2021

CERTIFICATE OF CALIBRATION

P T TELKOM INDONESIA Tbk
KAN ACCREDITED CALIBRATION LABORATORY (LK-016-IDN)

Jakarta : Jl. Percetakan Negara No.17-19 Jakarta Pusat 10570 Phone 021-21480341
Medan : Jl. Gaharu No. 1 Medan 20235 Phone 061-4531311
Surabaya : Jl. Gayungan PTT No. 17-19 Surabaya 60235 Phone 031-8283678
Makassar : Jl. AP Pettarani No. 4 Makassar 90221 Phone 0411-861153

CS Support
☎ 081-16-4-17025

Certificate Number
JCL/25/0349/HS

Approved Signatory


M. Ilyas

Date of Issue : 02-Jun-2025
Submitted by : PT. TELKOM INDONESIA, Tbk.
Laboratorium Telkom Test House (TTH)
Attention : Mgr. Standardization & Suitability Assurance
Description : OPTICAL POWER METER
Manufacturer/Model : EXFO / FTBx-1750-031-4
Serial Number : 1636843- CH4 (215/CAL)
Environment : 22.4 °C ± 0.8 °C 57 % ± 1.2 % RH
Calibration Location : Onsite
Date Calibrated : 28-May-2025
Date Received : 27-May-2025

PT. Telkom Indonesia, Tbk. - Telkom Certifies that this instrument has been calibrated under the environmental condition stated above using telkom standard (s) which is (are) traceable to the international system of Units (SI) through SCL Hong Kong.

Method of Calibration :

The calibration was carried out based on the established Standard Telkom Calibration Procedure, TCL-WI-O011 and by comparison against the following standard(s) and instrument(s) which is (are) calibrated on schedule to maintain traceability and required accuracy :

Description	S/N	Cal Date	Due Date
1. Optical Fiber Power Meter	1030788-CH1	11-Apr-2025	10-Apr-2028
2. Variable Optical Broadband Source	1082690	23-May-2025	22-May-2026
3. Optical Varibel Attenuator	1025153	11-Apr-2025	10-Apr-2028

CERTIFICATE OF CALIBRATION

Checked By : 

Certificate Number : JCL/25/0349/HS

1. ABSOLUTE POWER CALIBRATION (1310.0 nm)

No.	APPLIED VALUE	UUT INDICATED VALUE	CORRECTION	UNCERTAINTY
1.	0.588 dBm	0.297 dBm	0.291 dB	± 0.25 dB

2. LINEARITY TEST (1310.0 nm)

No.	APPLIED VALUE	UUT INDICATED VALUE	CORRECTION	UNCERTAINTY
1	-1.279 dBm	-1.593 dBm	0.314 dB	± 0.25 dB
2	-4.243 dBm	-4.565 dBm	0.322 dB	± 0.25 dB
3	-7.263 dBm	-7.592 dBm	0.329 dB	± 0.25 dB
4	-10.255 dBm	-10.593 dBm	0.338 dB	± 0.25 dB
5	-13.265 dBm	-13.601 dBm	0.336 dB	± 0.25 dB
6	-16.254 dBm	-16.594 dBm	0.340 dB	± 0.25 dB
7	-19.259 dBm	-19.597 dBm	0.338 dB	± 0.25 dB
8	-22.253 dBm	-22.601 dBm	0.348 dB	± 0.25 dB
9	-25.262 dBm	-25.599 dBm	0.337 dB	± 0.25 dB
10	-28.261 dBm	-28.596 dBm	0.335 dB	± 0.25 dB
11	-31.230 dBm	-31.579 dBm	0.349 dB	± 0.25 dB
12	-34.228 dBm	-34.575 dBm	0.347 dB	± 0.25 dB
13	-37.217 dBm	-37.568 dBm	0.351 dB	± 0.25 dB
14	-40.237 dBm	-40.549 dBm	0.312 dB	± 0.25 dB
15	-43.208 dBm	-43.546 dBm	0.338 dB	± 0.25 dB
16	-46.186 dBm	-46.542 dBm	0.356 dB	± 0.25 dB
17	-49.119 dBm	-49.533 dBm	0.414 dB	± 0.25 dB
18	-52.120 dBm	-52.542 dBm	0.422 dB	± 0.25 dB

CERTIFICATE OF CALIBRATION

Checked By : *U*

Certificate Number : JCL/25/0349/HS

3. ABSOLUTE POWER CALIBRATION (1550.0 nm)

No.	APPLIED VALUE	UUT INDICATED VALUE	CORRECTION	UNCERTAINTY
1.	0.341 dBm	0.077 dBm	0.264 dB	± 0.25 dB

4. LINEARITY TEST (1550.0 nm)

No.	APPLIED VALUE	UUT INDICATED VALUE	CORRECTION	UNCERTAINTY
1	-1.387 dBm	-1.595 dBm	0.208 dB	± 0.25 dB
2	-4.348 dBm	-4.555 dBm	0.207 dB	± 0.25 dB
3	-7.366 dBm	-7.571 dBm	0.205 dB	± 0.25 dB
4	-10.366 dBm	-10.570 dBm	0.204 dB	± 0.25 dB
5	-13.374 dBm	-13.575 dBm	0.201 dB	± 0.25 dB
6	-16.368 dBm	-16.569 dBm	0.201 dB	± 0.25 dB
7	-19.366 dBm	-19.573 dBm	0.207 dB	± 0.25 dB
8	-22.381 dBm	-22.578 dBm	0.197 dB	± 0.25 dB
9	-25.380 dBm	-25.576 dBm	0.196 dB	± 0.25 dB
10	-28.384 dBm	-28.581 dBm	0.197 dB	± 0.25 dB
11	-31.366 dBm	-31.572 dBm	0.206 dB	± 0.25 dB
12	-34.357 dBm	-34.565 dBm	0.208 dB	± 0.25 dB
13	-37.358 dBm	-37.566 dBm	0.208 dB	± 0.25 dB
14	-40.354 dBm	-40.565 dBm	0.211 dB	± 0.25 dB
15	-43.363 dBm	-43.568 dBm	0.205 dB	± 0.25 dB
16	-46.365 dBm	-46.571 dBm	0.206 dB	± 0.25 dB
17	-49.366 dBm	-49.572 dBm	0.206 dB	± 0.25 dB
18	-52.383 dBm	-52.591 dBm	0.208 dB	± 0.25 dB