Popple 631/637 LSO

DOCUMENTATION WORKSHEET: RETAIN IN PATIENT RECORD

Doctor: _____ **Fitter:** _____

Patient Name: _____ **Date:** _____

Patient #: _____ **Additional Follow-Up Dates:** _____

TOOLS NECESSARY: Scissors • Heat Gun • Tape Measure


FOR USE WITH PRODUCTS MANUFACTURED BY ASPEN MEDICAL PRODUCTS ONLY. THIS PRODUCT IS INTENDED FOR APPLICATION BY HEALTH CARE PRACTITIONERS AS DIRECTED BY A PHYSICIAN OR OTHER QUALIFIED MEDICAL AUTHORITY. THIS IS A PREFABRICATED ORTHOSIS. IT IS INTENDED TO BE CUSTOMIZED TO AN INDIVIDUAL PATIENT. FOLLOW THE STEPS BELOW TO CUSTOMIZE.

STEP 1 - MEASUREMENTS

1. Lower abdomen circumference = _____

2. T9 to Sacrococcygeal Junction = _____


SIZING GUIDE		
SIZE	**CIRCUMFERENCE**	
Small	31 in - 37 in	78.74 cm - 93.98 cm
Medium	36 in - 48 in	91.44 cm - 121.92 cm
Large	47 in - 68 in	119.38 cm - 172.72 cm

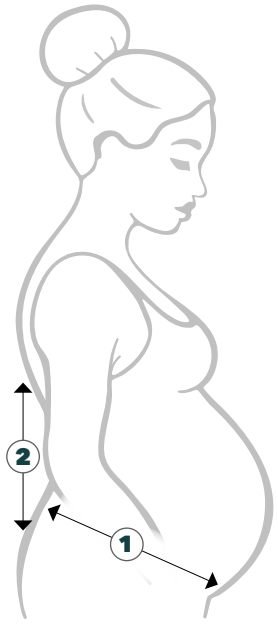

TIME SPENT: _____

STEP 2 - CUSTOMIZE BACK PANEL TO ANATOMY

A. Measure patient's lordosis then customize back panel to anatomy.
B. To customize back panel, remove the panel, heat, trim, and reassemble.

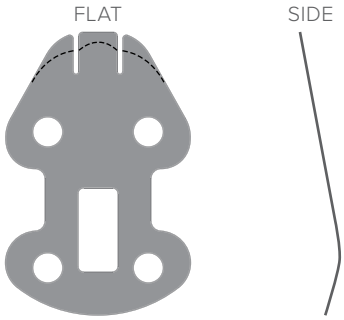


Patient's Lordosis Degree: _____

Heat form to individual patient's anatomy and contour to create intimate fit for individual lordosis and soft tissue. Trim for individual patient's anatomy based on 2 _____

TIME SPENT: _____


STEP 3 - CUSTOMIZE SIZING AND TIGHTENING MECHANISM

SIZING IS CRITICAL TO PROPER PERFORMANCE
Use the measurements below to customize to patient's anatomy.

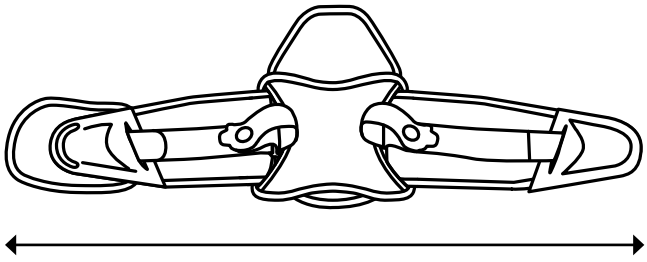


A. Use lower abdomen circumference 1 _____

B. To change the size of the belt, peel up the inside end of the side panel on each side. Adjust to proper fit and reattach.

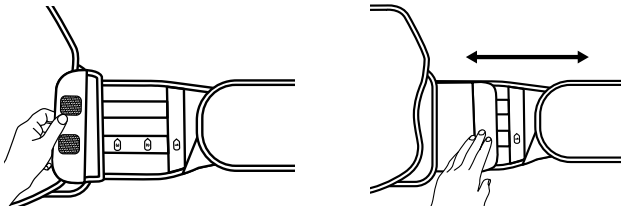

C. Strap Length Modification. Compression straps can be made longer or shorter. Peel up hook end and adjust length before placing back down.

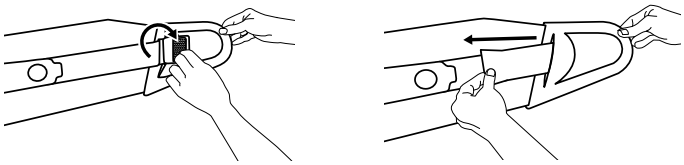

TIME SPENT: _____

© 2025 Aspen Medical Products, LLC · All rights reserved · 6481 Oak Canyon, Irvine, CA 92618-5202, USA
800-295-2776 · 949-681-0200 · aspenmp.com · Pat. aspenmp.com/patents · 12/25

Popple 631/637 LSO

DOCUMENTATION WORKSHEET: RETAIN IN PATIENT RECORD

Doctor: **Fitter:**


Patient Name: **Date:**

Patient #: **Additional Follow-Up Dates:**

TOOLS NECESSARY: Scissors • Heat Gun • Tape Measure

STEP 4 - MODIFY RIGID PANELS

MODIFY ANTERIOR PANEL AS NECESSARY

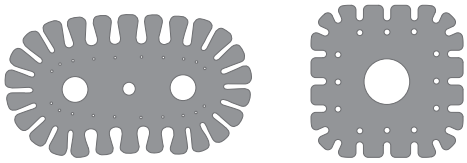



- ☐ Remove and trim to accommodate small and extra small anatomy.
- ☐ Remove and heat mold anterior panel as necessary.

TIME SPENT: _____

STEP 5 - LATERAL PANELS (637 ONLY)

A. With brace extended fully, place one lateral panel on the midline of each side panel of the brace. Press down to secure to brace.
B. When brace is properly fit to the patient, the lateral panels should fit at patient's midline.

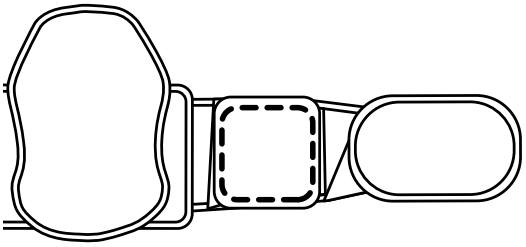



TIME SPENT: _____

STEP 6: EDUCATION

EDUCATE PATIENTS
Proper education is needed to maintain proper fit throughout total time of wear.

Items to educate patients on:

- ☐ Compression mechanics
- ☐ Proper cleaning
- ☐ Follow up appointments
- ☐ Don and doffing
- ☐ Proper placement of brace

TIME SPENT: _____

CLINICAL JUSTIFICATION FOR CUSTOMIZING BRACE

TOTAL TIME TO CUSTOMIZE BRACE: _____

© 2025 Aspen Medical Products, LLC · All rights reserved · 6481 Oak Canyon, Irvine, CA 92618-5202, USA
800-295-2776 · 949-681-0200 · aspenmp.com · Pat. aspenmp.com/patents · 12/25