


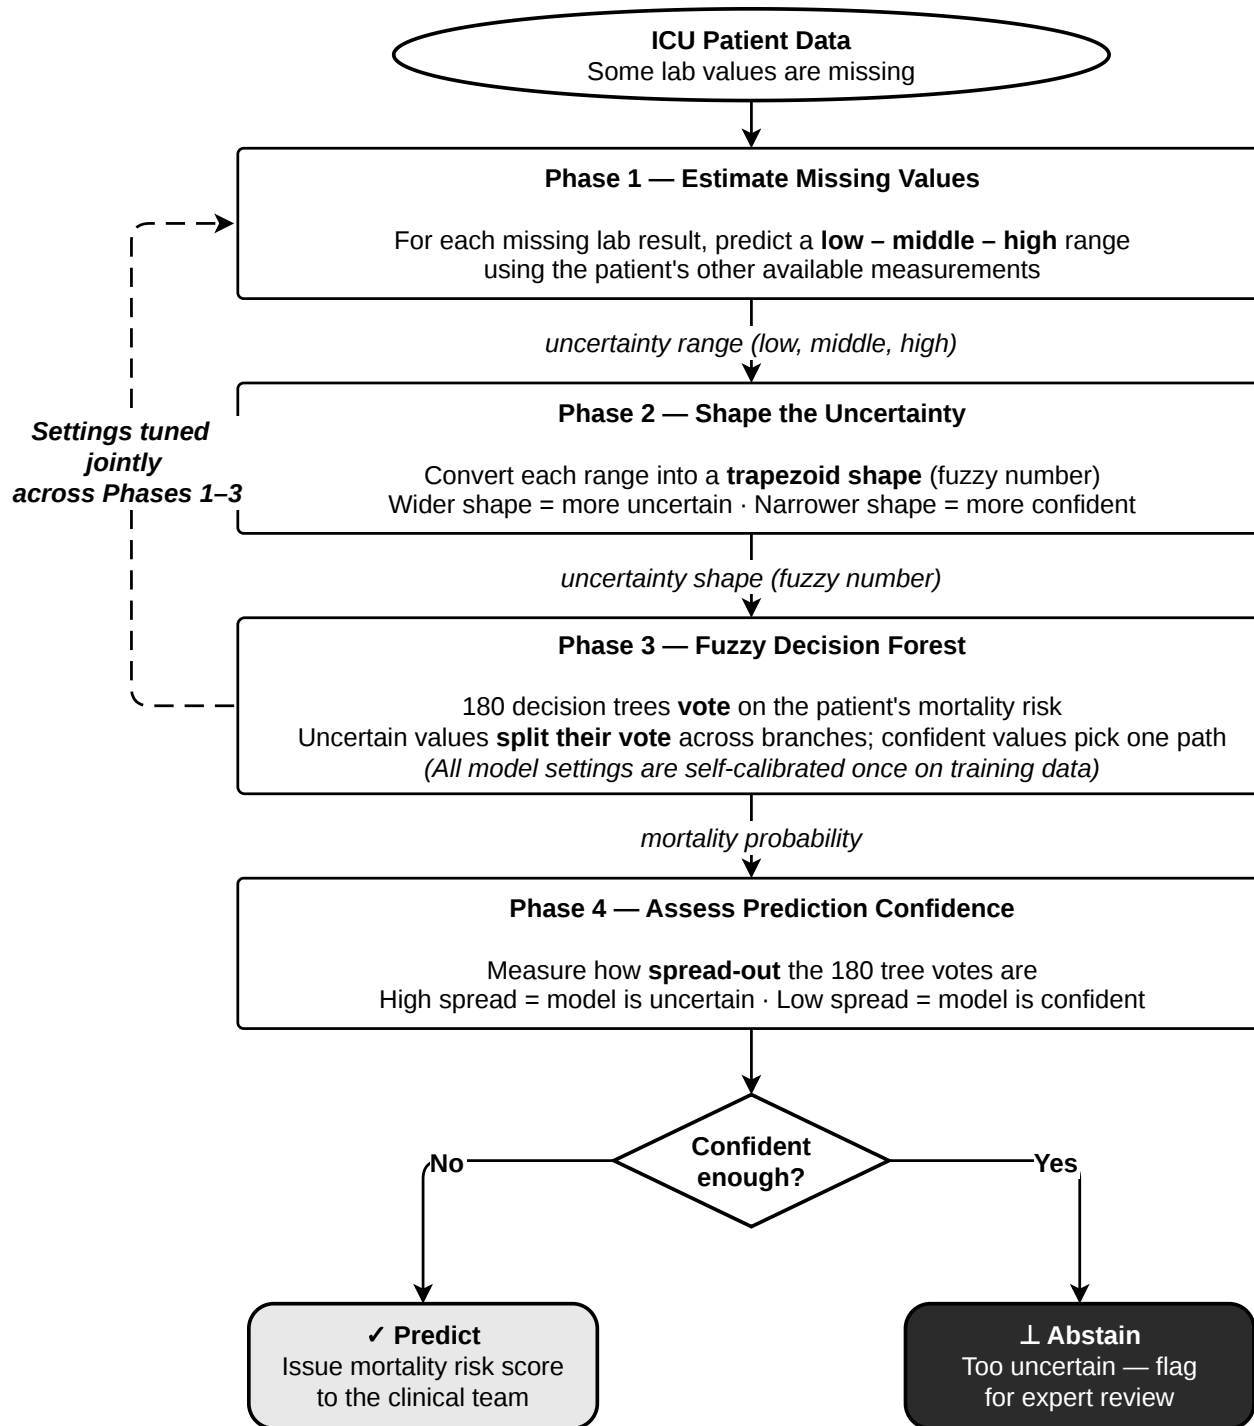

*Model settings are jointly self-calibrated once on training data and applied unchanged to all patients, including external validation.*