
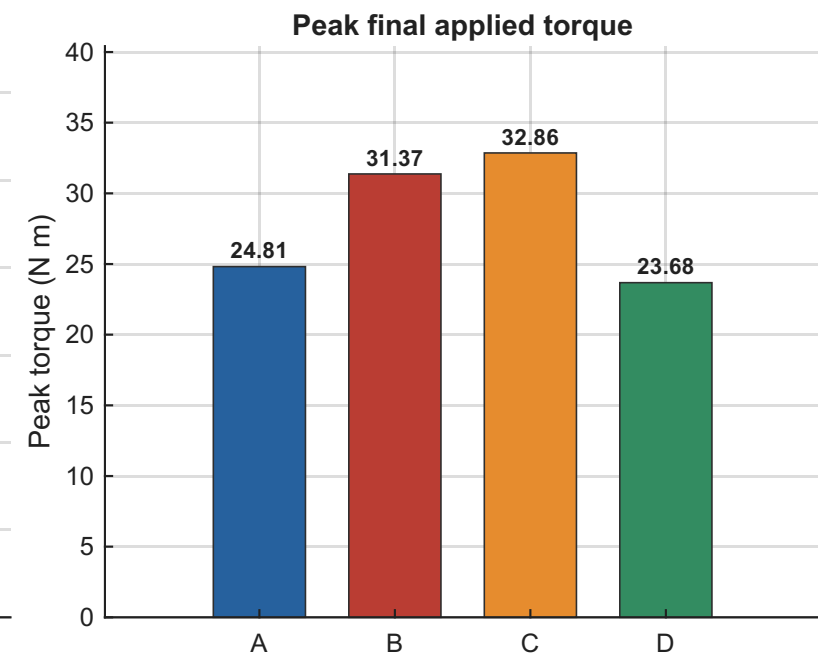
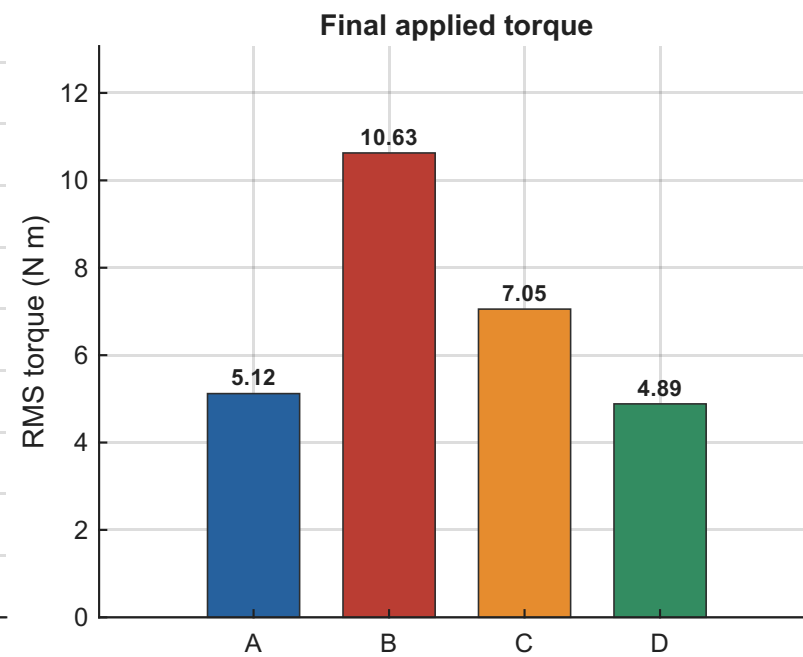
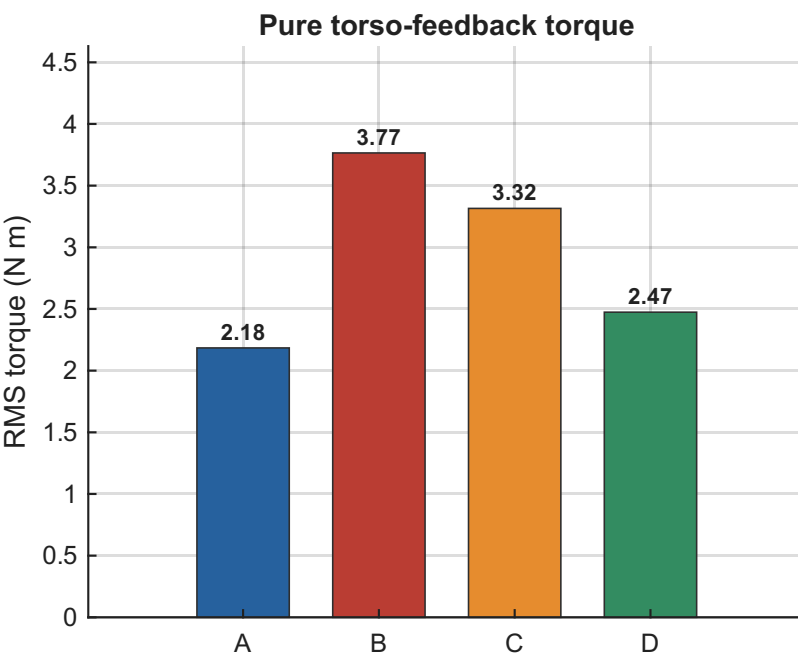
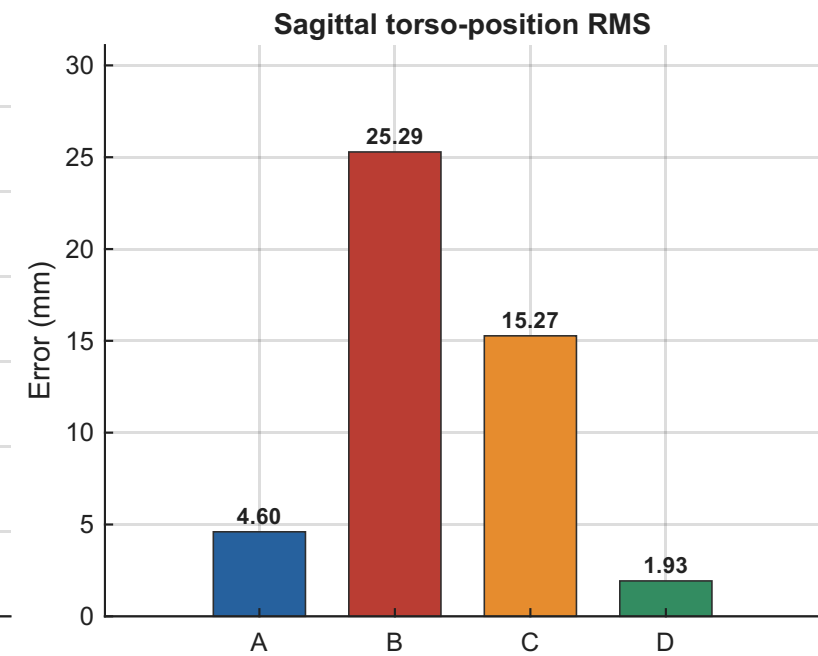
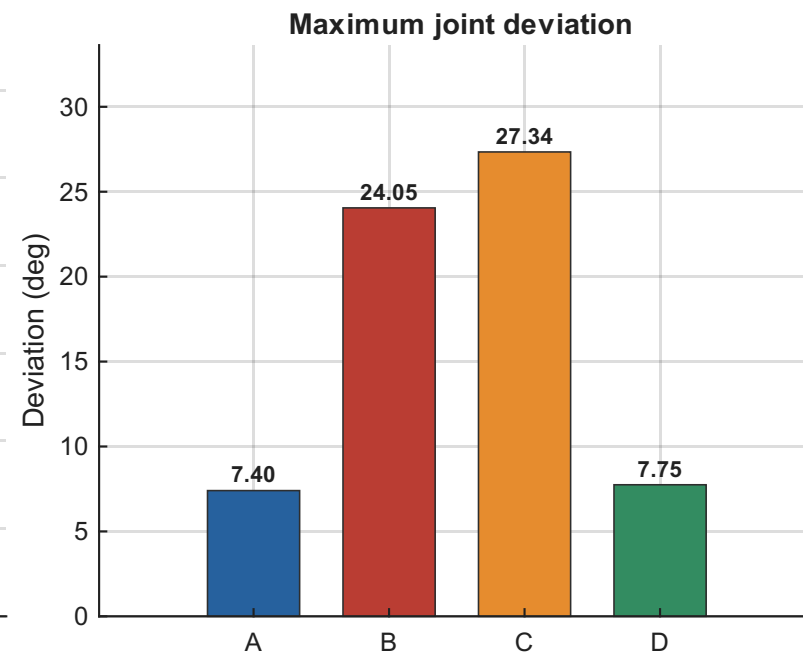


Gravity and nominal-command four-case ablation

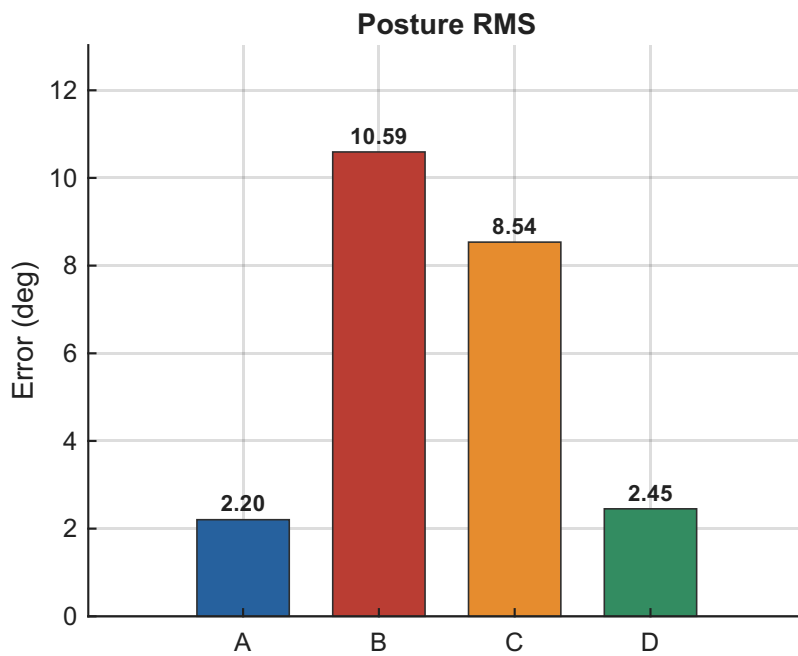

Controller configuration