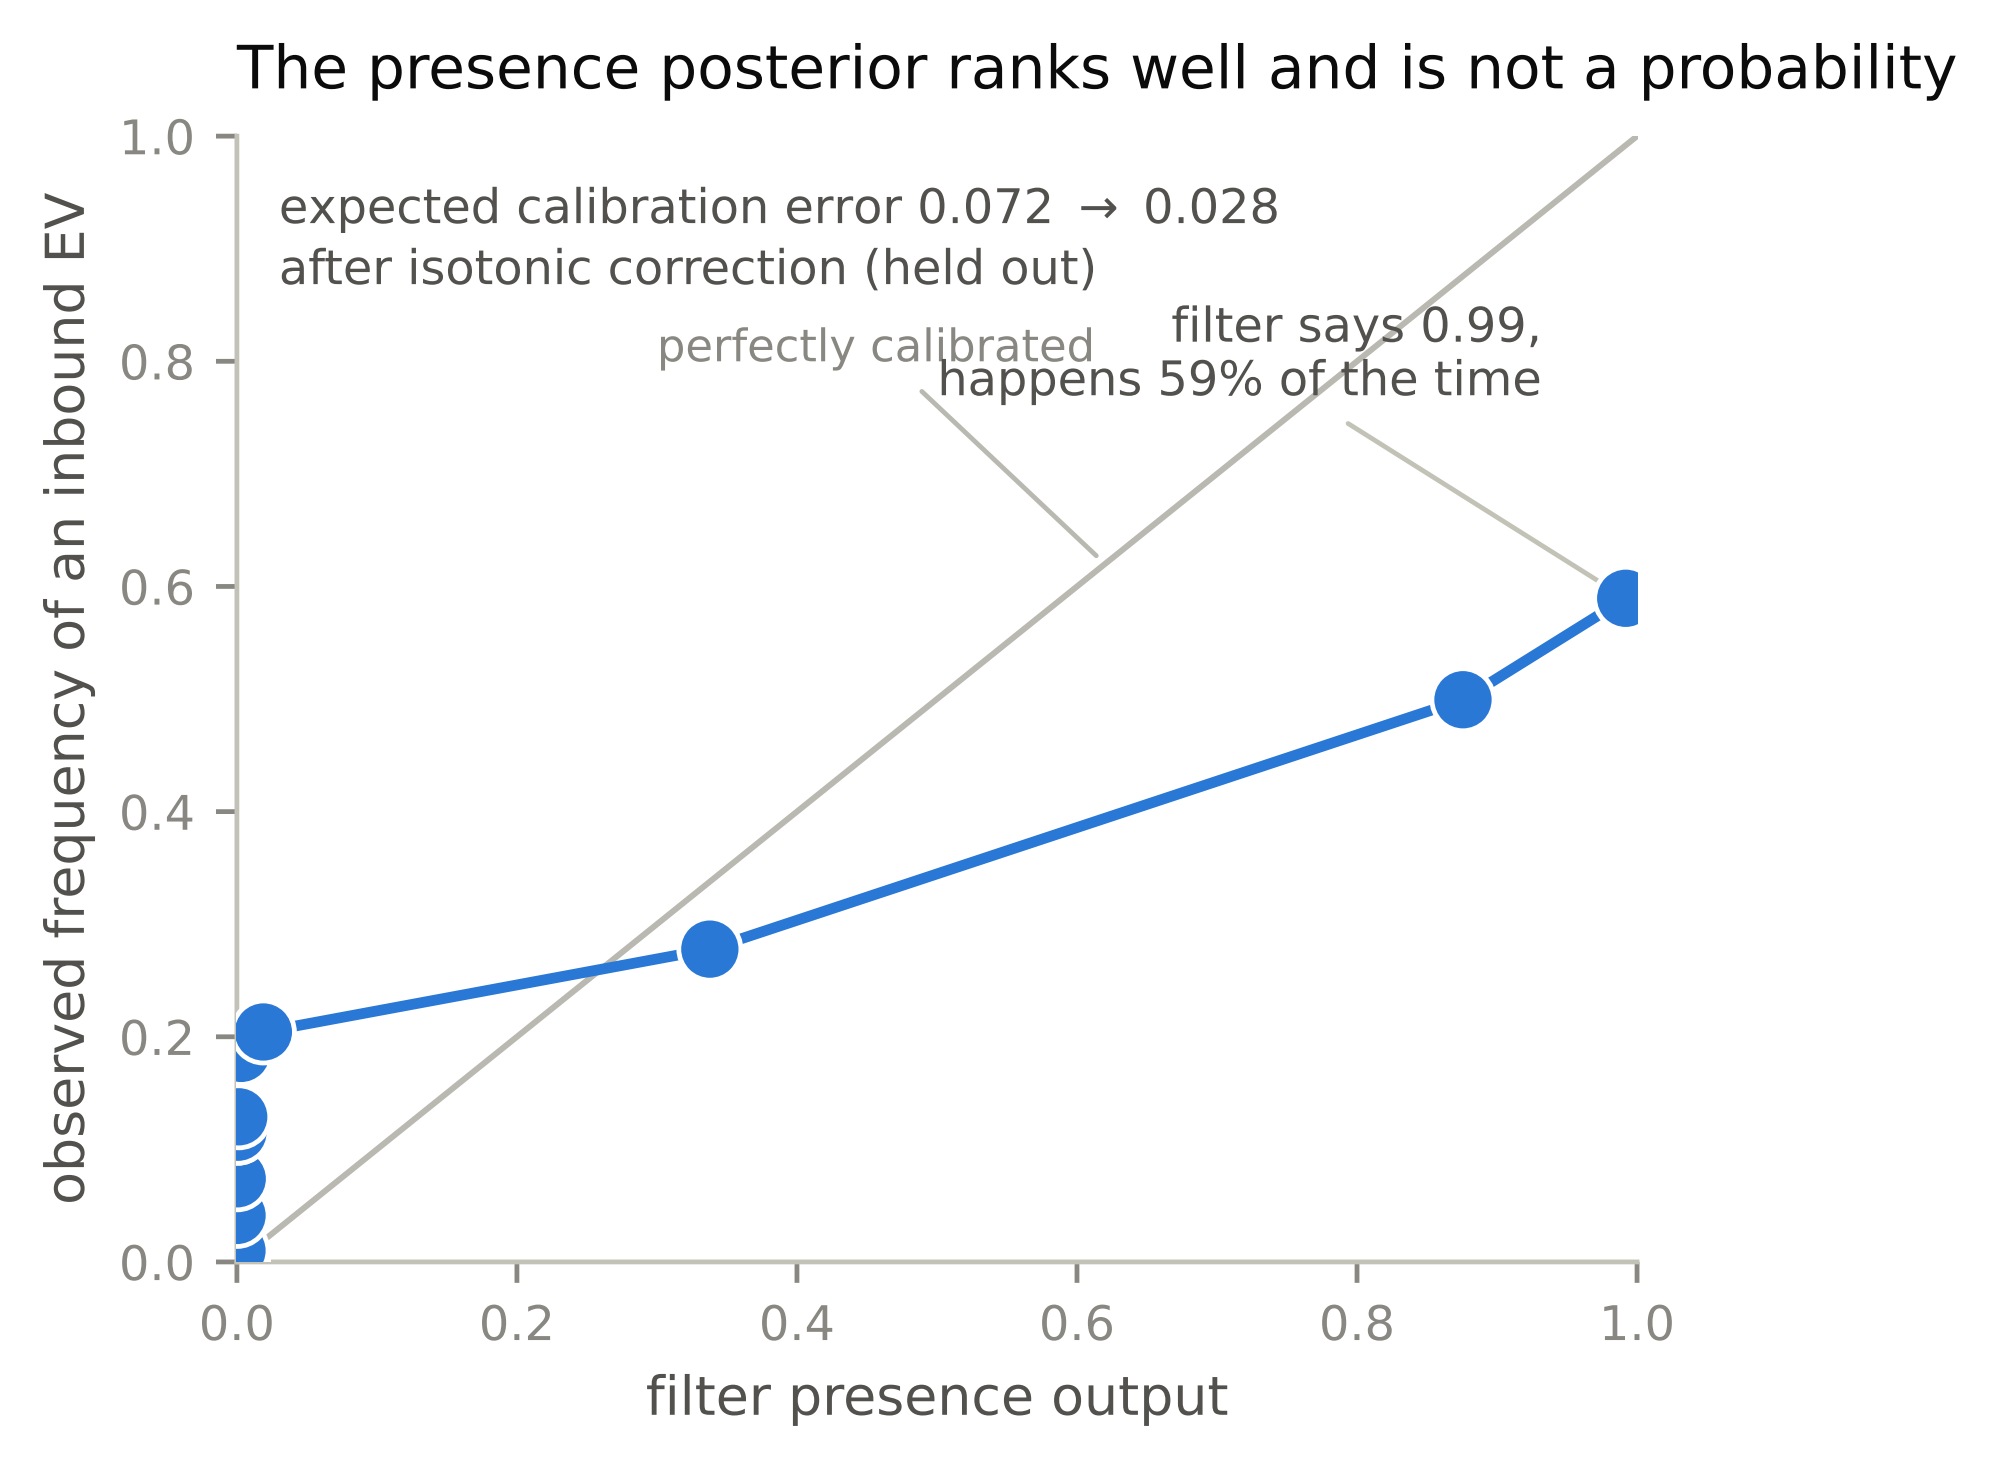
The presence posterior ranks well and is not a probability
expected calibration error 0.072 → 0.028
after isotonic correction (held out)
perfectly calibrated
filter says 0.99,
happens 59% of the time
observed frequency of an inbound EV
filter presence output
0.0
0.2
0.4
0.6
0.8
1.0