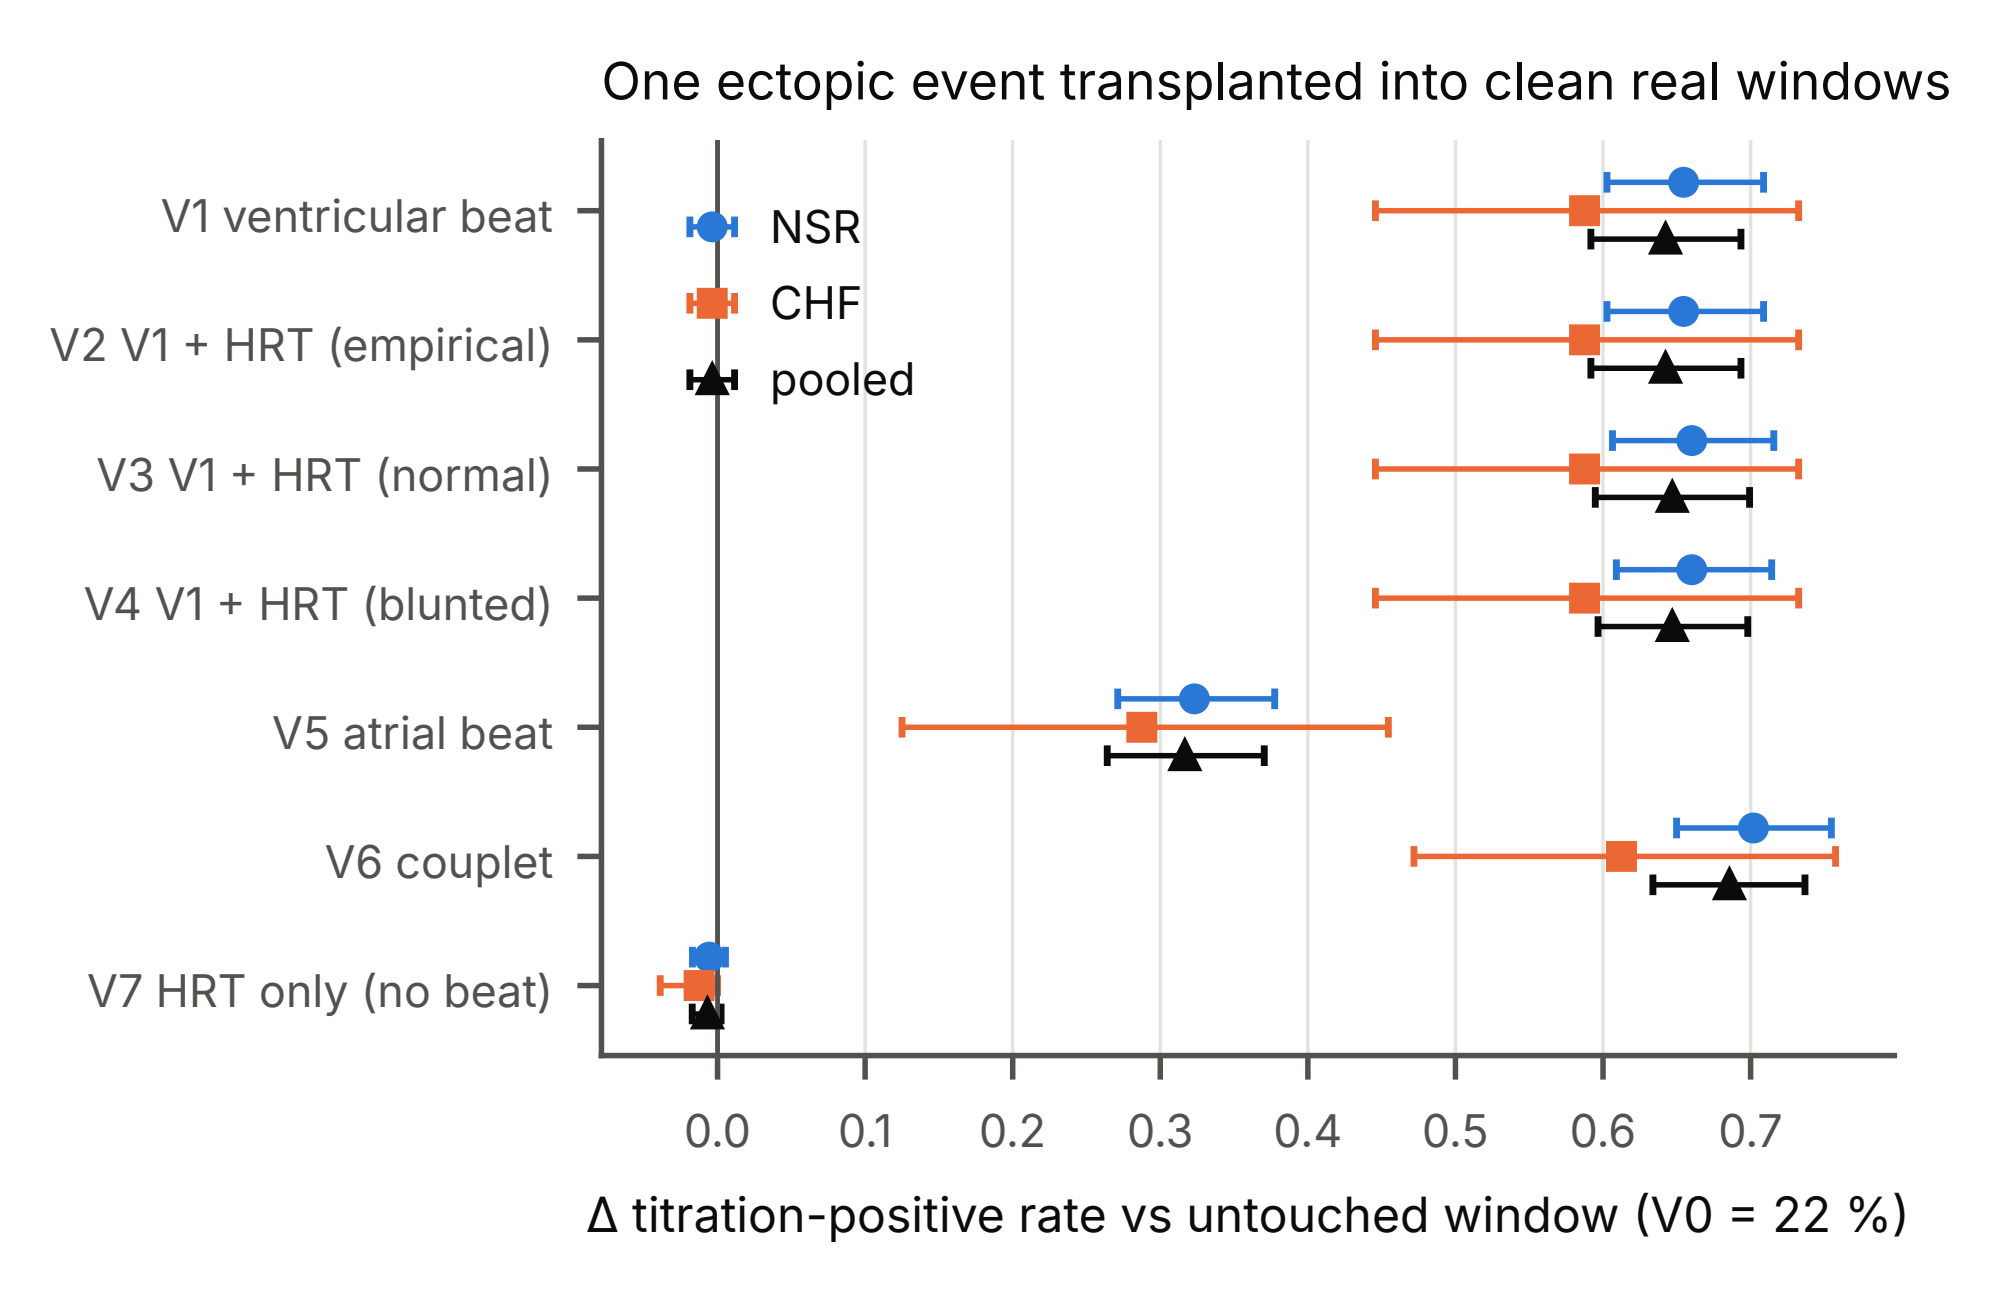
One ectopic event transplanted into clean real windows
V1 ventricular beat
V2 V1 + HRT (empirical)
V3 V1 + HRT (normal)
V4 V1 + HRT (blunted)
V5 atrial beat
V6 couplet
V7 HRT only (no beat)
NSR
CHF
pooled
0.0
0.1
0.2
0.3
0.4
0.5
0.6
0.7
Δ titration-positive rate vs untouched window (V0 = 22 %)