

SHOP PACKET - EASW

REFERENCE	HW3CE700	ODR. QTY (PCS)	4,500	RS(2) QC(5)	ISSUED DATE	14/02/2022
ITEM CODE	H010004	PACK SIZE	50/Box		LOT NO.	B21404
ITEM DESCRIPTION	Hydrocyn Aqua, 100ml (Spray Mist)	CUSTOMER	VMD		MFG. DATE	14/02/2022
PREPARED BY	NAME : NUR SHAHIRA <i>gxt</i> DATE : 14/02/2022	VERIFIED BY	NAME : RATNASEGARAN <i>Nel</i> DATE : 14/02/2022		EXP. DATE	2024-02
UDI-DI NO. (1st Packaging) - Bottle/Box/Bag	N/A	UDI-DI NO. (2nd Packaging) - Carton		N/A	INT. ORDER	IO/VMD/110222/01
UDI-PI NO. (1st Packaging) - Bottle/Box/Bag	N/A	UDI-PI NO. (2nd Packaging) - Carton		N/A		
PROCESS	INPUT BOTTLE	OUTPUT BOTTLE	REJECT	OPERATOR	IPQC APPROVAL	REMARKS
STOCK SOLUTION PREPARATION						
TIME START : DATE : TIME COMPLETE : DATE :	8:00 pm 23-02-22 8:15 Am 24-02-22	4507	4507	Nil	Ryandan (893) 24/2/22	Tank 500L / T1 03HB230222055
UDI PRINTING (Label/Box/Carton)				N/A		UDI NOT REQUIRED FOR THIS LOT
TIME START : DATE : TIME COMPLETE : DATE :	11:30 AM 26-02-22 6:30 PM 26-02-22	4507	4507	Nil	Lina (1131) 26/2/22	Poshini 6:20 pm 26/2/22
SOLUTION FILLING & CAPPING						
TIME START : DATE : TIME COMPLETE : DATE :	11:30 am 26-02-22 6:30 pm 26-02-22	4507	4507	Nil	Era (932)	Poshini 6:30 pm 26/2/22
LABELLING						
TIME START : DATE : TIME COMPLETE : DATE :	11:30 am 26-02-22 6:30 pm 26-02-22	4507	4493	14	Era (932)	Poshini 6:30 pm 26/2/22
PRINTING LOT NUMBER						
TIME START : DATE : TIME COMPLETE : DATE :	11:30 am 26-02-22 6:30 pm 26-02-22	4507	4507	Nil	Era (932)	Poshini 6:30 pm 26/2/22
CAP SEALING (Applicable for 100mL)						
TIME START : DATE : TIME COMPLETE : DATE :	11:40 AM 26-02-22 7:00 PM 26-02-22	4507	4507	Nil	Bashirah (1117) Suri (1125)	Poshini 7:00 26/2/22
BOX PACKING & PRINTING (Applicable for 100ml only)						
TIME START : DATE : TIME COMPLETE : DATE :	4:30 PM 26-02-22 8:40 PM 26-02-22	4507	4507	Nil	Farah (1051) Viki (1094)	Poshini 8:40 pm 26/02/22
MANUAL UDI LABELLING (Applicable for 100 mL & Bags only)				N/A		UDI NOT REQUIRED FOR THIS LOT
TIME START : DATE : TIME COMPLETE : DATE :						
FINAL CONTROL						
TIME START : DATE : TIME COMPLETE : DATE :	4:30 PM 26-02-22 8:40 26-02-22	4507	4507	Nil	Farah (1051) Viki (1094)	Poshini 8:50 AM 28/02/22
CARTON PACK						
TIME START : DATE : TIME COMPLETE : DATE :	11:00 AM 28-02-22 3:00 PM 28-02-22	90 Ctn	90 Ctn	Nil	Fari (1054) RABIN (1086) Herdii (1055) Nurin (1123)	Nurin 28/02/2022
UDI LABELLING				N/A		UDI NOT REQUIRED FOR THIS LOT
TIME START : DATE : TIME COMPLETE : DATE :						

QUANTITY PRODUCED : 4507 Lts
 QUANTITY FOR QC / RETAIN SAMPLE : 2055 Ltr
 SHIPMENT QUANTITY PCS / CTNS : 4500 Lts / 90 Ctn
 FINAL SHIPMENT DATE :
 COMPLETE / PARTIAL : COMPLETE PARTIAL

Checked by (PR), Signature : <i>Nel</i> Name : <i>Ratnasegaran</i> Date : <i>13/3/2022</i>	Approved by (QA), Signature : <i>fmz</i> Name : <i>Rithamza Channa</i> Date : <i>3/3/2022</i>	Released by (QC), Signature : <i>3. J. S. M.</i> Name : <i>MARTINI</i> Designation : IPQC SUP Date : <i>1/3/2022</i> Stamp : <i>IPQC SDN BHD</i>
Remarks:		



VIGILENZ®

ELECTRO ACTIVATED SUPER-OXIDIZED WATER (EASW)

Doc. No	QC-LC002
Rev.	00


Item Description	Hydrogen Aqua, 100ml (spray mist)
Reference	Hw3CE700
Lot No.	B21404

No.	Checklist	Yes	No	Performed by (Signature / Date)	Verified by QC (Signature / Date)	Remarks	Responsibility
1	Flush machine HD-01 with approximately 20L of RODI water & 10L of EASW solution before each production batch	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<i>Wah</i> 26/02/2022	<i>Wah</i> 26/02/2022	N/A	Technician
2	All machine components which are directly in contact with the product materials are thoroughly cleaned and free from rust / dirt / dust and foreign particles	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<i>Wah</i> 26/02/2022	<i>Wah</i> 26/02/2022	N/A	Technician
i)	Starwheel	<input checked="" type="checkbox"/>	<input type="checkbox"/>				
ii)	Nozzle	<input checked="" type="checkbox"/>	<input type="checkbox"/>				
iii)	Stopper Insertor	<input checked="" type="checkbox"/>	<input type="checkbox"/>				
iv)	Cap Dispenser	<input checked="" type="checkbox"/>	<input type="checkbox"/>				
v)	Cap Pusher	<input checked="" type="checkbox"/>	<input type="checkbox"/>				
3	Working area are cleaned and free from any dirt / dust and foreign particles	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<i>Wah</i> 26/02/2022	<i>Wah</i> 26/02/2022	N/A	Production
4	All finished goods, materials and rejected items related to previous lot are cleared and removed from working area	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<i>Wah</i> 26/02/2022	<i>Wah</i> 26/02/2022	N/A	Production

Title:

QC IN-PROCESS INSPECTION RECORD ELECTRO ACTIVATED SUPER-OXIDIZED WATER (EASW)

Document type:
FORMDoc Id:
QC-IP002-09Issue Date:
15/11/2021Page:
1(3)

			 Bactiguard
--	--	--	---

Item Description	Hydrocyn Aqua, 100ml (spray mist)
Reference / Lot No.	Hw3CE700 / B21404
Order Qty	4500
Volume Specification	105 ± 5 ml

A. Filling Process

Sampling / Frequency	Volume Inspected (ml)	No contamination of foreign material / dirt	Functionality of Sprayer or Dispenser (applicable to bottle only)	Proper Cap Sealing/Stopper	No Leaking Observed	Test Disposition
10/10	105 mL	↙	↙	↙	↙	PASS
1/300	105 mL	↙	↙	↙	↙	FAIL
1/300	105 mL	↙	↙	↙	↙	FAIL
1/300	105mL	↙	↙	↙	↙	FAIL
1/300	105mL	↙	↙	↙	↙	FAIL
1/300	105mL	↙	↙	↙	↙	FAIL
1/300	105mL	↙	↙	↙	↙	FAIL
1/300	105mL	↙	↙	↙	↙	FAIL

B. Labelling, Lot No, Manufacturing Date and Expiry Date Process

Sampling / Frequency	Label printing is clear and legible (inclusive of special printing when applicable)	Reference No, Lot No, Manufacturing Date and Expiry Date are corresponding to Shop	Correct Position of Labelling on Packaging	Correct UDI number printing on labelling (Product Code, Manufacturing Date,	Test Disposition
10/10	↙	↙	↙	↙	PASS
1/300	↙	↙	↙	↙	FAIL
1/300	↙	↙	↙	↙	FAIL
1/300	↙	↙	↙	↙	FAIL
1/300	↙	↙	↙	↙	FAIL
1/300	↙	↙	↙	↙	FAIL
1/300	↙	↙	↙	↙	FAIL

QC IN-PROCESS INSPECTION RECORD ELECTRO ACTIVATED SUPER-OXIDIZED WATER (EASW)



Document type:
FORM

Doc Id:
QC-IP002-09

Issue Date:
15/11/2021

Page:
1(3)

Item Description	<i>Hydrogen Peroxide, 100ml (spray mist)</i>	
Reference / Lot No.	<i>HW3CE700 / B21404</i>	
Order Qty	<i>4500</i>	
Volume Specification	<i>10.5</i>	<i>± 5 ml</i>

A. Filling Process

Sampling / Frequency	Volume Inspected (ml)	No contamination of foreign material / dirt	Functionality of Sprayer or Dispenser (applicable to bottle only)	Proper Cap Sealing/Stopper	No Leaking Observed	Test Disposition
<i>1/300</i>	<i>105ml</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>
<i>1/300</i>	<i>105ml</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>
<i>1/300</i>	<i>105ml</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>
<i>1/300</i>	<i>105ml</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>
<i>1/300</i>	<i>105ml</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>
<i>1/300</i>	<i>105ml</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>
<i>1/300</i>	<i>105ml</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>
<i>1/300</i>	<i>105ml</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>

B. Labelling, Lot No, Manufacturing Date and Expiry Date Process

Sampling / Frequency	Label printing is clear and legible (inclusive of special printing when applicable)	Reference No, Lot No, Manufacturing Date and Expiry Date are corresponding to Shop	Correct Position of Labelling on Packaging	Correct UDI number printing on labelling (Product Code, Manufacturing Date,	Test Disposition
<i>1/300</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>
<i>1/300</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>
<i>1/300</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>
<i>1/300</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>
<i>1/300</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>
<i>1/300</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>
<i>1/300</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>	<i>↙</i>

*Wash
26.2.22*

Title: QC IN-PROCESS INSPECTION RECORD ELECTRO ACTIVATED SUPER-OXIDIZED WATER (EASW)		 Bactiguard	Page: 1(3)
Document type: FORM	Doc Id: QC-IP002-09	Issue Date: 15/11/2021	

Item Description	<i>Hydrocyn Aquas, 100 ml (spray mist)</i>
Reference / Lot No.	<i>Hw3CE700 / B21404</i>
Order Qty	<i>4500</i>
Volume Specification	<i>105 ± 5 ml</i>

A. Filing Process

B. Labelling, Lot No., Manufacturing Date and Expiry Date Process

QC IN-PROCESS INSPECTION RECORD ELECTRO ACTIVATED SUPER-OXIDIZED WATER (EASW)

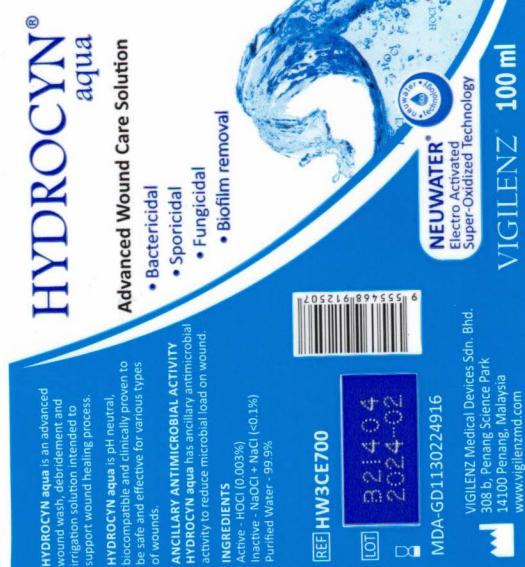
Document type:
FORM

Doc Id:
QC-IP002-09

Issue Date:
15/11/2021

Page:
2(3)

C. Attachment (First Printed Label)



Bactiguard

INDICATION HYDROCYN aqua is indicated as a wound wash, debridement and irrigation solution for acute and chronic wounds such as stage I-IV ulcers, venous stasis & diabetic ulcerations, post-surgery wounds, burns (1 st -2 nd degree) and bed sores. It also helps in moistening wound and control malodour.	B21404 2024-02 <i>Wish 26/12/22</i>	Issue Date: 15/11/2021	Page: 2(3)
---	---	---------------------------	---------------

Disposition of the Lot : PASS FAIL

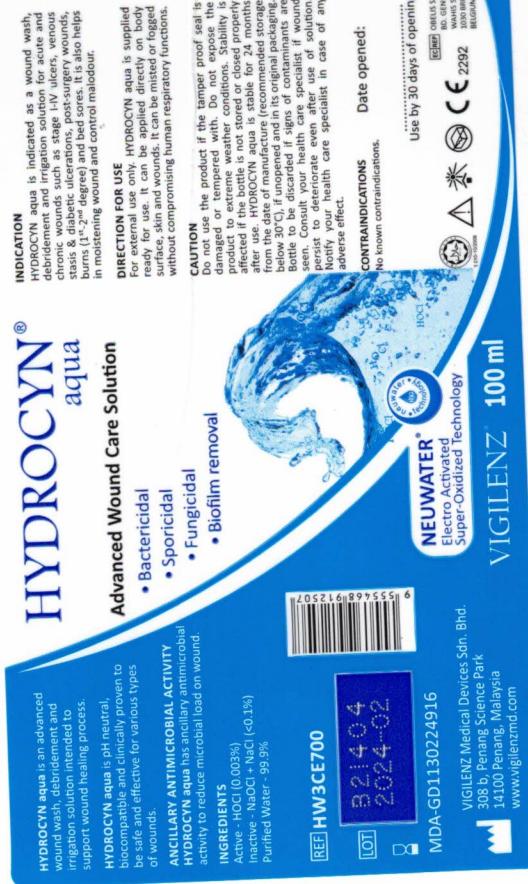
Inspected by : Wish

Name : Wish Wish

Date : 26/12/22

Title:

QC IN-PROCESS INSPECTION RECORD ELECTRO ACTIVATED SUPER-OXIDIZED WATER (EASW)

Document type:
FORMDoc Id:
QC-IP002-09Issue Date:
15/11/2021Page:
3(3)**D. Attachment (Last Printed Label)**

QC IN-PROCESS INSPECTION RECORD ELECTRO ACTIVATED SUPER-OXIDIZED WATER (EASW)	Bactiguard
Document type: FORM	Doc Id: QC-IP002-09

Disposition of the Lot :

 PASS FAIL

Inspected by : Roly
 Name : Poorni
 Date : 26/11/24

VIGILENZ®

FINAL CONTROL TEST REPORT -
ELECTRO ACTIVATED SUPER-OXIDIZED WATER (EASW)

ITEM DESCRIPTION	: <i>Hypochlorous Acid, 100ml</i>	Doc. No.	QC-FC004
REFERENCE	: <i>HWEF100</i>	Rev.	09

ITEM DESCRIPTION : *Hypochlorous Acid, 100ml*

REFERENCE : *HWEF100*

LOT NO. : *B2104*

QTY. PRODUCED (pcs) :

RETAIN SAMPLE QTY. (pcs) :

No.	Inspection Criteria	Sampling Details	Sample Size	AQL		Accept	Reject	Results	Status
				Accept	Reject				
1	Legible and clean printing of label.	<i>S3, 0.15</i>	<i>80</i>	<i>0</i>	<i>1</i>	<i>80</i>	<i>0</i>	<i>pass</i>	<i>pass</i>
2	Free from contamination, deformed or damaged on packaging.	<i>S3, 0.15</i>	<i>80</i>	<i>0</i>	<i>1</i>	<i>80</i>	<i>0</i>	<i>pass</i>	<i>pass</i>
3	Proper sealing and no leaking.	<i>S3, 0.15</i>	<i>80</i>	<i>0</i>	<i>1</i>	<i>80</i>	<i>0</i>	<i>pass</i>	<i>pass</i>
4	Free from contamination / particle / foreign materials on product solution.	<i>S3, 0.15</i>	<i>80</i>	<i>0</i>	<i>1</i>	<i>80</i>	<i>0</i>	<i>pass</i>	<i>pass</i>
5	Correct volume filled (against reference sample).	<i>S3, 0.15</i>	<i>80</i>	<i>0</i>	<i>1</i>	<i>80</i>	<i>0</i>	<i>pass</i>	<i>pass</i>

Remarks :

N/P

Inspected By

Raj

Name

Roshni

Date

26/2/2022

Approved By

M. A. D. T. N. I.

Name

M. A. D. T. N. I.

Date

1/3/2022

DATE :	16/02/2022
REF :	HW3CE700
LOT NO. :	B21404

SHOP PACKET QTY (pes) :	4500
CUSTOMER :	VMD (MALAYSIA)
LO NO. :	IOVMD/110222/01

NO.	SYSTEM CODE	ITEM DESCRIPTION 1	DESCRIPTION 2	LOT NO.	UOM	REQUIRED	ISSUED	QUANTITY (pes)	CONSUMPTION	RECEIVED BY
1	P0100288	100ML HDPE BOTTLE	(NATURAL COLOUR WITH VIGILENZ LOGO)	H075211201	pes	4507	4507	4507	4507	<i>1 Conqueror</i>
2	P0100287	JQ-24A-PP	24/40 MIST SPRAYER, RIBBED, 316 SPRING, HALF CAP. PP, TUBE:90mm	H018200701	pes	4507	4507	4507	4507	<i>1 Conqueror</i>
3	N/A	STOCK SOLUTION	N/A	N/A	ltr	473	473	473	473	<i>1 Conqueror</i>

(2) PRODUCT PACKAGING

NO	SYSTEM CODE	ITEM DESCRIPTION 1	LOT NO.	QTY REQUIRED (pes)	RECEIVED BY	NO	SYSTEM CODE	ITEM DESCRIPTION 1	LOT NO.	QTY REQUIRED (pes)	RECEIVED BY
1	P0100265	Secure Capsel (For 100ml /250ml Hydrocy) - Size: 47 x 0.04 x 5.5 mm (IC+P)	H019210901	4508	<i>Conqueror</i>	1	P0100678	100ml Hydrocyn Aqua Carton-440L X 220W X 156H	H164220101	90	<i>manohly</i>
2	P0100640	LBH-100-R0 - Hydrocyn Aqua 100ml Spray Mist Label, Size : 120mm x 70mm, Material : White PP	L187220201	4508	<i>Conqueror</i>	2	P0100682	100ml LAYER PAD-	H043220101	810	<i>manohly</i>
3	P0100639	100ml Hydrocy Box (Printed) - Material : ArtCard S Coated 300gsm, Size : 40mmx40mmx148mm	H02210901	4508	<i>Conqueror</i>			N/A			

(3) OVER WRAPPING AND CARTON PACK

NO	SYSTEM CODE	ITEM DESCRIPTION 1	LOT NO.	QTY REQUIRED (pes)	RECEIVED BY	NO	SYSTEM CODE	ITEM DESCRIPTION 1	LOT NO.	QTY REQUIRED (pes)	RECEIVED BY
1						1	P0100678	100ml Hydrocyn Aqua Carton-440L X 220W X 156H	H164220101	90	<i>manohly</i>
2						2	P0100682	100ml LAYER PAD-	H043220101	810	<i>manohly</i>
3								N/A			

(4) SPECIAL REQUIREMENT

NO	SYSTEM CODE	ITEM DESCRIPTION 1	LOT NO.	QTY REQUIRED (pes)	RECEIVED BY
1	P0100324	"SAMPLE NOT FOR SALE" Sticker - Size: 35mm x 18mm, Material: Transparent PE, Colour: Red (2 layers)		N/A	<i>Conqueror</i>
2				#N/A	
3				#N/A	

ISSUED BY (MM) :

LOVIN
Signature : _____
Name : _____
Date : 16/02/2022

VERIFIED BY (PR) :

*Not
Received*
Signature : _____
Name : _____
Date : 1/3/22

VIGILENZ®

**PRODUCT RELEASE TEST REPORT –
ELECTRO ACTIVATED SUPER-OXIDIZED WATER (EASW)**

Doc No.	QC-PC007
Rev.	06

Description	Hydrogen Aquo, 100ml (spray mist)	Reference No.	HW3CE700	Date of Inspection	01/03/2023
Lot No.	B21409	Sample Size	500 ml (100ml)		

Release Criteria:

Analysis of Electro Activated Super-Oxidized Water (EASW)					
pH	ORP (mV)	FAC (ppm)	Test Disposition (PASS / FAIL)		
Spec: 6.50 - 8.00	Spec: ≥ 850	Spec: 95 - 140			
Result	Instrument	Result	Instrument	Result	Instrument
7.19	Q1-78	863	Q1-67	111	Q1-80
					Pass

RO water and product bioburden meeting the acceptance criteria.

Remarks : *n/p*

Disposition of the Lot : RELEASE ON-HOLD

Analyzed By : *Rajeshwari*
Name : *Pearl*
Date : *01/03/2023*

Approved By : *M. R. T. N.*
Name : *M. R. T. N.*
Date : *01/03/2023*

