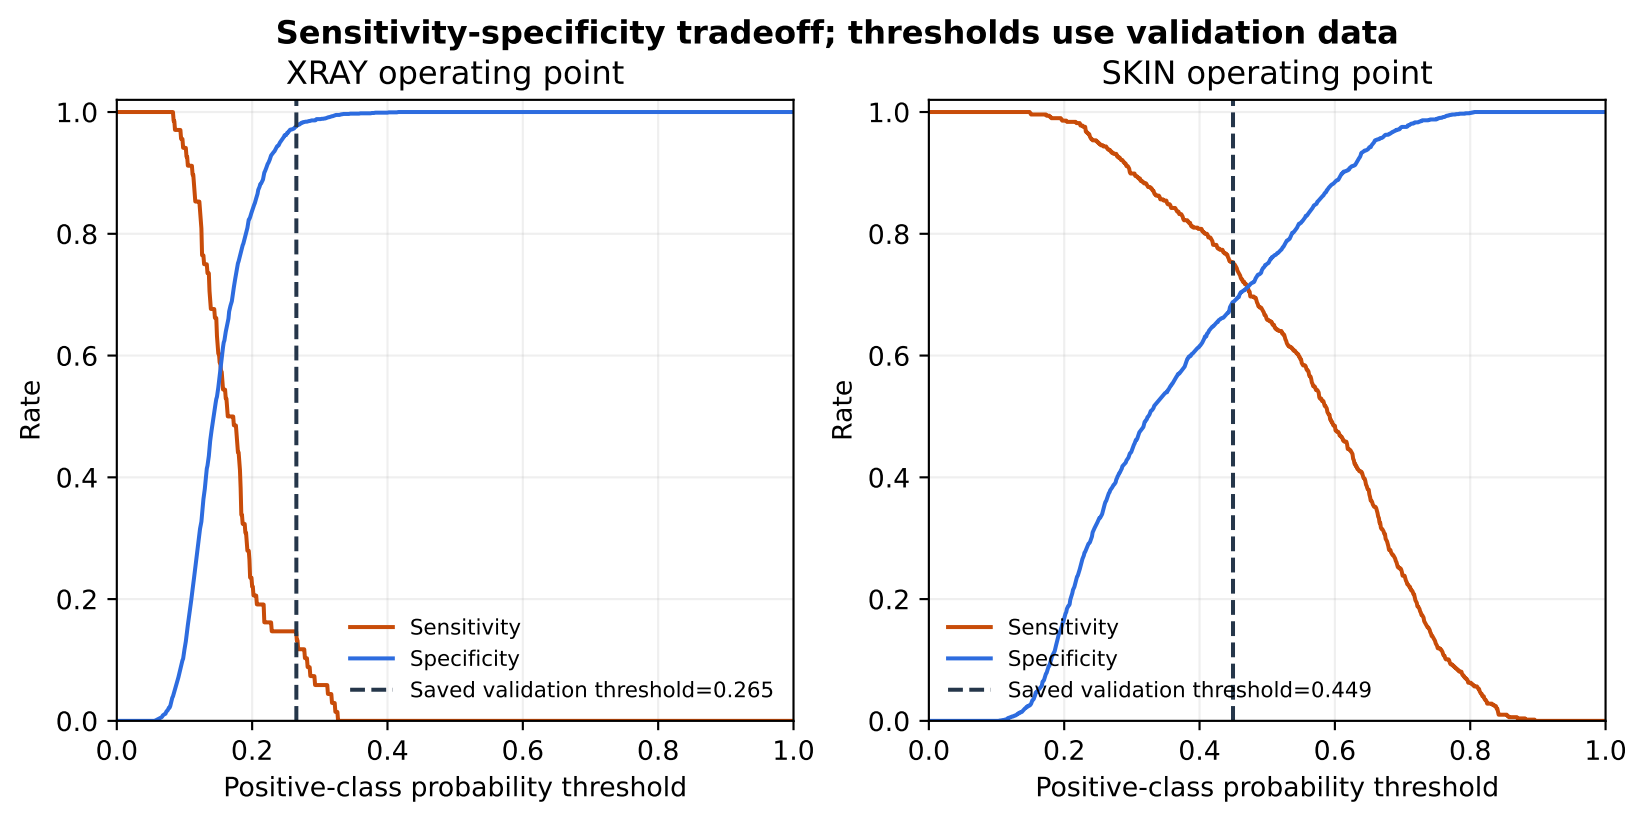
Sensitivity-specificity tradeoff; thresholds use validation data
XRAY operating point
SKIN operating point
Rate
Positive-class probability threshold
Sensitivity
Specificity
Saved validation threshold=0.265
Saved validation threshold=0.449
0.0
0.2
0.4
0.6
0.8
1.0