

POWER

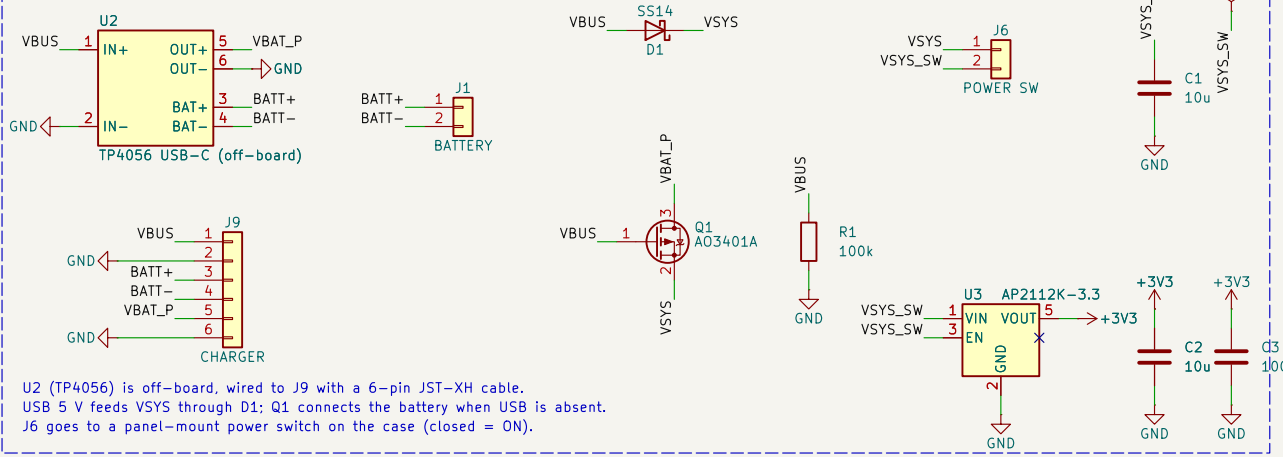


U2 (TP4056) is off-board, wired to J9 with a 6-pin JST-XH cable.
USB 5 V feeds VSYS through D1; Q1 connects the battery when USB is absent.
J6 goes to a panel-mount power switch on the case (closed = ON).

MCU

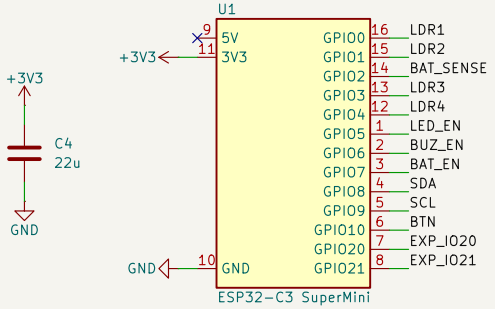


SuperMini 5V pin intentionally unconnected. Antenna end over keepout / board edge.

BATTERY SENSE

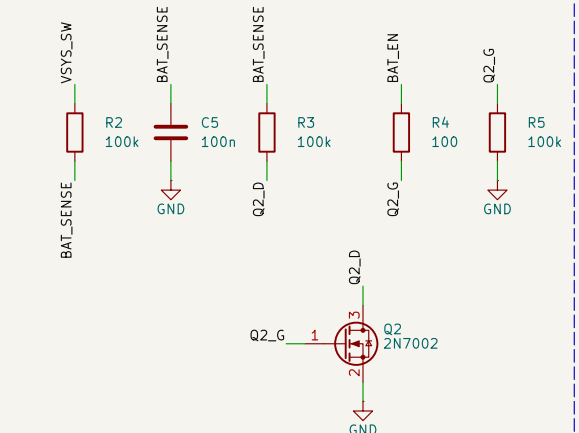


GPIO7 high enables the divider; BAT_SENSE = VSYS_SW / 2

SENSORS (LDR strip)

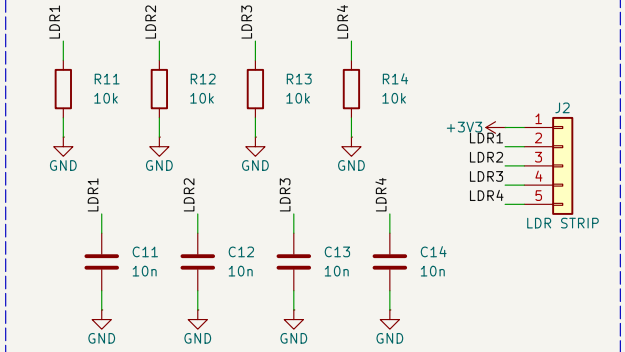


R11–R14 value is a placeholder: tune for the LDRs used

LED (drip chamber)




BUZZER

Buzzer off-board on J7; D3 stays on board

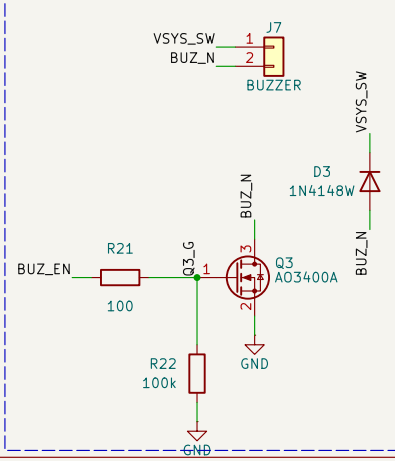

OLED / BUTTON / EXPANSION

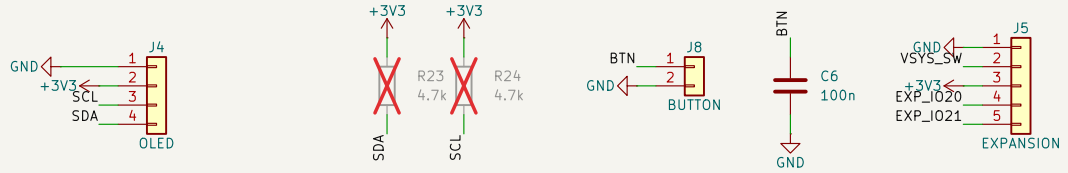

R23/R24 DNP: most OLED modules already have I2C pull-ups

Battery-powered IV drip monitor — main board

Sheet: /
File: ivflow.kicad_sch

Title: IVFlow

Size: A4	Date: 2026-11-01	**Rev: v1**
KiCad E.D.A. 10.0.8		Id: 1/1