



Signal Info

Digital Filters


Signal Info:

Filename	100.dat
Description	
Signal Resolution	11 bits
Zero Signal	1024
Gain	200.000000
Number Of Samples	650000
Frequency	360 Hz
Range	10 mV

Signal:

ECG Signal HRV Analysis QRS Classification HRT Analysis ST Segment QT Interval

Plot:

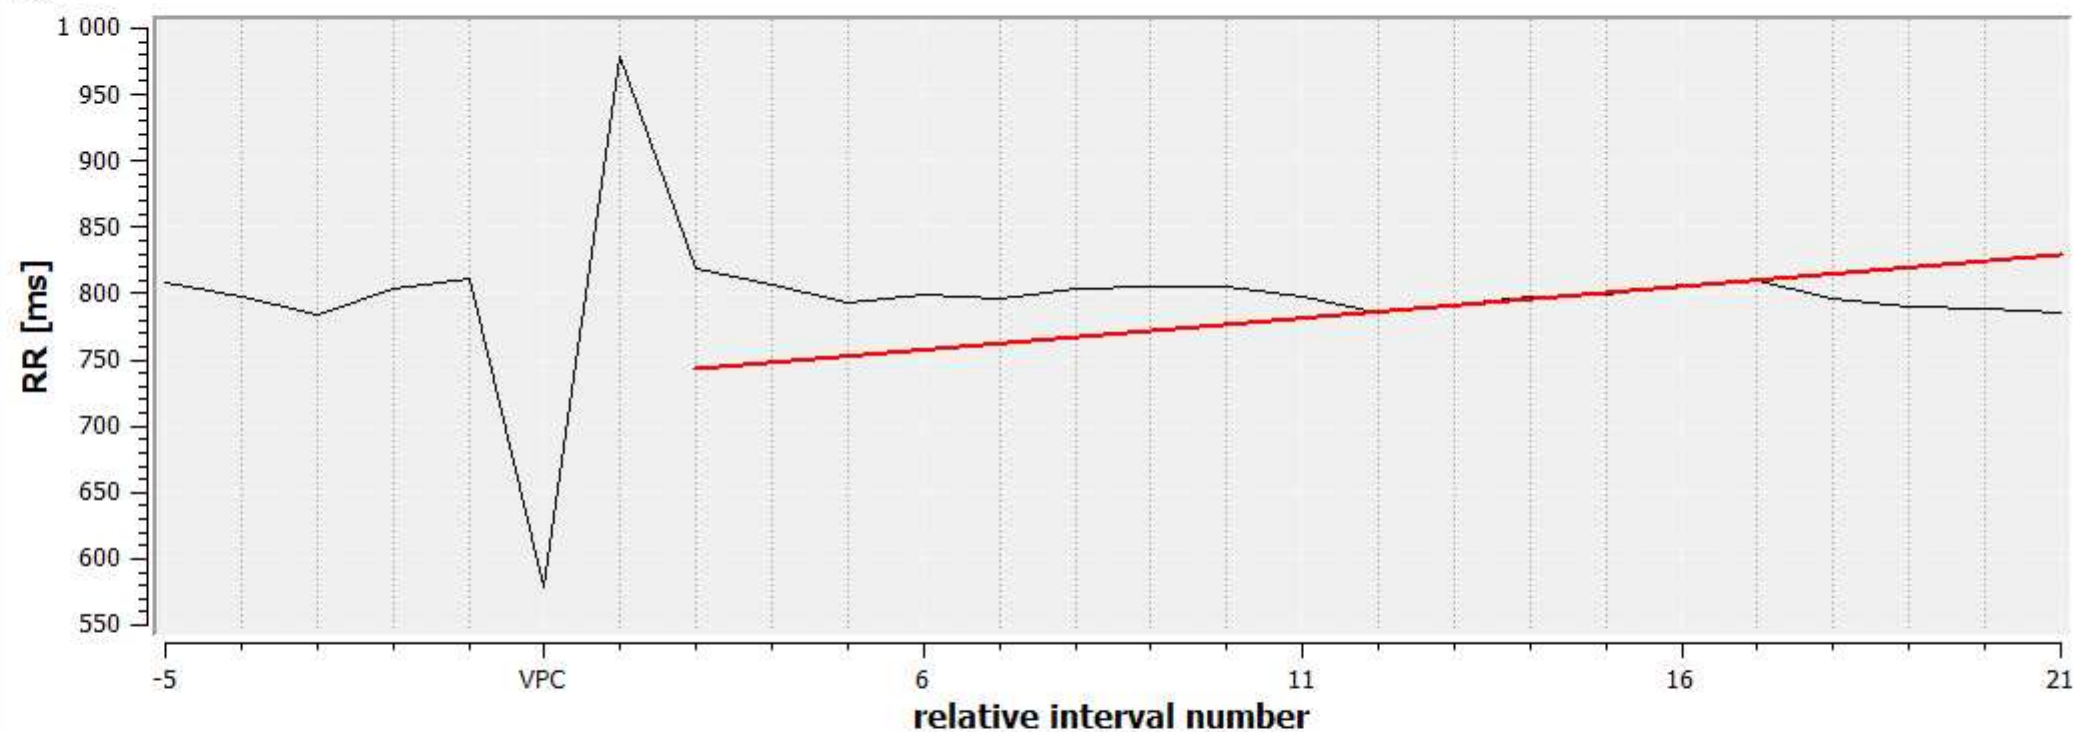

Data:

Number of VPC fulfilling criteria	16
Is the number enough to analyze	YES
TS	4.73125
TO average	0.688718