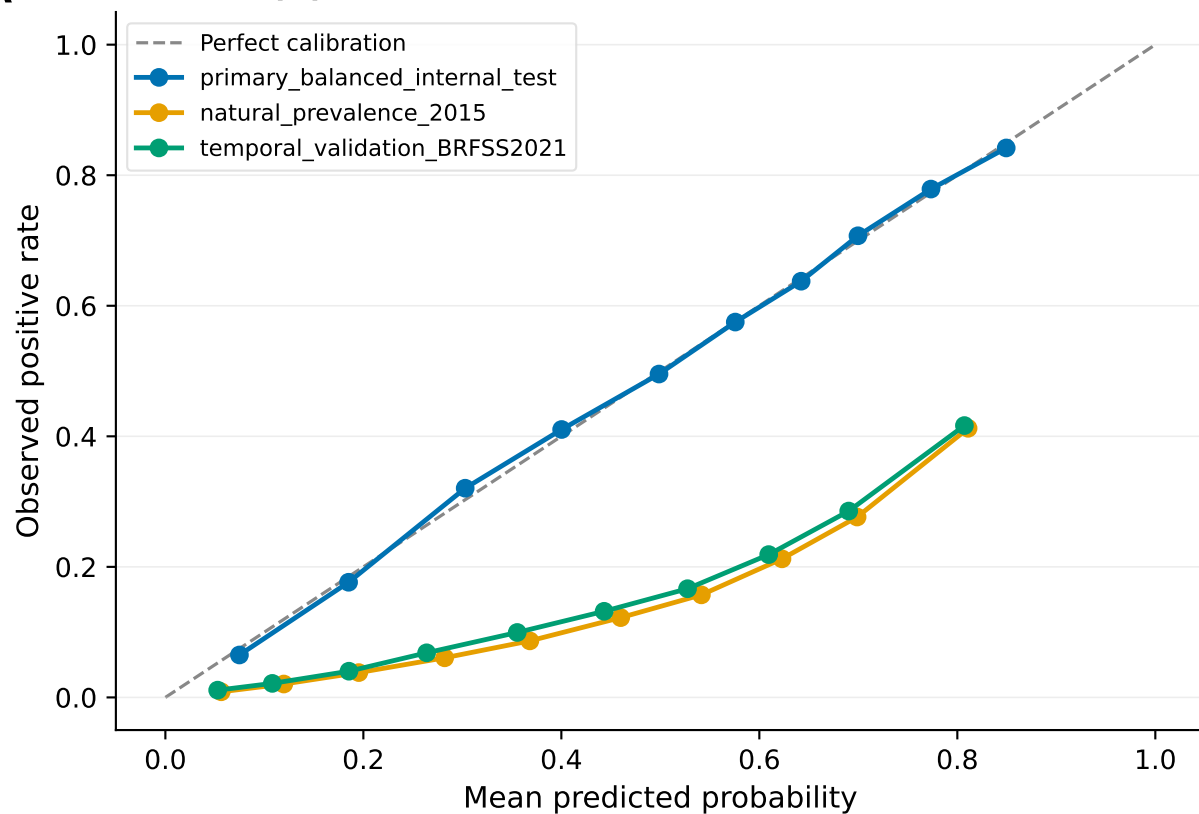
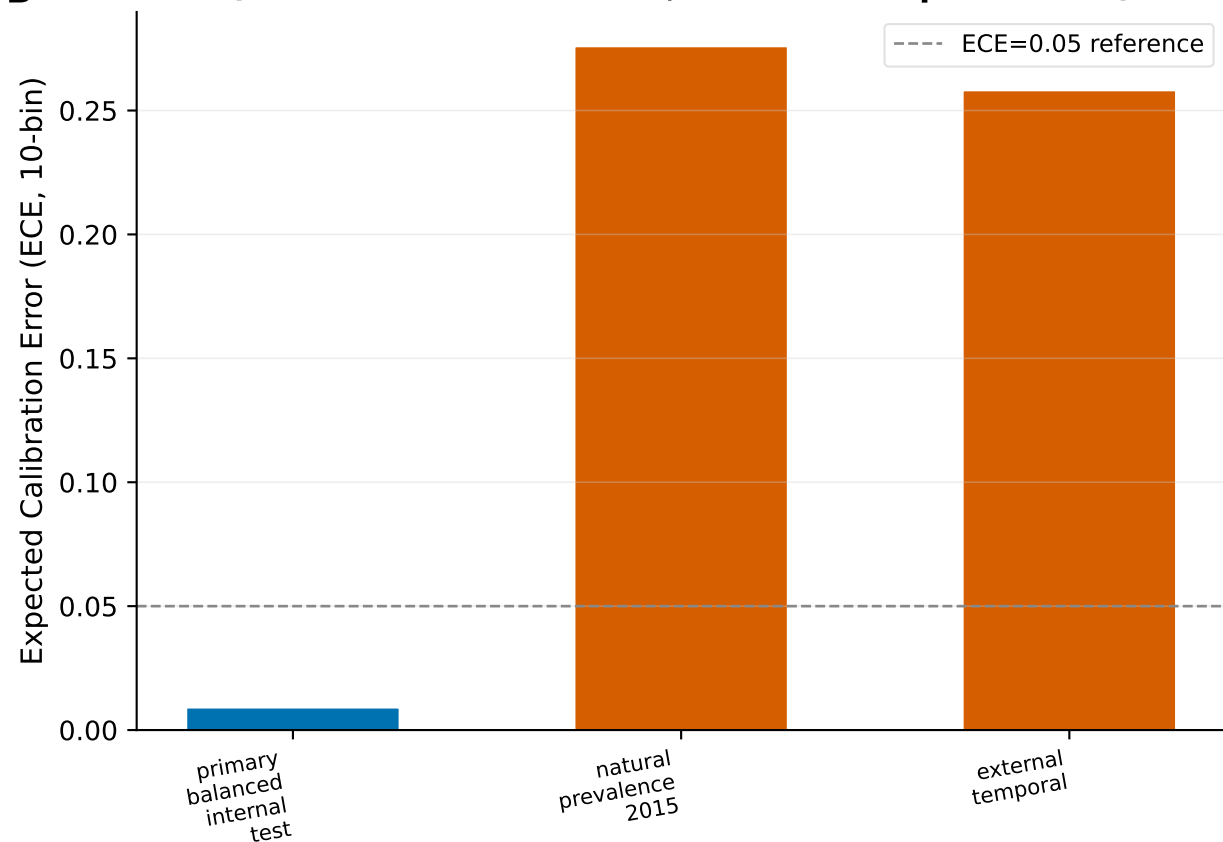


Calibration analysis across balanced and natural-prevalence evaluation sets

A**(A) Calibration curves — all evaluation sets****B****(B) ECE by evaluation set**
(blue=balanced internal; red=natural prevalence)

Note (C2): ECE rises from 0.009 (balanced) to 0.276 (natural prevalence). Calibration intercept=-1.82 at natural prevalence = systematic overestimation. Prevalence-adjusted recalibration required before deployment.