Appendices

Appendix A

Mobile Application Interface

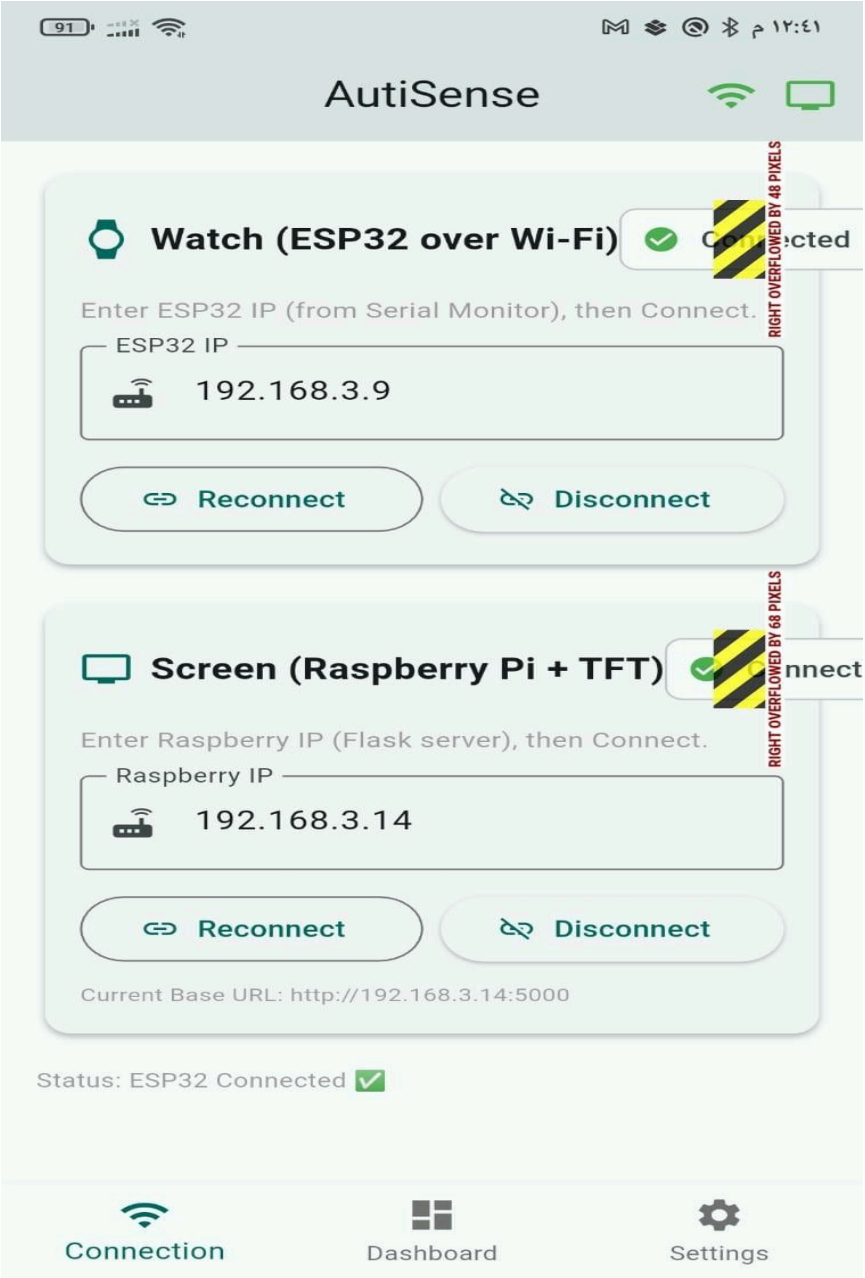

Figure A.1: Device Connection Setup Using IP Addresses

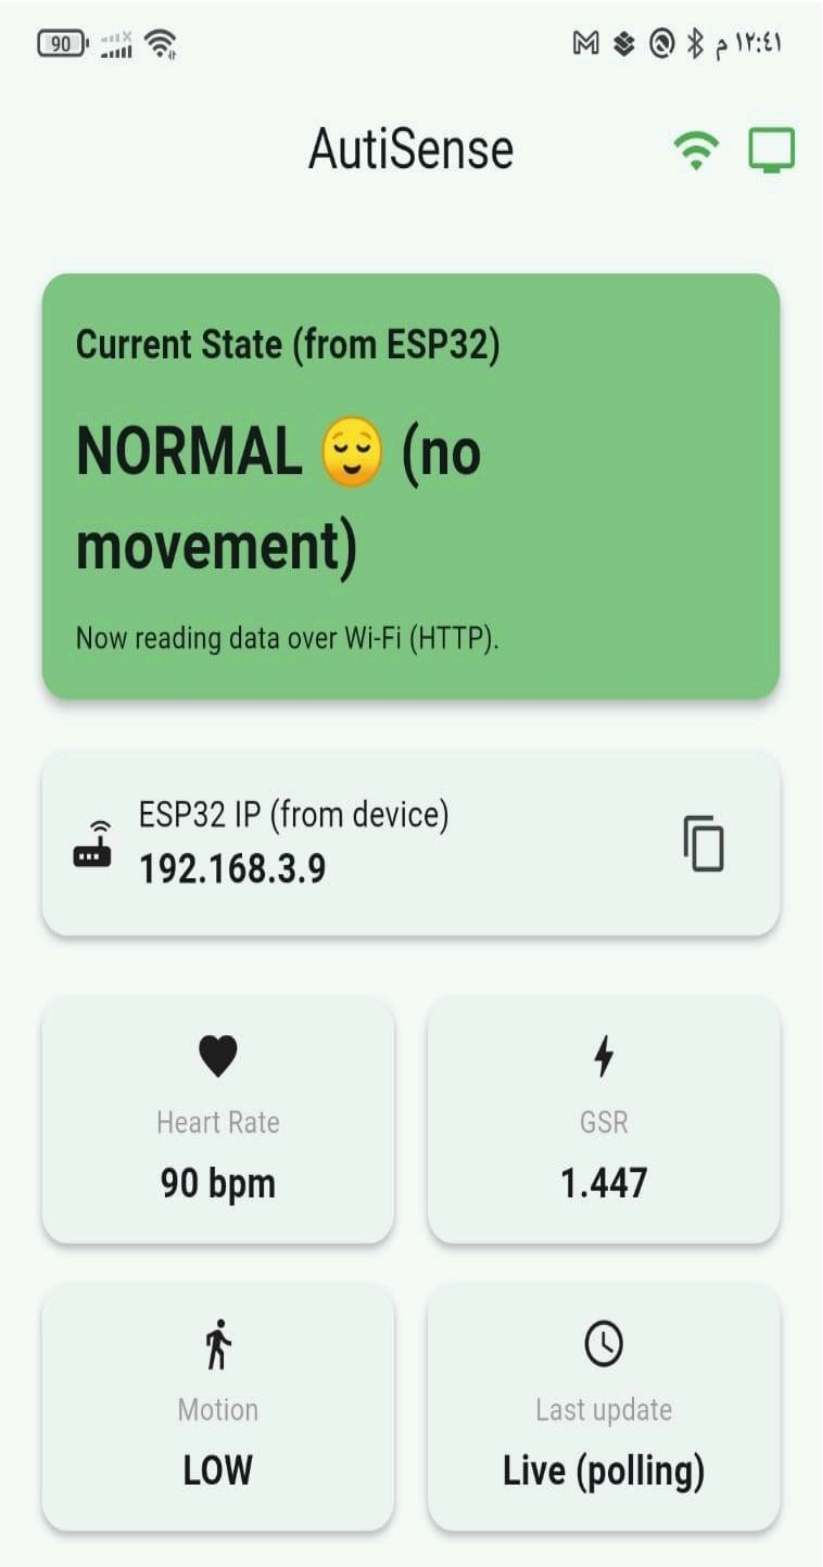

Figure A.2: Real-Time Physiological Data Monitoring

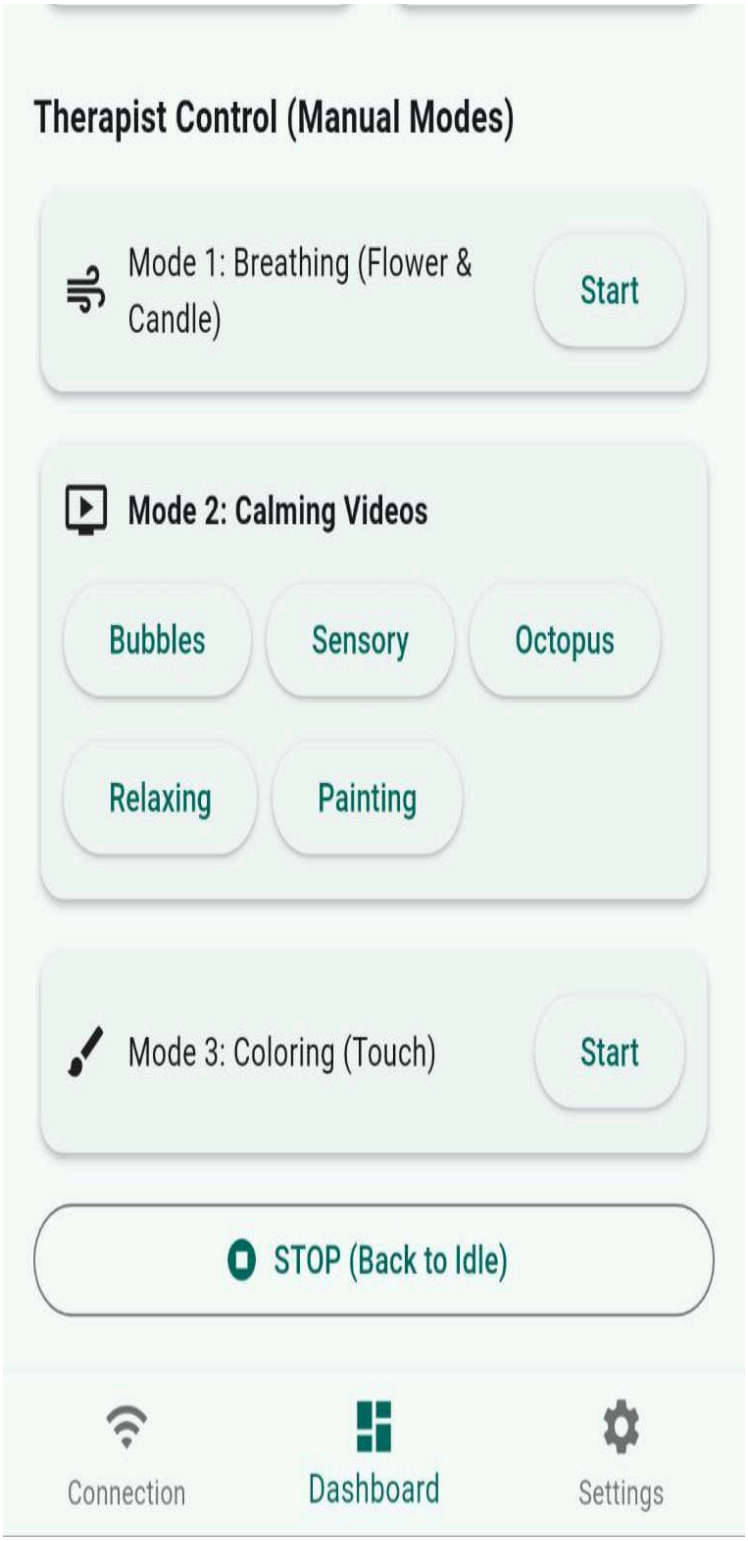

Figure A.3:Calming Mode Selection Interface

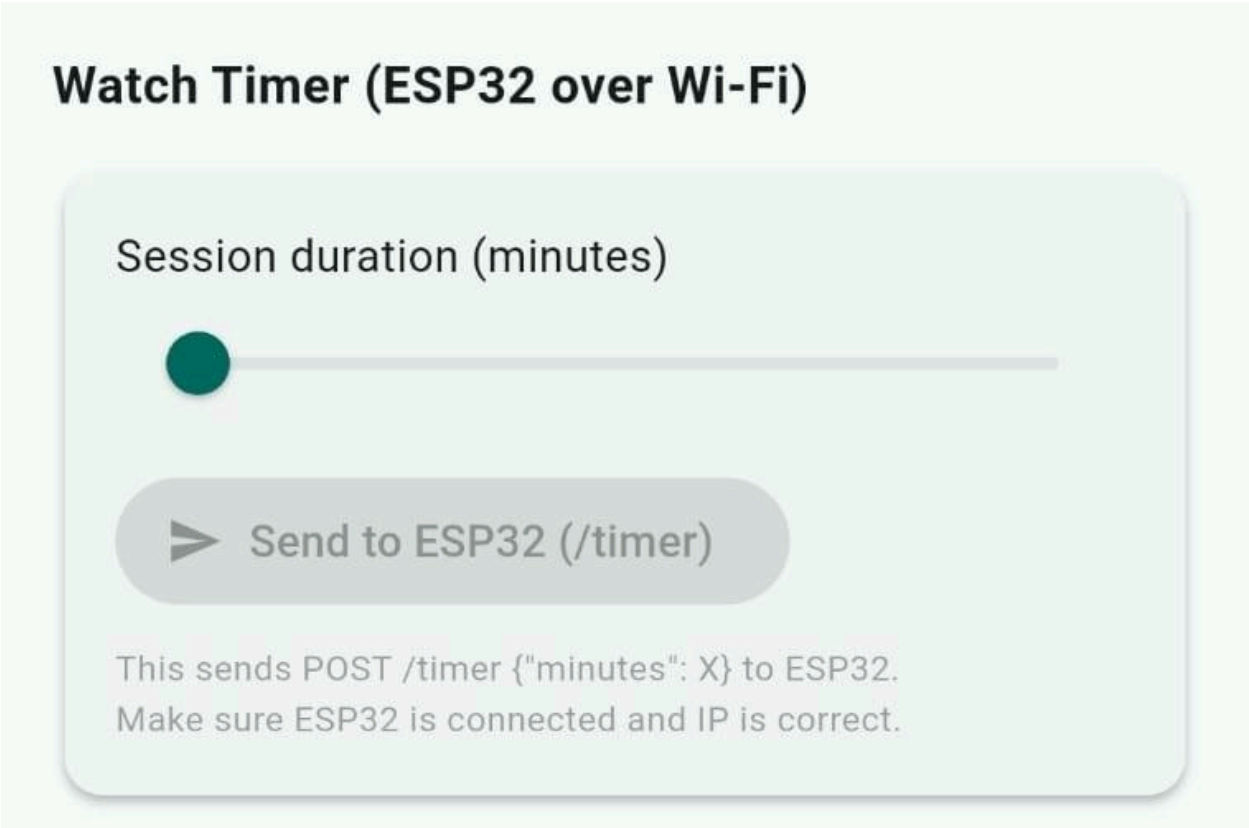

Figure A.4: Manual Control of the NeoPixel Activity Timer