

Development of 3-D Ultrasound System for Assessment of Adolescent Idiopathic Scoliosis (AIS): and System Validation

Chung-Wai James Cheung, Siu-Yin Law, Yong-Ping Zheng, *Senior Member*

Abstract—Adolescent idiopathic scoliosis (AIS) is a common spinal disease and the prevalence of AIS is 2 to 4 % of the youngsters in the United States. Radiograph based Cobb's method is regarded as the gold standard. AIS patients normally have to undergo regular X-ray assessment every 4 to 6 months until skeletal maturity is reached. Because of radiation hazard, X-ray images cannot be taken frequently, and thus it is difficult to perform close monitoring for the disease progression and treatment outcomes. In this study, a free-hand 3D ultrasound imaging system has been successfully developed for the radiation-free assessment of AIS. A series of B-mode ultrasound images with their spatial information were exploited to form a spine model for measuring the spine curvature. Sixteen spine phantoms with different simulated deformity were scanned by both conventional X-ray imaging and the 3D ultrasound system. The results showed that there was a strong correlation ($R^2 = 0.759$) between the Cobb's angles obtained by the two methods. The results also demonstrated a very good intra- and inter-observer reproducibility with ICC of 0.99 and 0.89, respectively. The findings suggest that it is feasible to use 3D ultrasound imaging for the assessment of scoliosis and deserves further clinical tests on patients with spine deformity.

I. INTRODUCTION

Scoliosis is a medical condition of persons with lateral curvature in their spines, and it is often associated with the abnormality in the sagittal plane profile and the axial rotational deformities. In the United States, approximately 20 million people are suffered from scoliosis, and the prevalence of AIS in general population is 2% to 4% [1]. The prevalence of AIS is about 3% in Hong Kong [2]. The most prevalent form of scoliosis among the youngsters (10 to 16 years old) is adolescent idiopathic scoliosis (AIS). By definition, AIS describes those patients with the lateral curvature of the spine more than 10 degrees in the coronal plane, as measured using Cobb's method, which is currently the gold standard for assessing scoliosis, on X-ray radiograph [3]. According to the Scoliosis Research Society, the Cobb's angle is defined as the angle between of the two most tilted end-plates of the vertebral bodies in a standing radiograph.

*Research supported by Research Grant Council of Hong Kong (PolyU5332/07E) and the Hong Kong Innovation and Technology Commission (UIM/213).

C.W.J Cheung is with the Interdisciplinary Division of Biomedical Engineering, the Hong Kong Polytechnic University, Hung Hom, Hong Kong, CHINA (e-mail: JamesCheungWai.Cheung@connect.polyu.hk).

S.Y. Law is with the Interdisciplinary Division of Biomedical Engineering the Hong Kong Polytechnic University, Hung Hom, Hong Kong, CHINA (e-mail: htyenlaw@polyu.edu.hk).


Y.P. Zheng is with the Interdisciplinary Division of Biomedical Engineering, the Hong Kong Polytechnic University, Hung Hom, Hong Kong, CHINA (phone: 852-2766-7664; e-mail: ypzheng@ieee.org).

To identify the type of spine structure problem, clinical examinations are normally used to screen and evaluate the spine deformity before X-ray imaging. During the examinations, information such as gender, age, height, weight, leg length, onset of menarche, family history, and diseases are collected for determining a tentative prognosis; physical and spinal examination including forward bend test, neurological examination, spine side-to-side symmetry, shoulder height, iliac crest symmetry, and lateral examination are exploited to evaluate suspected AIS [4]. When the hump's angle of trunk rotation (ATR) is greater than 7 degrees measured by inclinometer under forward bend test, the patient is recommended for undergoing the standard radiographic evaluation for suspected scoliosis [5]. Evaluating the scoliosis is undertaken by measurement of the Cobb angle. AIS's patients with a Cobb angle of 20 degrees or less, clinical observation is recommended. The patients with immature skeletal and a Cobb's angle of between 20 to 40 degrees are warranted for brace treatment. For those patients with Cobb's angle greater than 40 degrees and immature skeletal or Cobb's angle greater than 50 degrees and mature skeletal are warranted for surgical management [6]. Skeletally immature patients at risk for curve progression can be followed up with posteroanterior radiographs every 6 to 12 months [7]. As Reamy and Slakey [8] reported, there are about 10% of those patients with curve progression warrant intervention. This finding indicates that 90% of the patients are subject to unnecessary radiation.

Regardless the radiation nature of Cobb's method, intrinsic errors exist in radiograph measurement. It is sometimes difficult to identify the oblique projections of the twisting spine in X-ray images, and there is also a considerable variation in the Cobb's angle between the images obtained with different projection angles of the X-ray beam. Intra-observer variation 3- 5° and inter-observer variation 6-9° have been reported in the measurement of the Cobb angle [9] [10][11]. The vertebral rotation of spine is also important for predicting prognosis and monitoring the progression; however, no rotation information can be directly acquired by a standard chest radiograph, the accurate measurement of degree of rotation cannot be undertaken [12]. Two radiographs stitched together to produce whole spine view for assessment are occasionally exploited [13], aggravating risk of radiation exposure. Therefore, it is very necessary to provide a system that can accurately measure spine deformity for AIS mass screening and longitudinal follow-up during treatments without any hazard of radiation.

A number of radiation-free systems have been developed for scoliosis screening, and among them, optical and surface topography techniques are most commonly used. Quantec spinal image system (Quantec Image Processing, Warrington,

It has been reported that the spinal deformity indices, such as vertebra rotation can be derived by ultrasound B-mode image [17]. Despite of simplicity of the approach, the Cobb's angle could not be accurately measured. Although it is possible to obtain high quality volumetric images of spine using MRI without the hazard of radiation; high cost and low accessibility hamper the application. Most importantly, it has been shown that the Cobb's angle derived from the supine posture required by MRI scanning is significantly and spontaneously corrected from the standing posture [12]. Recently, freehand 3D systems have been developed by various groups [18][19][20] for different clinical applications. However, few studies have been reported to use 3D ultrasound systems for scoliosis assessment. Accordingly, the objectives of this study were to develop a 3D ultrasound imaging system for the assessment of AIS and to perform a validation using spine phantoms for this new method.

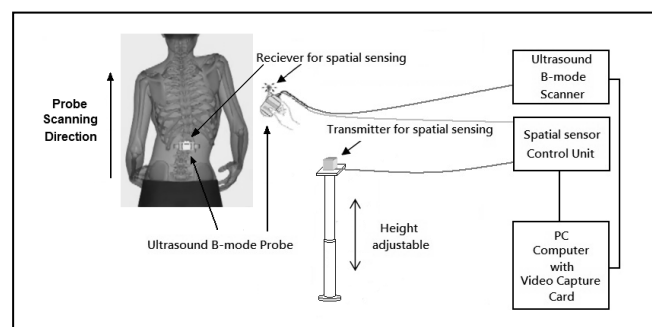

ultrasound method. This pairs of selected vertebra were identified in the 3D model of spine for the corresponding measurement. A line was drawn along the markers of traverse and superior articular processes for each selected vertebrae. In the projection plane, the angle between these two lines was measured to represent the Cobb's angle (Figure 3).

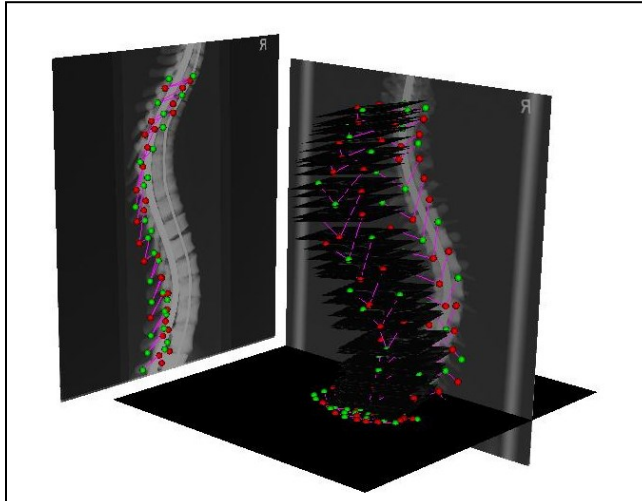


Figure 2. Spine Virtual Model with 3 plane projections

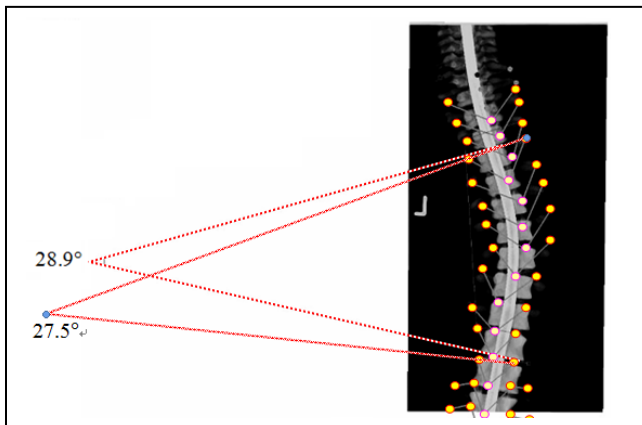


Figure 3. Measurement of curvature using Cobb's method

The intra-observer reproducibility between the results of the repeated sets of 3D ultrasound scanning was tested using intra-class coefficient (ICC) and linear correlation. Linear correlation and Bland-Altman plot were used to test the correlation between the Cobb's angles obtained using the 3D ultrasound and X-ray methods. For this correlation, the mean of two repeated measurements using X-ray images and the mean of the nine repeated measurements using 3D ultrasound imaging were used.

III. RESULTS

The results demonstrated that the 3D ultrasound imaging system could reliably collect images with body landmarks from the spine phantoms. With the help of the program, the virtual spine model was successfully formed for each phantom using the extracted landmarks. The intra- and inter- observer reproducibility test showed that the proposed measurement was highly repeatable with ICC value of 0.99 ($p < 0.001$) and 0.89 ($p < 0.001$), respectively. It has been achieved to view the

deformity of the spine phantom in three orthogonal planes through the projection of the virtual model in different direction. The Cobb's angle of the 16 spine phantoms ranged from 10° to 54°. A very good linear correlation ($R^2 = 0.7586$) was found between the Cobb's angles obtained using the 3D ultrasound and X-ray methods (Figure 4). The Bland-Altman plot showed that there was a good agreement between the results obtained by the two methods with all data points located inside ± 1.96 SD from the mean, with a mean difference of -0.55° and 95% confidence interval (between -2.72° and 1.62°) (Figure 5).

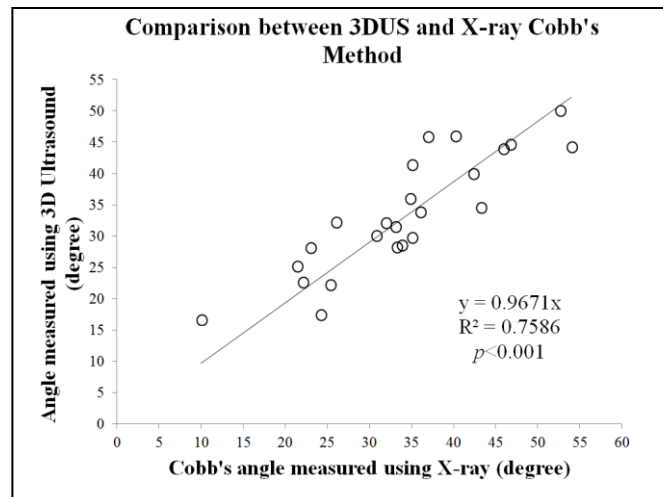


Figure 4. Correlation between 3DUS and X-ray Cobb's method

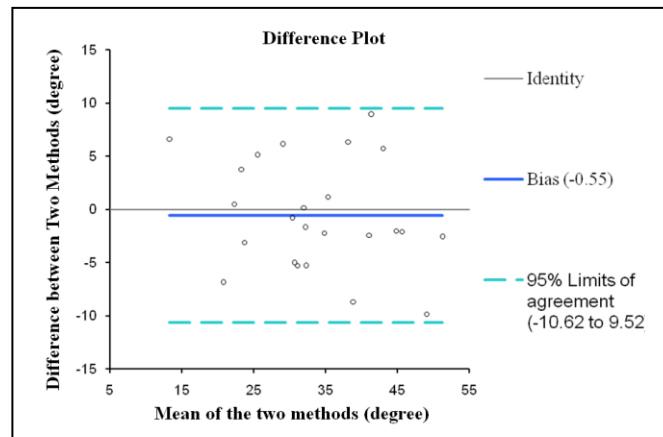


Figure 5. Bland-Altman plot

IV. DISCUSSION

In this study, we have successfully developed a 3D ultrasound imaging method for the radiation-free assessment of scoliosis, and the results of spine phantom tests showed that the new method was reliable and had very good intra- and inter- operator repeatability. Since a virtual 3D model of spine (from L5 to T1) could be formed based on the bony landmarks extracted from ultrasound images, the system provided the deformity of the spine phantom in three orthogonal planes. In this study, we only used the data projected in the coronal plane for comparing with X-ray images. We have also demonstrated

that the spine rotation could be obtained; further studies are needed.

The validation of other radiation-free assessment systems for scoliosis has recently been reported. It was reported that the spine curvature measured by the Quantec system (y) has a linear correlation with the X-ray Cobb's angle (x) with $R^2 = 0.66$ and $y = 2.91 + 0.52 \cdot x$ [21]. For Orthoscan800 system, it was reported that the correlation between the results of the Orthoscan measurement and the Cobb's method was poor ($R^2 = 0.42$ for thoracic curvature data, and $R^2 = 0.017$ for lumbar curvature data) [22]. In this study, we demonstrated that there was a very good correlation between the Cobb's angles measured based on the 3D ultrasound measurement (y) and X-ray method (x) ($R^2 = 0.759$, $Y = 0.967 \cdot x$). It should be noted that the data reported for the two commercial systems were from human subjects, while the data reported in the current study were obtained from the phantoms. The future clinical study of using the 3D ultrasound method should be conducted. Nevertheless, the results of this study showed that 3D ultrasound method is a promising alternative method for the assessment of scoliosis without the hazard of radiation and low cost; longitudinal study of AIS patient becomes more viable. With portable ultrasound system and movable framework, this system can be mobile, allowing operation in small clinic or school for mass-screening. No restriction of frequency use and period time for monitoring patient's spine is obliged while undergoing observation or treatment.

AIS is increasingly treated as a 3D spine deformity problem. Yazici et al. [12] suggested that AIS should be evaluated on coronal, sagittal, and traverse plane with standing images. Although CT and MRI can provide high resolution images in 3D, they require patients being imaged in supine position; measurement of rotation is disputable. The virtual 3D model of spine in this study revealed that the vertebra rotation and the spinal deformity can be measured in three orthogonal planes. It has been previously reported that there was a correlation between the Cobb's angle and the vertebra rotation according to a relatively simple ultrasound measurement [17]. Therefore, the vertebra rotation information may be an important factor to improve the measurement of Cobb's angle using the 3D ultrasound method. Future studies need to be conducted along this direction.

In spite of the encouraging results demonstrated, we identified some limitations. The manually placing of marker is a timely procedure with accuracy depending on the quality of ultrasound images and the subjective interpretation from the operator. We demonstrated the intra-operator repeatability was very high for the spine phantom measurement, but the image quality might be reduced in human subjects because of obesity and complexity of muscle layering. Ultrasound image enhancement, automatic or semi-automatic tip identification methods have to be developed to alleviate the manual efforts in placing the markers.

In summary, we have developed a 3D ultrasound imaging system for the radiation-free assessment of scoliosis. The results of spine phantom study demonstrated that the Cobb's angle measured using the new system correlated well with the result obtained by X-ray method. It was also demonstrated that the virtual 3D model of spine formed by the bony landmarks extracted from ultrasound images could provide the deformity

of spine in different planes as well as the vertebrae rotation information. Clinical trials of using the new system for assessing scoliosis patients are ongoing to further demonstrate its potential for the practical use.

ACKNOWLEDGMENT

The authors would like to thank the Dr. Patrick Y.M. Lai, Department of Health Technology and Informatics, who generously assisted us in the radiograph study.

REFERENCES

- [1] C.R. Good, "The genetic basis of adolescent," *J. Spinal Res. Found.*, 2009, vol. 4, no. 1, pp. 15–64.
- [2] S.P. Tang, J.C.Y. Cheng, B.K.W. Ng, T.P. Lam, "Adolescent idiopathic scoliosis (AIS): An overview of the etiology and basic management principles," *HK J. Paediatr.*, 2003, vol.8, pp. 299–306.
- [3] J.R. Cobb, "Outline for the study of scoliosis," In *American Academy of Orthopaedic Surgeons, Instructional Course Lectures*. St Louis, CV Mosby, 1948, pp. 261-275
- [4] M.J. Bueche, "Scoliosis and Kyphosis. (L.S. Neinstein, ed.)," in *Adolescent Healthcare: A Practical Guide*, Philadelphia:Lippincott, 2008, pp. 235-242.
- [5] W.P. Bunnel, "An objective criterion for scoliosis screening," *J. Bone Joint Surg. Am.*, 1984, vol. 66, pp. 1381-1387.
- [6] H. Kim, H.S. Kim, E.S. Moon, C.S. Yoon, T.S. Chung, H.T. Song, F.S. Suh, Y.H. Lee, S.J. Kim, "Scoliosis imaging: what radiologists should know," *RadioGraphics*, 2010, vol. 30, pp.1823–1842.
- [7] M. Thomsen, R. Abel, "Imaging in scoliosis from the orthopaedic surgeon's point of view," *Eur. J. Radiol.*, 2006, vol. 58, pp. 41-47.
- [8] B.V. Reamy, J.B. Slakey, "Adolescent idiopathic scoliosis: review and current concepts," *Am. Fam. Physician*, 2001, vol. 64, pp.111–116.
- [9] D.L. Carman, R.H. Browne, J.G. Birch, "Measurement of scoliosis and kyphosis radiographs. Intraobserver and interobserver variation," *J. Bone Joint Surg. Am.*, 1990, vol. 72, pp.328-333.
- [10] R.T. Morrissy, G.S. Goldsmith, E.C. Hall, D. Kehl, G.H. Cowie, "Measurement of the Cobb angle on radiographs of patients who have scoliosis," *J. Bone Joint Surg.*, 1990, vol. 72, pp.320-327.
- [11] J.E.H. Puijss, M.A.P.E. Hageman, W. Kessen, R. van der Meer, J.C. van Wieringen, "Variation in Cobb angle measurements in scoliosis," *Skeletal Radiol.*, 1994, vol. 23, pp. 517-520.
- [12] M. Yazici, E.R. Acaroglu, A. Alanay, V. Deviren, A. Cila, A. Surat, "Measurement of vertebral rotation in standing versus supine position in AIS," *J. Ped. Orthop.* 2001, vol. 21, pp. 252-256.
- [13] D. Malfair, A.K. Flemming, M.F. Dvorak, P.L. Munk, A.T. Vertinsky, M.K. Heran, D.A. Graeb, "Radiograph evaluation of scoliosis: Review," *American Journal of Roentgenology*, 2010, vol. 194, no. 3, pp. S8-S22.
- [14] M. Idesawa, T. Yatagai, T. Soma, "Scanning moiré method and automatic measurement of 3-D shapes," *Appl. Opt.* 1977, vol. 16, pp.2152-2162.
- [15] J.G. Thometz, R. Lamdany, X.C. Liu, R.J. Lyon, "Relationship between quantec measurement and Cobb angle in patients with idiopathic scoliosis," *Pediatr. Orthop.*, 2000, vol. 20, no. 4, pp.512-516.
- [16] D. Dickman, O. Caspi, "Assessment of scoliosis with ortelius 800 – preliminary results," *Clin. Appl. Notes*, pp.1-7, April 2001.
- [17] S. Suzuki, T. Yamamuro, J. Shikata, K. Shimizu, H. Iida, "Ultrasound measurement of vertebral rotation in idiopathic scoliosis," *J. Bone Joint Surg.*, 1989, vol. 78(B), pp. 252-255.
- [18] T.R. Nelson, D.H. Pretorius, "Three-dimensional ultrasound imaging," *Ultrasound Med. Biol.*, 1998, vol. 24, pp.1243-1270.
- [19] A. Fenster, D.B. Downey, H.N. Cardinal, "Three-dimensional ultrasound imaging," *Phys. Med. Biol.* 2001, vol. 46, pp. R67-R99.
- [20] Q.H. Huang, Y.P. Zheng YP, M.H. Lu, Z.R. Chi, "Development of a portable 3D ultrasound imaging system for musculoskeletal tissues," *Ultrasonics*, 2005, vol. 43, pp.153-163.
- [21] C. Goldberg, M. Kaliszer, D.P. Moore, E.E. Fogarty, F.E. Dowling, "Surface topography, Cobb angles, and cosmetic change in scoliosis," *Spine* 2001, vol. 26, no. 4, pp. E55-EE63.
- [22] P. Knott, S. Mardjetko, D. Nance, M. Dunn. *Electromagnetic Topographical Technique of Curve Evaluation for Adolescent Idiopathic Scoliosis*. *Spine* 2006; vol. 31, no. 24: pp. E911-E915