

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB3026 2/3 3min 800C 3C/m 1h B 2x1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-048930-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

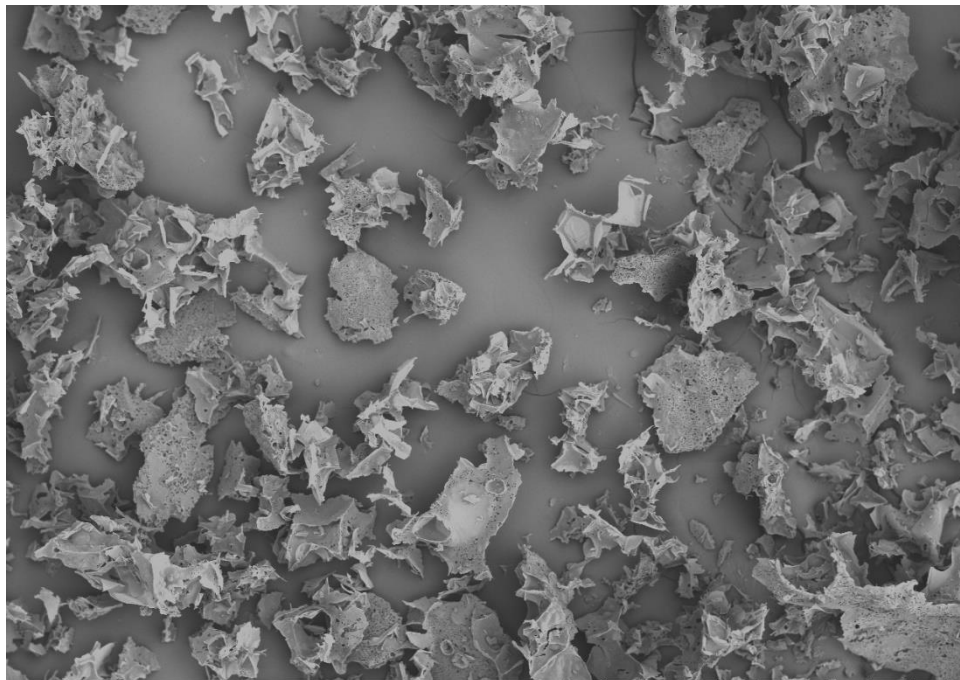

Clariant SU7000 5.00kV 4.9mm x100 UD+LD+MD 01/13/2025 500µm

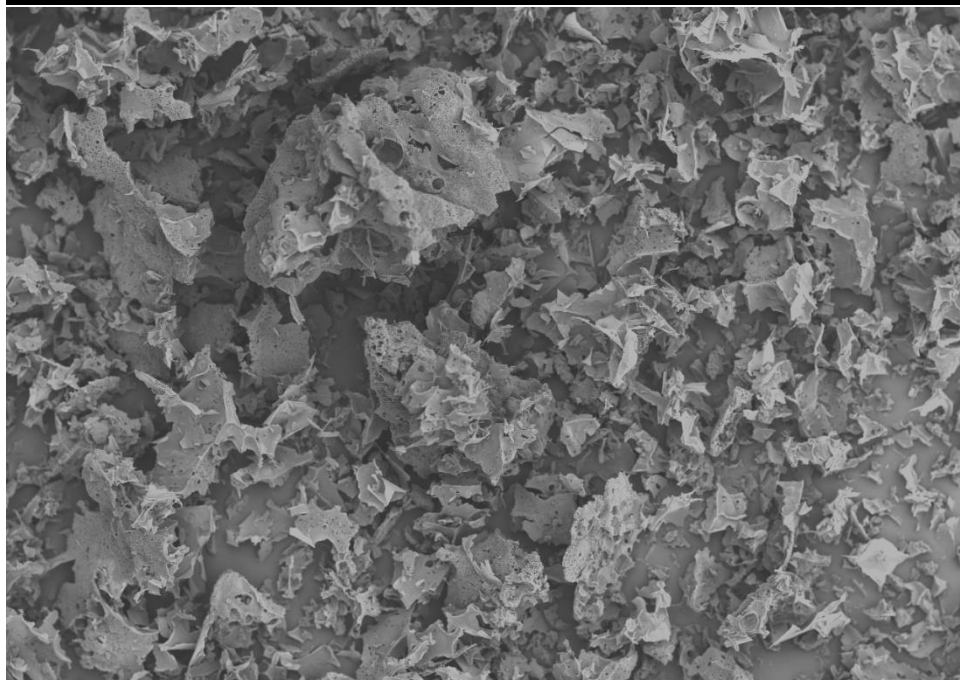

Clariant SU7000 5.00kV 4.9mm x100 UD+LD+MD 01/13/2025 500µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB3026 2/3 3min 800C 3C/m 1h B 2x1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-048930-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

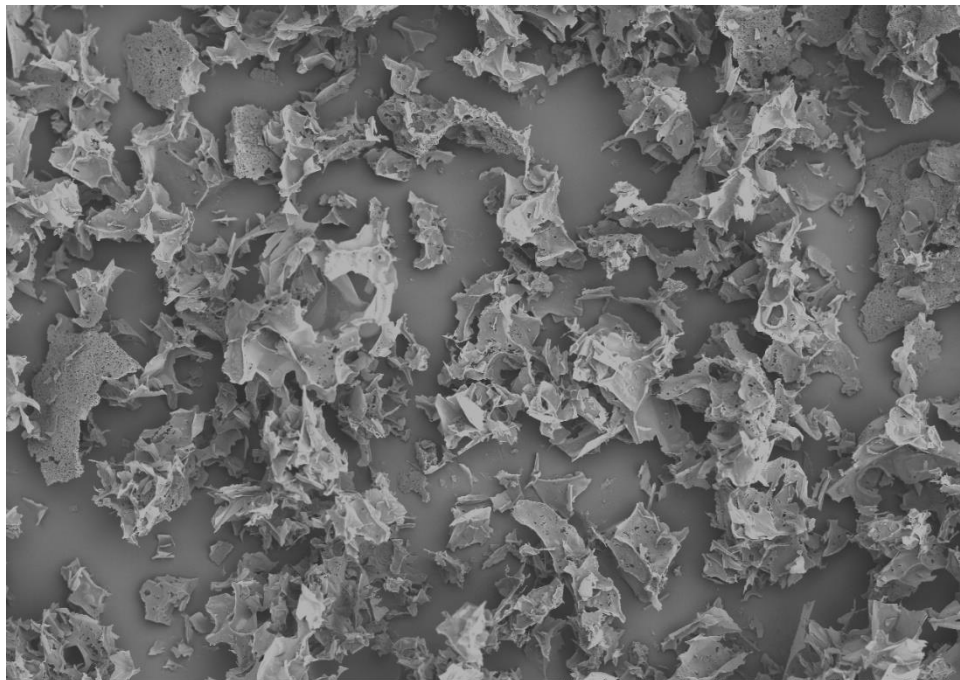

Clariant SU7000 5.00kV 4.9mm x100 UD+LD+MD 01/13/2025 500µm

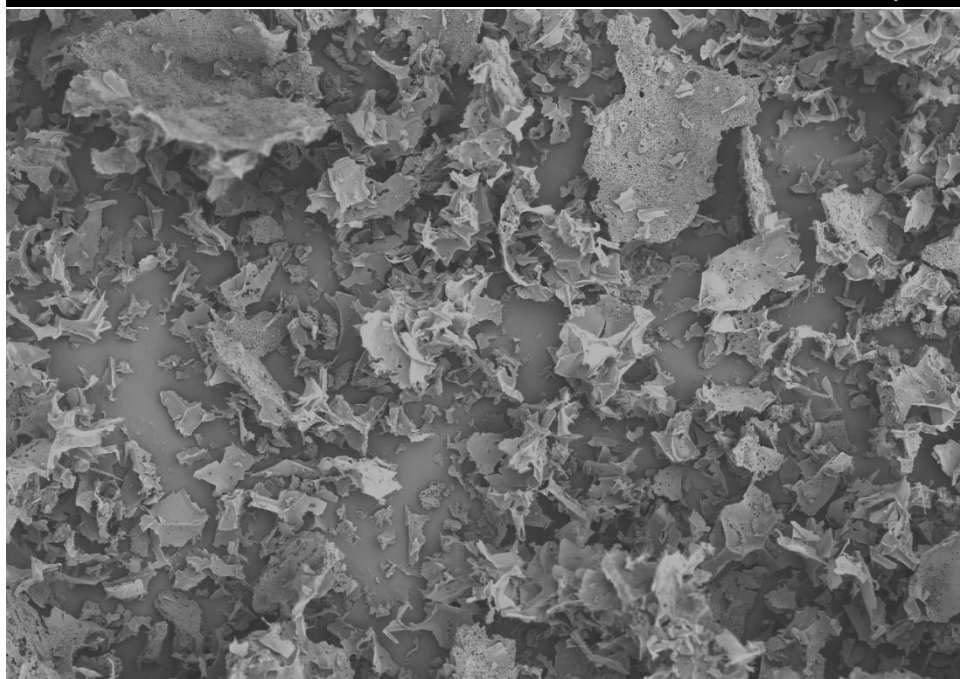

Clariant SU7000 5.00kV 5.0mm x100 UD+LD+MD 01/13/2025 500µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB3026 2/3 3min 800C 3C/m 1h B 2x1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-048930-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

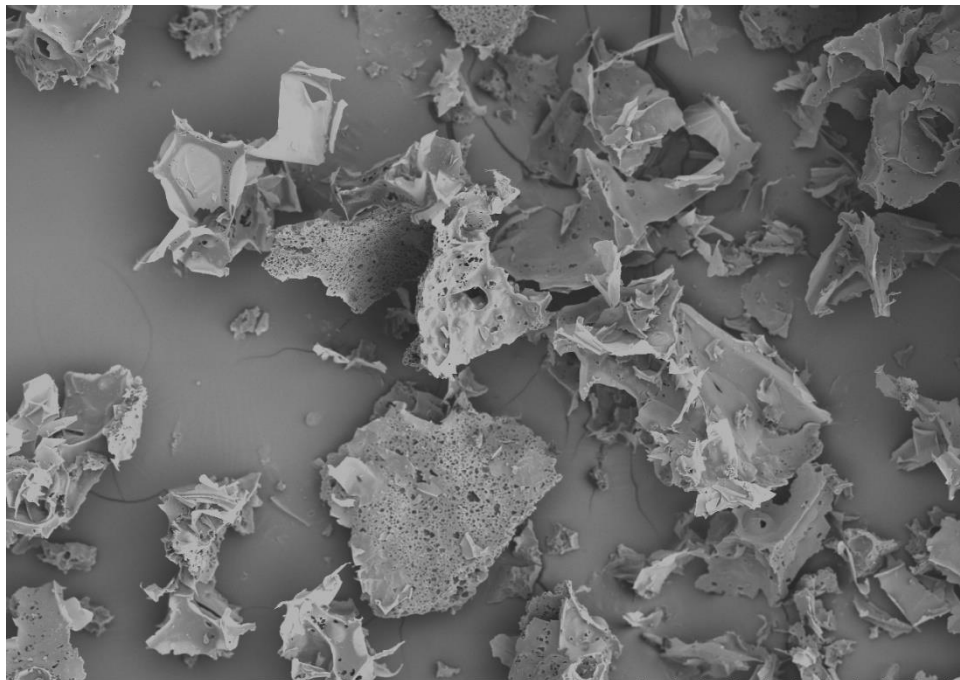

Clariant SU7000 5.00kV 4.9mm x200 UD+LD+MD 01/13/2025 200µm

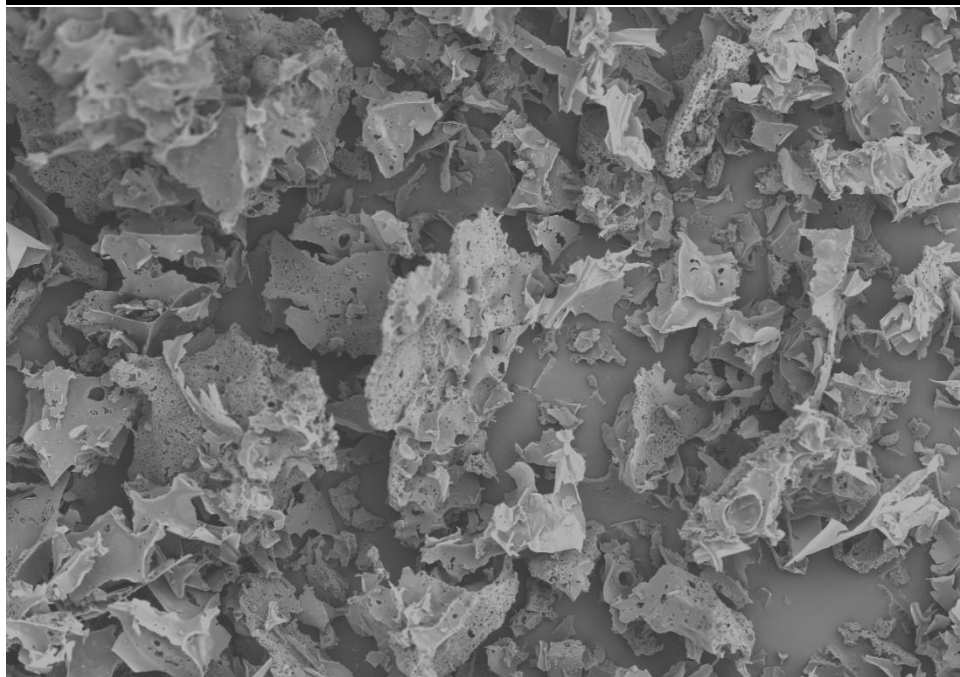

Clariant SU7000 5.00kV 5.0mm x200 UD+LD+MD 01/13/2025 200µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB3026 2/3 3min 800C 3C/m 1h B 2x1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-048930-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

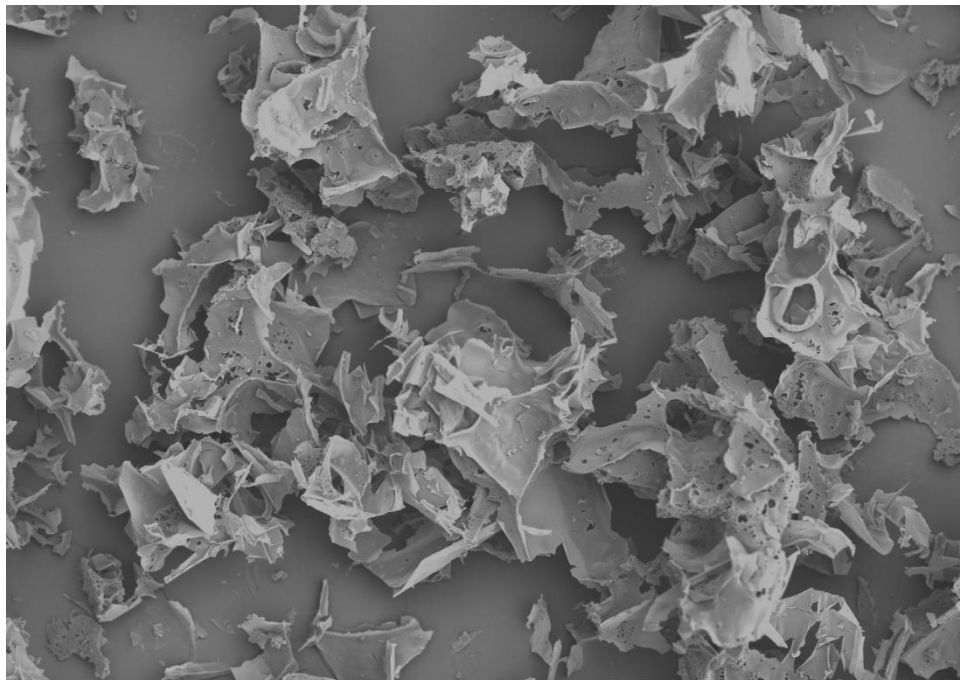

Clariant SU7000 5.00kV 4.9mm x200 UD+LD+MD 01/13/2025 200µm

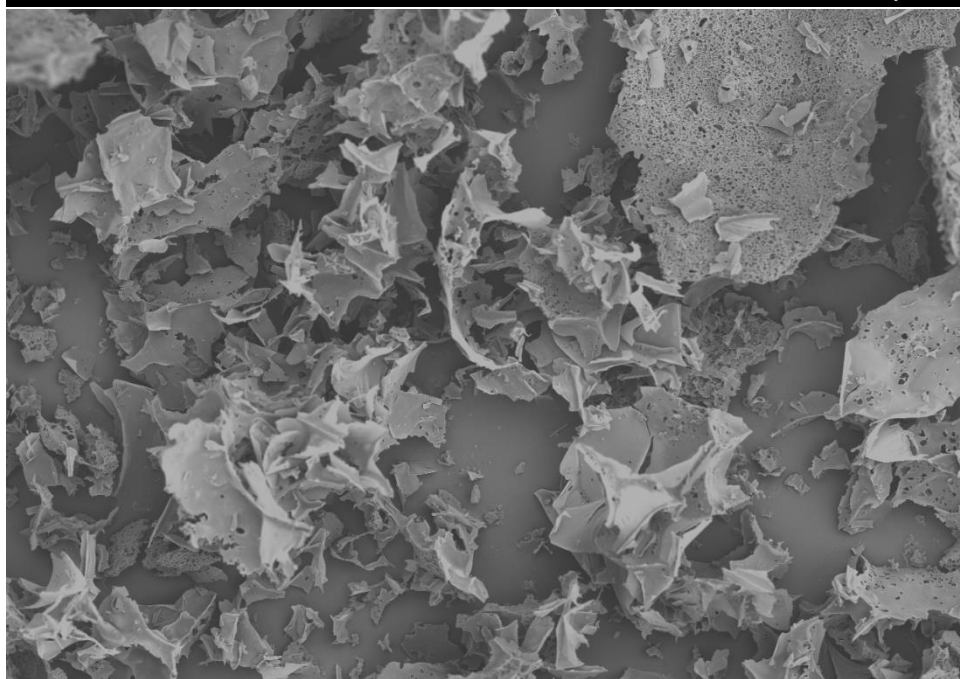

Clariant SU7000 5.00kV 5.0mm x200 UD+LD+MD 01/13/2025 200µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB3026 2/3 3min 800C 3C/m 1h B 2x1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-048930-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

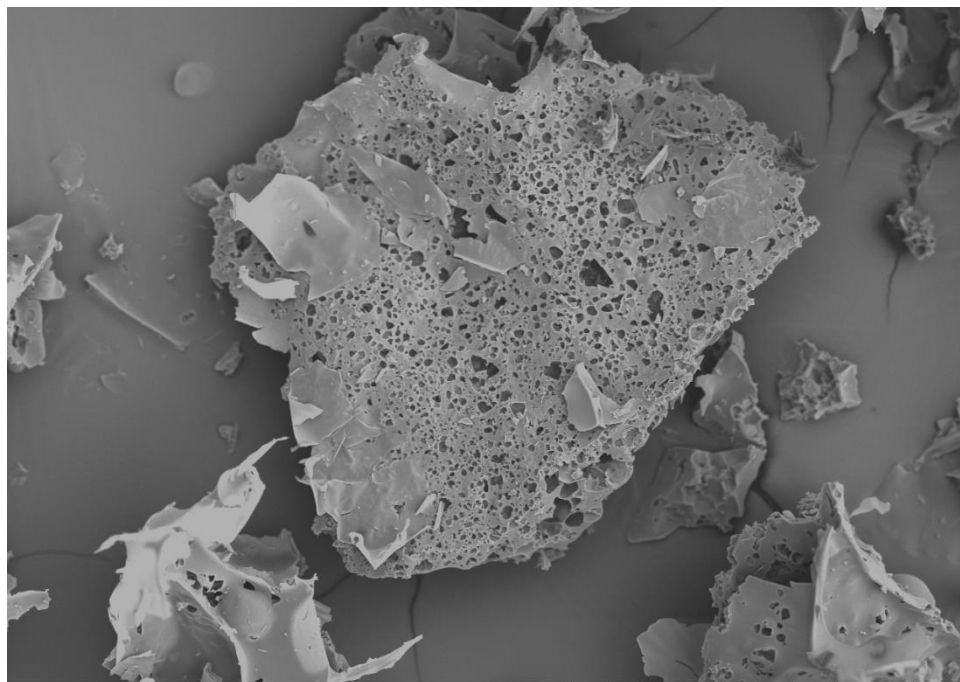

Clariant SU7000 5.00kV 4.9mm x500 UD+LD+MD 01/13/2025 100µm

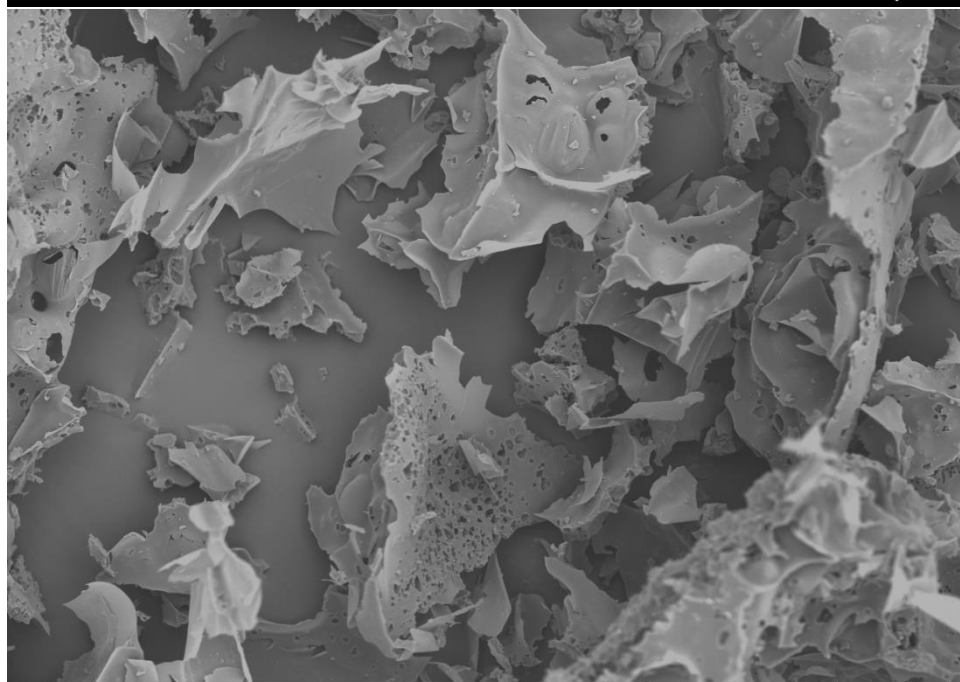

Clariant SU7000 5.00kV 5.0mm x500 UD+LD+MD 01/13/2025 100µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB3026 2/3 3min 800C 3C/m 1h B 2x1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-048930-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

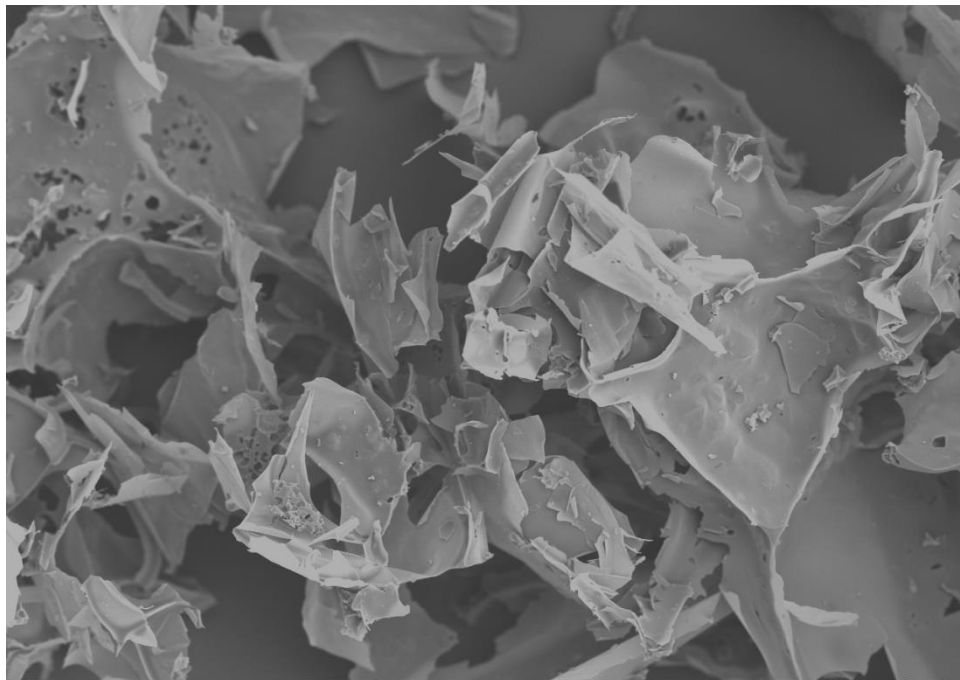

Clariant SU7000 5.00kV 4.9mm x500 UD+LD+MD 01/13/2025 100µm

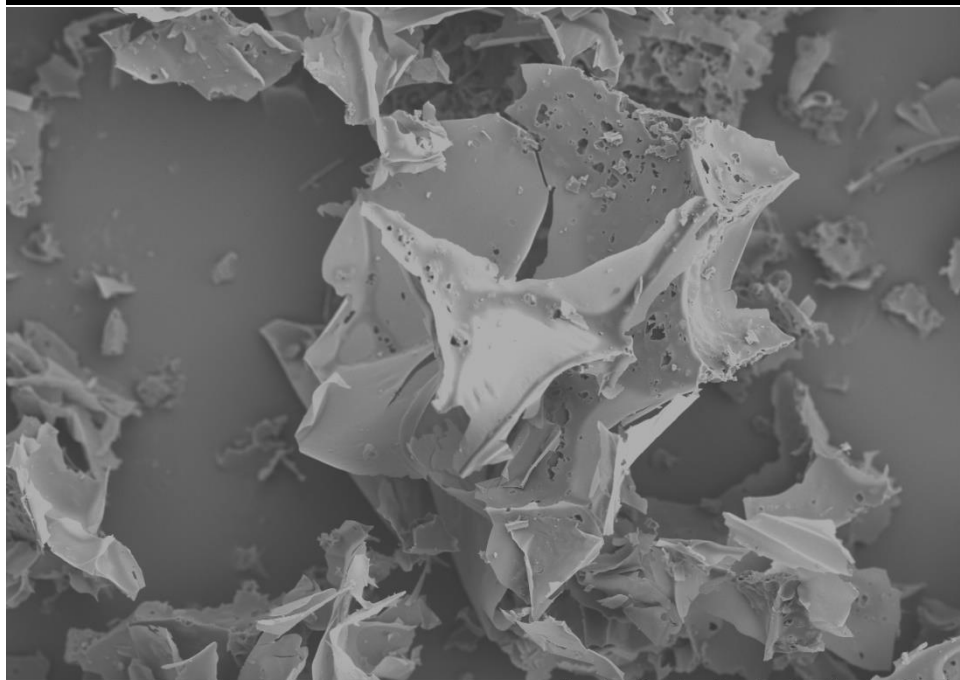

Clariant SU7000 5.00kV 4.9mm x500 UD+LD+MD 01/13/2025 100µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB3026 2/3 3min 800C 3C/m 1h B 2x1.3P

Ordering customer: Dr. Torsten Busch

Dept./Plant: Curia Germany GmbH

Order number: 25-048930-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

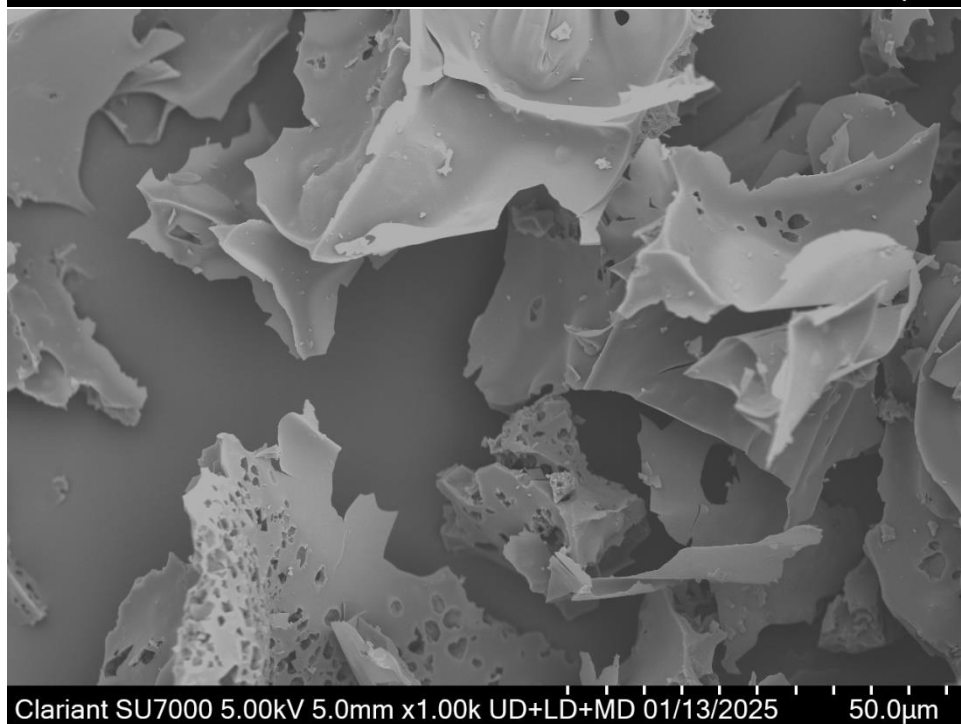

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB3026 2/3 3min 800C 3C/m 1h B 2x1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-048930-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

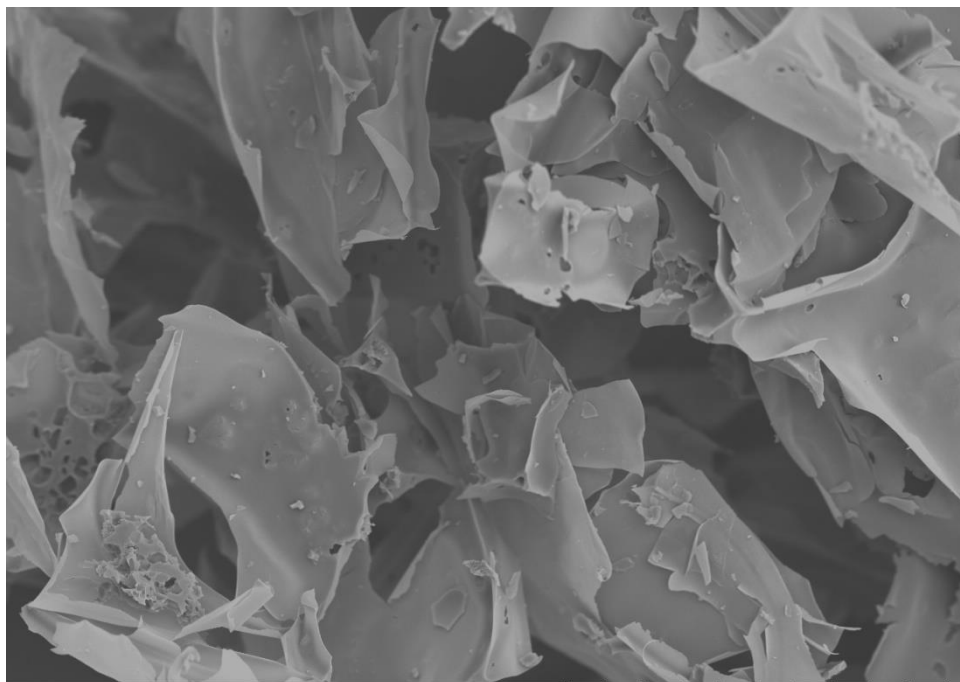

Clariant SU7000 5.00kV 4.9mm x1.00k UD+LD+MD 01/13/2025 50.0µm

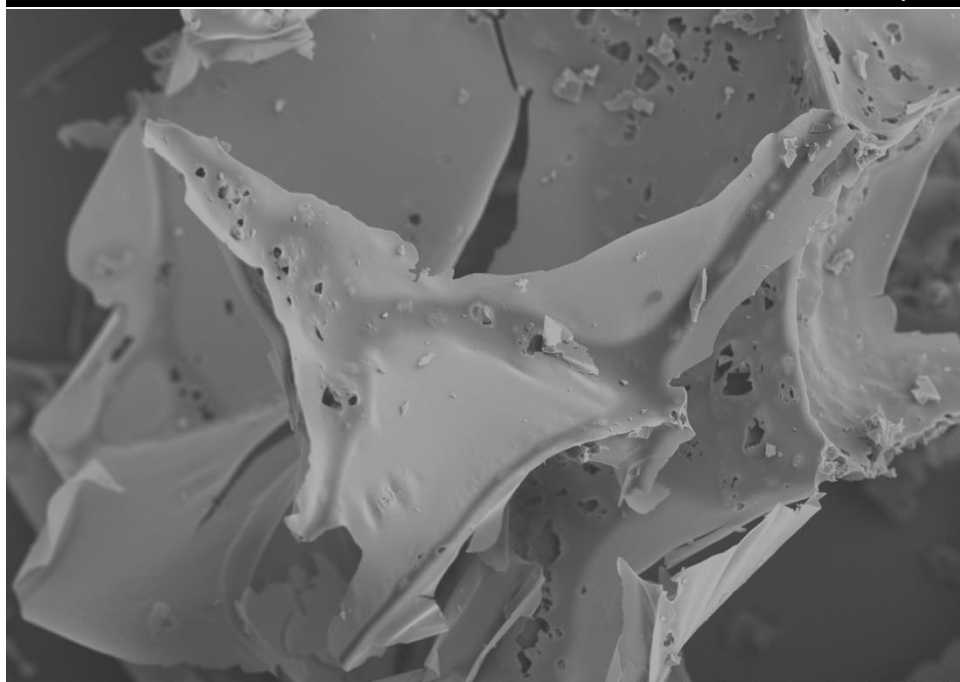

Clariant SU7000 5.00kV 4.9mm x1.00k UD+LD+MD 01/13/2025 50.0µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB3026 2/3 3min 800C 3C/m 1h B 2x1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-048930-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

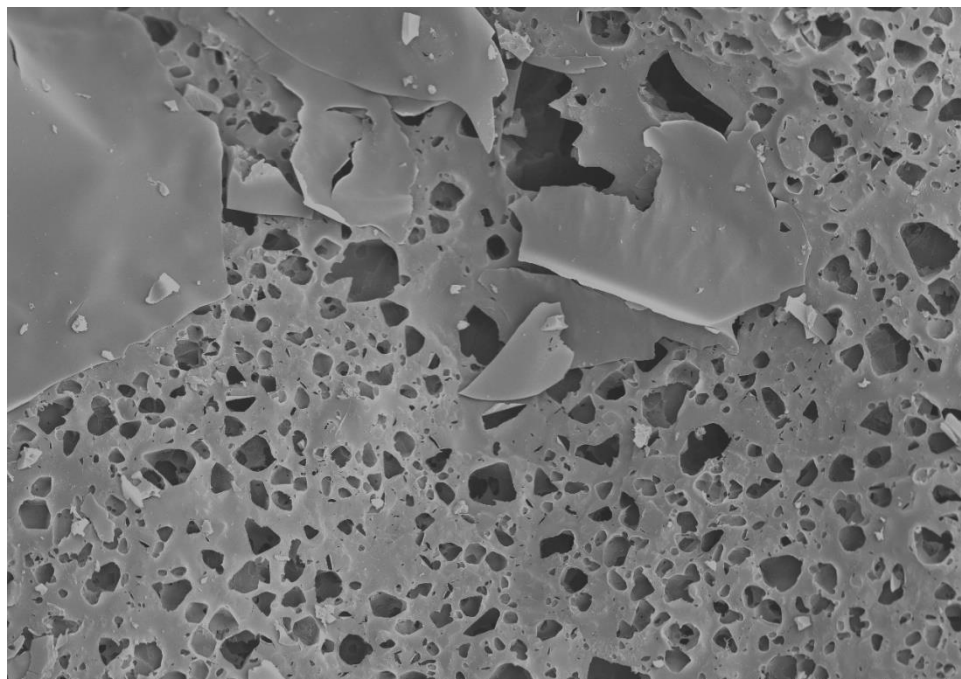

Clariant SU7000 5.00kV 5.0mm x2.00k UD+LD+MD 01/13/2025 20.0µm

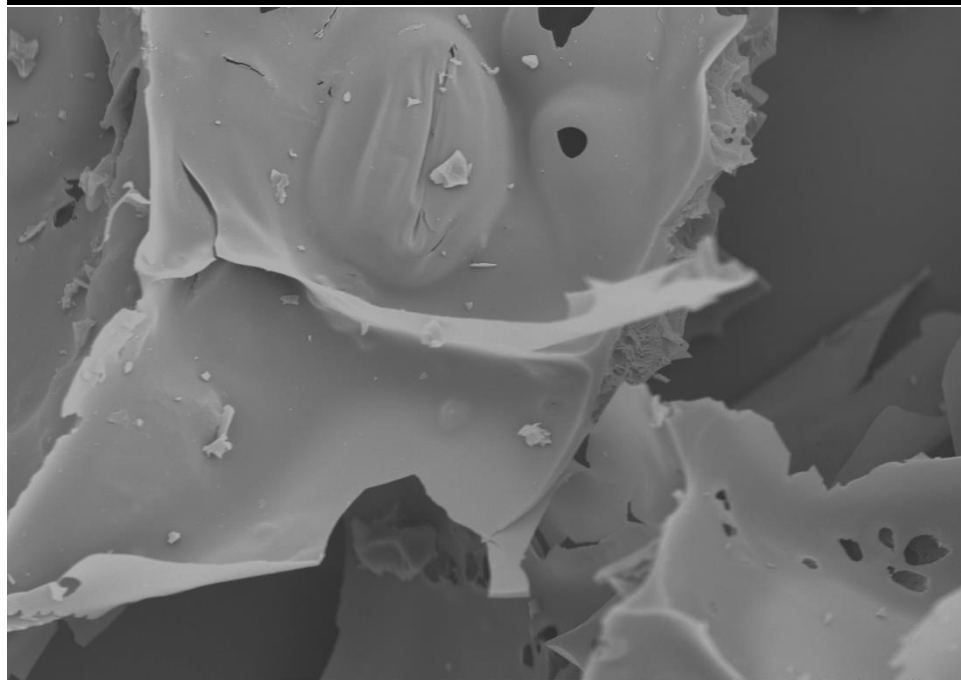

Clariant SU7000 5.00kV 5.0mm x2.00k UD+LD+MD 01/13/2025 20.0µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB3026 2/3 3min 800C 3C/m 1h B 2x1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-048930-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

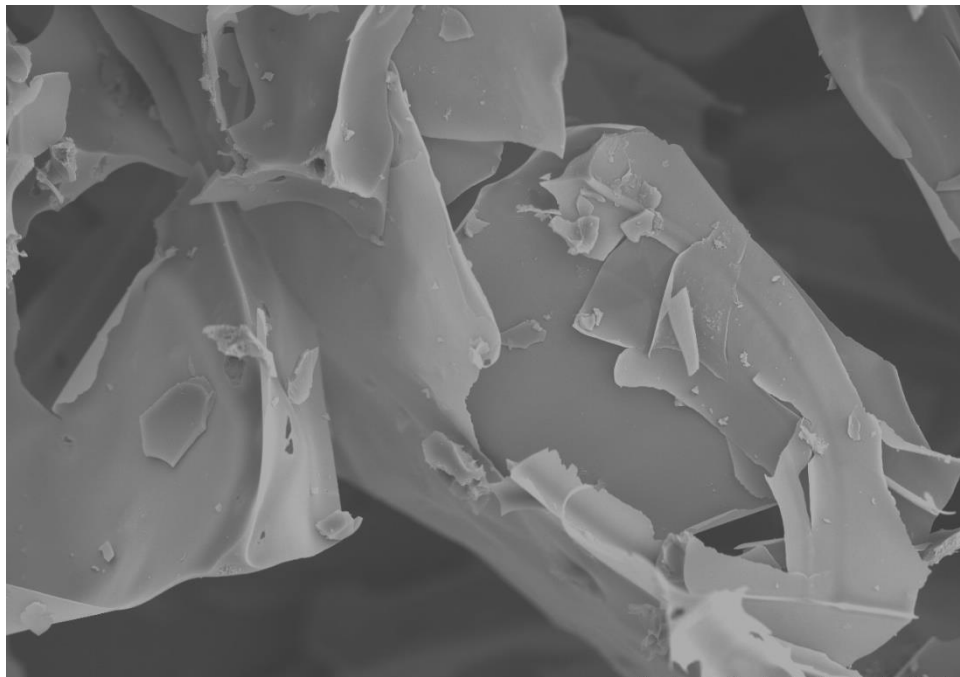

Clariant SU7000 5.00kV 4.9mm x2.00k UD+LD+MD 01/13/2025 20.0µm

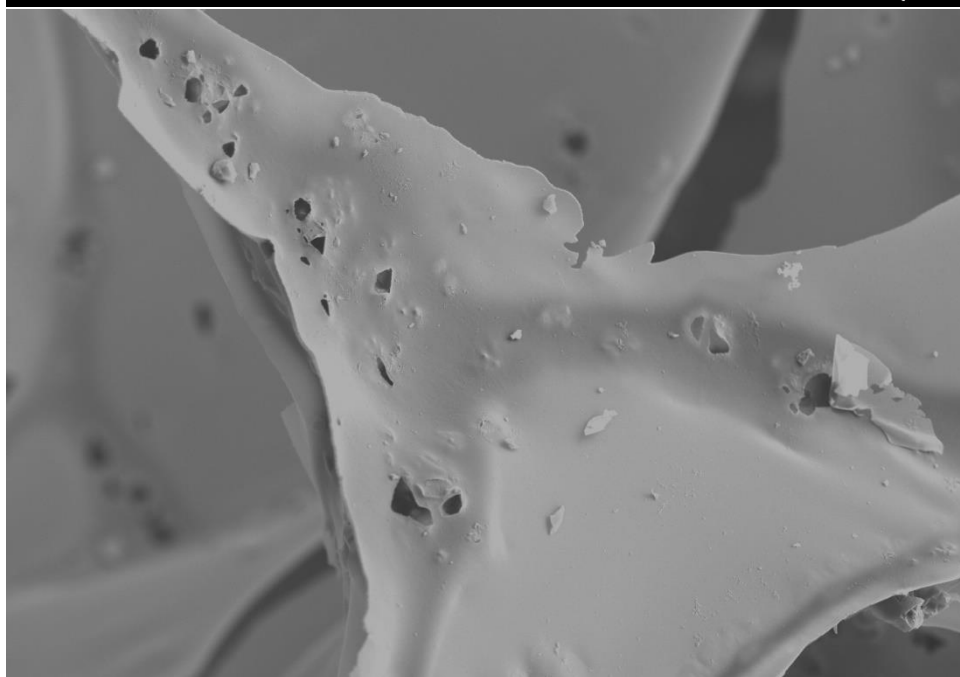


Clariant SU7000 5.00kV 4.9mm x2.00k UD+LD+MD 01/13/2025 20.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB3026 2/3 3min 800C 3C/m 1h B 2x1.3P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 25-048930-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

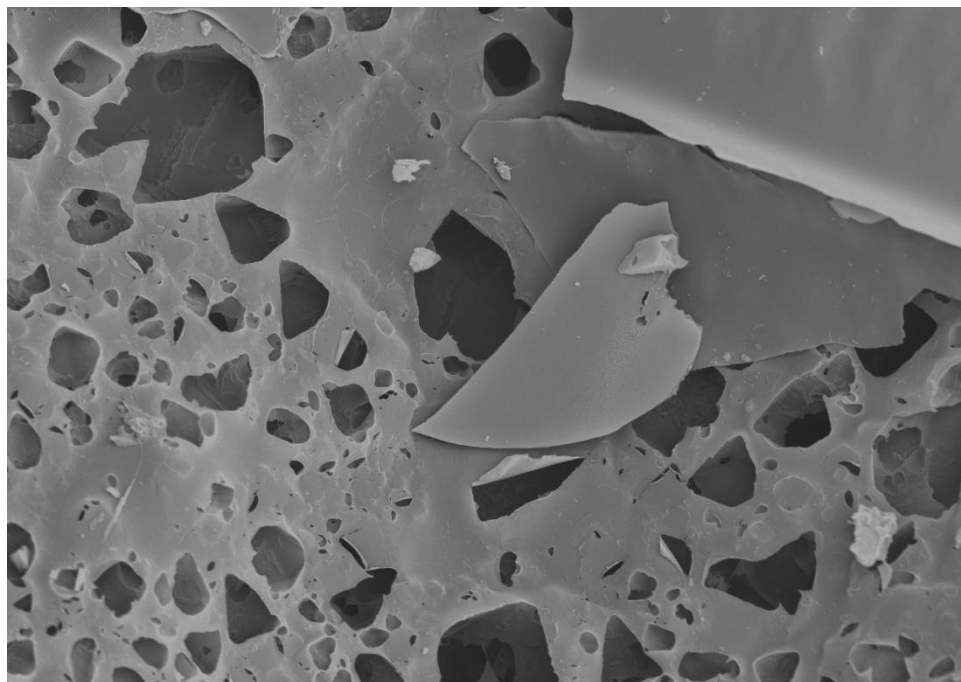

Clariant SU7000 5.00kV 5.0mm x5.00k UD+LD+MD 01/13/2025 10.0µm

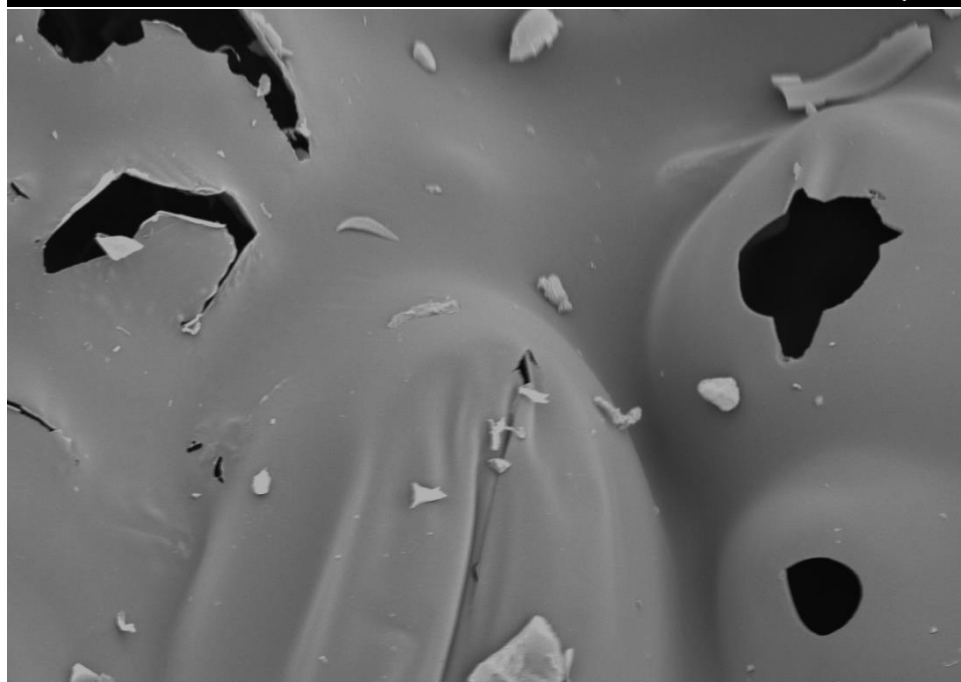

Clariant SU7000 5.00kV 5.0mm x5.00k UD+LD+MD 01/13/2025 10.0µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB3026 2/3 3min 800C 3C/m 1h B 2x1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-048930-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

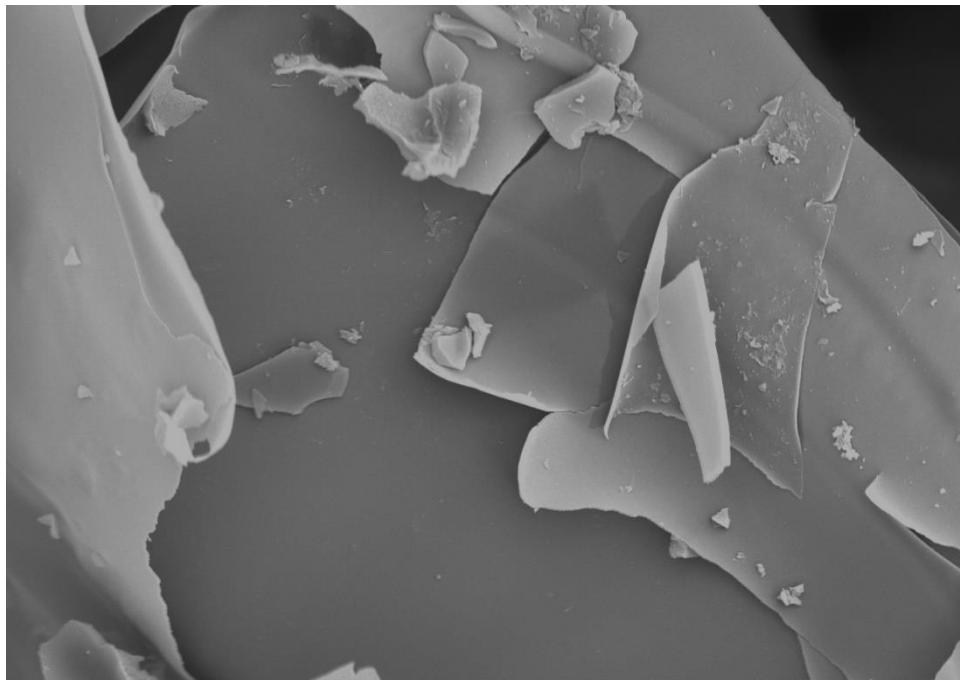

Clariant SU7000 5.00kV 4.9mm x5.00k UD+LD+MD 01/13/2025 10.0µm

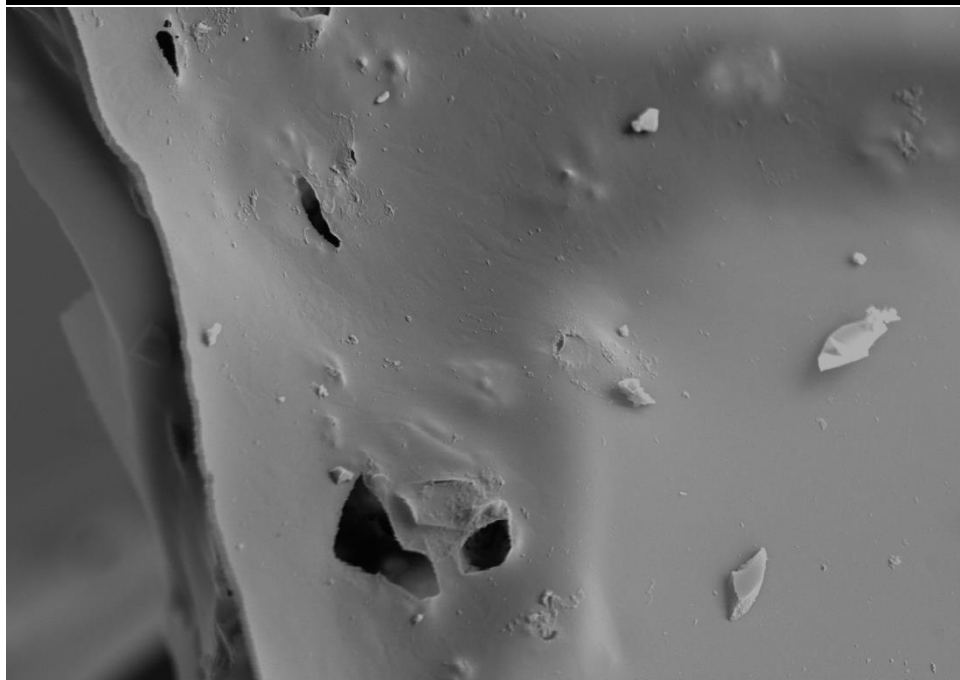

Clariant SU7000 5.00kV 4.9mm x5.00k UD+LD+MD 01/13/2025 10.0µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB3026 2/3 3min 800C 3C/m 1h B 2x1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-048930-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

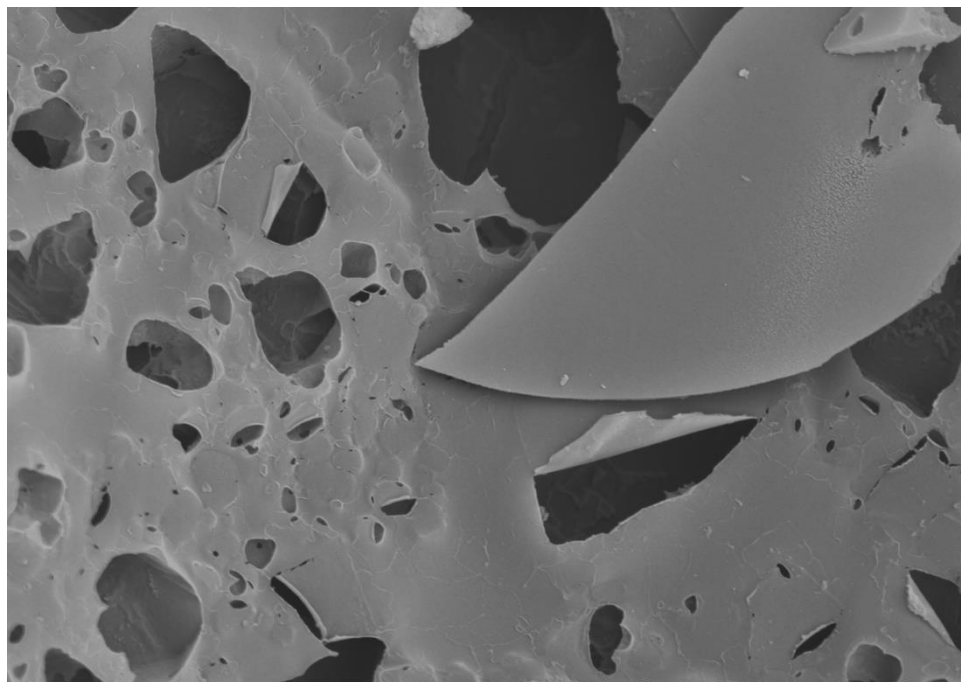

Clariant SU7000 5.00kV 5.0mm x10.0k UD+LD+MD 01/13/2025 5.00µm

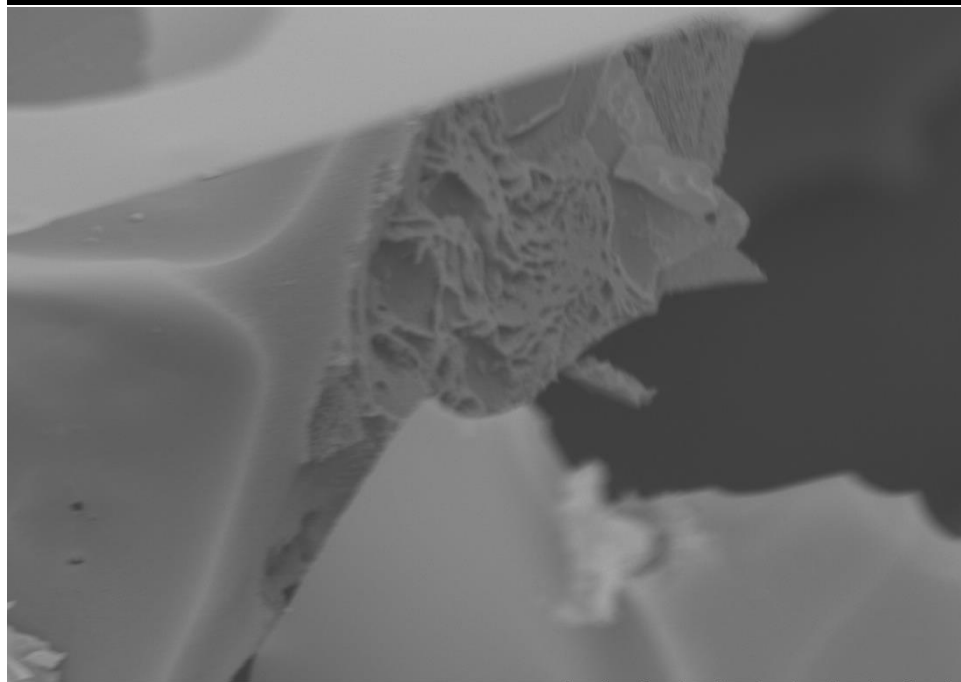

Clariant SU7000 5.00kV 5.0mm x10.0k UD+LD+MD 01/13/2025 5.00µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB3026 2/3 3min 800C 3C/m 1h B 2x1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-048930-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

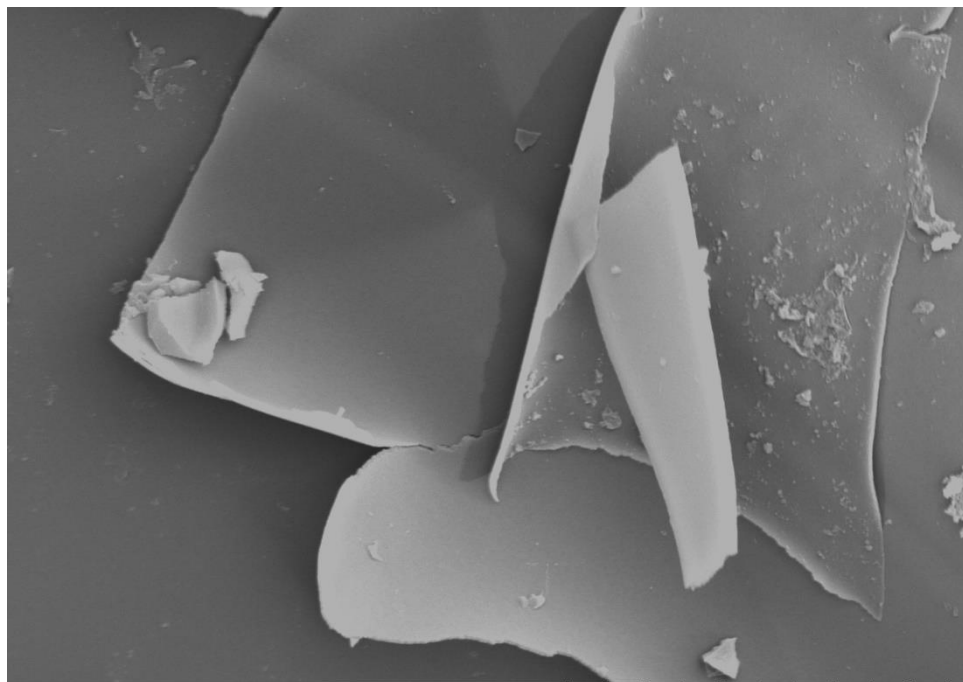

Clariant SU7000 5.00kV 4.9mm x10.0k UD+LD+MD 01/13/2025 5.00μm

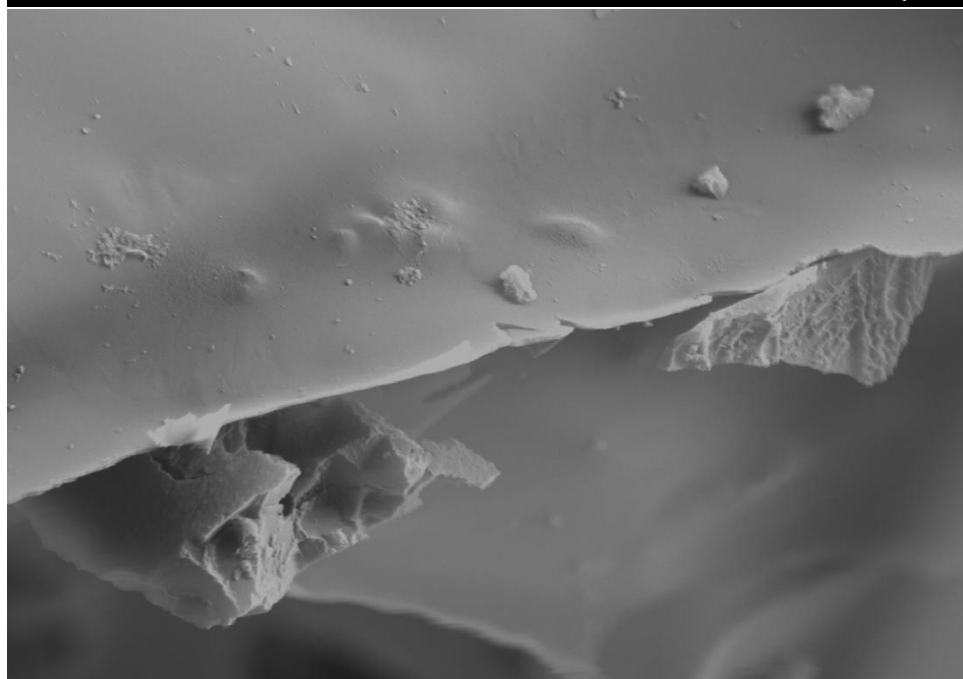

Clariant SU7000 5.00kV 4.9mm x10.0k UD+LD+MD 01/13/2025 5.00μm

SCANNING ELECTRON MICROSCOPE (SEM)



Sample name: MB3026 2/3 3min 800C 3C/m 1h B 2x1.3P

Ordering customer: Dr. Torsten Busch

Dept./Plant: Curia Germany GmbH

Order number: 25-048930-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

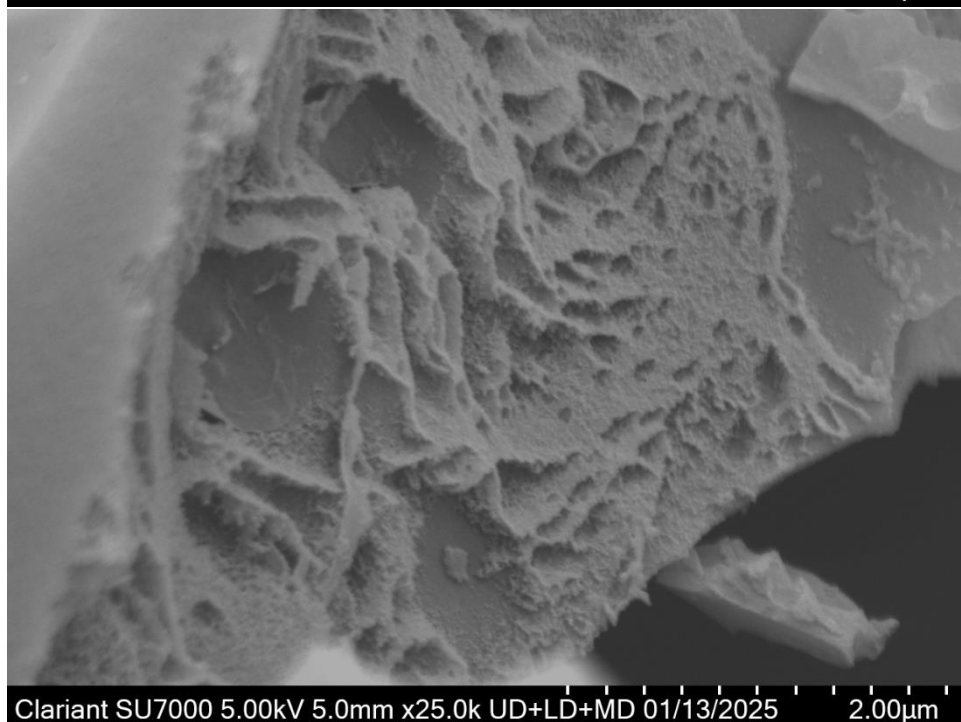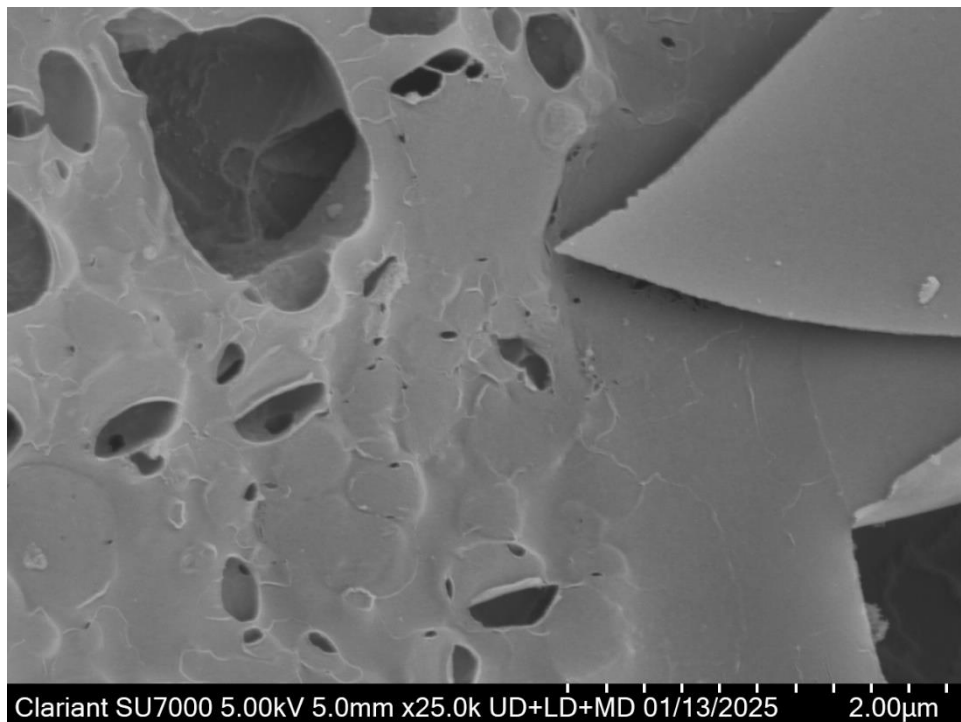

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: MB3026 2/3 3min 800C 3C/m 1h B 2x1.3P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 25-048930-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

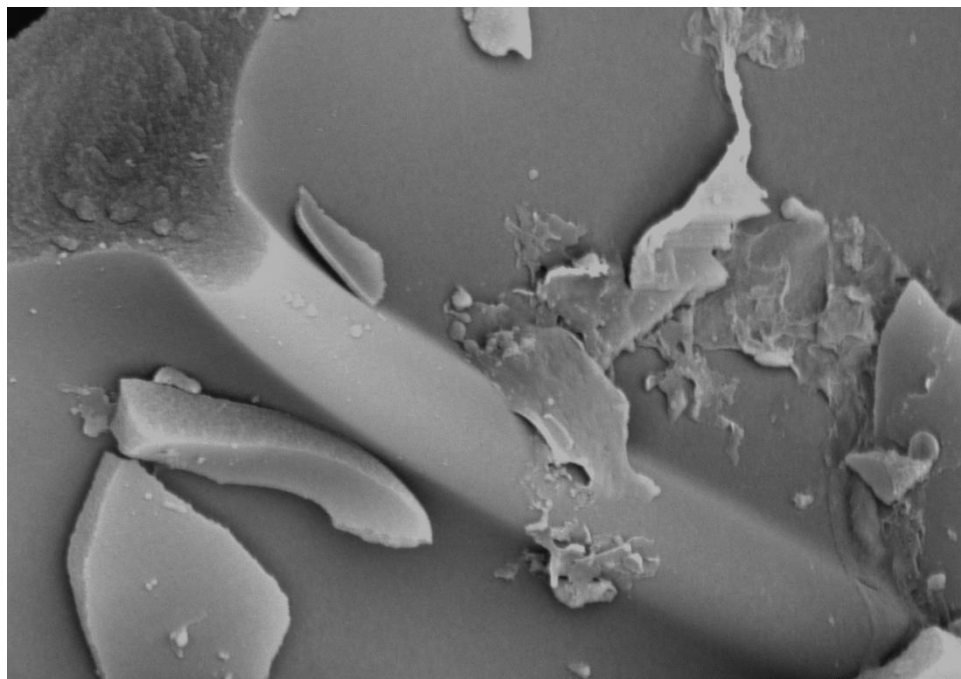

Clariant SU7000 5.00kV 4.9mm x25.0k UD+LD+MD 01/13/2025 2.00µm

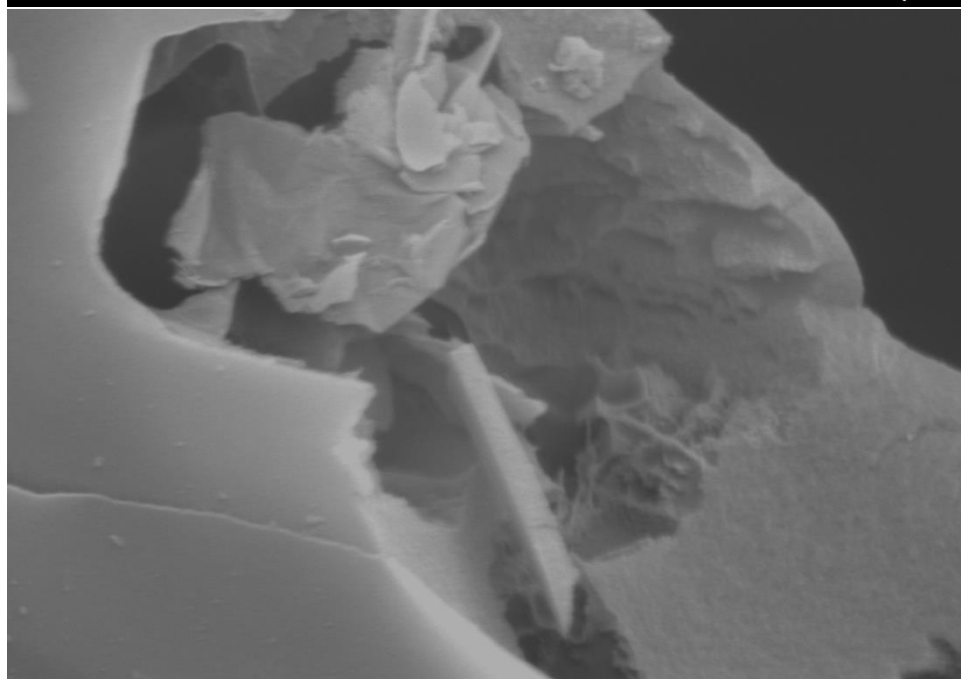

Clariant SU7000 5.00kV 5.0mm x25.0k UD+LD+MD 01/13/2025 2.00µm