



## SCANNING ELECTRON MICROSCOPE (SEM)

**Sample name:** MB3017B 2/3 20% NaOH 35Hz10min 800C 3C/m 1h B 2.6np  
**Ordering customer:** Dr. Torsten Busch  
**Dept./Plant:** Curia Germany GmbH  
**Order number:** 24-048601-2

**Sample treatment:** The sample was subjected to platinum sputter coating and then measured.

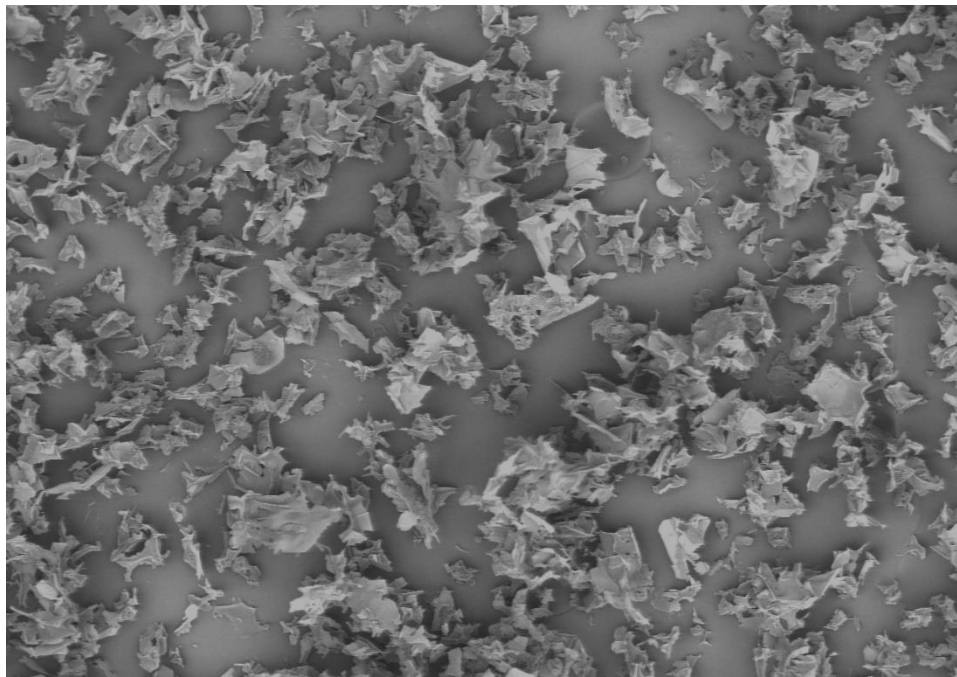

Clariant SU7000 5.00kV 6.6mm x100 UD+LD+MD 11/18/2024 500µm

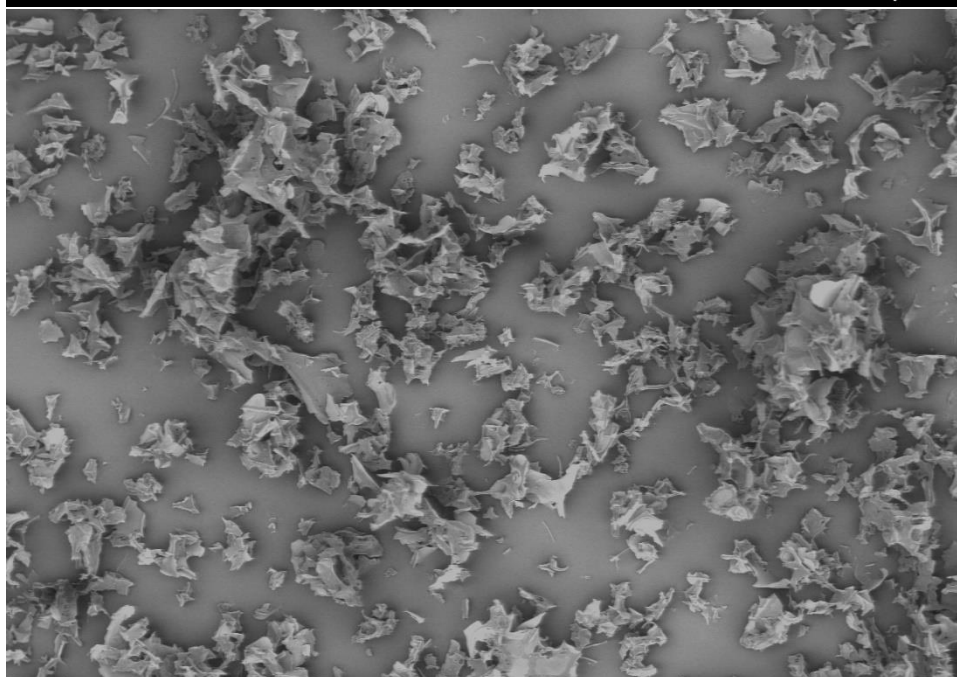


Clariant SU7000 5.00kV 6.5mm x100 UD+LD+MD 11/18/2024 500µm


## SCANNING ELECTRON MICROSCOPE (SEM)

**Sample name:** MB3017B 2/3 20% NaOH 35Hz10min 800C 3C/m 1h B 2.6np  
**Ordering customer:** Dr. Torsten Busch  
**Dept./Plant:** Curia Germany GmbH  
**Order number:** 24-048601-2

**Sample treatment:** The sample was subjected to platinum sputter coating and then measured.

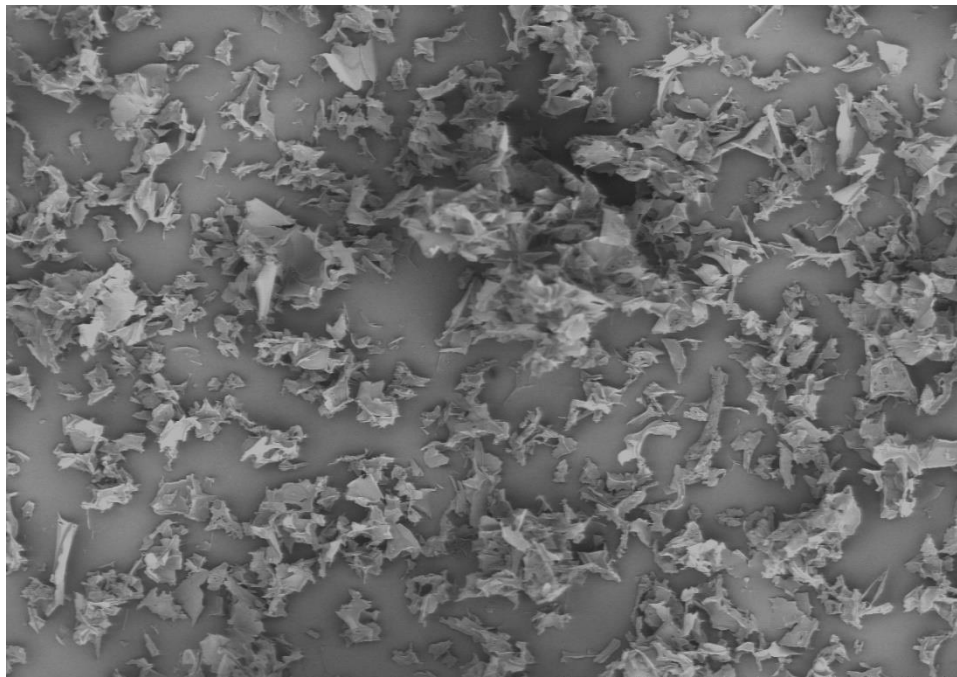

Clariant SU7000 5.00kV 6.5mm x100 UD+LD+MD 11/18/2024 500µm

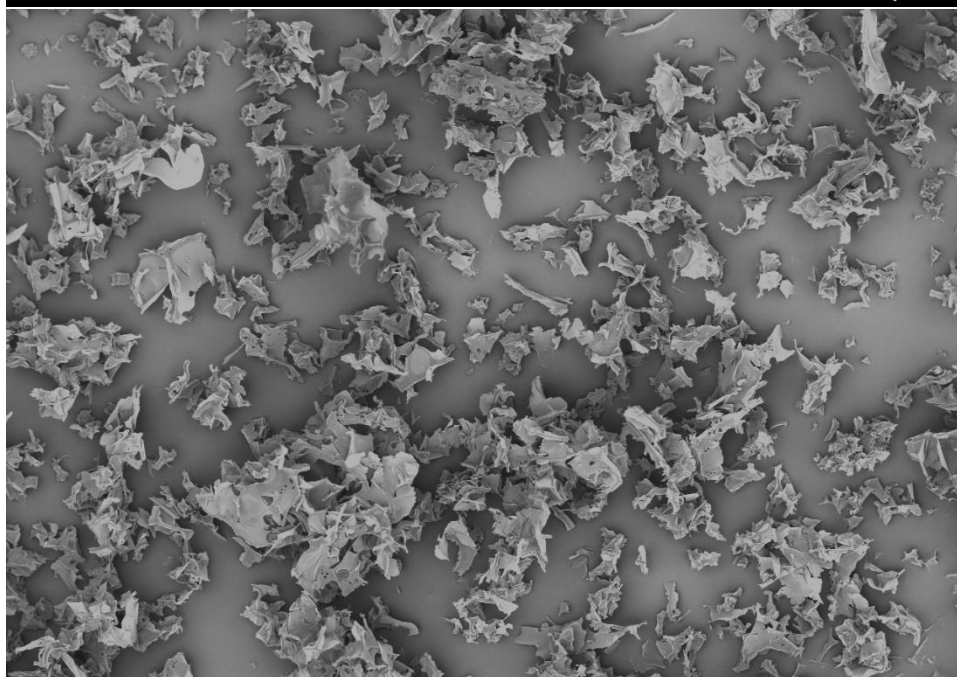


Clariant SU7000 5.00kV 6.5mm x100 UD+LD+MD 11/18/2024 500µm


## SCANNING ELECTRON MICROSCOPE (SEM)

**Sample name:** MB3017B 2/3 20% NaOH 35Hz10min 800C 3C/m 1h B 2.6np  
**Ordering customer:** Dr. Torsten Busch  
**Dept./Plant:** Curia Germany GmbH  
**Order number:** 24-048601-2

**Sample treatment:** The sample was subjected to platinum sputter coating and then measured.

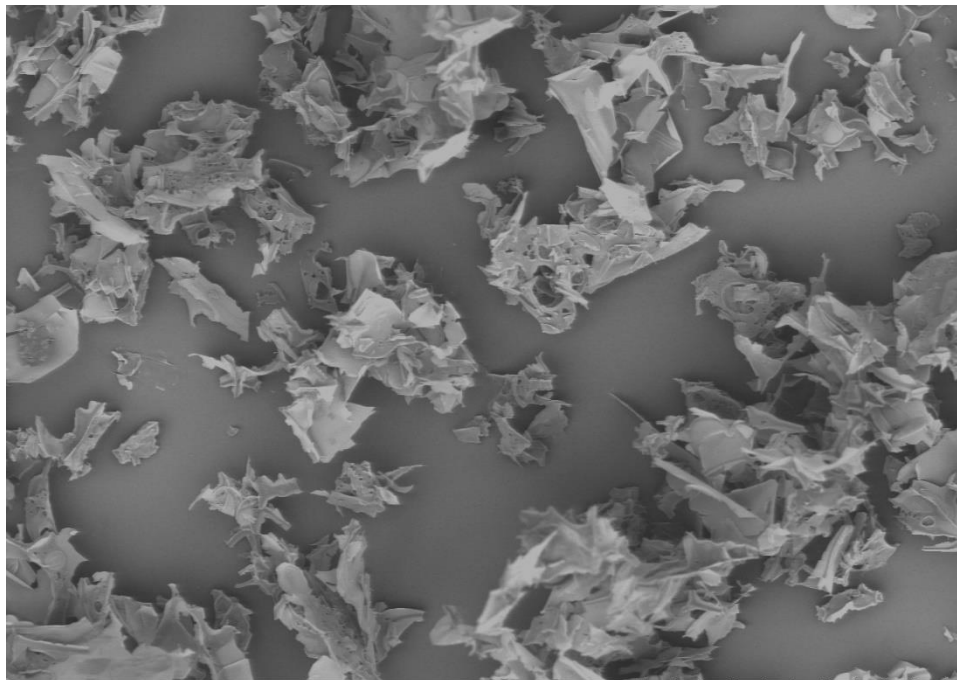

Clariant SU7000 5.00kV 6.6mm x200 UD+LD+MD 11/18/2024 200µm

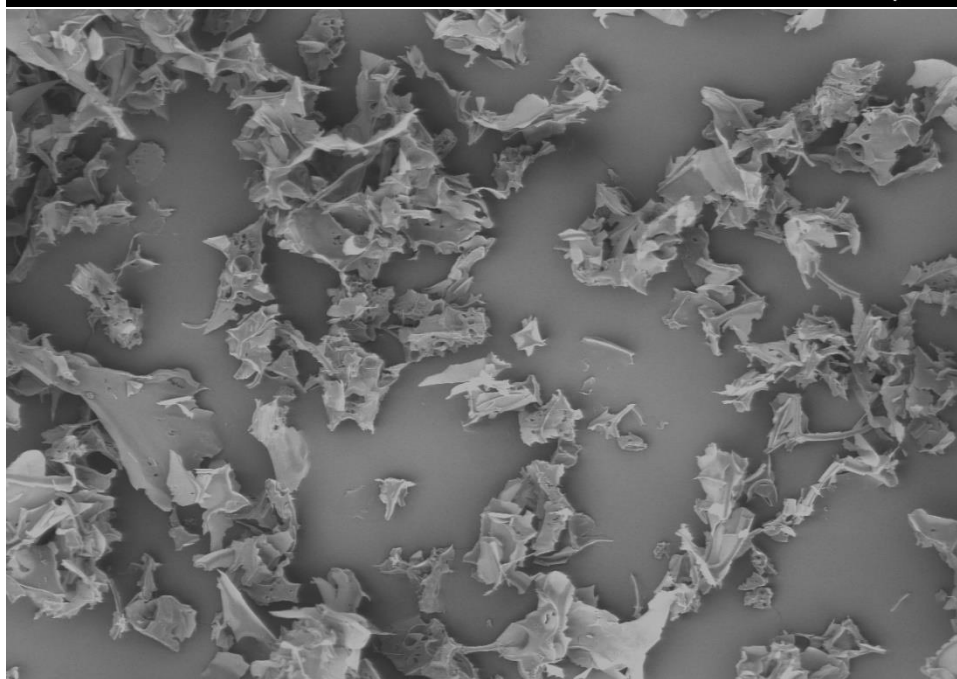


Clariant SU7000 5.00kV 6.5mm x200 UD+LD+MD 11/18/2024 200µm


## SCANNING ELECTRON MICROSCOPE (SEM)

**Sample name:** MB3017B 2/3 20% NaOH 35Hz10min 800C 3C/m 1h B 2.6np  
**Ordering customer:** Dr. Torsten Busch  
**Dept./Plant:** Curia Germany GmbH  
**Order number:** 24-048601-2

**Sample treatment:** The sample was subjected to platinum sputter coating and then measured.

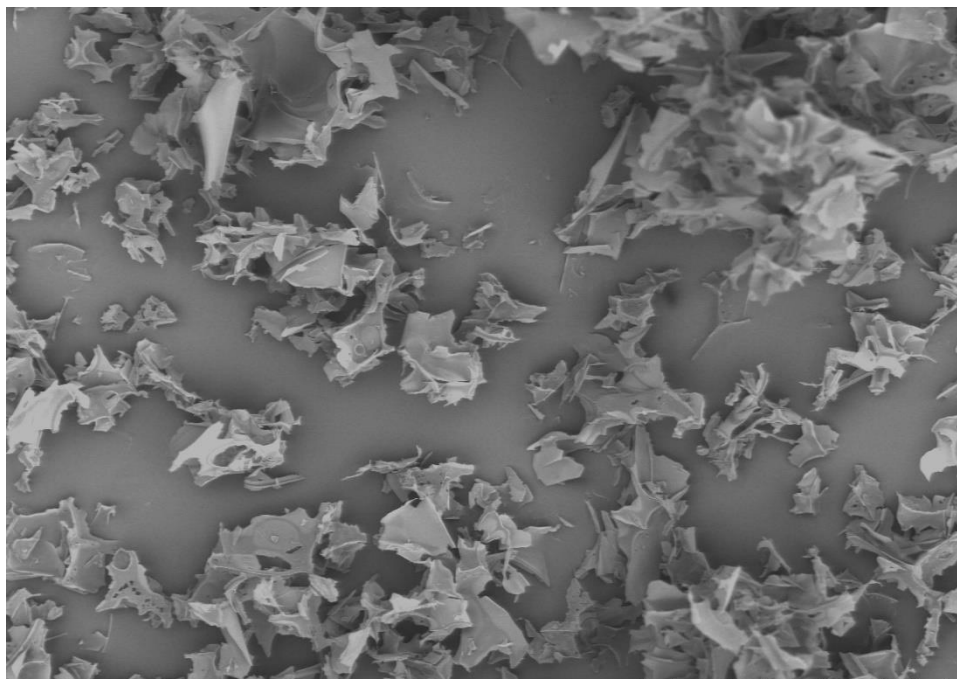

Clariant SU7000 5.00kV 6.5mm x200 UD+LD+MD 11/18/2024 200µm

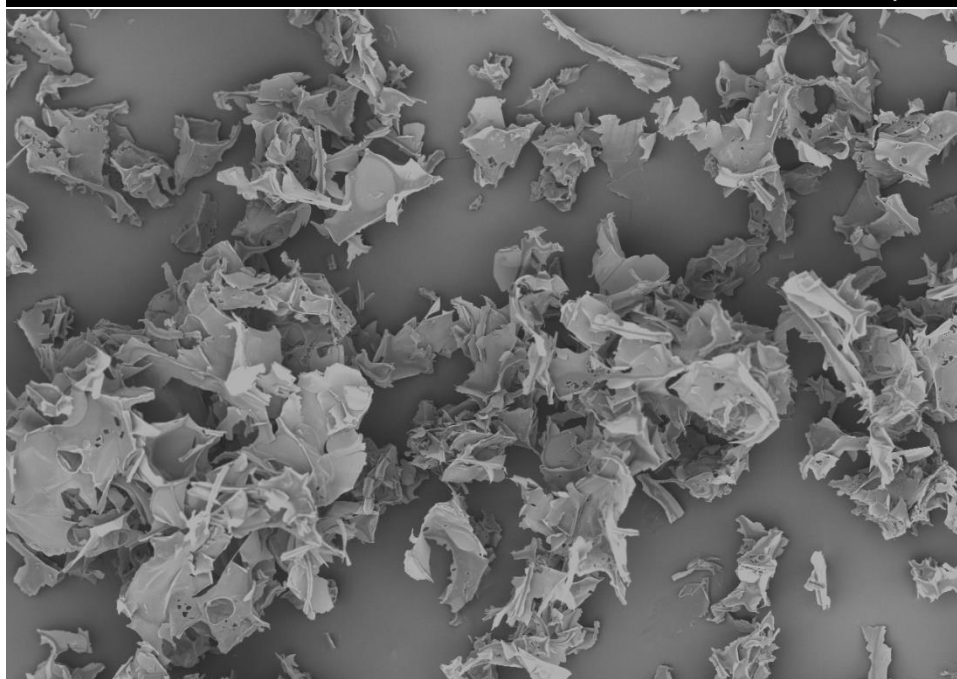


Clariant SU7000 5.00kV 6.5mm x200 UD+LD+MD 11/18/2024 200µm


## SCANNING ELECTRON MICROSCOPE (SEM)

**Sample name:** MB3017B 2/3 20% NaOH 35Hz10min 800C 3C/m 1h B 2.6np  
**Ordering customer:** Dr. Torsten Busch  
**Dept./Plant:** Curia Germany GmbH  
**Order number:** 24-048601-2

**Sample treatment:** The sample was subjected to platinum sputter coating and then measured.

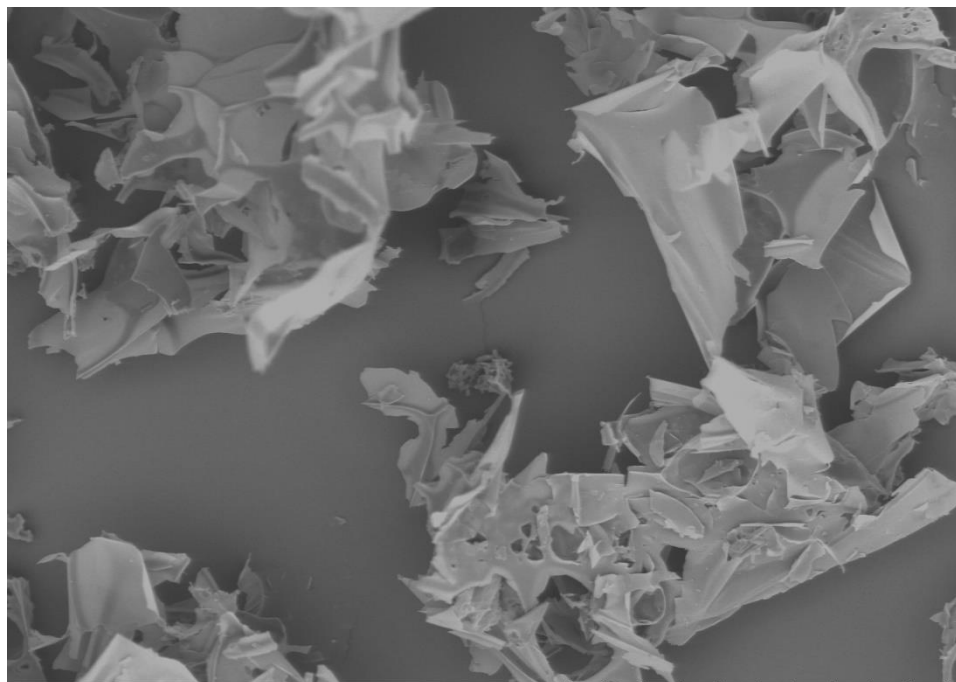

Clariant SU7000 5.00kV 6.6mm x500 UD+LD+MD 11/18/2024 100µm

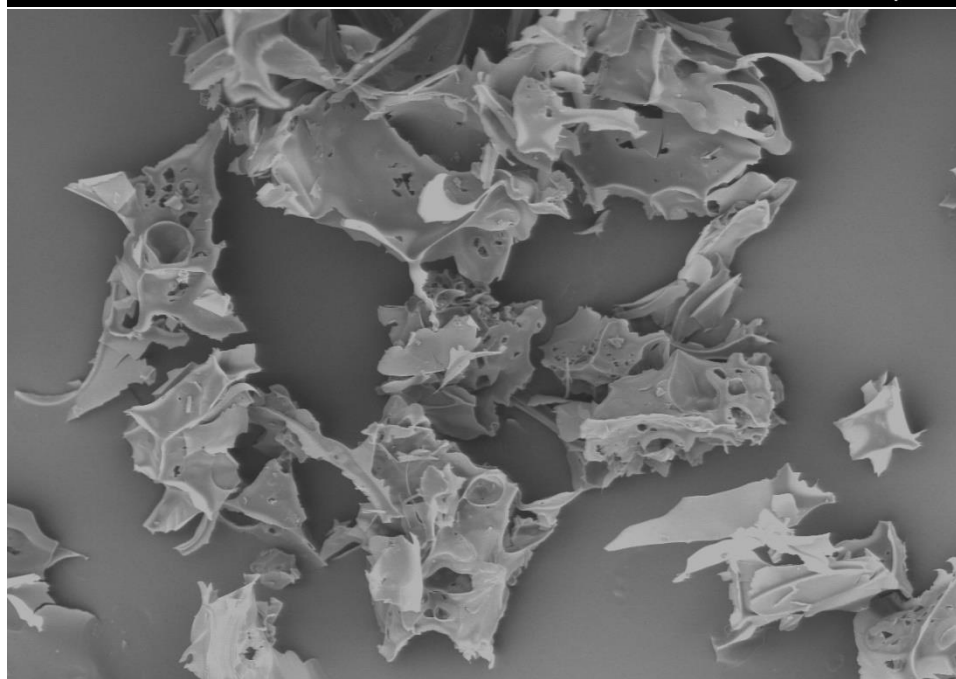


Clariant SU7000 5.00kV 6.5mm x500 UD+LD+MD 11/18/2024 100µm




## SCANNING ELECTRON MICROSCOPE (SEM)

**Sample name:** MB3017B 2/3 20% NaOH 35Hz10min 800C 3C/m 1h B 2.6np  
**Ordering customer:** Dr. Torsten Busch  
**Dept./Plant:** Curia Germany GmbH  
**Order number:** 24-048601-2

**Sample treatment:** The sample was subjected to platinum sputter coating and then measured.

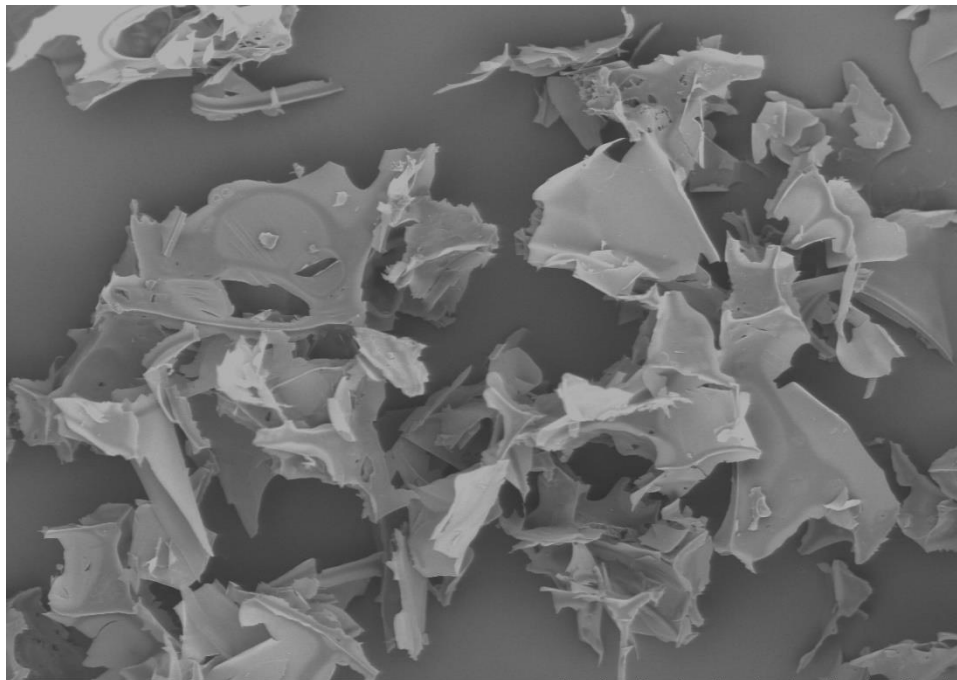

Clariant SU7000 5.00kV 6.5mm x500 UD+LD+MD 11/18/2024 100µm

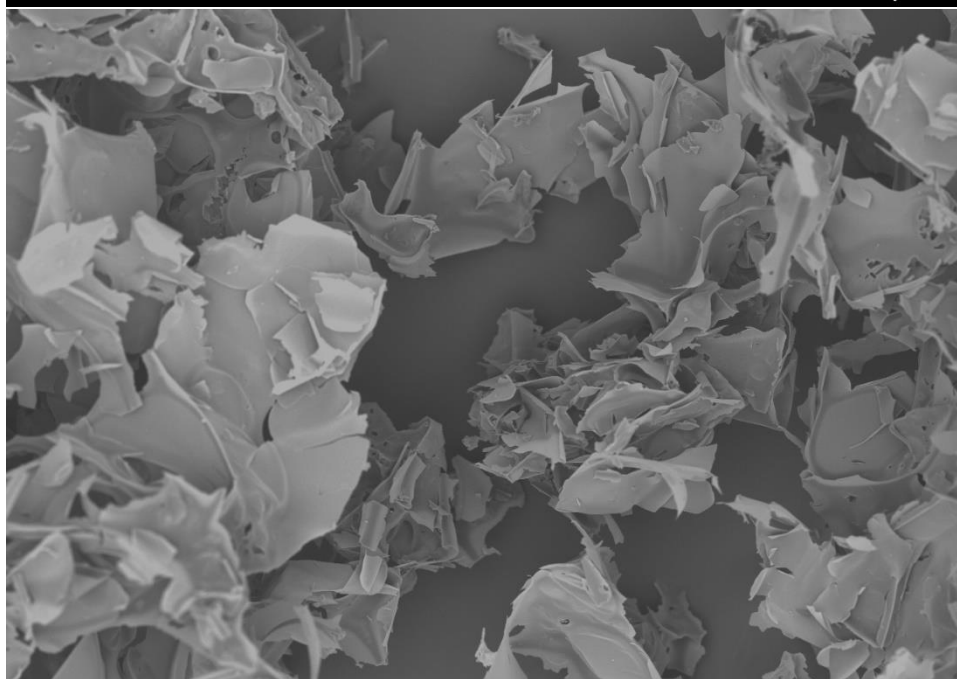

Clariant SU7000 5.00kV 6.5mm x500 UD+LD+MD 11/18/2024 100µm

---


**SCANNING ELECTRON MICROSCOPE (SEM)**

---


**Sample name:** MB3017B 2/3 20% NaOH 35Hz10min 800C 3C/m 1h B 2.6np  
**Ordering customer:** Dr. Torsten Busch  
**Dept./Plant:** Curia Germany GmbH  
**Order number:** 24-048601-2

---

**Sample treatment:** The sample was subjected to platinum sputter coating and then measured.

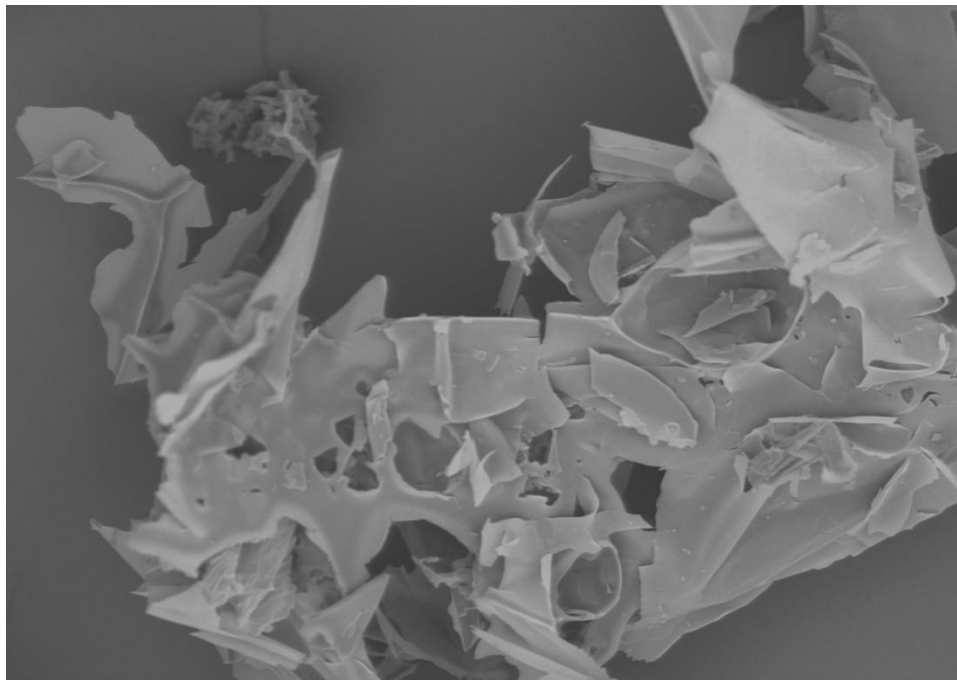

Clariant SU7000 5.00kV 6.6mm x1.00k UD+LD+MD 11/18/2024 50.0µm

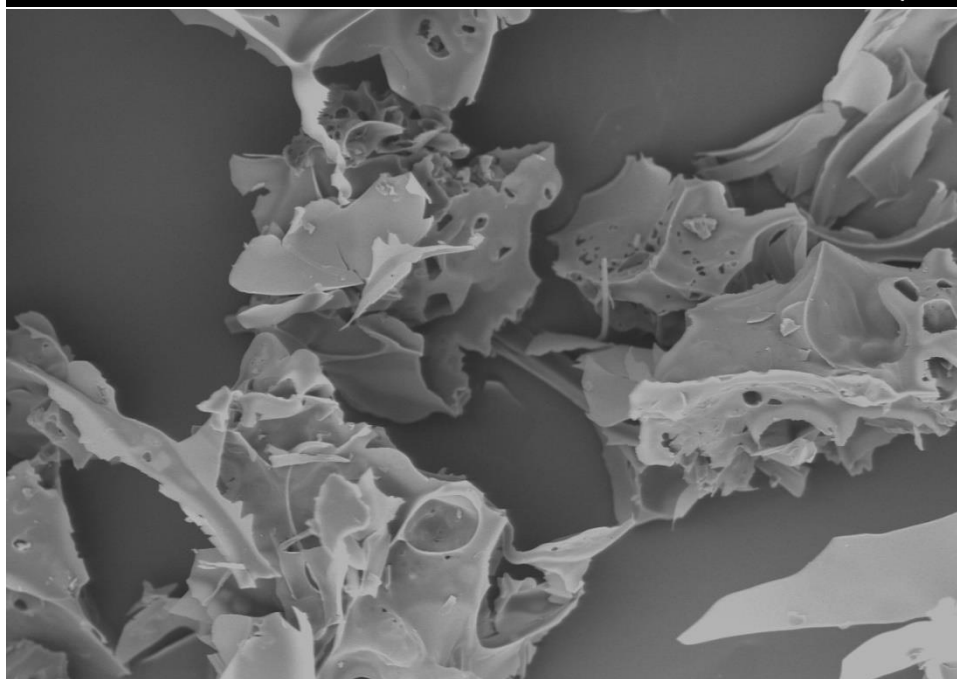

Clariant SU7000 5.00kV 6.5mm x1.00k UD+LD+MD 11/18/2024 50.0µm

---


**SCANNING ELECTRON MICROSCOPE (SEM)**

---


**Sample name:** MB3017B 2/3 20% NaOH 35Hz10min 800C 3C/m 1h B 2.6np  
**Ordering customer:** Dr. Torsten Busch  
**Dept./Plant:** Curia Germany GmbH  
**Order number:** 24-048601-2

---

**Sample treatment:** The sample was subjected to platinum sputter coating and then measured.

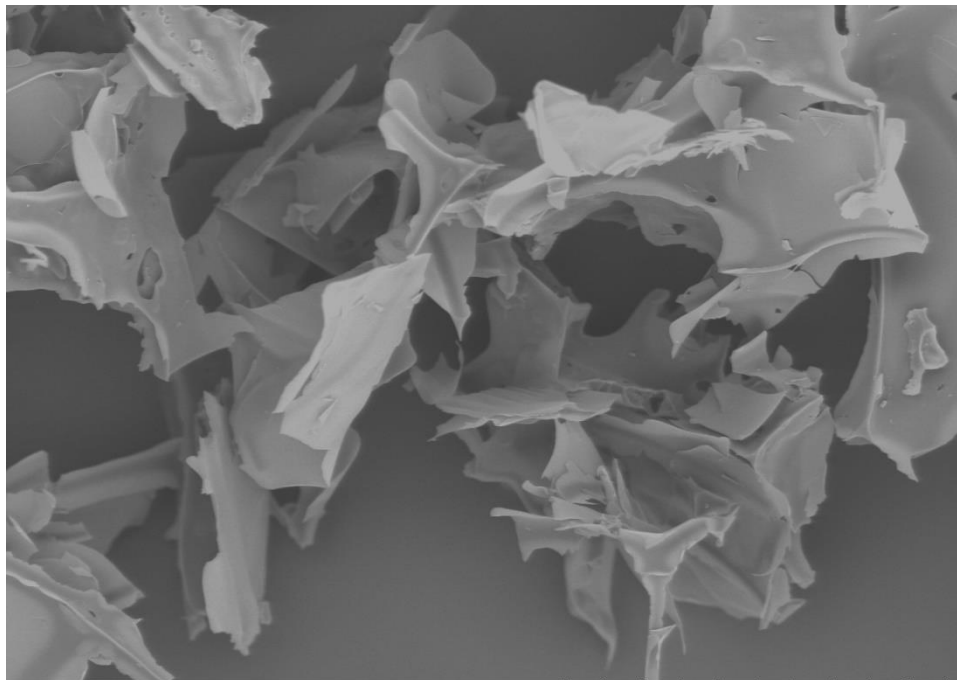

Clariant SU7000 5.00kV 6.4mm x1.00k UD+LD+MD 11/18/2024 50.0µm

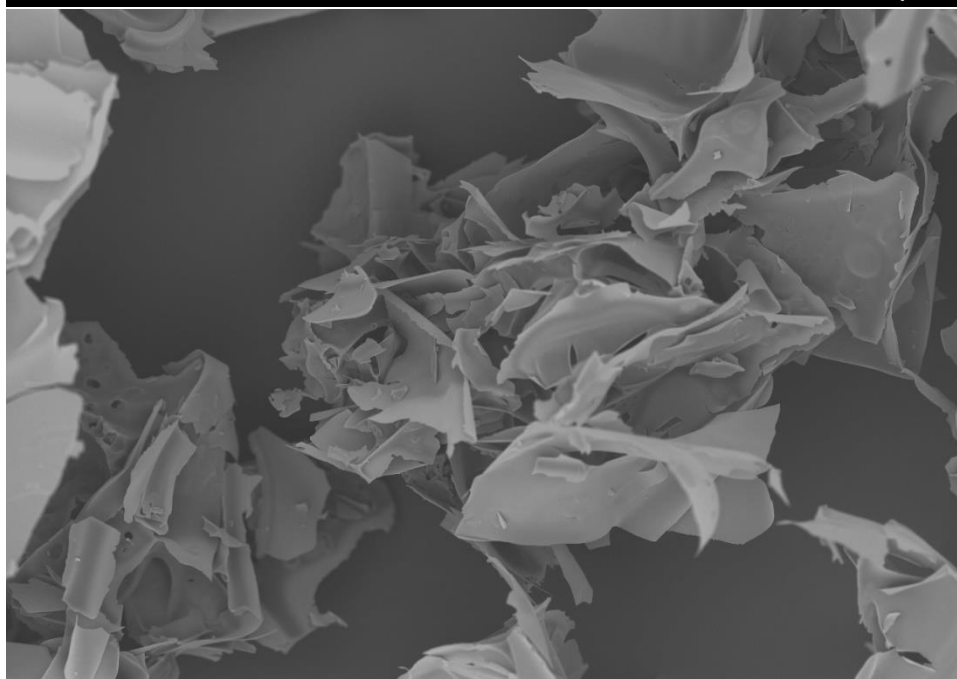


Clariant SU7000 5.00kV 6.5mm x1.00k UD+LD+MD 11/18/2024 50.0µm




## SCANNING ELECTRON MICROSCOPE (SEM)

**Sample name:** MB3017B 2/3 20% NaOH 35Hz10min 800C 3C/m 1h B 2.6np  
**Ordering customer:** Dr. Torsten Busch  
**Dept./Plant:** Curia Germany GmbH  
**Order number:** 24-048601-2

**Sample treatment:** The sample was subjected to platinum sputter coating and then measured.

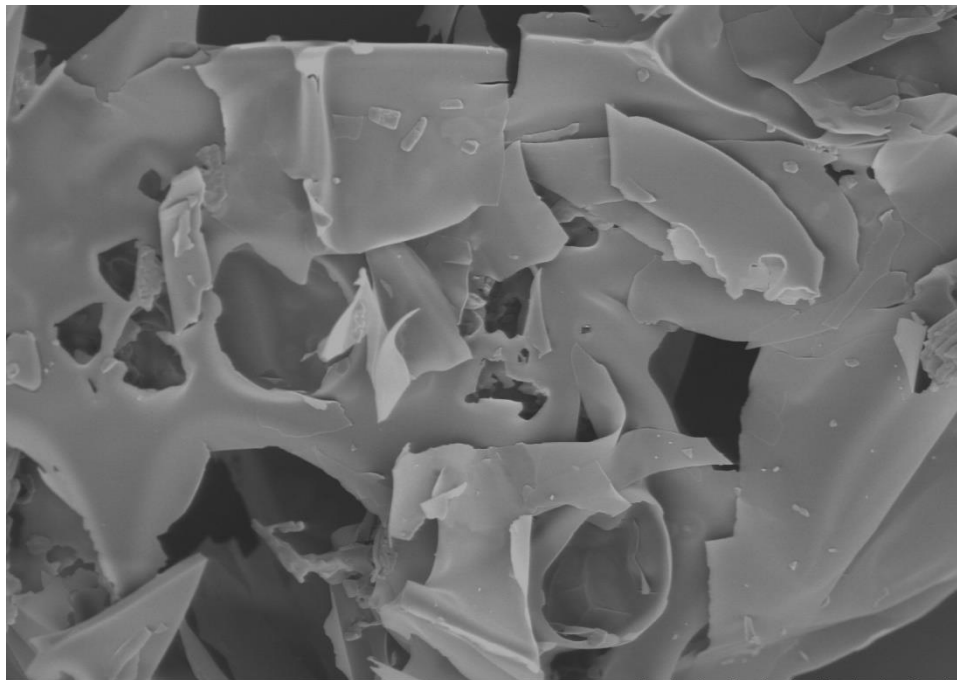

Clariant SU7000 5.00kV 6.6mm x2.00k UD+LD+MD 11/18/2024 20.0μm

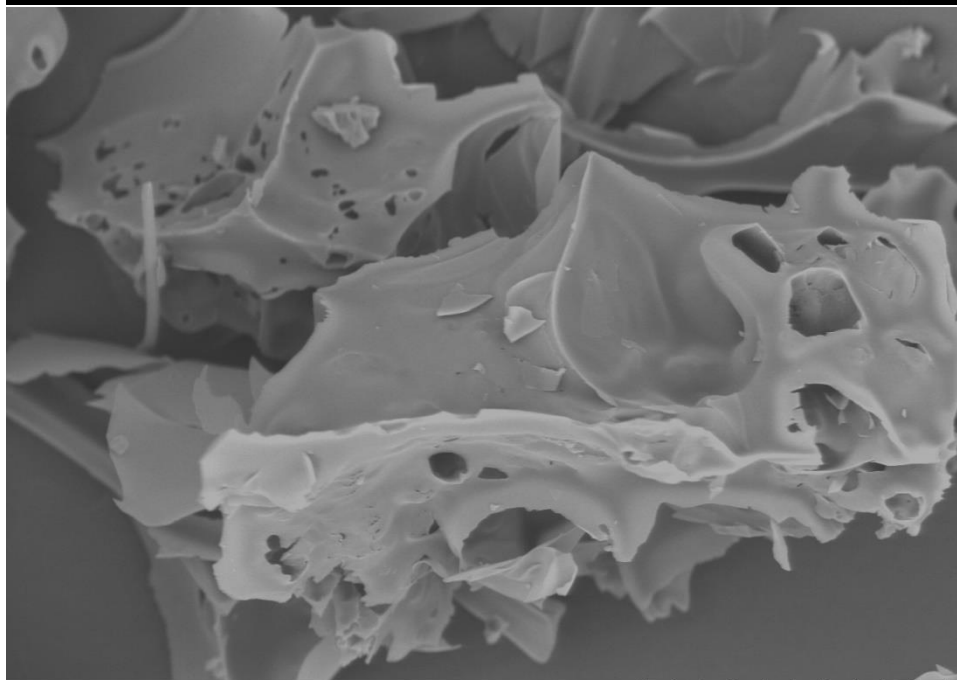


Clariant SU7000 5.00kV 6.5mm x2.00k UD+LD+MD 11/18/2024 20.0μm


## SCANNING ELECTRON MICROSCOPE (SEM)

**Sample name:** MB3017B 2/3 20% NaOH 35Hz10min 800C 3C/m 1h B 2.6np  
**Ordering customer:** Dr. Torsten Busch  
**Dept./Plant:** Curia Germany GmbH  
**Order number:** 24-048601-2

**Sample treatment:** The sample was subjected to platinum sputter coating and then measured.

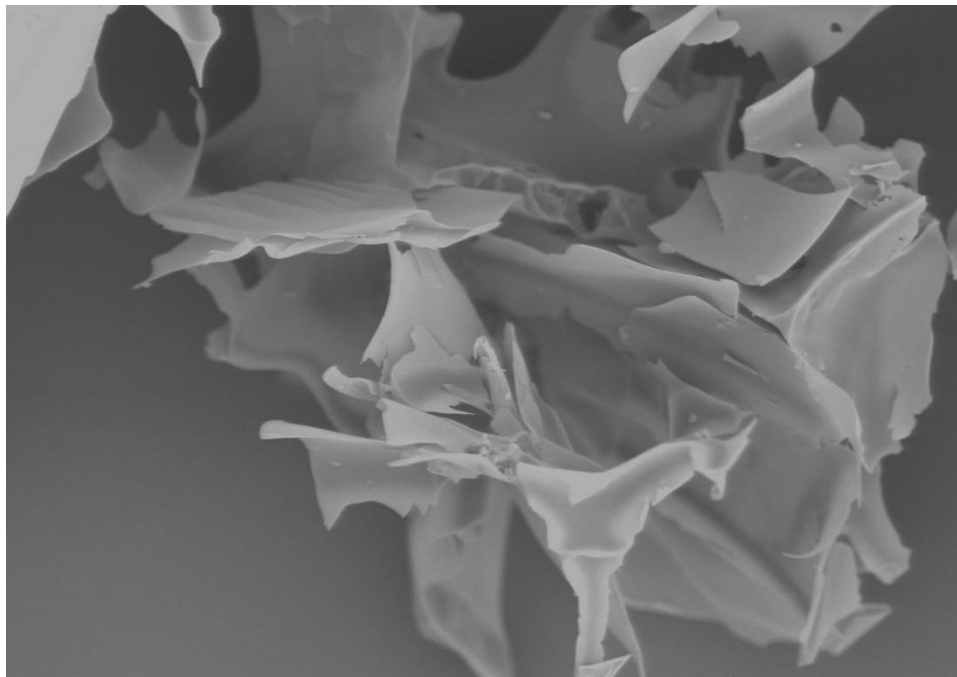

Clariant SU7000 5.00kV 6.4mm x2.00k UD+LD+MD 11/18/2024 20.0µm

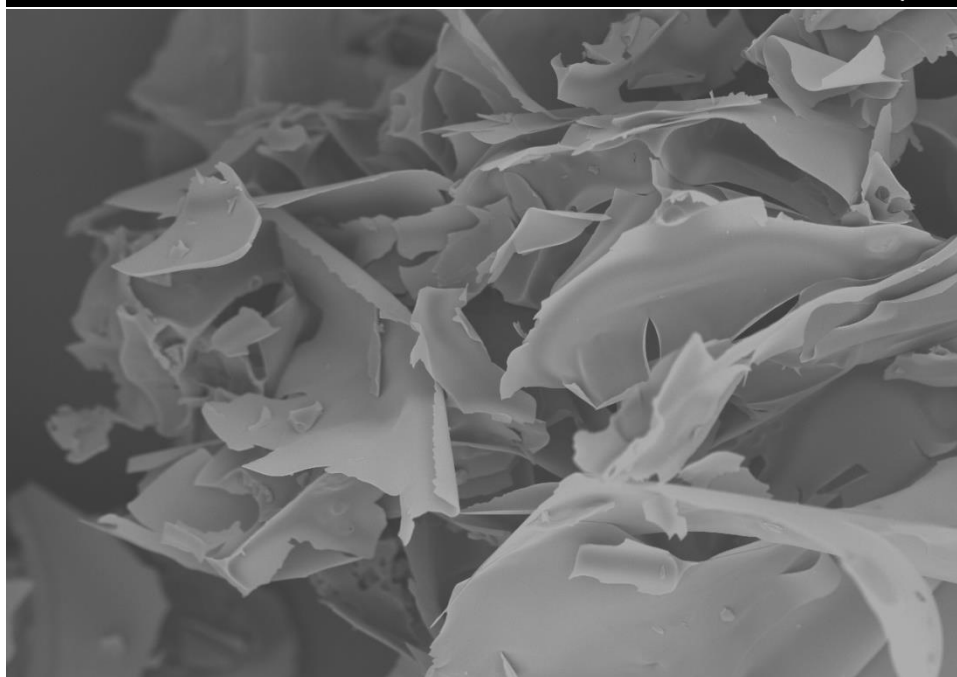


Clariant SU7000 5.00kV 6.5mm x2.00k UD+LD+MD 11/18/2024 20.0µm


## SCANNING ELECTRON MICROSCOPE (SEM)

**Sample name:** MB3017B 2/3 20% NaOH 35Hz10min 800C 3C/m 1h B 2.6np  
**Ordering customer:** Dr. Torsten Busch  
**Dept./Plant:** Curia Germany GmbH  
**Order number:** 24-048601-2

**Sample treatment:** The sample was subjected to platinum sputter coating and then measured.

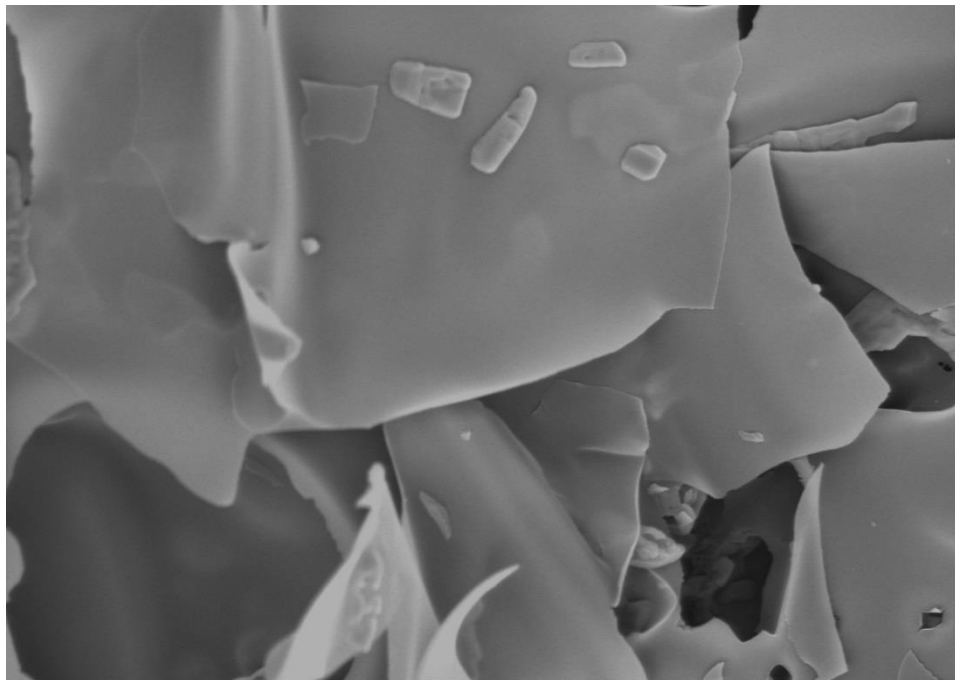

Clariant SU7000 5.00kV 6.6mm x5.00k UD+LD+MD 11/18/2024 10.0µm

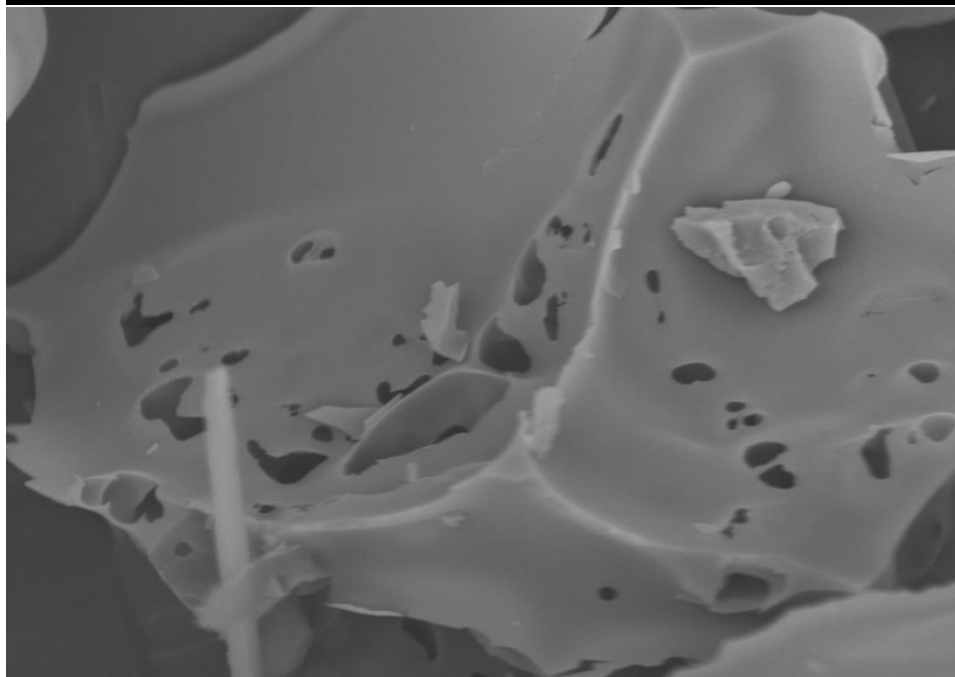


Clariant SU7000 5.00kV 6.5mm x5.00k UD+LD+MD 11/18/2024 10.0µm


## SCANNING ELECTRON MICROSCOPE (SEM)

**Sample name:** MB3017B 2/3 20% NaOH 35Hz10min 800C 3C/m 1h B 2.6np  
**Ordering customer:** Dr. Torsten Busch  
**Dept./Plant:** Curia Germany GmbH  
**Order number:** 24-048601-2

**Sample treatment:** The sample was subjected to platinum sputter coating and then measured.

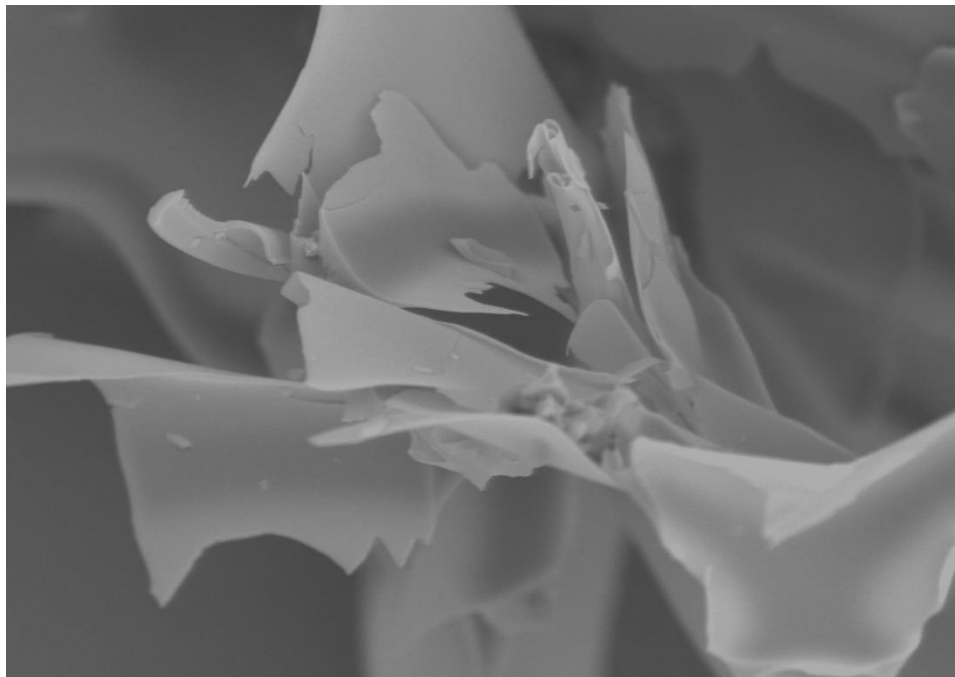

Clariant SU7000 5.00kV 6.4mm x5.00k UD+LD+MD 11/18/2024 10.0µm

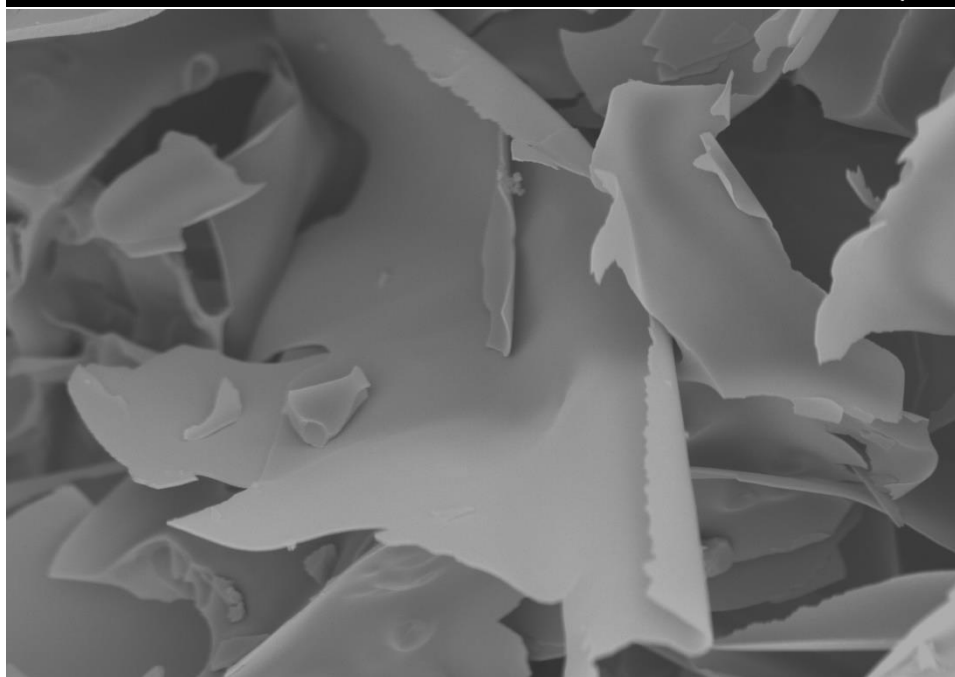


Clariant SU7000 5.00kV 6.5mm x5.00k UD+LD+MD 11/18/2024 10.0µm


## SCANNING ELECTRON MICROSCOPE (SEM)

**Sample name:** MB3017B 2/3 20% NaOH 35Hz10min 800C 3C/m 1h B 2.6np  
**Ordering customer:** Dr. Torsten Busch  
**Dept./Plant:** Curia Germany GmbH  
**Order number:** 24-048601-2

**Sample treatment:** The sample was subjected to platinum sputter coating and then measured.

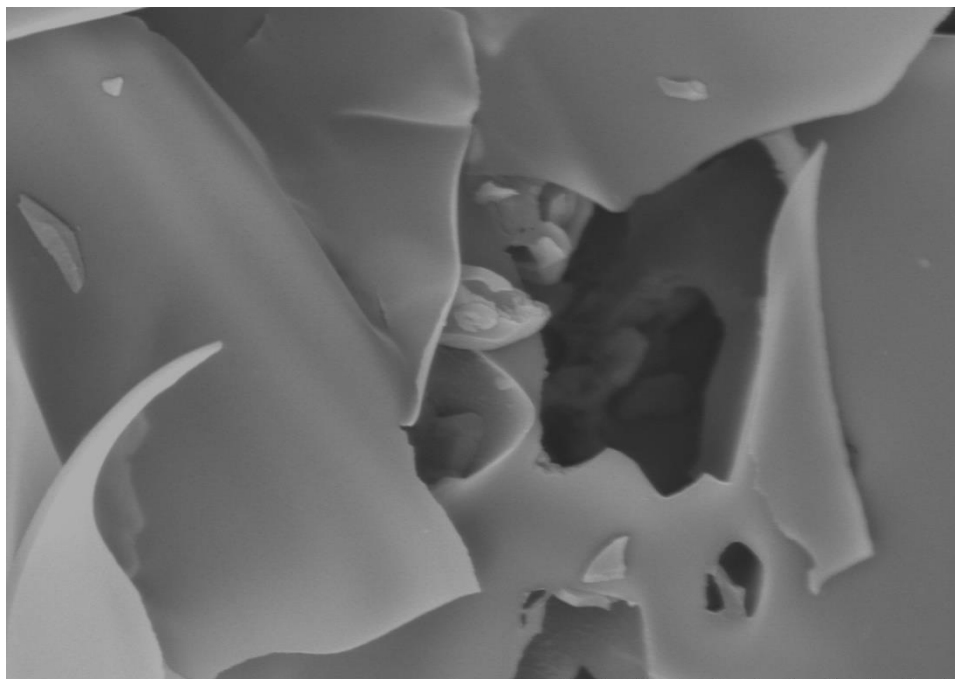

Clariant SU7000 5.00kV 6.6mm x10.0k UD+LD+MD 11/18/2024 5.00µm

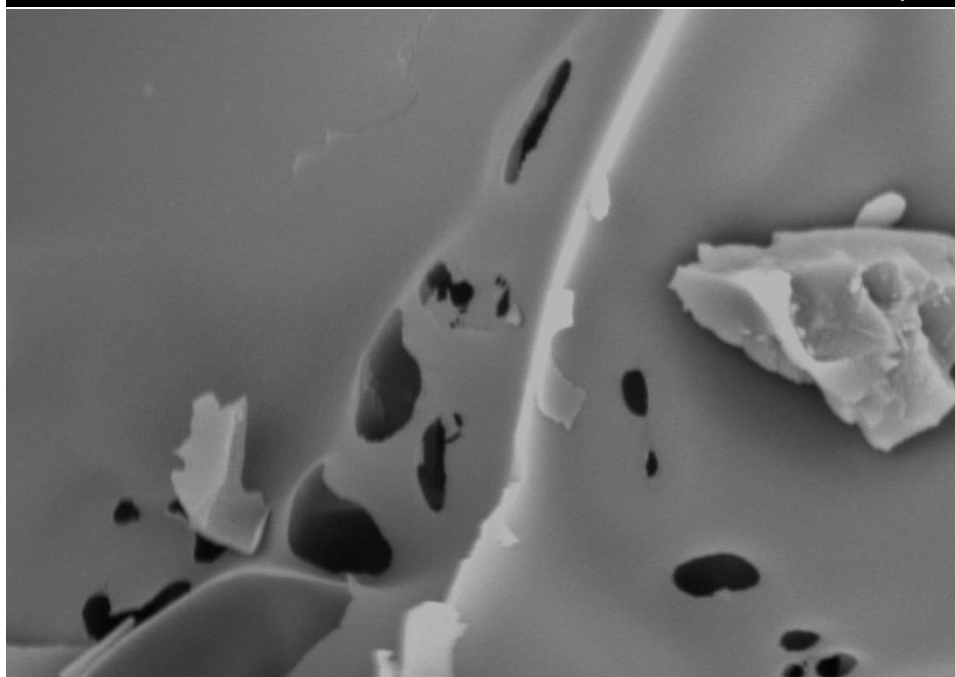


Clariant SU7000 5.00kV 6.5mm x10.0k UD+LD+MD 11/18/2024 5.00µm


## SCANNING ELECTRON MICROSCOPE (SEM)

**Sample name:** MB3017B 2/3 20% NaOH 35Hz10min 800C 3C/m 1h B 2.6np  
**Ordering customer:** Dr. Torsten Busch  
**Dept./Plant:** Curia Germany GmbH  
**Order number:** 24-048601-2

**Sample treatment:** The sample was subjected to platinum sputter coating and then measured.

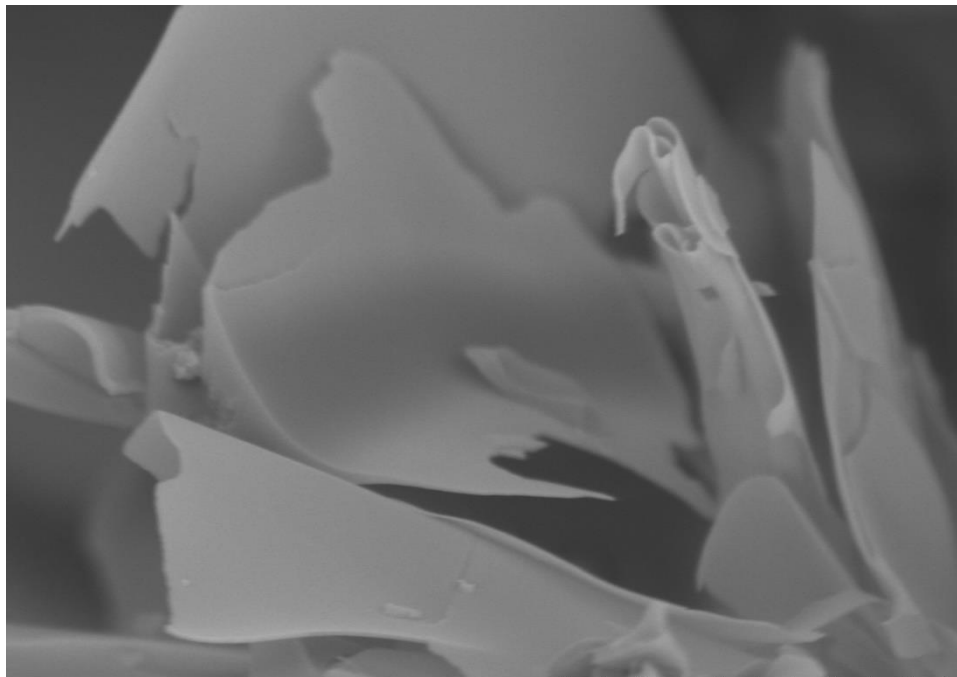

Clariant SU7000 5.00kV 6.4mm x10.0k UD+LD+MD 11/18/2024 5.00µm

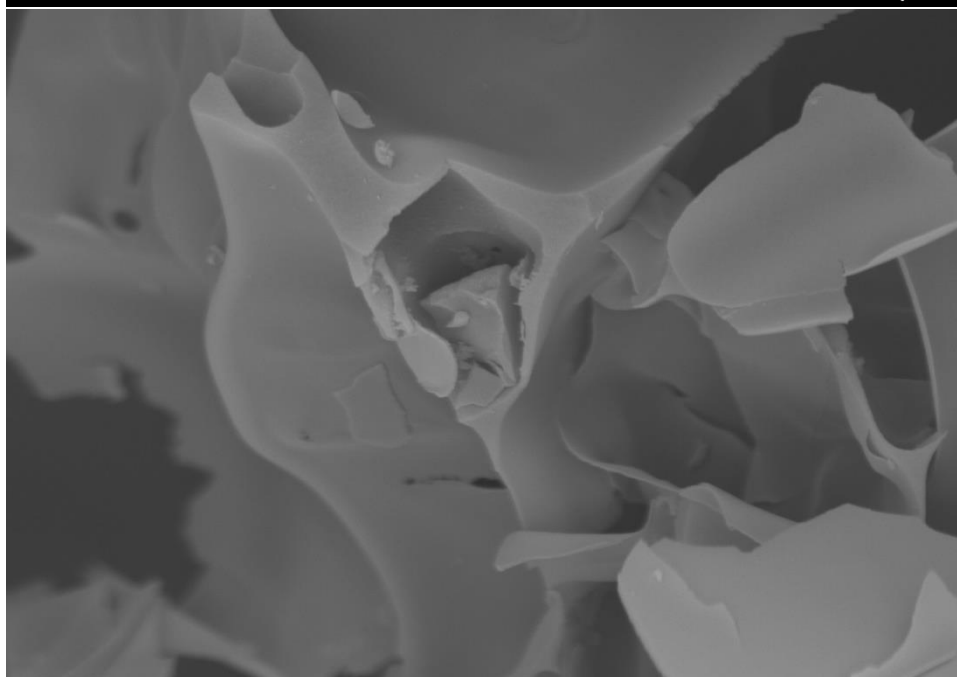


Clariant SU7000 5.00kV 6.5mm x10.0k UD+LD+MD 11/18/2024 5.00µm




## SCANNING ELECTRON MICROSCOPE (SEM)

**Sample name:** MB3017B 2/3 20% NaOH 35Hz10min 800C 3C/m 1h B 2.6np  
**Ordering customer:** Dr. Torsten Busch  
**Dept./Plant:** Curia Germany GmbH  
**Order number:** 24-048601-2

**Sample treatment:** The sample was subjected to platinum sputter coating and then measured.

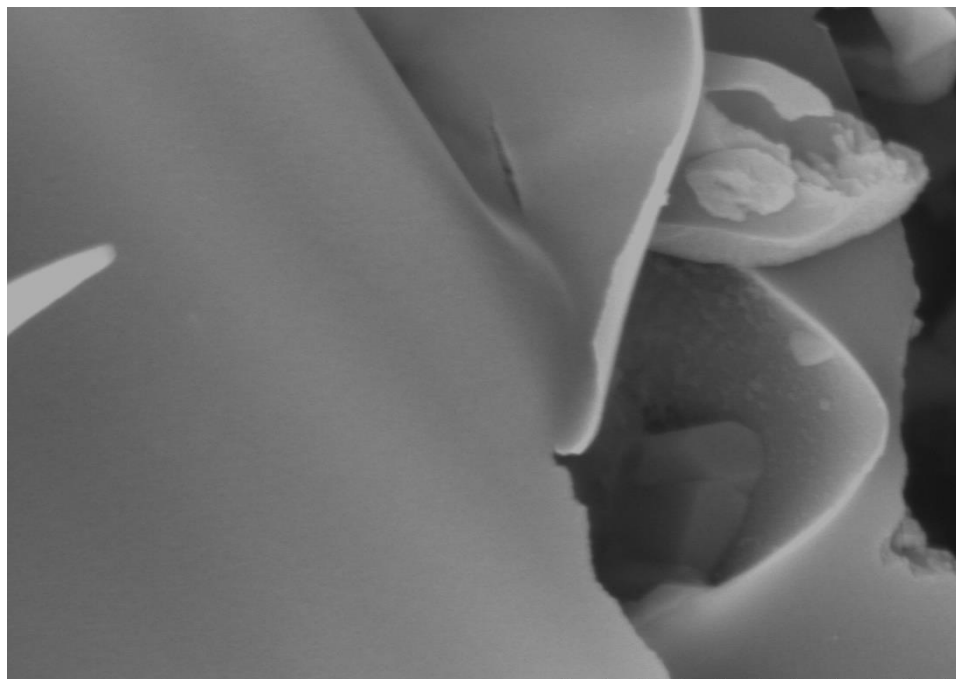

Clariant SU7000 5.00kV 6.6mm x25.0k UD+LD+MD 11/18/2024 2.00µm

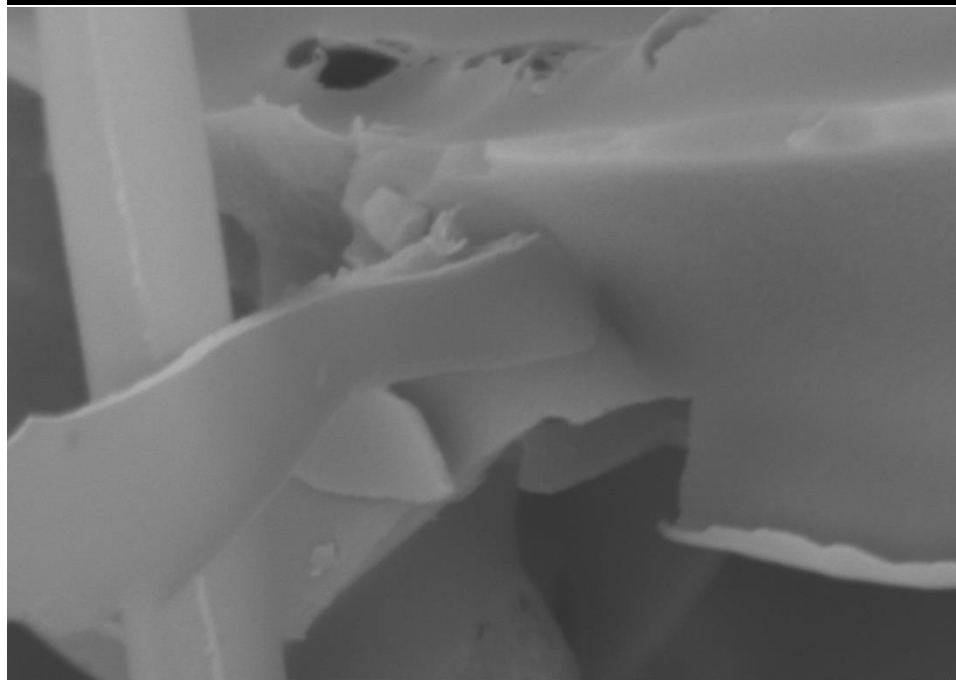

Clariant SU7000 5.00kV 6.5mm x25.0k UD+LD+MD 11/18/2024 2.00µm

## SCANNING ELECTRON MICROSCOPE (SEM)

**Sample name:** MB3017B 2/3 20% NaOH 35Hz10min 800C 3C/m 1h B 2.6np  
**Ordering customer:** Dr. Torsten Busch  
**Dept./Plant:** Curia Germany GmbH  
**Order number:** 24-048601-2

**Sample treatment:** The sample was subjected to platinum sputter coating and then measured.

