



SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: KJo-0178 2/3 1-5m 800C 3C/m 1h A 2x2.0P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-048023-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

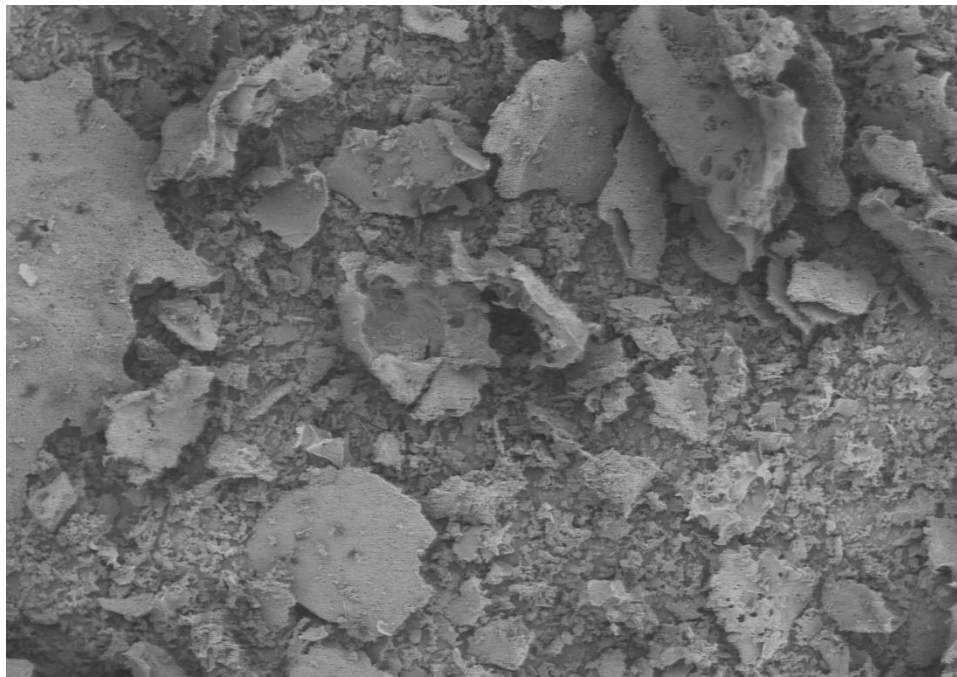

Clariant SU7000 5.00kV 6.7mm x100 UD+LD+MD 09/16/2024 500µm

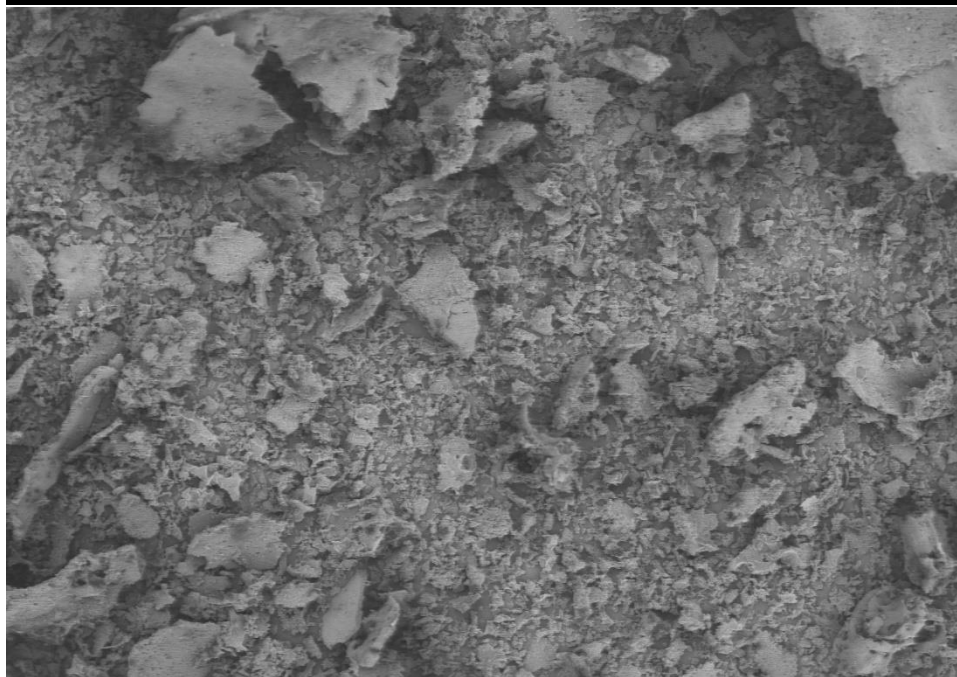

Clariant SU7000 5.00kV 6.9mm x100 UD+LD+MD 09/16/2024 500µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: KJo-0178 2/3 1-5m 800C 3C/m 1h A 2x2.0P

Ordering customer: Dr. Torsten Busch

Dept./Plant: Curia Germany GmbH

Order number: 24-048023-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

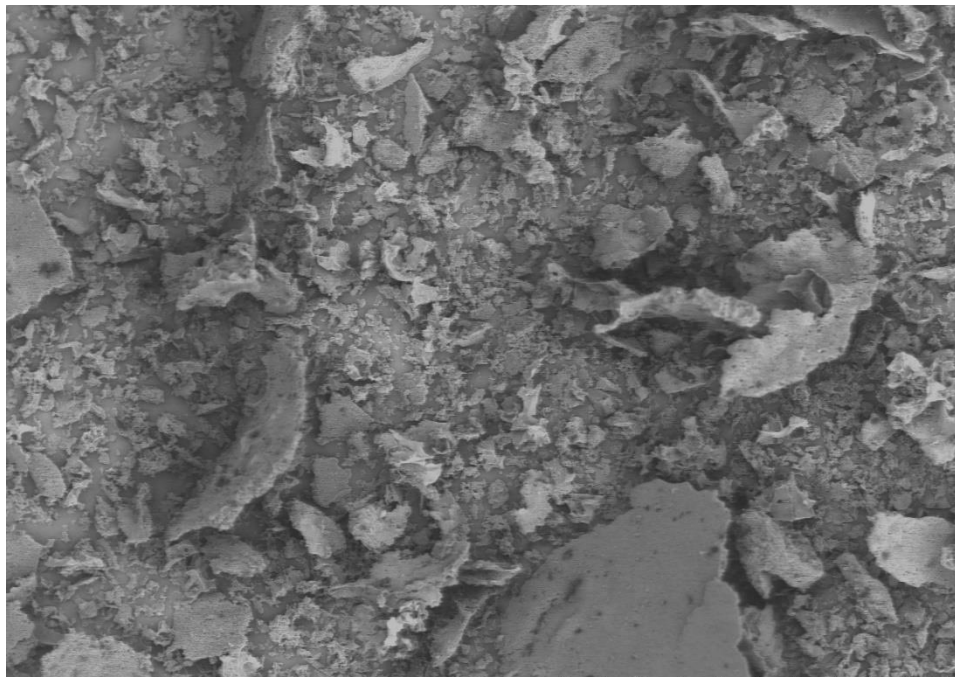

Clariant SU7000 5.00kV 6.8mm x100 UD+LD+MD 09/16/2024 500µm




Clariant SU7000 5.00kV 6.9mm x100 UD+LD+MD 09/16/2024 500µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: KJo-0178 2/3 1-5m 800C 3C/m 1h A 2x2.0P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-048023-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

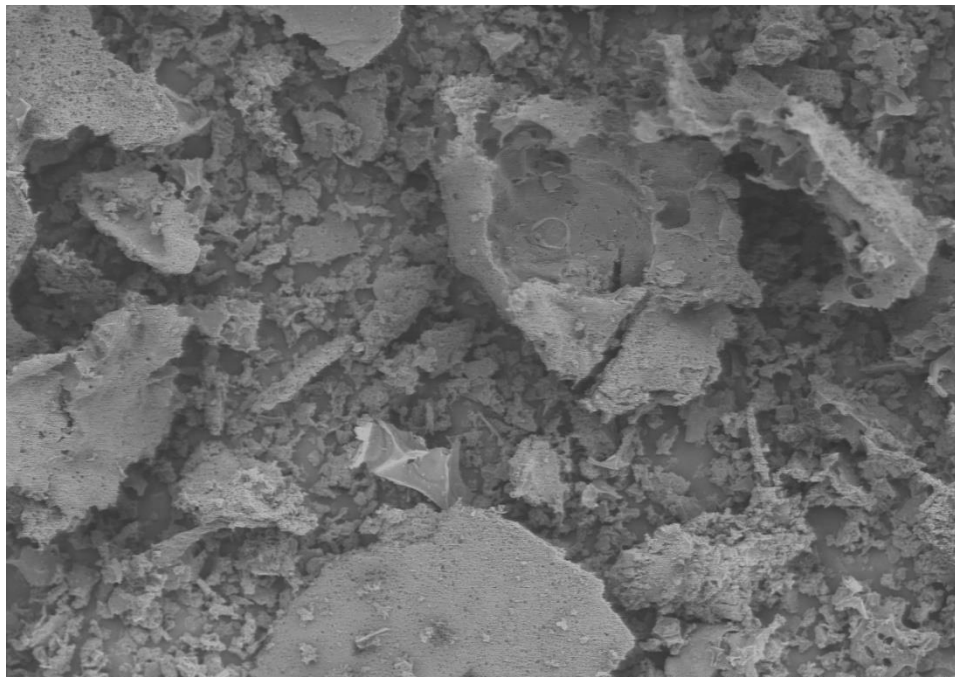

Clariant SU7000 5.00kV 6.7mm x200 UD+LD+MD 09/16/2024 200µm

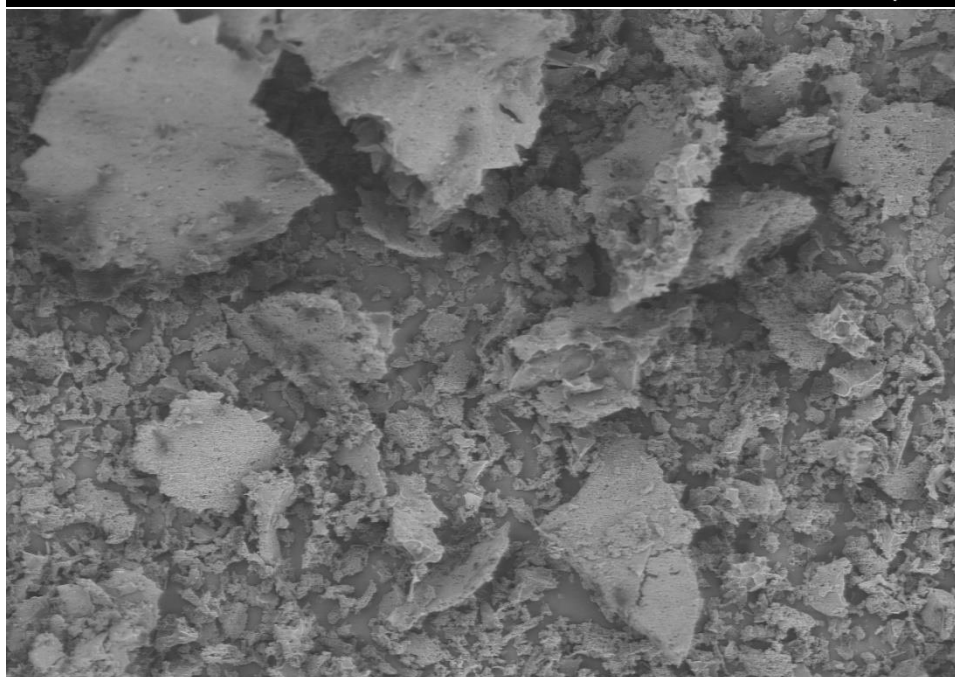


Clariant SU7000 5.00kV 6.9mm x200 UD+LD+MD 09/16/2024 200µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: KJo-0178 2/3 1-5m 800C 3C/m 1h A 2x2.0P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-048023-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

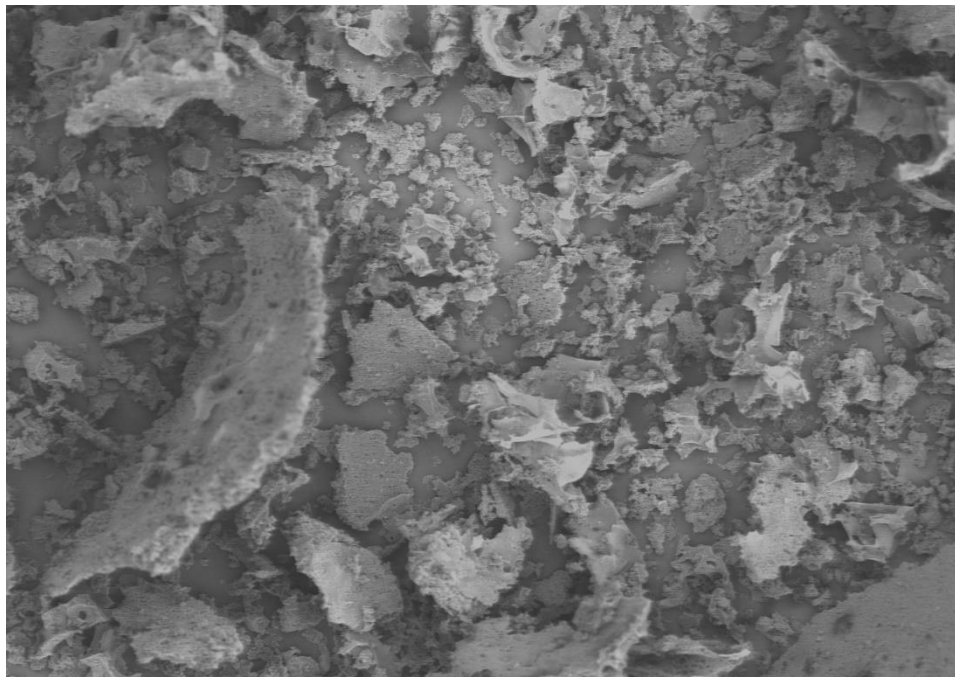

Clariant SU7000 5.00kV 6.8mm x200 UD+LD+MD 09/16/2024 200µm

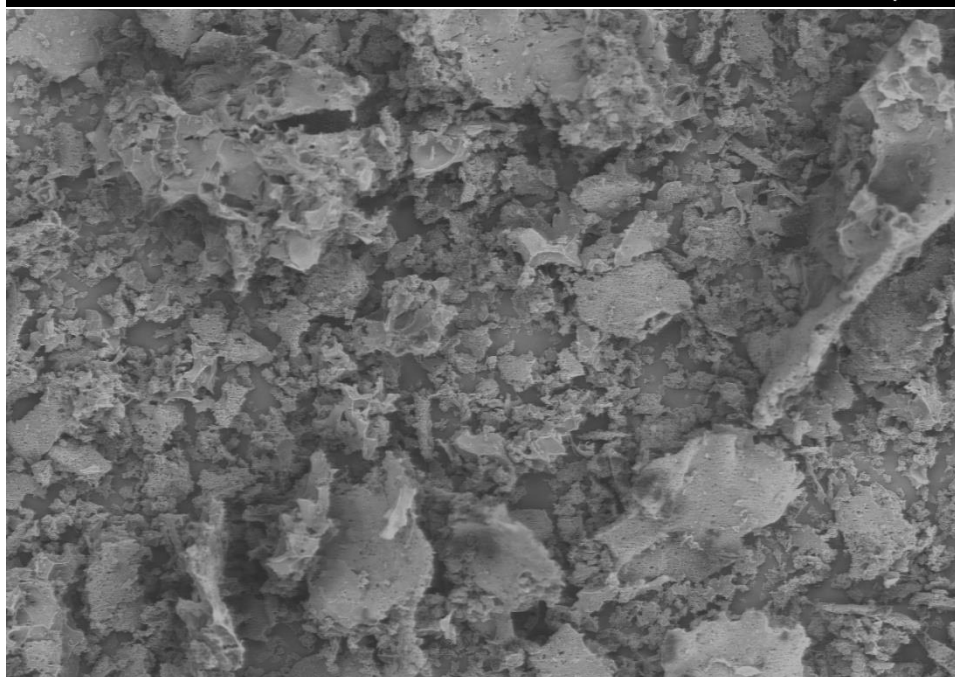

Clariant SU7000 5.00kV 6.9mm x200 UD+LD+MD 09/16/2024 200µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: KJo-0178 2/3 1-5m 800C 3C/m 1h A 2x2.0P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-048023-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

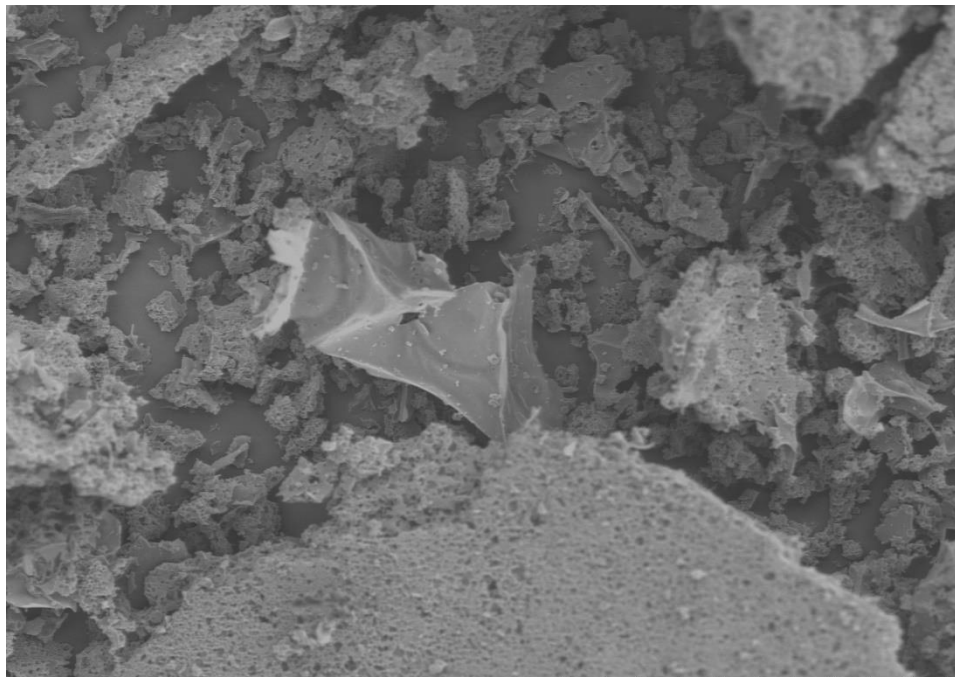

Clariant SU7000 5.00kV 6.9mm x500 UD+LD+MD 09/16/2024 100µm

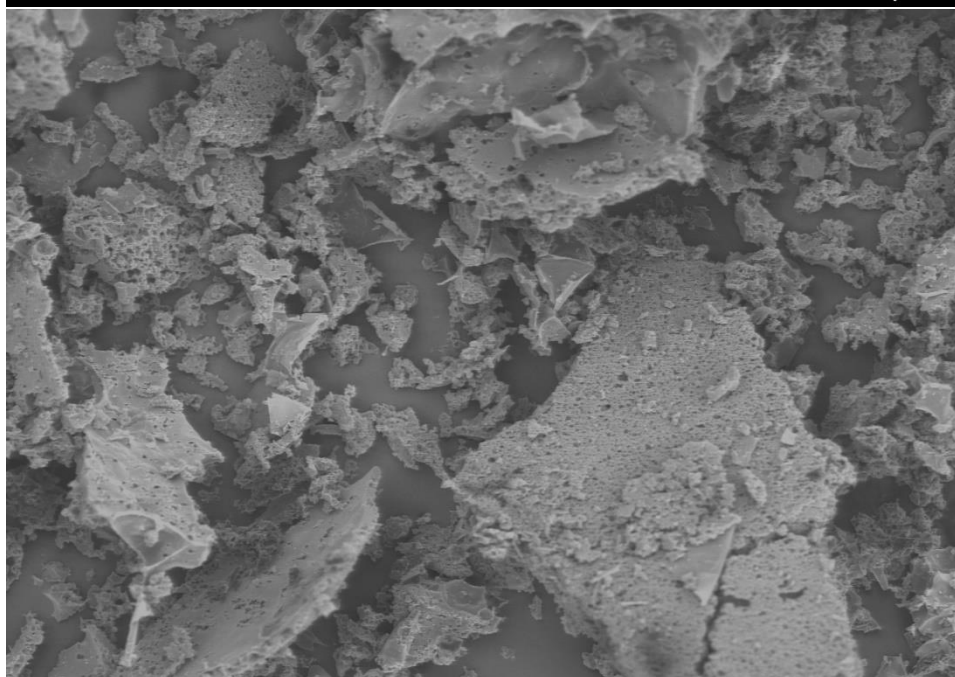


Clariant SU7000 5.00kV 6.9mm x500 UD+LD+MD 09/16/2024 100µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: KJo-0178 2/3 1-5m 800C 3C/m 1h A 2x2.0P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-048023-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

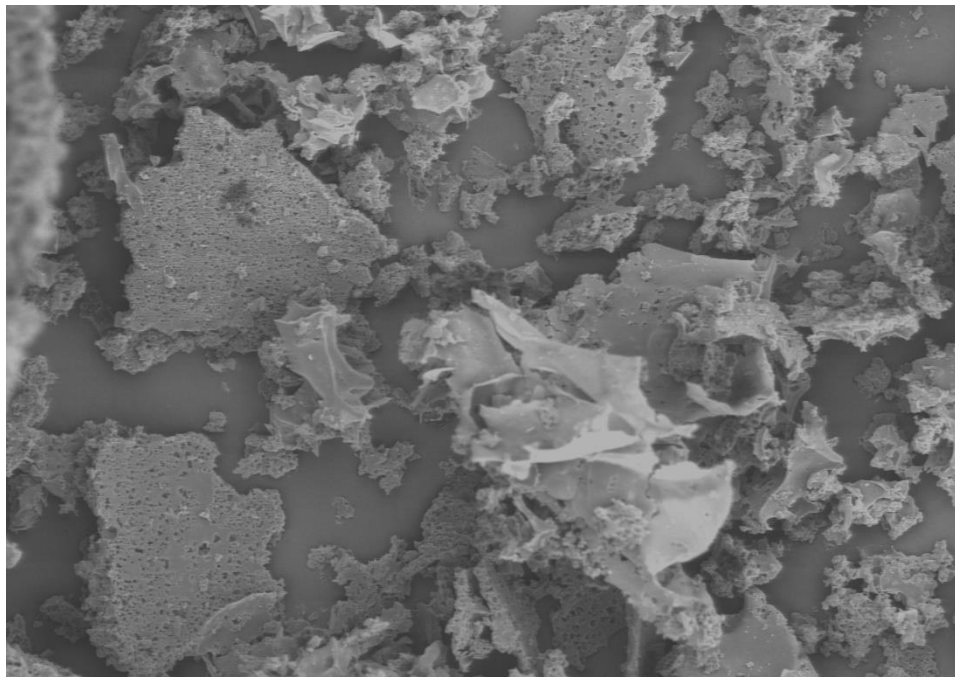

Clariant SU7000 5.00kV 6.8mm x500 UD+LD+MD 09/16/2024 100µm

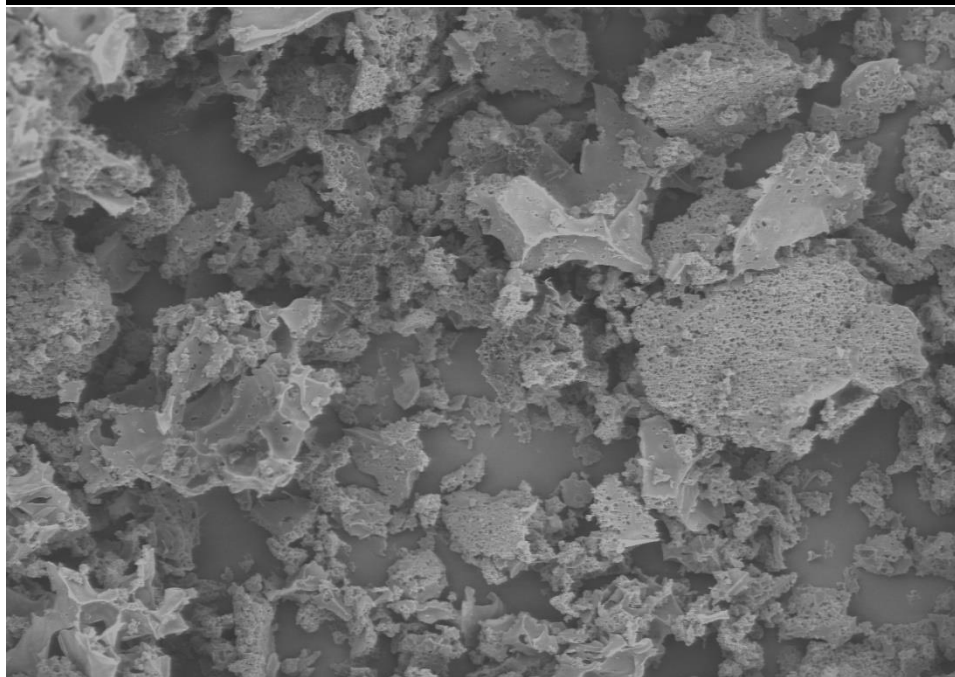

Clariant SU7000 5.00kV 6.9mm x500 UD+LD+MD 09/16/2024 100µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: KJo-0178 2/3 1-5m 800C 3C/m 1h A 2x2.0P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-048023-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

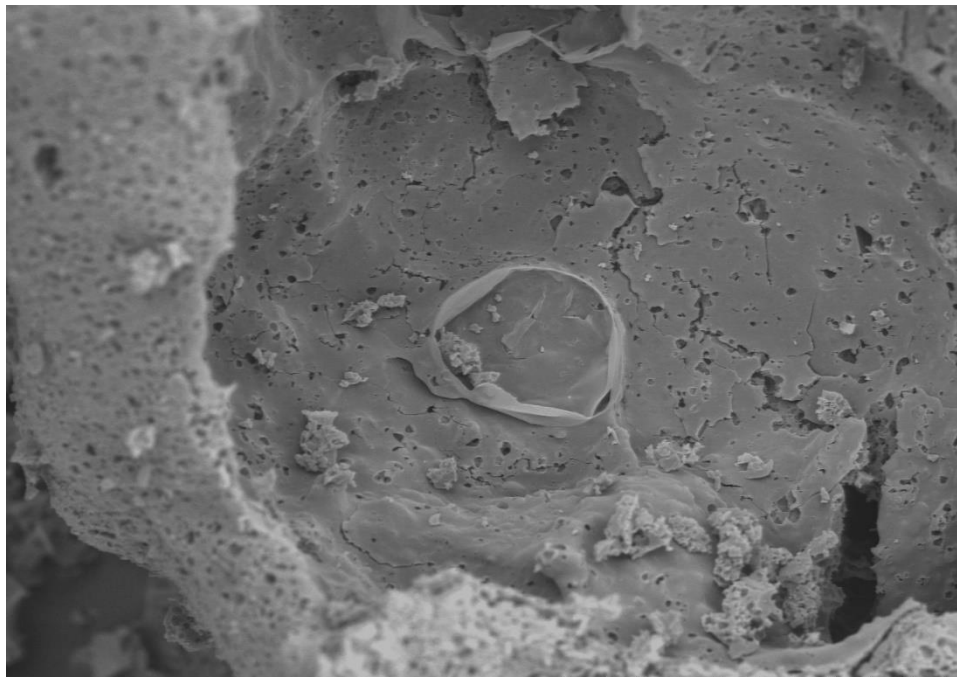

Clariant SU7000 5.00kV 6.8mm x1.00k UD+LD+MD 09/16/2024 50.0µm

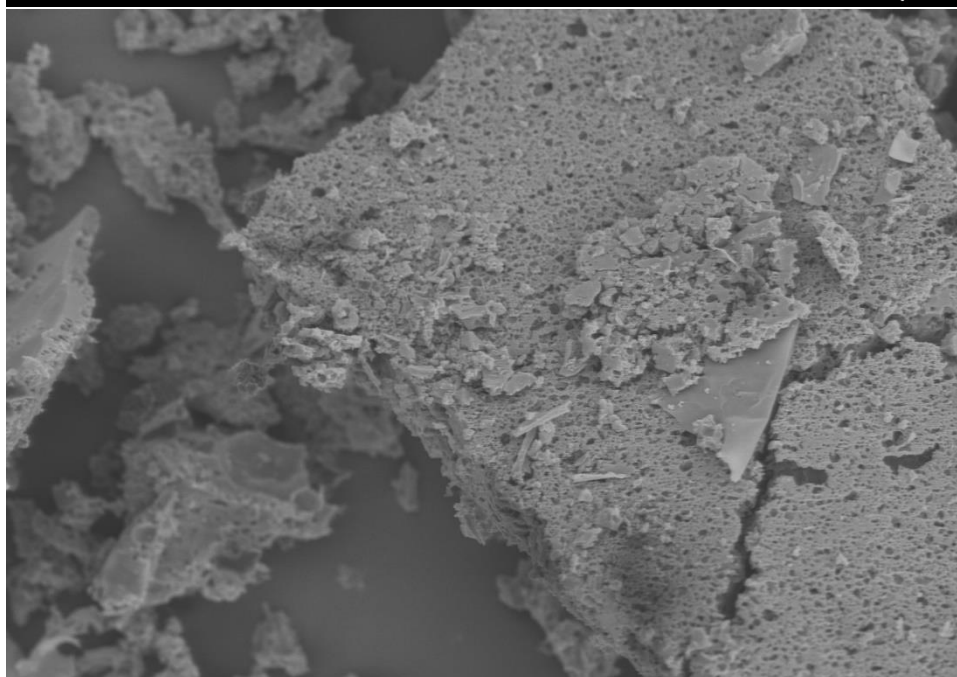

Clariant SU7000 5.00kV 6.8mm x1.00k UD+LD+MD 09/16/2024 50.0µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: KJo-0178 2/3 1-5m 800C 3C/m 1h A 2x2.0P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-048023-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

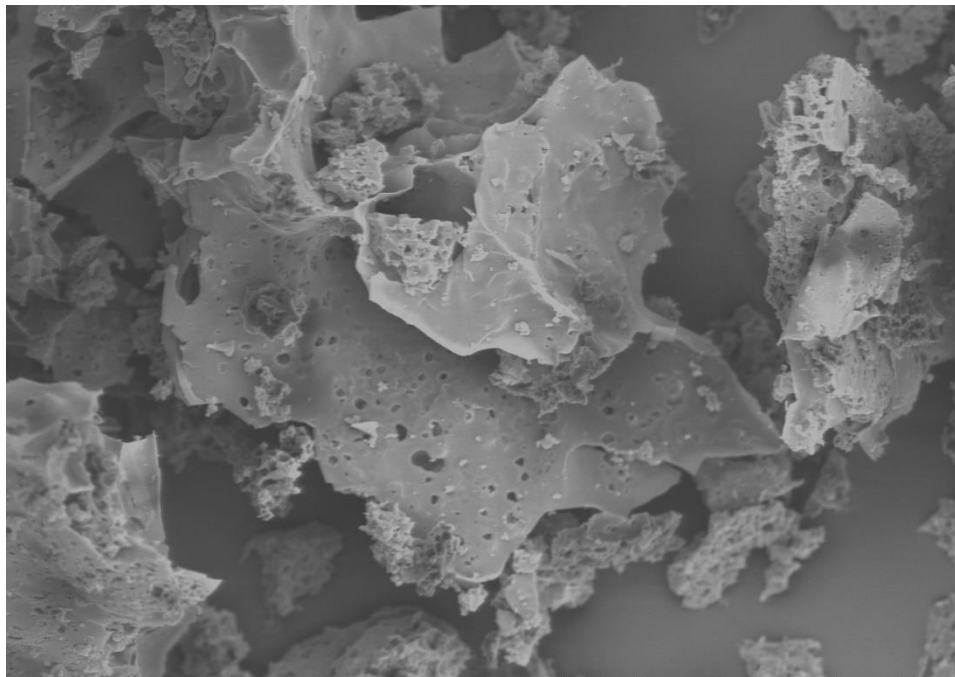

Clariant SU7000 5.00kV 6.8mm x1.00k UD+LD+MD 09/16/2024 50.0µm

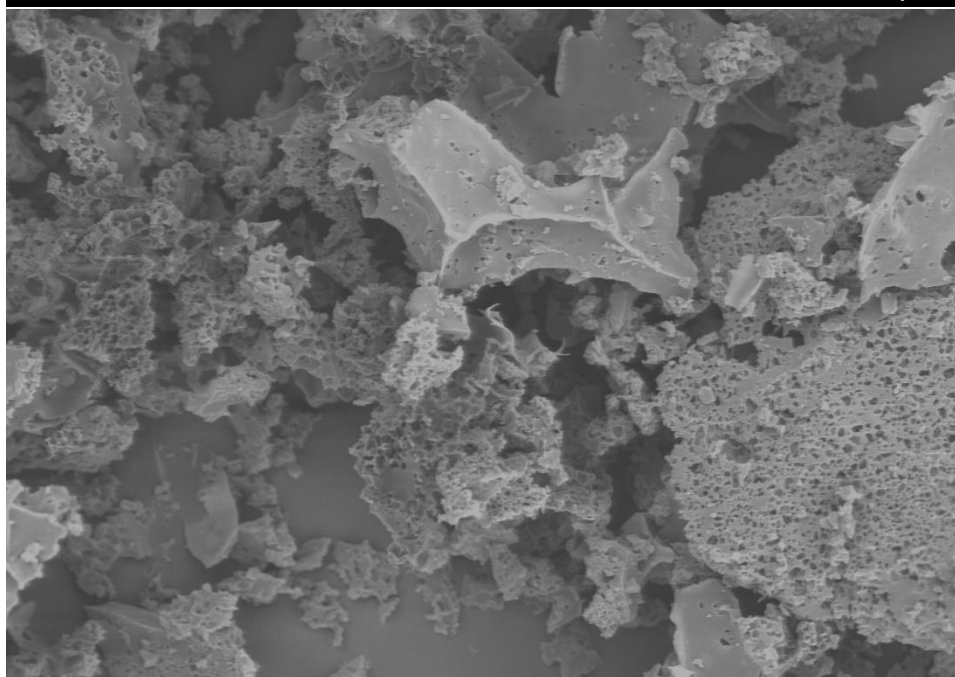


Clariant SU7000 5.00kV 6.9mm x1.00k UD+LD+MD 09/16/2024 50.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: KJo-0178 2/3 1-5m 800C 3C/m 1h A 2x2.0P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-048023-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

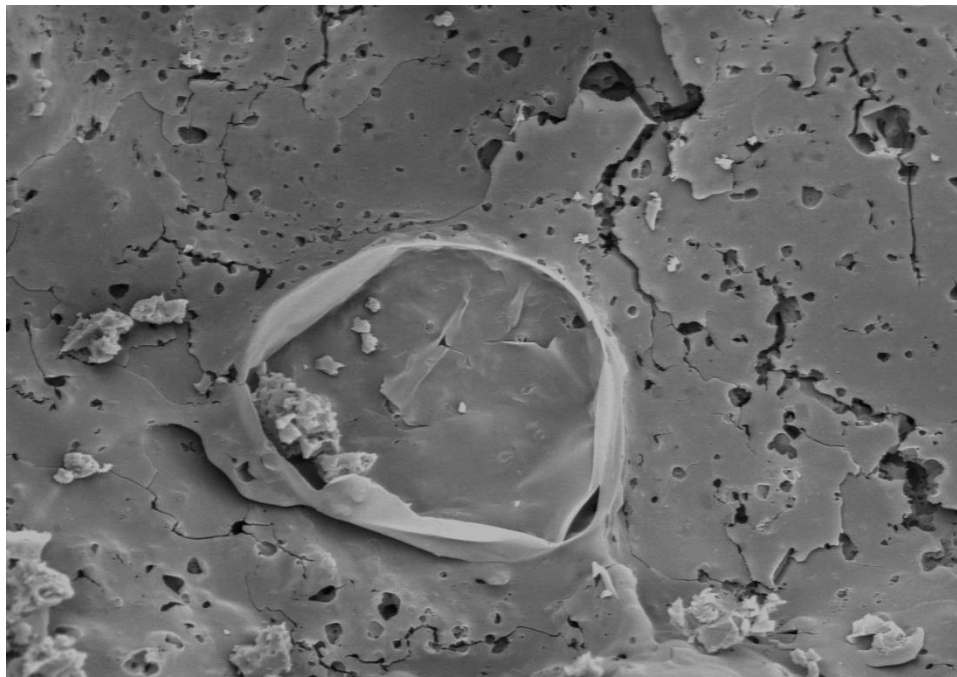

Clariant SU7000 5.00kV 6.8mm x2.00k UD+LD+MD 09/16/2024 20.0µm

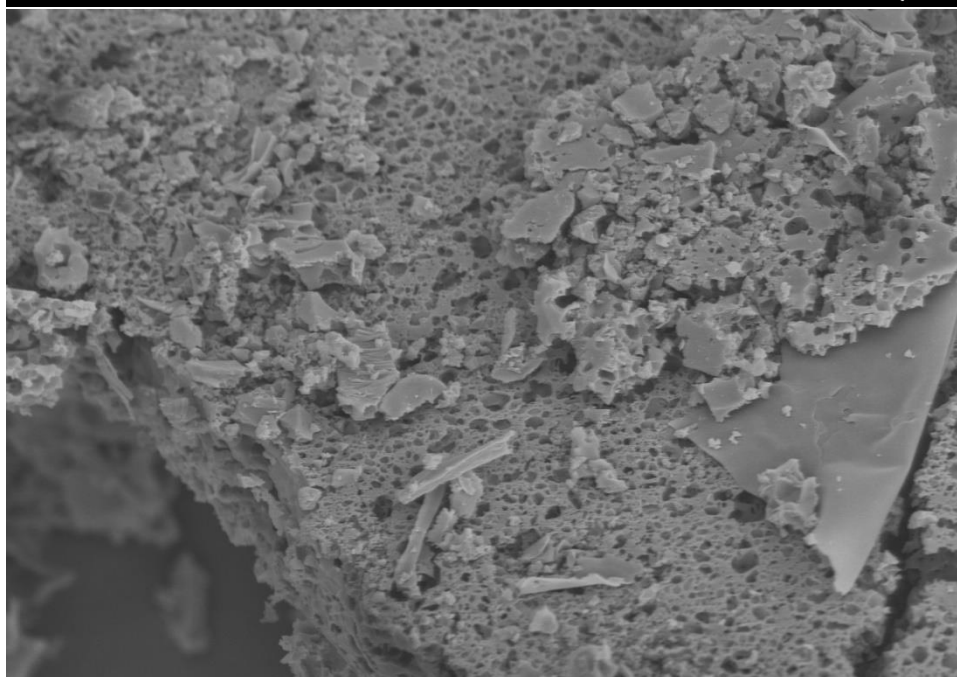

Clariant SU7000 5.00kV 6.8mm x2.00k UD+LD+MD 09/16/2024 20.0µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: KJo-0178 2/3 1-5m 800C 3C/m 1h A 2x2.0P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-048023-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

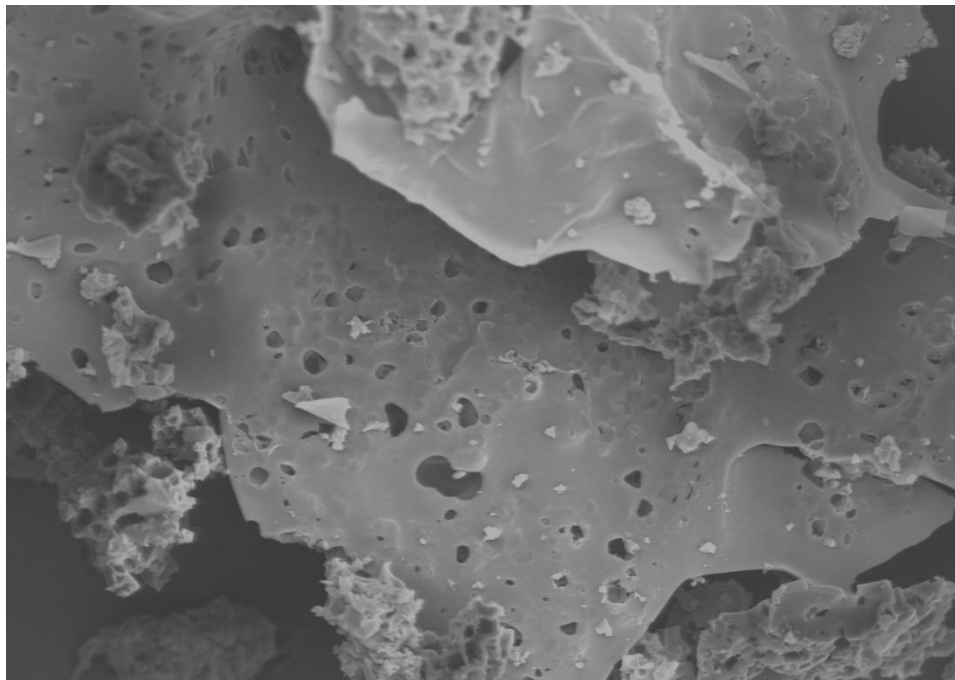

Clariant SU7000 5.00kV 6.8mm x2.00k UD+LD+MD 09/16/2024 20.0µm

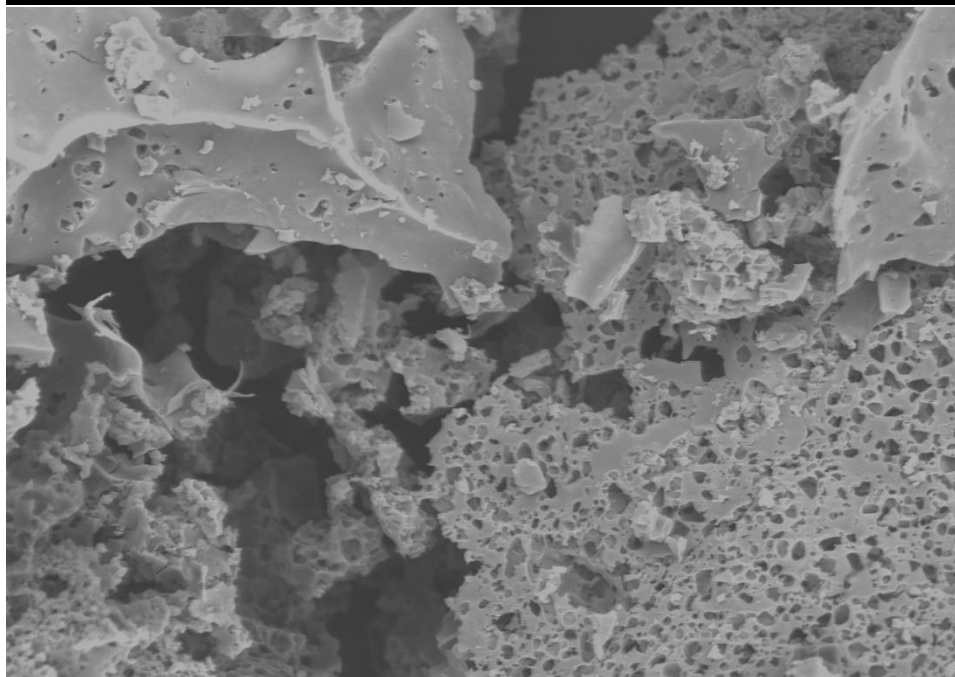


Clariant SU7000 5.00kV 6.9mm x2.00k UD+LD+MD 09/16/2024 20.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: KJo-0178 2/3 1-5m 800C 3C/m 1h A 2x2.0P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-048023-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

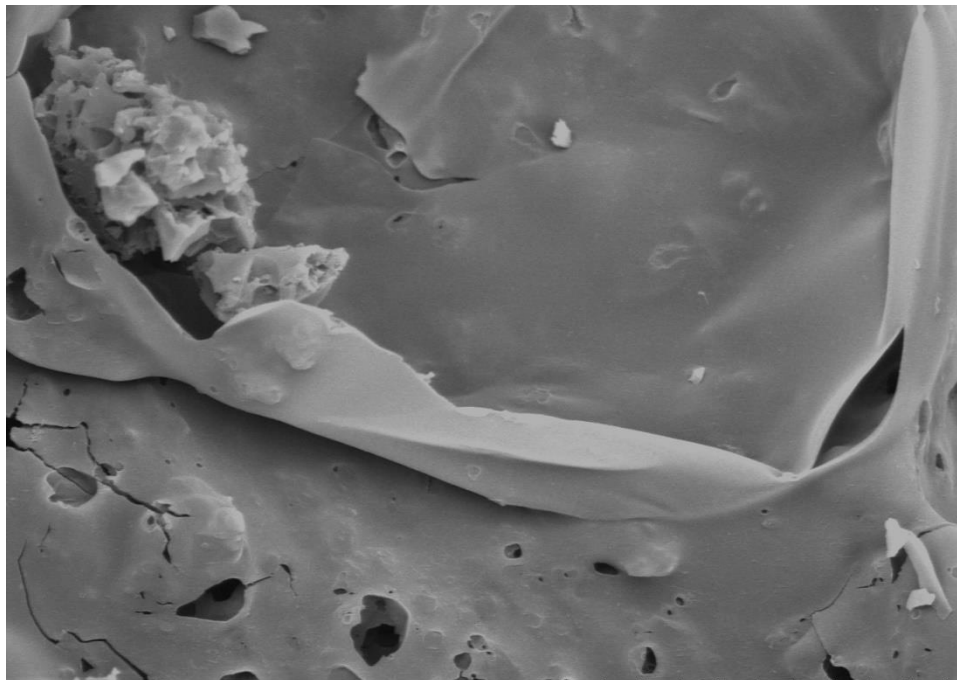

Clariant SU7000 5.00kV 6.8mm x5.00k UD+LD+MD 09/16/2024 10.0µm

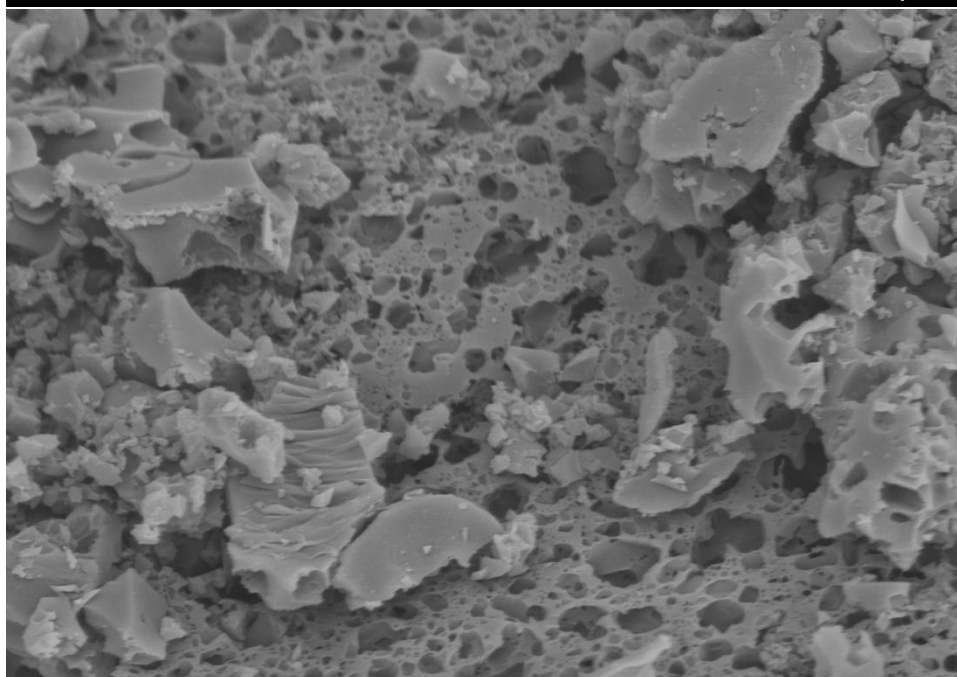

Clariant SU7000 5.00kV 6.8mm x5.00k UD+LD+MD 09/16/2024 10.0µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: KJo-0178 2/3 1-5m 800C 3C/m 1h A 2x2.0P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-048023-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

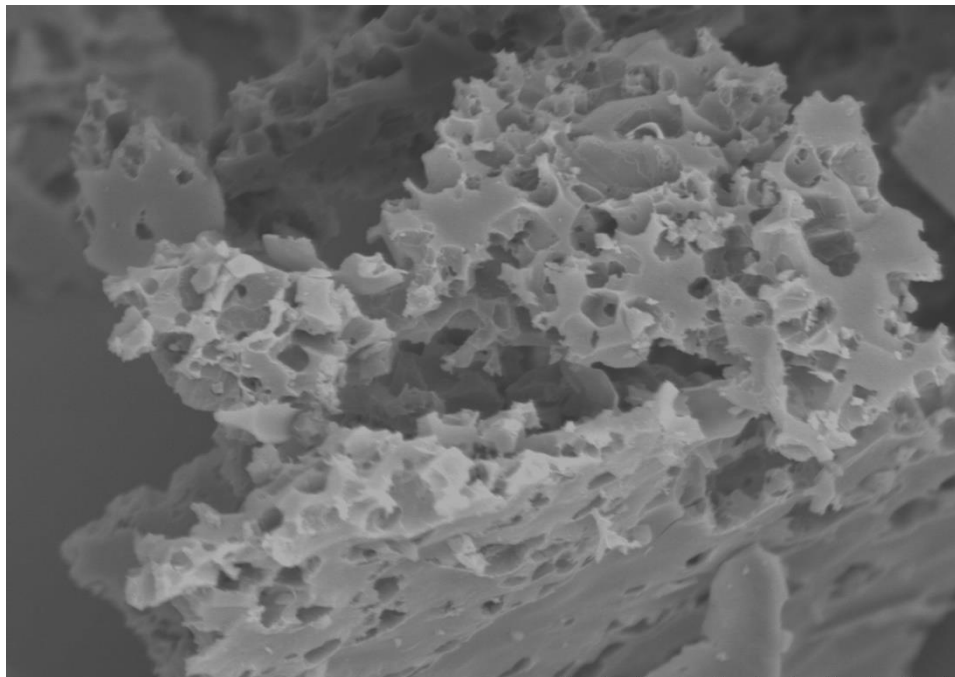

Clariant SU7000 5.00kV 6.8mm x5.00k UD+LD+MD 09/16/2024 10.0µm

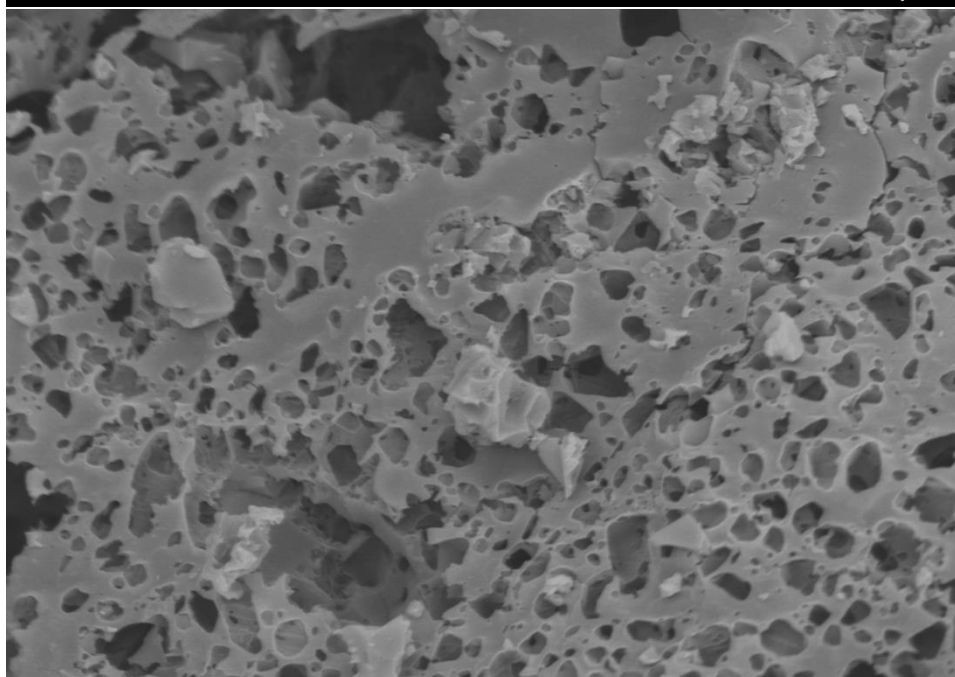


Clariant SU7000 5.00kV 6.9mm x5.00k UD+LD+MD 09/16/2024 10.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: KJo-0178 2/3 1-5m 800C 3C/m 1h A 2x2.0P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-048023-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

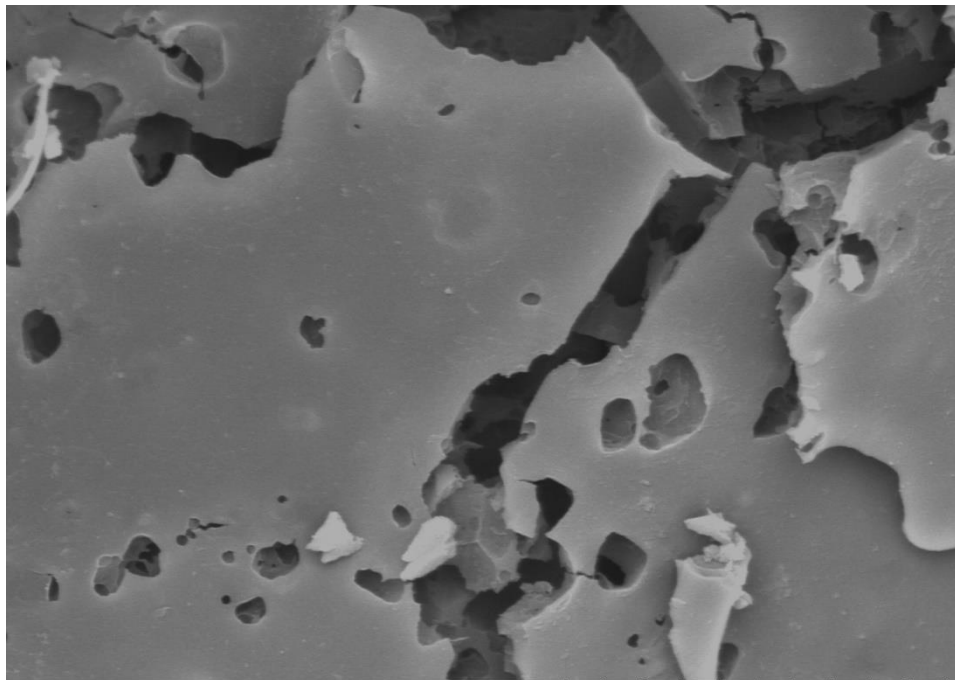

Clariant SU7000 5.00kV 6.8mm x10.0k UD+LD+MD 09/16/2024 5.00µm

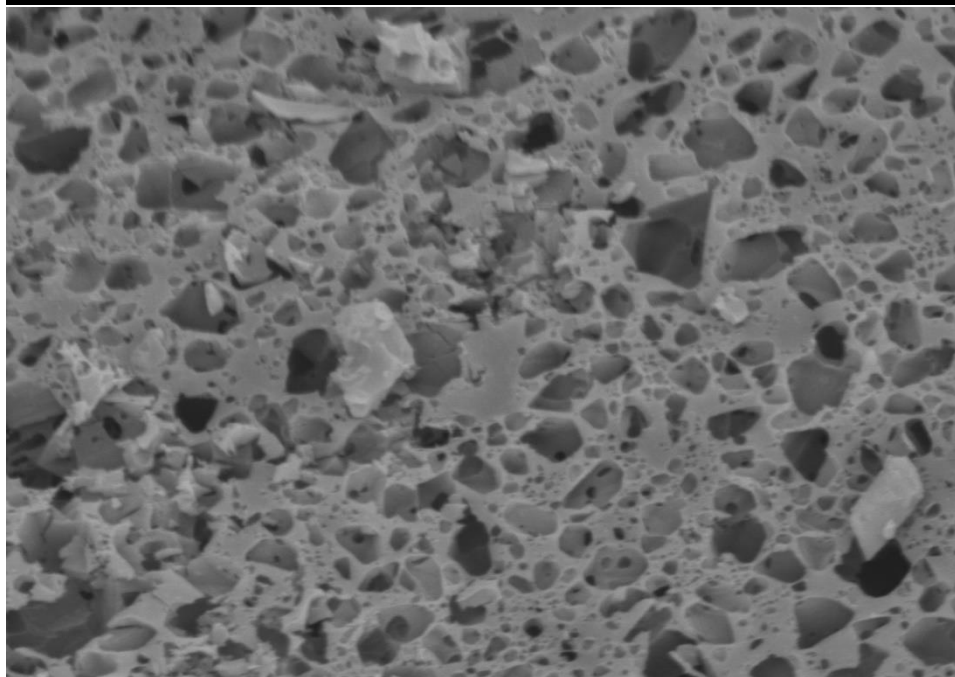

Clariant SU7000 5.00kV 6.8mm x10.0k UD+LD+MD 09/16/2024 5.00µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: KJo-0178 2/3 1-5m 800C 3C/m 1h A 2x2.0P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-048023-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

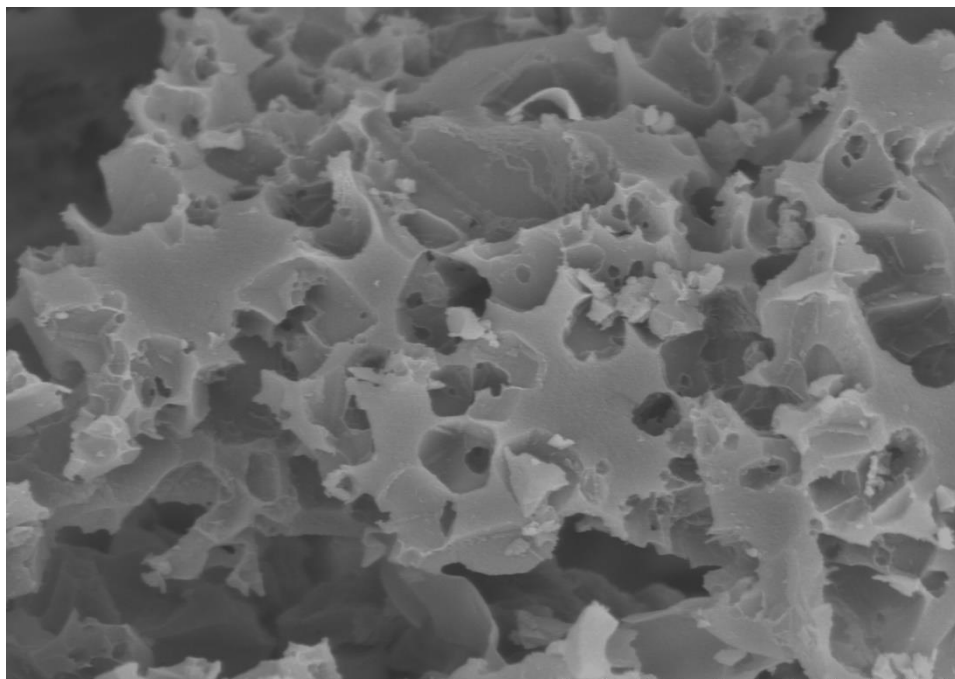

Clariant SU7000 5.00kV 6.8mm x10.0k UD+LD+MD 09/16/2024 5.00µm

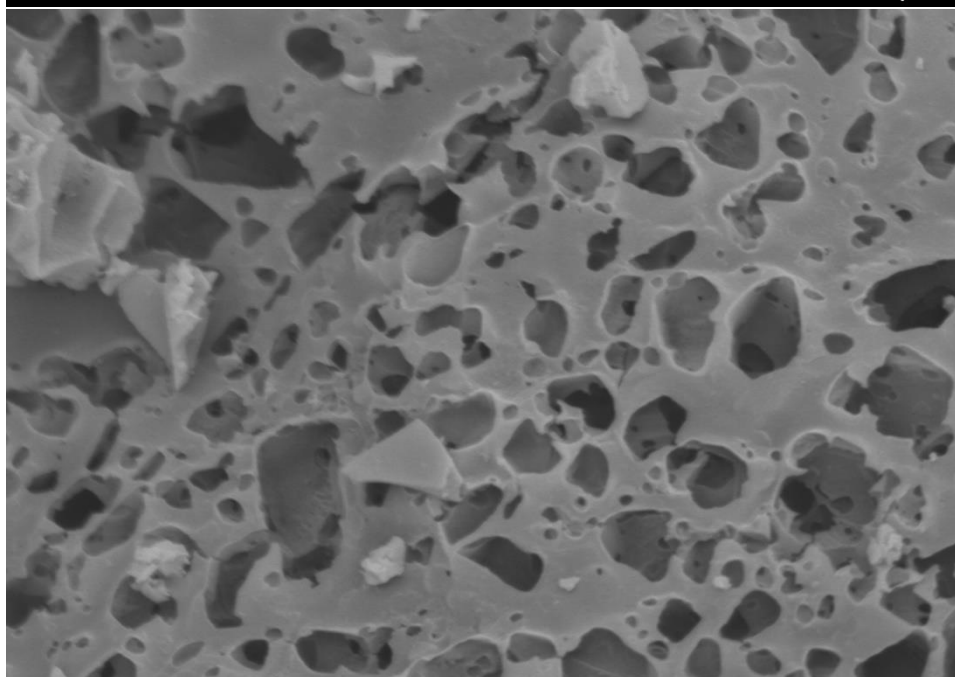

Clariant SU7000 5.00kV 6.9mm x10.0k UD+LD+MD 09/16/2024 5.00µm

SCANNING ELECTRON MICROSCOPE (SEM)


Sample name: KJo-0178 2/3 1-5m 800C 3C/m 1h A 2x2.0P

Ordering customer: Dr. Torsten Busch


Dept./Plant: Curia Germany GmbH

Order number: 24-048023-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

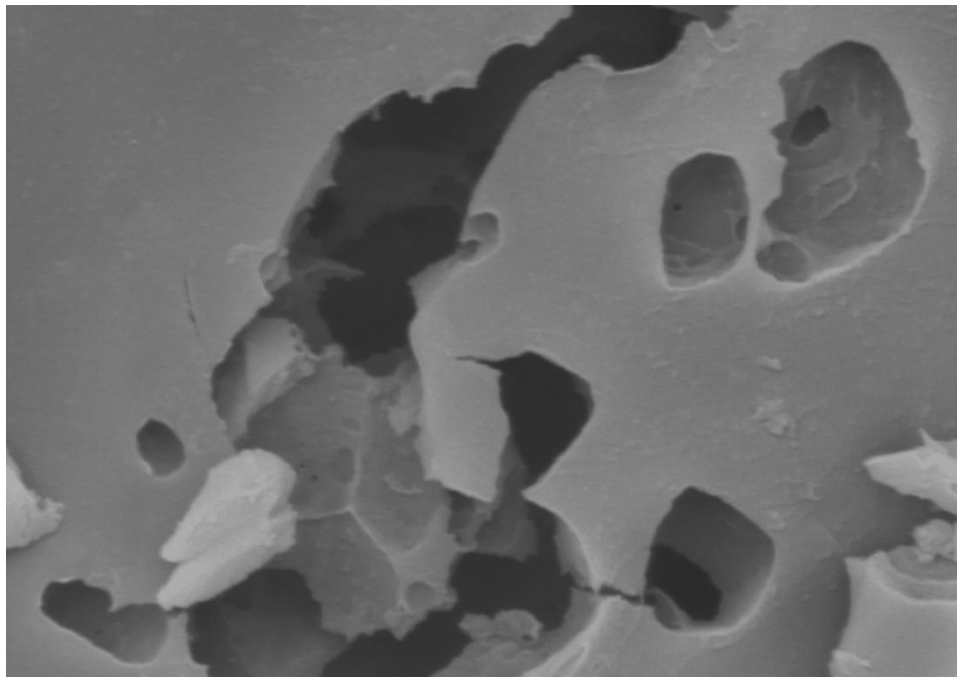

Clariant SU7000 5.00kV 6.8mm x25.0k UD+LD+MD 09/16/2024 2.00µm

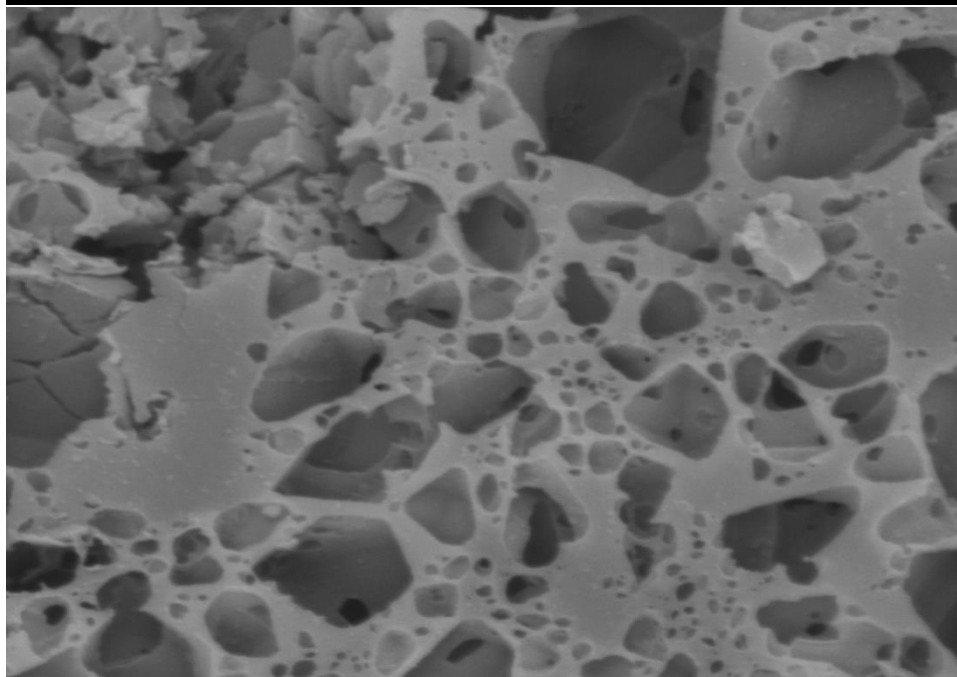


Clariant SU7000 5.00kV 6.9mm x25.0k UD+LD+MD 09/16/2024 2.00µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: KJo-0178 2/3 1-5m 800C 3C/m 1h A 2x2.0P
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-048023-5

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

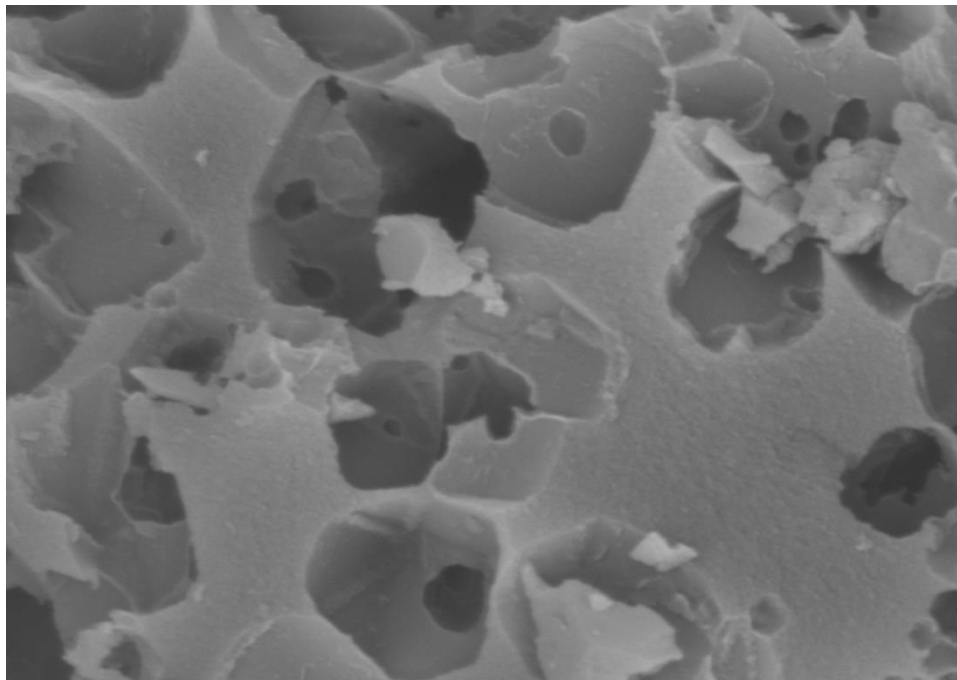

Clariant SU7000 5.00kV 6.8mm x25.0k UD+LD+MD 09/16/2024 2.00µm

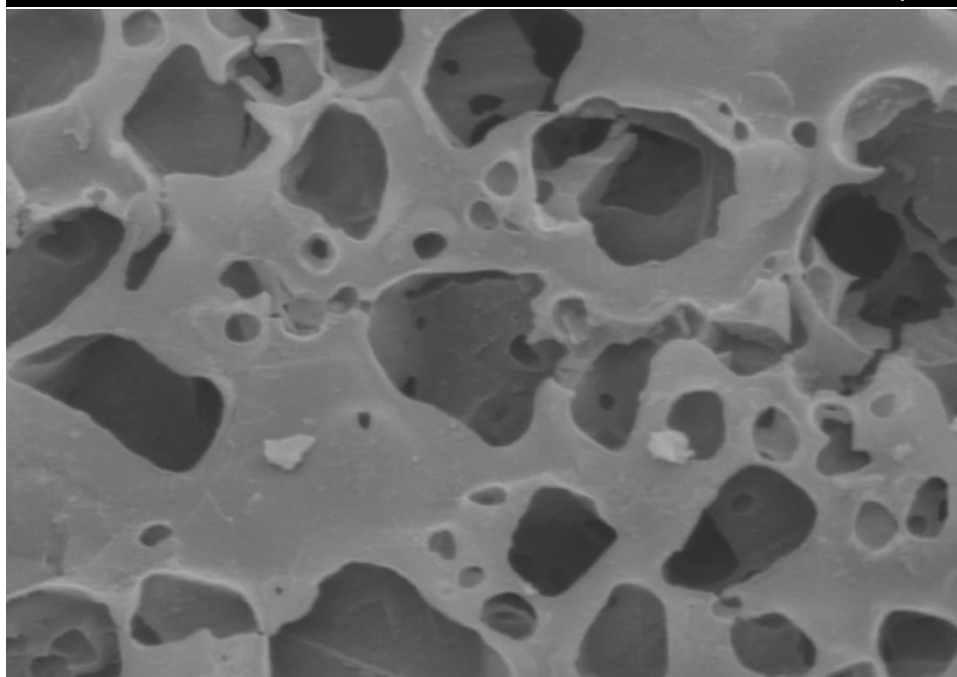

Clariant SU7000 5.00kV 6.9mm x25.0k UD+LD+MD 09/16/2024 2.00µm