



SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB2962A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047529-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

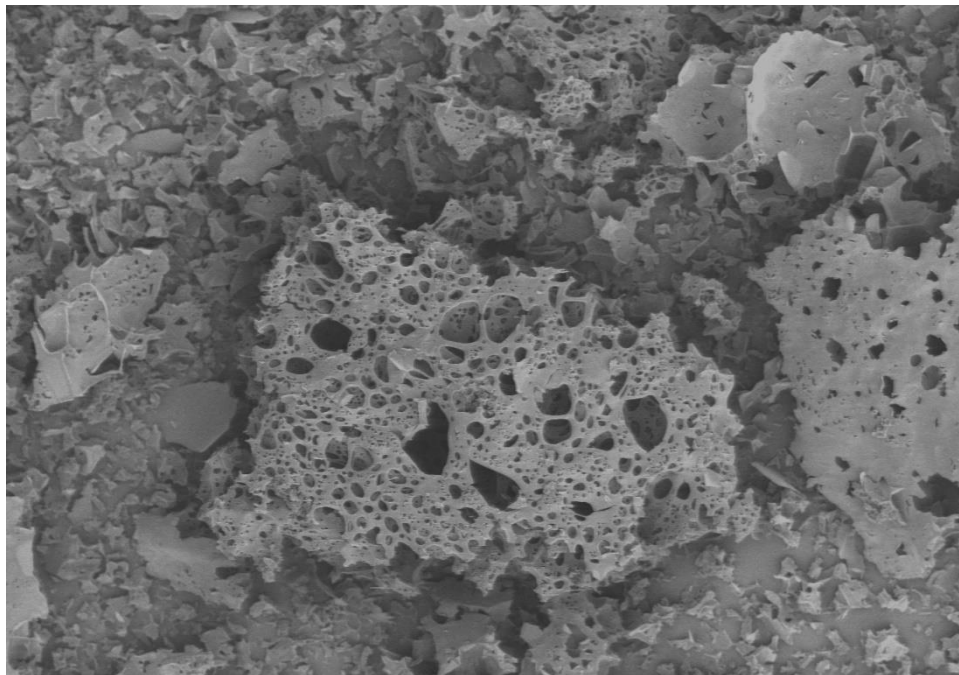

Clariant SU7000 5.00kV 6.5mm x100 UD+LD+MD 07/10/2024 500µm

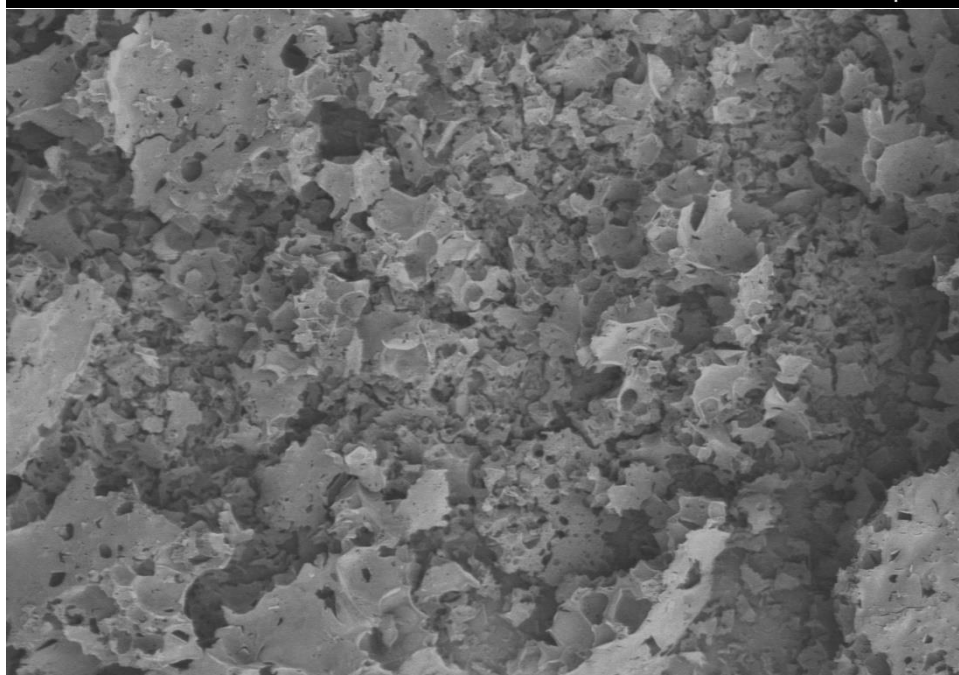


Clariant SU7000 5.00kV 6.5mm x100 UD+LD+MD 07/10/2024 500µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB2962A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047529-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

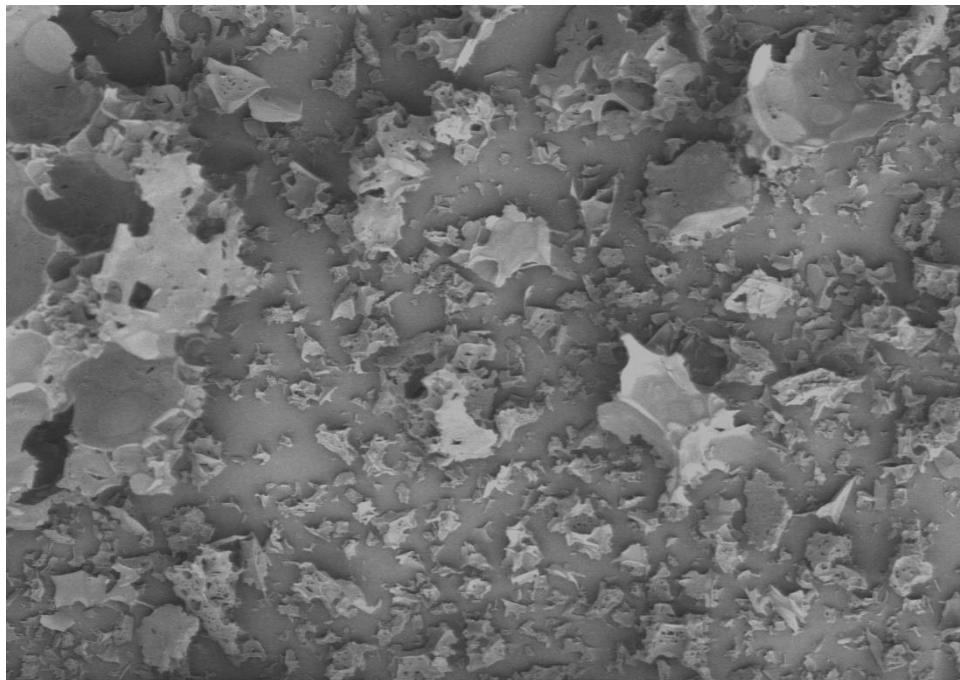

Clariant SU7000 5.00kV 7.1mm x100 UD+LD+MD 07/10/2024 500µm

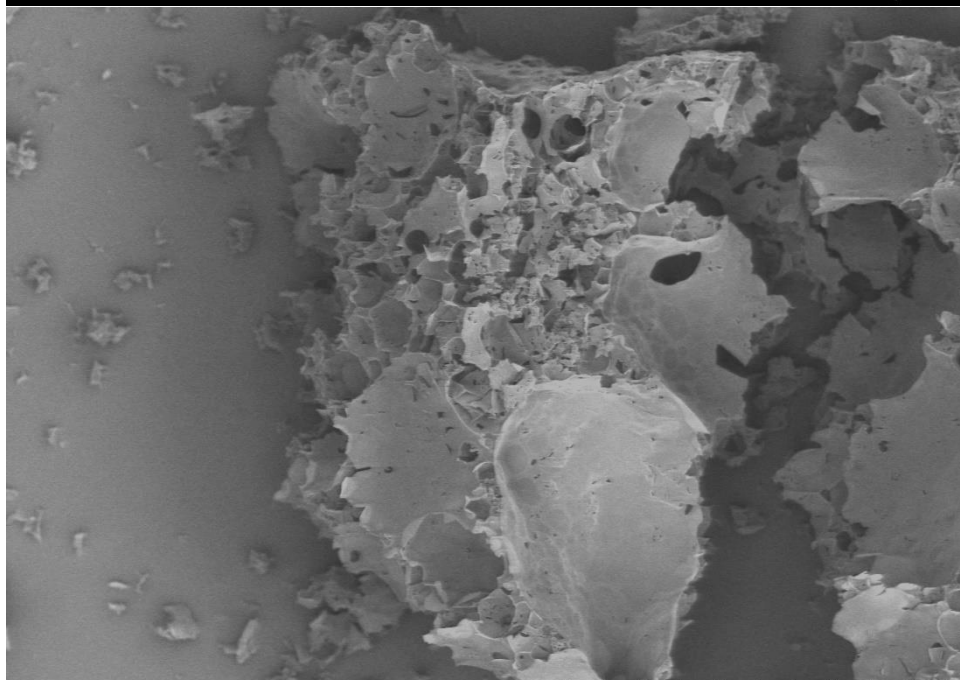


Clariant SU7000 5.00kV 6.2mm x100 UD+LD+MD 07/10/2024 500µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB2962A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047529-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

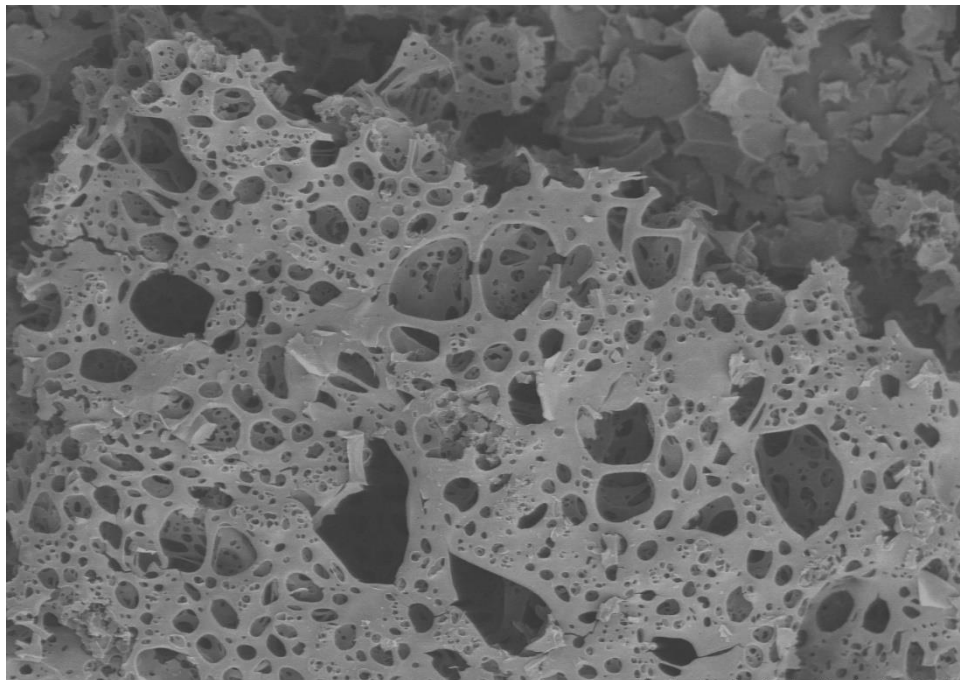

Clariant SU7000 5.00kV 6.5mm x200 UD+LD+MD 07/10/2024 200µm

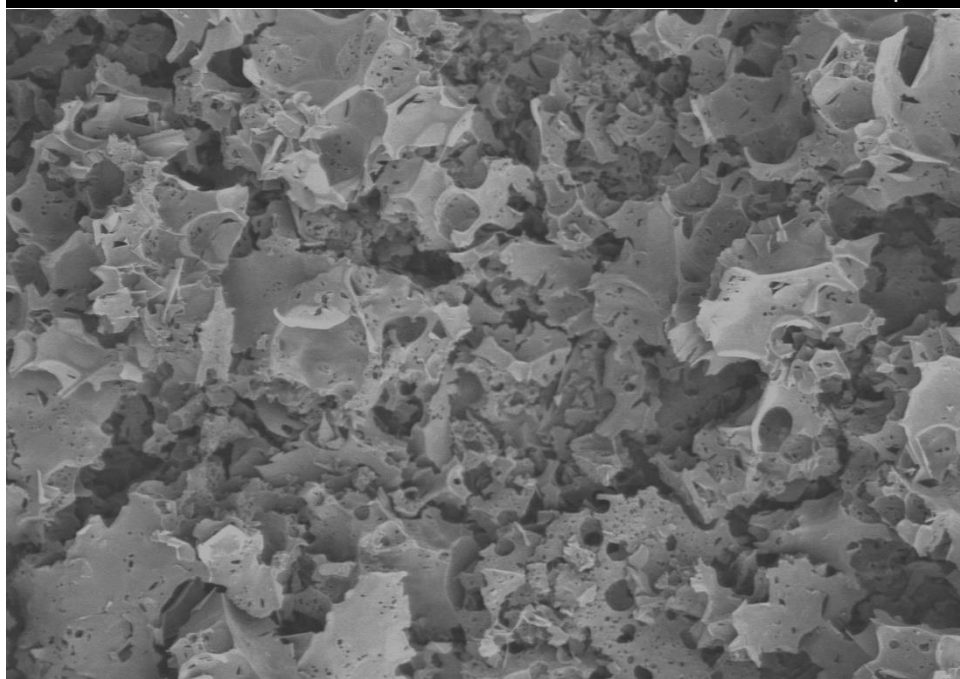


Clariant SU7000 5.00kV 6.7mm x200 UD+LD+MD 07/10/2024 200µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB2962A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047529-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

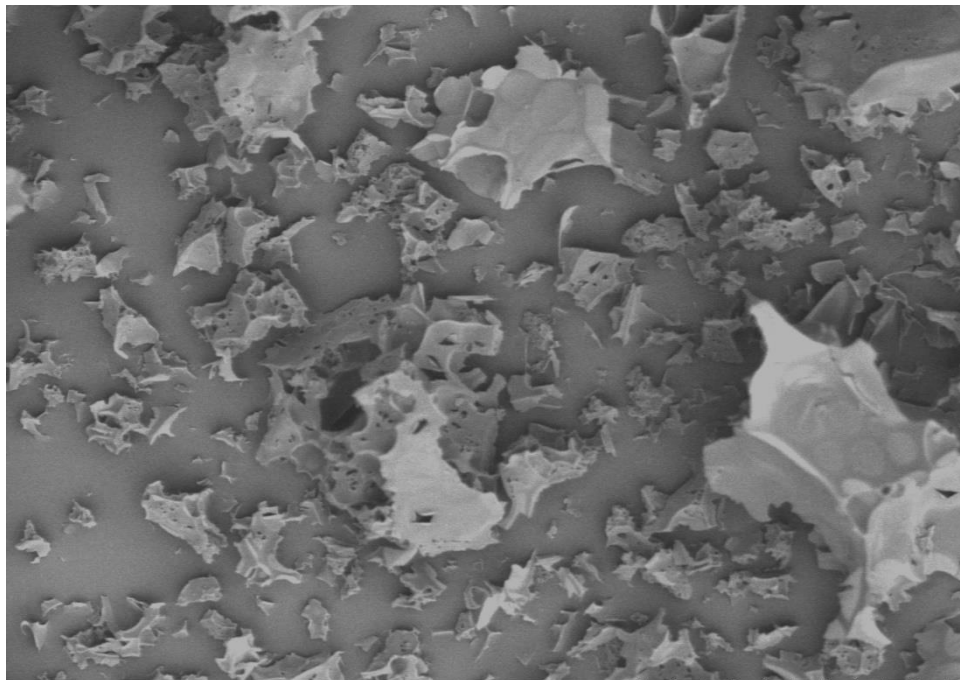

Clariant SU7000 5.00kV 7.0mm x200 UD+LD+MD 07/10/2024 200µm

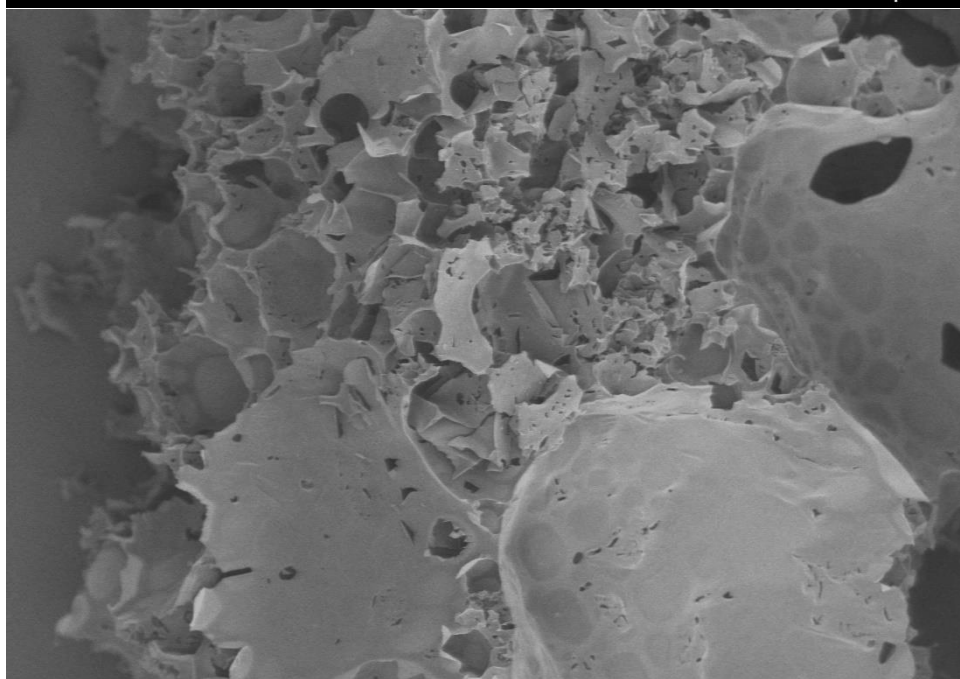


Clariant SU7000 5.00kV 6.2mm x200 UD+LD+MD 07/10/2024 200µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB2962A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047529-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

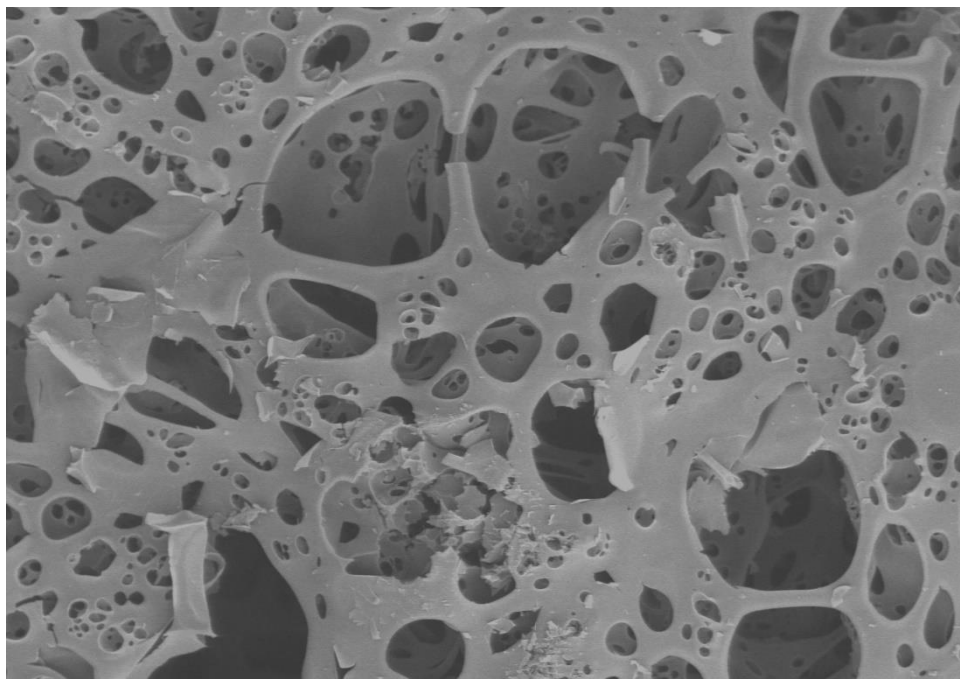

Clariant SU7000 5.00kV 6.5mm x450 UD+LD+MD 07/10/2024 100µm

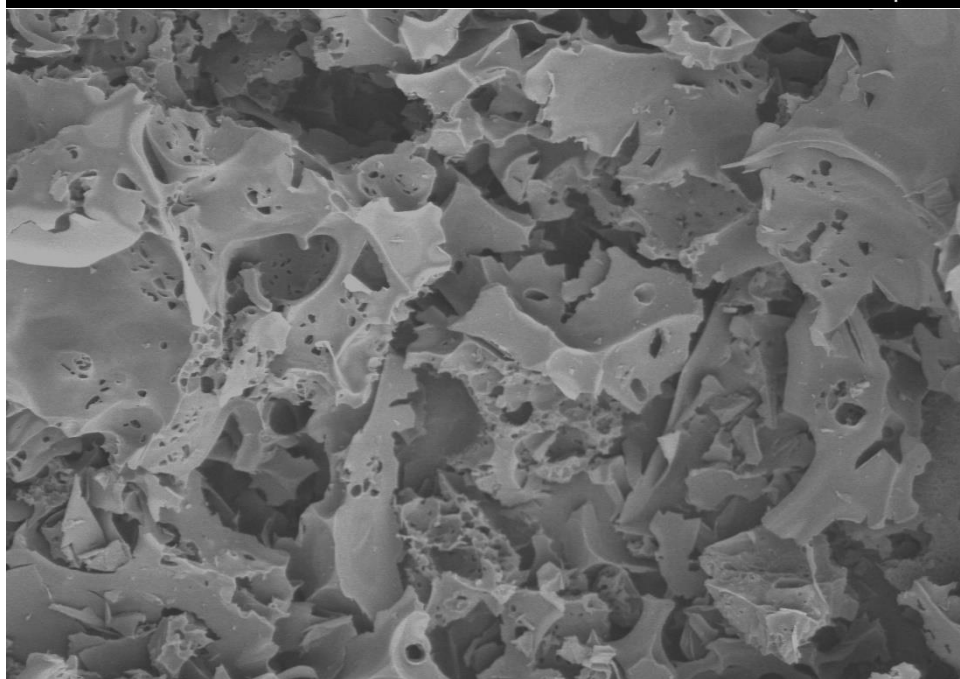


Clariant SU7000 5.00kV 6.8mm x500 UD+LD+MD 07/10/2024 100µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB2962A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047529-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

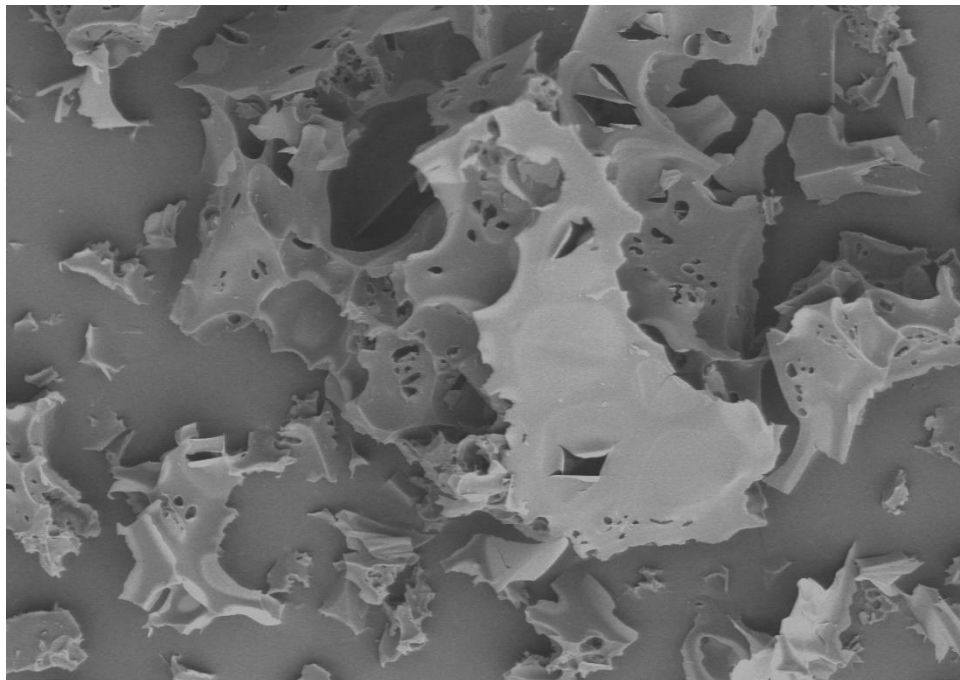

Clariant SU7000 5.00kV 6.8mm x500 UD+LD+MD 07/10/2024 100µm

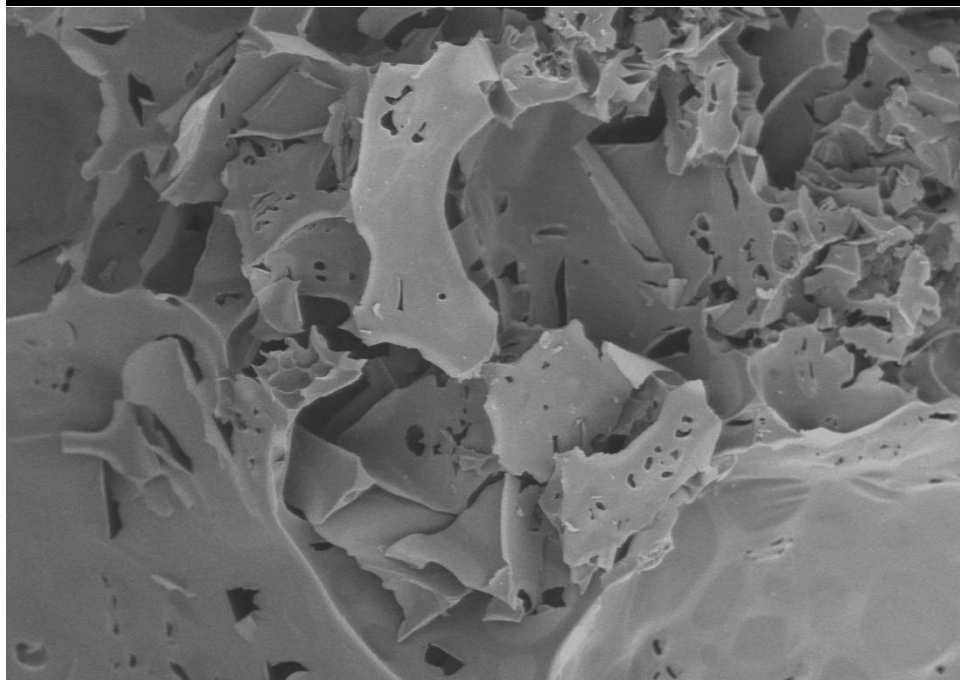


Clariant SU7000 5.00kV 6.2mm x500 UD+LD+MD 07/10/2024 100µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB2962A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047529-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

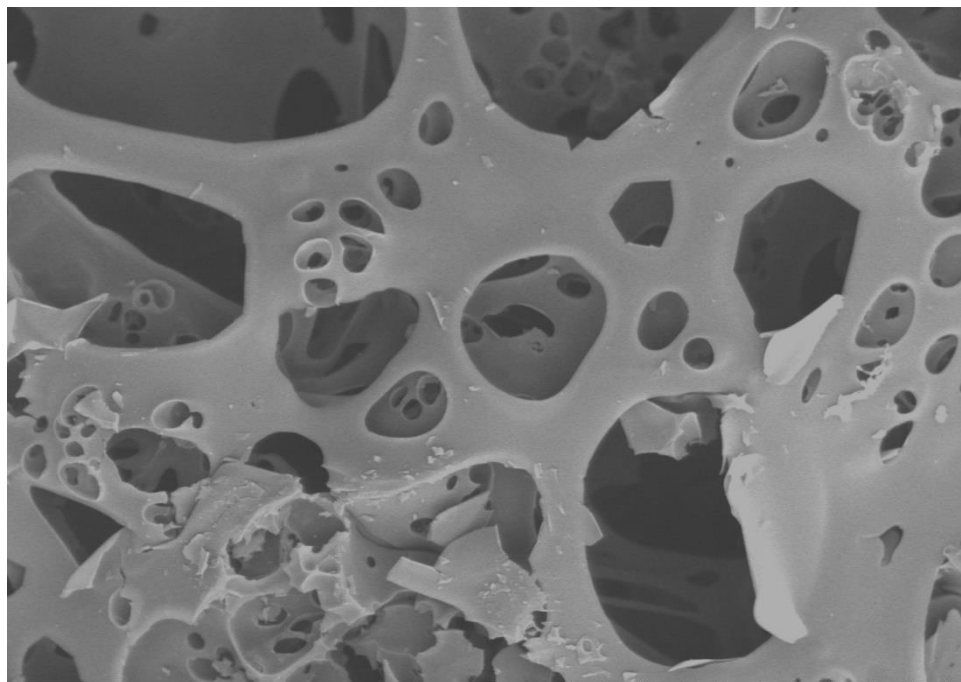

Clariant SU7000 5.00kV 6.5mm x1.00k UD+LD+MD 07/10/2024 50.0µm

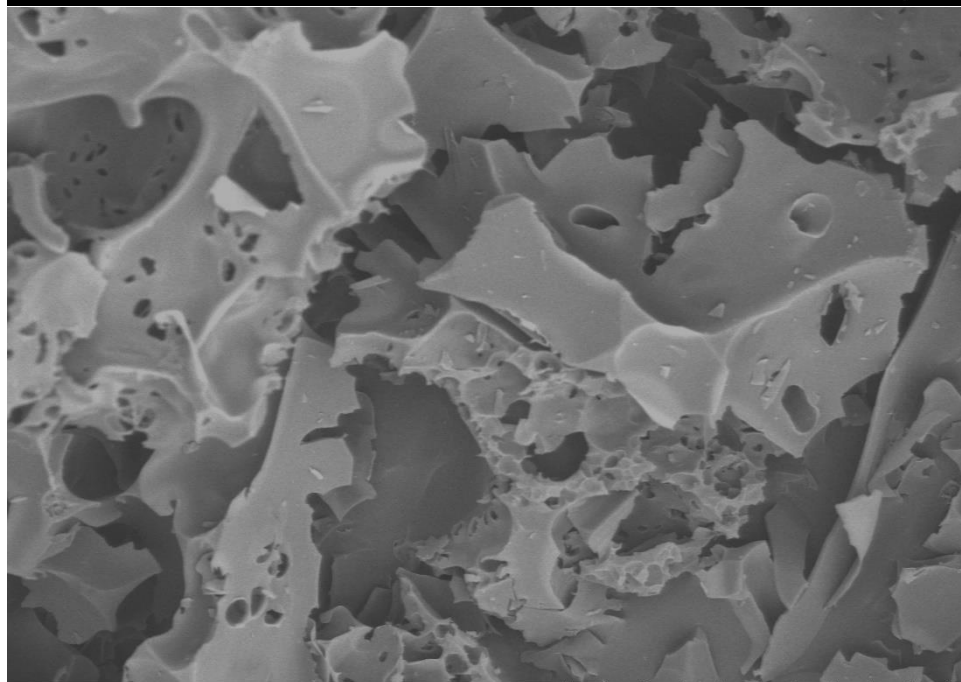


Clariant SU7000 5.00kV 6.9mm x1.00k UD+LD+MD 07/10/2024 50.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB2962A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047529-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

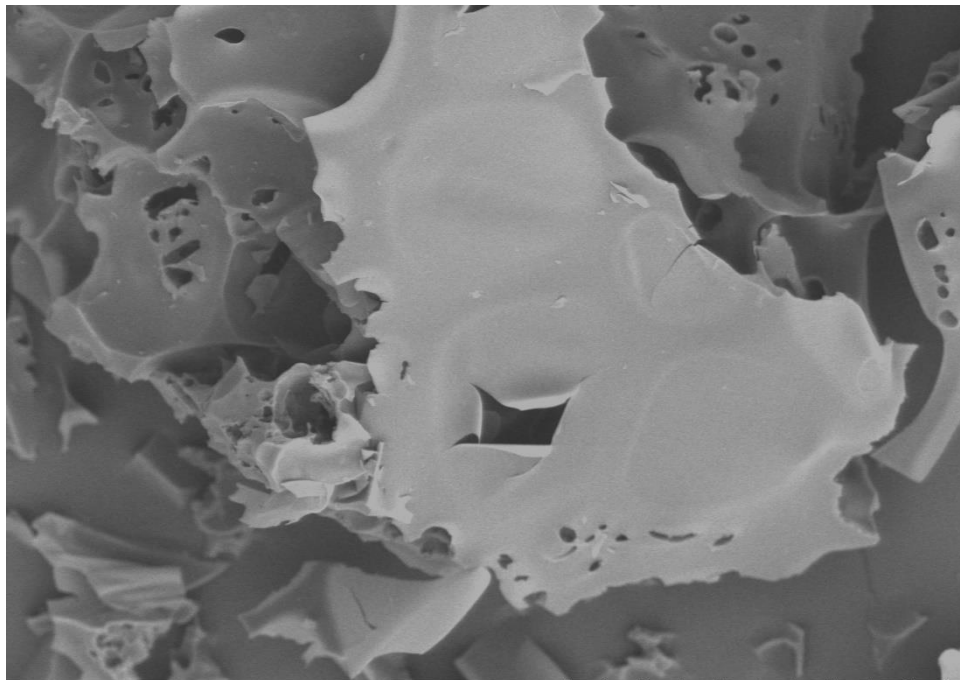

Clariant SU7000 5.00kV 6.7mm x1.00k UD+LD+MD 07/10/2024 50.0µm

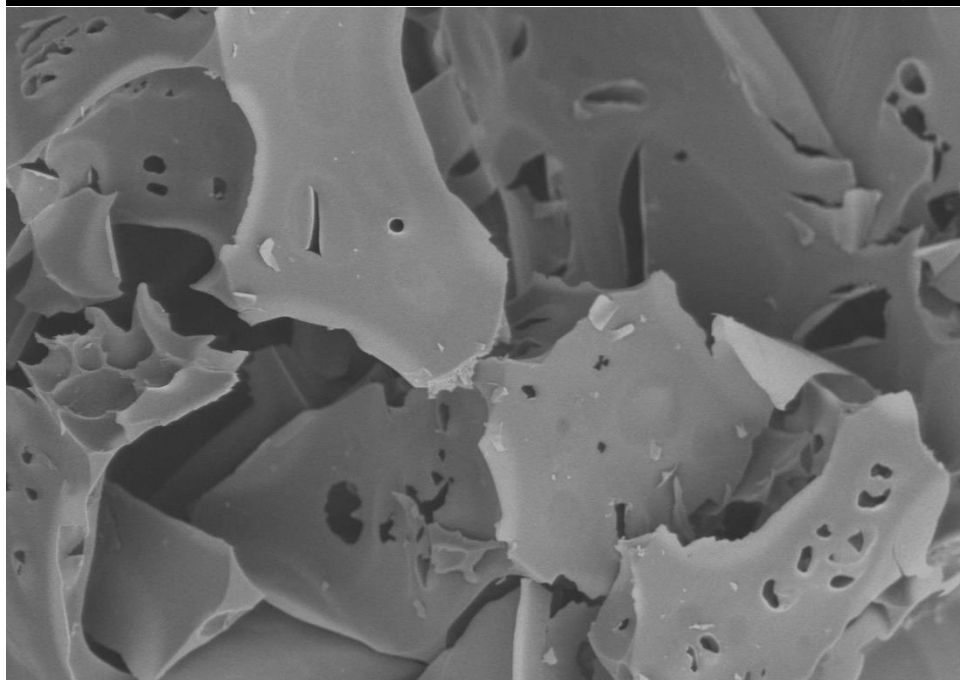


Clariant SU7000 5.00kV 6.2mm x1.00k UD+LD+MD 07/10/2024 50.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB2962A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047529-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

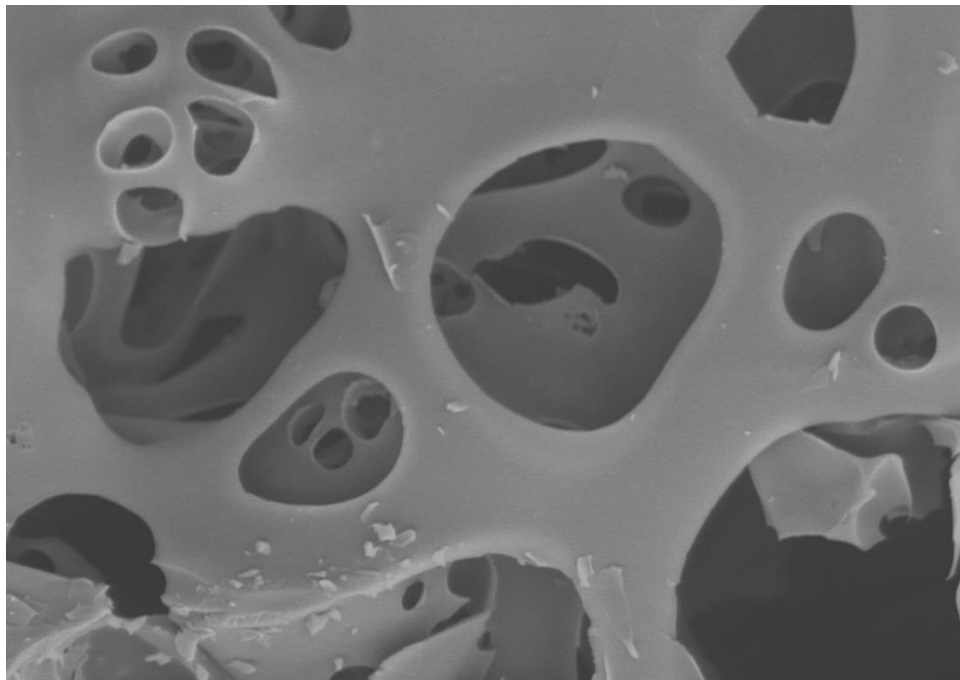

Clariant SU7000 5.00kV 6.5mm x2.00k UD+LD+MD 07/10/2024 20.0µm

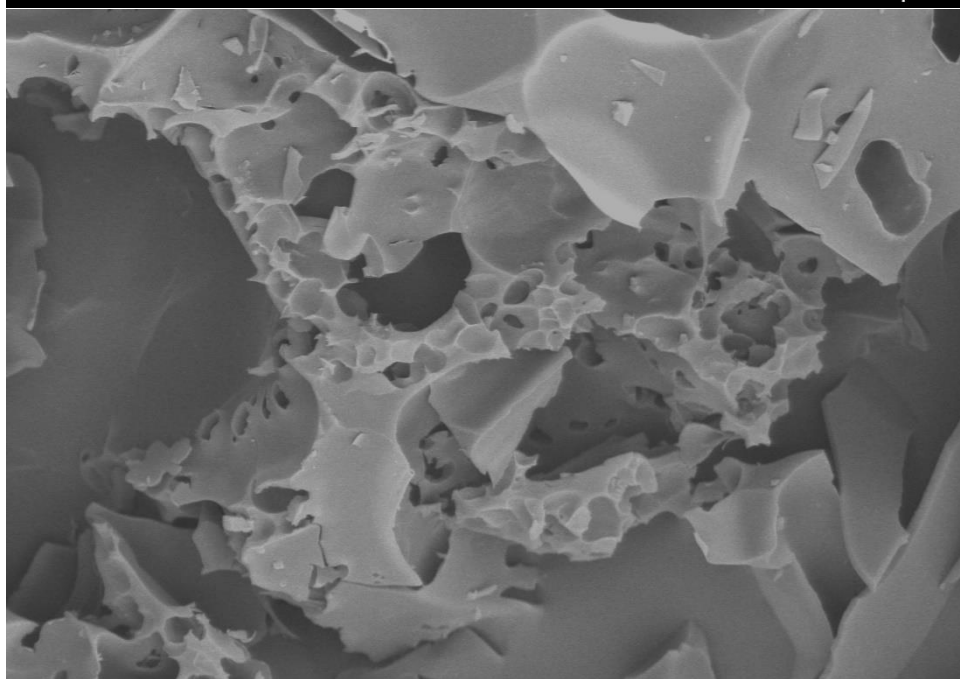


Clariant SU7000 5.00kV 6.9mm x2.00k UD+LD+MD 07/10/2024 20.0µm

SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB2962A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047529-1


Sample treatment: The sample was subjected to platinum sputter coating and then measured.

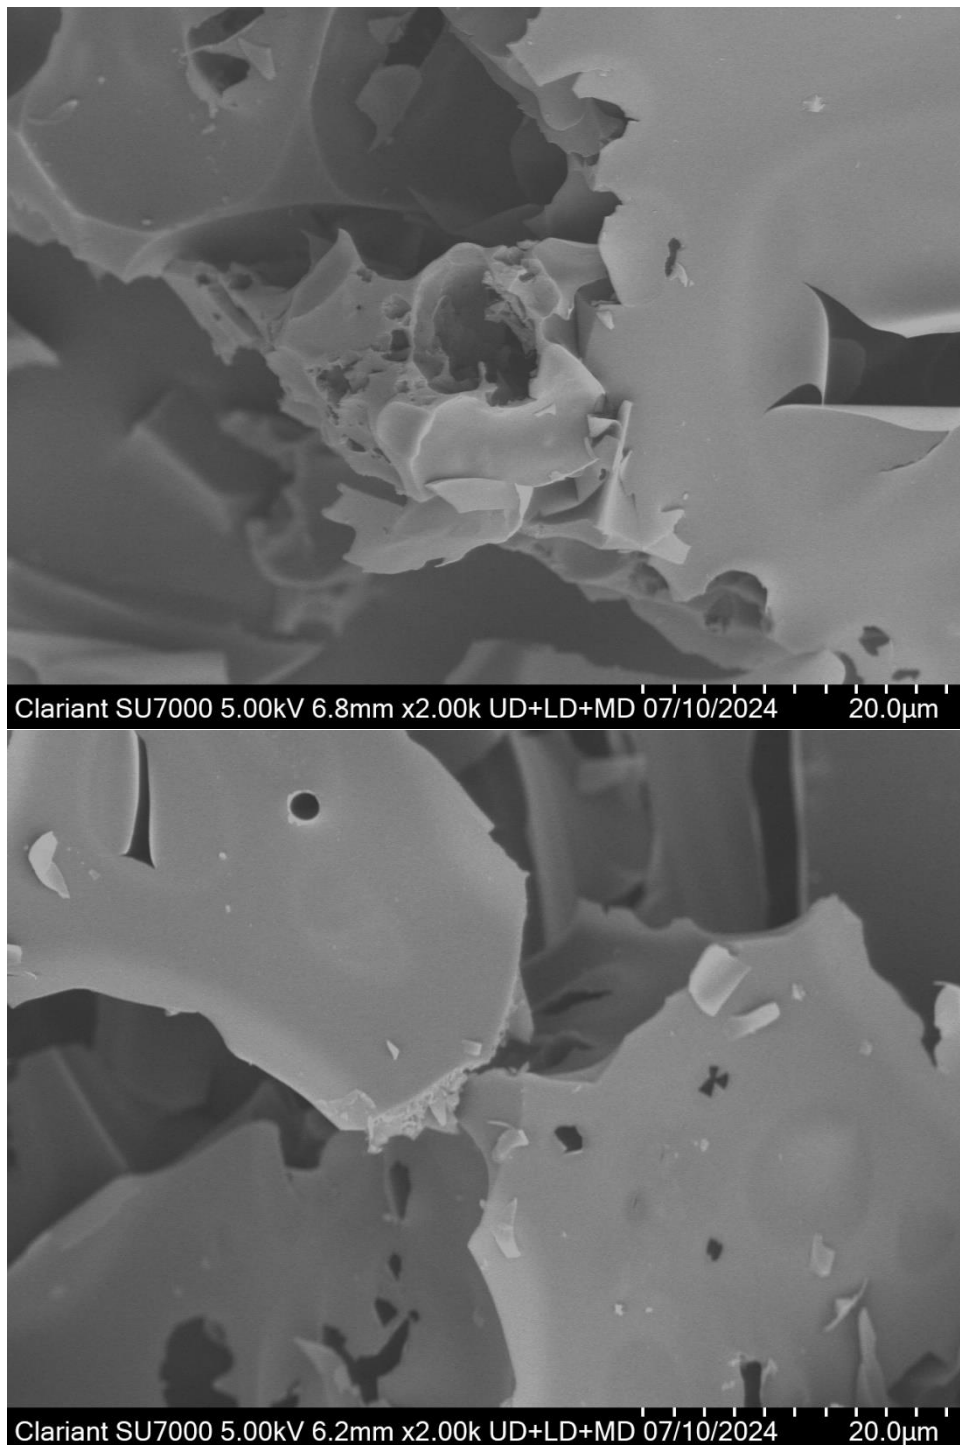


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB2962A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047529-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

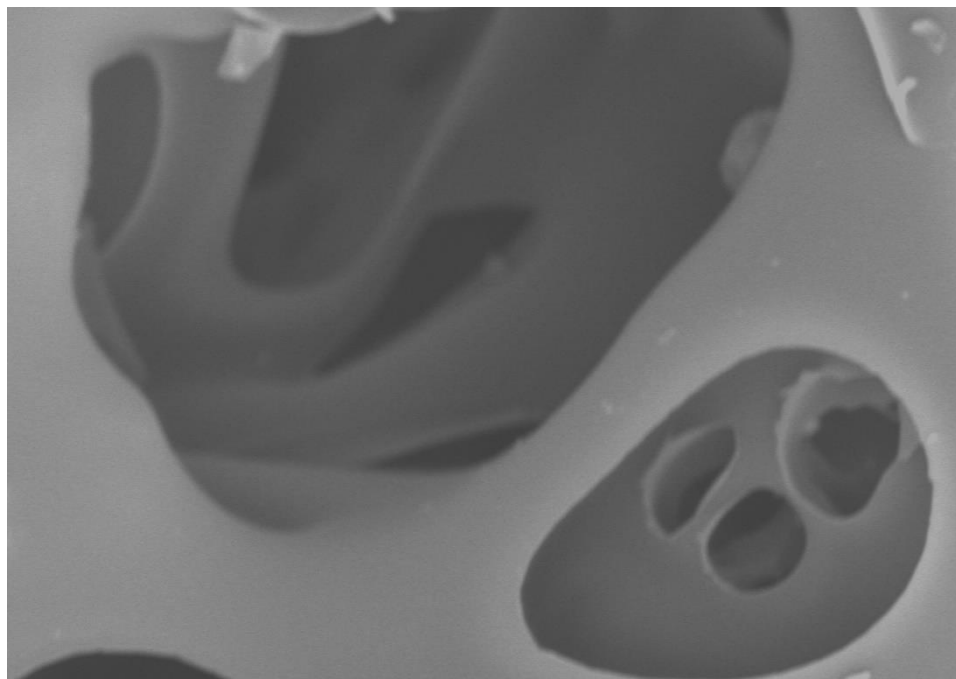

Clariant SU7000 5.00kV 6.5mm x5.00k UD+LD+MD 07/10/2024 10.0µm

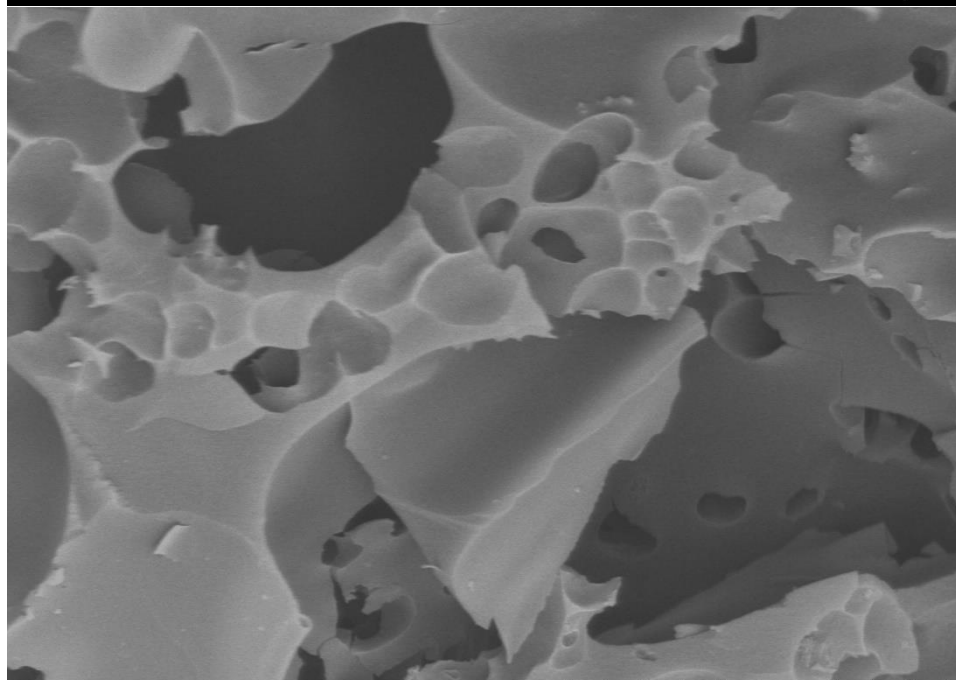


Clariant SU7000 5.00kV 6.9mm x5.00k UD+LD+MD 07/10/2024 10.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB2962A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047529-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

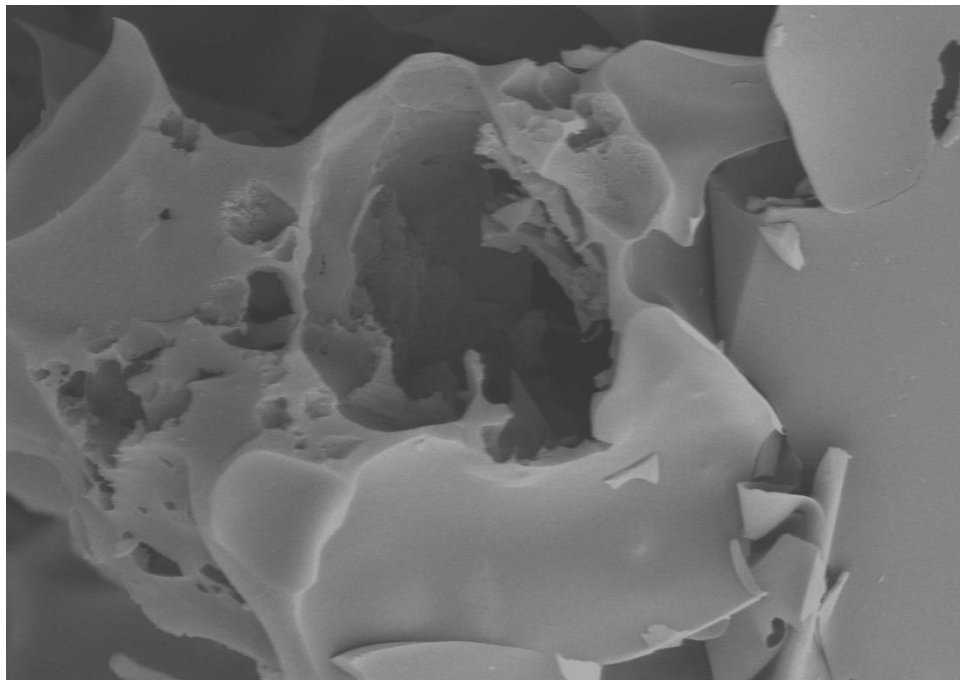

Clariant SU7000 5.00kV 6.8mm x5.00k UD+LD+MD 07/10/2024 10.0µm

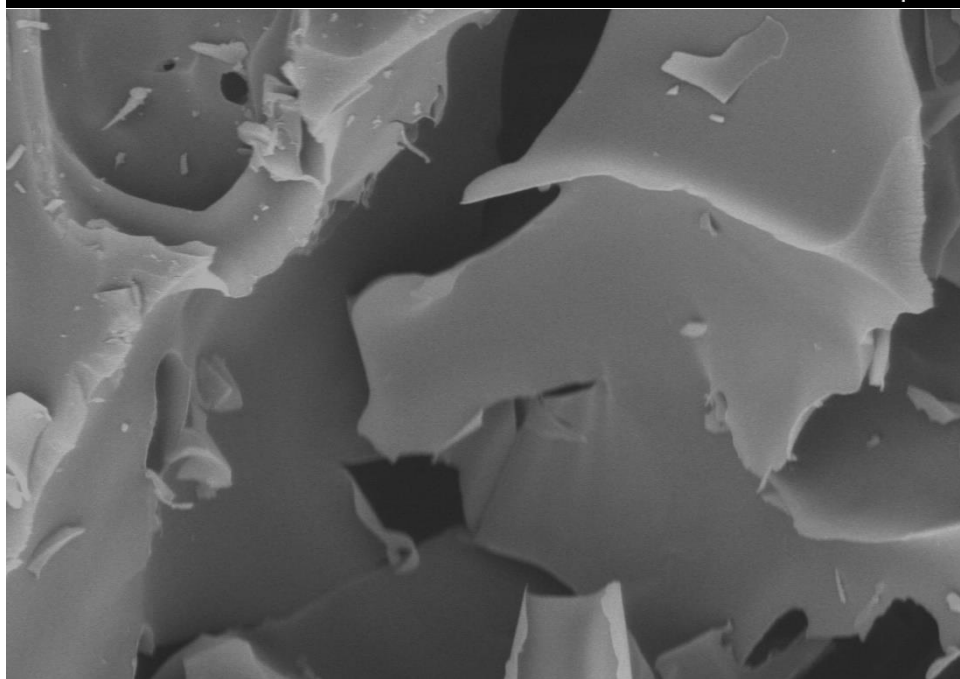


Clariant SU7000 5.00kV 6.4mm x5.00k UD+LD+MD 07/10/2024 10.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB2962A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047529-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

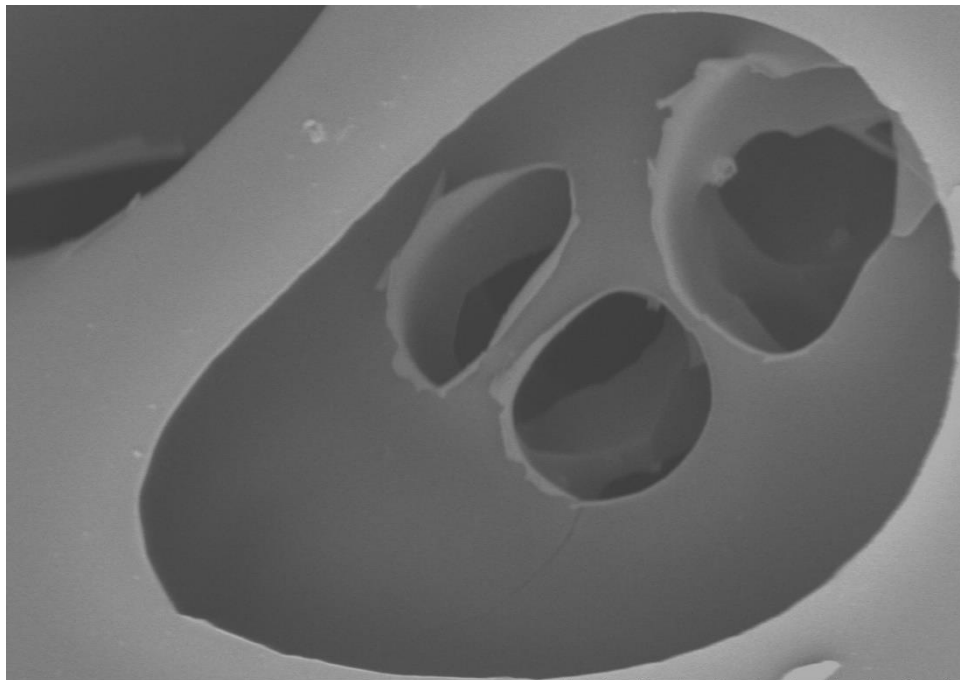

Clariant SU7000 5.00kV 6.6mm x10.0k UD+LD+MD 07/10/2024 5.00µm

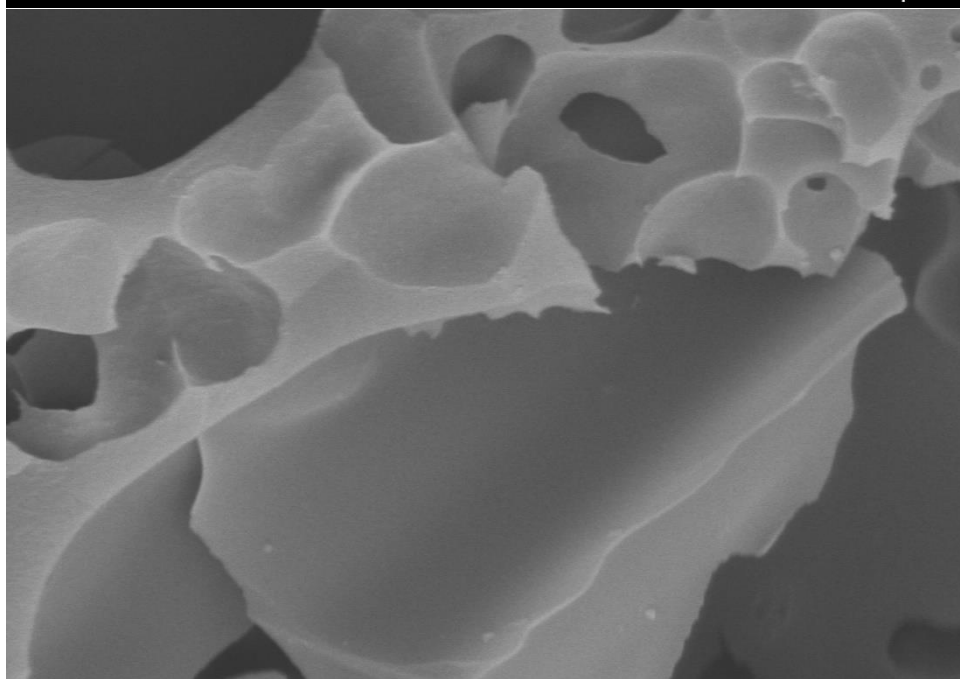


Clariant SU7000 5.00kV 6.9mm x10.0k UD+LD+MD 07/10/2024 5.00µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB2962A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047529-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

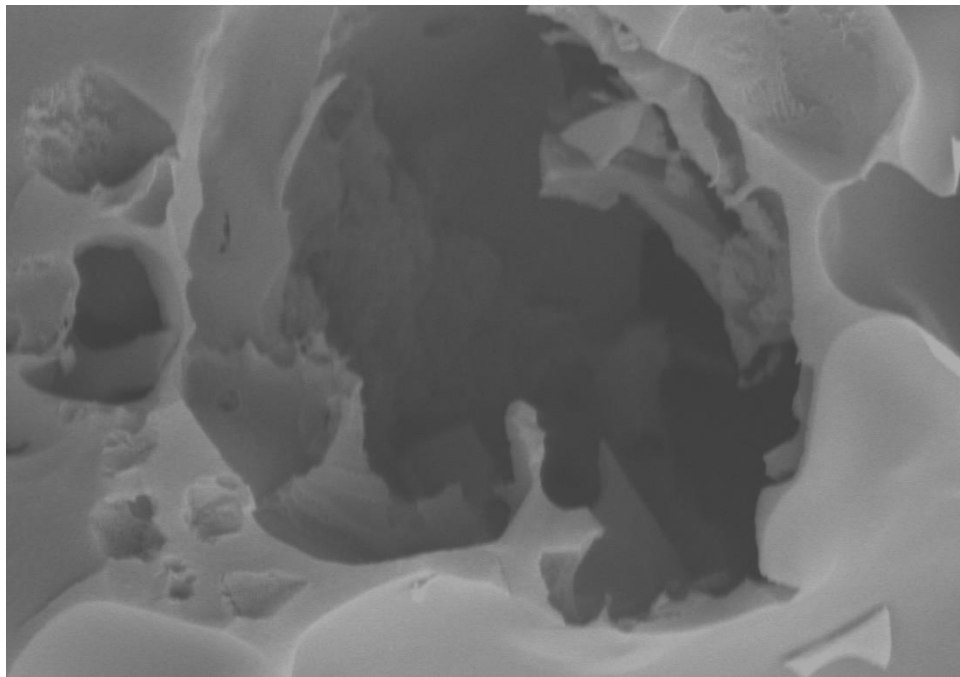

Clariant SU7000 5.00kV 6.8mm x10.0k UD+LD+MD 07/10/2024 5.00µm

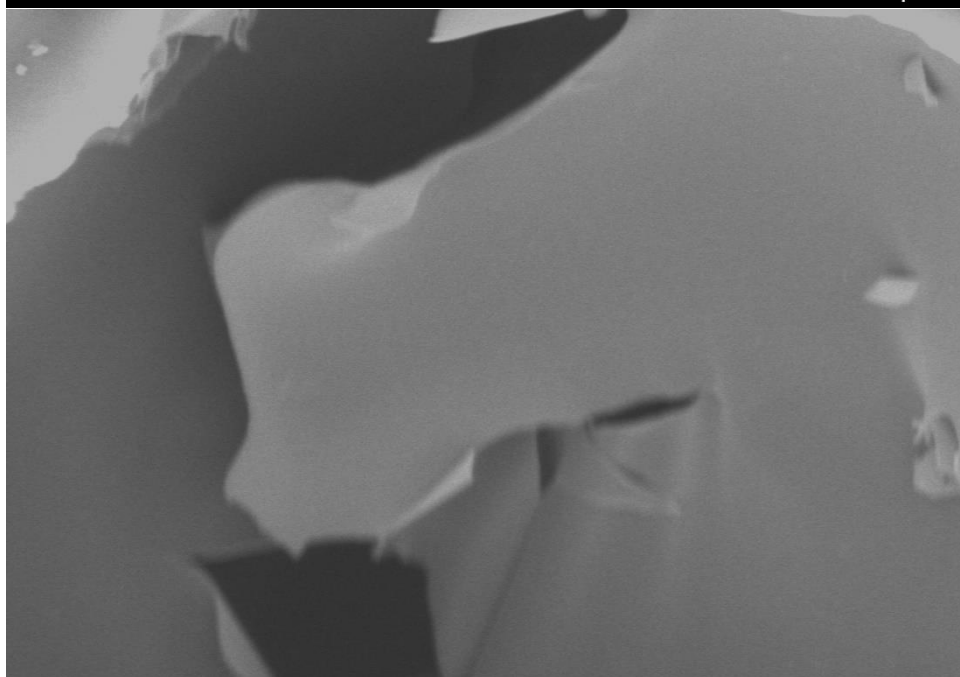


Clariant SU7000 5.00kV 6.4mm x10.0k UD+LD+MD 07/10/2024 5.00µm

SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB2962A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047529-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

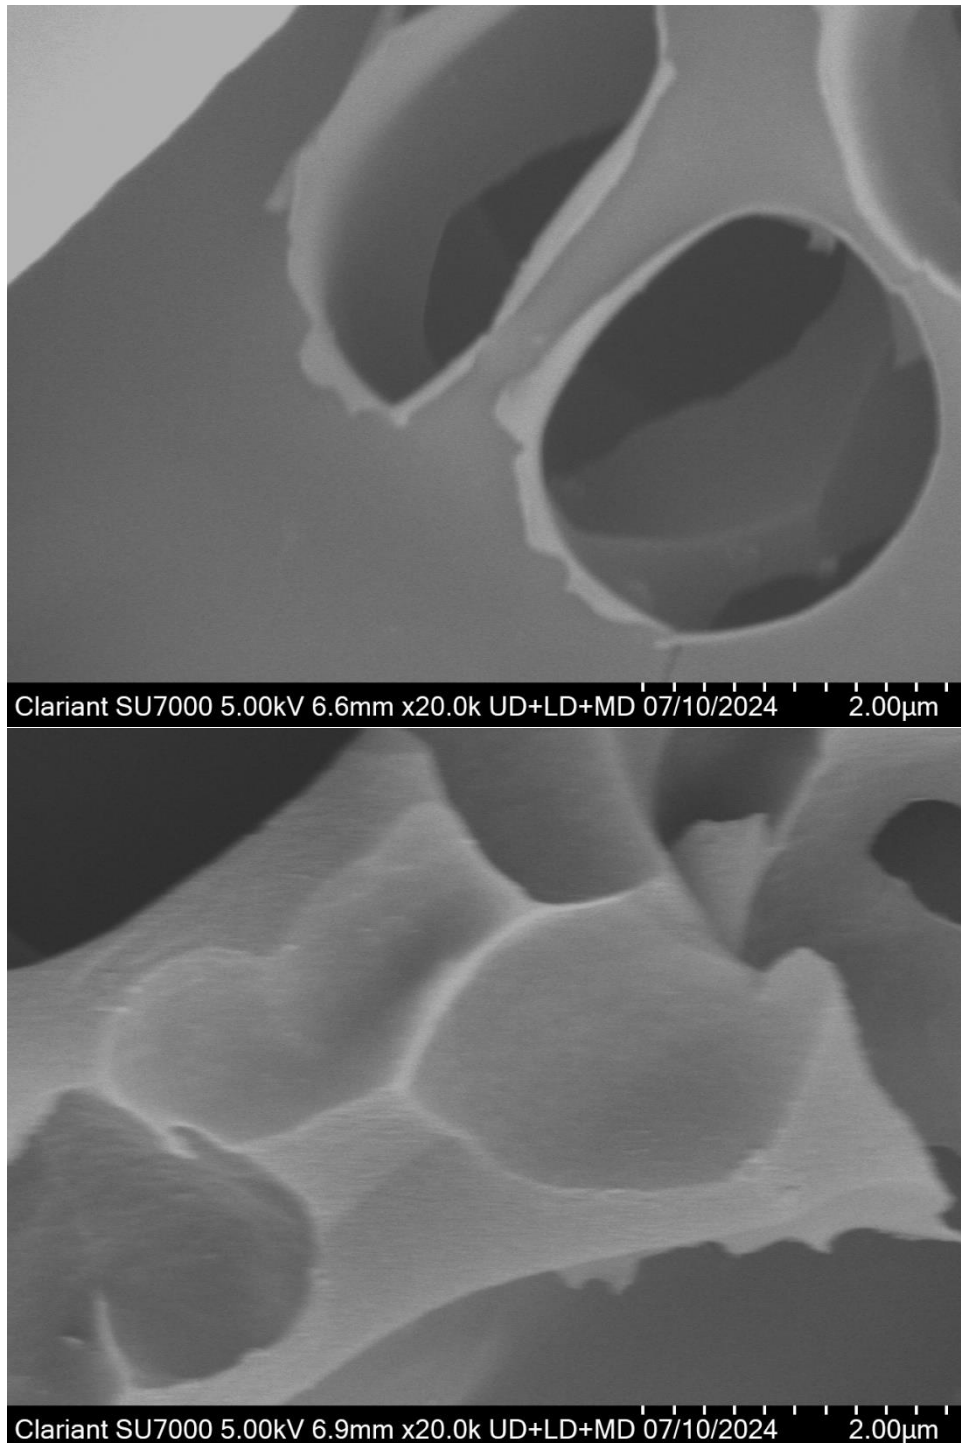

SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: MB2962A
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047529-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

