



SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-1
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047592-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

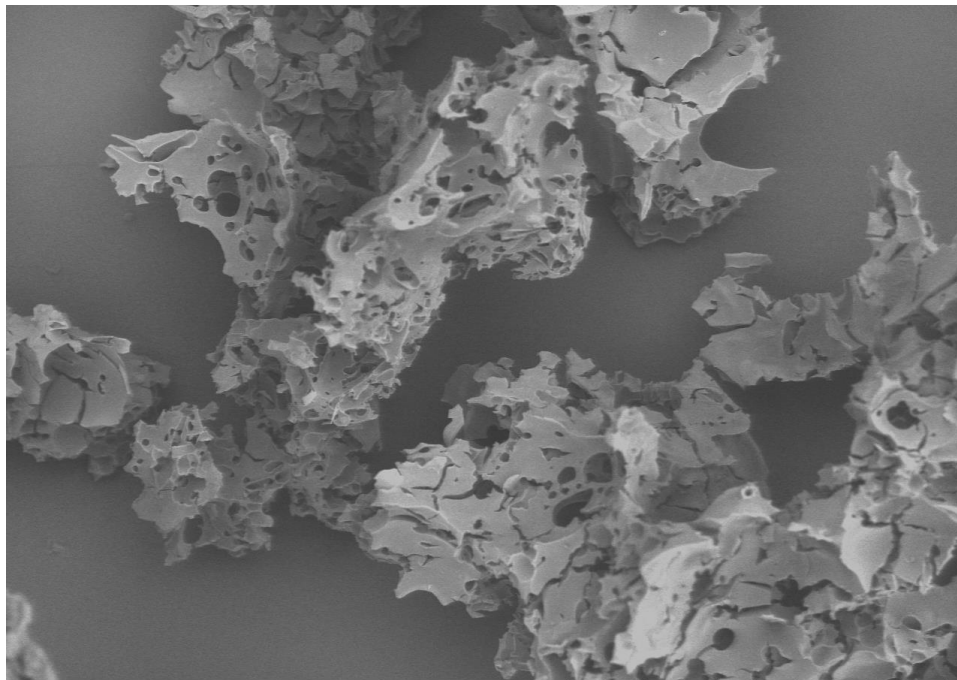

Clariant SU7000 5.00kV 5.1mm x100 UD+LD+MD 07/17/2024 500µm

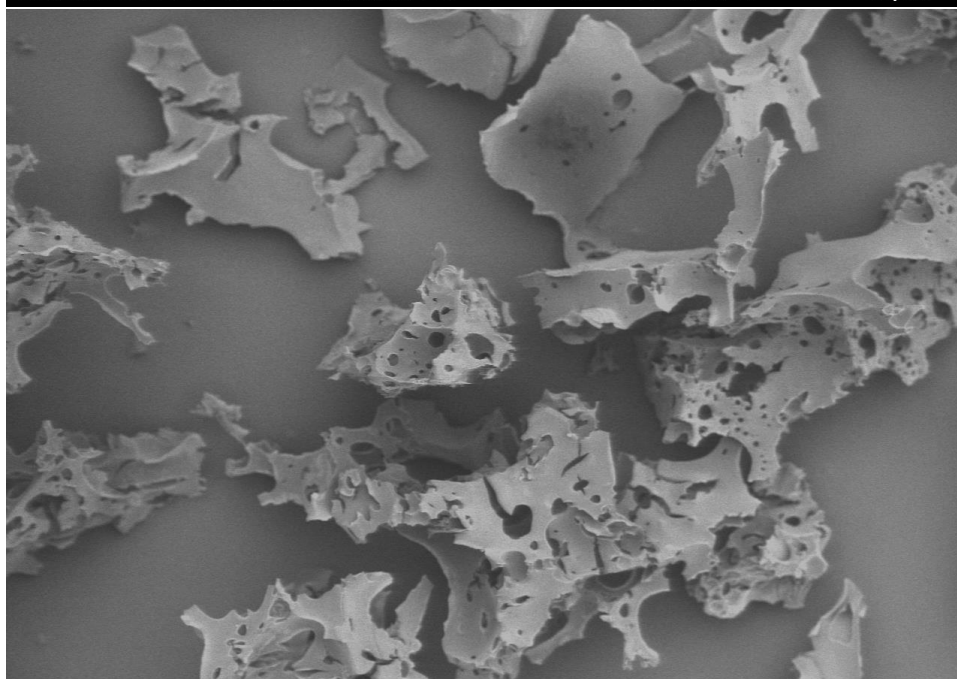


Clariant SU7000 5.00kV 4.9mm x100 UD+LD+MD 07/17/2024 500µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-1
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047592-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

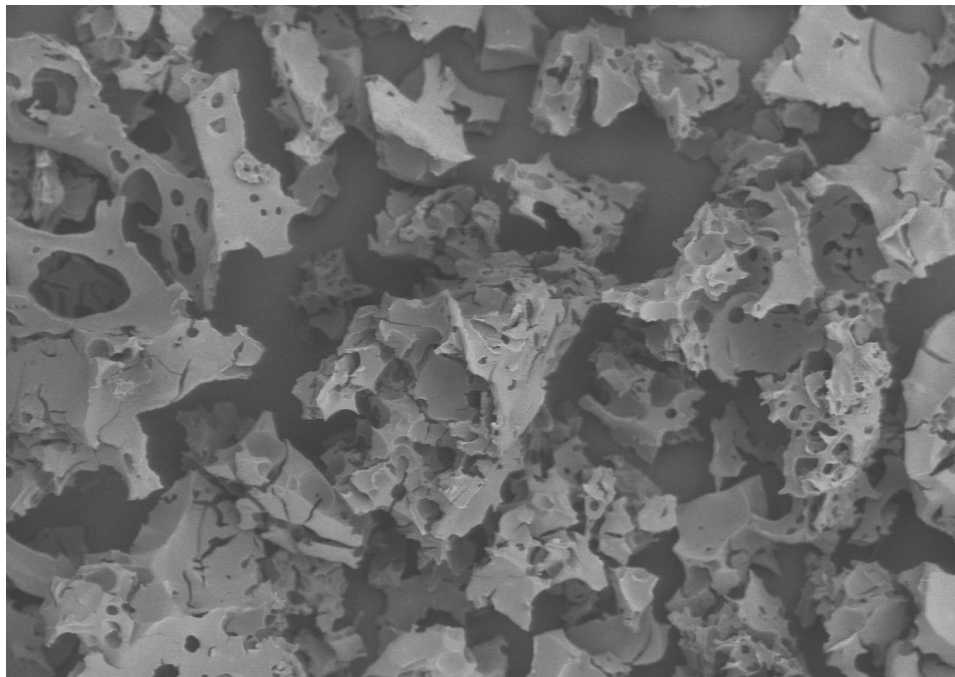

Clariant SU7000 5.00kV 4.8mm x100 UD+LD+MD 07/17/2024 500µm

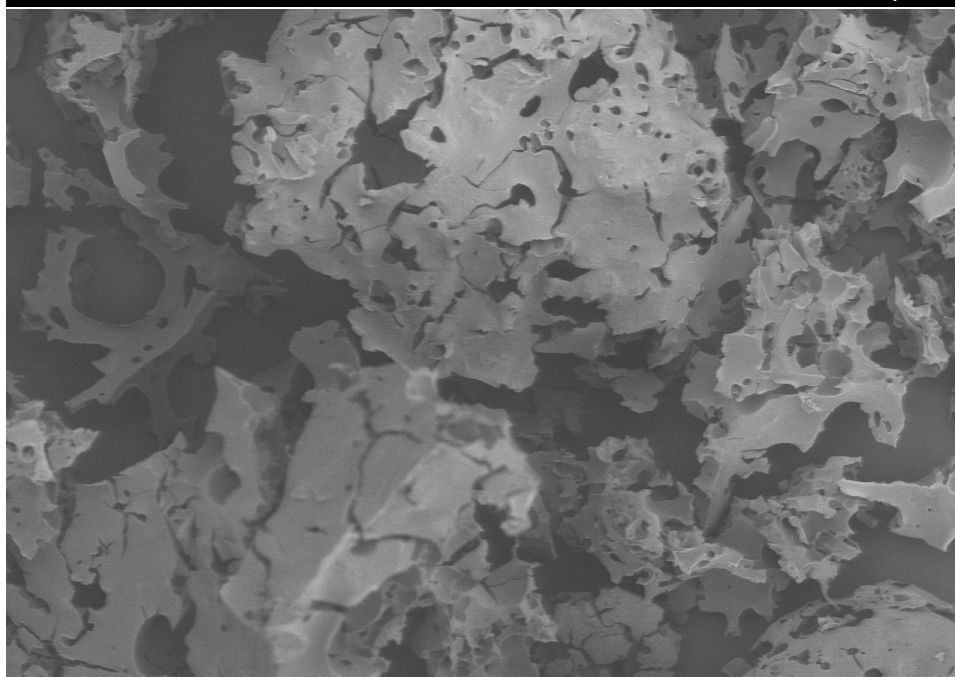


Clariant SU7000 5.00kV 5.1mm x100 UD+LD+MD 07/17/2024 500µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-1
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047592-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

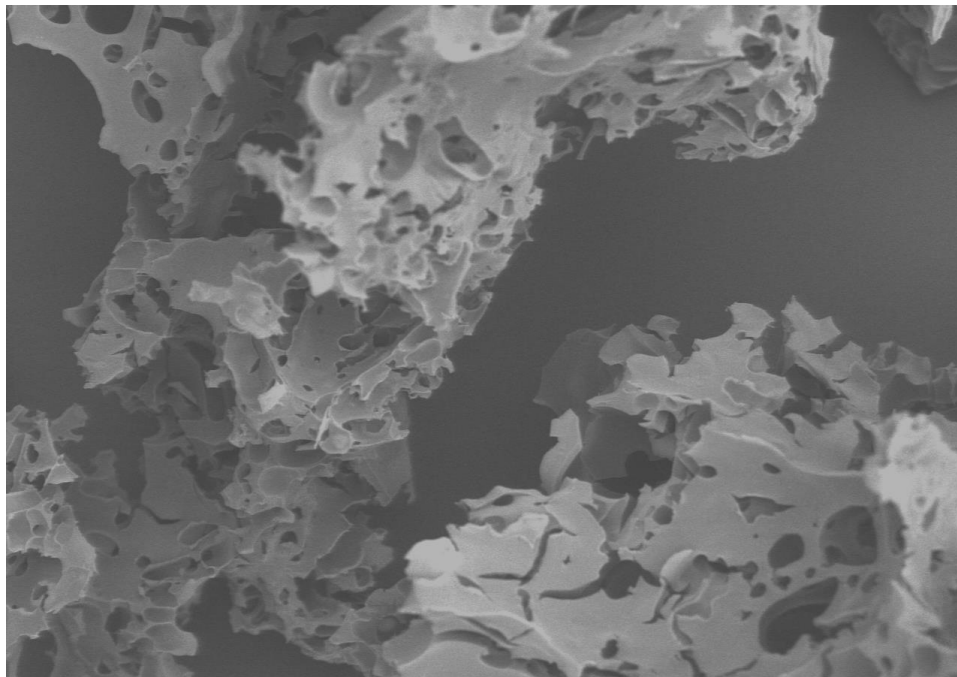

Clariant SU7000 5.00kV 5.1mm x200 UD+LD+MD 07/17/2024 200µm

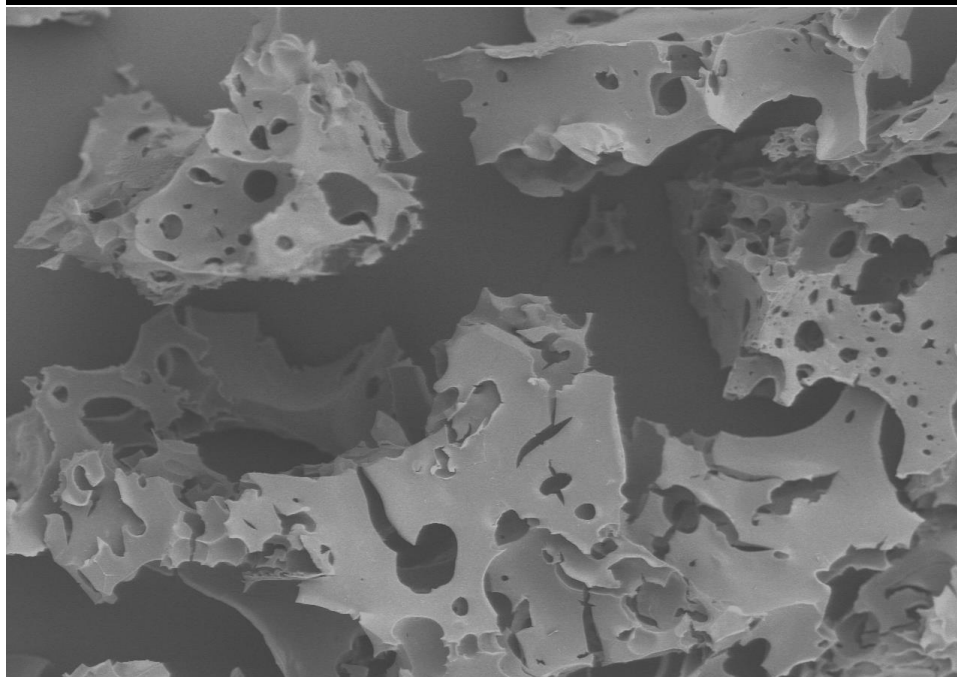


Clariant SU7000 5.00kV 5.2mm x200 UD+LD+MD 07/17/2024 200µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-1
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047592-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

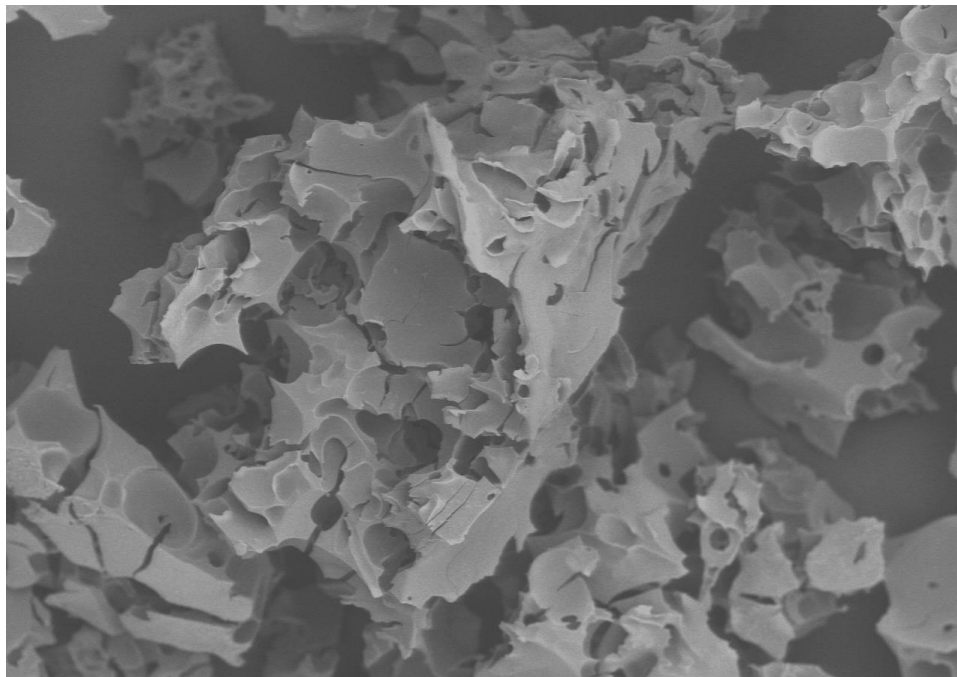

Clariant SU7000 5.00kV 4.9mm x200 UD+LD+MD 07/17/2024 200µm

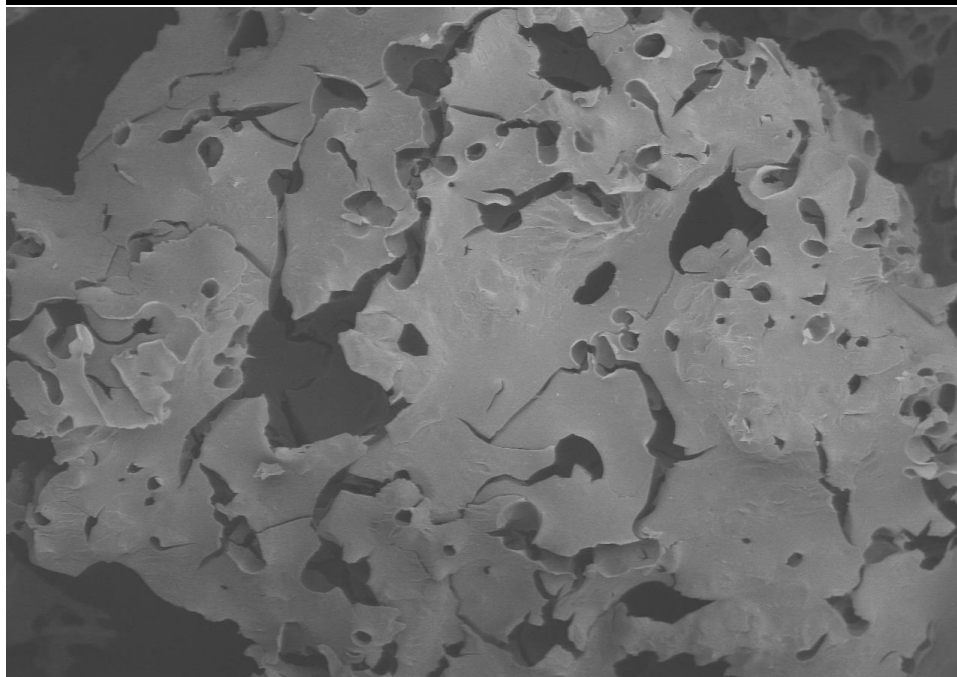


Clariant SU7000 5.00kV 4.9mm x200 UD+LD+MD 07/17/2024 200µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-1
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047592-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

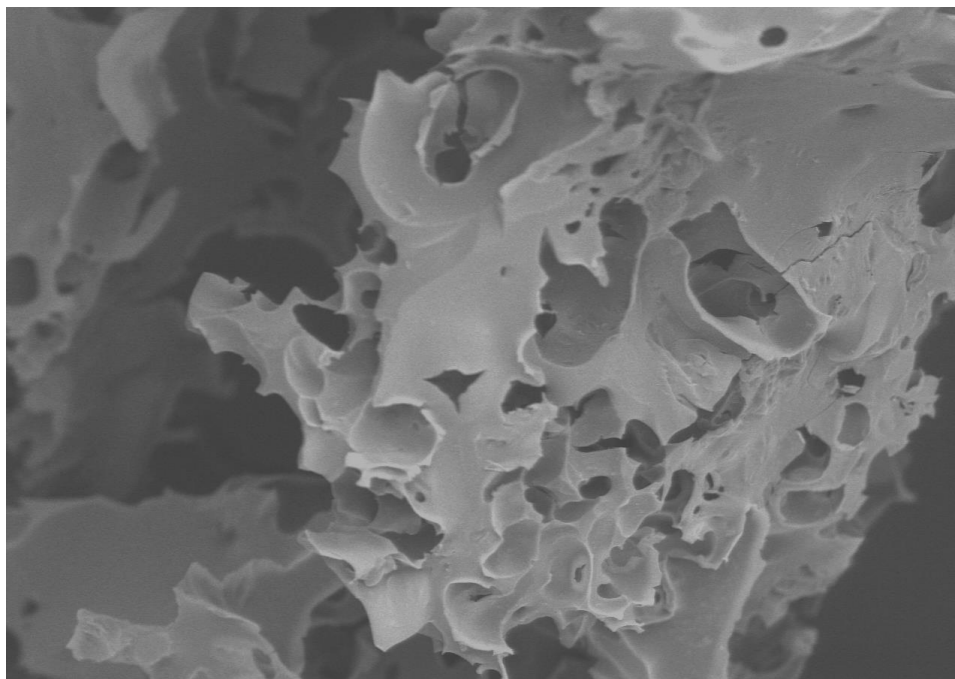

Clariant SU7000 5.00kV 4.9mm x500 UD+LD+MD 07/17/2024 100µm

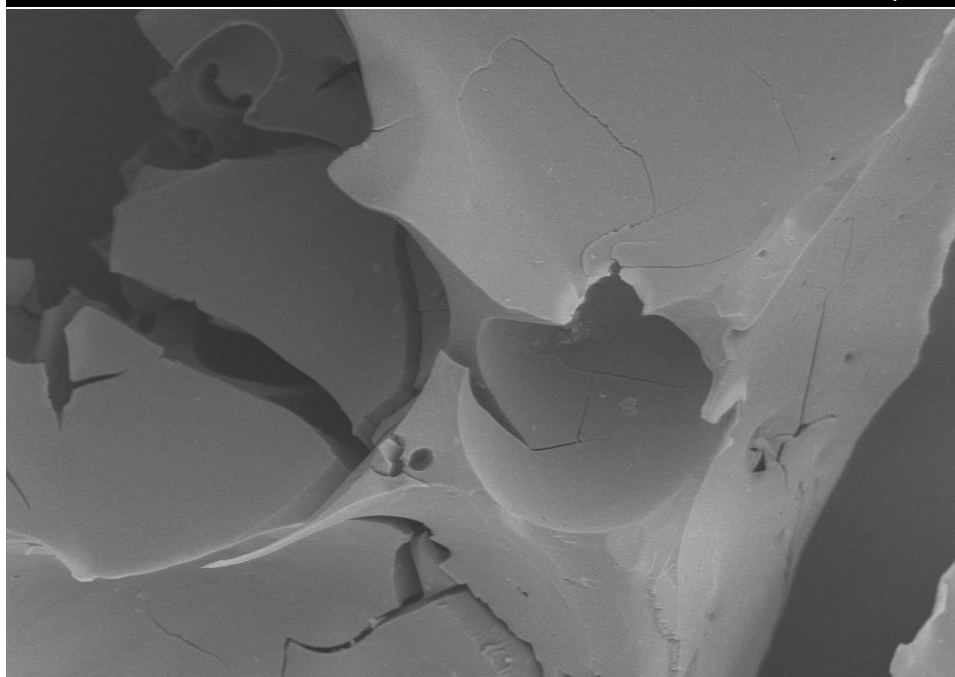


Clariant SU7000 5.00kV 5.3mm x500 UD+LD+MD 07/17/2024 100µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-1
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047592-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

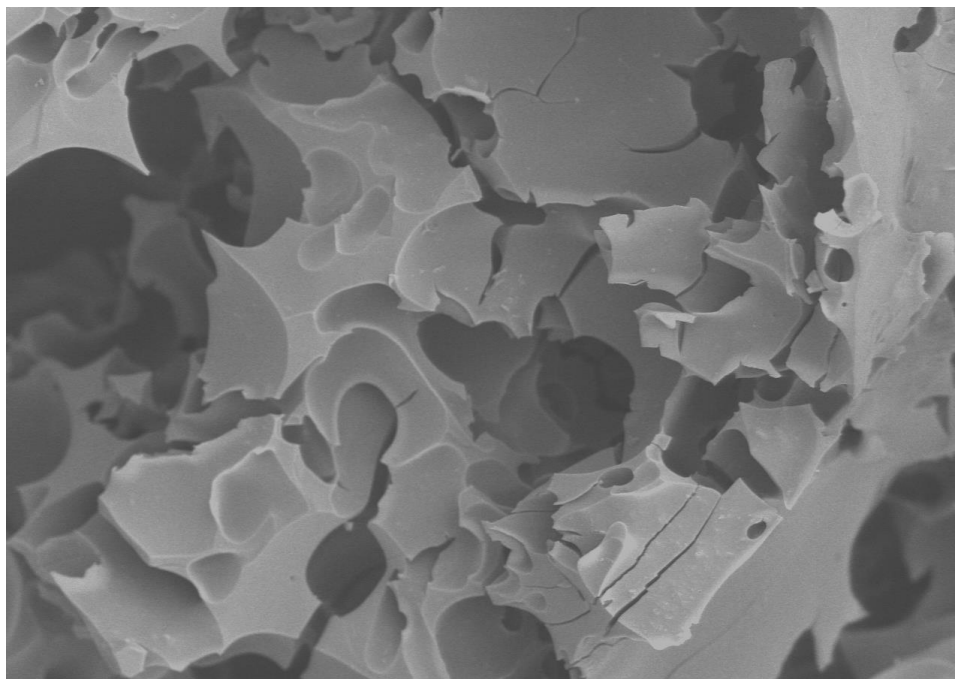

Clariant SU7000 5.00kV 4.9mm x500 UD+LD+MD 07/17/2024 100µm

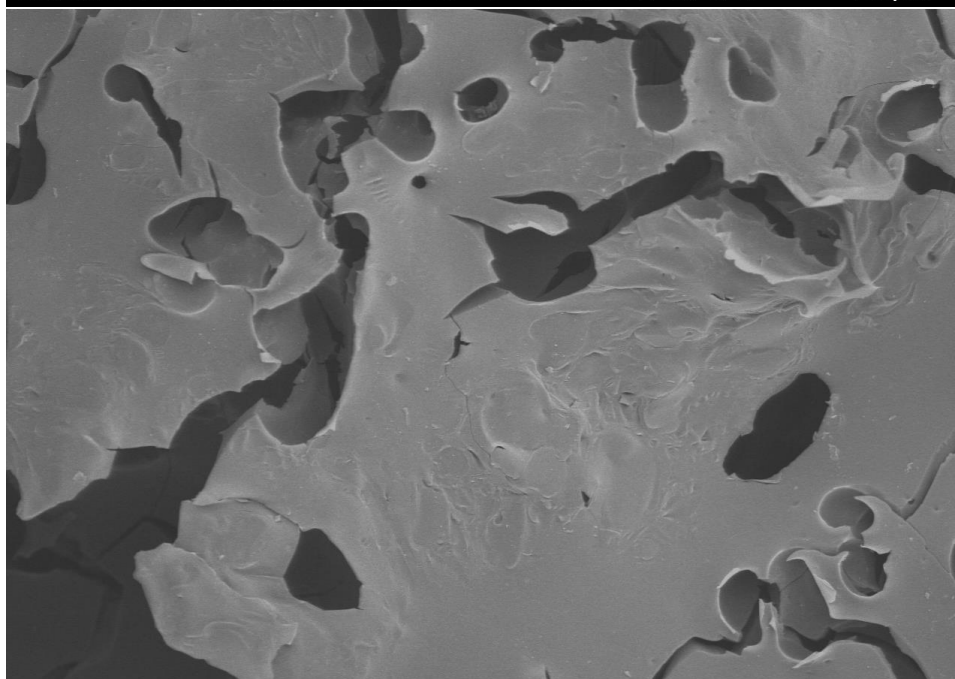


Clariant SU7000 5.00kV 4.9mm x500 UD+LD+MD 07/17/2024 100µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-1
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047592-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

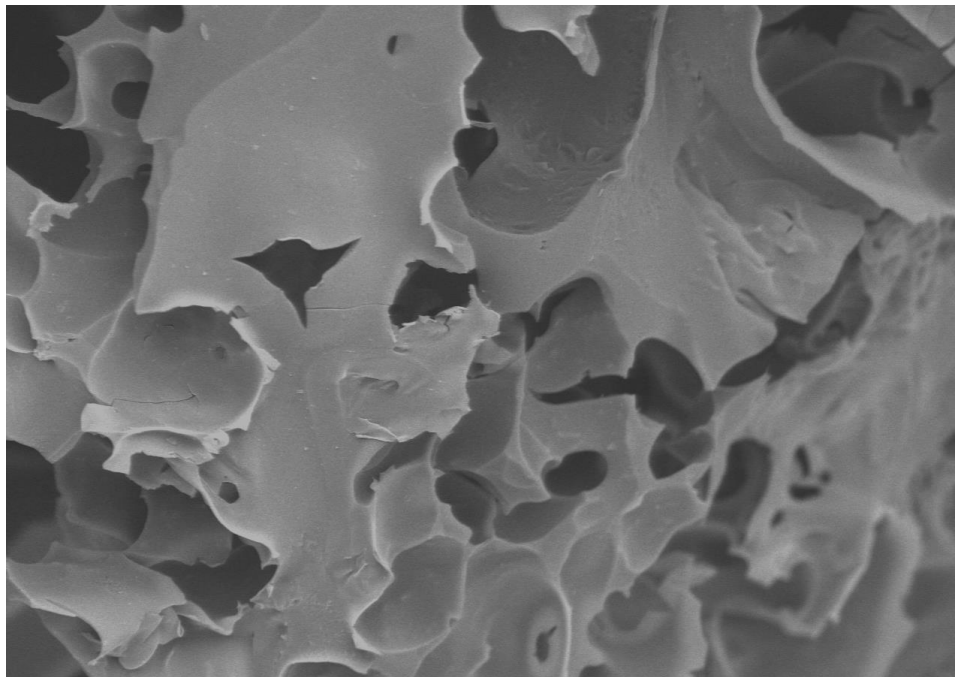

Clariant SU7000 5.00kV 4.8mm x1.00k UD+LD+MD 07/17/2024 50.0µm

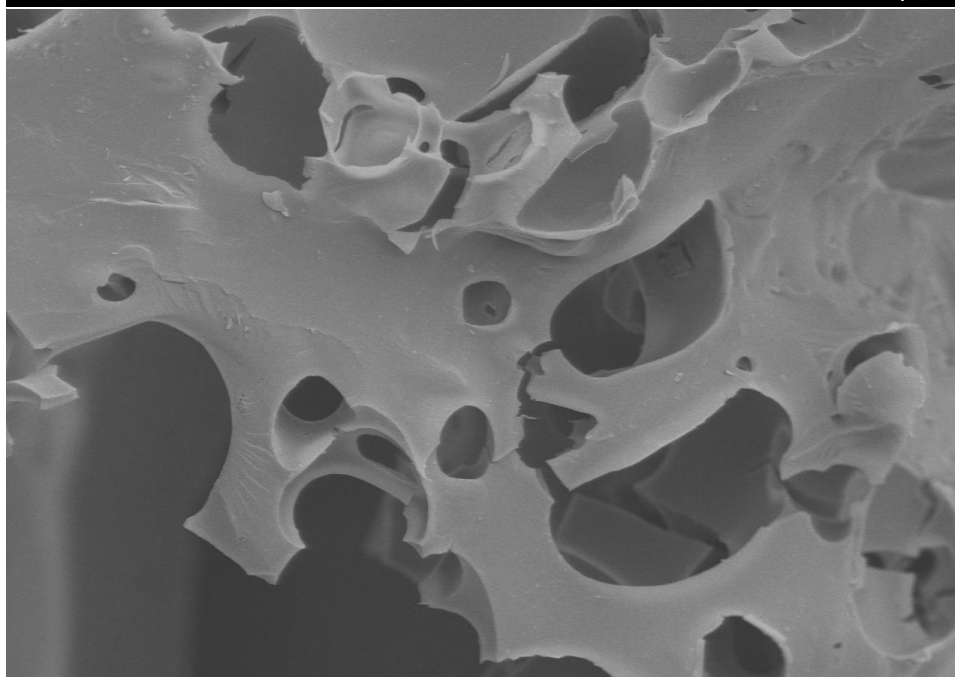


Clariant SU7000 5.00kV 5.0mm x1.00k UD+LD+MD 07/17/2024 50.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-1
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047592-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

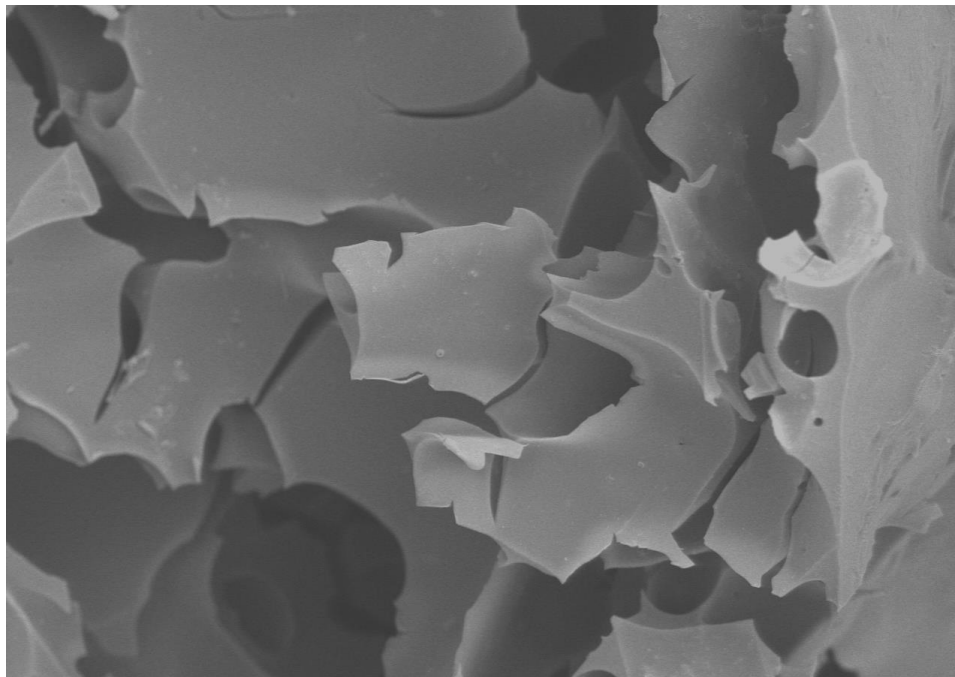

Clariant SU7000 5.00kV 4.9mm x1.00k UD+LD+MD 07/17/2024 50.0µm

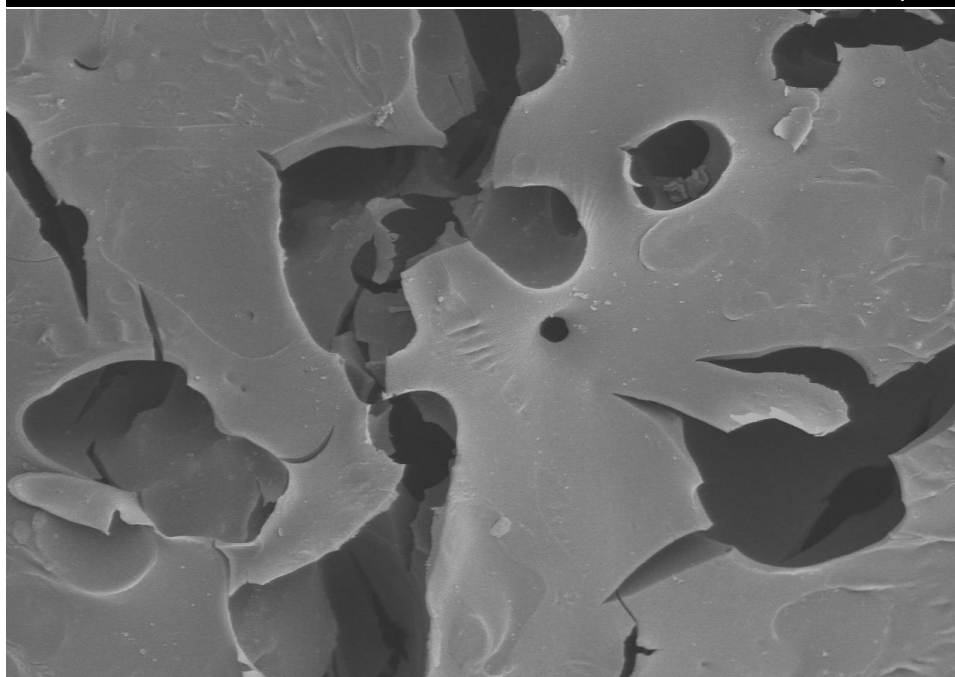


Clariant SU7000 5.00kV 4.9mm x1.00k UD+LD+MD 07/17/2024 50.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-1
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047592-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

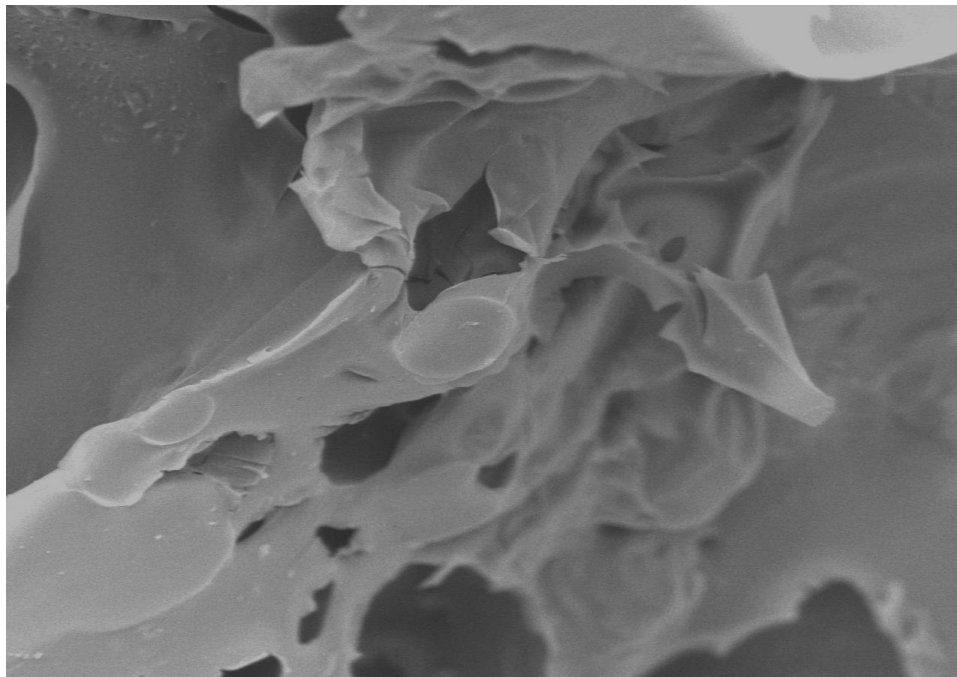

Clariant SU7000 5.00kV 4.7mm x2.00k UD+LD+MD 07/17/2024 20.0µm

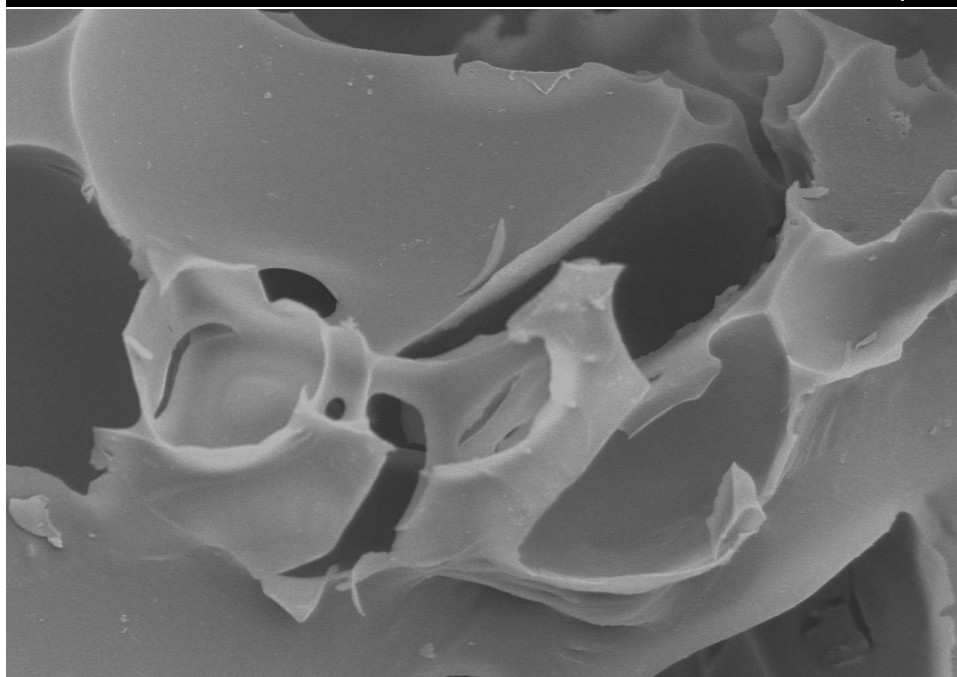


Clariant SU7000 5.00kV 5.0mm x2.00k UD+LD+MD 07/17/2024 20.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-1
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047592-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

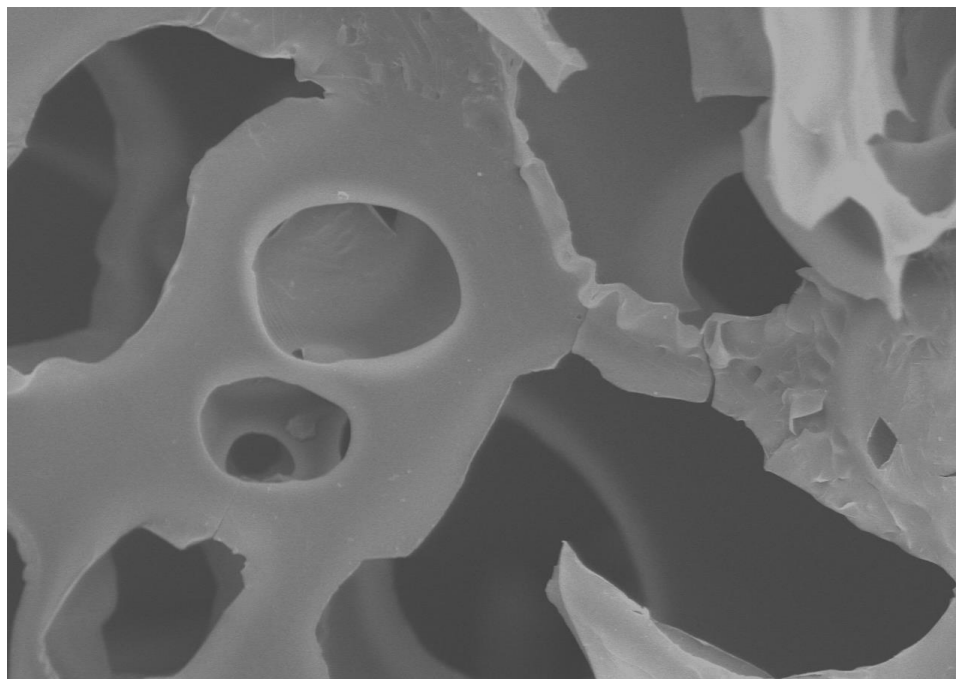

Clariant SU7000 5.00kV 5.0mm x2.00k UD+LD+MD 07/17/2024 20.0µm

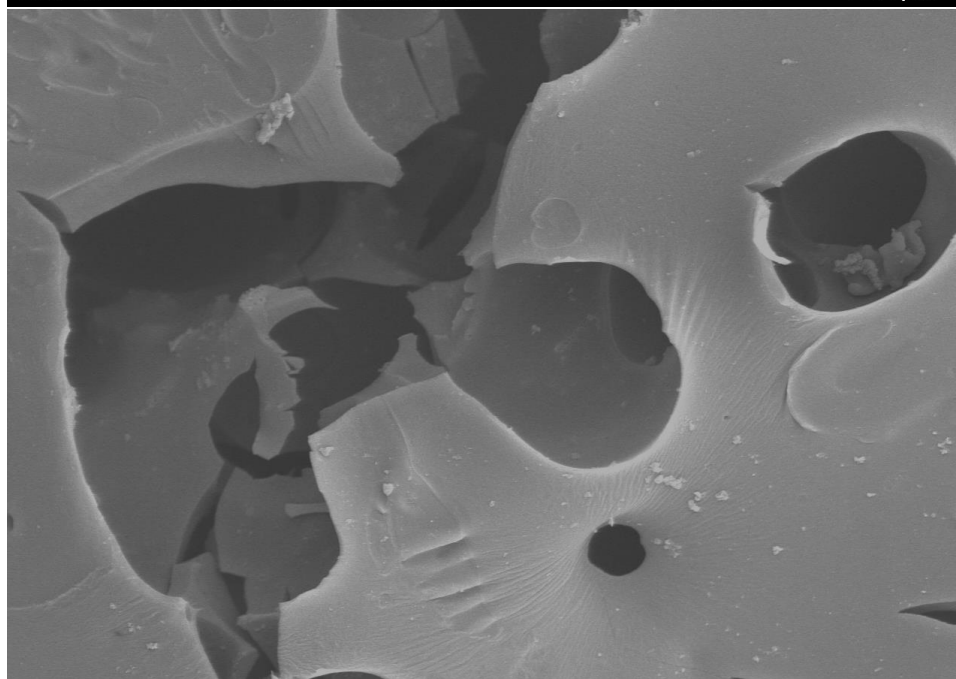


Clariant SU7000 5.00kV 4.9mm x2.00k UD+LD+MD 07/17/2024 20.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-1
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047592-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

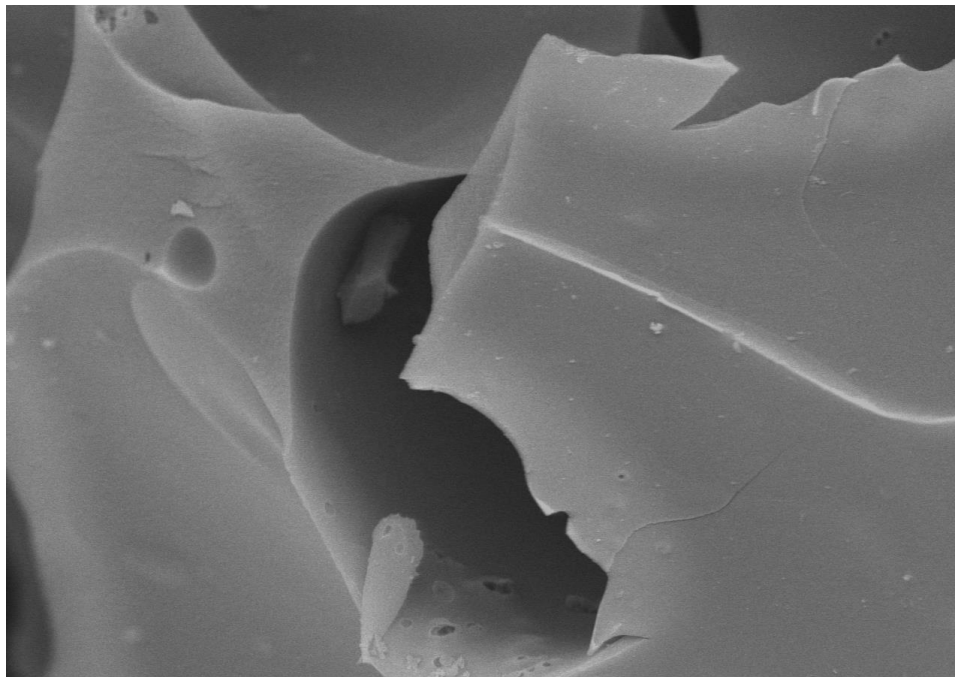

Clariant SU7000 5.00kV 4.9mm x5.00k UD+LD+MD 07/17/2024 10.0µm

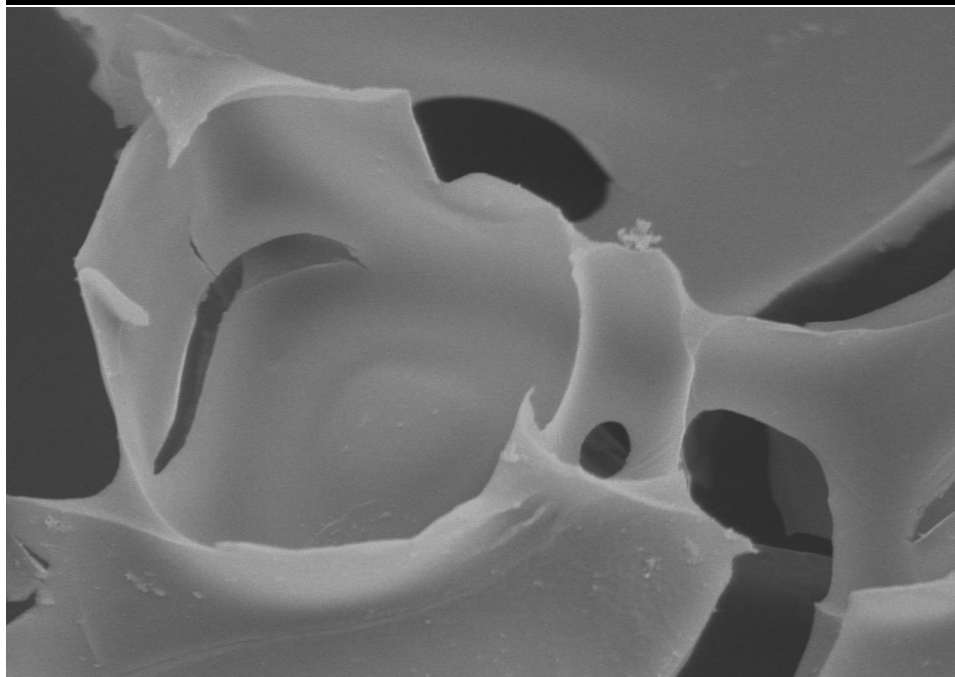


Clariant SU7000 5.00kV 5.0mm x5.00k UD+LD+MD 07/17/2024 10.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-1
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047592-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

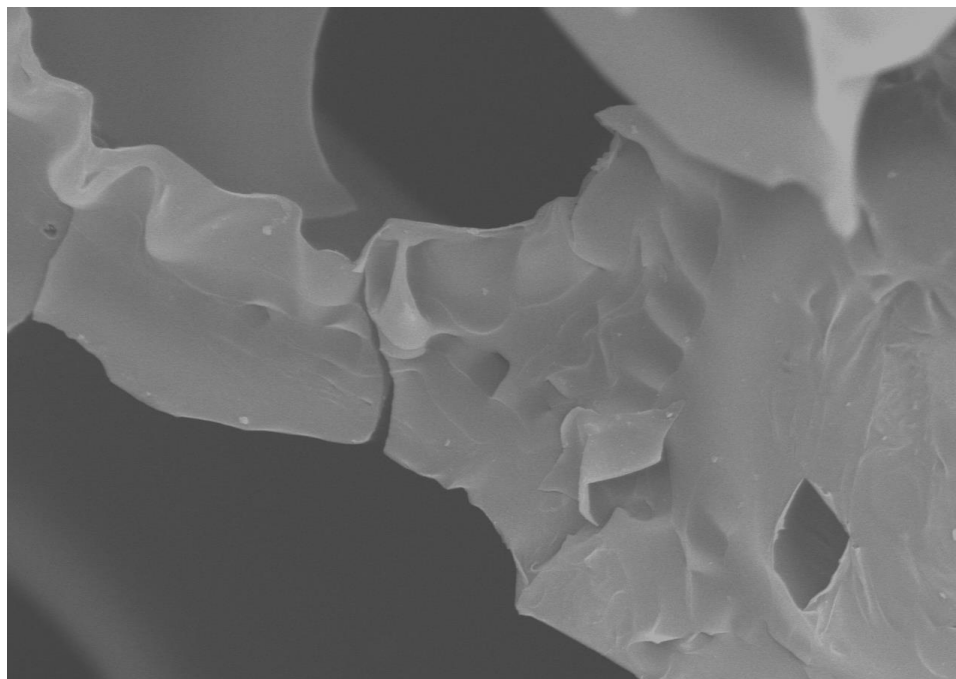

Clariant SU7000 5.00kV 5.0mm x5.00k UD+LD+MD 07/17/2024 10.0µm

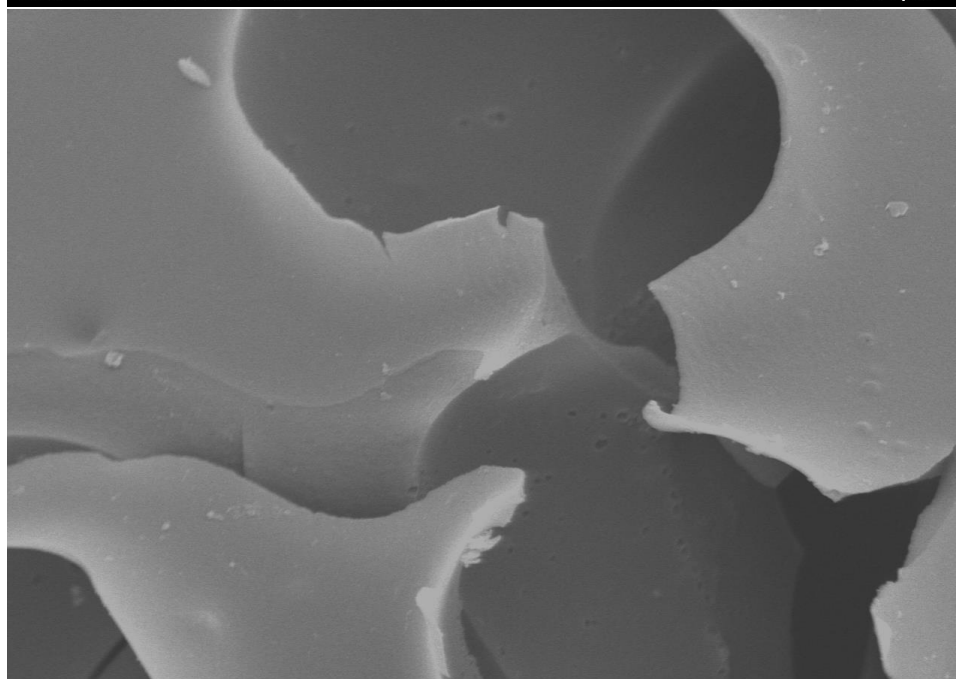


Clariant SU7000 5.00kV 4.9mm x5.00k UD+LD+MD 07/17/2024 10.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-1
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047592-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

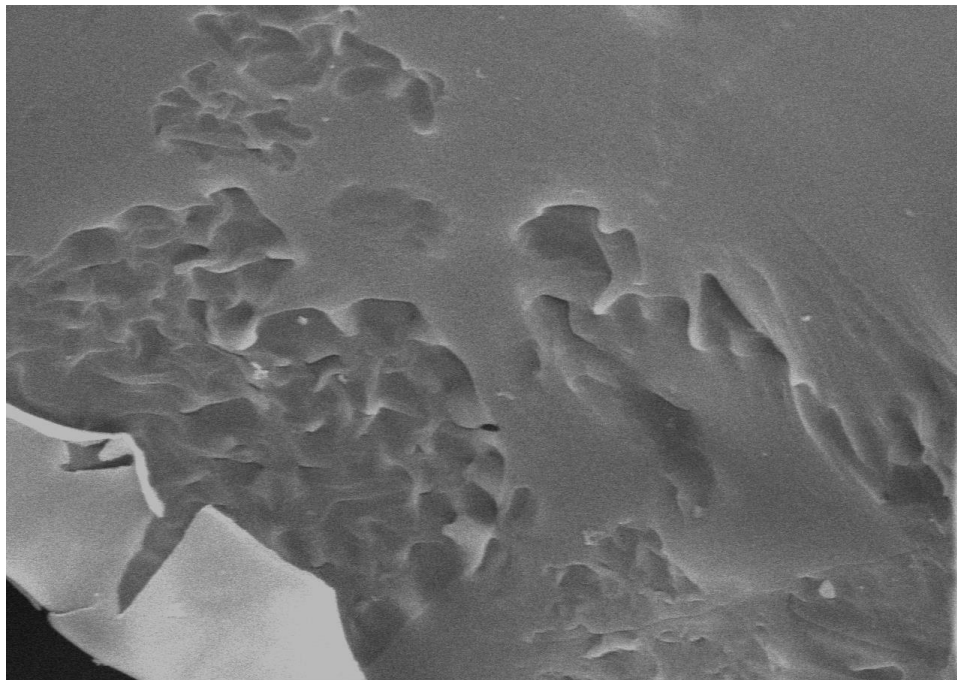

Clariant SU7000 5.00kV 5.0mm x10.0k UD+LD+MD 07/17/2024 5.00μm

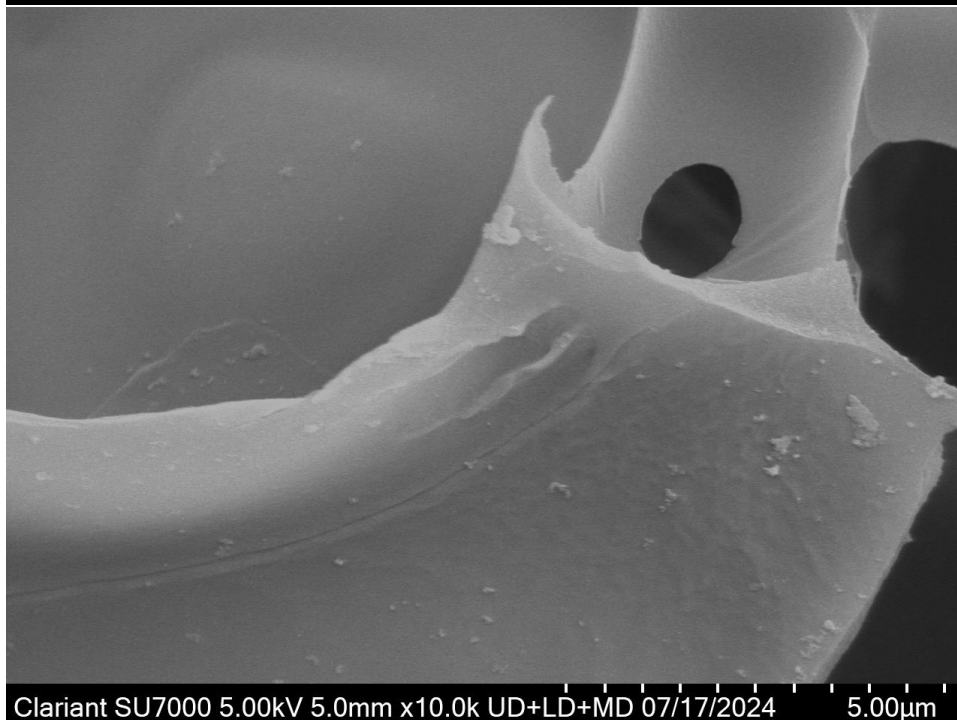


Clariant SU7000 5.00kV 5.0mm x10.0k UD+LD+MD 07/17/2024 5.00μm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-1
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047592-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

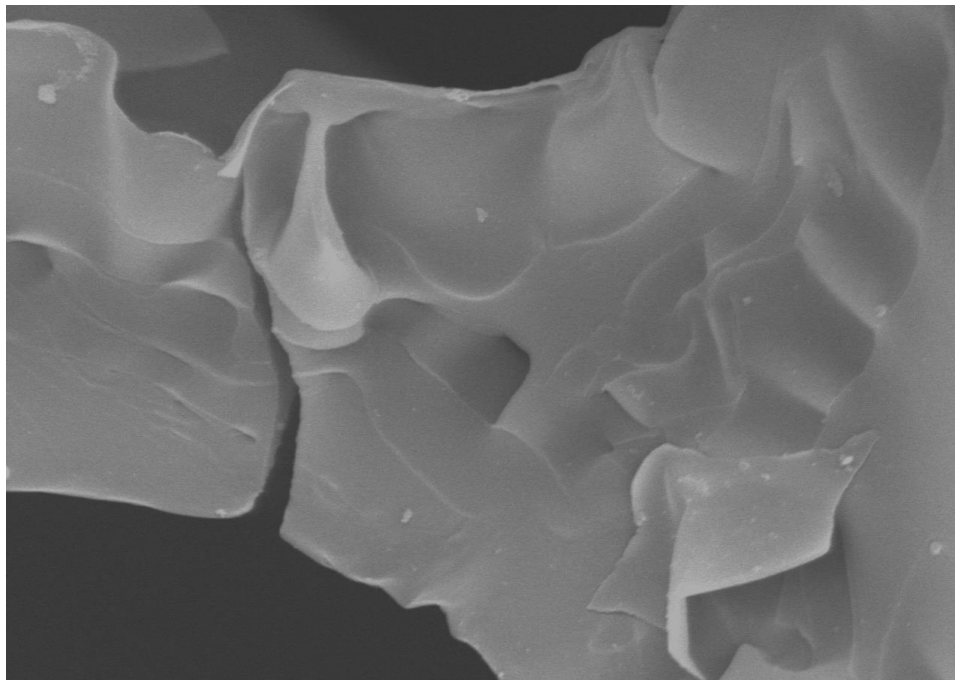

Clariant SU7000 5.00kV 5.0mm x10.0k UD+LD+MD 07/17/2024 5.00µm

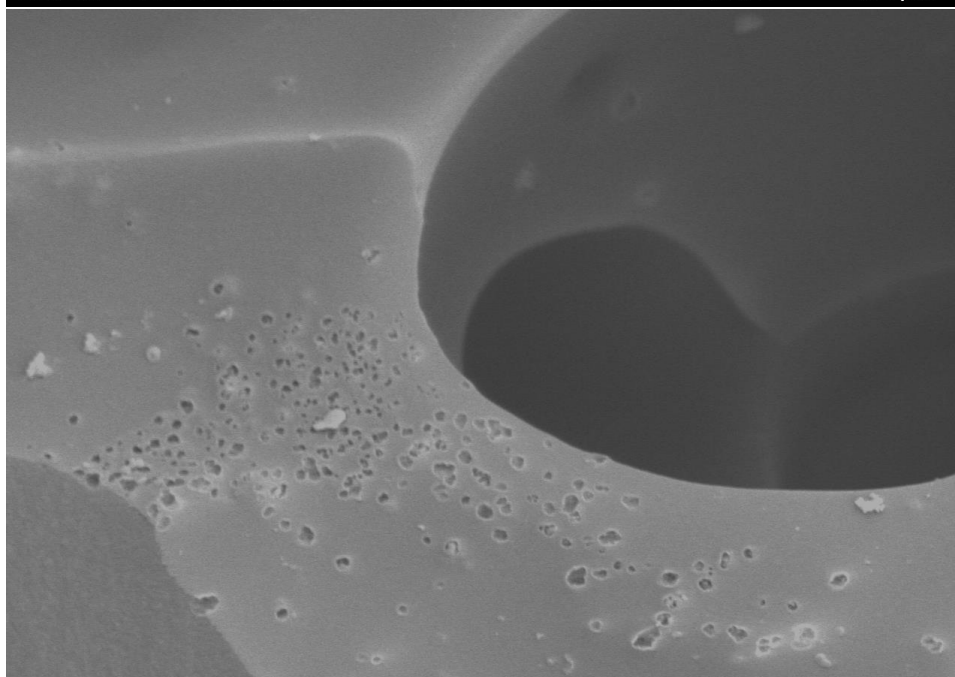


Clariant SU7000 5.00kV 5.3mm x10.0k UD+LD+MD 07/17/2024 5.00µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-1
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047592-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

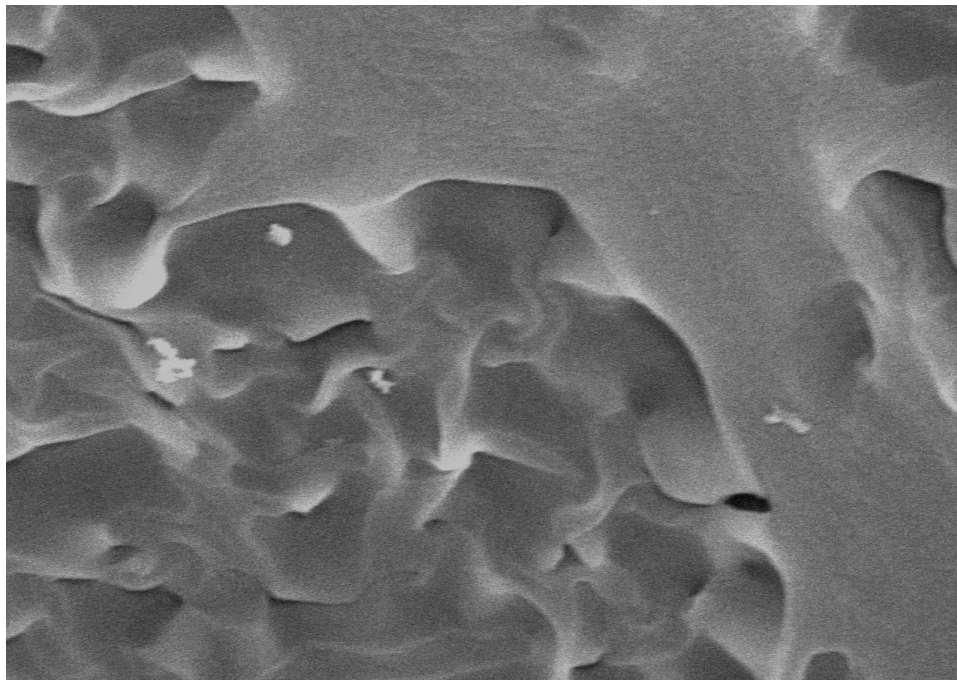

Clariant SU7000 5.00kV 5.0mm x25.0k UD+LD+MD 07/17/2024 2.00µm

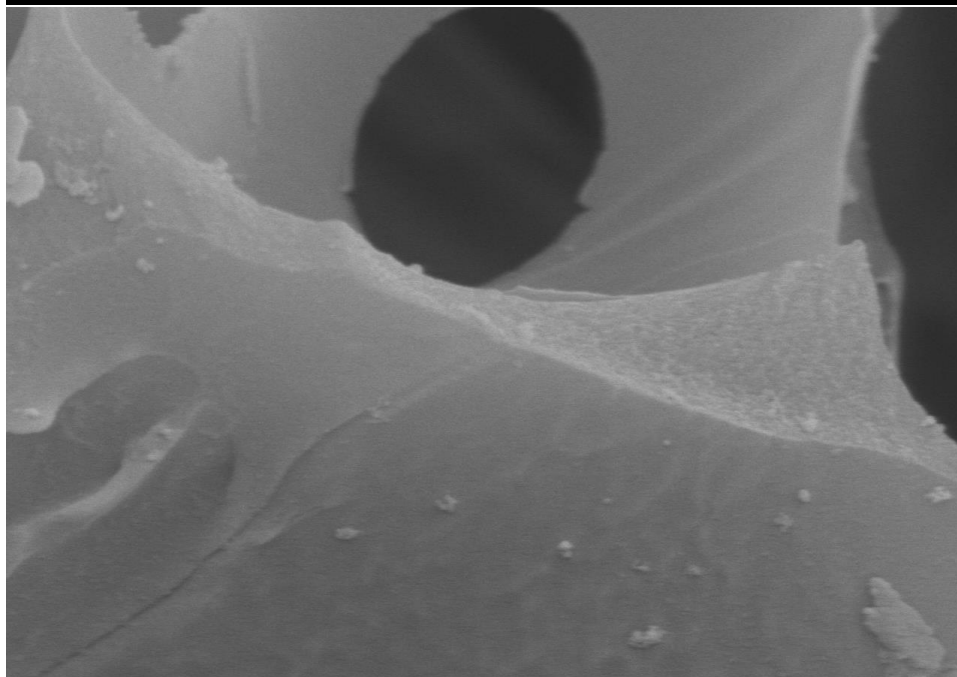


Clariant SU7000 5.00kV 5.0mm x25.0k UD+LD+MD 07/17/2024 2.00µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-1
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047592-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

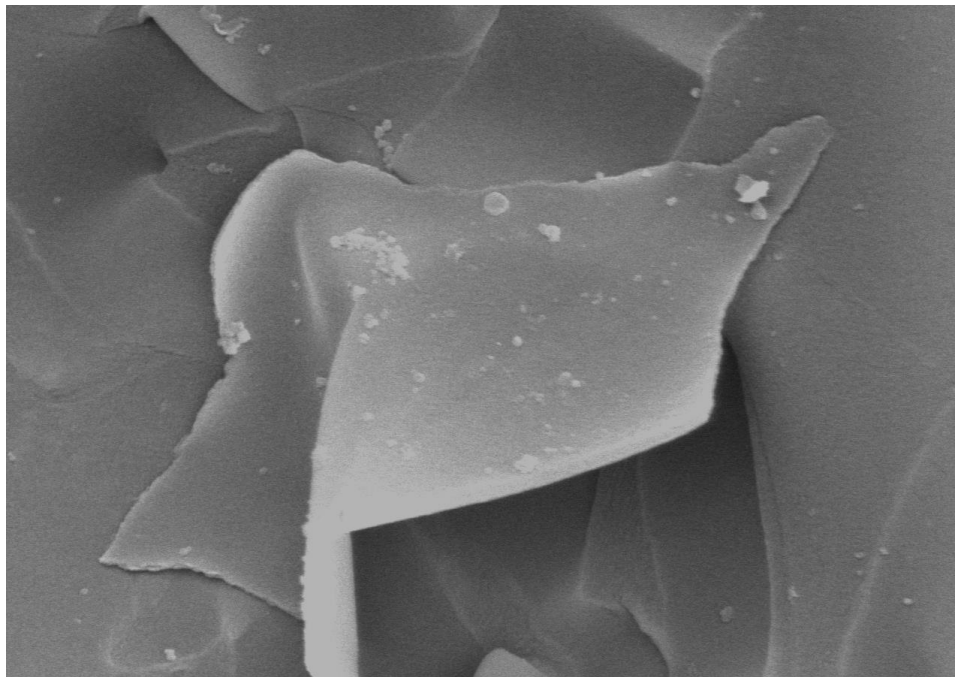

Clariant SU7000 5.00kV 5.0mm x25.0k UD+LD+MD 07/17/2024 2.00µm

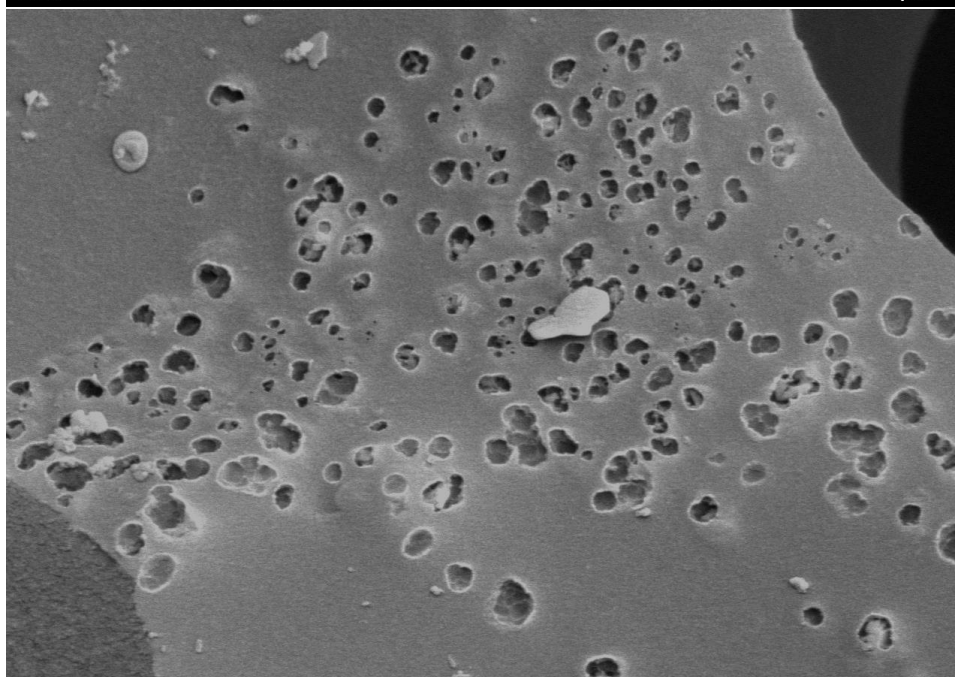

Clariant SU7000 5.00kV 5.3mm x25.0k UD+LD+MD 07/17/2024 2.00µm