



SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-2
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047623-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

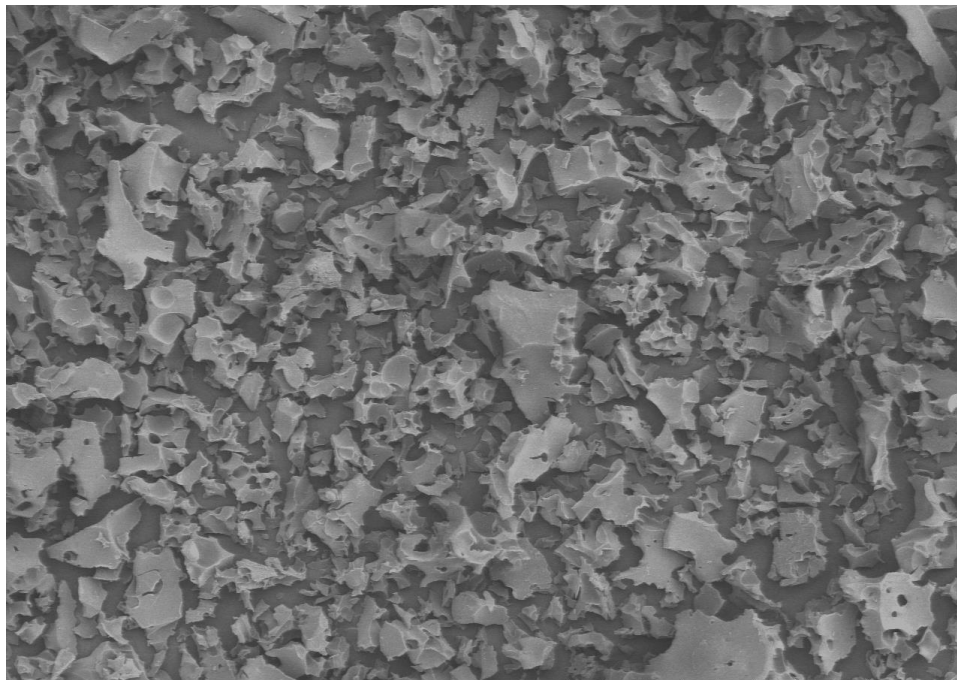

Clariant SU7000 5.00kV 5.1mm x100 UD+LD+MD 07/19/2024 500µm

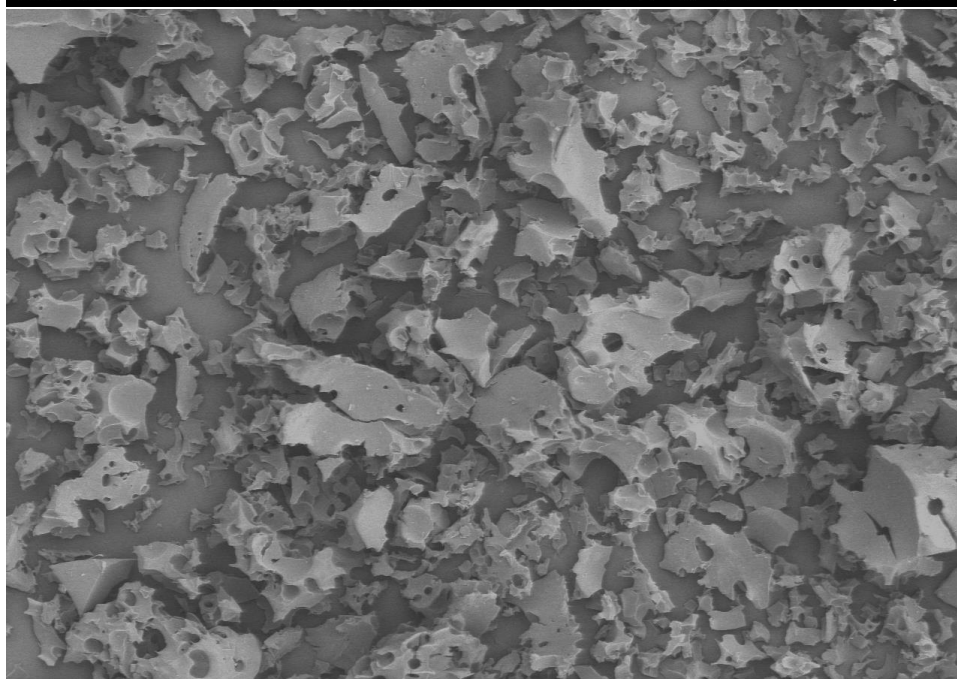


Clariant SU7000 5.00kV 5.1mm x100 UD+LD+MD 07/19/2024 500µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-2
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047623-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

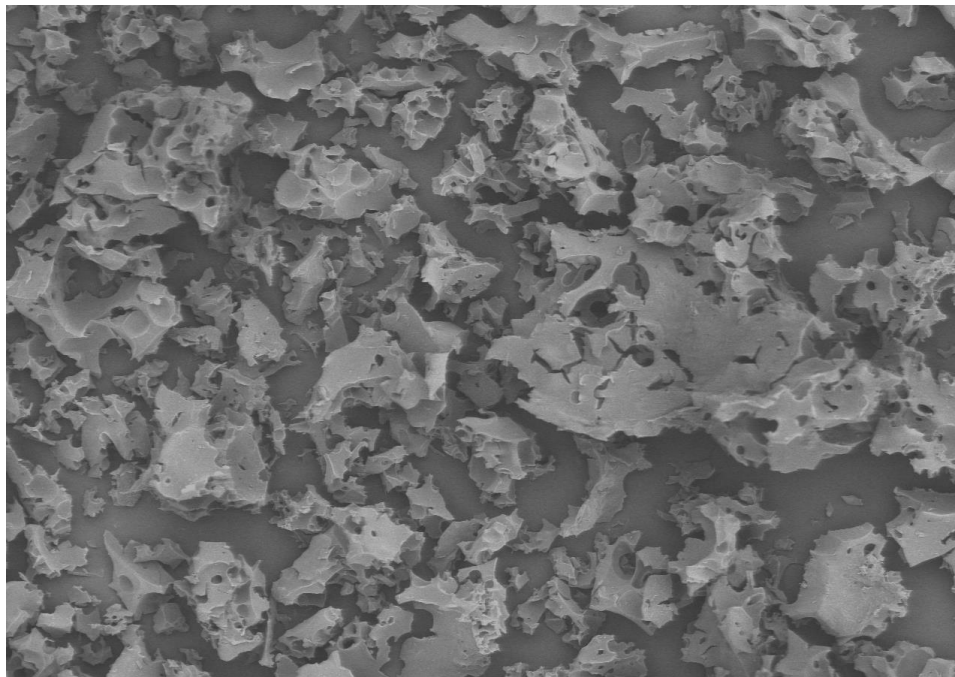

Clariant SU7000 5.00kV 5.1mm x100 UD+LD+MD 07/19/2024 500µm

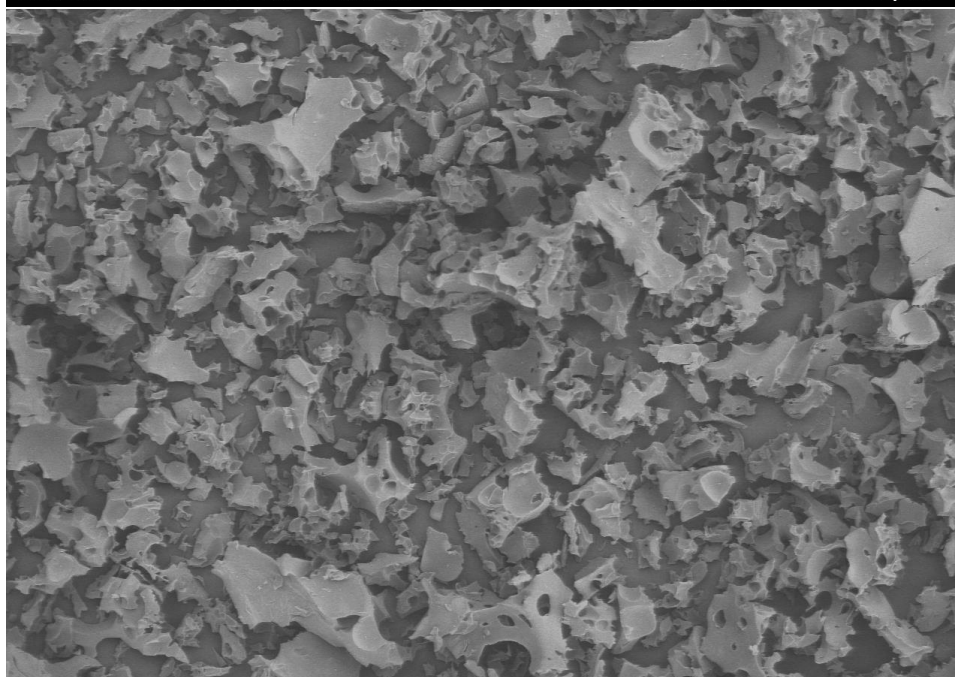


Clariant SU7000 5.00kV 5.1mm x100 UD+LD+MD 07/19/2024 500µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-2
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047623-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

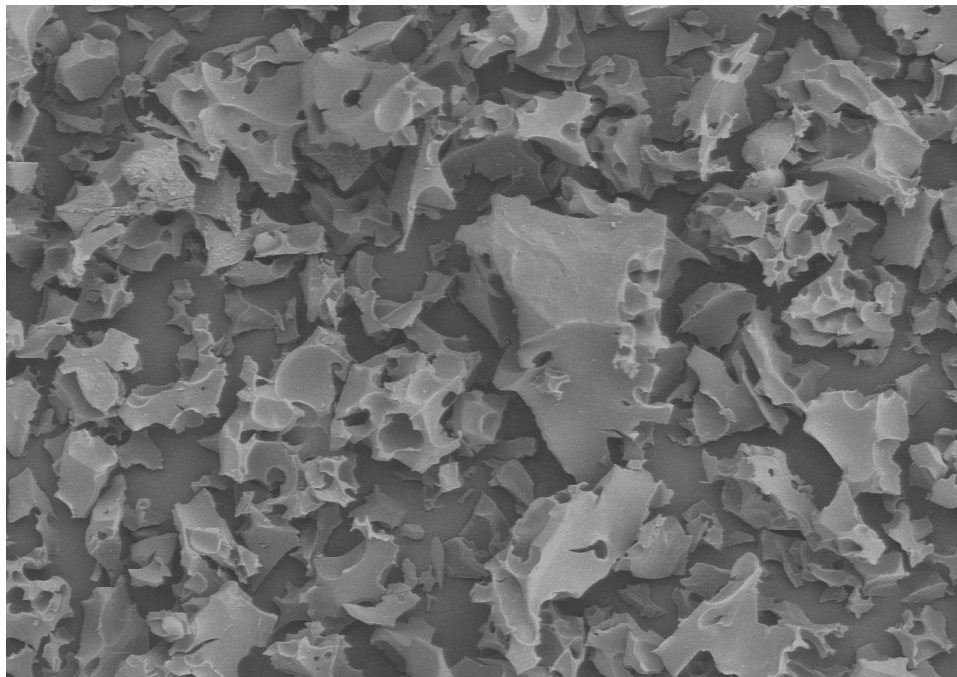

Clariant SU7000 5.00kV 5.1mm x200 UD+LD+MD 07/19/2024 200µm

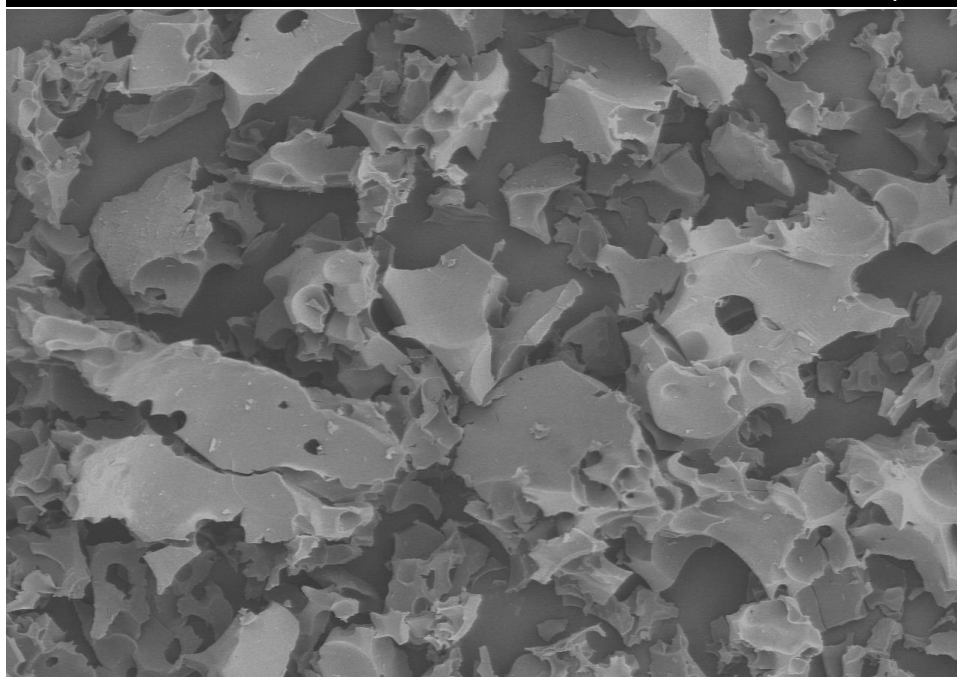


Clariant SU7000 5.00kV 5.1mm x200 UD+LD+MD 07/19/2024 200µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-2
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047623-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

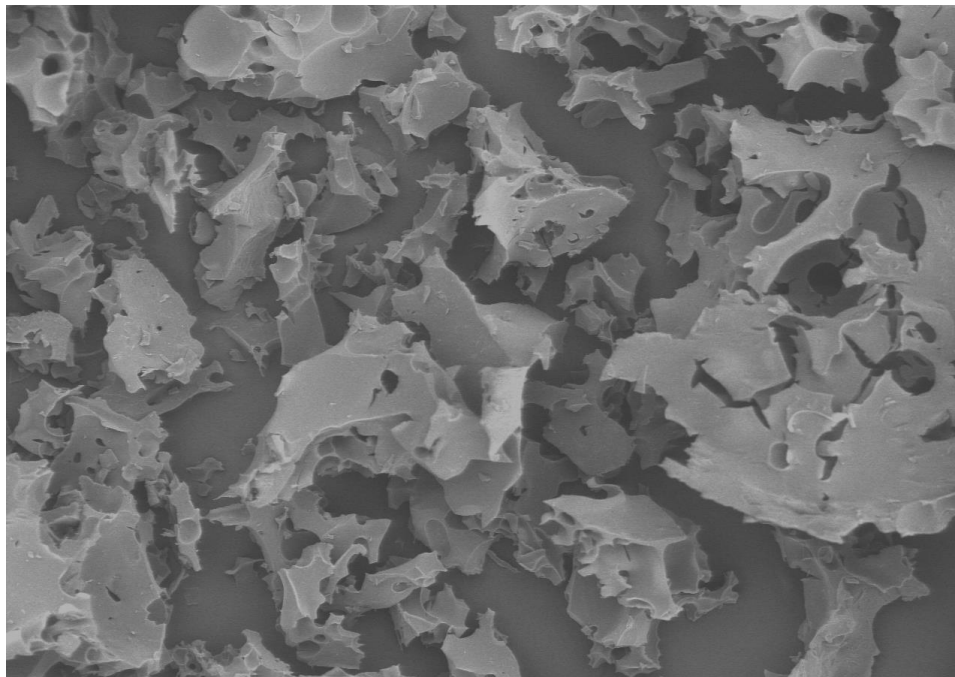

Clariant SU7000 5.00kV 5.1mm x200 UD+LD+MD 07/19/2024 200μm

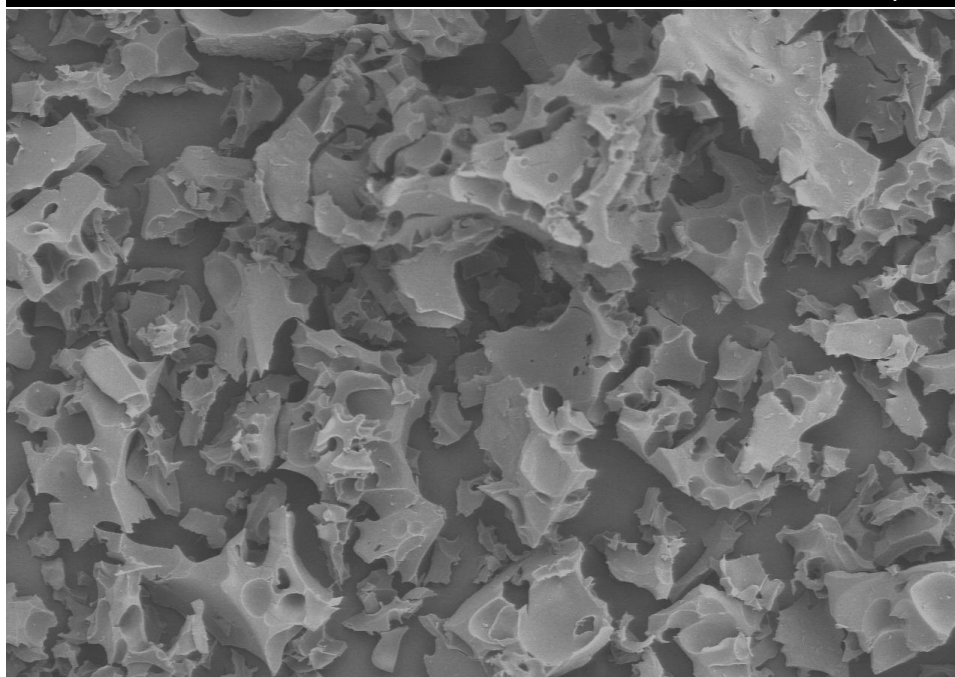


Clariant SU7000 5.00kV 5.1mm x200 UD+LD+MD 07/19/2024 200μm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-2
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047623-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

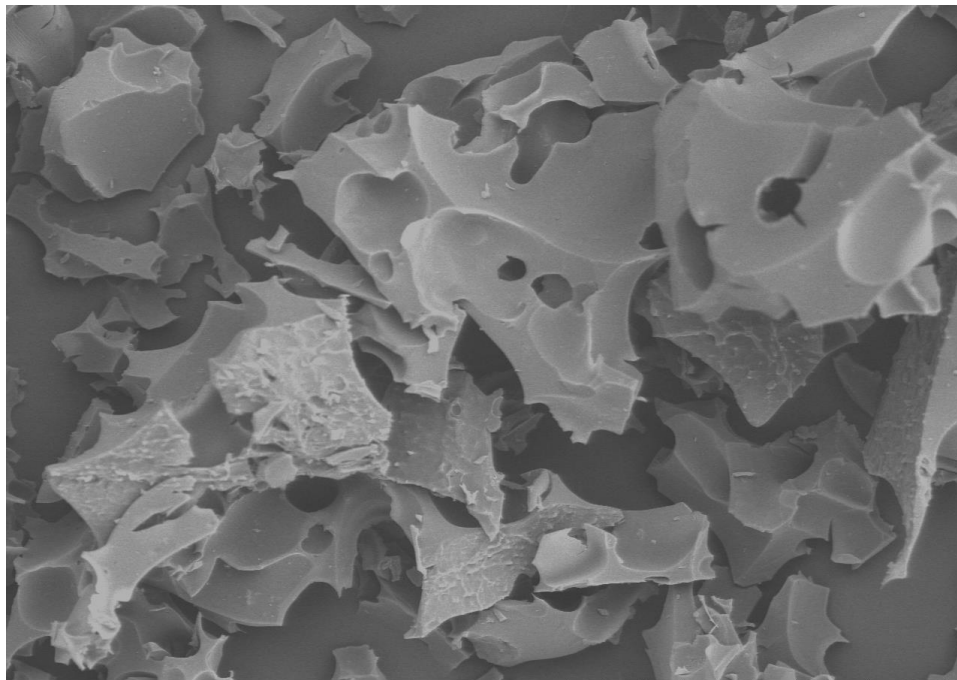

Clariant SU7000 5.00kV 5.1mm x500 UD+LD+MD 07/19/2024 100µm

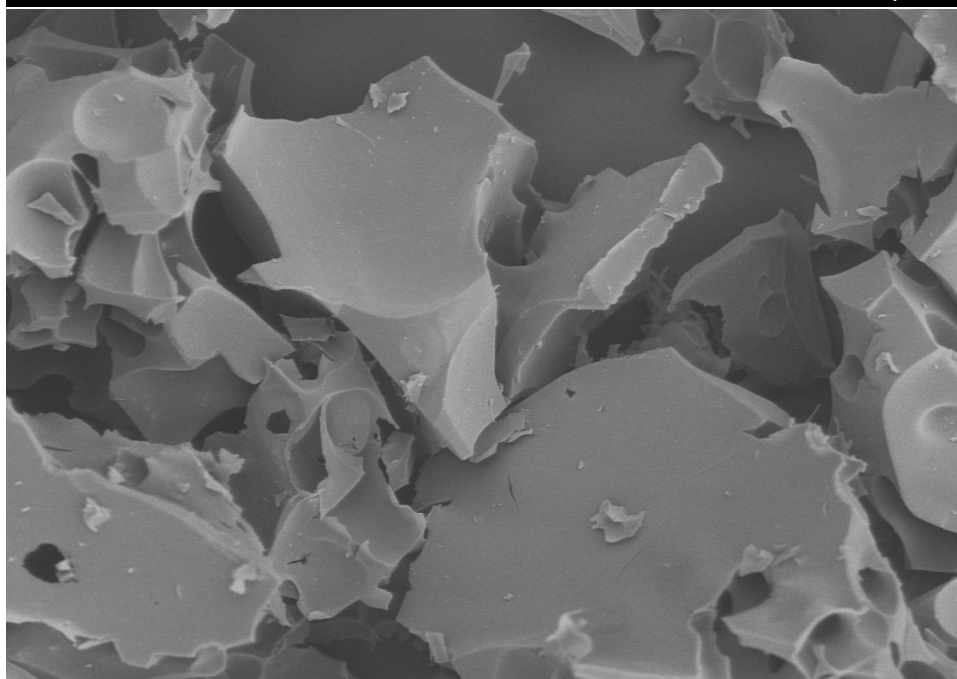


Clariant SU7000 5.00kV 5.1mm x500 UD+LD+MD 07/19/2024 100µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-2
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047623-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

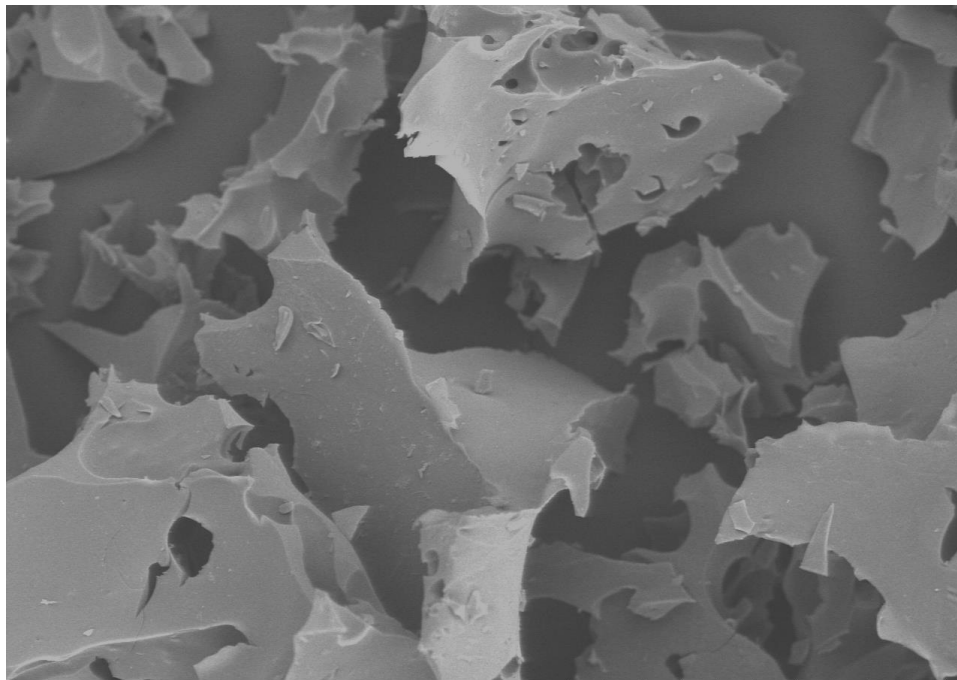

Clariant SU7000 5.00kV 5.1mm x500 UD+LD+MD 07/19/2024 100µm

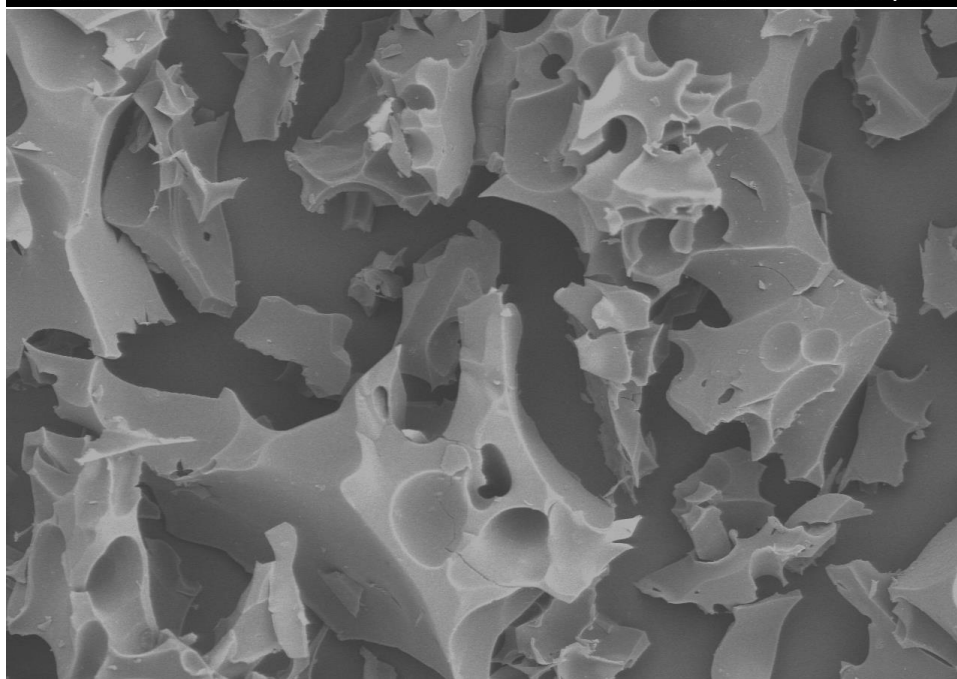


Clariant SU7000 5.00kV 5.1mm x500 UD+LD+MD 07/19/2024 100µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-2
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047623-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

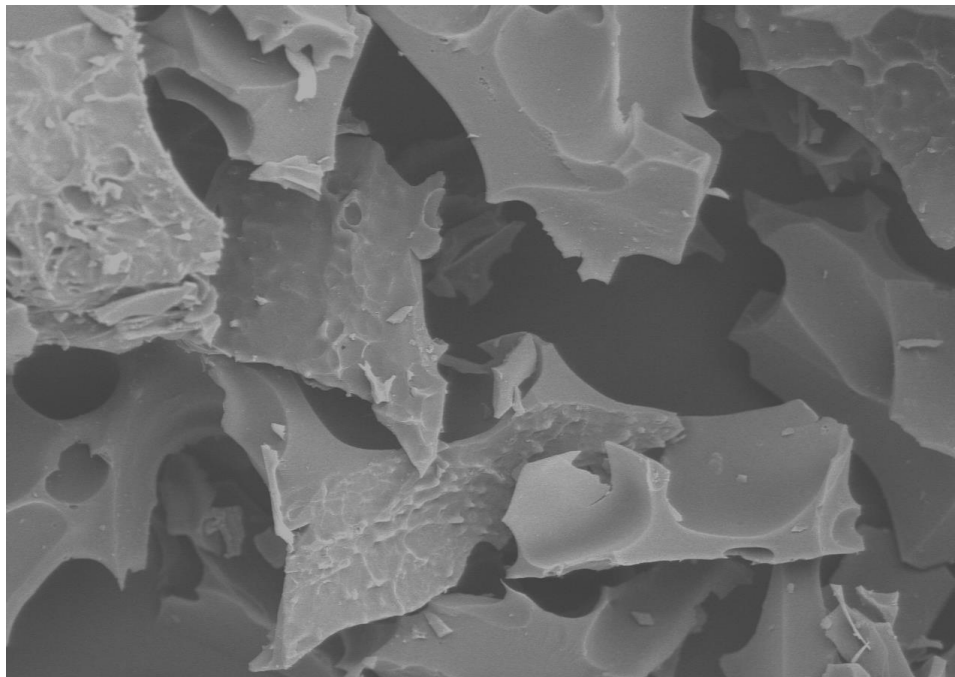

Clariant SU7000 5.00kV 5.1mm x1.00k UD+LD+MD 07/19/2024 50.0µm

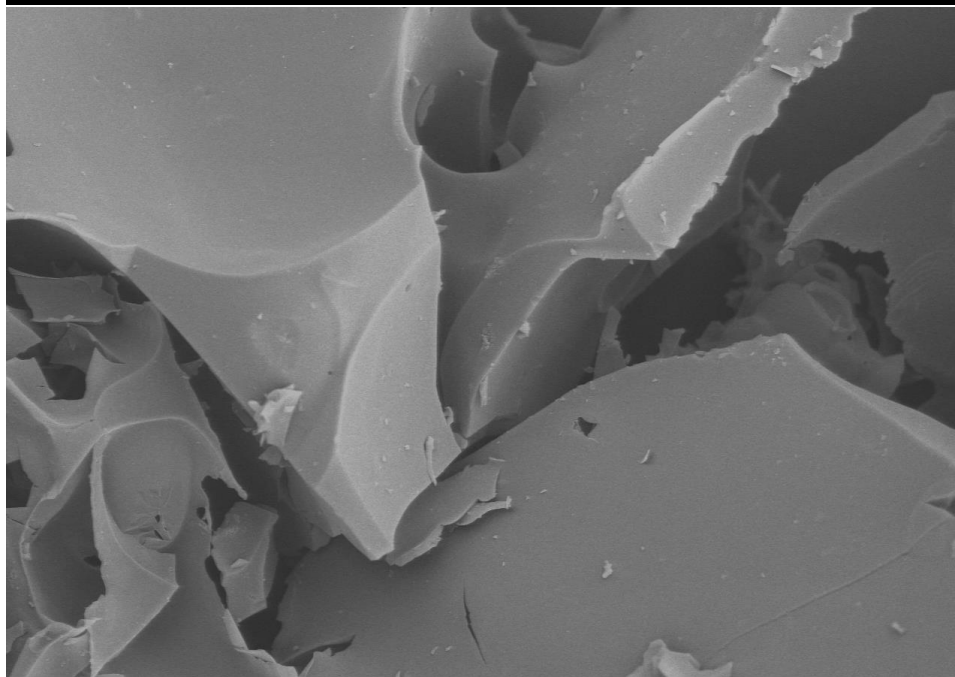


Clariant SU7000 5.00kV 5.1mm x1.00k UD+LD+MD 07/19/2024 50.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-2
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047623-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

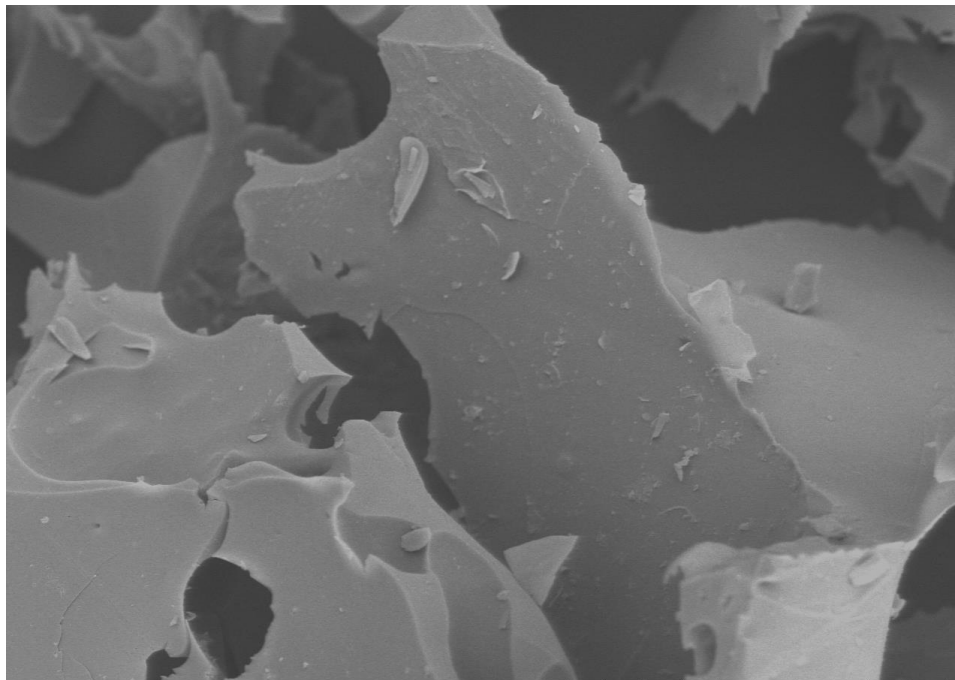

Clariant SU7000 5.00kV 5.1mm x1.00k UD+LD+MD 07/19/2024 50.0µm

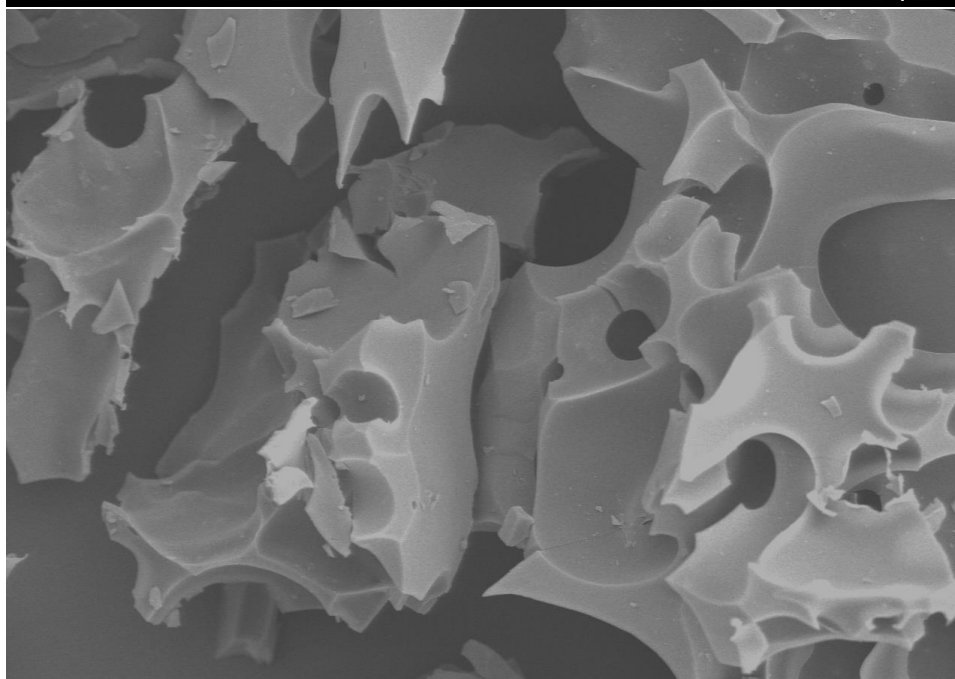


Clariant SU7000 5.00kV 5.1mm x1.00k UD+LD+MD 07/19/2024 50.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-2
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047623-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

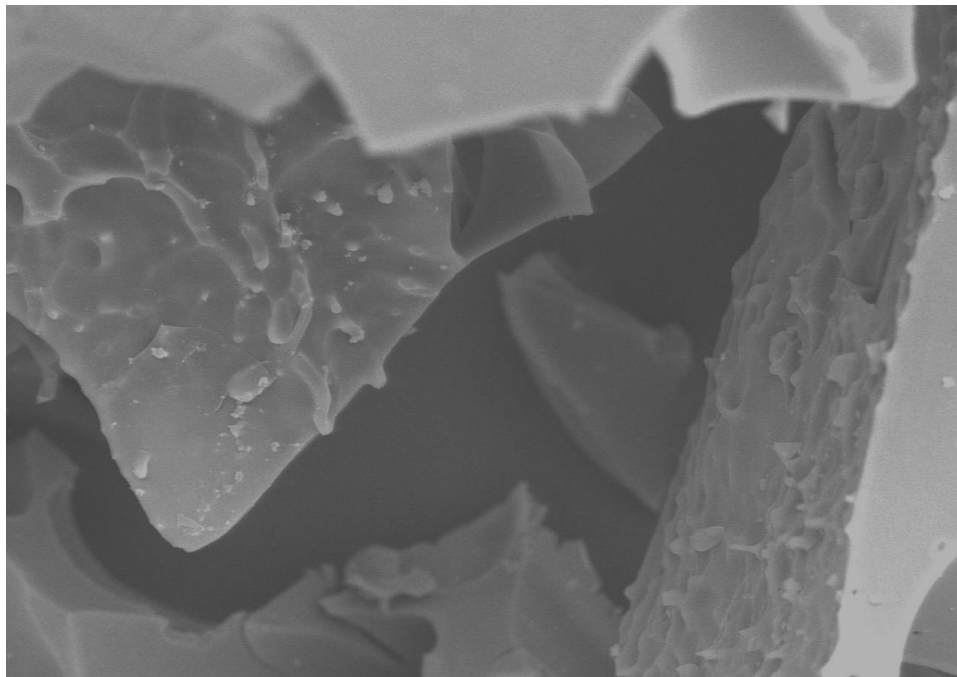

Clariant SU7000 5.00kV 5.1mm x2.00k UD+LD+MD 07/19/2024 20.0µm

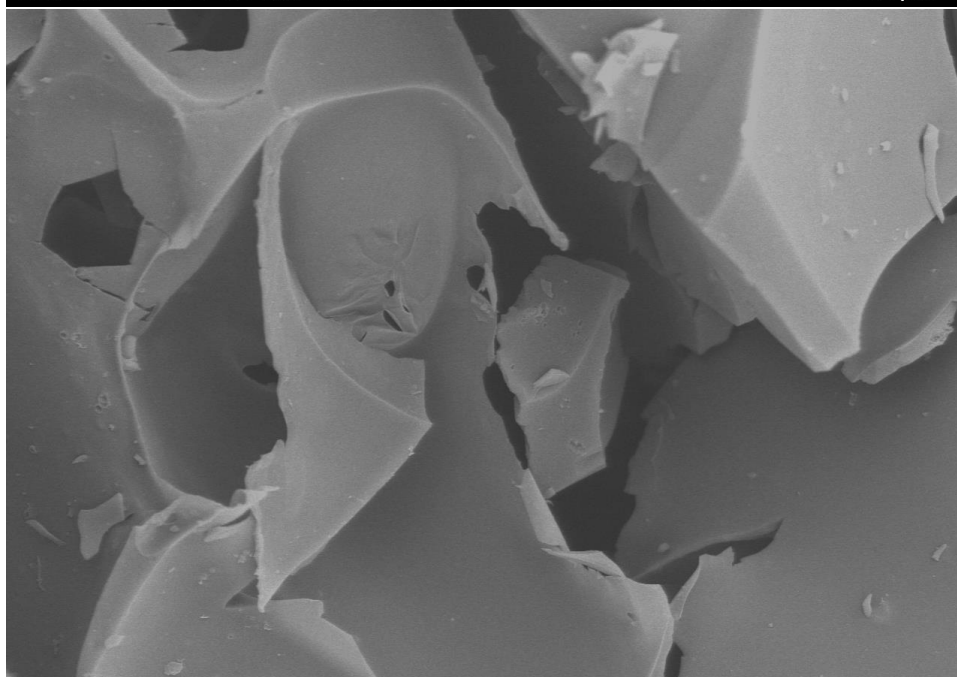


Clariant SU7000 5.00kV 5.1mm x2.00k UD+LD+MD 07/19/2024 20.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-2
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047623-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

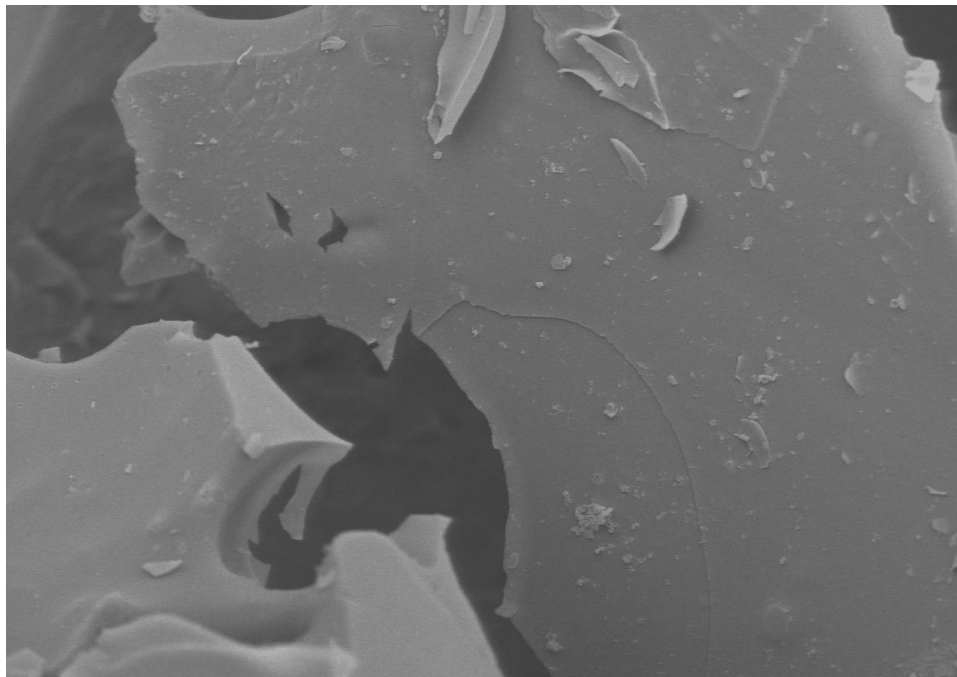

Clariant SU7000 5.00kV 5.1mm x2.00k UD+LD+MD 07/19/2024 20.0µm

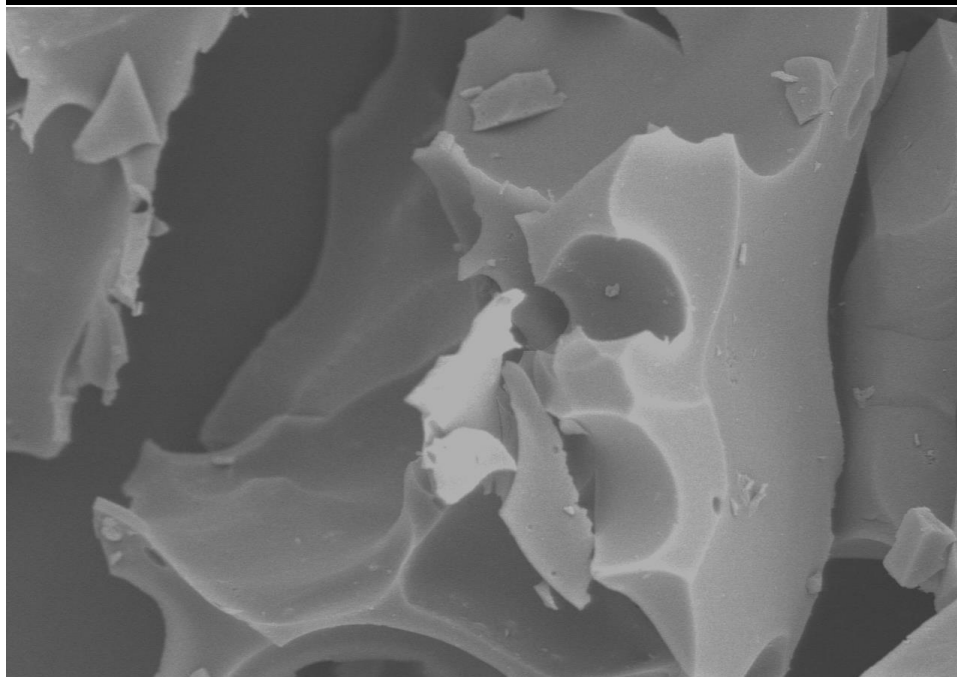


Clariant SU7000 5.00kV 5.1mm x2.00k UD+LD+MD 07/19/2024 20.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-2
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047623-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

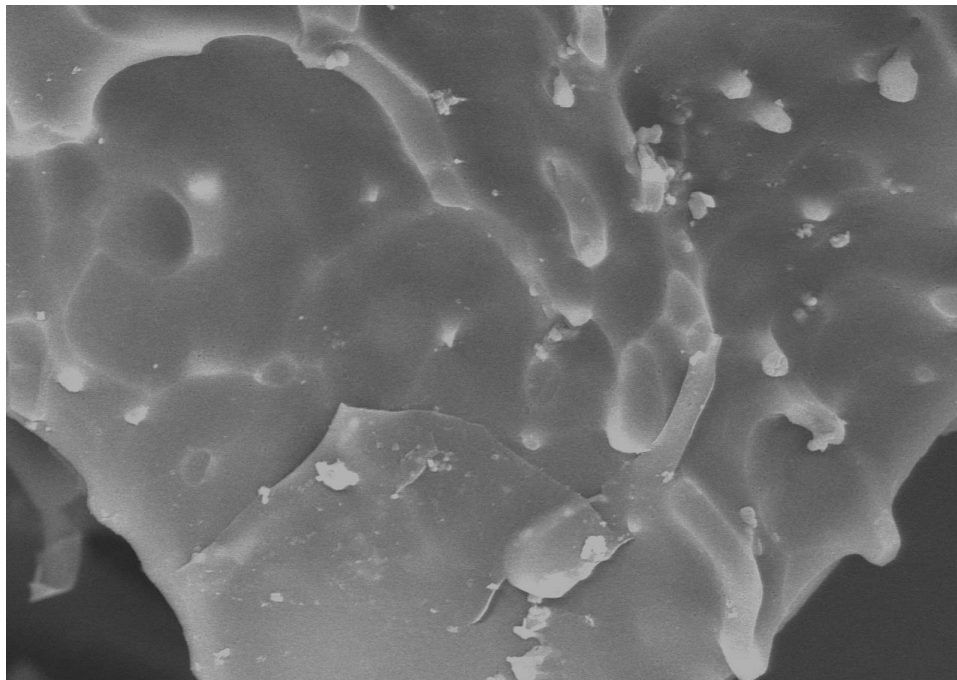

Clariant SU7000 5.00kV 5.1mm x5.00k UD+LD+MD 07/19/2024 10.0µm

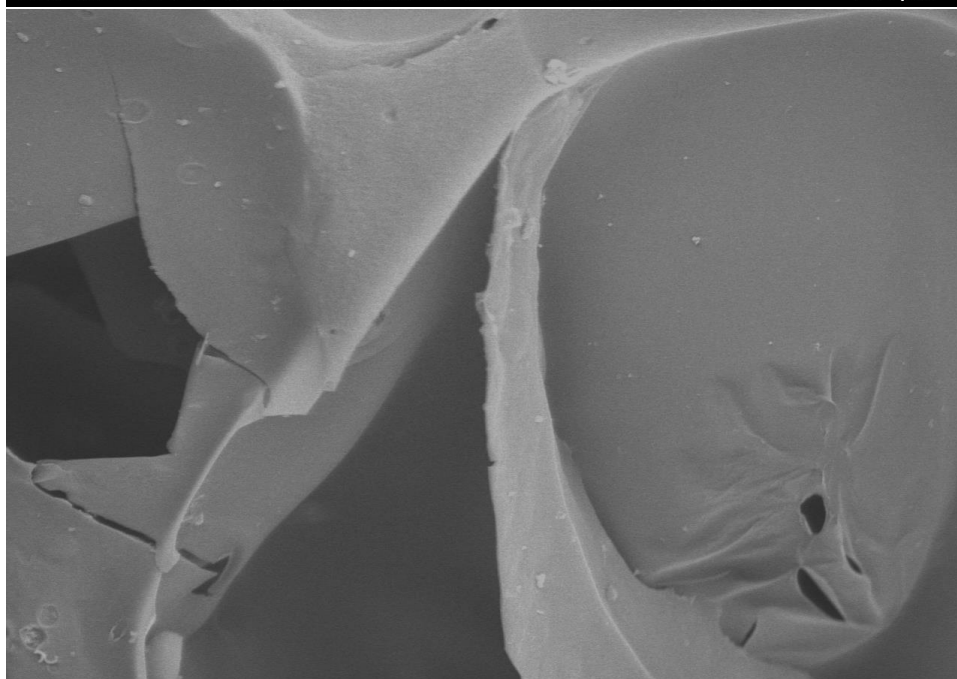


Clariant SU7000 5.00kV 5.1mm x5.00k UD+LD+MD 07/19/2024 10.0µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-2
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047623-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

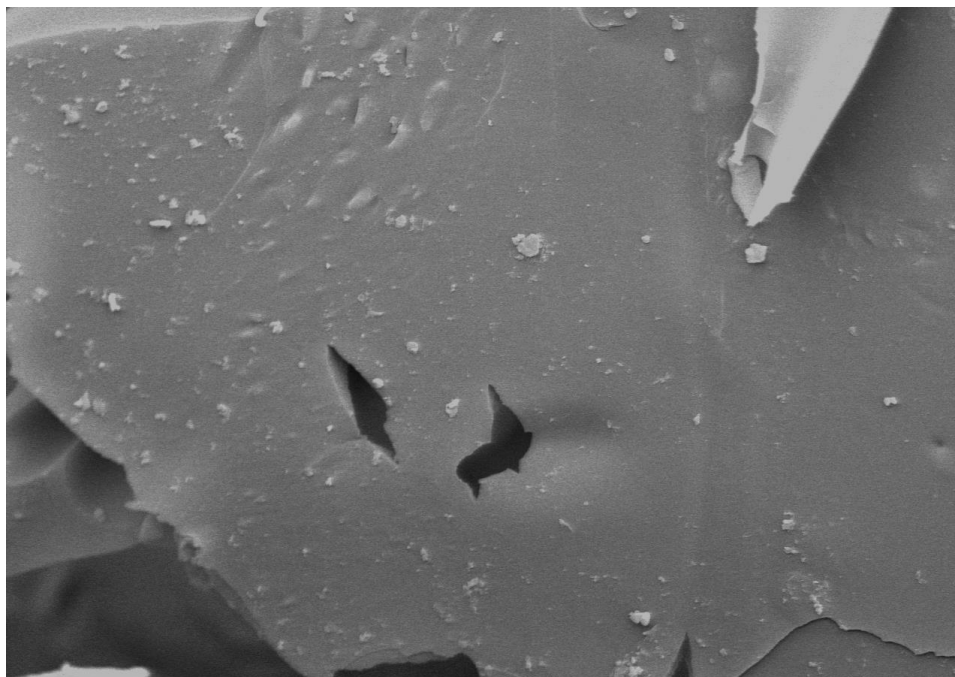

Clariant SU7000 5.00kV 5.1mm x5.00k UD+LD+MD 07/19/2024 10.0μm

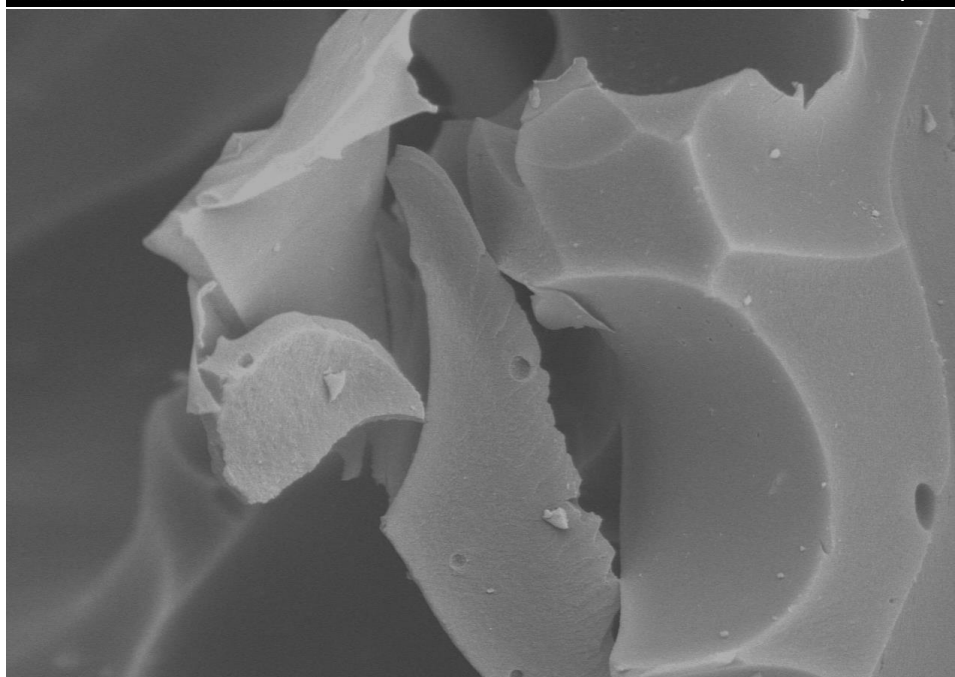


Clariant SU7000 5.00kV 5.1mm x5.00k UD+LD+MD 07/19/2024 10.0μm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-2
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047623-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

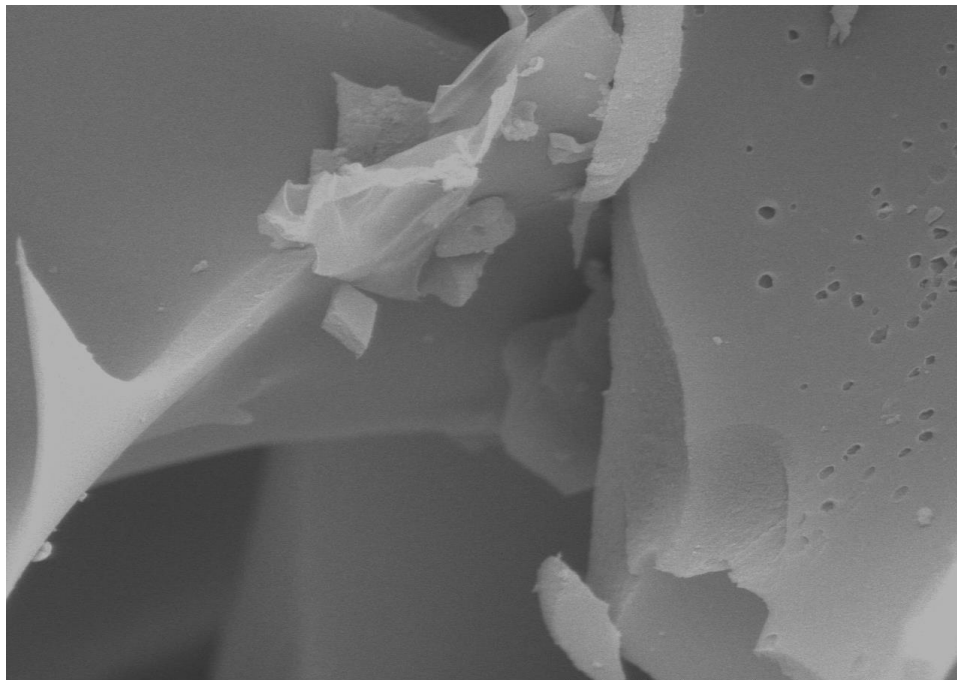

Clariant SU7000 5.00kV 5.1mm x10.0k UD+LD+MD 07/19/2024 5.00µm

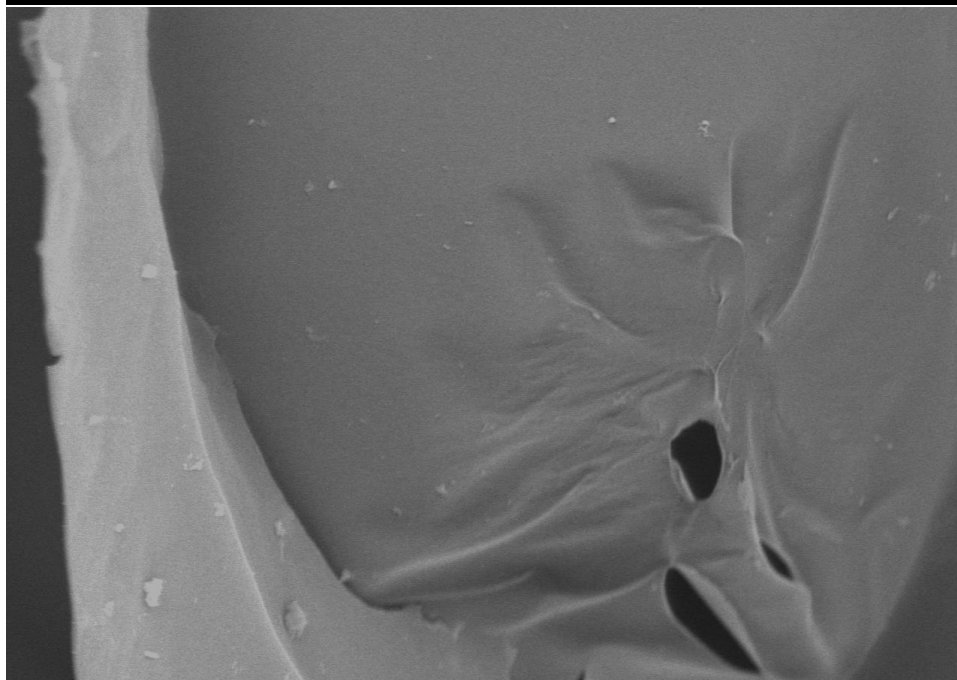


Clariant SU7000 5.00kV 5.1mm x10.0k UD+LD+MD 07/19/2024 5.00µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-2
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047623-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

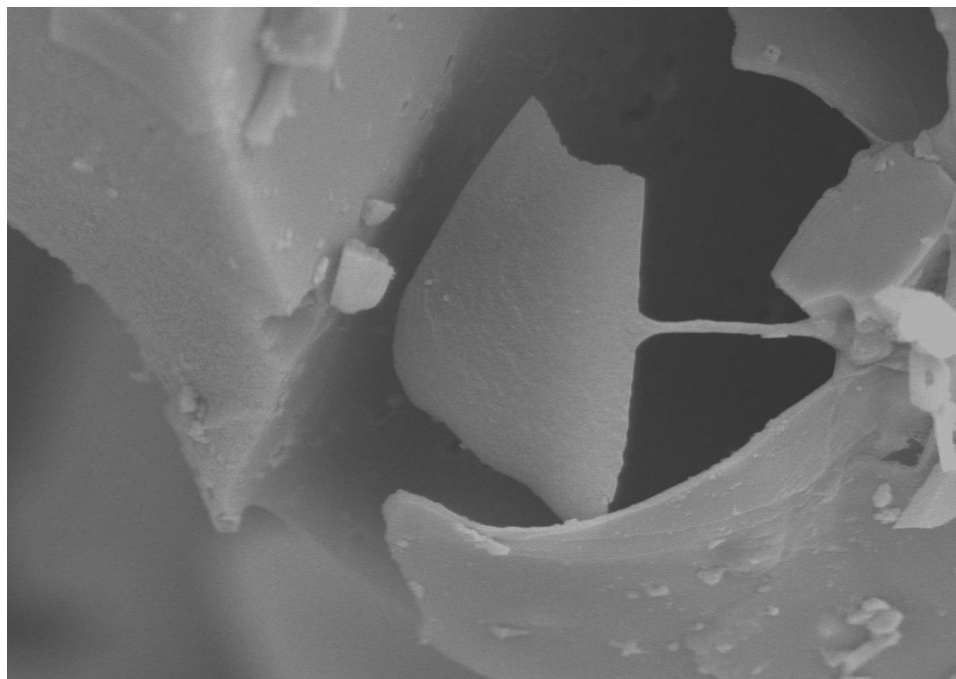

Clariant SU7000 5.00kV 5.0mm x10.0k UD+LD+MD 07/19/2024 5.00µm

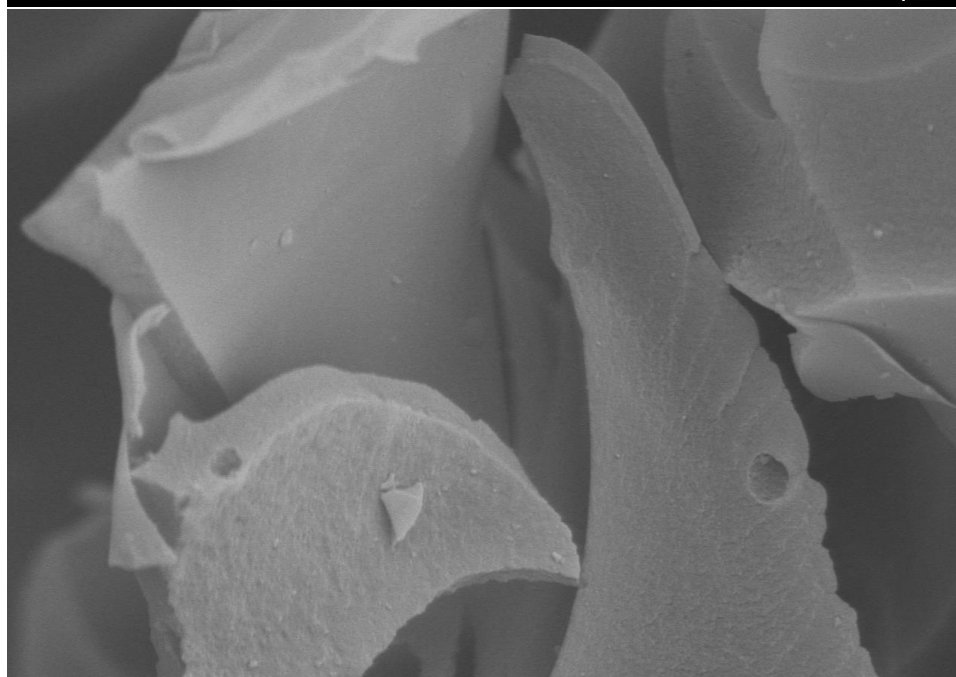


Clariant SU7000 5.00kV 5.1mm x10.0k UD+LD+MD 07/19/2024 5.00µm


SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-2
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047623-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

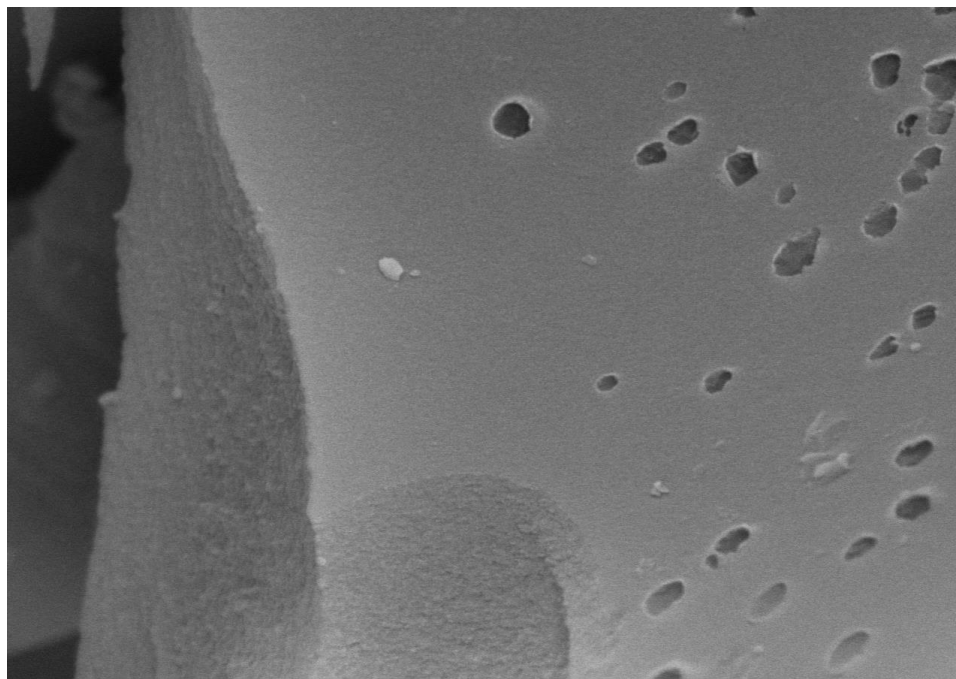

Clariant SU7000 5.00kV 5.1mm x25.0k UD+LD+MD 07/19/2024 2.00µm

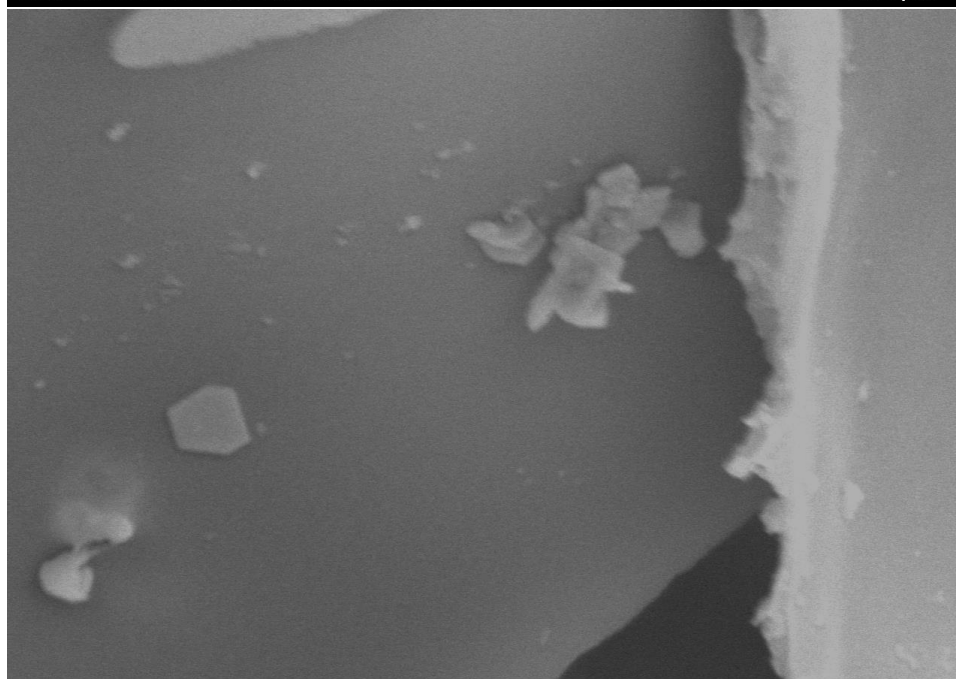

Clariant SU7000 5.00kV 5.1mm x25.0k UD+LD+MD 07/19/2024 2.00µm

SCANNING ELECTRON MICROSCOPE (SEM)

Sample name: TB1137-2
Ordering customer: Dr. Torsten Busch
Dept./Plant: Curia Germany GmbH
Order number: 24-047623-1

Sample treatment: The sample was subjected to platinum sputter coating and then measured.

